

Date: 2024/5/24

System Check_835MHz

D835V2-SN:4d162

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.921$ S/m; $\epsilon_r = 43.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(9.49, 9.49, 9.49); Calibrated: 2023/6/6
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2024/3/14
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Area Scan (42.0 mm x 210.0 mm): Measurement Grid: 7.0 mm x 15.0 mm

SAR (1g) = 2.52 W/kg; SAR (10g) = 1.63 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.53 W/kg; SAR (10g) = 1.67 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 88.5 %

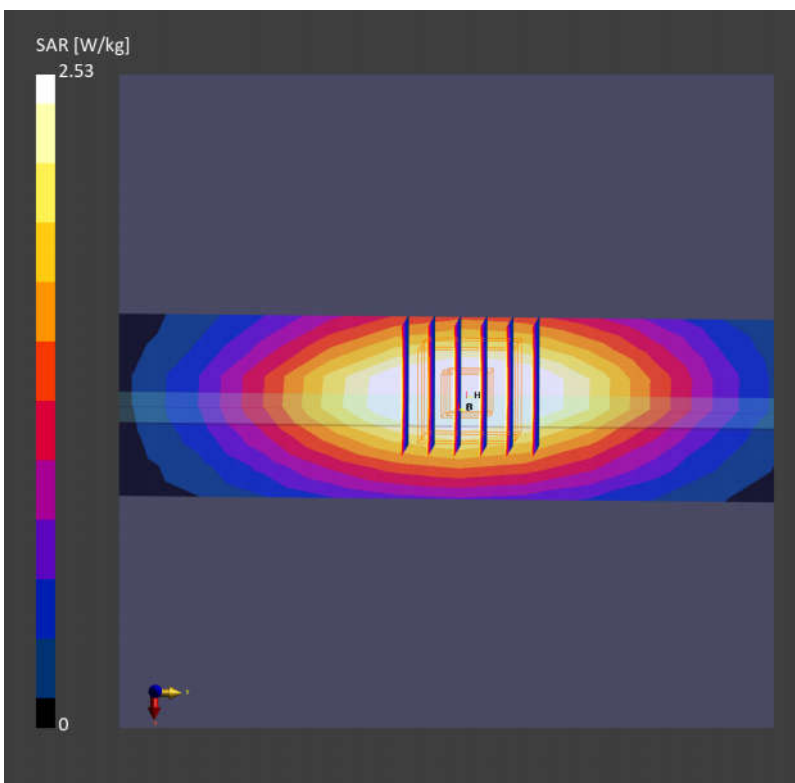

System Check_1750MHz

D1750V2-SN:1137

Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.36$ S/m; $\epsilon_r = 41.8$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(8.58, 8.58, 8.58); Calibrated: 2023/6/6
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2024/3/14
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 8.83 W/kg; SAR (10g) = 4.78 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 8.93 W/kg; SAR (10g) = 4.81 W/kg

Smallest distance from peaks to all points 3 dB below = 9.9 mm

Ratio of SAR at M2 to SAR at M1 = 83.1 %

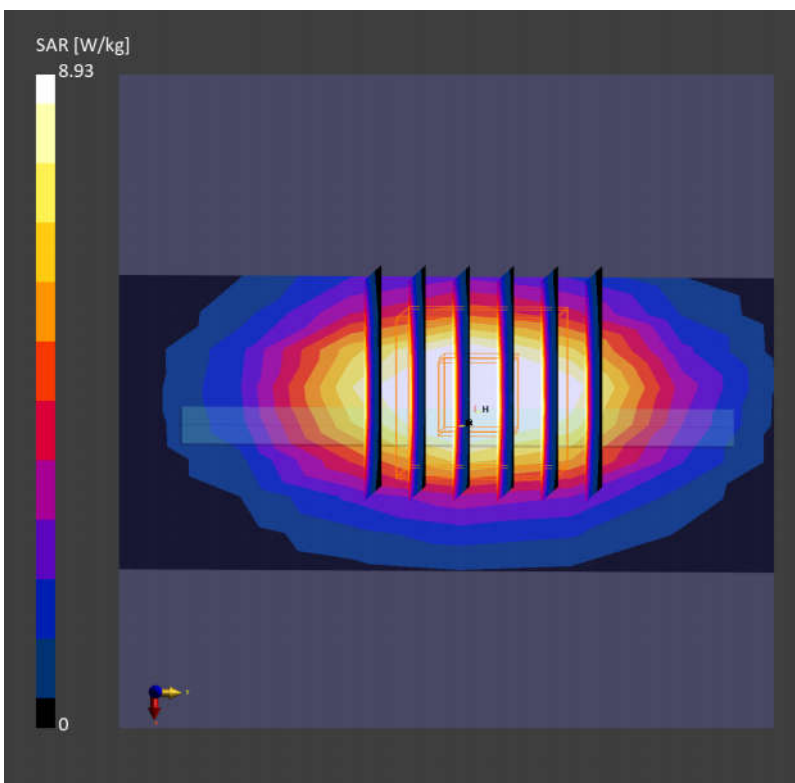

System Check_1900MHz

D1900V2-SN:5d182

Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 41.5$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(8.29, 8.29, 8.29); Calibrated: 2023/6/6
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2024/3/14
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
SAR (1g) = 10.6 W/kg; SAR (10g) = 5.41 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 10.5 W/kg; SAR (10g) = 5.38 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 82.6 %

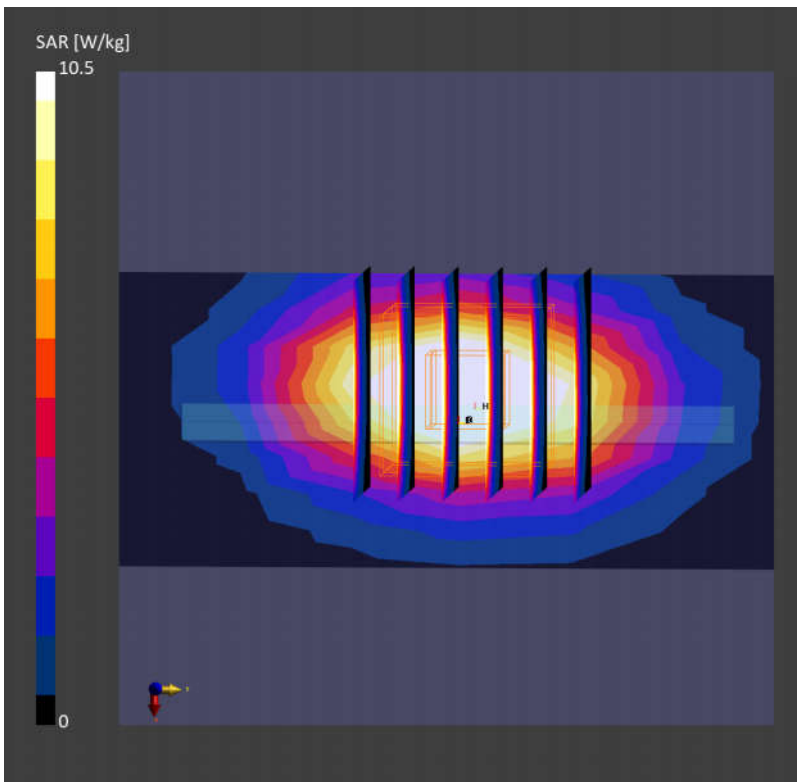

System Check_2600MHz

D2600V2-SN:1070

Communication System: CW; Frequency: 2600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.91$ S/m; $\epsilon_r = 40.3$
Ambient Temperature: 23.6°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.55, 7.55, 7.55); Calibrated: 2023/6/6
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1437; Calibrated: 2024/3/14
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.8 W/kg; SAR (10g) = 6.05 W/kg;

Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 14.2 W/kg; SAR (10g) = 6.18 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.1 %

