

Schmid & Partner Engineering AG

Zaughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

900 MHz System Validation Dipole

Type:

D900V2

Serial Number:

078

Place of Calibration:

Zurich

Date of Calibration:

August 23, 2001

Calibration Interval:

24 months


Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:



Approved by:



**Schmid & Partner
Engineering AG**

Zaughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

DASY

Dipole Validation Kit

Type: D900V2

Serial: 078

Manufactured: August 21, 2000

Calibrated: August 23, 2001

1. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with head simulating solution of the following electrical parameters at 900 MHz:

Relative Dielectricity	40.3	± 5%
Conductivity	0.95 mho/m	± 5%

The DASY3 System (Software version 3.1c) with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.27 at 900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW ± 3 %. The results are normalized to 1W input power.

2. SAR Measurement

Standard SAR-measurements were performed with the phantom according to the measurement conditions described in section 1. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

averaged over 1 cm ³ (1 g) of tissue:	11.3 mW/g
averaged over 10 cm ³ (10 g) of tissue:	7.12 mW/g

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well.

1. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with head simulating solution of the following electrical parameters at 900 MHz:

Relative Dielectricity	40.3	± 5%
Conductivity	0.95 mho/m	± 5%

The DASY3 System (Software version 3.1c) with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.27 at 900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW ± 3%. The results are normalized to 1W input power.

2. SAR Measurement

Standard SAR-measurements were performed with the phantom according to the measurement conditions described in section 1. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

averaged over 1 cm ³ (1 g) of tissue:	11.3 mW/g
averaged over 10 cm ³ (10 g) of tissue:	7.12 mW/g

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well.

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	1.410 ns	(one direction)
Transmission factor:	0.988	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 900 MHz:	$\text{Re}\{Z\} = $ 50.5 Ω
---------------------------------	---

	$\text{Im}\{Z\} = $ -4.6 Ω
--	---

Return Loss at 900 MHz	-26.7 dB
------------------------	-----------------

4. Handling



The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Do not apply excessive force to the dipole arms, because they might bend. If the dipole arms have to be bent back, take care to release stress to the soldered connections near the feedpoint, they might come off.

After prolonged use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Validation Dipole D900V2 SN:078, d = 15 mm

Frequency: 900 MHz; Antenna Input Power: 250 [mW]
SAM Phantom; Flat Section; Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0
Probe: ET3DV6 - SN1567; ConvF(6.27,6.27,6.27) at 900 MHz; IEEE 1528 900 MHz; $\sigma = 0.95$ mho/m $\epsilon_r = 40.3$ $\rho = 1.00$ g/cm³
Cubes (2); Peak: 4.57 mW/g ± 0.02 dB, SAR (1g): 2.82 mW/g ± 0.02 dB, SAR (10g): 1.73 mW/g ± 0.02 dB, SAR (Worst-case extrapolation)
Penetration depth: 11.5 (10.2, 13.1) [mm]
Powerdrift: -0.01 dB

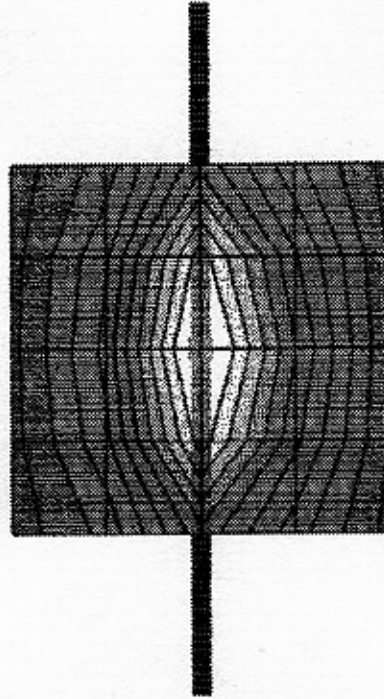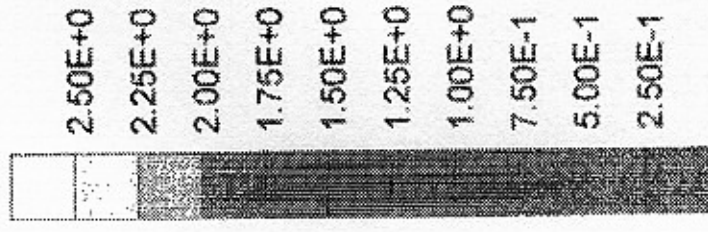

CH1 011 1 U FS

0.52457 n -4.5445 p 38.075 pF

900.000 000 MHz

Y

Del


PKn

Cor


Avg

16

T

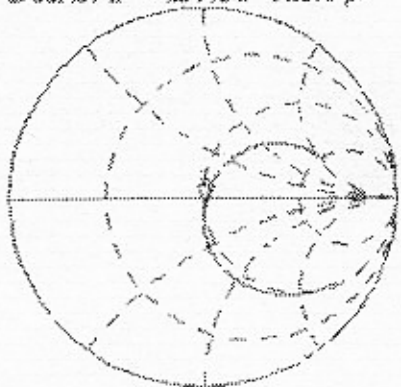

CH2 011 LOG 0 dB REF 0 dB 1-25.525 dB 900.000 000 MHz

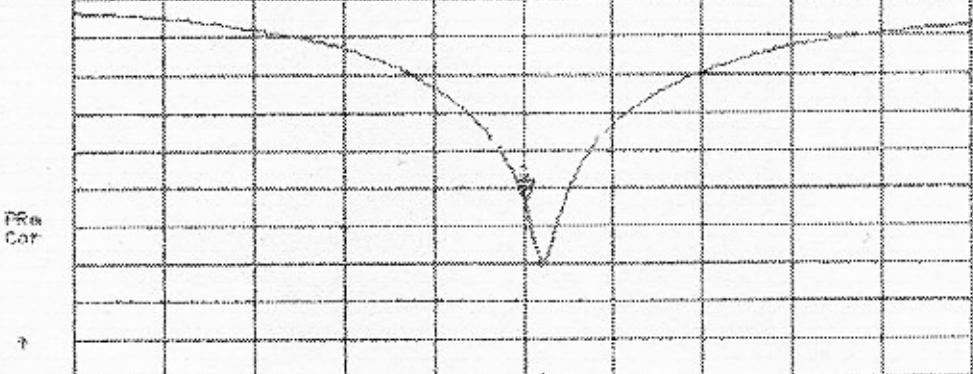

START 700.000 000 MHz

900

1000

STOP 1.100.000 000 MHz

T

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

1800 MHz System Validation Dipole

Type:

D1800V2

Serial Number:

259

Place of Calibration:

Zurich

Date of Calibration:

January 25, 2002

Calibration Interval:

24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

N. Kolaski Neviara

Approved by:

Blaini Kufner

**Schmid & Partner
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

DASY

Dipole Validation Kit

Type: D1800V2

Serial: 259

Manufactured: December 23, 1999
Calibrated: January 25, 2002

1. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with head simulating solution of the following electrical parameters at 1800 MHz:

Relative Dielectricity	39.6	± 5%
Conductivity	1.37 mho/m	± 5%

The DASY3 System (Software version 3.1d) with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 5.31 at 1800 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 20mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW ± 3%. The results are normalized to 1W input power.

2. SAR Measurement

Standard SAR-measurements were performed with the phantom according to the measurement conditions described in section 1 (description of the modifications performed on the dipole are presented in section 4.). The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

averaged over 1 cm ³ (1 g) of tissue:	39.3 mW/g
averaged over 10 cm ³ (10 g) of tissue:	20.6 mW/g

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well.

6. Dipole Impedance and Return Loss (w/o Teflon rings)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

$$\text{Feedpoint impedance at 1800 MHz:} \quad \text{Re}\{Z\} = 47.3 \, \Omega$$

$$\text{Im}\{Z\} = -6.2 \, \Omega$$

$$\text{Return Loss at 1800 MHz} \quad -23.2 \, \text{dB}$$

7. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

8. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.



9. Power Test

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Validation Dipole D1800V2 SN:259, d = 10 mm (with Teflon rings)

Frequency: 1800 MHz, Antenna Input Power: 250 [mW]
 SAM Phantom; Flat Section; Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0
 Probe: ET3DV6 - SN1507; ConvF(5.31,5.31,5.31) at 1800 MHz; IEEE1528 1800 MHz; $\sigma = 1.37$ mho/m $\epsilon_r = 39.6$ $\rho = 1.00$ g/cm³
 Cubes (2): Peak: 18.5 mW/g ± 0.01 dB, SAR (1g): 9.83 mW/g ± 0.02 dB, SAR (10g): 5.15 mW/g ± 0.01 dB, (Worst-case extrapolation)
 Penetration depth: 8.3 (7.8, 9.3) [mm]
 Powerdrift: 0.00 dB

SAR_{Tot} [mW/g]

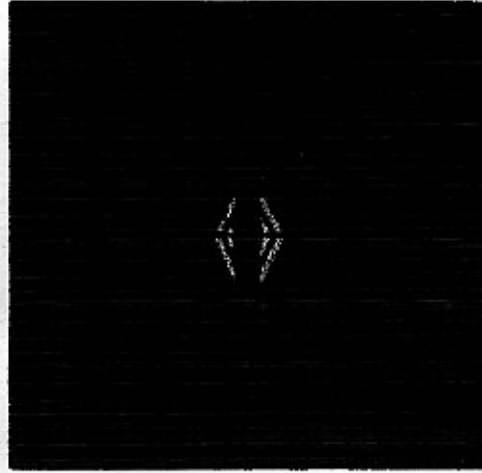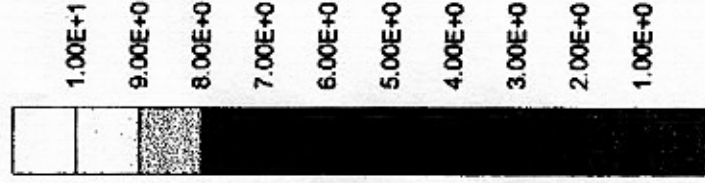

25 Jan 2002 15:48:33

CH1 S11 1 U FS

1: 52.838 α 5.5547 α 491.14 pH


1 800.000 000 MHz

Del

Cor

Avg
16

↑

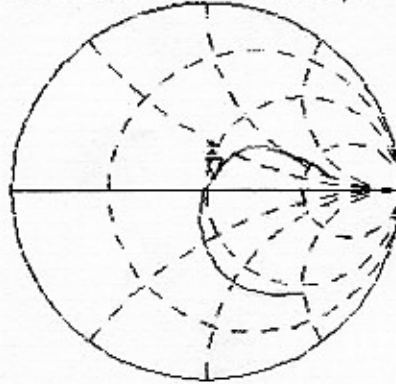


CH2 S11 LOG 3 dB/REF 0 dB 1:-24.350 dB 1 800.000 000 MHz

Cor

Avg
16

↑


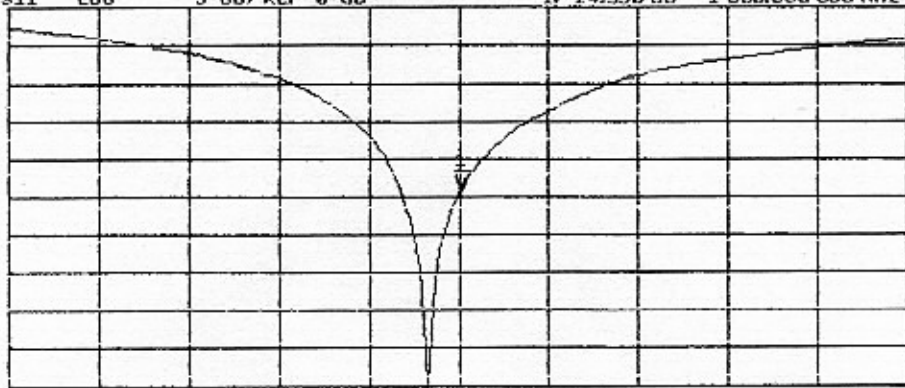


CENTER 1 800.000 000 MHz

SPAN 800.000 000 MHz

Validation Dipole D1800V2 SN:259, d = 10 mm (w/o Teflon rings)

Frequency: 1800 MHz; Antenna Input Power: 250 [mW]
 SAM Phantom; Flat Section; Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0
 Probe: ET3DV6 - SN1507; ConvF(5.31, 5.31, 5.31) at 1800 MHz; IEEE1528 1800 MHz; $\sigma = 1.37$ mho/m $\epsilon_r = 39.6$ $\rho = 1.00$ g/cm³
 Cubes (2): Peak: 19.1 mW/g ± 0.03 dB, SAR (1g): 10.1 mW/g ± 0.01 dB, SAR (10g): 5.25 mW/g ± 0.01 dB, (Worst-case extrapolation)
 Penetration depth: 8.3 (7.8, 9.3) [mm]
 Powerdrift: -0.03 dB

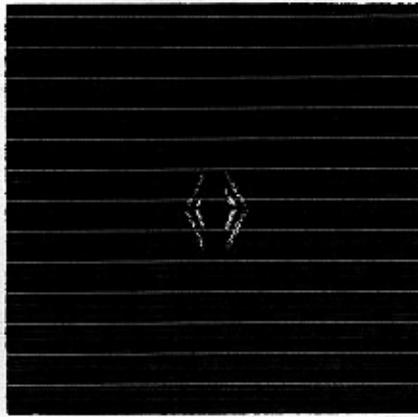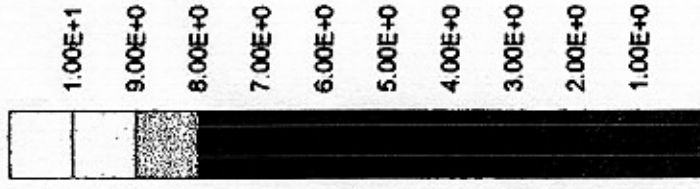SAR_{Tot} [mW/g]

25 Jan 2002 15:46:50

[CH1] S11 1 U FS

1: 47.332 μ -6.2207 μ 14.214 pF


1 000.000 000 MHz

Del

Cor

Avg
16

f

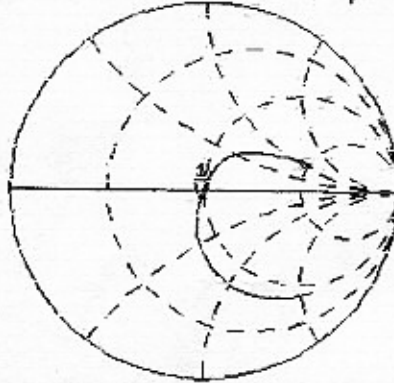


CH2 S11 LOG 5 dB/REF 0 dB 1: -23.174 dB 1 000.000 000 MHz

Cor

Avg
16

f

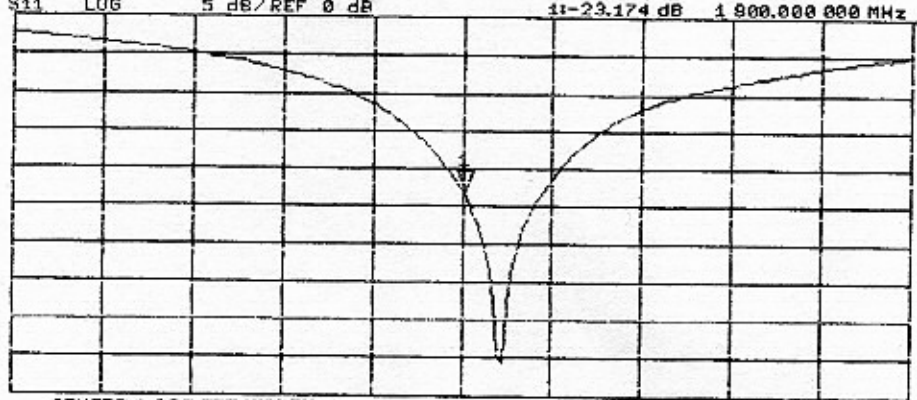

CENTER 1 000.000 000 MHz

SPAN 000.000 000 MHz

Interim Dipole Correlation Certificate

FCD-0359, Rev.001

Dipole Serial Number:	F 092	Last Calibration Date:	3-Jan-01
Dipole Type (MHz):	900 MHz	Calibration Due:	3-Jan-03
		Manufacturer:	SPEAG

-Manufacturer's Original Calibration Information-

Dipole to be correlated: [Serial Number: 092]

1g SAR normalized to 1W forward power (mW/g):	10.12 mW/g
Relative Dielectric:	40.6
Conductivity:	0.85
Probe Serial Number:	SN 1507
Forward Power:	250mW +/- 3%

Primary Dipole Referenced: [Serial Number: 077]

1g SAR normalized to 1W forward power (mW/g):	11.4 mW/g
Relative Dielectric:	40.3
Conductivity:	0.95
Probe Serial Number:	SN 1507
Forward Power:	250mW +/- 3%

-Correlation Method Utilized- per DOI-1265

(select one)

By Similarity:

By Transfer Calibration:

-Measured Data-

Probe S/N:	SN 1513	Conductivity (meas.):	0.97
Robot Cell #:	RVD #8	Permittivity (meas.):	42.3

Primary Standard (average of 0-degree & 90-degree 1g cubes):

2.875 mW/g	N/R	N/R
(if required)	(if required)	(if required)

Secondary Standard (average of 0-degree & 90-degree 1g cubes):

2.885 mW/g	N/R	N/R
(if required)	(if required)	(if required)

-NEW Correlated Target-

1g SAR normalized to 1W forward power (mW/g):	11.4 mW/g
Relative Dielectric:	40.3
Conductivity:	0.95

Approved by: *Anton, Feneand*

Date: 11/13/2001

Comments:

Secondary dipole measured -2.4% from primary dipole.

Interim Dipole Correlation Certificate

FCD-0359, Rev.001

Dipole Serial Number:	272(TR)	Last Calibration Date:	14-Nov-02
Dipole Type (MHz):	D1800V2 w Teflon rings	Calibration Due:	14-Nov-04
		Manufacturer:	SPEAG

-Manufacturer's Original Calibration Information-

Dipole to be correlated: [Serial Number: 272TR]

1g SAR normalized to 1W forward power (mW/g):	36.4 mW/g
Relative Dielectric:	40.2
Conductivity:	1.35
Probe Serial Number:	1507
Forward Power:	250

Primary Dipole Referenced: [Serial Number: 246TR]

1g SAR normalized to 1W forward power (mW/g):	38.8 mW/g
Relative Dielectric:	39.6
Conductivity:	1.37
Probe Serial Number:	1507
Forward Power:	250

-Correlation Method Utilized- per DOI-1265

(select one)

By Similarity: By Transfer Calibration:

-Measured Data-

Probe S/N:	1515	Conductivity (meas.):	1.38
Robot Cell #:	PCS-2	Permittivity (meas.):	40.7

Primary Standard (average of 0-degree & 90-degree 1g cubes):

9.84 mW/g		
	(if required)	(if required)

Secondary Standard (average of 0-degree & 90-degree 1g cubes):

9.96 mW/g		
	(if required)	(if required)


=====

-NEW Correlated Target-

1g SAR normalized to 1W forward power (mW/g):	38.8 mW/g
Relative Dielectric:	39.6
Conductivity:	1.37

=====

Approved by:



Date:

1/10/03

Comments:

Correlated to get worst case extrapolation targets. Secondary measured within 2% of the primary standard.

Interim Dipole Correlation Certificate

FCD-0359, Rev.001

Dipole Serial Number:	273(TR)	Last Calibration Date:	July 17, 2002
Dipole Type (MHz):	D1800V2 w/ Teflon Rings	Calibration Due:	July 17, 2004
		Manufacturer:	SPEAG

-Manufacturer's Original Calibration Information-

Dipole to be correlated: [Serial Number: 273(TR)]

1g SAR normalized to 1W forward power (mW/g):	39.6 mW/g
Relative Dielectric:	40.3
Conductivity:	1.36
Probe Serial Number:	1507
Forward Power:	250mW

Primary Dipole Referenced: [Serial Number: 246(TR)]

1g SAR normalized to 1W forward power (mW/g):	38.8 mW/g
Relative Dielectric:	39.6
Conductivity:	1.37
Probe Serial Number:	1507
Forward Power:	250mW

-Correlation Method Utilized- per DOI-1265

(select one)

By Similarity: By Transfer Calibration:

-Measured Data-

Probe S/N:	1515	Conductivity (meas.):	1.36
Robot Cell #:	PCS-2	Permittivity (meas.):	38.9

Primary Standard (average of 0-degree & 90-degree 1g cubes):

9.805 mW/g		
	(if required)	(if required)

Secondary Standard (average of 0-degree & 90-degree 1g cubes): Mayo Tic

9.900 mW/g		
	(if required)	(if required)

=====

-NEW Correlated Target-

1g SAR normalized to 1W forward power (mW/g):	38.8 mW/g
Relative Dielectric:	39.6
Conductivity:	1.37

=====

Approved by:  Date: 7-Nov-02

Comments: Secondary dipole measured +1% from primary dipole.
(this correlation required for use with Teflon ring endcaps.)

Interim Dipole Correlation Certificate

FCD-0359, Rev.001

Dipole Serial Number:	425(TR)	Last Calibration Date:	13-Nov-02
Dipole Type (MHz):	835MHz dipole with Teflon rings	Calibration Due:	13-Nov-04
		Manufacturer:	SPEAG

-Manufacturer's Original Calibration Information-

Dipole to be correlated: [Serial Number: 425TR]

1g SAR normalized to 1W forward power (mW/g):	9.2 mW/g
Relative Dielectric:	43.05
Conductivity:	0.90
Probe Serial Number:	1507
Forward Power:	250 mW

Primary Dipole Referenced: [Serial Number: 423tr]

1g SAR normalized to 1W forward power (mW/g):	10.04 mW/g
Relative Dielectric:	41.9
Conductivity:	0.89
Probe Serial Number:	1507
Forward Power:	250mW

-Correlation Method Utilized- per DOI-1265

(select one)

By Similarity: By Transfer Calibration:

-Measured Data-

Probe S/N:	1522	Conductivity (meas.):	0.94
Robot Cell #:	PCS-3	Permittivity (meas.):	43.1

Primary Standard (average of 0-degree & 90-degree 1g cubes):

2.79 mW/g (1W)		
	(if required)	(if required)

Secondary Standard (average of 0-degree & 90-degree 1g cubes):

2.76 mW/g (1W)		
	(if required)	(if required)

=====

-NEW Correlated Target-

1g SAR normalized to 1W forward power (mW/g):	10.04 mW/g
Relative Dielectric:	41.9
Conductivity:	0.89

=====

Approved by:  Date: 12/12/2002

Comments: Correlated to get worst case extrapolation targets. Secondary measured within 1% of the primary standard.