

HAC_E_Dipole_835

DUT: HAC-Dipole 835 MHz

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1
 Medium: Air Medium parameters used: $\sigma = 0$ S/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³
 Ambient Temperature : 23.8 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn910; Calibrated: 2018/6/21
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

E Scan - measurement distance from the probe sensor center to CD835 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x361x1): Interpolated grid:

dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 131.7 V/m; Power Drift = -0.02 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 114.9 V/m

Average value of Total=(114.6+114.9) / 2 = 114.75 V/m

PMF scaled E-field



Grid 1 M4 111.4 V/m	Grid 2 M4 114.6 V/m	Grid 3 M4 113.2 V/m
Grid 4 M4 64.73 V/m	Grid 5 M4 66.19 V/m	Grid 6 M4 65.38 V/m
Grid 7 M4 112.8 V/m	Grid 8 M4 114.9 V/m	Grid 9 M4 112.9 V/m

Cursor:

Total = 114.9 V/m

E Category: M4

Location: 0, 70.5, 9.7 mm



0 dB = 114.9 V/m = 41.21 dBV/m

HAC_E_Dipole_1880

DUT: HAC Dipole 1880 MHz

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1
 Medium: Air Medium parameters used: $\sigma = 0$ S/m, $\epsilon_r = 1$; $\rho = 0$ kg/m³
 Ambient Temperature : 23.8 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn910; Calibrated: 2018/6/21
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

E Scan - measurement distance from the probe sensor center to CD1880 = 10mm & 15mm/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid:

dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 143.3 V/m; Power Drift = 0.04 dB

PMR not calibrated. PMF = 1.000 is applied.

E-field emissions = 92.75 V/m

Average value of Total=(90.04+92.75) / 2 = 91.395 V/m

PMF scaled E-field



Grid 1 M3 89.23 V/m	Grid 2 M3 90.04 V/m	Grid 3 M3 88.02 V/m
Grid 4 M3 72.14 V/m	Grid 5 M3 73.44 V/m	Grid 6 M3 72.66 V/m
Grid 7 M3 91.09 V/m	Grid 8 M3 92.75 V/m	Grid 9 M3 90.88 V/m

Cursor:

Total = 92.75 V/m

E Category: M3

Location: 0, 31, 9.7 mm

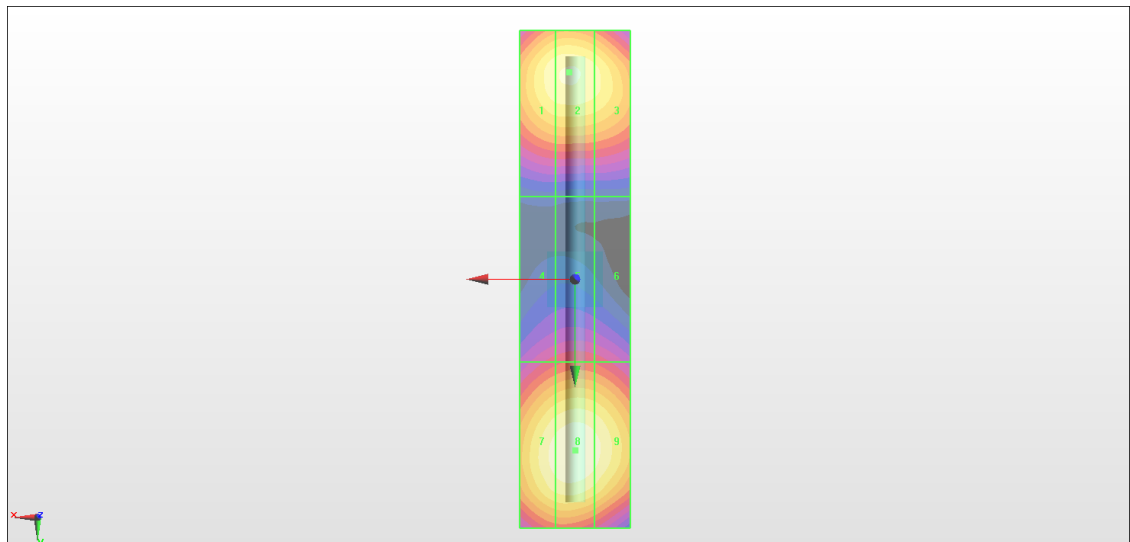

0 dB = 92.75 V/m = 39.35 dBV/m