

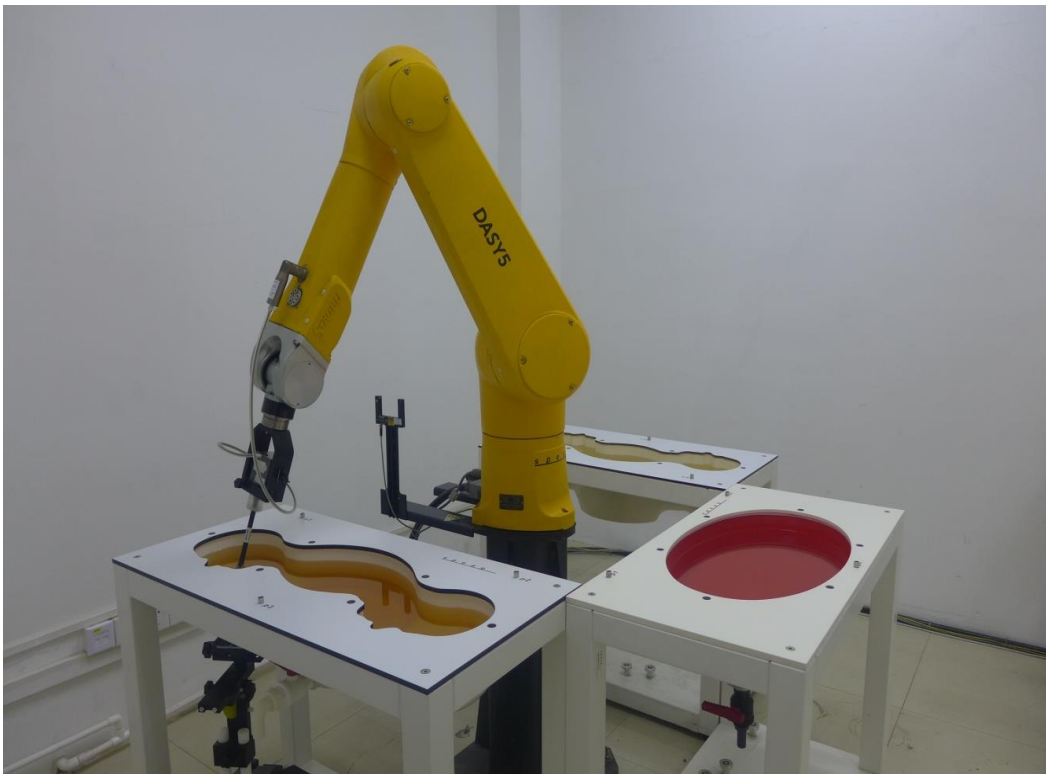


Appendix D

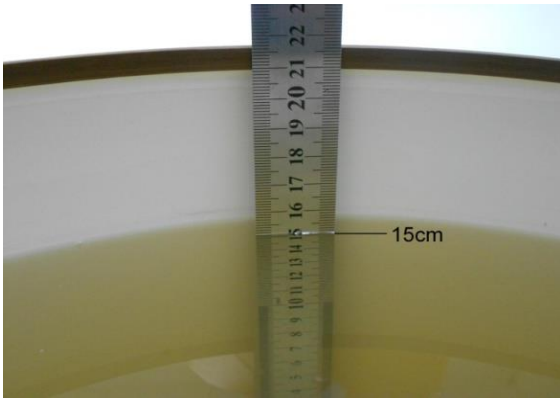

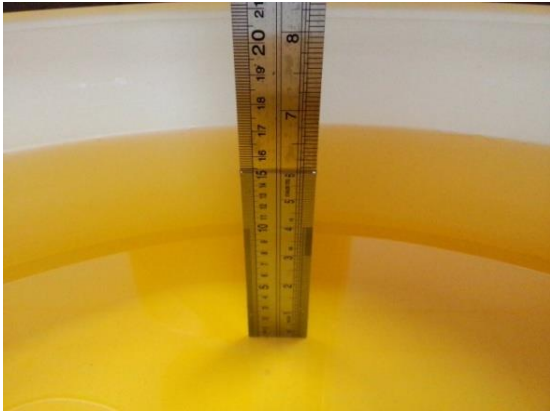

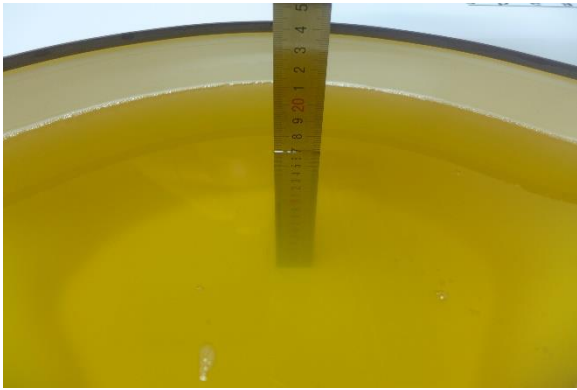
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

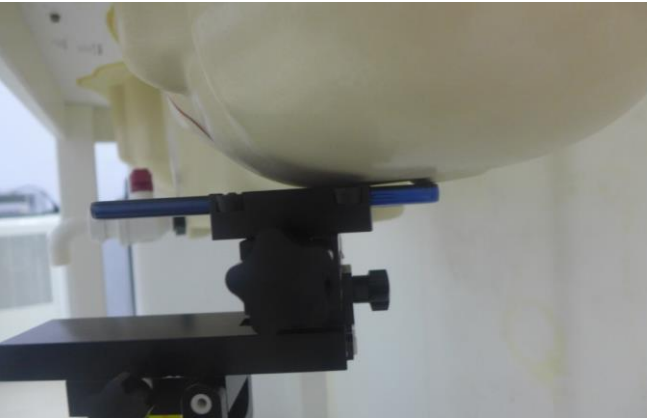
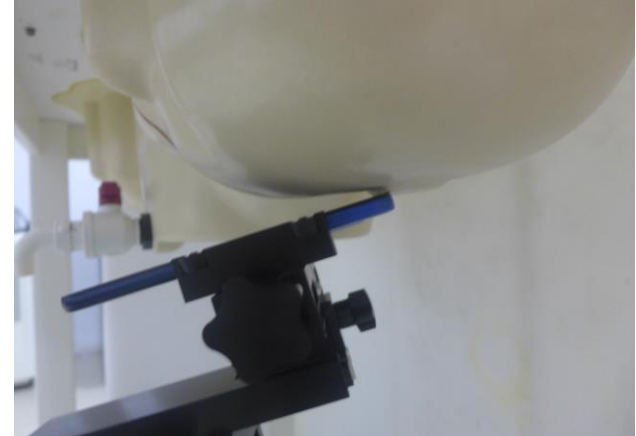
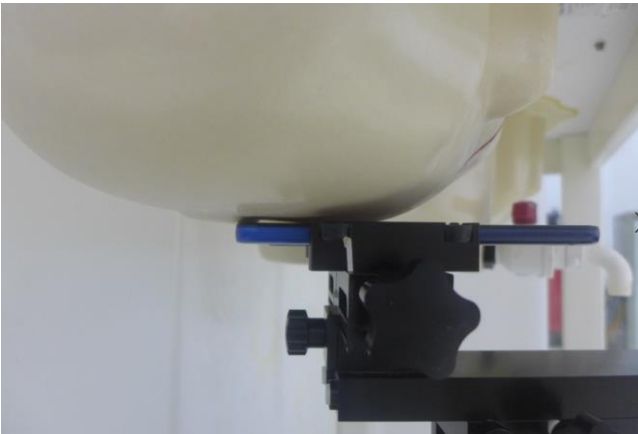
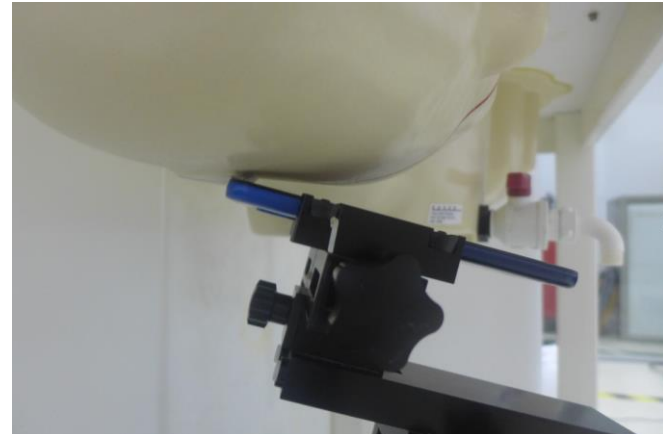


1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Head 1750</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 4: Tissue Simulant Liquid for Head 2450</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2600</p>	<p>NA</p>
	<p>NA</p>

3. Photographs of EUT test position

<p align="center">Photo 6: Left cheek</p>	<p align="center">Photo 7: Left tilted</p>
	
<p align="center">Photo 8: Right cheek</p>	<p align="center">Photo 9: Right tilted</p>
	
<p align="center">Photo 10: Front side 5mm</p>	<p align="center">Photo 11: Back side 5mm</p>
	

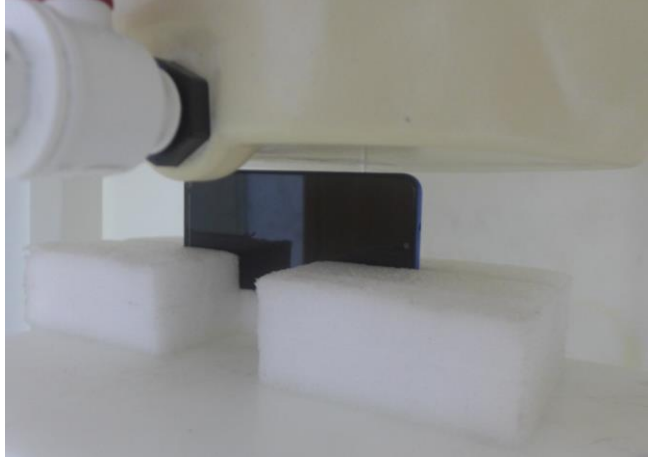

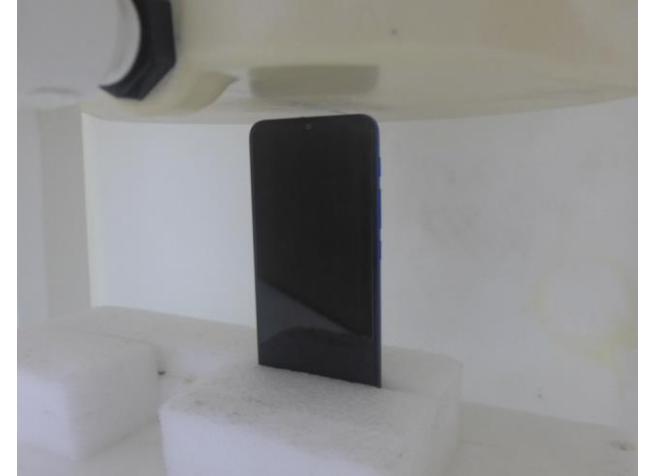
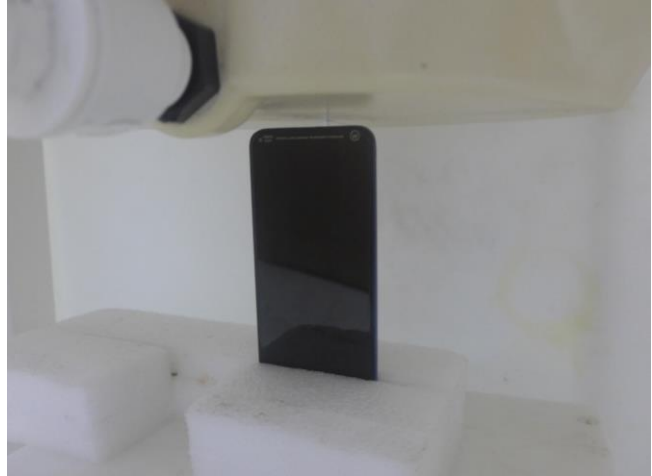

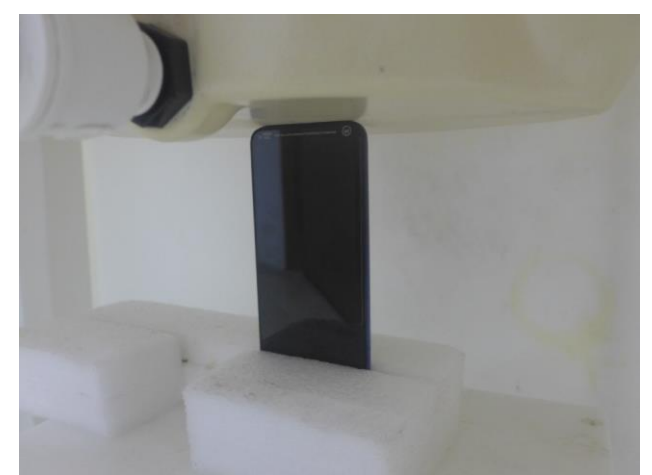




<p>Photo 12: Left side 5mm</p>	<p>Photo 13: Right side 5mm</p>
	
<p>Photo 14: Top side 5mm</p>	<p>Photo 15: Bottom side 5mm</p>
	
<p>Photo 16: Back side 0mm</p>	<p>Photo 15: Bottom side 0mm</p>
	

Photo 17: Back side with headset 5mm	NA
 A microscopic image showing the back side of a headset component. The component is dark and has a blue fiber optic cable attached to it. The background is light and slightly out of focus.	NA

4. EUT Constructional Details

Photo 18: Front View	Photo 19: Back View
	
Photo 20: Accessory	NA
	<p style="text-align: center;">NA</p>