

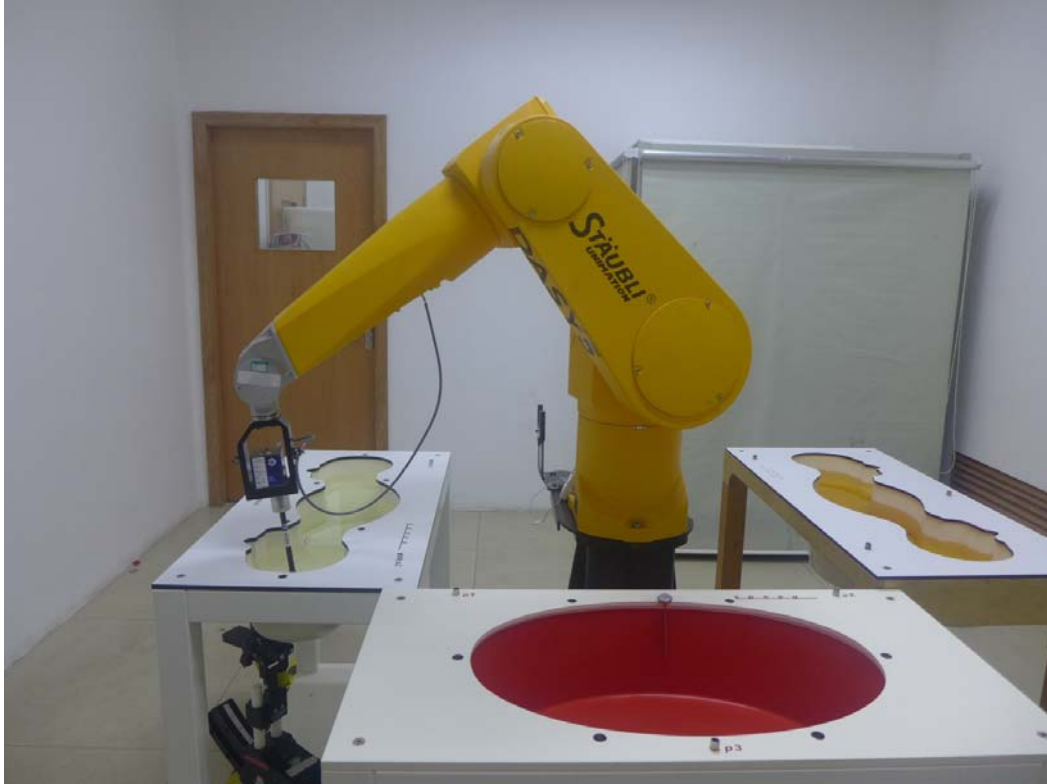


Appendix D

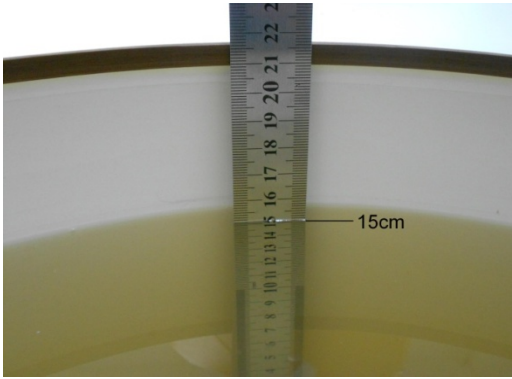



Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

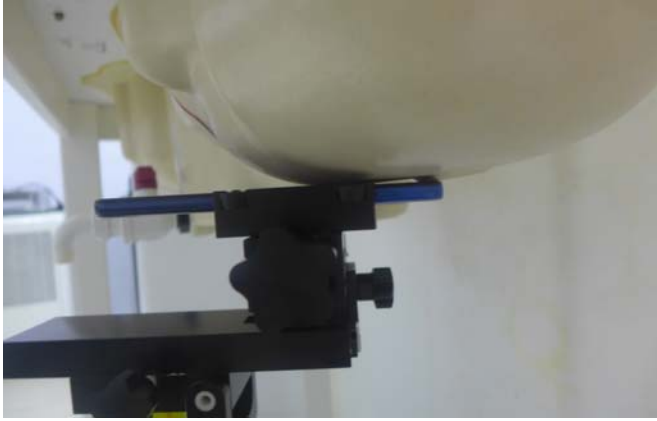

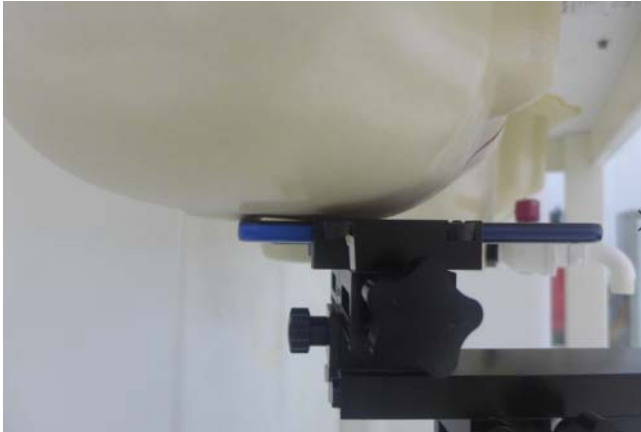
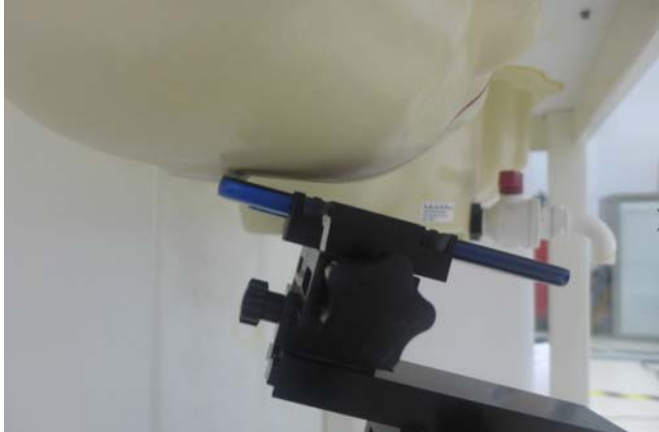


1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 1900
 <p>15cm</p>	
Photo 3: Tissue Simulant Liquid for Head 2450	Photo 4: Tissue Simulant Liquid for Head 2600
	

3. Photographs of EUT test position

<p>Photo 5: Left touch cheek</p>	<p>Photo 6: Left tilted 15 degree</p>
	
<p>Photo 7: Right touch cheek</p>	<p>Photo 8: Right tilted 15 degree</p>
	
<p>Photo 9: Front side 5mm</p>	<p>Photo 10: Back side 5mm</p>
	

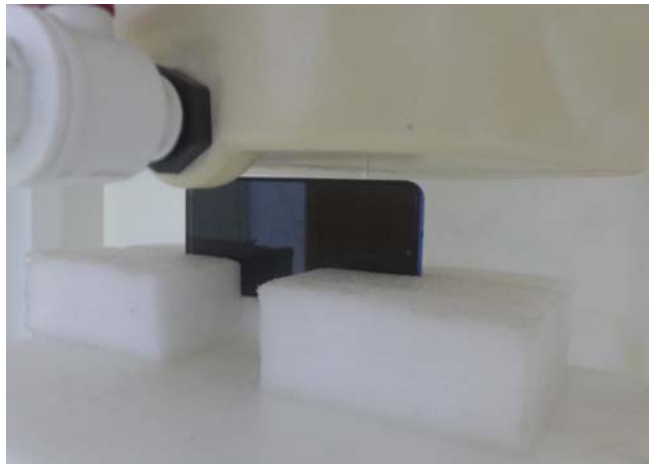

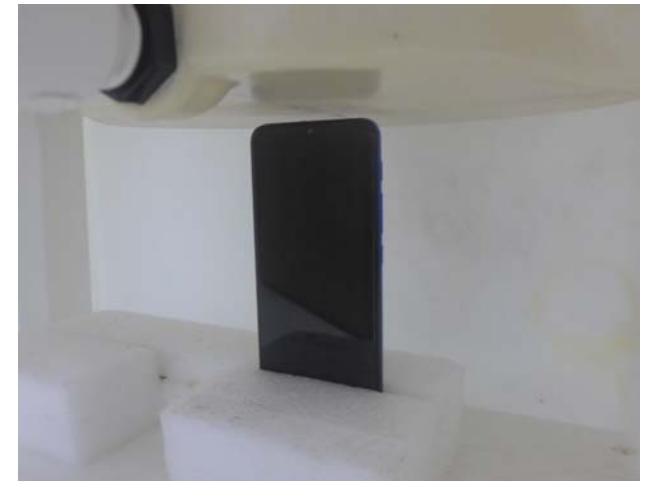







<p>Photo 11: Left side 5mm</p>	<p>Photo 12: Right side 5mm</p>
	
<p>Photo 13: Top side 5mm</p>	<p>Photo 14: Bottom side 5mm</p>
	
<p>Photo 15: Back side 0mm</p>	<p>Photo 15: Bottom side 0mm</p>
	

Photo 16: Back side with headset 5mm	NA
	NA

4. EUT Constructional Details

<p align="center">Photo 17: Front View</p>	<p align="center">Photo 18: Back View</p>
	
<p align="center">Photo 19: Accessory</p>	<p align="center">NA</p>
	<p align="center">NA</p>