



Appendix D

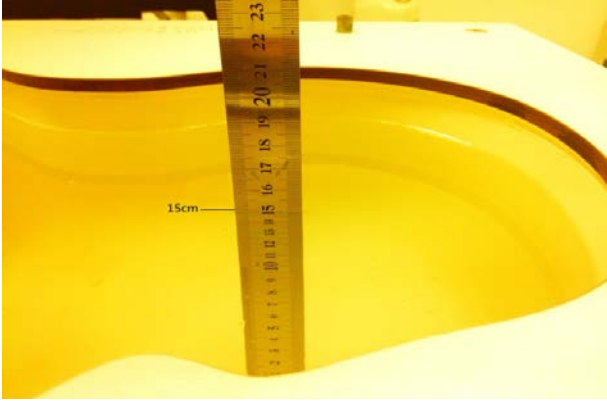
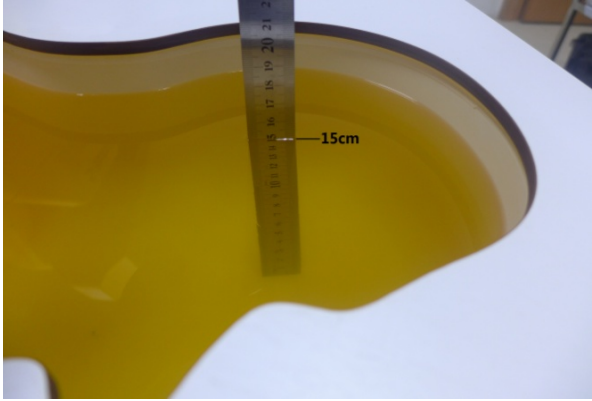
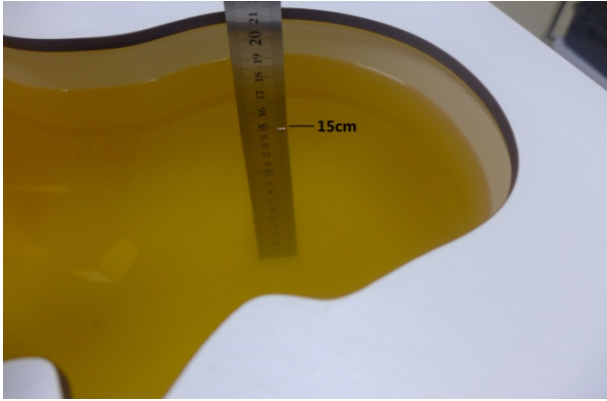
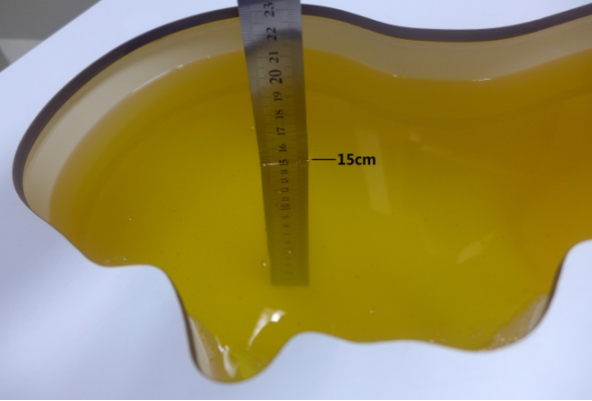
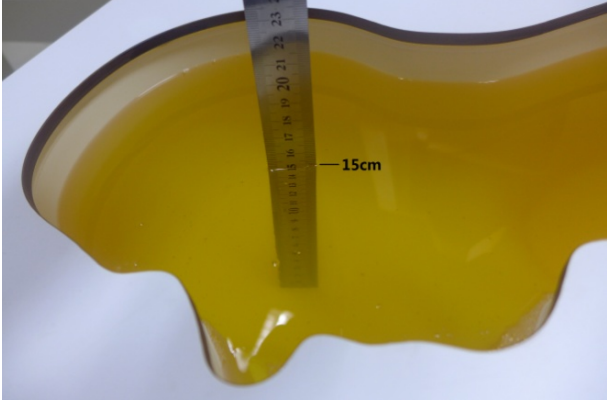
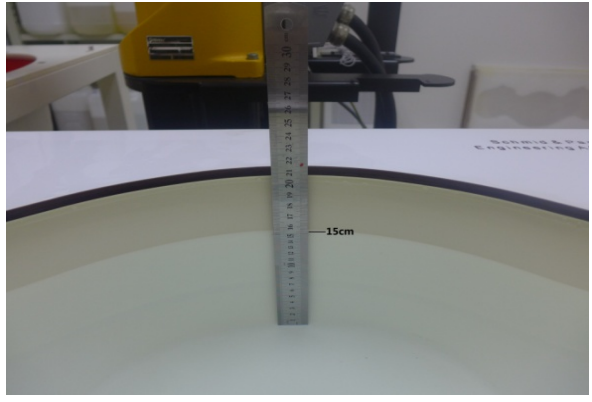
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

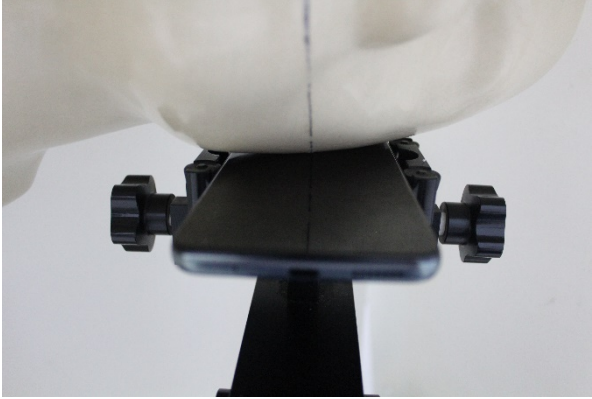
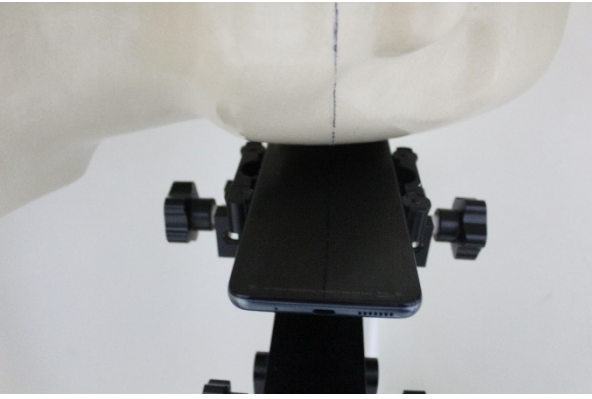

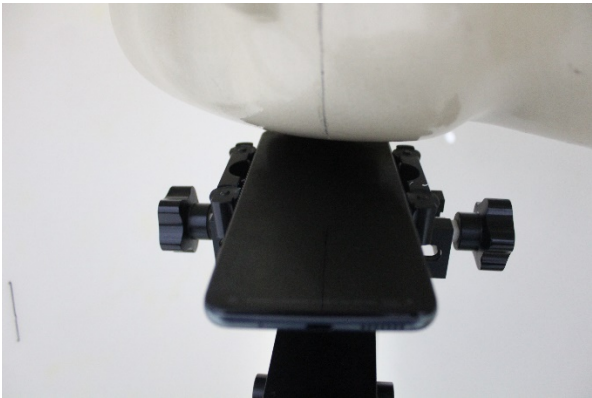


1. SAR measurement System







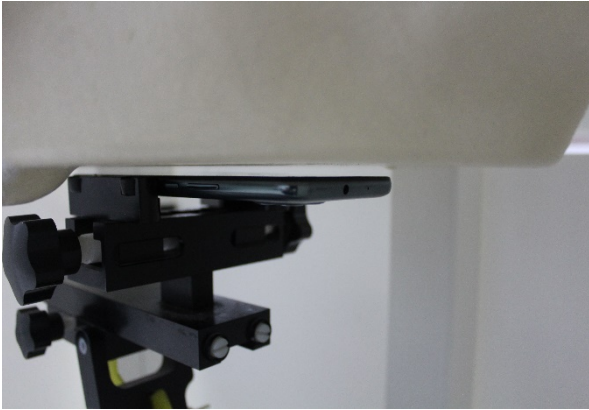

2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Head 1750</p>
	
<p>Photo 3: issue Simulant Liquid for Head 1900</p>	<p>Photo 4: Tissue Simulant Liquid for Head 2450</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2600</p>	<p>Photo 6: Tissue Simulant Liquid for Head 5G</p>
	



3. Photographs of EUT test position

<p>Photo 7: Left cheek</p>	<p>Photo 8: Left tilted</p>
	
<p>Photo 9: Right cheek</p>	<p>Photo 10: Right tilted</p>
	
<p>Photo 11: Front side 5mm</p>	<p>Photo 12: Back side 5mm</p>
	

<p>Photo 13: Left side 5mm</p>	<p>Photo 14: Right side 5mm</p>
	
<p>Photo 15: Top side 5mm</p>	<p>Photo 16: Bottom side 5mm</p>
	
<p>Photo 17: Front side 0mm</p>	<p>Photo 18: Back side 0mm</p>
	

<p>Photo 19: Left side 0mm</p>	<p>Photo 20: Right side 0mm</p>
	
<p>Photo 21: Top side 0mm</p>	<p>Photo 22: Bottom side 0mm</p>
	
<p>Photo 23: Front side 4mm</p>	<p>Photo 24: Front side 10mm</p>
	

<p>Photo 25: Back side 6mm</p>	<p>Photo 26: Back side 17mm</p>
	
<p>Photo 27: Left side 4mm</p>	<p>Photo 28: Left side 7mm</p>
	
<p>Photo 29: Right side 11mm</p>	<p>Photo 30: Bottom side 7mm</p>
	

Photo 31: Bottom side 13mm	Photo 32: Back side with headset 5mm
	

4. EUT Constructional Details

Photo 33: Front View	Photo 34: Back View
