

Calibration Certificate

Certificate number **25-20**

Page 2 of 2

Calibration is performed by using

Model	Model Description	Equipment ID	Cal Due Date	Certificate Number	Trace Value
M 546	Reference power meter	163	24 March 2022	1/111-174-20	RF Power
M 568	Reference power meter	164	24 March 2022	1/111-175-20	RF Power
G4-161	Signal generator	3	10 July 2020	22-19	RF Power
G4-186	Signal generator	5	10 July 2020	23-19	RF Power
V7-34	Universal voltmeter	0067787	27 September 2020	1994-42	DC Voltage
RCH3-72	Frequency meter	931200	13 September 2020	2261-43	Frequency
P6-133	Horn antenna	15005	23 September 2021	2374-43	Gain

Calibration conditions

Temperature: 22.5 °C.
Humidity: 43.0 %.
Pressure: 101.0 kPa.

Calibration results are given in the measurement report # 25-20

#	Parameter	Specifications required	Specifications tested and measured
1	Frequency range	40 – 60 GHz	Corresponds
2	Antenna Gain	22.6* dBi	Corresponds (Table 1)
3	Antenna Factor	41.5 dB/m	Corresponds (Table 1)

* – Expanded uncertainty of measurements 2.5 dB.

The uncertainty evaluation has been performed in accordance with ISO/IEC Guide 98-3:2008 (GUM). The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %. This probability corresponds to a coverage factor of $k=2$ for a normal distribution.

Signature of the person who has performed calibration



/ Engineer

**Calibration Laboratory of
Microwave Measuring Equipment**

Accreditation certificate

No. BY/112 5.0065

Address: 6, P. Brovki str., Minsk

220013, Belarus

Phone/Fax: +375 17 2938496



Technical Manager

July 10, 2020

MEASUREMENT REPORT # 25-20

July 10, 2020

Customer:	SPORTON INTERNATIONAL (SHENZHEN) INC. 1/F, 2/F, Bldg 5, Shiling Industrial Zone, Xinwei Village, Xili, Nanshan Shenzhen, 518055, People's Republic of China
Item calibrated:	Antenna QWH-UPRR00 # 01
Method of calibration:	GOST 20271.1, MK KL 8.2-16
Number of samples:	One
Delivery date of the sample:	09.06.2020
Date of calibration:	From 09.06.2020 to 10.07.2020

MEASUREMENT CONDITIONS

Temperature: 22.5 °C	Humidity: 43 %	Pressure: 101.0 kPa
----------------------	----------------	---------------------

MEASUREMENT EQUIPMENT

Model	Model Description	Equipment ID	Cal Due Date	Certificate Number	Trace Value
M 546	Reference power meter	163	24 March 2022	1/111-174-20	RF Power
M 568	Reference power meter	164	24 March 2022	1/111-175-20	RF Power
G4-161	Signal generator	3	10 July 2020	22-19	RF Power
G4-186	Signal generator	5	10 July 2020	23-19	RF Power
V7-34	Universal voltmeter	0067787	27 September 2020	1994-42	DC Voltage
RCH3-72	Frequency meter	931200	13 September 2020	2261-43	Frequency
P6-133	Horn antenna	15005	23 September 2021	2374-43	Gain

MEASUREMENT RESULTS

Distance between tested and generating antenna 2 m.


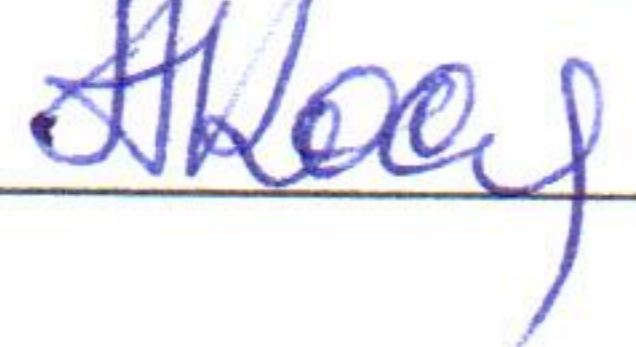
Table 1

Frequency, GHz	40	50	60
Power density of electromagnetic field, W/m ²	0.049	0.067	0.072
Maximum level of measured power, dBm	-14.7	-14.4	-15.2
Gain, dBi	21.9	22.7	23.3
Expanded uncertainty, dB	2.5	2.5	2.5
Antenna Factor, dB/m	40.4	41.5	42.5

The uncertainty evaluation has been performed in accordance with ISO/IEC Guide 98-3:2008 (GUM). The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %. This probability corresponds to a coverage factor of $k=2$ for a normal distribution.

Engineer

Quality Manager

This measurement report issued in duplicate and sent to:

1. SPORTON INTERNATIONAL (SHENZHEN) INC. 1/F, 2/F, Bldg 5, Shiling Industrial Zone, Xinwei Village, Xili, Nanshan Shenzhen, 518055, People's Republic of China

2. Calibration Laboratory of Microwave Measuring Equipment

Duplication of Measurement report (complete or partial) must be authorized by the laboratory.

Calibration Laboratory of Microwave Measuring Equipment
of MWMLab



ISO 17025
ACCREDITED LABORATORY

Calibration certificate



Accreditation certificate No. № BY/112 5.0065 of 09.01.2015

Certificate number 29-20 Date when calibrated 10.07.20 Page 1 of 2

Item calibrated Antenna QWH-VPRR00 # 1002000003

Customer SPORTON INTERNATIONAL (SHENZHEN) INC.
1/F, 2/F, Bldg 5, Shiling Industrial Zone, Xinwei Village, Xili, Nanshan
Shenzhen, 518055, People's Republic of China

Method of calibration GOST 20271.1, MK KL 8.2-16

All measurements are traceable to the SI units which are realized by national measurement standards of NMI and state standards of RF. Conversion loss measurements above 178 GHz are to confirm operation functionality and traceable only to MWMLab standards and OML. This certificate shall not be reproduced, except in full. Any publication extracts from the calibration certificate requires written permission of the issuing calibration laboratory of microwave measuring equipment.

Authorising
signature



/ Technical manager Date of issue 10.07.20

Calibration Certificate

Certificate number **29-20**

Page 2 of 2

Calibration is performed by using

Model	Model Description	Equipment ID	Cal Due Date	Certificate Number	Trace Value
M 546	Reference power meter	163	24 March 2022	1/111-175-20	RF Power
M 568	Reference power meter	164	24 March 2022	1/111-175-20	RF Power
G4-186	Signal generator	5	10 July 2020	23-19	RF Power
G4-161	Signal generator	3	10 July 2020	22-19	RF Power
V7-34	Universal voltmeter	0067787	27 September 2020	1994-42	DC Voltage
RCH3-72	Frequency meter	931200	13 September 2020	2261-43	Frequency
P6-134	Measuring horn antenna	14002	23 September 2021	2372-43	Gain

Calibration conditions

Temperature: 22.5 °C.
Humidity: 43.0 %.
Pressure: 101.0 kPa.

Calibration results are given in the measurement report # 29-20

#	Parameter	Specifications required	Specifications tested and measured
1	Frequency range	50 – 75 GHz	Corresponds
2	Antenna Gain	22.6* dBi	Corresponds (Table 1)
3	Antenna Factor	43.0 dB/m	Corresponds (Table 1)

* – Expanded uncertainty of measurements 2.5 dB.

The uncertainty evaluation has been performed in accordance with ISO/IEC Guide 98-3:2008 (GUM). The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %. This probability corresponds to a coverage factor of $k=2$ for a normal distribution.

Signature of the person who has performed calibration



/ Engineer

**Calibration Laboratory of
Microwave Measuring Equipment**
Accreditation certificate
No. BY/112 5.0065
Address: 6, P. Brovki str., Minsk
220013, Belarus
Phone/Fax: +375 17 2938496



Technical Manager

July 10, 2020

MEASUREMENT REPORT # 29-20

July 10, 2020

Customer:	SPORTON INTERNATIONAL (SHENZHEN) INC. 1/F, 2/F, Bldg 5, Shiling Industrial Zone, Xinwei Village, Xili, Nanshan Shenzhen, 518055, People's Republic of China
Item calibrated:	Antenna QWH-VPRR00 # 1002000003
Method of calibration:	GOST 20271.1, MK KL 8.2-16
Number of samples:	One
Delivery date of the sample:	09.06.2020
Date of calibration:	From 09.06.2020 to 10.07.2020

MEASUREMENT CONDITIONS

Temperature: 22.5 °C	Humidity: 43 %	Pressure: 101.0 kPa
----------------------	----------------	---------------------

MEASUREMENT EQUIPMENT

Model	Model Description	Equipment ID	Cal Due Date	Certificate Number	Trace Value
M 546	Reference power meter	163	24 March 2022	1/111-175-20	RF Power
M 568	Reference power meter	164	24 March 2022	1/111-175-20	RF Power
G4-186	Signal generator	5	10 July 2020	23-19	RF Power
G4-161	Signal generator	3	10 July 2020	22-19	RF Power
V7-34	Universal voltmeter	0067787	27 September 2020	1994-42	DC Voltage
RCH3-72	Frequency meter	931200	13 September 2020	2261-43	Frequency
P6-134	Measuring horn antenna	14002	23 September 2021	2372-43	Gain

MEASUREMENT RESULTS

Distance between tested and generating antenna 1.8 m.


Table 1

Frequency, GHz	50	62.5	75
Power density of electromagnetic field, W/m ²	0.048	0.067	0.081
Maximum level of measured power, dBm	-16.7	-16.4	-16.9
Gain, dBi	21.9	22.7	23.0
Expanded uncertainty, dB	2.2	2.2	2.2
Antenna Factor, dB/m	42.3	43.5	44.7

The uncertainty evaluation has been performed in accordance with ISO/IEC Guide 98-3:2008 (GUM). The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %. This probability corresponds to a coverage factor of $k=2$ for a normal distribution.

Engineer

Quality Manager

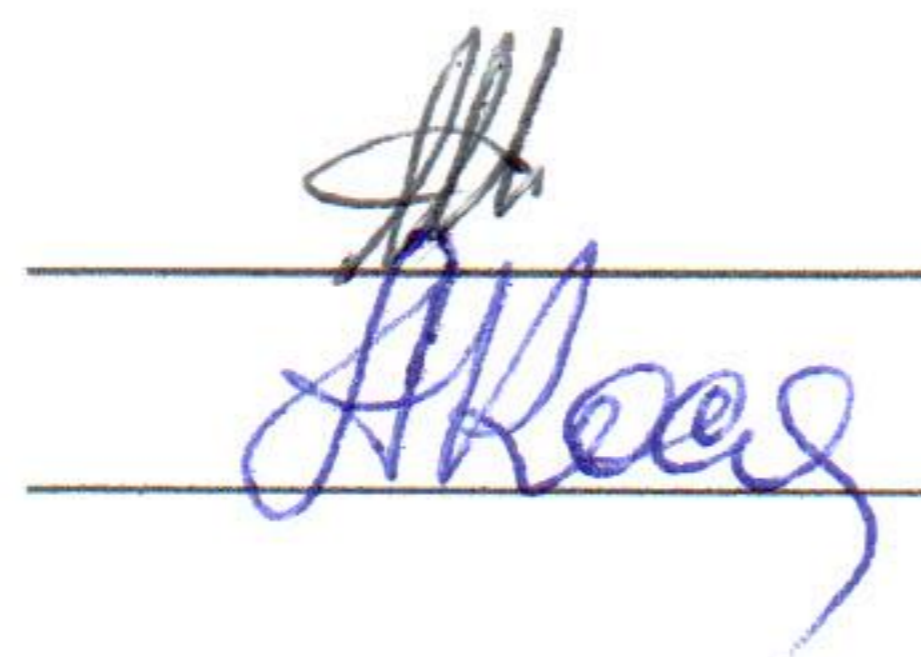

This measurement report issued in duplicate and sent to:

1. SPORTON INTERNATIONAL (SHENZHEN) INC. 1/F, 2/F, Bldg 5, Shiling Industrial Zone, Xinwei Village, Xili, Nanshan Shenzhen, 518055, People's Republic of China

2. Calibration Laboratory of Microwave Measuring Equipment

Duplication of Measurement report (complete or partial) must be authorized by the laboratory.

Calibration Laboratory of Microwave Measuring Equipment
of MWMLab



Calibration certificate

ISO 17025
ACCREDITED LABORATORY



Accreditation certificate No. № BY/112 5.0065 of 09.01.2015

Certificate number 31-20 Date when calibrated 10.07.20 Page 1 of 2

Item calibrated Antenna QWH-EPRR00 # 1012700010

Customer SPORTON INTERNATIONAL (SHENZHEN) INC.
1/F, 2/F, Bldg 5, Shiling Industrial Zone, Xinwei Village, Xili, Nanshan
Shenzhen, 518055, People's Republic of China

Method of calibration GOST 20271.1, MK KL 8.2-16

All measurements are traceable to the SI units which are realized by national measurement standards of NMI and state standards of RF. Conversion loss measurements above 178 GHz are to confirm operation functionality and traceable only to MWMLab standards and OML. This certificate shall not be reproduced, except in full. Any publication extracts from the calibration certificate requires written permission of the issuing calibration laboratory of microwave measuring equipment.

Authorising
signature



/ Technical manager Date of issue 10.07.20

Calibration Certificate

Certificate number **31-20**

Page 2 of 2

Calibration is performed by using

Model	Model Description	Equipment ID	Cal Due Date	Certificate Number	Trace Value
M 546	Reference power meter	163	24 March 2022	1/111-175-20	RF Power
M 534	Reference power meter	161	24 March 2022	1/111-173-20	RF Power
G4-186	Signal generator	5	10 July 2020	23-19	RF Power
RG4-14	Signal generator	22	10 July 2020	24-19	RF Power
V7-34	Universal voltmeter	0067787	27 September 2020	1994-42	DC Voltage
RCH3-72	Frequency meter	931200	13 September 2020	2261-43	Frequency
P6-134	Measuring horn antenna	14002	23 September 2021	2372-43	Gain
P6-31A	Measuring horn antenna	35864	23 September 2021	2368-43	Gain

Calibration conditions

Temperature: 22.5 °C.
Humidity: 43.0 %.
Pressure: 101.0 kPa.


Calibration results are given in the measurement report # 31-20

#	Parameter	Specifications required	Specifications tested and measured
1	Frequency range	60 – 90 GHz	Corresponds
2	Antenna Gain	22.6* dBi	Corresponds (Table 1)
3	Antenna Factor	45.0 dB/m	Corresponds (Table 1)

* – Expanded uncertainty of measurements 2.5 dB.

The uncertainty evaluation has been performed in accordance with ISO/IEC Guide 98-3:2008 (GUM). The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %. This probability corresponds to a coverage factor of $k=2$ for a normal distribution.

Signature of the person who has performed calibration



/ Engineer

**Calibration Laboratory of
Microwave Measuring Equipment**
Accreditation certificate
No. BY/112 5.0065
Address: 6, P. Brovki str., Minsk
220013, Belarus
Phone/Fax: +375 17 2938496



MEASUREMENT REPORT # 31-20
July 10, 2020

Customer:	SPORTON INTERNATIONAL (SHENZHEN) INC. 1/F, 2/F, Bldg 5, Shiling Industrial Zone, Xinwei Village, Xili, Nanshan Shenzhen, 518055, People's Republic of China
Item calibrated:	Antenna QWH-EPRR00 # 1012700010
Method of calibration:	GOST 20271.1, MK KL 8.2-16
Number of samples:	One
Delivery date of the sample:	09.06.2020
Date of calibration:	From 09.06.2020 to 10.07.2020