

1) The device is set to operate at a defined level. During test, continuous transmit is forced by means of applicant supplied software. All tests are done using this software, so including power measurements, power drift measurements and the measurements of spot SAR drift during SAR evaluation. Should the device not transmit at max power, one or more of the drift or power measurements would have revealed that.

EMC report lists max transmit peak power as per 47 CFR § 15.247 and § 15 subpart E. A description of the measurement procedure for 15.247 is annexed. Please note that no Spectrum Analyzer is involved. For 15.407, the measurement is in accordance with FCC Public Notice DA 02-2138 (August 30, 2002), Appendix A, peak conducted transmit output power, test method #3. Plots of the measurements are included in the test report as per the above referenced Public Notice. Video BW and RBW are given in the plots in the test report. SAR report lists average conducted power measured at the antenna terminal, or the sum of this power and antenna gain whichever is higher. Measurement is done with a broadband power sensor, in this case a HP 8184A. Explanation applies for both 2.4 and 5 GHz.

2) In general, Probe linearity is proven in the calibration report of the probe, which is annexed to the SAR report. The probe is checked as part of the probe calibration for values of up to 100 W/kg. In addition we did a full 3d scan using the system validation power feed setup as per the P1528 system validation. The source was modulated OFDM 6 Mbit/s. Using body liquid psaSAR measured is 4.52 W/kg (1g). When changing to unmodulated source, and leaving everything in place, the psaSAR measured was 4.705 W/kg (1g), a difference of 4% or 0.17 dB. The measurements were performed with body liquid, at the waveguide frequency: 5740 MHz. Earlier the system validation showed 36.6 W/kg (1g), where the reference (as per Ghani, see SAR report) is 39.46 W/kg (1g), which is off 7.8%. We believe we have sufficiently shown that the probe's response to modulated signals is valid. Note: All measurements are performed May 12, 2004.

3) Liquids were within accordance of P1528 and other guidelines within 10% of targets. Assuming your question is targeted at using target values rather than measured values in consecutive processing: Other liquid values to be used in calculations can be reasonably accurate corrected with a first order approximation. However, in our opinion target values should be used in order to prevent unnecessary propagation of uncertainties: Although field strengths are measured in a liquid with deviation from target (albeit within 10%), the target value should be used in consecutive calculations to predict psaSAR as accurately as possible.

4) Liquids recipes are propriety. In SAR report p 14. Specs are according P1528 (see tables in SAR report). Bristol university claims to be within 3.5% for all properties.

.All Tissue Equivalent Liquids are obtained from Bristol University.

Contact details:

Medical Physics Department

University of Bristol, Bristol Haemotology & Oncology Centre

Horfield road, Bristol BS2 8 ED, United Kingdom

Tel. 44 117 928 2469.

5) SAR plots entire device

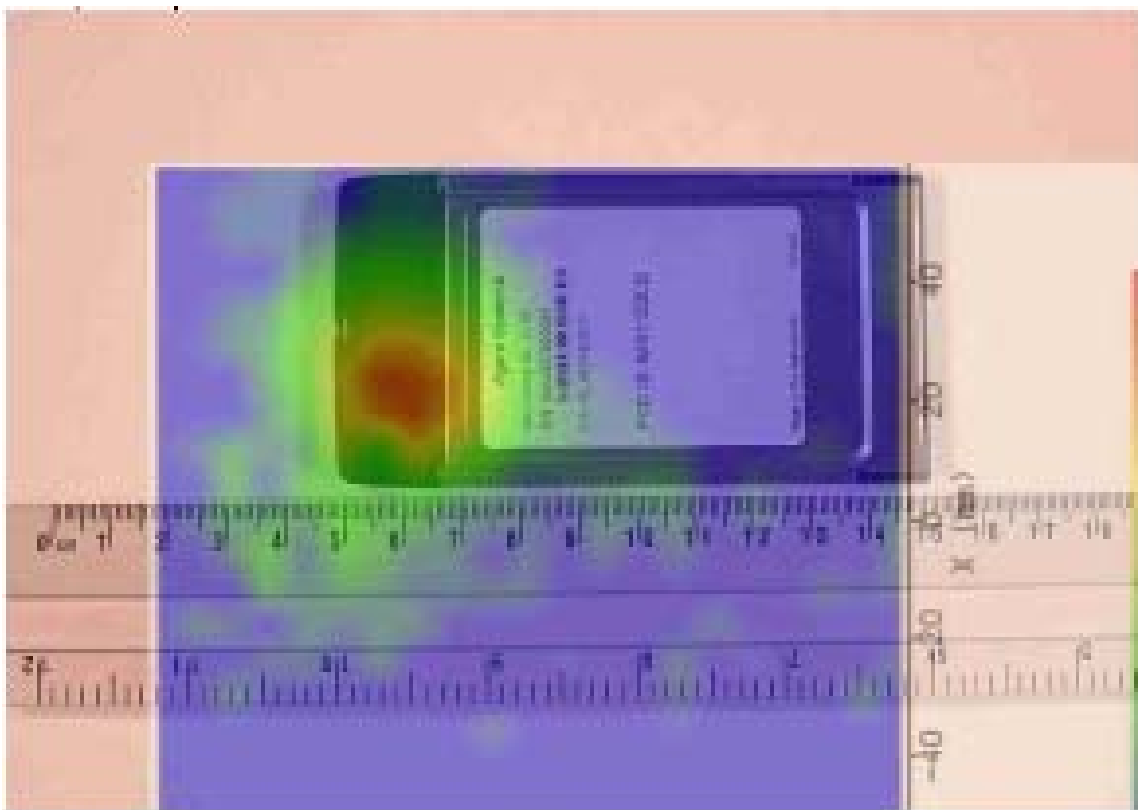


Figure 1: 5 GHz contour plot entire device

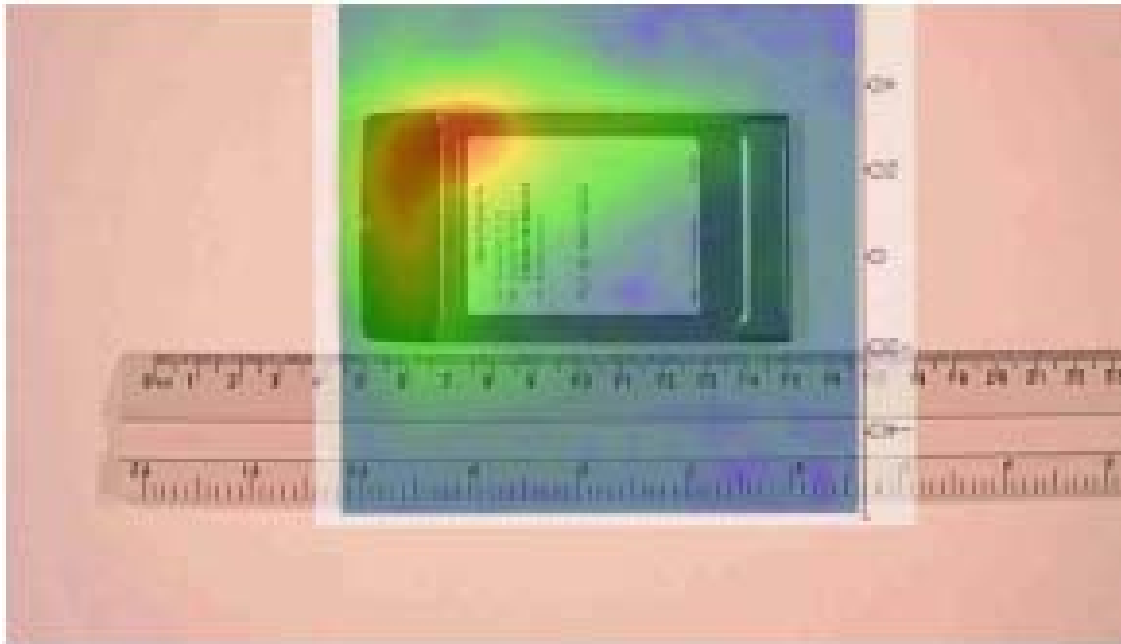


Figure 2. 2437 MHz contour plot entire device

6) Contour plots:

Please find below the missing plots

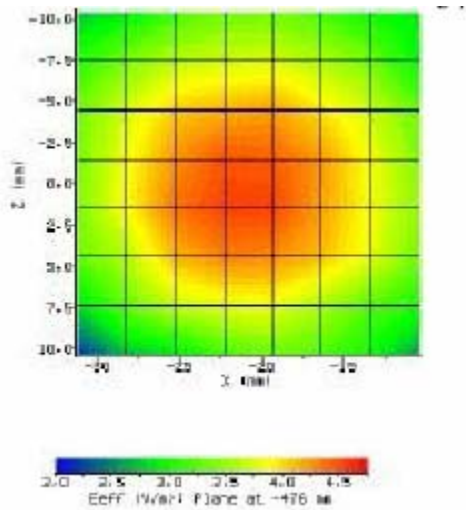


Figure 3 channel 149 lapheld

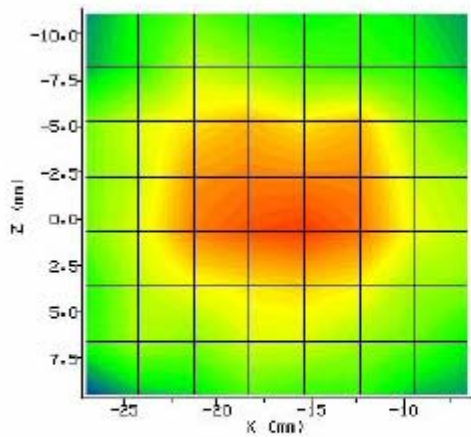


Figure 5: lapheld ch 164


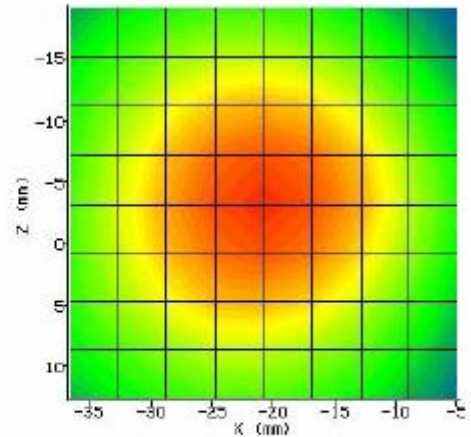


Figure 4: perpendiculat ch 6