

|                                                                                  |                                                    |                                                           |                                                           |                                                                                                                        |
|----------------------------------------------------------------------------------|----------------------------------------------------|-----------------------------------------------------------|-----------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------|
|  | <u>Date(s) of Evaluation</u><br>September 19, 2014 | <u>Test Report Serial No.</u><br>091614IPH-1307-SNA       | <u>Test Report Revision No.</u><br>Rev. 1.3 (3rd Release) | <br>Test Lab Certificate No. 2470.01 |
|                                                                                  | <u>Test Report Issue Date</u><br>December 17, 2014 | <u>Description of Test(s)</u><br>Specific Absorption Rate | <u>RF Exposure Category</u><br>Gen. Pop. / Uncontrolled   |                                                                                                                        |

## APPENDIX E - DIPOLE CALIBRATION

|                         |                                                                                                                      |                  |                                       |            |                    |                                                                                       |
|-------------------------|----------------------------------------------------------------------------------------------------------------------|------------------|---------------------------------------|------------|--------------------|---------------------------------------------------------------------------------------|
| <b>Applicant:</b>       | <b>Garmin International Inc.</b>                                                                                     | <b>FCC ID:</b>   | <b>IPH-02257</b>                      | <b>IC:</b> | <b>1792A-02257</b> |  |
| <b>Model:</b>           | <b>A02257</b>                                                                                                        | <b>DUT Type:</b> | <b>Wireless Extremity-Worn Device</b> |            |                    |                                                                                       |
| 2014 Celltech Labs Inc. | This document is not to be reproduced in whole or in part without the prior written permission of Celltech Labs Inc. |                  |                                       |            |                    | Page 32 of 34                                                                         |



|                                                                                  |                                      |                                 |                                                                                                                        |
|----------------------------------------------------------------------------------|--------------------------------------|---------------------------------|------------------------------------------------------------------------------------------------------------------------|
|  | <u>Date:</u><br>June 15, 2014        | <u>Revision No.</u><br>Rev. 1.3 | <br>Test Lab Certificate No. 2470.01 |
|                                                                                  | 2450 MHz Dipole Extended Calibration |                                 |                                                                                                                        |

Dipole: D2450V2  
Serial Number: 825  
Last Calibrated: Apr. 25, 2012


| Antenna Parameters with Head TSL     |                          |                       |                                  |                       |                     |                       |
|--------------------------------------|--------------------------|-----------------------|----------------------------------|-----------------------|---------------------|-----------------------|
|                                      | Impedance<br>Real (ohms) | Deviation<br>from cal | Impedance<br>Imaginary<br>(ohms) | Deviation<br>from cal | Return Loss<br>(dB) | Deviation<br>from Cal |
| <b>Last Calibration</b>              | 53.0                     | -                     | +5.5                             | -                     | -24.3               | -                     |
| <b>Extended Cal<br/>Jul 10, 2013</b> | 53.0                     | 0                     | +7.5                             | 2.0                   | -22.3               | 8.2%                  |
| <b>Extended Cal<br/>Jun 12, 2014</b> | 53.4                     | 0.4                   | +6.3                             | 0.8                   | -23.2               | -4.5%                 |

| Antenna Parameters with Body TSL      |                          |                                 |                                  |                                 |                     |                              |
|---------------------------------------|--------------------------|---------------------------------|----------------------------------|---------------------------------|---------------------|------------------------------|
|                                       | Impedance<br>Real (ohms) | Deviation<br>from cal<br>(ohms) | Impedance<br>Imaginary<br>(ohms) | Deviation<br>from cal<br>(ohms) | Return Loss<br>(dB) | Deviation<br>from Cal<br>(%) |
| <b>Last Calibration</b>               | 50.4                     | -                               | +6.1                             | -                               | -24.3               | -                            |
| <b>Extended Cal<br/>Jun 17, 2013</b>  | 49.0                     | 1.4                             | +7.9                             | 1.8                             | -21.3               | 12.3%                        |
| <b>Extended Cal<br/>June 15, 2014</b> | 50.4                     | 0.0                             | +4.8                             | 1.3                             | -26.2               | 7.8%                         |



## Antenna VSWR with Head TSL

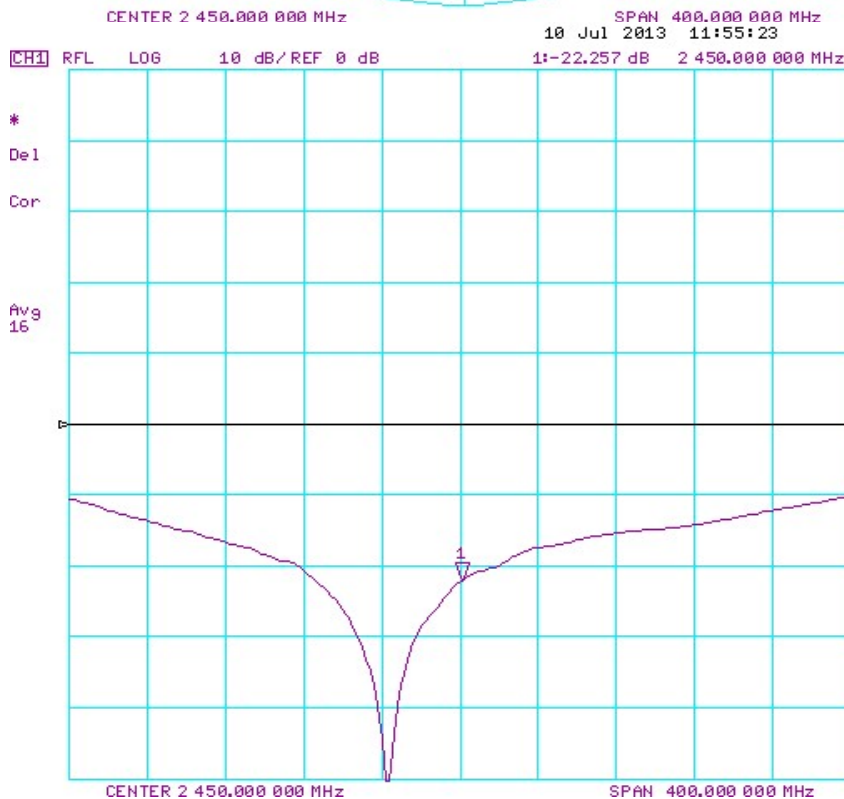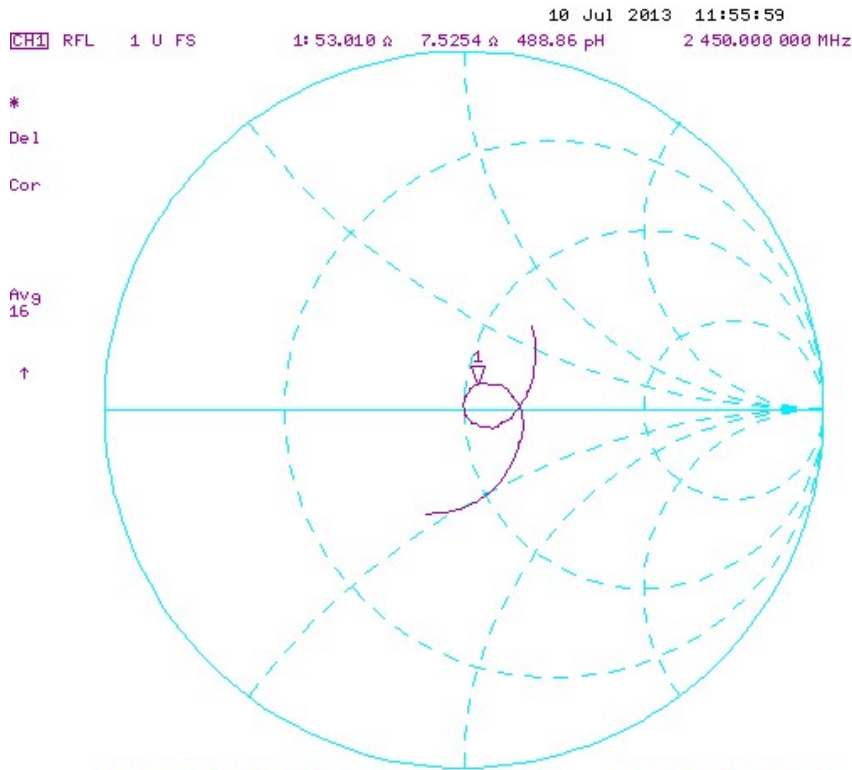

## Antenna VSWR with Body TSL

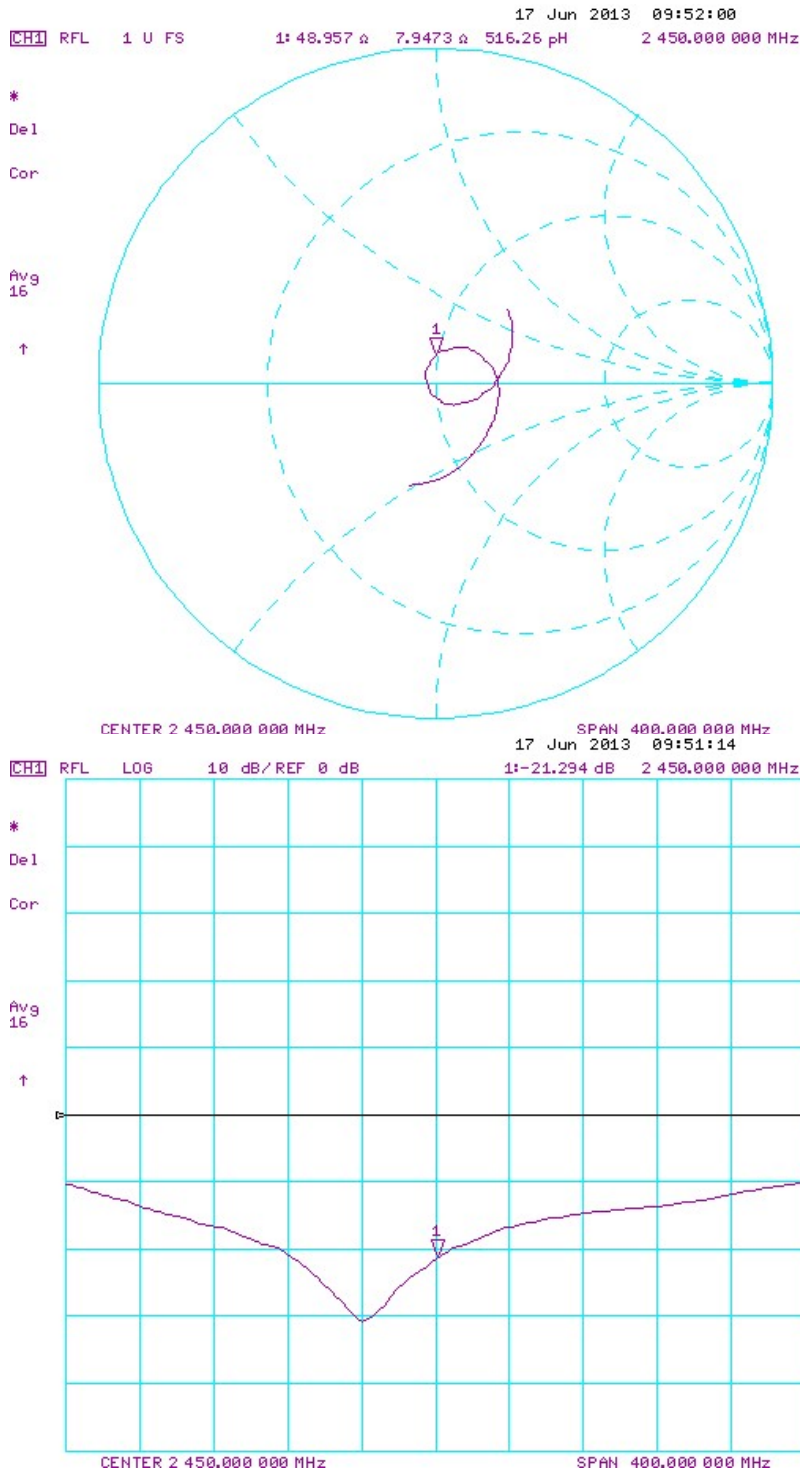


## Antenna VSWR with Head TSL

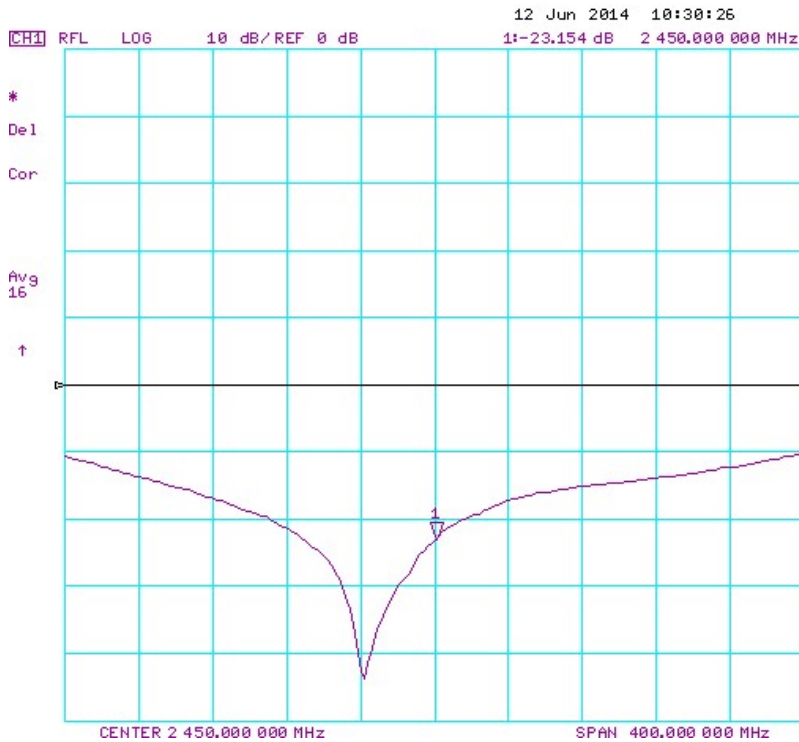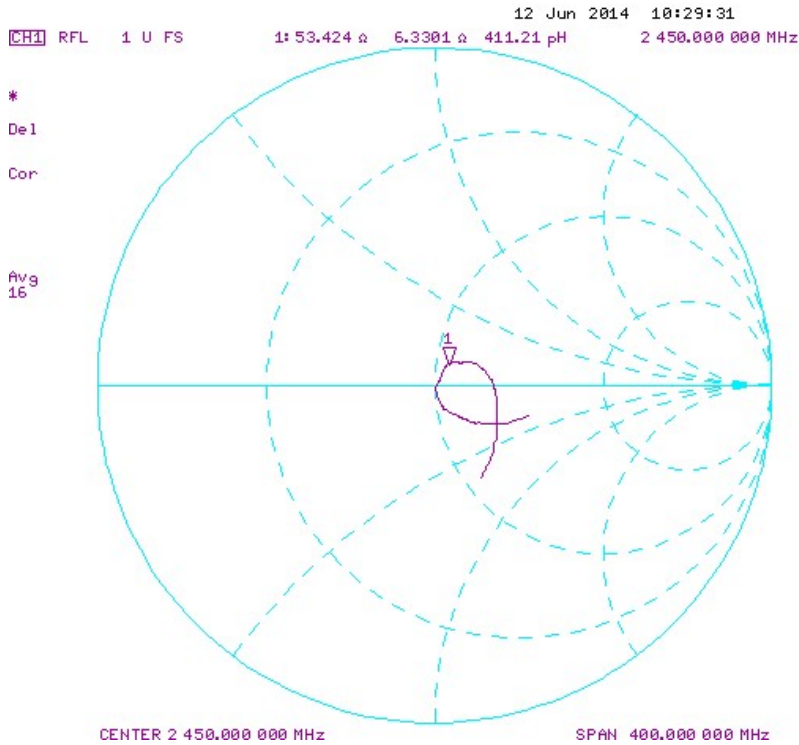

**2450 MHz Dipole Extended Calibration**

15 Jun 2014 09:26:30  
CH1 S11 1 U FS 1: 50.451  $\Omega$  4.8457  $\Omega$  314.78  $\mu\text{H}$  2 450.000 000 MHz


\*  
Del  
Cor  
Avg  
16  
↑

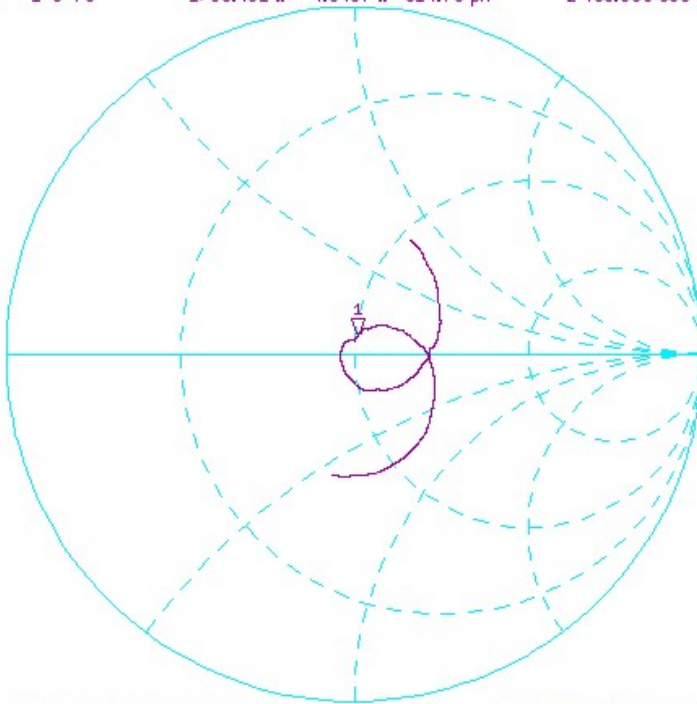

CENTER 2 450.000 000 MHz SPAN 400.000 000 MHz

15 Jun 2014 09:27:05  
CH1 S11 LOG 10 dB/REF 0 dB 1: -26.160 dB 2 450.000 000 MHz

\*  
Del  
Cor  
Avg  
14  
↑

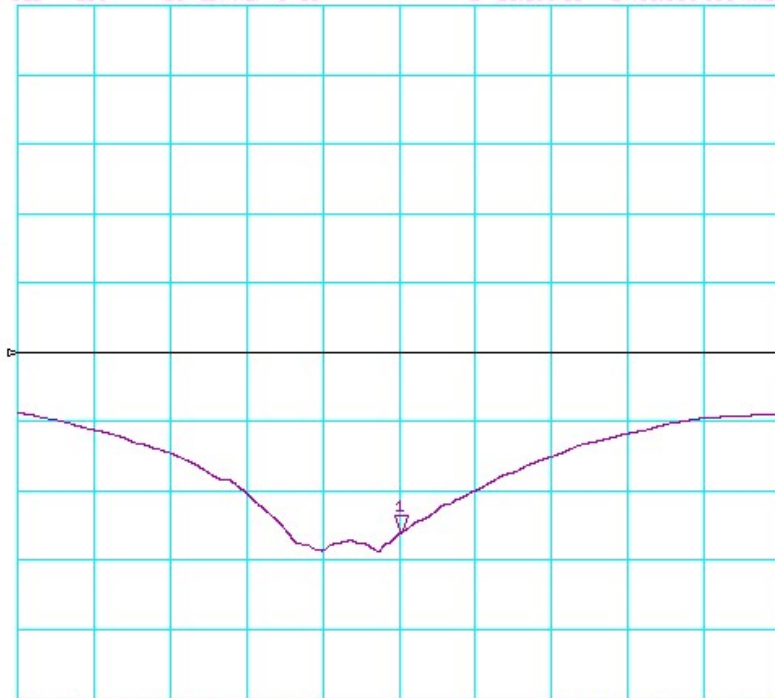

CENTER 2 450.000 000 MHz SPAN 400.000 000 MHz



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Celltech**

Certificate No: **D2450V2-825\_Apr12**

## CALIBRATION CERTIFICATE

Object **D2450V2 - SN: 825**

Calibration procedure(s) **QA CAL-05.v8**  
**Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **April 25, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704         | 05-Oct-11 (No. 217-01451)         | Oct-12                 |
| Power sensor HP 8481A       | US37292783         | 05-Oct-11 (No. 217-01451)         | Oct-12                 |
| Reference 20 dB Attenuator  | SN: 5058 (20k)     | 27-Mar-12 (No. 217-01530)         | Apr-13                 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 27-Mar-12 (No. 217-01533)         | Apr-13                 |
| Reference Probe ES3DV3      | SN: 3205           | 30-Dec-11 (No. ES3-3205_Dec11)    | Dec-12                 |
| DAE4                        | SN: 601            | 04-Jul-11 (No. DAE4-601_Jul11)    | Jul-12                 |
| Secondary Standards         | ID #               | Check Date (in house)             | Scheduled Check        |
| Power sensor HP 8481A       | MY41092317         | 18-Oct-02 (in house check Oct-11) | In house check: Oct-13 |
| RF generator R&S SMT-06     | 100005             | 04-Aug-99 (in house check Oct-11) | In house check: Oct-13 |
| Network Analyzer HP 8753E   | US37390585 S4206   | 18-Oct-01 (in house check Oct-11) | In house check: Oct-12 |

|                |                |                       |           |
|----------------|----------------|-----------------------|-----------|
|                | Name           | Function              | Signature |
| Calibrated by: | Jeton Kastrati | Laboratory Technician |           |
| Approved by:   | Katja Pokovic  | Technical Manager     |           |

Issued: April 25, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

### Glossary:

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

### Additional Documentation:

- DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                        |             |
|------------------------------|------------------------|-------------|
| DASY Version                 | DASY5                  | V52.8.1     |
| Extrapolation                | Advanced Extrapolation |             |
| Phantom                      | Modular Flat Phantom   |             |
| Distance Dipole Center - TSL | 10 mm                  | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm      |             |
| Frequency                    | 2450 MHz $\pm$ 1 MHz   |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters             | 22.0 °C             | 39.2           | 1.80 mho/m           |
| Measured Head TSL parameters            | (22.0 $\pm$ 0.2) °C | 39.6 $\pm$ 6 % | 1.81 mho/m $\pm$ 6 % |
| Head TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Head TSL

|                                                       |                    |                                |
|-------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                                |
| SAR measured                                          | 250 mW input power | 12.7 mW / g                    |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 50.8 mW / g $\pm$ 17.0 % (k=2) |

|                                                         |                    |                                |
|---------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                                |
| SAR measured                                            | 250 mW input power | 5.90 mW / g                    |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 23.6 mW / g $\pm$ 16.5 % (k=2) |

## Body TSL parameters

The following parameters and calculations were applied.

|                                         | Temperature         | Permittivity   | Conductivity         |
|-----------------------------------------|---------------------|----------------|----------------------|
| Nominal Body TSL parameters             | 22.0 °C             | 52.7           | 1.95 mho/m           |
| Measured Body TSL parameters            | (22.0 $\pm$ 0.2) °C | 52.4 $\pm$ 6 % | 1.98 mho/m $\pm$ 6 % |
| Body TSL temperature change during test | < 0.5 °C            | ----           | ----                 |

## SAR result with Body TSL

|                                                       |                    |                                |
|-------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL | Condition          |                                |
| SAR measured                                          | 250 mW input power | 12.7 mW / g                    |
| SAR for nominal Body TSL parameters                   | normalized to 1W   | 50.4 mW / g $\pm$ 17.0 % (k=2) |

|                                                         |                    |                                |
|---------------------------------------------------------|--------------------|--------------------------------|
| SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL | condition          |                                |
| SAR measured                                            | 250 mW input power | 5.91 mW / g                    |
| SAR for nominal Body TSL parameters                     | normalized to 1W   | 23.5 mW / g $\pm$ 16.5 % (k=2) |

## Appendix

### Antenna Parameters with Head TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 53.0 $\Omega$ + 5.5 j $\Omega$ |
| Return Loss                          | - 24.3 dB                      |

### Antenna Parameters with Body TSL

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 50.4 $\Omega$ + 6.1 j $\Omega$ |
| Return Loss                          | - 24.3 dB                      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.159 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

|                 |                   |
|-----------------|-------------------|
| Manufactured by | SPEAG             |
| Manufactured on | December 11, 2008 |

## DASY5 Validation Report for Head TSL

Date: 25.04.2012

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 825**

Communication System: CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.81$  mho/m;  $\epsilon_r = 39.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.45, 4.45, 4.45); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 99.271 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 26.216 mW/g


**SAR(1 g) = 12.7 mW/g; SAR(10 g) = 5.9 mW/g**

Maximum value of SAR (measured) = 16.5 mW/g

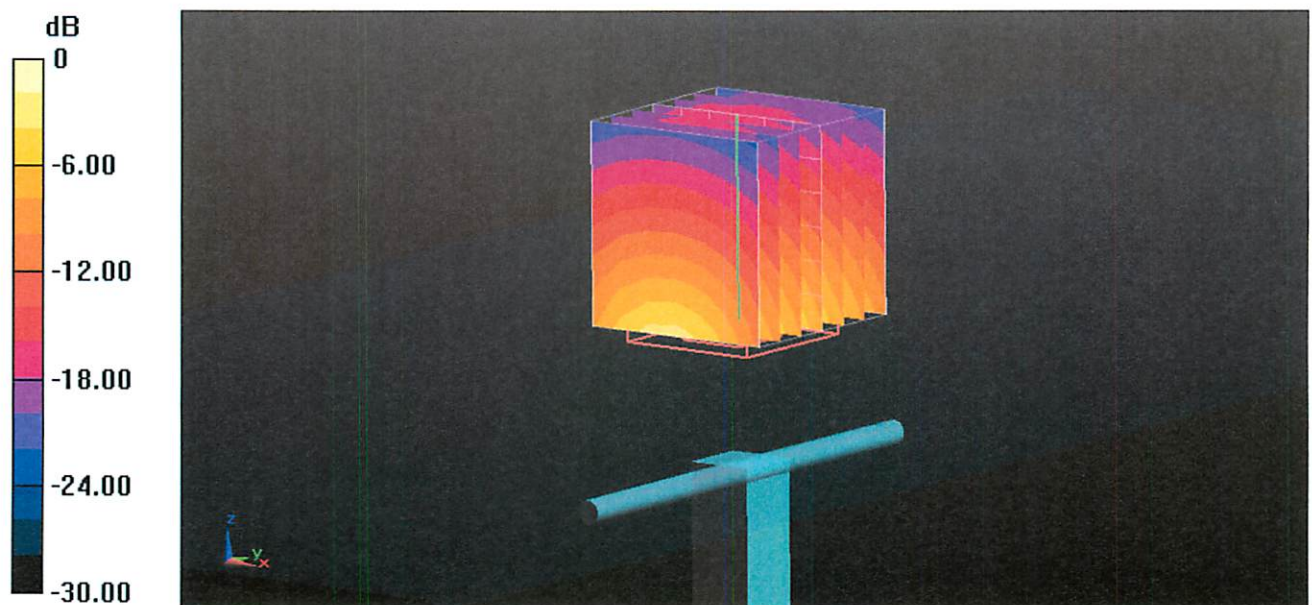

0 dB = 16.5 mW/g = 24.35 dB mW/g

## Impedance Measurement Plot for Head TSL

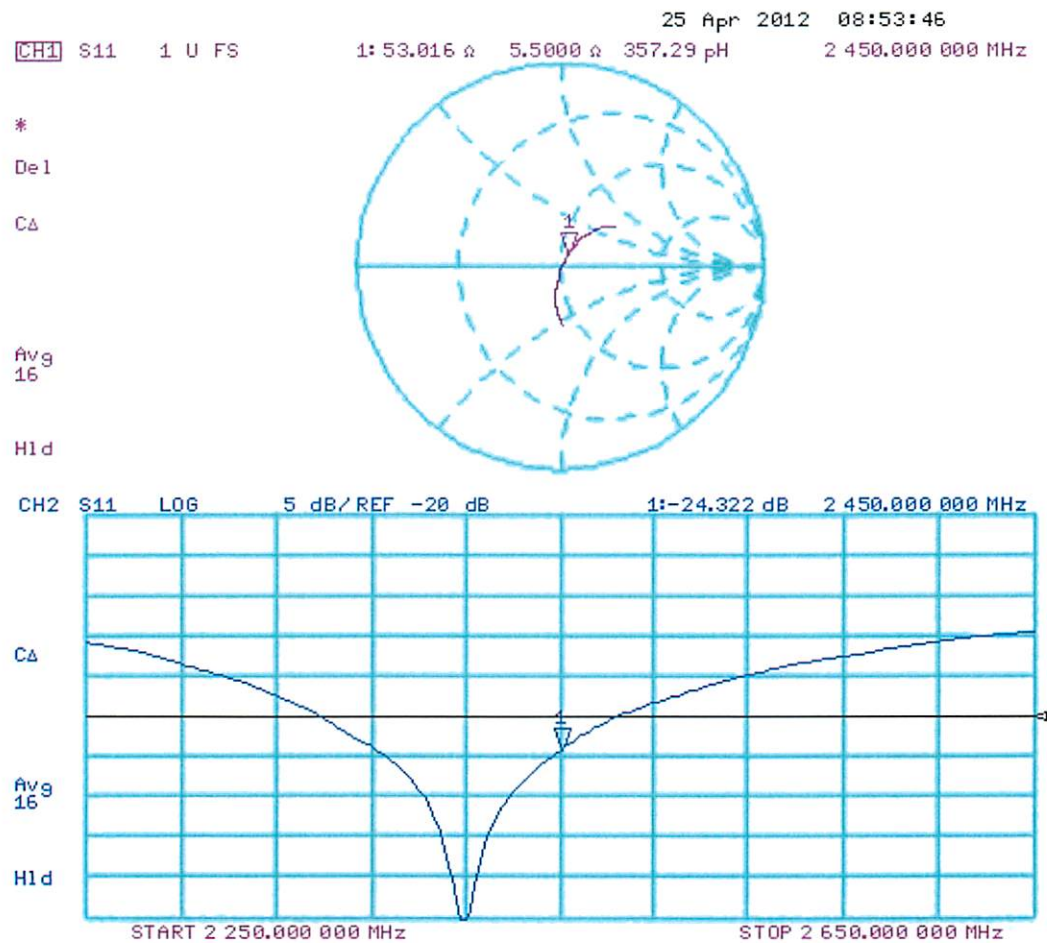

## DASY5 Validation Report for Body TSL

Date: 25.04.2012

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 825**

Communication System: CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.98$  mho/m;  $\epsilon_r = 52.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.26, 4.26, 4.26); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

**Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.157 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 25.807 mW/g


**SAR(1 g) = 12.7 mW/g; SAR(10 g) = 5.91 mW/g**

Maximum value of SAR (measured) = 16.7 mW/g

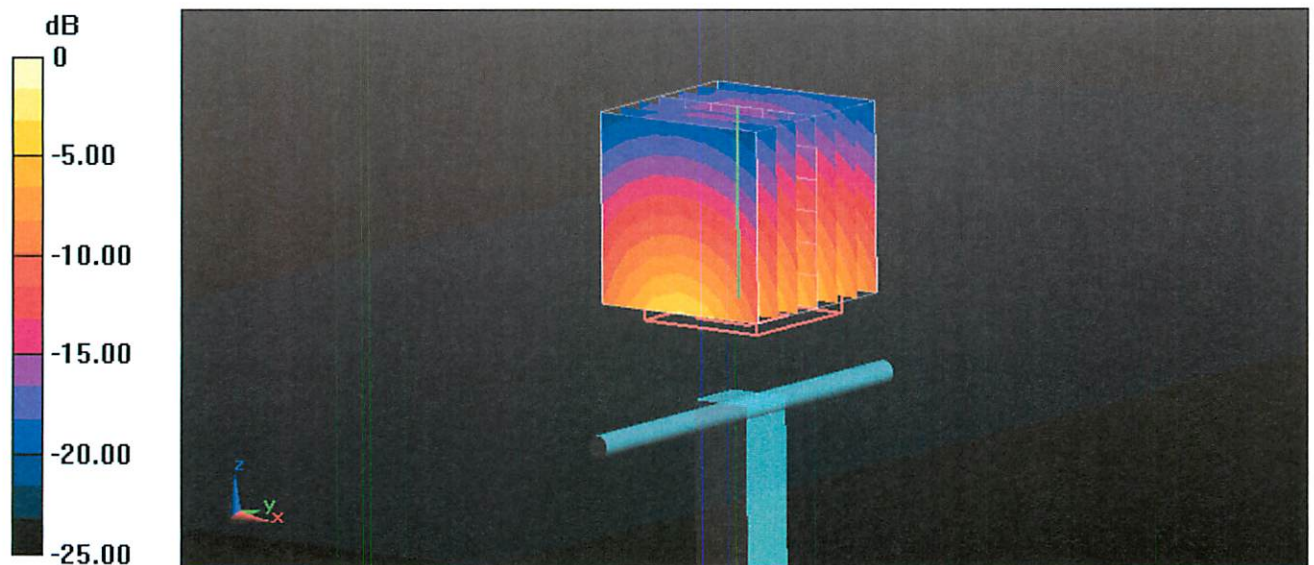

0 dB = 16.7 mW/g = 24.45 dB mW/g

## Impedance Measurement Plot for Body TSL

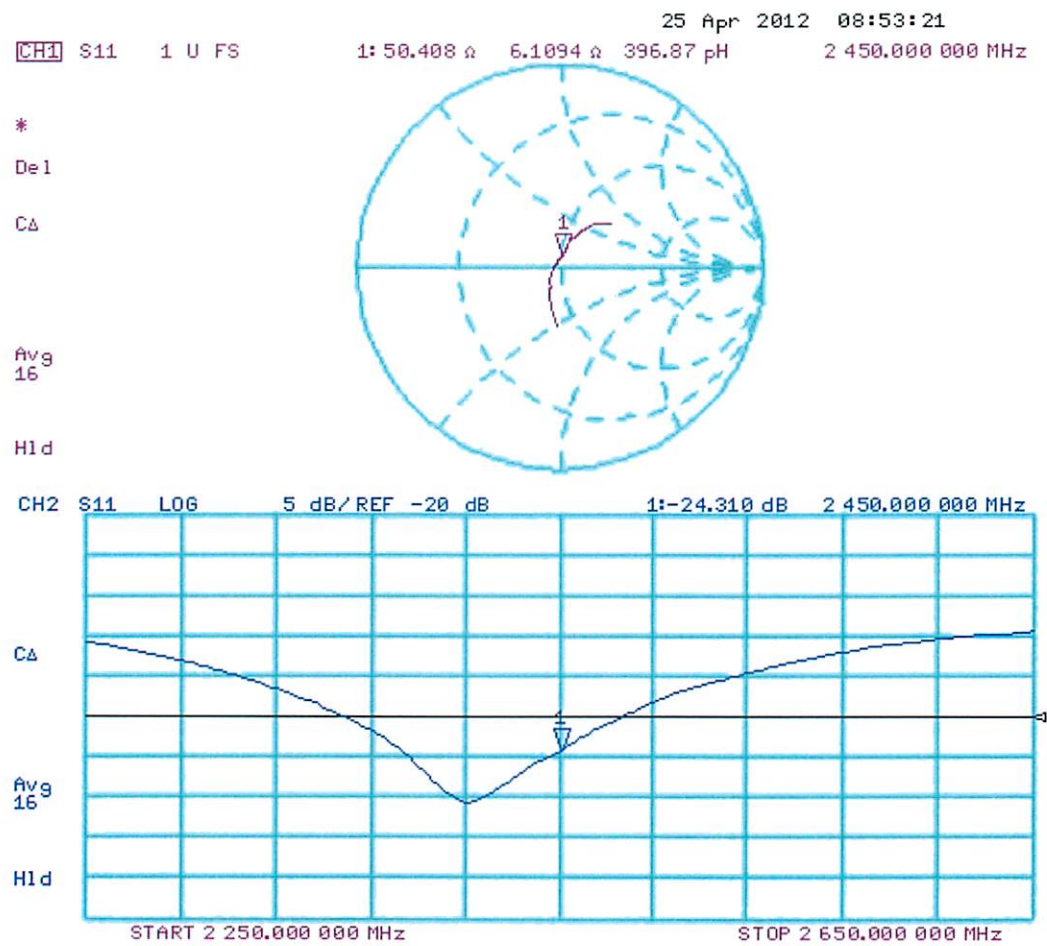

|                                                                                  |                                                    |                                                           |                                                           |                                                                                                                        |
|----------------------------------------------------------------------------------|----------------------------------------------------|-----------------------------------------------------------|-----------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------|
|  | <u>Date(s) of Evaluation</u><br>September 19, 2014 | <u>Test Report Serial No.</u><br>091614IPH-1307-SNA       | <u>Test Report Revision No.</u><br>Rev. 1.3 (3rd Release) | <br>Test Lab Certificate No. 2470.01 |
|                                                                                  | <u>Test Report Issue Date</u><br>December 17, 2014 | <u>Description of Test(s)</u><br>Specific Absorption Rate | <u>RF Exposure Category</u><br>Gen. Pop. / Uncontrolled   |                                                                                                                        |

## APPENDIX F - PROBE CALIBRATION

|                         |                                                                                                                      |                  |                                       |            |                    |                                                                                       |
|-------------------------|----------------------------------------------------------------------------------------------------------------------|------------------|---------------------------------------|------------|--------------------|---------------------------------------------------------------------------------------|
| <b>Applicant:</b>       | <b>Garmin International Inc.</b>                                                                                     | <b>FCC ID:</b>   | <b>IPH-02257</b>                      | <b>IC:</b> | <b>1792A-02257</b> |  |
| <b>Model:</b>           | <b>A02257</b>                                                                                                        | <b>DUT Type:</b> | <b>Wireless Extremity-Worn Device</b> |            |                    |                                                                                       |
| 2014 Celltech Labs Inc. | This document is not to be reproduced in whole or in part without the prior written permission of Celltech Labs Inc. |                  |                                       |            |                    | Page 33 of 34                                                                         |



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Celltech**

Certificate No: **EX3-3600\_Apr14**

## CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3600**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,  
 QA CAL-25.v6  
 Calibration procedure for dosimetric E-field probes**

Calibration date: **April 15, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 03-Apr-14 (No. 217-01911)         | Apr-15                 |
| Power sensor E4412A        | MY41498087      | 03-Apr-14 (No. 217-01911)         | Apr-15                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 03-Apr-14 (No. 217-01915)         | Apr-15                 |
| Reference 20 dB Attenuator | SN: S5277 (20x) | 03-Apr-14 (No. 217-01919)         | Apr-15                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 03-Apr-14 (No. 217-01920)         | Apr-15                 |
| Reference Probe ES3DV2     | SN: 3013        | 30-Dec-13 (No. ES3-3013_Dec13)    | Dec-14                 |
| DAE4                       | SN: 660         | 13-Dec-13 (No. DAE4-660_Dec13)    | Dec-14                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Apr-13)  | In house check: Apr-16 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-13) | In house check: Oct-14 |

|                                                                                                                 | Name           | Function              | Signature |
|-----------------------------------------------------------------------------------------------------------------|----------------|-----------------------|-----------|
| Calibrated by:                                                                                                  | Jeton Kastrati | Laboratory Technician |           |
| Approved by:                                                                                                    | Katja Pokovic  | Technical Manager     |           |
| Issued: April 15, 2014                                                                                          |                |                       |           |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |                |                       |           |



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C, D               | modulation dependent linearization parameters                                                                                                           |
| Polarization $\varphi$   | $\varphi$ rotation around probe axis                                                                                                                    |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |
| Connector Angle          | information used in DASY system to align probe sensor X to the robot coordinate system                                                                  |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

# Probe EX3DV4

## SN:3600

Manufactured: January 10, 2007  
Calibrated: April 15, 2014

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3600

### Basic Calibration Parameters

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|-----------------------------------------------------------|----------|----------|----------|-----------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 0.50     | 0.49     | 0.40     | ± 10.1 %  |
| DCP (mV) <sup>B</sup>                                     | 99.8     | 92.9     | 97.6     |           |

### Modulation Calibration Parameters

| UID | Communication System Name |   | A<br>dB | B<br>dB $\sqrt{\mu\text{V}}$ | C   | D<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-----|---------------------------|---|---------|------------------------------|-----|---------|----------|---------------------------|
| 0   | CW                        | X | 0.0     | 0.0                          | 1.0 | 0.00    | 122.9    | ±3.3 %                    |
|     |                           | Y | 0.0     | 0.0                          | 1.0 |         | 125.6    |                           |
|     |                           | Z | 0.0     | 0.0                          | 1.0 |         | 123.5    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3600

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 150                  | 52.3                               | 0.76                            | 9.80    | 9.80    | 9.80    | 0.00               | 1.00                    | ± 13.3 %    |
| 300                  | 45.3                               | 0.87                            | 9.02    | 9.02    | 9.02    | 0.11               | 1.10                    | ± 13.3 %    |
| 450                  | 43.5                               | 0.87                            | 9.40    | 9.40    | 9.40    | 0.20               | 1.30                    | ± 13.3 %    |
| 750                  | 41.9                               | 0.89                            | 8.55    | 8.55    | 8.55    | 0.28               | 1.13                    | ± 12.0 %    |
| 835                  | 41.5                               | 0.90                            | 8.23    | 8.23    | 8.23    | 0.24               | 1.30                    | ± 12.0 %    |
| 900                  | 41.5                               | 0.97                            | 8.09    | 8.09    | 8.09    | 0.38               | 0.85                    | ± 12.0 %    |
| 1950                 | 40.0                               | 1.40                            | 6.56    | 6.56    | 6.56    | 0.73               | 0.60                    | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 6.19    | 6.19    | 6.19    | 0.29               | 0.91                    | ± 12.0 %    |
| 5200                 | 36.0                               | 4.66                            | 4.56    | 4.56    | 4.56    | 0.30               | 1.80                    | ± 13.1 %    |
| 5500                 | 35.6                               | 4.96                            | 4.31    | 4.31    | 4.31    | 0.35               | 1.80                    | ± 13.1 %    |
| 5800                 | 35.3                               | 5.27                            | 4.01    | 4.01    | 4.01    | 0.40               | 1.80                    | ± 13.1 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3600

### Calibration Parameter Determined in Body Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha <sup>G</sup> | Depth <sup>G</sup> (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 150                  | 61.9                               | 0.80                            | 8.81    | 8.81    | 8.81    | 0.00               | 1.00                    | ± 13.3 %    |
| 300                  | 58.2                               | 0.92                            | 9.20    | 9.20    | 9.20    | 0.09               | 1.15                    | ± 13.3 %    |
| 450                  | 56.7                               | 0.94                            | 9.05    | 9.05    | 9.05    | 0.12               | 1.30                    | ± 13.3 %    |
| 750                  | 55.5                               | 0.96                            | 8.14    | 8.14    | 8.14    | 0.35               | 0.97                    | ± 12.0 %    |
| 835                  | 55.2                               | 0.97                            | 8.11    | 8.11    | 8.11    | 0.50               | 0.82                    | ± 12.0 %    |
| 900                  | 55.0                               | 1.05                            | 7.92    | 7.92    | 7.92    | 0.41               | 0.92                    | ± 12.0 %    |
| 1950                 | 53.3                               | 1.52                            | 6.79    | 6.79    | 6.79    | 0.56               | 0.73                    | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 6.26    | 6.26    | 6.26    | 0.77               | 0.57                    | ± 12.0 %    |
| 5200                 | 49.0                               | 5.30                            | 4.06    | 4.06    | 4.06    | 0.40               | 1.90                    | ± 13.1 %    |
| 5500                 | 48.6                               | 5.65                            | 3.65    | 3.65    | 3.65    | 0.40               | 1.90                    | ± 13.1 %    |
| 5800                 | 48.2                               | 6.00                            | 3.65    | 3.65    | 3.65    | 0.50               | 1.90                    | ± 13.1 %    |


<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

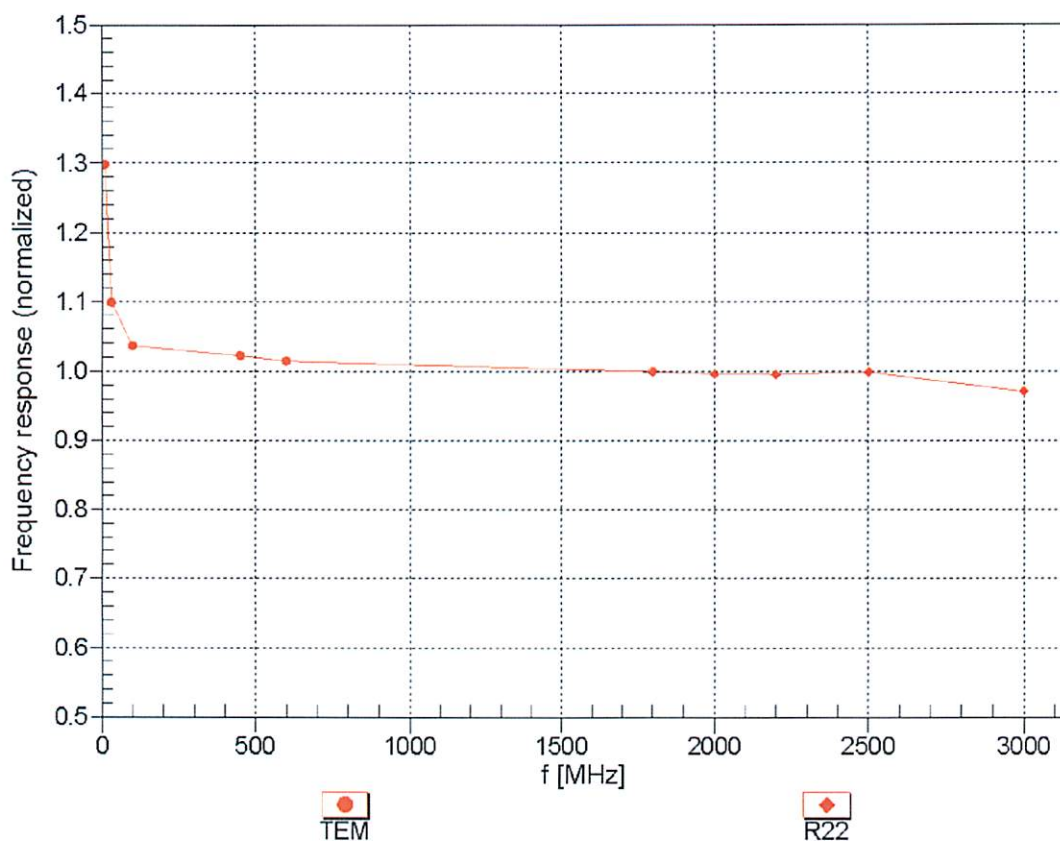



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

## Receiving Pattern ( $\phi$ ), $\vartheta = 0^\circ$

f=600 MHz, TEM

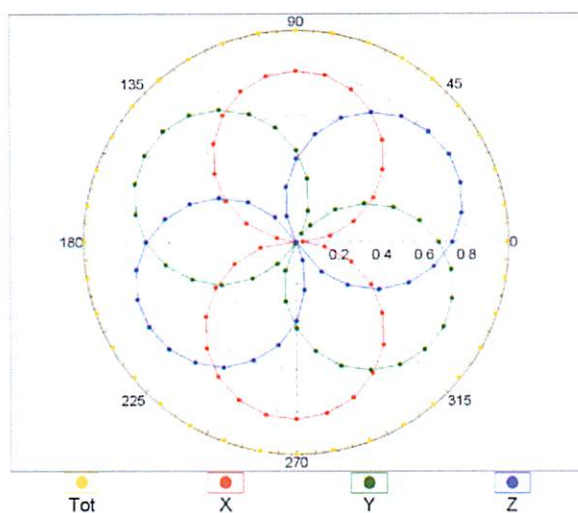



f=1800 MHz, R22

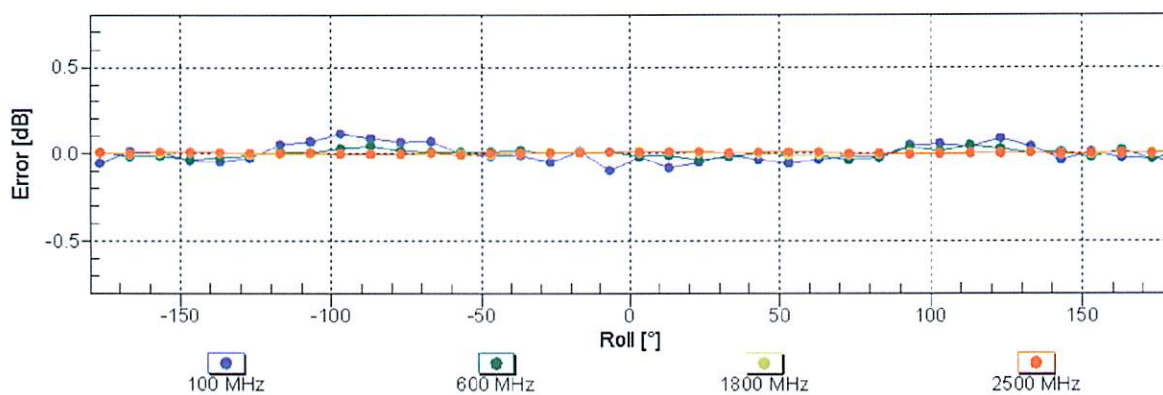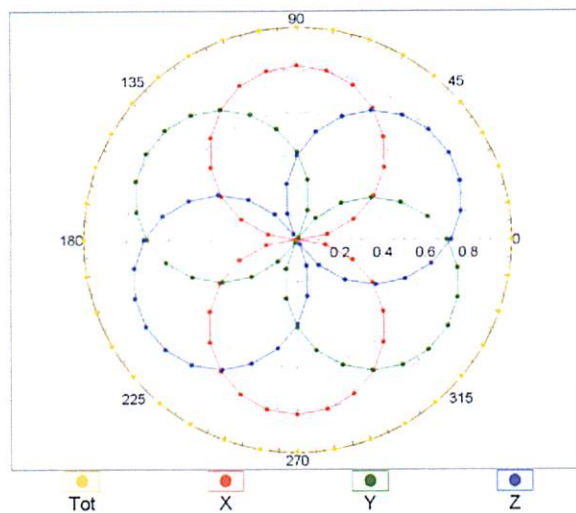

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )


## Dynamic Range f(SAR<sub>head</sub>)

(TEM cell , f<sub>eval</sub>= 1900 MHz)

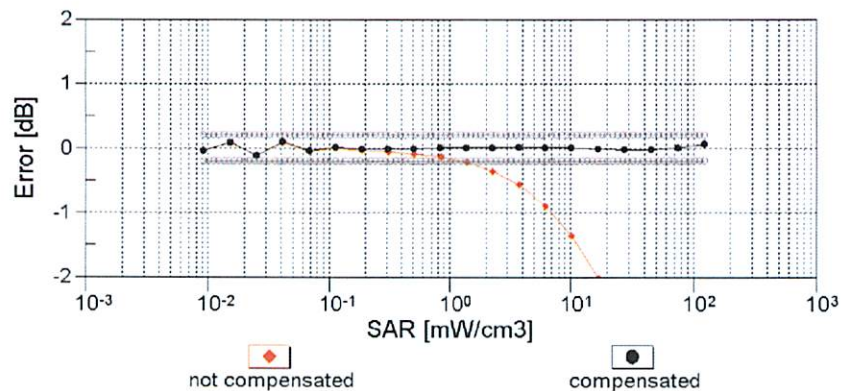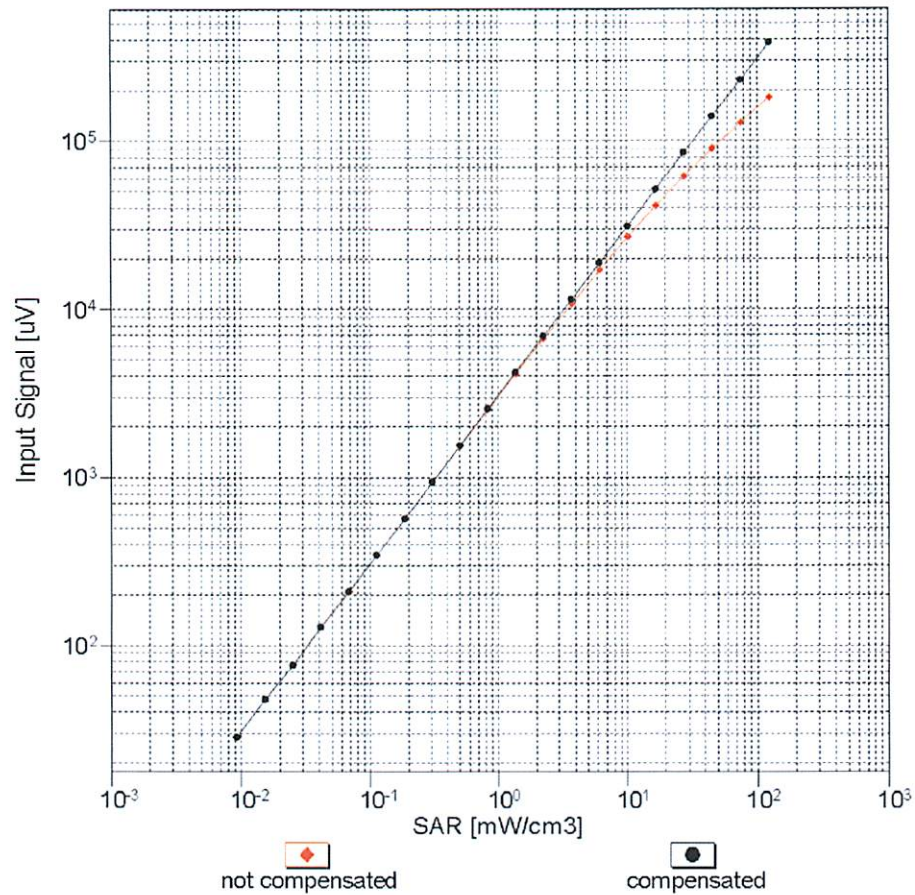


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  (k=2)

## Conversion Factor Assessment

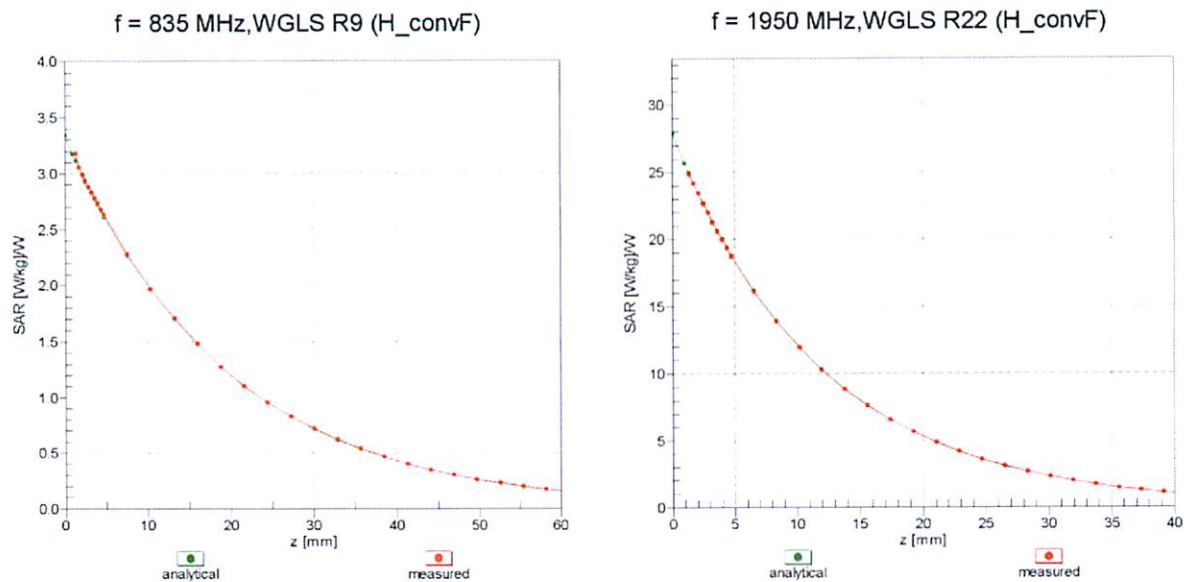

## Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ),  $f = 900 \text{ MHz}$

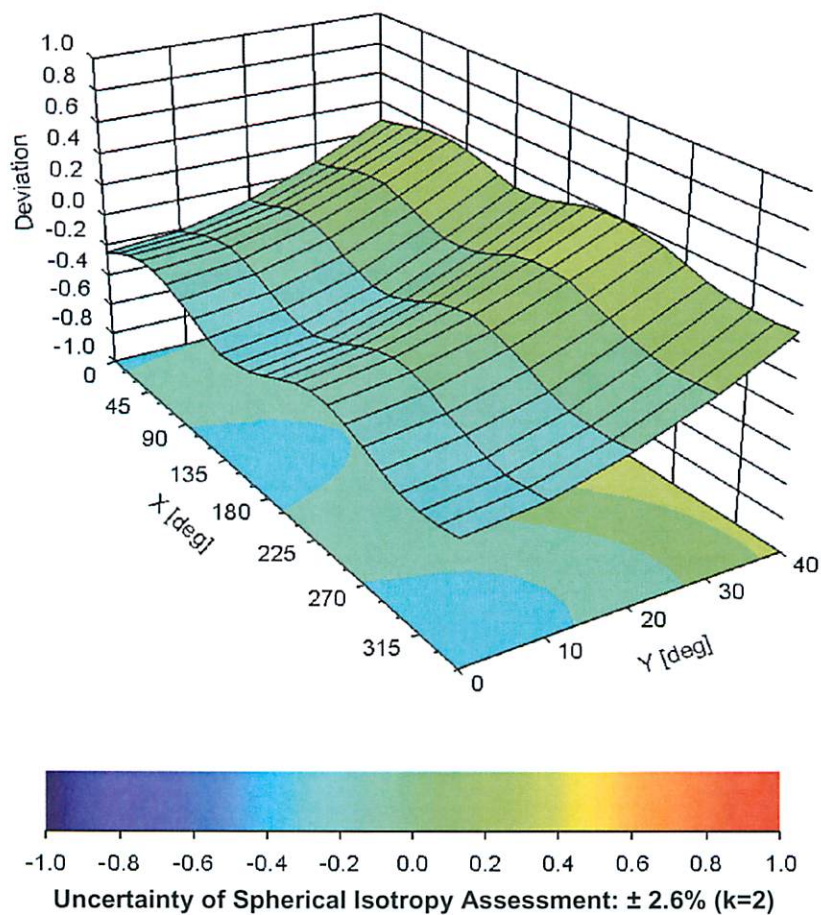

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3600

### Other Probe Parameters

|                                               |            |
|-----------------------------------------------|------------|
| Sensor Arrangement                            | Triangular |
| Connector Angle (°)                           | -146.9     |
| Mechanical Surface Detection Mode             | enabled    |
| Optical Surface Detection Mode                | disabled   |
| Probe Overall Length                          | 337 mm     |
| Probe Body Diameter                           | 10 mm      |
| Tip Length                                    | 9 mm       |
| Tip Diameter                                  | 2.5 mm     |
| Probe Tip to Sensor X Calibration Point       | 1 mm       |
| Probe Tip to Sensor Y Calibration Point       | 1 mm       |
| Probe Tip to Sensor Z Calibration Point       | 1 mm       |
| Recommended Measurement Distance from Surface | 2 mm       |

|                                                                                  |                                                    |                                                           |                                                           |                                                                                                                        |
|----------------------------------------------------------------------------------|----------------------------------------------------|-----------------------------------------------------------|-----------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------|
|  | <u>Date(s) of Evaluation</u><br>September 19, 2014 | <u>Test Report Serial No.</u><br>091614IPH-1307-SNA       | <u>Test Report Revision No.</u><br>Rev. 1.3 (3rd Release) | <br>Test Lab Certificate No. 2470.01 |
|                                                                                  | <u>Test Report Issue Date</u><br>December 17, 2014 | <u>Description of Test(s)</u><br>Specific Absorption Rate | <u>RF Exposure Category</u><br>Gen. Pop. / Uncontrolled   |                                                                                                                        |

## APPENDIX G - PHANTOM CERTIFICATE OF CONFORMITY

|                         |                                                                                                                      |                  |                                       |            |                    |                                                                                       |
|-------------------------|----------------------------------------------------------------------------------------------------------------------|------------------|---------------------------------------|------------|--------------------|---------------------------------------------------------------------------------------|
| <b>Applicant:</b>       | <b>Garmin International Inc.</b>                                                                                     | <b>FCC ID:</b>   | <b>IPH-02257</b>                      | <b>IC:</b> | <b>1792A-02257</b> |  |
| <b>Model:</b>           | <b>A02257</b>                                                                                                        | <b>DUT Type:</b> | <b>Wireless Extremity-Worn Device</b> |            |                    |                                                                                       |
| 2014 Celltech Labs Inc. | This document is not to be reproduced in whole or in part without the prior written permission of Celltech Labs Inc. |                  |                                       |            |                    | Page 34 of 34                                                                         |

Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com

## Certificate of Conformity / First Article Inspection

|              |                                                                         |
|--------------|-------------------------------------------------------------------------|
| Item         | Oval Flat Phantom ELI 5.0                                               |
| Type No      | QD OVA 002 A                                                            |
| Series No    | 1108 and higher                                                         |
| Manufacturer | Untersee Composites<br>Knebelstrasse 8, CH-8268 Mannenbach, Switzerland |

### Tests

Complete tests were made on the prototype units QD OVA 001 A, pre-series units QD OVA 001 B as well as on some series units QD OVA 001 B. Some tests are made on all series units QD OVA 002 A.

| Test                 | Requirement                                                                         | Details                                                                                      | Units tested              |
|----------------------|-------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------|---------------------------|
| Shape                | Internal dimensions, depth and sagging are compatible with standards                | Bottom elliptical 600 x 400 mm, Depth 190 mm, dimension compliant with [1] for $f > 375$ MHz | Prototypes                |
| Material thickness   | Bottom: 2.0mm +/- 0.2mm                                                             | dimension compliant with [3] for $f > 800$ MHz                                               | all                       |
| Material parameters  | rel. permittivity 2 – 5, loss tangent $\leq 0.05$ , at $f \leq 6$ GHz               | rel. permittivity 3.5 +/- 0.5 loss tangent $\leq 0.05$                                       | Material samples          |
| Material resistivity | Compatibility with tissue simulating liquids .                                      | Compatible with SPEAG liquids. **                                                            | Phantoms, Material sample |
| Sagging              | Sagging of the flat section in tolerance when filled with tissue simulating liquid. | within tolerance for filling height up to 155 mm                                             | Prototypes, samples       |

\*\* Note: Compatibility restrictions apply certain liquid components mentioned in the standard, containing e.g. DGBE, DGMHE or Triton X-100. Observe technical note on material compatibility.

### Standards

- [1] OET Bulletin 65, Supplement C, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", Edition 01-01
- [2] IEEE 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques, December 2003
- [3] IEC 62209–1 ed1.0, "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", 2005-02-18
- [4] IEC 62209–2 ed1.0, "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", 2010-03-30

### Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of **body-worn** SAR measurements and system performance checks as specified in [1 – 4] and further standards.

Date 25.7.2011

Signature / Stamp

**s p e a g**

Schmid & Partner Engineering AG  
 Zeughausstrasse 43, 8004 Zurich, Switzerland  
 Phone +41 44 245 9700, Fax +41 44 245 9779  
 info@speag.com, http://www.speag.com