



Specific Absorption Rate (SAR) Test Report

for

CRETE SYSTEMS INC.

on the

Tablet computer

Report No. : FA840719
Trade Name : CReTE
Model Name : DR886 EX
FCC ID : IR5DR886EX

Date of Testing : Aug. 09, 2008 ~ Aug. 11, 2008

Date of Report : Aug. 13, 2008 Date of Review : Aug. 22, 2008

- Without written approval of SPORTON International Inc., the test report shall not be reproduced except in full.
- Report Version: Rev. 02

SPORTON International Inc.

No. 52, Hwa Ya 1st Rd., Hwa Ya Technology Park, Kwei-Shan Hsiang, Tao Yuan Hsien, Taiwan, R.O.C.



Table of Contents

		nent of Compliance	
2.		nistration Data	
	2.1	Testing Laboratory	
	2.2	Detail of Applicant	2
	2.3	Detail of Manufacturer	
	2.4	Application Details	
3.		al Information	3
	3.1	Description of Device Under Test (DUT)	
	3.2	Basic Description of Accessories	
	3.3	Product Photos	
	3.4	Applied Standards	
	3.5	Device Category and SAR Limits	
	3.6	Test Conditions	
		3.6.1 Ambient Condition	
		3.6.2 Test Configuration	
4.	Specif	ic Absorption Rate (SAR)	
	4.1	Introduction	
	4.2	SAR Definition	
5.	SAR N	Measurement Setup	€
	5.1	DASY4 E-Field Probe System	7
		5.1.1 ET3DV6 E-Field Probe Specification	
		5.1.2 ET3DV6 and EX3DV3 E-Field Probe Calibration	
	5.2	DATA Acquisition Electronics (DAE)	9
	5.3	Robot	9
	5.4	Measurement Server	9
	5.5	SAM Twin Phantom	.10
	5.6	Device Holder for SAM Twin Phantom	. 11
	5.7	Data Storage and Evaluation	.12
		5.7.1 Data Storage	
		5.7.2 Data Evaluation	
	5.8	Test Equipment List	
6.	Tissue	e Simulating Liquids	.15
7.	Uncer	tainty Assessment	.16
		leasurement Evaluation	
	8.1	Purpose of System Performance Check	.19
	8.2	System Setup	.19
	8.3	Validation Results	
9.	Descr	iption for DUT Testing Position	.27
10.	Measu	rement Procedures	.23
	10.1	Spatial Peak SAR Evaluation	
	10.2	Scan Procedures	
	10.3	SAR Averaged Methods	
11.		est Results	
	11.1	Conducted Power	
	11.2	Test Record	
12.		ence	

Appendix A - System Performance Check Data Appendix B - SAR Measurement Data Appendix C - Calibration Data

Appendix D - Product Photos

Appendix E - Test Setup Photos



1. Statement of Compliance

The Specific Absorption Rate (SAR) maximum result found during testing for the CReTE SYSTEMS INC. Tablet computer CReTE DR886 EX on the 802.11a/b/g body SAR are as follows (with expanded uncertainty 21.9% for 2.4GHz Band and 25.9% for 5GHz Band):

802.11b/g	802.11a	802.11a
(2400MHz~2483.5MHz)	(5150MHz~5350MHz)	(5725MHz~5850MHz)
Body SAR	Body SAR	Body SAR
(W/kg)	(W/kg)	(W/kg)
0.789	0.302	0.497

They are in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1999 and had been tested in accordance with the measurement methods and procedures specified in OET Bulletin 65 Supplement C (Edition 01-01).

Approved by

Roy Wu Manager



2. Administration Data

2.1 Testing Laboratory

Company Name: Sporton International Inc.

Address: No.52, Hwa-Ya 1st RD., Hwa Ya Technology Park, Kwei-Shan Hsiang,

Test Report No : FA840719

TaoYuan Hsien, Taiwan, R.O.C.

Telephone Number: 886-3-327-3456 **Fax Number:** 886-3-328-4978

2.2 Detail of Applicant

Company Name: CReTE SYSTEMS INC.

Address: 7F,No.250,Sec.3,Pei Shen Rd.,Shen Keng Hsiang,Taipei County,Taiwan

2.3 Detail of Manufacturer

Company Name: CReTE SYSTEMS INC.

Address: 7F,No.250,Sec.3,Pei Shen Rd.,Shen Keng Hsiang,Taipei County,Taiwan

2.4 Application Details

Date of reception of application:Apr. 07, 2008Start of test:Aug. 09, 2008End of test:Aug. 11, 2008



3. General Information

3.1 Description of Device Under Test (DUT)

Product Feature & Specification					
DUT Type :	Tablet computer				
Trade Name :	CReTE				
Model Name :	DR886 EX				
FCC ID :	IR5DR886EX				
Frequency Range :	802.11b/g : 2400 MHz ~ 2483.5 MHz 802.11a : 5150 MHz ~ 5250 MHz, 5250 MHz ~ 5350 MHz, 5725 MHz ~ 5850 MHz				
Maximum Output Power to Antenna :	<2400 MHz ~ 2483.5 MHz> 802.11b : 20.63 dBm 802.11g : 24.13 dBm <5150 MHz ~ 5350 MHz> 802.11a : 18.86 dBm <5725 MHz ~ 5850 MHz> 802.11a : 20.39 dBm				
Type of Antenna Connector :	N/A				
Antenna Type :	PIFA Antenna				
Type of Modulation :	DSSS / OFDM				
DUT Stage :	Production Unit				
Application Type :	Certification				

3.2 Basic Description of Accessories

	Brand Name	FranMar
AC Adapter	Model Name	F10903-A
ric riuipici	Power Rating	I/P: 100-240Vac, 50-60Hz, 1.2A; O/P: 19Vdc, 4.75A
	Brand Name	J.S. POWER
Dattany	Model Name	BD83A
Battery	Power Rating	11.1Vdc, 4800mAh
	Type	Li-ion

Remark: Above EUT's information was declared by manufacturer. Please refer to the specifications of manufacturer or User's Manual for more detailed features description.

3.3 Product Photos

Refer to Appendix D.



3.4 Applied Standards

The Specific Absorption Rate (SAR) testing specification, method and procedure for this Tablet computer is in accordance with the following standards:

47 CFR Part 2 (2.1093),
IEEE C95.1-1999,
IEEE C95.3-2002,
IEEE P1528 -2003, and
OET Bulletin 65 Supplement C (Edition 01-01)
KDB 248227 r1.2 SAR Measurement Procedures for 802.11abg Transmitters
KDB 447498 D01 v03r01 Mobile and Portable Device RF Exposure Procedures

3.5 Device Category and SAR Limits

This device belongs to portable device category because its radiating structure is allowed to be used within 20 centimeters of the body of the user. Limit for General Population/Uncontrolled exposure should be applied for this device, it is 1.6 W/kg as averaged over any 1 gram of tissue.

3.6 Test Conditions

3.6.1 Ambient Condition

Item	MSL_2450	MSL_5200	MSL_5800
Ambient Temperature (°C)		$20\sim24^{\circ}\!\mathrm{C}$	
Tissue simulating liquid temperature (°C)	21.4 °C	21.3 °C	21.3 °C
Humidity (%)		< 60%	

3.6.2 Test Configuration

For WLAN link mode, engineering testing software installed on the EUT can provide continuous transmitting RF signal. This RF signal utilized in SAR measurement has almost 100% duty cycle and its crest factor is 1. Measurements were performed on the lowest, middle, and highest channel for each testing position. However, measurements were performed only on the middle channel if the SAR is below 3 dB of limit for body SAR testing.

The data rates for WLAN SAR testing were set in 1Mbps for 802.11b, 6Mbps for 802.11g and 802.11a due to highest output power.



4. Specific Absorption Rate (SAR)

4.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The FCC recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

4.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density. ρ). The equation description is as below:

$$\mathbf{SAR} = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$\mathbf{SAR} = C \frac{\delta T}{\delta t}$$

, where C is the specific head capacity, δT is the temperature rise and δt the exposure duration,

or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\sigma |E|^2}{\rho}$$

, where σ is the conductivity of the tissue, ρ is the mass density of the tissue and E is the rms electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.



5. SAR Measurement Setup

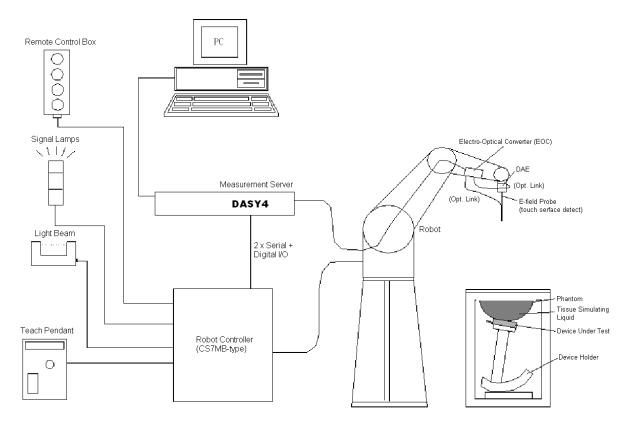


Fig. 5.1 DASY4 system

The DASY4 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- A dosimetric probe equipped with an optical surface detector system
- > The electro-optical converter (ECO) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- > A probe alignment unit which improves the accuracy of the probe positioning
- ➤ A computer operating Windows XP
- ➤ DASY4 software
- Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- > The SAM twin phantom
- ➤ A device holder
- > Tissue simulating liquid
- Dipole for evaluating the proper functioning of the system

Some of the components are described in details in the following sub-sections.



5.1 DASY4 E-Field Probe System

The SAR measurement is conducted with the dosimetric probe ET3DV6 and EX3DV3 (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency. This probe has a built in optical surface detection system to prevent from collision with phantom.

5.1.1 <u>ET3DV6 E-Field Probe Specification</u>

<ET3DV6>

Construction Symmetrical design with triangular core

Built-in optical fiber for surface detection

system

Built-in shielding against static charges PEEK enclosure material (resistant to organic

solvents)

Frequency 10 MHz to 3 GHz

Directivity ± 0.2 dB in brain tissue (rotation around probe

axis)

 \pm 0.4 dB in brain tissue (rotation perpendicular to

probe axis)

Dynamic Range 5 μ W/g to 100mW/g; Linearity: \pm 0.2dB

Surface Detection ± 0.2 mm repeatability in air and clear liquids on

reflecting surface

Dimensions Overall length: 330mm

Tip length: 16mm Body diameter: 12mm Tip diameter: 6.8mm

Distance from probe tip to dipole centers: 2.7mm

Application General dosimetry up to 3GHz

Compliance tests for mobile phones and Wireless

LAN

Fast automatic scanning in arbitrary phantoms



Construction Symmetrical design with triangular core

Built-in shielding against static charges PEEK enclosure material (resistant to organic

solvents)

Frequency 10 MHz to 6 GHz; Linearity: \pm 0.2 dB (30 MHz

to 3 GHz)

Directivity ± 0.3 dB in HSL (rotation around probe axis)

 \pm 0.5 dB in tissue material (rotation normal to

probe axis)

Dynamic Range 10 μ W/g to 100 mW/g; Linearity: \pm 0.2 dB

(noise: typically $< 1 \mu W/g$)

Dimensions Overall length: 330 mm (Tip: 20 mm)

Tip diameter: 2.5 mm (Body: 12 mm)

Typical distance from probe tip to dipole centers:

1 mm

Application High precision dosimetric measurements in any

exposure scenario (e.g., very strong gradient fields). Only probe which enables compliance testing for frequencies up to 6 GHz with precision

of better 30%.



Fig. 5.2 Probe Setup on Robot



Fig. 5.3 EX3DV3 E-field Probe



5.1.2 <u>ET3DV6 and EX3DV3 E-Field Probe Calibration</u>

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy shall be evaluated and within \pm 0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data are as below:

> ET3DV6 sn1787

Sensitivity	X axis : 1.63 μV X axis : 92 mV		Y axis : 1.66 μV Y axis : 96 mV		Z axis : 2.08 μV
Diode compression point					Z axis : 91 mV
Conversion factor	Frequency (MHz)	X axis		Y axis	Z axis
(Head / Body)	2350~2550	4.50 / 4.02		4.50 / 4.02	4.50 / 4.02
Boundary effect	Frequency (MHz)	Alp	ha	Depth	
(Head / Body)	2350~2550	0.67 /	0.65	1.81 / 2.15	

> EX3DV3 sn3514

Sensitivity	X axis : 0.6	50 μV	Y axis : 0.690 μV		Z axis : 0.580 μV	
Diode compression point	X axis : 95	X axis : 95 mV		xis : 93 mV	Z axis : 96 mV	
	Frequency (MHz)	X axis		Y axis	Z axis	
Conversion factor	5100~5300	4.34		4.34	4.34	
(Body)	5200~5400	4.0	06	4.06	4.06	
	5700~5900	900 4.20		4.20	4.20	
	Frequency (MHz)	Alp	oha	Depth		
Boundary effect	5100~5300	0.3	5	1.70		
(Body)	5200~5400	0.3	8	1.70		
	5700~5900	0.3	0	1.70		

NOTE: The probe parameters have been calibrated by the SPEAG.



5.2 <u>DATA Acquisition Electronics (DAE)</u>

The data acquisition electronics (DAE4) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.

5.3 Robot

The DASY4 system uses the high precision robots RX90BL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY4 system, the CS7MB robot controller version from Stäubli is used. The RX robot series have many features that are important for our application:

- ➤ High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- > Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- ► 6-axis controller

5.4 Measurement Server

The DASY4 measurement server is based on a PC/104 CPU board with 166 MHz CPU 32 MB chipset and 64 MB RAM

Communication with the DAE4 electronic box the 16-bit AD-converter system for optical detection and digital I/O interface.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.



5.5 SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- ➤ Left head
- Right head
- > Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

The phantom can be used with the following tissue simulating liquids:

- *Water-sugar based liquid
- *Glycol based liquids

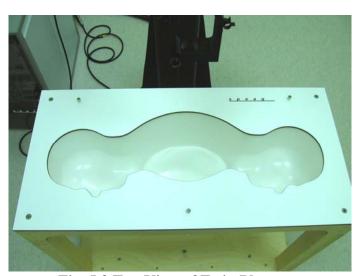


Fig. 5.3 Top View of Twin Phantom



Fig. 5.4 Bottom View of Twin Phantom



5.6 <u>Device Holder for SAM Twin Phantom</u>

The SAR in the Phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source in 5 mm distance, a positioning uncertainty of ± 0.5 mm would produce a SAR uncertainty of $\pm 20\%$. An accurate device position is therefore crucial for accurate and repeatable measurement. The position in which the devices must be measured, are defined by the standards.

The DASY4 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation center for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The DASY4 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $\varepsilon_r = 3$ and loss tangent $\delta = 0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



Fig. 5.5 Device Holder



5.7 <u>Data Storage and Evaluation</u>

5.7.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The post-processing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [A/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a non-louse media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

5.7.2 Data Evaluation

The DASY4 post-processing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters :	- Sensitivity	$Norm_i$, a_{i0} , a_{i1} , a_{i2}
	- Conversion factor	$ConvF_i$
	- Diode compression point	dep_i
Device parameters :	- Frequency	f
	- Crest factor	cf
Media parameters:	- Conductivity	σ
	- Density	ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power.





The formula for each channel can be given as:

$$Vi = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with

 V_i = compensated signal of channel i (i = x, y, z)

 U_i = input signal of channel i (i = x, y, z)

cf = crest factor of exciting field (DASY parameter)

 $dcp_i = diode\ compression\ point\ (DASY\ parameter)$

From the compensated input signals, the primary field data for each channel can be evaluated:

E-field probes : $E_i = \sqrt{\frac{V_i}{Norm_i ConvF}}$

 $\text{H-field probes}: \ \ H_{i} \ \ = \ \ \sqrt{V_{i}} \frac{a_{i0+} a_{i1} f + a_{i2} f^{2}}{f}$

with

 V_i = compensated signal of channel i (i = x, y, z)

 $Norm_i$ = sensor sensitivity of channel i (i = x, y, z)

 μ V/(V/m)2 for E-field Probes

ConvF = sensitivity enhancement in solution

 a_{ii} = sensor sensitivity factors for H-field probes

 \vec{f} = carrier frequency [GHz]

 E_i = electric field strength of channel i in V/m

 H_i = magnetic field strength of channel *i* in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_X^2 + E_Y^2 + E_Z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with

SAR = local specific absorption rate in mW/g

Etot = total field strength in V/m

 $\sigma = \text{conductivity in [mho/m] or [Siemens/m]}$

 ρ = equivalent tissue density in g/cm³

* Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or $P_{pwe} = H_{tot}^2 \cdot 37.7$

with

 P_{pwe} = equivalent power density of a plane wave in mW/cm²

 E_{tot} = total electric field strength in V/m

 H_{tot} = total magnetic field strength in A/m



5.8 Test Equipment List

Manufacture	Name of Equipment	Type/Model	Serial Number	Calibration		
Manufacture	Name of Equipment	1 ype/Model	Seriai Number	Last Cal.	Due Date	
SPEAG	Dosimetric E-Filed Probe	ET3DV6	1787	Aug. 28, 2007	Aug. 27, 2008	
SPEAG	Dosimetric E-Filed Probe	EX3DV3	3514	Jan. 31, 2008	Jan. 31, 2009	
SPEAG	2450MHz System Validation Kit	D2450V2	736	Jul. 12, 2007	Jul. 12, 2009	
SPEAG	5GHz System Validation Kit	D5GHzV2	1006	Jan. 24, 2008	Jan. 24, 2010	
SPEAG	Data Acquisition Electronics	DAE4	778	Sep. 17, 2007	Sep. 17, 2008	
SPEAG	Device Holder	N/A	N/A	NCR	NCR	
SPEAG	Phantom	QD 000 P40 C	TP-1303	NCR	NCR	
SPEAG	Phantom	QD 000 P40 C	TP-1383	NCR	NCR	
SPEAG	Phantom	QD 0VA 001 BB	1029	NCR	NCR	
SPEAG	Robot	Staubli RX90BL	F03/5W15A1/A/01	NCR	NCR	
SPEAG	Software	DASY4 V4.7 Build 55	N/A	NCR	NCR	
SPEAG	Software	SEMCAD V1.8 Build 176	N/A	NCR	NCR	
SPEAG	Measurement Server	SE UMS 001 BA	1021	NCR	NCR	
Agilent	Wireless Communication Test Set	E5515C	GB46311322	Dec. 22, 2006	Dec. 22, 2008	
Agilent	PNA Series Network Analyzer	E8358A	US40260131	Apr. 02, 2008	Apr. 01, 2009	
Agilent	Dielectric Probe Kit	85070D	US01440205	NCR	NCR	
Agilent	Dual Directional Coupler	778D	50422	NCR	NCR	
AR	Power Amplifier	5S1G4M2	0328767	NCR	NCR	
R&S	Power Meter	NRVD	101394	Oct. 31, 2007	Oct. 30, 2008	
R&S	Power Sensor	NRV-Z1	100130	Oct. 31, 2007	Oct. 30, 2008	

Table 5.1 Test Equipment List



6. Tissue Simulating Liquids

For the measurement of the field distribution inside the SAM phantom with DASY4, the phantom must be filled with around 25 liters of homogeneous body tissue simulating liquid. The liquid height from the ear reference point (ERP) of the phantom to the liquid top surface is (head SAR) or from the flat phantom to the liquid top surface (body SAR) is 15.2cm.

The dielectric parameters of the liquids were verified prior to the SAR evaluation using an Agilent 85070D Dielectric Probe Kit and an Agilent Network Analyzer.

Table 6.1 shows the measuring results for muscle simulating liquid.

Band	Frequency (MHz)	Conductivity (σ)	Permittivity (ε _r)	Measurement date
000 111,/~	2412	1.89	54.0	
802.11b/g (2400~2450 MHz)	2437	1.92	53.9	Aug. 09, 2008
(2400~2430 MITIZ)	2462	1.95	53.8	
802.11a	5180	5.30	48.7	
(5150~5350 MHz)	5260	5.42	48.6	Aug. 11, 2008
(3130~3330 MITZ)	5320	5.50	48.4	
902.11a	5745	6.05	47.5	
802.11a (5725~5850 MHz)	5785	6.09	47.4	Aug. 11, 2008
(3/23~3630 MITZ)	5825	6.13	47.2	

Table 6.1 Measuring Results for Muscle Simulating Liquid

The measuring data are consistent with ε r = 52.7 ± 5%, σ = 1.95 ± 5% for 2400~2483.5MHz, ε r = 49.0 ± 5% and σ = 5.30 ± 5% for 5150~5350MHz, and ε r = 48.2 ±5%, 6 = 6.00 ± 5% for body 5725~5850MHz.



7. Uncertainty Assessment

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table 7.1

Uncertainty Distributions	Normal	Rectangular	Triangular	U-shape
Multiplying factor ^(a)	1/k (b)	1/√3	1/√6	1/√2

⁽a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity

Table 7.1 Standard Uncertainty for Assumed Distribution

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY4 uncertainty Budget is showed in Table 7.2.

⁽b) κ is the coverage factor



Error Description	Uncertainty Value ± %	Probability Distribution	Divisor	Ci (1g)	Standard Unc. (1g)	vi or Veff
Measurement Equipment						
Probe Calibration	±5.9 %	Normal	1	1	±5.9 %	∞
Axial Isotropy	±4.7 %	Rectangular	$\sqrt{3}$	0.7	±1.9 %	∞
Hemispherical Isotropy	±9.6 %	Rectangular	$\sqrt{3}$	0.7	±3.9 %	∞
Boundary Effects	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Linearity	±4.7 %	Rectangular	$\sqrt{3}$	1	±2.7 %	∞
System Detection Limits	±1.0 %	Rectangular	√3	1	±0.6 %	∞
Readout Electronics	±0.3 %	Normal	1	1	±0.3 %	∞
Response Time	±0.8 %	Rectangular	$\sqrt{3}$	1	±0.5 %	∞
Integration Time	±2.6 %	Rectangular	$\sqrt{3}$	1	±1.5 %	∞
RF Ambient Noise	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
RF Ambient Reflections	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
Probe Positioner	±0.4 %	Rectangular	$\sqrt{3}$	1	±0.2 %	∞
Probe Positioning	±2.9 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
Max. SAR Eval.	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Test Sample Related						
Device Positioning	±2.9 %	Normal	1	1	±2.9	145
Device Holder	±3.6 %	Normal	1	1	±3.6	5
Power Drift	±5.0 %	Rectangular	$\sqrt{3}$	1	±2.9	∞
Phantom and Setup						
Phantom Uncertainty	±4.0 %	Rectangular	$\sqrt{3}$	1	±2.3	∞
Liquid Conductivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.64	±1.8	∞
Liquid Conductivity (meas.)	±2.5 %	Normal	1	0.64	±1.6	∞
Liquid Permittivity (target)	±5.0 %	Rectangular	√3	0.6	±1.7	∞
Liquid Permittivity (meas.)	±2.5 %	Normal	1	0.6	±1.5	∞
Combined Standard Uncertainty					±10.9	387
Coverage Factor for 95 %		K=2				
Expanded uncertainty (Coverage factor = 2)					±21.9	

Table 7.2 Uncertainty Budget of DASY4 for 2.4GHz Band



Error Description	Uncertainty Value	Probability Distribution	Divisor	Ci (1g)	Standard Unc. (1g)	vi or Veff
Measurement System						
Probe Calibration	±6.8 %	Normal	1	1	±6.8 %	∞
Axial Isotropy	±4.7 %	Rectangular	$\sqrt{3}$	0.7	±1.9 %	∞
Hemispherical Isotropy	±9.6 %	Rectangular	$\sqrt{3}$	0.7	±3.9 %	∞
Boundary Effect	±2.0 %	Rectangular	$\sqrt{3}$	1	±1.2 %	8
Linearity	±4.7 %	Rectangular	$\sqrt{3}$	1	±2.7 %	∞
System Detection Limit	±1.0 %	Rectangular	√3	1	±0.6 %	8
Readout Electronics	±0.3 %	Normal	1	1	±0.3 %	∞
Response Time	±0.8 %	Rectangular	$\sqrt{3}$	1	± 0.5 %	∞
Integration Time	±2.6 %	Rectangular	$\sqrt{3}$	1	± 1.5 %	∞
RF Ambient Noise	±3.0 %	Rectangular	√3	1	±1.7 %	8
RF Ambient Reflections	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
Probe Positioner	±0.8 %	Rectangular	√3	1	±0.5 %	8
Probe Positioning	±9.9 %	Rectangular	$\sqrt{3}$	1	±5.7 %	8
Max. SAR Eval.	±4.0 %	Rectangular	$\sqrt{3}$	1	±2.3 %	∞
Test Sample Related						
Device Positioning	±2.9 %	Normal	1	1	±2.9 %	145
Device Holder	±3.6 %	Normal	1	1	±3.6 %	5
Power Drift	±5.0 %	Rectangular	$\sqrt{3}$	1	±2.9 %	∞
Phantom and Setup			_	_		
Phantom Uncertainty	±4.0 %	Rectangular	$\sqrt{3}$	1	±2.3 %	∞
Liquid Conductivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.64	±1.8 %	∞
Liquid Conductivity (meas.)	±2.5 %	Normal	1	0.64	±1.6 %	8
Liquid Permittivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.6	±1.7 %	∞
Liquid Permittivity (meas.)	±2.5 %	Normal	1	0.6	±1.5 %	∞
Combined Std. Uncertainty					±12.9 %	330
Coverage Factor for 95%	Kp=2					
Expanded STD Uncertainty					±25.9 %	

Table 7.3 Uncertainty Budget of DASY4 for 5GHz Band



8. SAR Measurement Evaluation

Each DASY4 system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY4 software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

8.1 Purpose of System Performance Check

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

8.2 System Setup

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave that comes from a signal generator at frequency 2450 MHz, 5200 MHz, and 5800 MHz. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

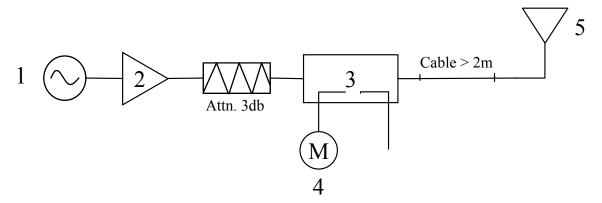


Fig. 8.1 System Setup for System Evaluation



- 1. Signal Generator
- 2. Amplifier
- 3. Directional Coupler
- 4. Power Meter
- 5. 2450 or 5200 or 5800 MHz Dipole

The output power on dipole port must be calibrated to 100 mW (20 dBm) before dipole is connected.

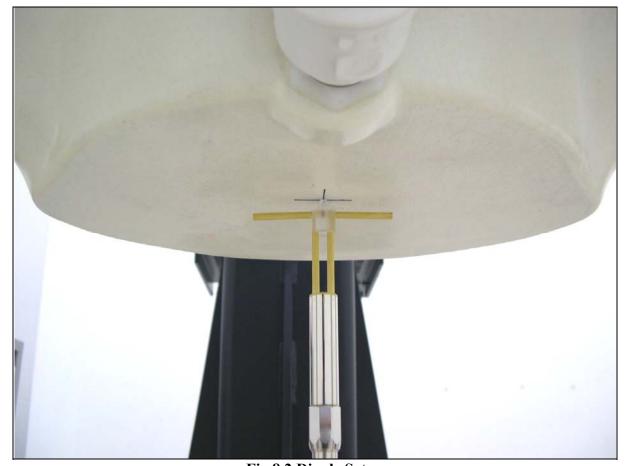


Fig 8.2 Dipole Setup



8.3 Validation Results

Comparing to the original SAR value provided by SPEAG, the validation data should within its specification of 10 %. Table 8.1 shows the target SAR and measured SAR after normalized to 1W input power.

Frequency	SAR	Target (W/kg)	Measurement data (W/kg)	Variation	Measurement date	
2450MHz	SAR (1g)	52.5	55.6	5.9 %	Aug 00 2008	
2450MHZ	SAR (10g)	24.4	26.5	8.6 %	Aug. 09, 2008	
5200MHz	SAR (1g)	76.8	77.5	0.9 %	Aug. 11, 2008	
	SAR (10g)	21.6	22.0	1.9 %		
5800MHz	SAR (1g)	69.4	68.5	-1.3 %	Aug 11 2000	
	SAR (10g)	19.3	18.7	-3.1 %	Aug. 11, 2008	

Table 8.1 Target and Measured SAR after Normalized

The table above indicates the system performance check can meet the variation criterion.

9. <u>Description for DUT Testing Position</u>

This DUT was tested in two different positions. They are "Bottom Side with 0cm Gap", and "Rear Face with 0cm Gap".

Test Report No : FA840719

Remark: Please refer to Appendix E for the test setup photos.



10.Measurement Procedures

The measurement procedures are as follows:

- ➤ Using engineering software to transmit RF power continuously (continuous Tx) in the low channel
- Placing the DUT in the positions described in the last section
- Setting scan area, grid size and other setting on the DASY4 software
- Taking data for the low channel
- Repeat the previous steps for the middle and high channels.

According to the IEEE P1528 draft standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- > Power reference measurement
- > Area scan
- Zoom scan
- Power reference measurement

10.1 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1528-2003 standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY4 software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

Base on the Draft: SCC-34, SC-2, WG-2-Computational Dosimetry, P1528/D1.2 (Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques), a new algorithm has been implemented. The spatial-peak SAR can be computed over any required mass.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.

The entire evaluation of the spatial peak values is performed within the post-processing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- extraction of the measured data (grid and values) from the Zoom Scan
- calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- generation of a high-resolution mesh within the measured volume
- interpolation of all measured values form the measurement grid to the high-resolution grid
- extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- calculation of the averaged SAR within masses of 1g and 10g



10.2 Scan Procedures

First Area Scan is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an Area Scan is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, Zoom Scan is required. The Zoom Scan measures 5x5x7 points with step size 8, 8 and 5 mm for 802.11b/g and 8x8x8 points with step size 4.3, 4.3 and 3 mm for 802.11a. The Zoom Scan is performed around the highest E-field value to determine the averaged SAR-distribution over 1 g.

10.3 SAR Averaged Methods

In DASY4, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.



11. SAR Test Results

11.1 Conducted Power

	802.11b			802.11g			
Channel	Data Rate (Mbps)	Power Setting	Peak Power (dBm)	Data Rate (Mbps)	Power Setting	Peak Power (dBm)	
1	1M	18	20.39	6M	20	24.12	
6	1M	18	20.15	6M	20	24.09	
11	1M	18	20.63	6M	20	24.13	

	802.11a				
Channel	Data Rate (Mbps)	Power Setting	Peak Power (dBm)		
36	6M	9.5	16.95		
52	6M	12.0	18.86		
64	6M	11.5	18.65		
149	6M	15.0	20.33		
157	6M	15.0	20.39		
165	6M	15.0	20.08		

11.2 Test Record

Position	Band	Chan.	Freq. (MHz)	Modulation Type	Measured 1g SAR (W/kg)	Power Drift	Limit (W/kg)	Result
Rear Face with 0cm Gap	802.11b	6	2437	CCK	0.516	0.193	1.6	Pass
Bottom Side with 0cm Gap	802.11b	6	2437	CCK	0.00978	0.189	1.6	Pass
Rear Face with 0cm Gap	802.11g	6	2437	OFDM	0.646	0.191	1.6	Pass
Rear Face with 0cm Gap	802.11g	1	2412	OFDM	0.789	0.169	1.6	Pass
Rear Face with 0cm Gap	802.11g	11	2462	OFDM	0.684	0.17	1.6	Pass
Rear Face with 0cm Gap	802.11a	52	5260	OFDM	0.172	0.181	1.6	Pass
Bottom Side with 0cm Gap	802.11a	52	5260	OFDM	N/A	N/A	1.6	Pass
Rear Face with 0cm Gap	802.11a	36	5180	OFDM	0.045	0.16	1.6	Pass
Rear Face with 0cm Gap	802.11a	64	5320	OFDM	0.302	0	1.6	Pass
Rear Face with 0cm Gap	802.11a	157	5785	OFDM	0.426	0.188	1.6	Pass
Bottom Side with 0cm Gap	802.11a	157	5785	OFDM	0.00156	0.199	1.6	Pass
Rear Face with 0cm Gap	802.11a	149	5745	OFDM	0.365	0.156	1.6	Pass
Rear Face with 0cm Gap	802.11a	165	5825	OFDM	0.497	0.199	1.6	Pass

Test Engineer: Gordon Lin and Jason



12.Reference

- [1] FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2] IEEE Std. P1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", April 21, 2003.
- [3] Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 97-01), "Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to RF Emissions", June 2001
- [4] IEEE Std. C95.3-2002, "IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields-RF and Microwave", 2002
- [5] IEEE Std. C95.1-1999, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", 1999
- [6] Robert J. Renka, "Multivariate Interpolation Of Large Sets Of Scattered Data", University of North Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988, pp. 139-148
- [7] DASY4 System Handbook



Appendix A - System Performance Check Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab Date: 2008/8/9

System Check_Body_2450MHz

DUT: Dipole 2450 MHz

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL_2450 Medium parameters used: f = 2450 MHz; $\sigma = 1.93$ mho/m; $\epsilon_r = 53.8$; $\rho = 1000$ kg/m³

Ambient Temperature : 22.9 °C; Liquid Temperature : 21.4 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.02, 4.02, 4.02); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 6.41 mW/g


Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.8 V/m; Power Drift = 0.006 dB

Peak SAR (extrapolated) = 11.8 W/kg

SAR(1 g) = 5.56 mW/g; SAR(10 g) = 2.65 mW/g

Maximum value of SAR (measured) = 6.26 mW/g

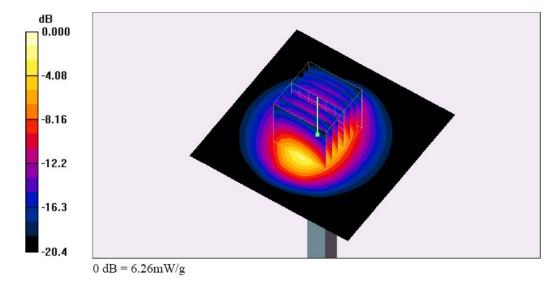



System Check Body 5200MHz

DUT: Dipole 5GHz

Communication System: CW; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: MSL_5000~6000 Medium parameters used: f = 5200 MHz; $\sigma = 5.33$ mho/m; $\epsilon_r = 48.6$; $\rho = 1000$ kg/m³

Ambient Temperature: 22.6°C; Liquid Temperature: 21.3°C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.34, 4.34, 4.34); Calibrated: 2008/1/31
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm


Maximum value of SAR (interpolated) = 14.4 mW/g

Pin=100mW/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 53.6 V/m; Power Drift = -0.033 dB

Peak SAR (extrapolated) = 29.2 W/kg

SAR(1 g) = 7.75 mW/g; SAR(10 g) = 2.2 mW/gMaximum value of SAR (measured) = 12.8 mW/g

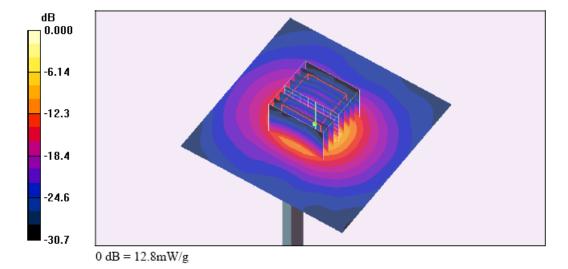



System Check Body 5800MHz

DUT: Dipole 5GHz

Communication System: 802.11a; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: MSL_5000~6000 Medium parameters used: f = 5800 MHz; $\sigma = 6.11 \text{ mho/m}$; $\epsilon_r = 47.4$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.6°C; Liquid Temperature: 21.3°C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.2, 4.2, 4.2); Calibrated: 2008/1/31
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm


Maximum value of SAR (interpolated) = 14.6 mW/g

Pin=100mW/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 50.4 V/m; Power Drift = -0.098 dB

Peak SAR (extrapolated) = 32.6 W/kg

SAR(1 g) = 6.85 mW/g; SAR(10 g) = 1.87 mW/gMaximum value of SAR (measured) = 13.9 mW/g

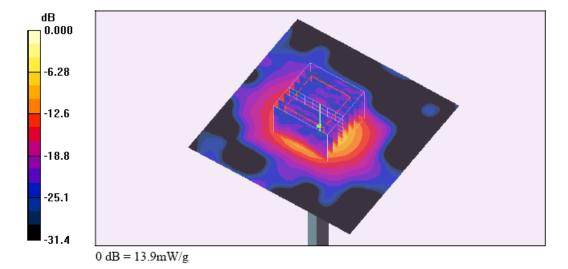



Appendix B - SAR Measurement Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab Date: 2008/8/9

Body_802.11b Ch6_Bottom Side with 0cm Gap

DUT: 840719

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL_2450 Medium parameters used: f = 2437 MHz; $\sigma = 1.92$ mho/m; $\epsilon_r = 53.9$; $\rho = 1000$ kg/m³

Ambient Temperature: 22.9 °C; Liquid Temperature: 21.4 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.02, 4.02, 4.02); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch6/Area Scan (221x61x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.012 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 0.000 V/m; Power Drift = 0.189 dB

Peak SAR (extrapolated) = 0.037 W/kg

SAR(1 g) = 0.00978 mW/g; SAR(10 g) = 0.00443 mW/g

Maximum value of SAR (measured) = 0.012 mW/g


Ch6/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 0.000 V/m; Power Drift = 0.189 dB

Peak SAR (extrapolated) = 0.013 W/kg

SAR(1 g) = 0.00705 mW/g; SAR(10 g) = 0.00401 mW/g

Maximum value of SAR (measured) = 0.008 mW/g

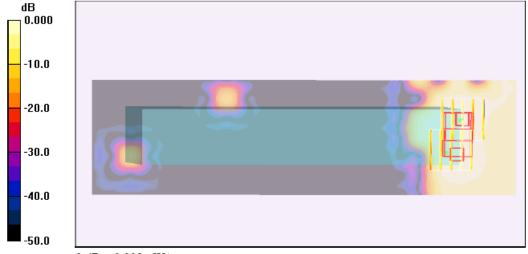

0 dB = 0.008 mW/g



Body_802.11g Ch1_Rear Face with 0cm Gap

DUT: 840719

Communication System: 802.11g; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: MSL_2450 Medium parameters used: f = 2412 MHz; $\sigma = 1.89$ mho/m; $\epsilon_r = 54$; $\rho = 1000$ kg/m³

Ambient Temperature: 22.9 °C; Liquid Temperature: 21.4 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.02, 4.02, 4.02); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch1/Area Scan (101x81x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.961 mW/g


Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 0.178 V/m; Power Drift = 0.169 dB

Peak SAR (extrapolated) = 1.72 W/kg

SAR(1 g) = 0.789 mW/g; SAR(10 g) = 0.373 mW/g

Maximum value of SAR (measured) = 0.889 mW/g

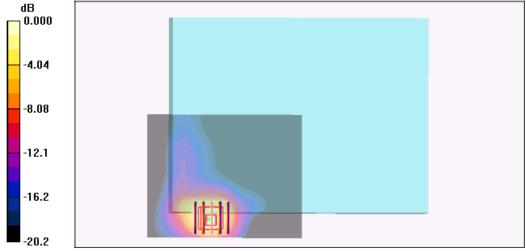

0 dB = 0.889 mW/g



Body_802.11a Ch64_Rear Face With 0cm Gap

DUT: 840719

Communication System: 802.11a; Frequency: 5320 MHz; Duty Cycle: 1:1

Medium: MSL 5000~6000 Medium parameters used: f = 5320 MHz; $\sigma = 5.5 \text{ mho/m}$; $\epsilon_r = 48.4$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 22.7 °C; Liquid Temperature: 21.3 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.06, 4.06, 4.06); Calibrated: 2008/1/31
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch64/Area Scan (101x101x1): Measurement grid: dx=10mm, dy=10mm


Maximum value of SAR (interpolated) = 0.630 mW/g

Ch64/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 0.000 V/m; Power Drift = 0.000 dB

Peak SAR (extrapolated) = 1.14 W/kg

SAR(1 g) = 0.302 mW/g; SAR(10 g) = 0.114 mW/gMaximum value of SAR (measured) = 0.591 mW/g

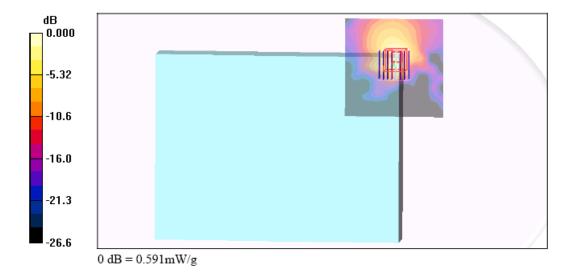



Body_802.11a Ch157_Bottom Side With 0cm Gap

DUT: 840719

Communication System: 802.11a; Frequency: 5785 MHz; Duty Cycle: 1:1

Medium: MSL_5000~6000 Medium parameters used: f = 5785 MHz; $\sigma = 6.09$ mho/m; $\epsilon_r = 47.4$; $\rho = 1000$ kg/m³

Ambient Temperature: 22.7 °C; Liquid Temperature: 21.3 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.2, 4.2, 4.2); Calibrated: 2008/1/31
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch157/Area Scan (101x331x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.002 mW/g


Ch157/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 0.000 V/m; Power Drift = 0.199 dB

Peak SAR (extrapolated) = 0.027 W/kg

SAR(1 g) = 0.00156 mW/g; SAR(10 g) = 0.000496 mW/g

Maximum value of SAR (measured) = 0.010 mW/g

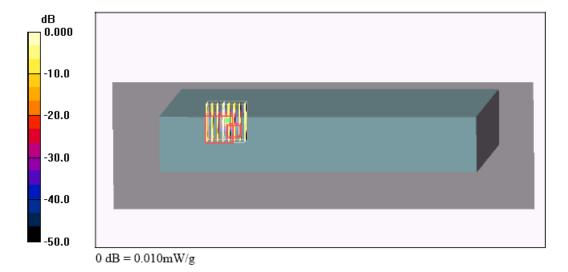



Body_802.11a Ch165_Rear Face With 0cm Gap

DUT: 840719

Communication System: 802.11a; Frequency: 5825 MHz; Duty Cycle: 1:1

Medium: MSL_5000~6000 Medium parameters used: f = 5825 MHz; $\sigma = 6.13$ mho/m; $\epsilon_r = 47.2$; $\rho = 1000$ kg/m³

Ambient Temperature: 22.6 °C; Liquid Temperature: 21.3 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.2, 4.2, 4.2); Calibrated: 2008/1/31
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch165/Area Scan (111x111x1): Measurement grid: dx=10mm, dy=10mm


Maximum value of SAR (interpolated) = 0.955 mW/g

Ch165/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 0.000 V/m; Power Drift = 0.199 dB

Peak SAR (extrapolated) = 2.08 W/kg

SAR(1 g) = 0.497 mW/g; SAR(10 g) = 0.173 mW/g Maximum value of SAR (measured) = 0.966 mW/g

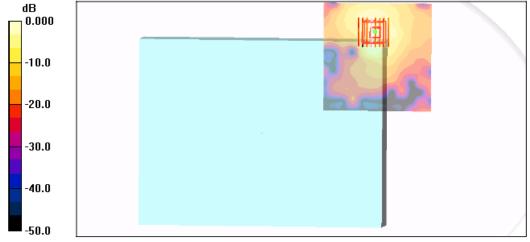



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab Date: 2008/8/9

Body 802.11g Ch1 Rear Face with 0cm Gap 2D

DUT: 840719

Communication System: 802.11g; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: MSL_2450 Medium parameters used: f = 2412 MHz; $\sigma = 1.89$ mho/m; $\varepsilon_r = 54$; $\rho = 1000$ kg/m³

Ambient Temperature: 22.9 °C; Liquid Temperature: 21.4 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.02, 4.02, 4.02); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch1/Area Scan (101x81x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 0.961 mW/g

Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 0.178 V/m; Power Drift = 0.169 dB

Peak SAR (extrapolated) = 1.72 W/kg

SAR(1 g) = 0.789 mW/g; SAR(10 g) = 0.373 mW/gMaximum value of SAR (measured) = 0.889 mW/g

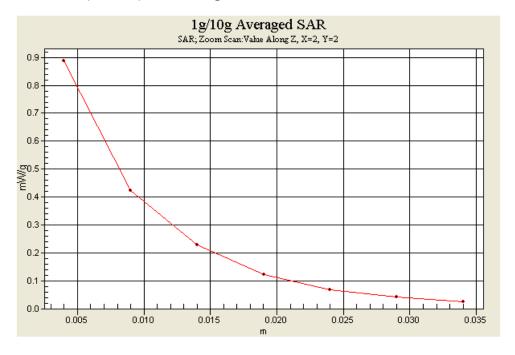



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab Date: 2008/8/11

Body 802.11a Ch64 Rear Face With 0cm Gap 2D

DUT: 840719

Communication System: 802.11a; Frequency: 5320 MHz; Duty Cycle: 1:1

Medium: MSL_5000~6000 Medium parameters used: f = 5320 MHz; $\sigma = 5.5$ mho/m; $\epsilon_r = 48.4$; $\rho = 1000$ kg/m³

Ambient Temperature: 22.7 °C; Liquid Temperature: 21.3 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.06, 4.06, 4.06); Calibrated: 2008/1/31
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch64/Area Scan (101x101x1): Measurement grid: dx=10mm, dy=10mm


Maximum value of SAR (interpolated) = 0.630 mW/g

Ch64/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 0.000 V/m; Power Drift = 0.000 dB

Peak SAR (extrapolated) = 1.14 W/kg

SAR(1 g) = 0.302 mW/g; SAR(10 g) = 0.114 mW/gMaximum value of SAR (measured) = 0.591 mW/g

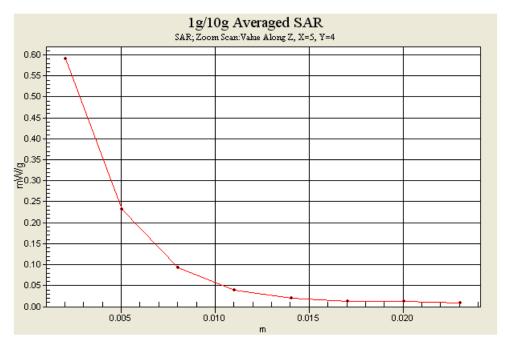



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab Date: 2008/8/11

Body 802.11a Ch165 Rear Face With 0cm Gap 2D

DUT: 840719

Communication System: 802.11a; Frequency: 5825 MHz; Duty Cycle: 1:1

Medium: MSL_5000~6000 Medium parameters used: f = 5825 MHz; $\sigma = 6.13$ mho/m; $\epsilon_r = 47.2$; $\rho = 1000$ kg/m³

Ambient Temperature: 22.6 °C; Liquid Temperature: 21.3 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.2, 4.2, 4.2); Calibrated: 2008/1/31
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2007/9/17
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch165/Area Scan (111x111x1): Measurement grid: dx=10mm, dy=10mm


Maximum value of SAR (interpolated) = 0.955 mW/g

Ch165/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 0.000 V/m; Power Drift = 0.199 dB

Peak SAR (extrapolated) = 2.08 W/kg

SAR(1 g) = 0.497 mW/g; SAR(10 g) = 0.173 mW/gMaximum value of SAR (measured) = 0.966 mW/g

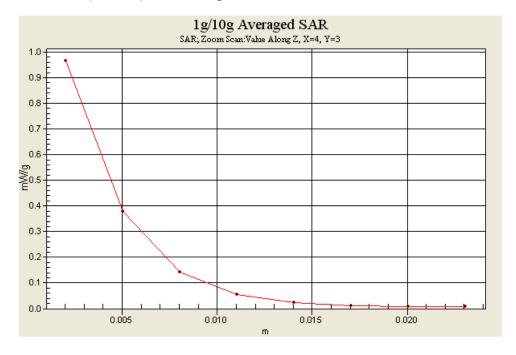



Appendix C - Calibration Data

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerlscher Kallbrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client S

Sporton (Auden)

Certificate No: D2450V2-736_Jul07

Accreditation No.: SCS 108

Object	D2450V2 - SN: 7	36	
Calibration procedure(s)	QA CAL-05.v6 Calibration proce	dure for dipole validation kits	
Calibration date:	July 12, 2007		
Condition of the calibrated item	In Tolerance		
All calibrations have been condu	cted in the closed shoreton		
		ry facility: environment temperature (22 ± 3)°C and	d humidity < 70%.
Calibration Equipment used (M& Primary Standards		ry facility: environment temperature (22 ± 3)*C and Cal Date (Calibrated by, Certificate No.)	d humidity < 70%. Scheduled Calibration
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV3	TE critical for calibration)		
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV3 DAE4	TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN 3025 SN 601	Cal Date (Calibrated by, Certificate No.) 03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No. 217-00591) 10-Aug-06 (METAS, No. 217-00591) 19-Oct-06 (SPEAG, No. ES3-3025_Oct06) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07 Jan-08
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV3	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN 3025	Cal Date (Calibrated by, Certificate No.) 03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591) 19-Oct-06 (SPEAG, No. ES3-3025_Oct06)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator Agilent E4421B	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN 3025 SN 601 ID # MY41092317 MY41090675 US37390585 S4206	Cal Date (Calibrated by, Certificate No.) 03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591) 19-Oct-06 (SPEAG, No. ES3-3025_Oct06) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Oct-06)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07 Jan-08 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Oct-07
Calibration Equipment used (M&Primary Standards Power meter EPM-442A Power sensor HP 8431A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator Agilent E4421B Network Analyzer HP 8753E	TE critical for calibration) ID #	Cal Date (Calibrated by, Certificate No.) 03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591) 19-Oct-06 (SPEAG, No. ES3-3025_Oct06) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Oct-06)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07 Jan-08 Scheduled Check In house check: Oct-07 In house check: Nov-07
Calibration Equipment used (M&Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator Agilent E4421B	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN 3025 SN 601 ID # MY41092317 MY41090675 US37390585 S4206	Cal Date (Calibrated by, Certificate No.) 03-Oct-06 (METAS, No. 217-00608) 03-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No 217-00591) 10-Aug-06 (METAS, No 217-00591) 19-Oct-06 (SPEAG, No. ES3-3025_Oct06) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Oct-06)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07 Jan-08 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Oct-07

Certificate No: D2450V2-736_Jul07

Page 1 of 9



Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S

Service suisse d'étalonnage

C Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z

N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D2450V2-736_Jul07

Page 2 of 9



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.6 ± 6 %	1.81 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm3 (1 g) of Head TSL	condition	
SAR measured	250 mW input power	13.3 mW / g
SAR normalized	normalized to 1W	53.2 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	52.7 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.17 mW / g
SAR normalized	normalized to 1W	24.7 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	24.5 mW / g ± 16.5 % (k=2)

Certificate No: D2450V2-736_Jul07

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.5 ± 6 %	1.94 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.0 mW / g
SAR normalized	normalized to 1W	52.0 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	52.5 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	6.05 mW / g
SAR normalized	normalized to 1W	24.2 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	24.4 mW / g ± 16.5 % (k=2)

Certificate No: D2450V2-736_Jul07

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.1 Ω + 3.0 jΩ	
Return Loss	- 27.6 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$48.7 \Omega + 4.6 j\Omega$	
Return Loss	- 26.3 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.158 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	August 26, 2003

Certificate No: D2450V2-736_Jul07

Page 5 of 9



DASY4 Validation Report for Head TSL

Date/Time: 12.07.2007 11:00:03

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB;

Medium parameters used: f = 2450 MHz; $\sigma = 1.81$ mho/m; $\varepsilon_r = 38.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section


Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025 (HF); ConvF(4.5, 4.5, 4.5); Calibrated: 19.10.2006
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 93.0 V/m; Power Drift = -0.004 dB Peak SAR (extrapolated) = 28.1 W/kg SAR(1 g) = 13.3 mW/g; SAR(10 g) = 6.17 mW/g Maximum value of SAR (measured) = 15.0 mW/g

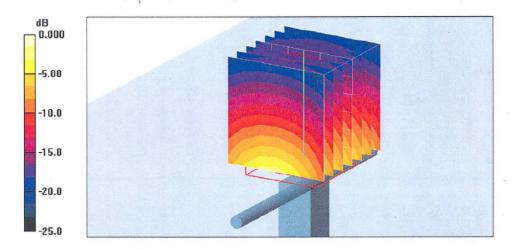


0~dB=15.0mW/g

Certificate No: D2450V2-736_Jul07

Page 6 of 9



Impedance Measurement Plot for Head TSL

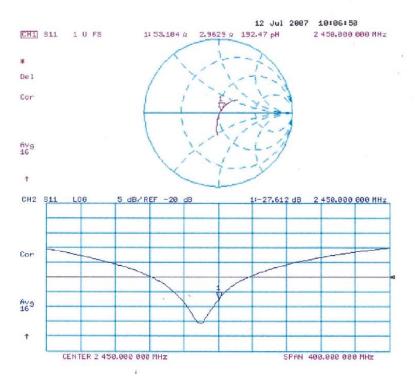

Certificate No: D2450V2-736_Jul07

Page 7 of 9



DASY4 Validation Report for Body TSL

Date/Time: 12.07.2007 12:28:49

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U10 BB;

Medium parameters used: f = 2450 MHz; $\sigma = 1.94$ mho/m; $\varepsilon_r = 53.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025 (HF); ConvF(4.16, 4.16, 4.16); Calibrated: 19.10.2006
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 88.6 V/m; Power Drift = 0.005 dB

Peak SAR (extrapolated) = 27.0 W/kg

SAR(1 g) = 13 mW/g; SAR(10 g) = 6.05 mW/g

Maximum value of SAR (measured) = 14.8 mW/g

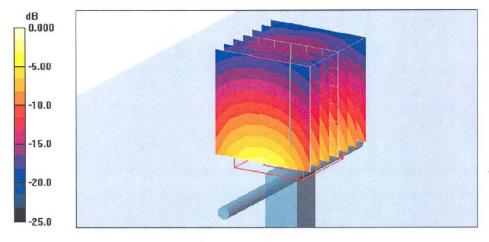


0 dB = 14.8 mW/g

Certificate No: D2450V2-736_Jul07

Page 8 of 9



Impedance Measurement Plot for Body TSL

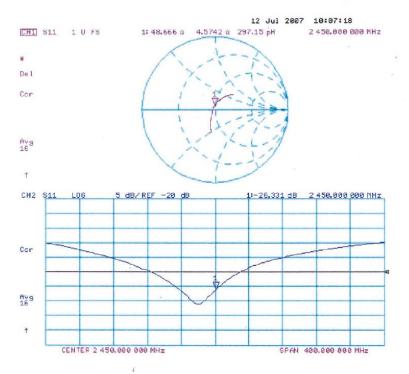

Certificate No: D2450V2-736_Jul07

Page 9 of 9



Calibration Laboratory of Schmid & Partner

Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

Sporton (Auden)

CALIBRATION CERTIFICATE

Accreditation No.: SCS 108

Certificate No: D5GHzV2-1006_Jan08

Calibration procedure(s) QA CAL-22.V1 Calibration procedure for dipole validation kits between 3-6 GHz Calibration date: January 24, 2008 Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Calibrated by, Certificate No.) Scheduled Calibration

ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
GB37480704	04-Oct-07 (METAS, No. 217-00736)	Oct-08
US37292783	04-Oct-07 (METAS, No. 217-00736)	Oct-08
SN: S5072.1 (20g)	07-Aug-07 (METAS, No 217-00718)	Aug-08
SN: 3503	9-Mar-07 (SREAG, No. EX3-3503_Mar07)	Mar-08
SN 601	3-Jan-08 (SPEAG, No. DAE4-601_Jan08)	Jan-09
ID#	Check Date (in house)	Scheduled Check
100005	4-Aug-99 (SPEAG, in house check Oct-07)	In house check: Oct-09
US37390585 S4206	18-Oct-01 (SPEAG, in house check Oct-07)	In house check: Oct-08
GB43310788	13-Aug-03 (SPEAG, in house check Oct-07)	In house check: Oct-08
MY41093315	10-Aug-03 (SPEAG, in house check Oct-07)	In house check: Oct-08
	~	
Name	Function -	Signature
Mike Meili	Laboratory Technician	T. Meili
Katja Pokovic	Technical Manager	eller Wil-
	GB37480704 US37292783 SN: S5072.1 (20g) SN: 3503 SN 601 ID # 100005 US37390585 S4206 GB43310788 MY41093315 Name Mike Meili	GB37480704 04-Oct-07 (METAS, No. 217-00736) US37292783 04-Oct-07 (METAS, No. 217-00736) SN: S5072.1 (20g) 07-Aug-07 (METAS, No. 217-00718) SN: 3503 9-Mar-07 (SREAG, No. EX3-3503_Mar07) SN 601 3-Jan-08 (SPEAG, No. DAE4-601_Jan08) ID # Check Date (in house) 100005 4-Aug-99 (SPEAG, in house check Oct-07) US37390585 S4206 18-Oct-01 (SPEAG, in house check Oct-07) GB43310788 13-Aug-03 (SPEAG, in house check Oct-07) MY41093315 10-Aug-03 (SPEAG, in house check Oct-07) Name Function Mike Meili Laboratory Technician

Certificate No: D5GHzV2-1006_Jan08

Page 1 of 14

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Issued: January 24, 2008

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Accircultation

Accreditation No.: SCS 108

Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC Std 62209 Part 2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation, and Procedures"; Part 2: "Procedure to determine the Specific Absorption Rate (SAR) for including accessories and multiple transmitters", Draft Version 0.9, December 2004
- b) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

c) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D5GHzV2-1006 Jan08

Page 2 of 14



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Area Scan resolution	dx, dy = 10 mm	14
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 2.5 mm	
Frequency	5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5200 MHz The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.0 ± 6 %	4.53 mho/m ± 6 %
Head TSL temperature during test	(21.2 ± 0.2) °C	****	

SAR result with Head TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	100 mW input power	8.24 mW / g
SAR normalized	normalized to 1W	82.4 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	82.4 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.31 mW / g
SAR normalized	normalized to 1W	23.1 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	23.0 mW / g ± 19.5 % (k=2)

Certificate No: D5GHzV2-1006_Jan08

Page 3 of 14

¹ Correction to nominal TSL parameters according to c), chapter "SAR Sensitivities



Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.5 ± 6 %	4.81 mho/m ± 6 %
Head TSL temperature during test	(21.1 ± 0.2) °C		

SAR result with Head TSL at 5500 MHz

SAR averaged over 1 cm3 (1 g) of Head TSL	condition	
SAR measured	100 mW input power	8.63 mW / g
SAR normalized	normalized to 1W	86.3 mW / g
SAR for nominal Head TSL parameters 2	normalized to 1W	86.2 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2,42 mW / g
SAR normalized	normalized to 1W	24.2 mW / g
SAR for nominal Head TSL parameters 2	normalized to 1W	24.1 mW / g ± 19.5 % (k=2)

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	5.11 mho/m ± 6 %
Head TSL temperature during test	(21.0 ± 0.2) °C		

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	100 mW input power	8.13 mW / g
SAR normalized	normalized to 1W	81.3 mW / g
SAR for nominal Head TSL parameters 2	normalized to 1W	80.8 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.27 mW / g
SAR normalized	normalized to 1W	22.7 mW / g
SAR for nominal Head TSL parameters 2	normalized to 1W	22.5 mW / g ± 19.5 % (k=2)

Certificate No: D5GHzV2-1006 Jan08

Page 4 of 14

² Correction to nominal TSL parameters according to c), chapter "SAR Sensitivities

Body TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	49.0	5.30 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.3 ± 6 %	5.27 mho/m ± 6 %
Body TSL temperature during test	(20.7 ± 0.2) °C		

SAR result with Body TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	condition	
SAR measured	100 mW input power	7.77 mW / g
SAR normalized	normalized to 1W	77.7 mW / g
SAR for nominal Body TSL parameters ³	normalized to 1W	76.8 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition)!
SAR measured	100 mW input power	2.18 mW / g
SAR normalized	normalized to 1W	21.8 mW / g
SAR for nominal Body TSL parameters ³	normalized to 1W	21.6 mW / g ± 19.5 % (k=2)

Body TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.6	5.65 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.6 ± 6 %	5.62 mho/m ± 6 %
Body TSL temperature during test	(20.7 ± 0.2) °C	****	

SAR result with Body TSL at 5500 MHz

SAR averaged over 1 cm3 (1 g) of Body TSL	condition	
SAR measured	100 mW input power	8.12 mW / g
SAR normalized	normalized to 1W ,	81.2 mW / g
SAR for nominal Body TSL parameters ³	normalized to 1W	80.1 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	A D
SAR measured	100 mW input power	2.26 mW / g
SAR normalized	normalized to 1W *	22.6 mW / g
SAR for nominal Body TSL parameters ³	normalized to 1W	22.3 mW / g ± 19.5 % (k=2)

Certificate No: D5GHzV2-1006_Jan08

Page 5 of 14

⁹ Correction to nominal TSL parameters according to c), chapter "SAR Sensitivities



Body TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.2	6.00 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	46.0 ± 6 %	6.04 mho/m ± 6 %
Body TSL temperature during test	(20.6 ± 0.2) °C		

SAR result with Body TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	condition	
SAR measured	100 mW input power	7.04 mW / g
SAR normalized	normalized to 1W	70.4 mW / g
SAR for nominal Body TSL parameters ⁴	normalized to 1W	69.4 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	1.95 mW / g
SAR normalized	normalized to 1W	19.5 mW / g
SAR for nominal Body TSL parameters 4	normalized to 1W	19.3 mW / g ± 19.5 % (k=2)

Certificate No: D5GHzV2-1006_Jan08

Page 6 of 14

⁴ Correction to nominal TSL parameters according to c), chapter "SAR Sensitivities



Appendix

Antenna Parameters with Head TSL at 5200 MHz

Impedance, transformed to feed point	52.7 Ω - 10.9 jΩ
Return Loss	-19.3 dB ·

Antenna Parameters with Head TSL at 5500 MHz

Impedance, transformed to feed point	49.4 Ω - 2.6 jΩ	
Return Loss	-31.2 dB	

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	56.0 Ω - 6.1 jΩ	
Return Loss	-21.9 dB	

Antenna Parameters with Body TSL at 5200 MHz

Impedance, transformed to feed point	52.8 Ω - 9.1 jΩ	
Return Loss	-20.7 dB	

Antenna Parameters with Body TSL at 5500 MHz

Impedance, transformed to feed point	49.3 Ω - 1.0 jΩ
Return Loss	-38.1 dB

Antenna Parameters with Body TSL at 5800 MHz

Impedance, transformed to feed point	56.1 Ω + 7.7 j Ω	
Return Loss	-20.7 dB	

Certificate No: D5GHzV2-1006_Jan08

General Antenna Parameters and Design

Electrical Delay (one direction)	1.202 ns

After long term use with 40 W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	August 28, 2003	

Certificate No: D5GHzV2-1006_Jan08

Page 8 of 14

DASY4 Validation Report for Head TSL

Date/Time: 18.01.2008 17:52:55

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1006

Communication System: CW-5GHz; Frequency: 5200 MHz, 5500 MHz, 5800 MHz; Duty Cycle: 1:1

Medium: HSL 5800 MHz;

Medium parameters used: f = 5200 MHz; $\sigma = 4.53$ mho/m; $\epsilon_r = 36$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5500 MHz; $\sigma = 4.81$ mho/m; $\epsilon_r = 35.5$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5800 MHz; $\sigma = 5.14$ mho/m; $\epsilon_r = 34.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: EX3DV4 SN3503; ConvF(5.56, 5.56, 5.56) ConvF(5.2, 5.2, 5.2) ConvF(4.97, 4.97, 4.97); Calibrated: 09.03.2007
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.01.2008
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

d=10mm, Pin=100mW, f=5200 MHz/Area Scan (91x91x1):

Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 17.6 mW/g

d=10mm, Pin=100mW, f=5200 MHz/Zoom Scan (8x8x10), dist=2mm (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 48.9 V/m; Power Drift = 0.055 dB

Peak SAR (extrapolated) = 31.1 W/kg

SAR(1 g) = 8.24 mW/g; SAR(10 g) = 2.31 mW/g

Maximum value of SAR (measured) = 16.1 mW/g

d=10mm, Pin=100mW, f=5500 MHz/Zoom Scan (8x8x10), dist=2mm 2 (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 48.1 V/m; Power Drift = 0.131 dB

Peak SAR (extrapolated) = 33.9 W/kg

SAR(1 g) = 8.63 mW/g; SAR(10 g) = 2.42 mW/g

Maximum value of SAR (measured) = 16.9 mW/g

d=10mm, Pin=100mW, f=5800 MHz/Zoom Scan (8x8x10), dist=2mm (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm


Reference Value = 45.2 V/m; Power Drift = 0.091 dB

Peak SAR (extrapolated) = 33.6 W/kg

SAR(1 g) = 8.13 mW/g; SAR(10 g) = 2.27 mW/g

Certificate No: D5GHzV2-1006_Jan08

Page 9 of 14

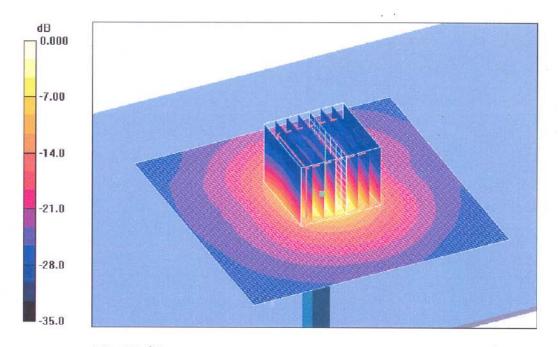


0 dB = 16.1 mW/g

Certificate No: D5GHzV2-1006_Jan08

Page 10 of 14



Impedance Measurement Plot for Head TSL

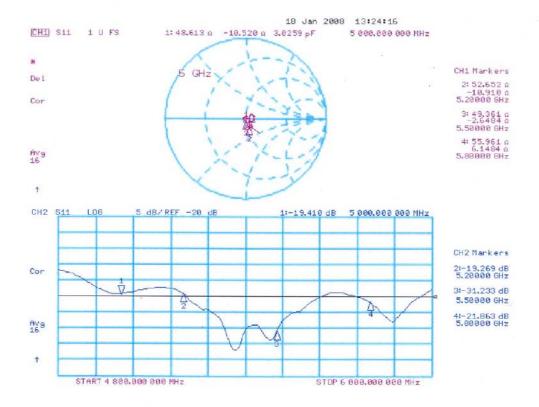

DASY4 Validation Report for Body TSL

Date/Time: 24.01.2008 15:14:55

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1006

Communication System: CW-5GHz; Frequency: 5200 MHz, 5500 MHz, 5800 MHz; Duty Cycle: 1:1

Medium: MSL 5800 MHz;

Medium parameters used: f = 5200 MHz; $\sigma = 5.37 \text{ mho/m}$; $\varepsilon_r = 47.3$; $\rho = 1000 \text{ kg/m}^3$

Medium parameters used: f = 5500 MHz; $\sigma = 5.73 \text{ mho/m}$; $\varepsilon_r = 46.6$; $\rho = 1000 \text{ kg/m}^3$

Medium parameters used: f = 5800 MHz; $\sigma = 6.16 \text{ mho/m}$; $\varepsilon_r = 46.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: EX3DV4 SN3503; ConvF(4.96, 4.96, 4.96)ConvF(4.63, 4.63, 4.63)ConvF(4.76, 4.76, 4.76); Calibrated: 09.03.2007
- · Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.01.2008
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

d=10mm, Pin=100mW, f=5200 MHz/Area Scan (61x61x1):

Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 17.0 mW/g

d=10mm, Pin=100mW, f=5200 MHz/Zoom Scan (8x8x10), dist=2mm (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 48.5 V/m; Power Drift = -0.066 dB

Peak SAR (extrapolated) = 28.0 W/kg

SAR(1 g) = 7.77 mW/g; SAR(10 g) = 2.18 mW/g

Maximum value of SAR (measured) = 15.5 mW/g

d=10mm, Pin=100mW, f=5500 MHz/Zoom Scan (8x8x10), dist=2mm (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 47.2 V/m; Power Drift = -0.067 dB

Peak SAR (extrapolated) = 32.2 W/kg

SAR(1 g) = 8.12 mW/g; SAR(10 g) = 2.26 mW/g

Maximum value of SAR (measured) = 16.6 mW/g

d=10mm, Pin=100mW, f=5800 MHz/Zoom Scan (8x8x10), dist=2mm (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 42.3 V/m; Power Drift = -0.131 dB


Peak SAR (extrapolated) = 28.9 W/kg

SAR(1 g) = 7.04 mW/g; SAR(10 g) = 1.95 mW/g

Maximum value of SAR (measured) = 14.5 mW/g

Certificate No: D5GHzV2-1006_Jan08


Page 12 of 14

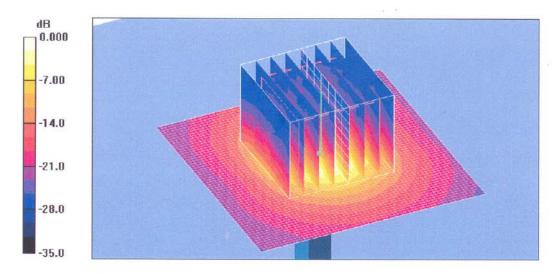

0 dB = 14.5 mW/g



Impedance Measurement Plot for Body TSL

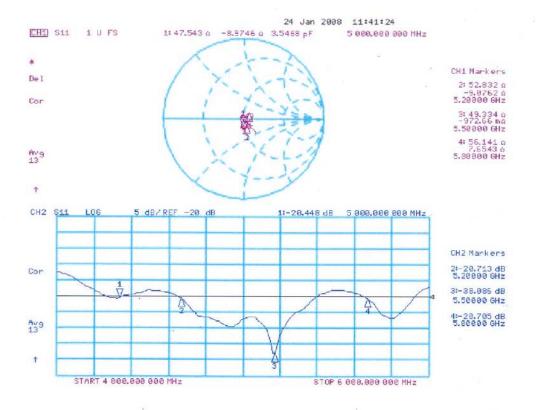



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 108

Certificate No: DAE4-778 Sep07

CALIBRATION CI	(Auden) ERTIFICATE		
Object	DAE4 - SD 000 D	04 BG - SN: 778	
Calibration procedure(s)	QA CAL-06.v12 Calibration proced	dure for the data acquisition elect	ronics (DAE)
Calibration date:	September 17, 20	007	
Condition of the calibrated item	In Tolerance		
All calibrations have been conducte Calibration Equipment used (M&TE		r facility: environment temperature (22 ± 3)°C	and humidity < 70%.
Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001	SN: 6295803 SN: 0810278	13-Oct-96 (Elcal AG, No: 5492) 03-Oct-96 (Elcal AG, No: 5478)	Oct-07 Oct-07
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Calibrator Box V1.1		25-Jun-07 (SPEAG, in house check)	In house check Jun-08
	2000000	200	
Calibrated by:	Name Dominique Steffen	Function Technician	Signature D Hulker
Approved by:	Fin Bomholt	R&D Director	.v. Relieue

Certificate No: DAE4-778_Sep07

Page 1 of 5

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schwelzerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE

data acquisition electronics

Connector angle

information used in DASY system to align probe sensor X to the robot

coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters contain technical information as a result from the performance test and require no uncertainty.
- DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
- Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
- Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
- AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
- Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
- Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
- Input resistance: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
- Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
- Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-778 Sep07

Page 2 of 5

DC Voltage Measurement

A/D - Converter Resolution nominal

Calibration Factors	χ .	Y	Z
High Range	404.715 ± 0.1% (k=2)	403.520 ± 0.1% (k=2)	405.065 ± 0.1% (k=2)
Low Range	3.99539 ± 0.7% (k=2)	3.96323 ± 0.7% (k=2)	3.97102 ± 0.7% (k=2)

Connector Angle

309°±1°

Certificate No: DAE4-778_Sep07



Appendix

1. DC Voltage Linearity

High Range	Input (μV)	Reading (μV)	Error (%)
Channel X + Input	200000	199999.5	0.00
Channel X + Input	20000	20004.41	0.02
Channel X - Input	20000	-20002.56	0.01
Channel Y + Input	200000	200000.3	0.00
Channel Y + Input	20000	20003.67	0.02
Channel Y - Input	20000	-20003.41	0.02
Channel Z + Input	200000	200000.3	0.00
Channel Z + Input	20000	20002.49	0.01
Channel Z - Input	20000	-20006.25	0.03

Low Range	Input (μV)	Reading (µV)	Error (%)
Channel X + Input	2000	1999.9	0.00
Channel X + Input	200	199.47	-0.26
Channel X - Input	200	-200.56	0.28
Channel Y + Input	2000	2000.1	0.00
Channel Y + Input	200	199.15	-0.43
Channel Y - Input	200	-200.77	0.39
Channel Z + Input	2000	2000	0.00
Channel Z + Input	200	199.22	-0.39
Channel Z - Input	200	-201.39	0.69

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	-6.00	-6.42
	- 200	7.17	6.60
Channel Y	200	-2.49	-2.64
	- 200	2.04	1.25
Channel Z	200	-10.83	-10.80
	- 200	9.19	8.80

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (µV)	Channel Z (μV)
Channel X	200	-	2.57	0.15
Channel Y	200	0.11	-	4.08
Channel Z	200	-1.80	1.03	-

Certificate No: DAE4-778_Sep07

Page 4 of 5



4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16068	16321
Channel Y	16180	16239
Channel Z	16405	16167

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

120	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	-0.14	-1.23	0.61	0.34
Channel Y	-0.85	-2.24	0.48	0.49
Channel Z	-1.24	-2.43	0.38	0.51

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	201.7
Channel Y	0.2000	201.7
Channel Z	0.1999	202.5

8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC	;)	
Supply (+ Vcc)	3	+7.9	
Supply (- Vcc)		-7.6	

9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)	
Supply (+ Vcc)	+0.0	<i>→</i> +6 ·	+14	
Supply (- Vcc)	-0.01	-8	-9	

Certificate No: DAE4-778_Sep07



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service sulsse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton (Auden)

Certificate No: ET3-1787_Aug07

Accreditation No.: SCS 108

Object	ET3DV6 - SN:1	787	
Calibration procedure(s)	QA CAL-01.v6 Calibration proc	edure for dosimetric E-field probes	
Calibration date:	August 28, 200	7	
Condition of the calibrated item	In Tolerance		
All calibrations have been condu	cted in the closed laborat	ory facility: environment temperature (22 ± 3)°C and	d humidity < 70%.
	9	Cal Date /Calibrated by Cardificate No.)	Schadulad Calibration
Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS: No. 217-00670)	Scheduled Calibration
Primary Standards Power meter E4419B	9	Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670)	Scheduled Calibration Mar-08 Mar-08
Primary Standards Power meter E4419B Power sensor E4412A	ID# GB41293874	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A	ID# GB41293874 MY41495277	29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670)	Mar-08 Mar-08
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5066 (20b)	29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00671)	Mar-08 Mar-08 Mar-08 Aug-08 Mar-08
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5066 (20b) SN: S5129 (30b)	29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00720)	Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5066 (20b)	29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00671)	Mar-08 Mar-08 Mar-08 Aug-08 Mar-08
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5096 (20b) SN: S5129 (30b) SN: 3013	29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07)	Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08 Jan-08
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3642U01700	29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) 20-Apr-07 (SPEAG, No. DAE4-654_Apr07)	Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08 Jan-08 Apr-08
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654	29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house)	Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08 Jan-08 Apr-08 Scheduled Check
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ID # GB41293874 MY41495277 MY41498087 SN: \$5054 (3c) SN: \$5056 (20b) SN: \$5129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585 Name	29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-0070) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-99 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Oct-06)	Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585	29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-99 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Oct-06)	Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07

Certificate No: ET3-1787_Aug07

Page 1 of 9

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL · NORMx,y,z tissue simulating liquid sensitivity in free space

ConF

sensitivity in TSL / NORMx,y,z

Polarization o

diode compression point φ rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at

measurement center), i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

 EC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This
 linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of
 the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1787_Aug07

Page 2 of 9



ET3DV6 SN:1787

August 28, 2007

Probe ET3DV6

SN:1787

Manufactured:

May 28, 2003

Last calibrated:

May 31, 2006

Recalibrated:

August 28, 2007

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)



ET3DV6 SN:1787

August 28, 2007

DASY - Parameters of Probe: ET3DV6 SN:1787

Sensitivity in Free Space ^A			Diode Compressio		3	
	NormX	1.63 ± 10.1%	$\mu V/(V/m)^2$	DCP X	92 mV	
	NormY	1.66 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	96 mV	
	NormZ	2.08 ± 10.1%	$\mu V/(V/m)^2$	DCP Z	91 mV	

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect

TSL	900 MHz	Typical SAR	gradient: 5 %	per mm

Sensor Cente	er to Phantom Surface Distance	3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	4.7	2.0
SAR _{be} [%]	With Correction Algorithm	0.1	0.0

TSL 1810 MHz Typical SAR gradient: 10 % per mm

Sensor Center	r to Phantom Surface Distance	3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	11.8	7.0
SAR _{be} [%]	With Correction Algorithm	0.2	0.4

Sensor Offset

Probe Tip to Sensor Center 2.7 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: ET3-1787_Aug07

Page 4 of 9

A The uncertainties of NormX,Y,Z do not affect the E2-field uncertainty inside TSL (see Page 8).


⁸ Numerical linearization parameter: uncertainty not required.

ET3DV6 SN:1787

August 28, 2007

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

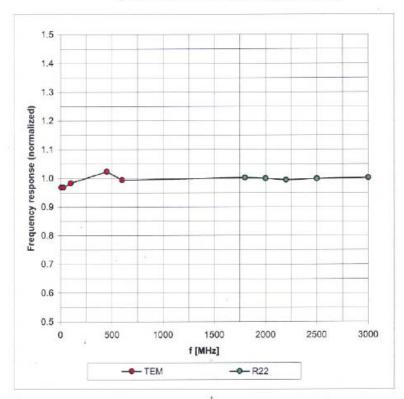


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Certificate No: ET3-1787_Aug07


Page 5 of 9

August 28, 2007

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

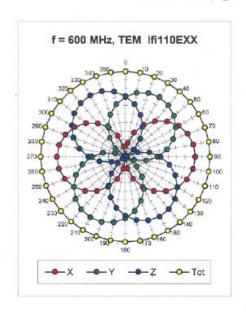



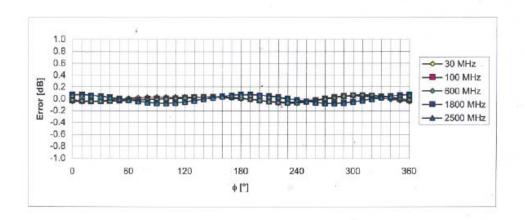

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Certificate No: ET3-1787_Aug07


Page 6 of 9

August 28, 2007

Dynamic Range f(SAR_{head})

(Waveguide R22, f = 1800 MHz)

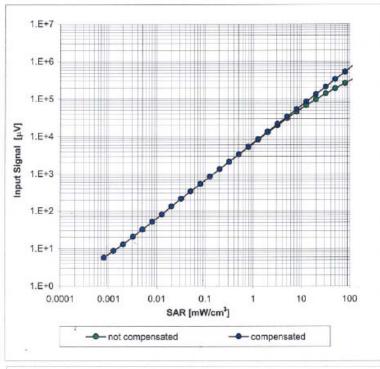

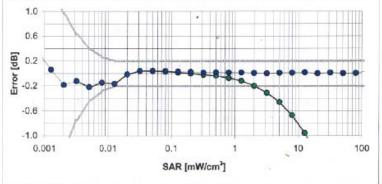

Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Certificate No: ET3-1787_Aug07


Page 7 of 9



August 28, 2007

Conversion Factor Assessment

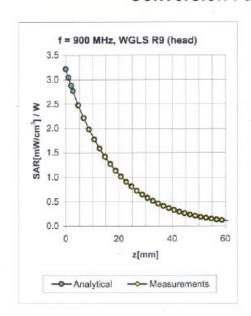

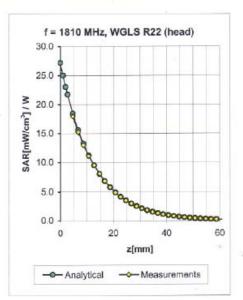

f [MHz]	Validity [MHz] ^c	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.32	2.42	6.58 ± 11.0% (k=2)
1810	± 50 / ± 100	Head	$40.0 \pm 5\%$	1.40 ± 5%	0.50	2.61	5.16 ± 11.0% (k=2)
2000	± 50 / ± 100	Head	$40.0 \pm 5\%$	1.40 ± 5%	0.55	2.45	4.80 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	0.67	1.81	4.50 ± 11.8% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.36	2.52	6.10 ± 11.0% (k=2)
1810	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.61	2.56	4.68 ± 11.0% (k=2)
2000	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.60	2.40	4.30 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.65	2.15	4.02 ± 11.8% (k=2)

Certificate No: ET3-1787_Aug07


Page 8 of 9

⁰ The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

August 28, 2007

Deviation from Isotropy in HSL

Error (6, 8), f = 900 MHz

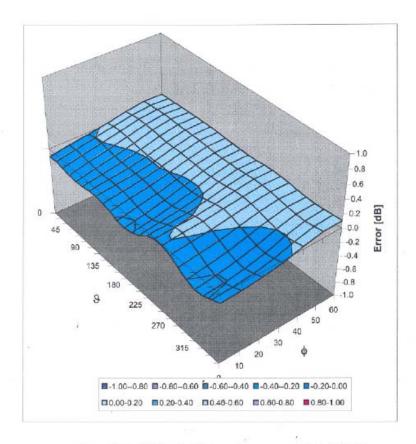

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ET3-1787_Aug07

Page 9 of 9

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 108

C

Calibration date: January 31, 2008 In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards D# Cal Date (Calibrated by, Certificate No.) Scheduled Calibration Power meter E4419B GB41293874 29-Mar-07 (METAS, No. 217-00670) Mar-08 Power sensor E4412A MY41498087 29-Mar-07 (METAS, No. 217-00670) Mar-08 Reference 3 dB Attenuator SN: \$5054 (3c) 8-Aug-07 (METAS, No. 217-00670) Aug-08 Reference 3 0 dB Attenuator SN: \$5084 (20) 29-Mar-07 (METAS, No. 217-00670) Aug-08 Reference 30 dB Attenuator SN: \$5086 (20) 29-Mar-07 (METAS, No. 217-00671) Aug-08 Reference 30 dB Attenuator SN: \$5084 (3c) SN: \$5086 (20) 29-Mar-07 (METAS, No. 217-00671) Aug-08 Reference 30 dB Attenuator Reference 30 dB Attenuator SN: \$5086 (20) 29-Mar-07 (METAS, No. 217-00671) Aug-08 Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator SN: \$5086 (20) 29-Mar-07 (METAS, No. 217-00671) Aug-08 Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator SN: \$5086 (20) 30: \$5086 (20)	Sporton (Aude	n)	Certific	cate No: EX3-3514_Jan08				
Calibration procedure(s) QA CAL-01.v6 and QA CAL.14.v3 Calibration procedure for dosimetric E-field probes Calibration procedure for dosimetric E-field probes Calibration procedure for dosimetric E-field probes Condition of the calibrated item In Tolerance Condition of the calibrated item In Tolerance Condition of the calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Calibrated by, Certificate No.) Scheduled Calibration Prover mature E4419B GB4128874 29-Mar-07 (METAS, No. 217-00670) Mar-08 Reference E4412A MY41498087 29-Mar-07 (METAS, No. 217-00670) Mar-08 Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 20 dB Attenuator SN: 55054 (3c) 8-Aug-07 (METAS, No. 217-0071) Aug-08 Reference 20 dB Attenuator Reference 20 dB Attenuator SN: 55058 (20b) 29-Mar-07 (METAS, No. 217-0077) Aug-08 Reference 20 dB Attenuator Reference 20 dB Attenuator SN: 55058 (3c) 8-Aug-07 (METAS, No. 217-0077) Aug-08 Reference Probe ES3DV2 SN: 3013 2-Jan 08 (SPEAG, No. E83-3013-Jan08) Jan-09	CALIBRATION C	CERTIFICAT						
Calibration procedure for dosimetric E-field probes Calibration date: January 31, 2008 In Tolerance Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Calibrated by, Certificate No.) Scheduled Calibration Prower meter E4419B GB41293874 29-Mar-07 (METAS, No. 217-00670) Mar-08 Prower sensor E4412A MY41495277 29-Mar-07 (METAS, No. 217-00670) Mar-08 Reference 3 dB Attenuator SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00670) Mar-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00670) Aug-08 Reference 30 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator Reference 30 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00719) Aug-08 SN: S508 (20b) 29-Mar-07 (METAS, No. 217-0071) Aug-08 Reference 30 dB Attenuator Reference 30 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Aug-08 SN: S508 (30b) 3013 2-Jan-08 (SPEAG, No. ES3-3013, Jan08) Jan-09 DAE4 SN: 654 20-Apr-07 (SPEAG, In house check Oct-07) In house check: Oct-08 Name Function Signature Calibrated by: Niels Kuster Quality Manager Niels Kuster Quality Manager	Object	EX3DV3 - SN:3	514					
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE-critical for calibration) Primary Standards ID #								
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Calibrated by, Certificate No.) Scheduled Calibration Power mater E4419B GB41293874 29-Mar-07 (METAS, No. 217-00670) Mar-08 Power sensor E4412A MY41495277 29-Mar-07 (METAS, No. 217-00670) Mar-08 Power sensor E4412A MY41496087 29-Mar-07 (METAS, No. 217-00670) Mar-08 Reference 3 dB Attenuator SN: \$5054 (3c) 8-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: \$5086 (20b) 29-Mar-07 (METAS, No. 217-0071) Mar-08 Reference 30 dB Attenuator SN: \$5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 2-Jan-08 (SPEAG, No. ES3-3013_Jan08) Jan-09 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (SPEAG, in house check Oct-07) In house check: Oct-08 Name Function Signature Calibrated by: Niels Kuster Quality Manager	Calibration date:	January 31, 200	18					
Power meter E4419B	Condition of the calibrated item	In Tolerance						
Power sensor E4412A MY41495277 29-Mar-07 (METAS, No. 217-00670) Mar-08 Power sensor E4412A MY41496087 29-Mar-07 (METAS, No. 217-00670) Mar-08 Reference 3 dB Attenuator SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 2-Jan-08 (SPEAG, No. ES3-3013_Jan08) Jan-09 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (SPEAG, in house check Oct-07) In house check: Oct-09 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Oct-07) In house check: Oct-08 Name Function Signature Calibrated by: Niels Kuster Quality Manager		ID#						
Prower sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 SN: S5129 (30b) S-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 2-Jan-08 (SPEAG, No. ES3-3013_Jan08) Jan-09 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Reference Probe ES3DV2 DAE4 ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 US37390585 US37390585 US37390585 Name Function Signature Calibrated by: Niels Kuster Quality Manager								
SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00719) Aug-08		A		A SECTION OF THE PROPERTY OF T				
Reference 20 dB Attenuator SN: \$5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: \$5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 2-Jan-08 (SPEAG, No. ES3-3013_Jan08) Jan-09 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (SPEAG, in house check Oct-07) In house check: Oct-09 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Oct-07) In house check: Oct-08 Name Function Signature Calibrated by: Niels Kuster Quality Manager								
Reference 30 dB Attenuator Reference Probe ES3DV2 Reference Probe ES								
Reference Probe ES3DV2 SN: 3013 2-Jan-08 (SPEAG, No. ES3-3013_Jan08) SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C Network Analyzer HP 8753E Name Function Signature Approved by: Niels Kuster Quality Manager Jan-09 Apr-08 Scheduled Check 4-Aug-99 (SPEAG, in house check Oct-07) In house check: Oct-09 In house check: Oct-09 Signature Quality Manager			•	* Commence				
Secondary Standards ID # Check Date (In house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (SPEAG, In house check Oct-07) In house check: Oct-09 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, In house check Oct-07) In house check: Oct-08 Name Function Signature Calibrated by: Katja Pokovic Technical Manager Niels Kuster Quality Manager								
RF generator HP 8648C Network Analyzer HP 8753E US3642U01700 US37390585 Name Function Function Signature Calibrated by: Niels Kuster Quality Manager			: 1915년 전 10 10 10 10 10 10 10 10 10 10 10 10 10					
Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, In house check Oct-07) In house check: Oct-08 Name Function Signature Calibrated by: Katja Pokovic Technical Manager Approved by: Niels Kuster Quality Manager	Secondary Standards	ID#	Check Date (in house)	Scheduled Check				
Calibrated by: Name Function Signature Calibrated by: Katja Pokovic Technical Manager Approved by: Niels Kuster Quality Manager	RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check					
Calibrated by: Katja Pokovic Technical Manager Approved by: Niels Kuster Quality Manager	Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check	Oct-07) In house check: Oct-08				
Approved by: Niels Kuster Quality Manager		DISTRICT SHAPE OF A STATE OF THE STATE OF	AND THE RESERVE OF THE PROPERTY OF THE PROPERT	Signature				
/ V/AN	Calibrated by:	Katja Pokovic	Technical Manager	politically				
leguadi Inguna 24 2009	Approved by:	Niels Kuster	Quality Manager	1/20				
				Issued: January 31, 2008				

Certificate No: EX3-3514_Jan08

Page 1 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst 5 Service suisse d'étalonnage C

Test Report No : FA840719

Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL NORMx,v,z tissue simulating liquid sensitivity in free space

ConF DCP

sensitivity in TSL / NORMx,y,z

Polarization φ

diode compression point φ rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at

measurement center), i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx, y,z: Assessed for E-field polarization θ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- . DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx, y, z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: EX3-3514_Jan08

Page 2 of 9



January 31, 2008

Probe EX3DV3

SN:3514

Manufactured:

December 15, 2002

Last calibrated:

February 21, 2007

Recalibrated:

January 31, 2008

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: EX3-3514_Jan08

Page 3 of 9



January 31, 2008

DASY - Parameters of Probe: EX3DV3 SN:3514

Sensitivity in Free	e Space ^A	Diode C	ompression ^B
9797	127921227 PR-1850	 D 0 D 1/	17

NormX 0.650 \pm 10.1% μ V/(V/m)² DCP X 95 mV NormY 0.690 \pm 10.1% μ V/(V/m)² DCP Y 93 mV NormZ 0.580 \pm 10.1% μ V/(V/m)² DCP Z 96 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect

TSL

000

2300 MHz Typical SAR gradient: 10 % per mm

Sensor Cente	r to Phantom Surface Distance	2.0 mm	3.0 mm	
SAR _{be} [%]	Without Correction Algorithm	5.9	3.3	
SAR _{be} [%]	With Correction Algorithm	0.5	0.8	

TSL 2600 MHz Typical SAR gradient: 11 % per mm

Sensor Cente	er to Phantom Surface Distance	2.0 mm	3.0 mm
SAR _{be} [%]	Without Correction Algorithm	6.3	3.4
SAR _{be} [%]	With Correction Algorithm	0.1	0.3

Sensor Offset

Probe Tip to Sensor Center 1.0 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: EX3-3514_Jan08

Page 4 of 9

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).


⁸ Numerical linearization parameter: uncertainty not required.



January 31, 2008

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

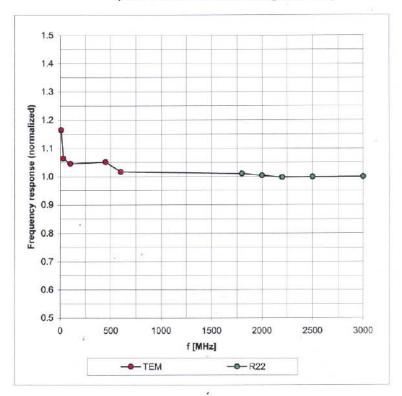


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Certificate No: EX3-3514_Jan08


Page 5 of 9

January 31, 2008

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

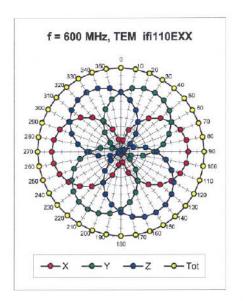



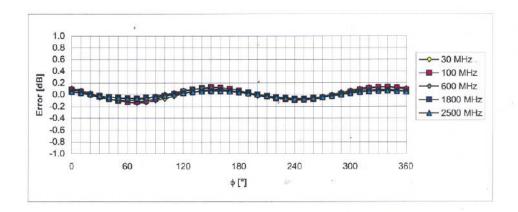

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Certificate No: EX3-3514_Jan08

Page 6 of 9

January 31, 2008

Dynamic Range f(SAR_{head})

(Waveguide R22, f = 1800 MHz)

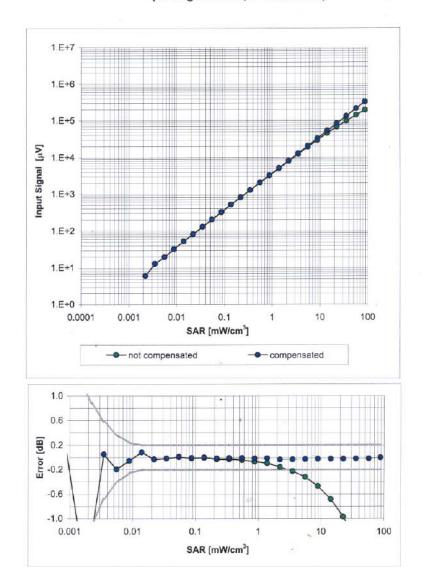


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Certificate No: EX3-3514_Jan08

Page 7 of 9

January 31, 2008

Conversion Factor Assessment

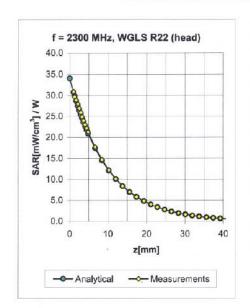



f [MHz]	Validity [MHz] ^C	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF	Uncertainty
2300	± 50 / ± 100	Head	$39.4 \pm 5\%$	1.71 ± 5%	0.76	0.52	7.73	± 11.8% (k=2)
2600	± 50 / ± 100	Head	39.0 ± 5%	1.96 ± 5%	0.62	0.60	7.31	± 11.8% (k=2)
3500	± 50 / ± 100	Head	37.9 ± 5%	2.91 ± 5%	0.36	1.03	7.09	± 13.1% (k=2)
2300	± 50 / ± 100	Body	52.8 ± 5%	1.85 ± 5%	0.63	0.64	7.59	± 11.8% (k=2)
2600	± 50 / ± 100	Body	52.5 ± 5%	2.16 ± 5%	0.52	, 0.76	6.91	± 11.8% (k=2)
3500	± 50 / ± 100	Body	51.3 ± 5%	$3.31 \pm 5\%$	0.40	1.33	6.32	± 13.1% (k=2)
5200	± 50 / ± 100	Body	49.0 ± 5%	5.30 ± 5%	0.35	1.70	4.34	± 13.1% (k=2)
5300	± 50 / ± 100	Body	48.9 ± 5%	5.42 ± 5%	0.38	1.70	4.06	± 13.1% (k=2)
5500	± 50 / ± 100	Body	48.6 ± 5%	5.65 ± 5%	0.43	1.70	3.98	± 13.1% (k=2)
5600	± 50 / ± 100	Body	48.5 ± 5%	5.77 ± 5%	0.35	1.70	4.19	± 13.1% (k=2)
5800	± 50 / ± 100	Body	48.2 ± 5%	6.00 ± 5%	0.30	1.70	4.20	± 13.1% (k=2)

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


Certificate No: EX3-3514_Jan08

Page 8 of 9

January 31, 2008

Deviation from Isotropy in HSL

Error (φ, θ), f = 900 MHz

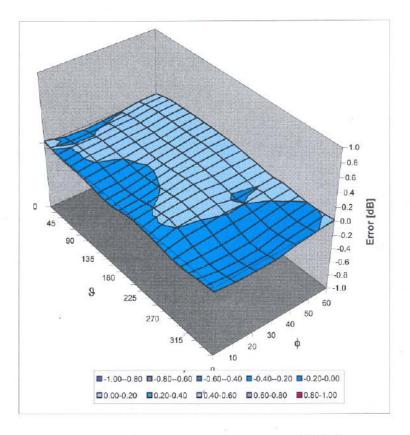

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: EX3-3514_Jan08

Page 9 of 9