

14. SAR System Calibration Data

The following pages show calibration certification data for the Schmid & Partner AG DASY4 SAR system.

m e t r a s
metrology and accreditation switzerland


Based on the Accreditation and Designation Ordinance dated 17 June 1996 (as of 9 December 2003) and on the advice of the Federal Accreditation Commission, the Swiss Accreditation Service (SAS) grants to


Schmid & Partner Engineering AG
Zeughausstrasse 43
CH-8004 Zürich

the accreditation as

Calibration Laboratory for Specific Electric and Magnetic RF Fields and SAR Measurements

in accordance with the Standard ISO/IEC 17025. The ranges and measurement uncertainties are listed in the Official SCS-Directory of the Accredited Calibration Laboratories.

Accreditation mark and number:  SCS 108
Date of accreditation: 17 September 2004
The accreditation is valid until: 16 September 2009

CH-3003 Berne-Wabern, 17 September 2004
Swiss Accreditation Service
The Head

Hanspeter Ischi

SAS is a signatory of the multilateral agreements of the European co-operation for Accreditation (EA) for calibration, testing, inspection and certification of products, personnel, quality and environmental management systems, of the International Accreditation Forum (IAF) for quality management systems and of the International Laboratory Accreditation Cooperation (ILAC) for calibration and testing.

Bundesamt für Metrologie und Akkreditierung Office fédéral de métrologie et d'accréditation Ufficio federale di metrologia e di accreditamento Swiss Federal Office of Metrology and Accreditation	Eidg. Justiz- und Polizeidepartement Département fédéral de justice et police Dipartimento federale di giustizia e polizia Swiss Federal Department of Justice and Police
---	--



Schweizerische Akkreditierungsstelle
 Service d'accréditation suisse
 Servizio di accreditamento svizzero
 Swiss Accreditation Service

SCS Directory

Accreditation number SCS 108

page 1 of 3

Calibration Laboratory for Specific Electric and Magnetic RF Fields and SAR Measurements

Schmid & Partner
 Engineering AG
 Zeughausstrasse 43
 8004 Zürich
 Phone 044/ 245 97 00
 Fax 044/ 245 97 79

Head of laboratory : Dr. Katja Pokovic
 Deputy of head of laboratory : Dr. Fin Bomholt
 Responsible person for QA : Prof. Dr. Niels Kuster
 First accreditation (d,m,y) : 17.09.2004
 Last accreditation (d,m,y) : 17.09.2004

Measured Quantity:

Electric field
 Magnetic field
 Specific Absorption Rate (SAR)
 Temperature
 DC Voltage

Change:

Staff :
 Scope extension : 01.10.2005
 Address :
 Edition : SCS108/D

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measured Quantity Instrument	Range	Conditions of measurements	Best Measurement Capability BMC at (22 ± 3) °C	Remarks
Electric field Calibration of E-field probes	0.8 V/m ... 800 V/m	10 MHz ... 3 GHz	5,1 %	e.g. ER3DV6x, EF3DVx, EU2DVx, EE3DVx
Magnetic field Calibration of H-field probes	2 mA/m ... 2 A/m	10 MHz ... 3 GHz	5,1 %	e.g. H2DVx, H3DVx
Specific absorption rate (SAR) Calibration of dosimetric E-field probes	E* field (typical ¹⁾ 0,5 V/m ... 500 V/m	300 MHz ... 450 MHz	6,7 % (13,3 % for SAR)	e.g. ET3DVx, ES3DVx, EX3DVx, ET1DVx, EU2DVx Temperature transfer calibration *) As example, the indicated range corresponds to 0,2 mW/kg - 200 W/kg for head tissue simulating liquid and f = 450 MHz



Schweizerische Akkreditierungsstelle
 Service d'accréditation suisse
 Servizio di accreditamento svizzero
 Swiss Accreditation Service

SCS Directory

Accreditation number SCS 108

page 2 of 3

Calibration Laboratory for Specific Electric and Magnetic RF Fields and SAR Measurements

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measured Quantity Instrument	Range	Conditions of measurements	Best Measurement Capability BMC at $(22 \pm 3) ^\circ\text{C}$	Remarks
Specific absorption rate (SAR) Calibration of dosimetric E-field probes	E* field (typical ¹) 0,45 V/m ... 450 V/m	800 MHz ... 2 GHz	5,5% (11,0 % for SAR)	e.g. ET3DVx, ES3DVx, EX3DVx, ET1DVx, EU2DVx Waveguide analytical calibration *) As example, the indicated range corresponds to 0,2 mW/kg - 200 W/kg for head tissue simulating liquid and $f = 1800$ MHz
	E* field (typical ¹) 0,4 V/m ... 400 V/m	2,45 GHz	5,9 % (11,8 % for SAR)	Waveguide analytical calibration *) As example, the indicated range corresponds to 0,2 mW/kg - 200 W/kg for head tissue simulating liquid and $f = 2450$ MHz
Specific absorption rate (SAR)	E* field (typical ¹) 0,4 V/m ... 450 V/m	3 GHz ... 6 GHz	6,5 % (13,1 % for SAR)	e.g. EX3DVx, ET1DVx Waveguide analytical calibration *) As example, the indicated range corresponds to 0,2 mW/kg - 200 W/kg for head tissue simulating liquid and $f = 5200$ MHz
Calibration of temperature SAR probes	0 °C ... +60 °C	Tissue simulating Liquids	0,15 K (5 % temperature gradient for SAR)	As example, the temperature gradient of T1Vx probe can be determined to 5 %, which is also contribution to SAR accuracy. (Noise is dominating the lower SAR threshold to typically 0,2 W/kg)



Schweizerische Akkreditierungsstelle
 Service d'accréditation suisse
 Servizio di accreditamento svizzero
 Swiss Accreditation Service

Accreditation number SCS 108

SCS Directory

page 3 of 3

Calibration Laboratory for Specific Electric and Magnetic RF Fields and SAR Measurements

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measured Quantity Instrument	Range	Conditions of measurements	Best Measurement Capability BMC at $(22 \pm 3) ^\circ\text{C}$	Remarks
Calibration of test system validation dipoles	SAR* 1 g and 10 g per 1 W input power	300 MHz ... 450 MHz 835 MHz ... 3 GHz	18,1 % for SAR 1 g 17,6 % for SAR 10 g 17,0 % for SAR 1 g 16,5 % for SAR 10 g	e.g. D835V2 - D3000V2 according to IEEE 1528-2003, for 1 g and 10 g SAR *) SAR given (as example) for head tissue simulating liquid
Calibration of test system validation dipoles	SAR* 1 g and 10 g per 1 W input power	3 GHz ... 6 GHz	19,9 % for SAR 1 g 19,5 % for SAR 10 g	e.g. D3500V2 – D5GHZV2 according to IEC 62209-2, for 1 g and 10 g SAR *) SAR given (as example) for head tissue simulating liquid
Calibration of dipoles in air	E* field per 0.1 W input power 30 V/m ... 300 V/m H* field per 0.1 W input power 0.07 A/m ... 0.7 A/m	800 MHz 3000 MHz	12,8 % for E field 8,2 % for H field	e.g. CD835V3 – CD2450V3 according to ANSI PC63.19- 2001, for E field and H field
DC Voltage Calibration of readout units for field and SAR probes	2 mV 200 mV		0,65 % 0,06 %	e.g. DAE3Vx, DAE4Vx, DAEasyVx

¹ Slightly depending on the frequency and probe type



Schweizerische Eidgenossenschaft
 Confédération suisse
 Confederazione Svizzera
 Confederaziun svizra

Federal Department of Economic Affairs DEA
State Secretariat for Economic Affairs SECO
 Swiss Accreditation Service SAS

Accreditation number **SCS 108**
Numero d'accreditamento

SCS Directory Registro SCS

Accreditation Standard ISO/IEC 17025:2005
 Norma d'accreditamento ISO/IEC

page/pagina 1 of/di 3

Calibration Laboratory for Specific Electric and Magnetic RF Fields and SAR measurements

Schmid & Partner
 Engineering AG
 Zeughausstrasse 43
 8004 Zürich
 ☎ +41 44 245 97 00
 Fax +41 44 245 97 79
<mailto:info@speag.com>
<http://www.speag.com>

Head of laboratory : Dr. Katja Poković
 Deputy of head of laboratory : Dr. Fin Bomholt
 Responsible person for QA : Prof. Dr. Niels Kuster
 First accreditation (d,m,y) : 17.09.2004
 Last accreditation (d,m,y) : 17.09.2004
 Actual version : <http://www.sas.ch/>

Measured Quantities:

Electric field
 Magnetic field
Specific Absorption Rate (SAR)
 Temperature
 DC Voltage

Change:

Staff :
 Scope extension : 01.10.05, 01.04.08
 Address :
 Edition : **SCS108/G**

The given extended measurement uncertainty is the standard uncertainty of the measurement multiplied by an extension factor $k = 2$, which corresponds to a confidence level of about 95% for a normal distribution.

Measured Quantity Instrument	Range	Condition of measurement	Best Measurement Capability CMC at (22 ± 3) °C	Remarks
Electric field Calibration of E-field probes	0.8 V/m ... 800 V/m	10 MHz ... 3 GHz	5,1 %	e.g. ER3DV6x, EF3DVx, EU2DVx, EE3DVx
Magnetic field Calibration of H-field probes	2 mA/m ... 2 A/m	10 MHz ... 3 GHz	5,1 %	e.g. H2DVx, H3DVx
Calibration of sensitivity for magnetic field probes in the audio range	0,001 ... 0,1 V/(A/m)	1 kHz 0,1 ... 1 A/m	2,2 %	e.g. AM1DVx
Calibration of magnetic field simulator	-30 ... +40 dB A/m	1 kHz		e.g. TMFS (Telephone Magnetic Field Simulator)



Schweizerische Eidgenossenschaft
 Confédération suisse
 Confederazione Svizzera
 Confederaziun svizra

Federal Department of Economic Affairs DEA
State Secretariat for Economic Affairs SECO
 Swiss Accreditation Service SAS

Accreditation number **SCS 108**
Numero d'accreditamento

SCS Directory Registro SCS

Accreditation Standard ISO/IEC 17025:2005
 Norma d'accreditamento ISO/IEC

page/pagina 2 of/di 3

Calibration Laboratory for Specific Electric and Magnetic fields and SAR measurements

Measured Quantity Instrument	Range	Condition of measurement	Best Measurement Capability CMC at (22 ± 3) °C	Remarks
Specific absorption rate (SAR) Calibration of dosimetric E-field probes	E* field (typical ¹) 0,5 V/m ... 500 V/m	300 MHz ... 450 MHz	6,7 % (13,3 % for SAR)	e.g. ET3DVx, ES3DVx, EX3DVx, ET1DVx, EU2DVx Temperature transfer calibration *) As example, the indicated range corresponds to 0,2 mW/kg ... 200 W/kg for head tissue simulating liquid and f = 450 MHz
	E* field (typical ¹) 0,45 V/m ... 450 V/m	800 MHz ... 3 GHz	5,5 % (11 % for SAR)	e.g. ET3DVx, ES3DVx, EX3DVx, ET1DVx, EU2DVx Waveguide analytical calibration *) As example, the indicated range corresponds to 0,2 mW/kg ... 200 W/kg for head tissue simulating liquid and f = 1800 MHz
	E* field (typical ¹) 0,4 V/m ... 450 V/m	3 GHz ... 6 GHz	6,5 % (13,1 % for SAR)	e.g. EX3DVx, ET1DVx Waveguide analytical calibration *) As example, the indicated range corresponds to 0,2 mW/kg ... 200 W/kg for head tissue simulating liquid and f = 5200 MHz
Calibration of temperature SAR probes	0 °C ... + 60 °C	Tissue simulating Liquids	0,15 K (5 % temperature gradient for SAR)	As example, the temperature gradient of T1Vx and T1V3LAB probes can be determined to 5 %, which is also contribution to SAR accuracy. (Noise is dominating the lower SAR threshold to typically 0,2 W/kg)



Schweizerische Eidgenossenschaft
 Confédération suisse
 Confederazione Svizzera
 Confederaziun svizra

Federal Department of Economic Affairs DEA
State Secretariat for Economic Affairs SECO
 Swiss Accreditation Service SAS

Accreditation number **SCS 108**
Numero d'accreditamento

SCS Directory Registro SCS

Accreditation Standard ISO/IEC 17025:2005
 Norma d'accreditamento ISO/IEC

page/pagina 3 of/di 3

Calibration Laboratory for Specific Electric and Magnetic fields and SAR measurements

Measured Quantity Instrument	Range	Condition of measurement	Best Measurement Capability CMC at (22 ± 3) °C	Remarks
Calibration of test system validation dipoles	SAR* 1 g and 10 g per 1 W input power	300 MHz ... 450 MHz	18,1 % for SAR 1 g 17,6 % for SAR 10 g	e.g. D835V2 ... D3000V2 according to IEEE 1528-2003, for 1 g and 10 g SAR *) SAR given (as example) for head tissue simulating liquid
		835 MHz ... 3 GHz	17,0 % for SAR 1 g 16,5 % for SAR 10 g	
	SAR* 1 g and 10 g per 1 W input power	3 GHz ... 6 GHz	19,9 % for SAR 1 g 19,5 % for SAR 10 g	e.g. D3500V2 ... D5GHzV2 according to IEC 62209-2, for 1 g and 10 g SAR *) SAR given (as example) for head tissue simulating liquid
Calibration of dipoles in air	E* field per 0,1 W input power 30 V/m ... 300 V/m	800 MHz ... 3 GHz	12,8 % for E field	e.g. CD835V3 ... CD2450V3 according to ANSI PC 63,19 2001, for E field and H field
	H* field per 0,1 W input power 0,07 A/m ... 0,7 A/m		8,2 % for H field	
DC Voltage				
Calibration of readout units for field and SAR probes	2 mV		0,65 %	e.g. DAE3Vx, DAE4Vx, DAEasyVx
	200 mV		0,06 %	

¹ Slightly depending on the frequency and probe type

**Calibration Laboratory of
 Schmid & Partner
 Engineering AG**
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Qualcomm USA**

Certificate No: **ET3-1733_Sep07**

CALIBRATION CERTIFICATE

Object **ET3DV6 - SN:1733**

Calibration procedure(s) **QA CAL-01.v6 and QA CAL-12.v5
 Calibration procedure for dosimetric E-field probes**

Calibration date: **September 4, 2007**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Power sensor E4412A	MY41495277	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Power sensor E4412A	MY41498087	29-Mar-07 (METAS, No. 217-00670)	Mar-08
Reference 3 dB Attenuator	SN: S5054 (3c)	8-Aug-07 (METAS, No. 217-00719)	Aug-08
Reference 20 dB Attenuator	SN: S5086 (20b)	29-Mar-07 (METAS, No. 217-00671)	Mar-08
Reference 30 dB Attenuator	SN: S5129 (30b)	8-Aug-07 (METAS, No. 217-00720)	Aug-08
Reference Probe ES3DV2	SN: 3013	4-Jan-07 (SPEAG, No. ES3-3013_Jan07)	Jan-08
DAE4	SN: 654	20-Apr-07 (SPEAG, No. DAE4-654_Apr07)	Apr-08
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Nov-05)	In house check: Nov-07
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Oct-06)	In house check: Oct-07

Calibrated by:	Name Katja Pokovic	Function Technical Manager	Signature
Approved by:	Name Niels Kuster	Function Quality Manager	

Issued: September 4, 2007

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
Polarization ϕ	ϕ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not effect the E^2 -field uncertainty inside TSL (see below *ConvF*).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * *frequency_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * *ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

ET3DV6 SN:1733

September 4, 2007

Probe ET3DV6

SN:1733

Manufactured:	September 27, 2002
Last calibrated:	September 22, 2006
Recalibrated:	September 4, 2007

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1733

September 4, 2007

DASY - Parameters of Probe: ET3DV6 SN:1733

Sensitivity in Free Space^A

NormX	1.52 ± 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$
NormY	1.50 ± 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	1.63 ± 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$

Diode Compression^B

DCP X	95 mV
DCP Y	92 mV
DCP Z	92 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect

TSL 900 MHz Typical SAR gradient: 5 % per mm

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	5.7	3.0
SAR _{be} [%]	With Correction Algorithm	0.3	0.1

TSL 1750 MHz Typical SAR gradient: 10 % per mm

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	11.7	8.0
SAR _{be} [%]	With Correction Algorithm	0.6	0.2

Sensor Offset

Probe Tip to Sensor Center 2.7 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).


^B Numerical linearization parameter: uncertainty not required.

ET3DV6 SN:1733

September 4, 2007

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)



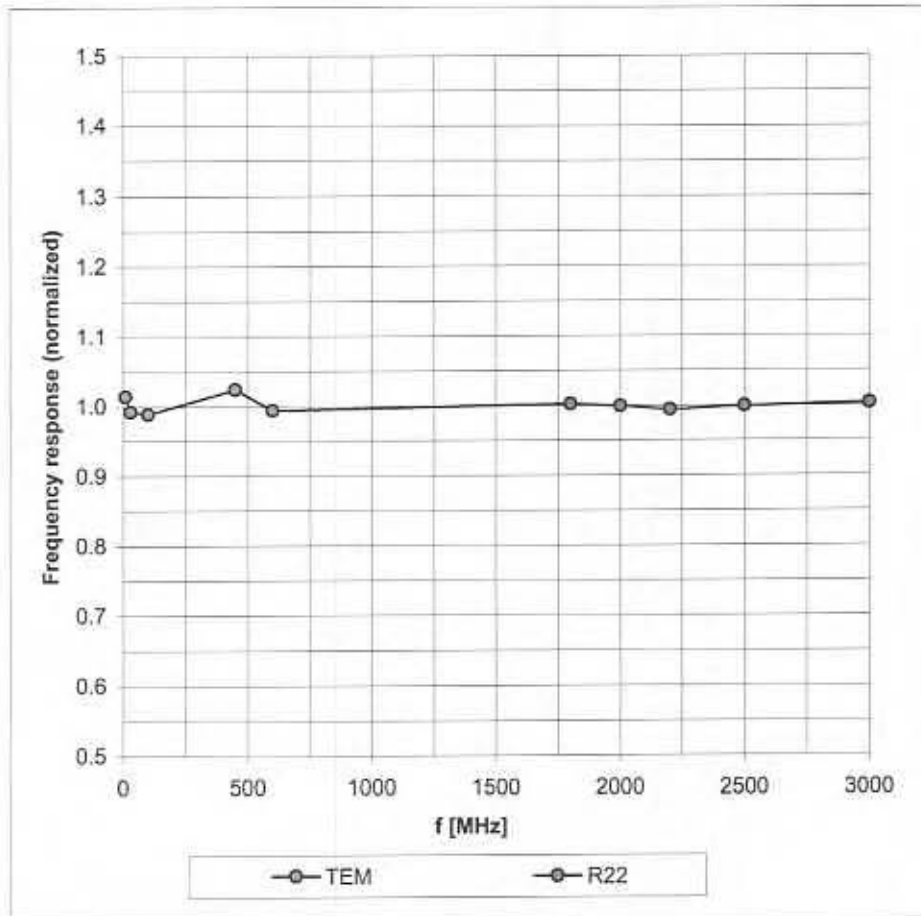


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

ET3DV6 SN:1733

September 4, 2007

Receiving Pattern (ϕ), $\vartheta = 0^\circ$

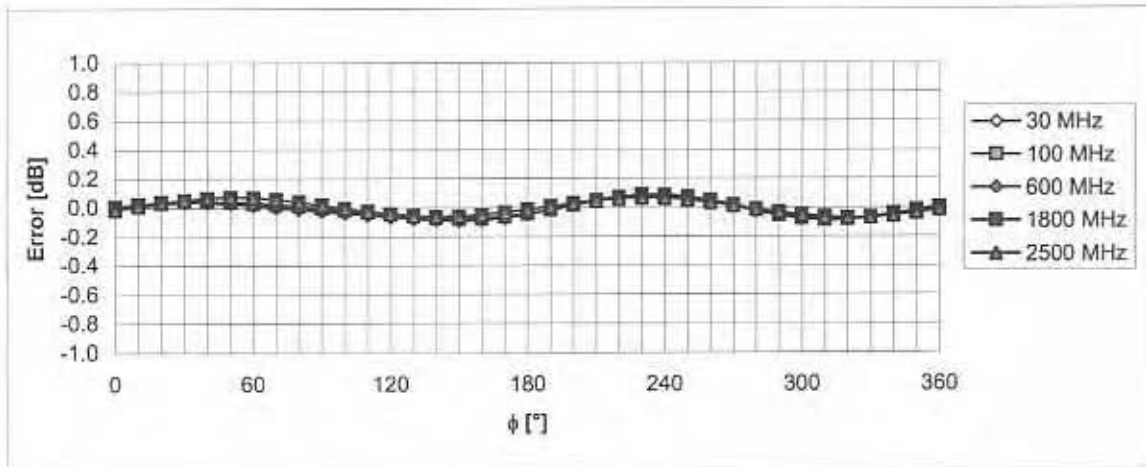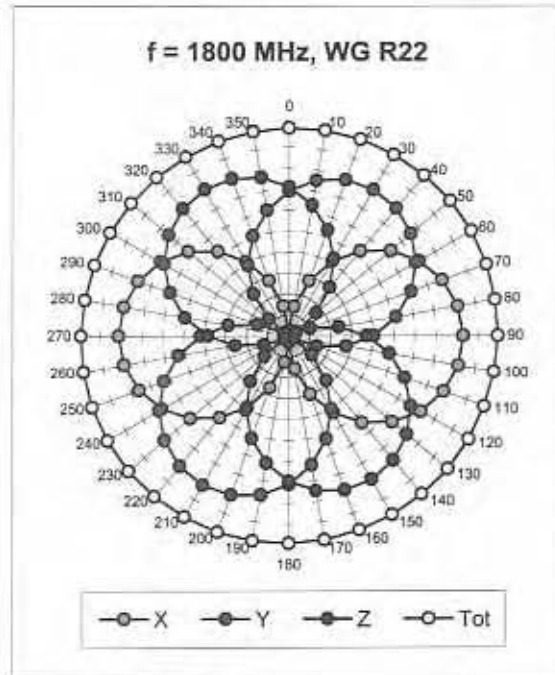
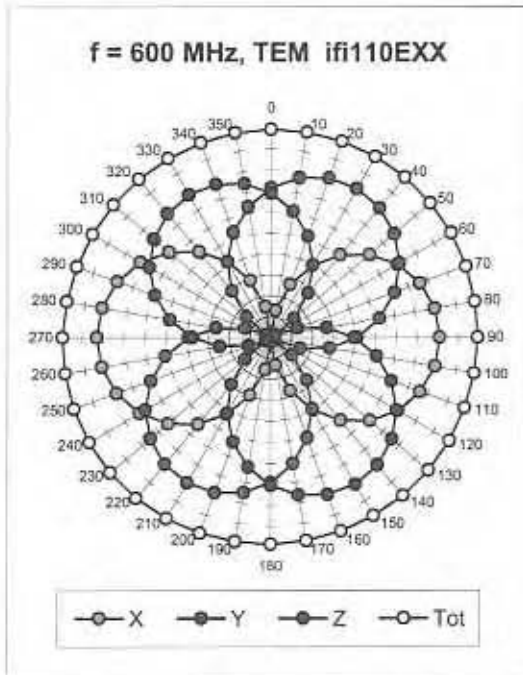


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

ET3DV6 SN:1733

September 4, 2007

Dynamic Range $f(\text{SAR}_{\text{head}})$ (Waveguide R22, $f = 1800 \text{ MHz}$)

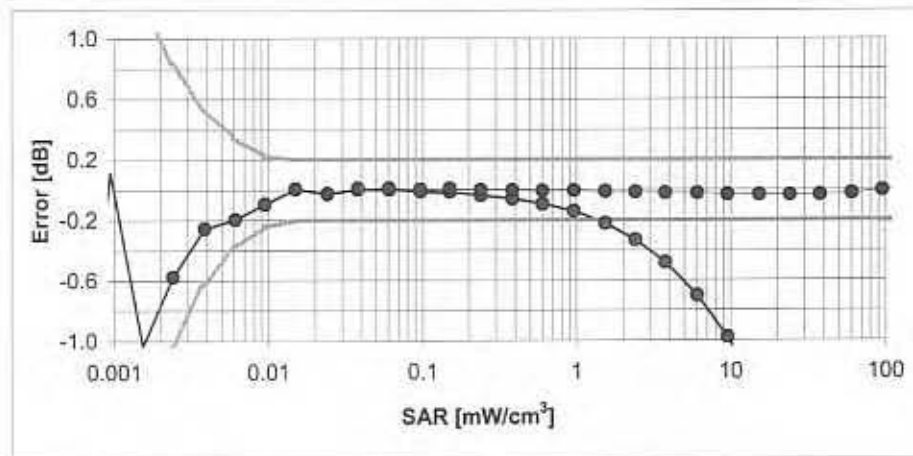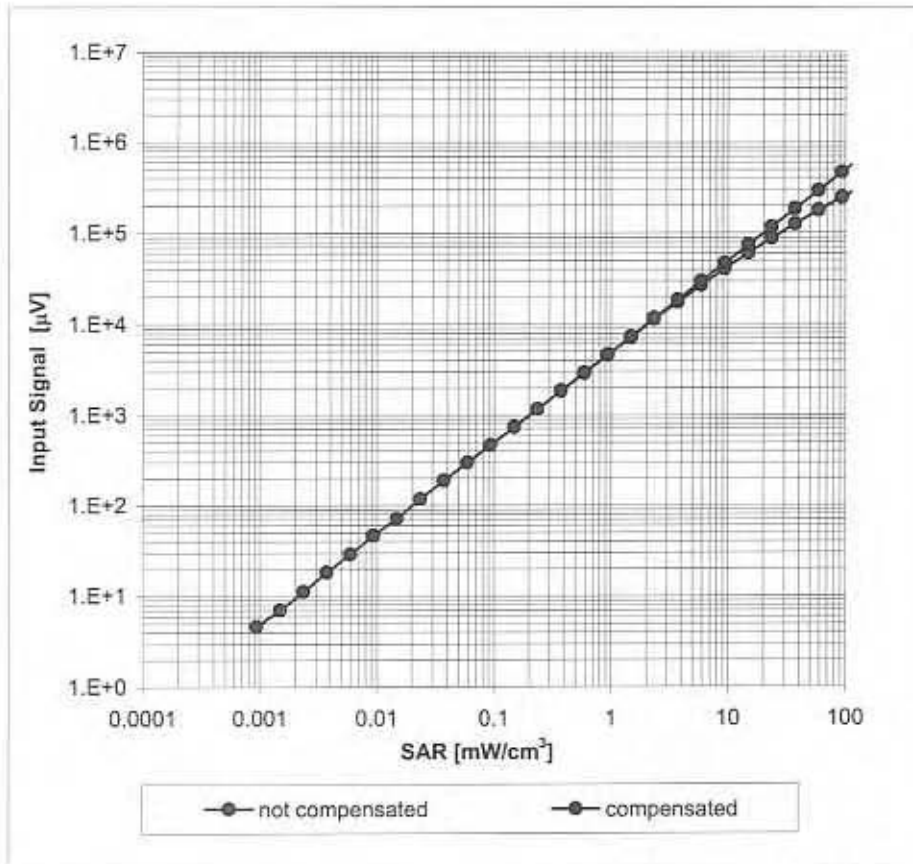


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

ET3DV6 SN:1733

September 4, 2007

Conversion Factor Assessment

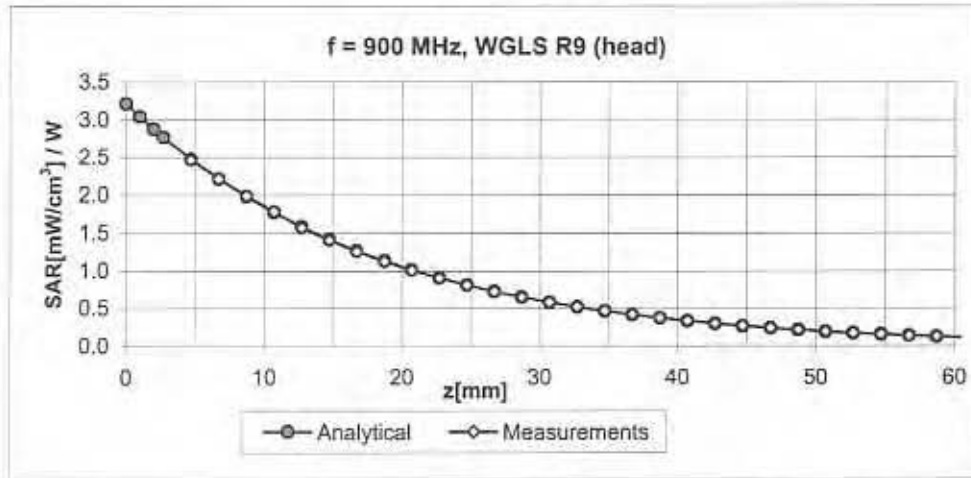

f [MHz]	Validity [MHz] ^c	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
450	± 50 / ± 100	Head	43.5 ± 5%	0.87 ± 5%	0.36	1.83	7.34 ± 13.3% (k=2)
835	± 50 / ± 100	Head	41.5 ± 5%	0.90 ± 5%	0.24	2.89	6.89 ± 11.0% (k=2)
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.29	2.89	6.72 ± 11.0% (k=2)
1640	± 50 / ± 100	Head	40.3 ± 5%	1.29 ± 5%	0.54	2.59	5.83 ± 11.0% (k=2)
1750	± 50 / ± 100	Head	40.1 ± 5%	1.37 ± 5%	0.64	2.36	5.42 ± 11.0% (k=2)
1900	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.55	2.77	5.24 ± 11.0% (k=2)
1950	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.55	2.75	5.06 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	0.62	2.11	4.56 ± 11.8% (k=2)
450	± 50 / ± 100	Body	56.7 ± 5%	0.94 ± 5%	0.33	2.65	7.68 ± 13.3% (k=2)
835	± 50 / ± 100	Body	55.2 ± 5%	0.97 ± 5%	0.35	2.89	6.57 ± 11.0% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.37	2.89	6.29 ± 11.0% (k=2)
1640	± 50 / ± 100	Body	53.8 ± 5%	1.40 ± 5%	0.50	2.84	5.27 ± 11.0% (k=2)
1750	± 50 / ± 100	Body	53.4 ± 5%	1.49 ± 5%	0.55	2.76	4.95 ± 11.0% (k=2)
1900	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.67	2.43	4.71 ± 11.0% (k=2)
1950	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.73	2.29	4.58 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.65	2.17	3.93 ± 11.8% (k=2)


^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

ET3DV6 SN:1733

September 4, 2007

Deviation from Isotropy in HSL

Error (ϕ, ϑ), $f = 900$ MHz

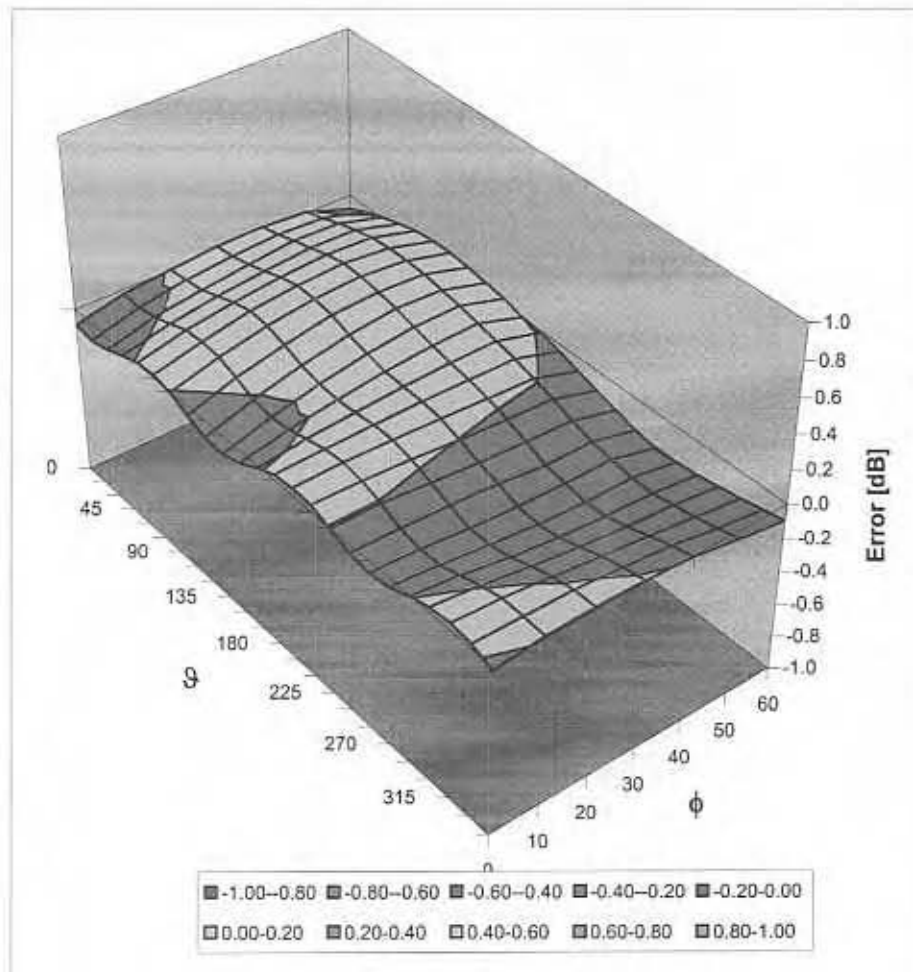

Uncertainty of Spherical Isotropy Assessment: $\pm 2.6\%$ ($k=2$)

**Calibration Laboratory of
 Schmid & Partner
 Engineering AG**
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Qualcomm USA**

Certificate No: **D1900V2-5d019_Nov07**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d019**

Calibration procedure(s) **QA CAL-05.v7
 Calibration procedure for dipole validation kits**

Calibration date: **November 13, 2007**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	04-Oct-07 (METAS, No. 217-00736)	Oct-08
Power sensor HP 8481A	US37292783	04-Oct-07 (METAS, No. 217-00736)	Oct-08
Reference 20 dB Attenuator	SN: 5086 (20g)	07-Aug-07 (METAS, No 217-00718)	Aug-08
Reference 10 dB Attenuator	SN: 5047.2 (10r)	07-Aug-07 (METAS, No 217-00718)	Aug-08
Reference Probe ET3DV6 (HF)	SN: 1507	26-Oct-07 (SPEAG, No. ET3-1507_Oct07)	Oct-08
DAE4	SN 601	30-Jan-07 (SPEAG, No. DAE4-601_Jan07)	Jan-08

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (SPEAG, in house check Oct-07)	In house check: Oct-08
RF generator R&S SMT-06	100005	4-Aug-99 (SPEAG, in house check Oct-07)	In house check: Oct-09
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (SPEAG, in house check Oct-07)	In house check: Oct-08

Calibrated by: **Claudio Leubler** (Laboratory Technician) [Signature]

Approved by: **Katja Pokovic** (Technical Manager) [Signature]

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kallbrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.8 ± 6 %	1.45 mho/m ± 6 %
Head TSL temperature during test	(21.4 ± 0.2) °C	—	—

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	250 mW input power	9.86 mW / g
SAR normalized	normalized to 1W	39.4 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	38.1 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.15 mW / g
SAR normalized	normalized to 1W	20.6 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	20.2 mW / g ± 16.5 % (k=2)

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.7 ± 6 %	1.54 mho/m ± 6 %
Body TSL temperature during test	(21.0 ± 0.2) °C	—	—

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.32 mW / g
SAR normalized	normalized to 1W	37.3 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	37.2 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	4.99 mW / g
SAR normalized	normalized to 1W	20.0 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	20.0 mW / g ± 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$53.0 \Omega + 2.3 j\Omega$
Return Loss	- 28.7 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$48.6 \Omega + 3.0 j\Omega$
Return Loss	- 29.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.197 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	June 04, 2002

DASY4 Validation Report for Head TSL

Date/Time: 05.11.2007 14:23:55

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d019

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB;

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.45$ mho/m; $\epsilon_r = 38.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507 (HF); ConvF(4.86, 4.86, 4.86); Calibrated: 26.10.2007
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 93.1 V/m; Power Drift = 0.036 dB



Peak SAR (extrapolated) = 17.4 W/kg

SAR(1 g) = 9.86 mW/g; SAR(10 g) = 5.15 mW/g

Maximum value of SAR (measured) = 11.1 mW/g

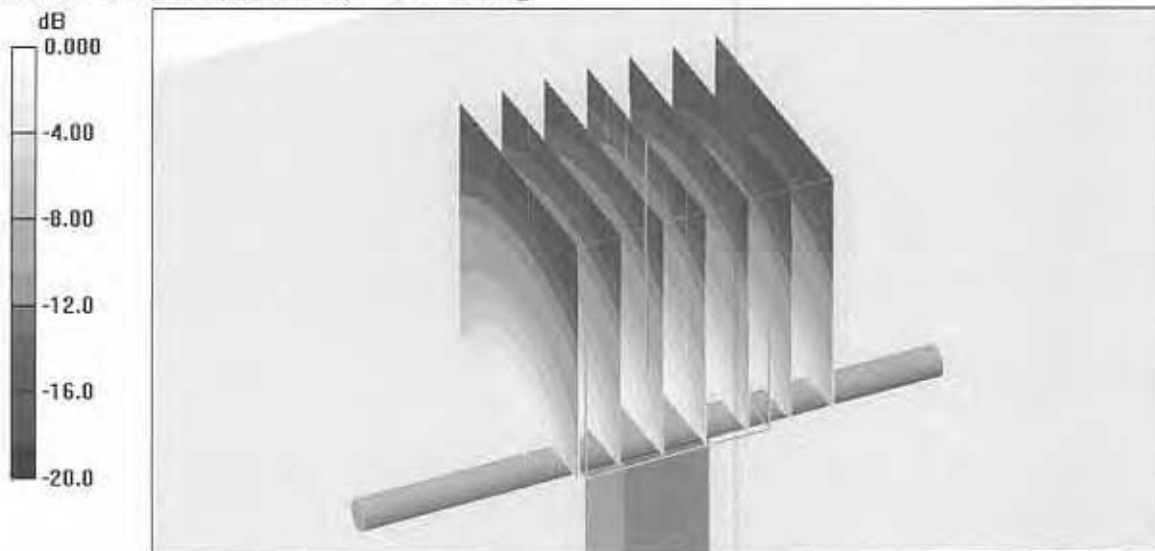

Impedance Measurement Plot for Head TSL

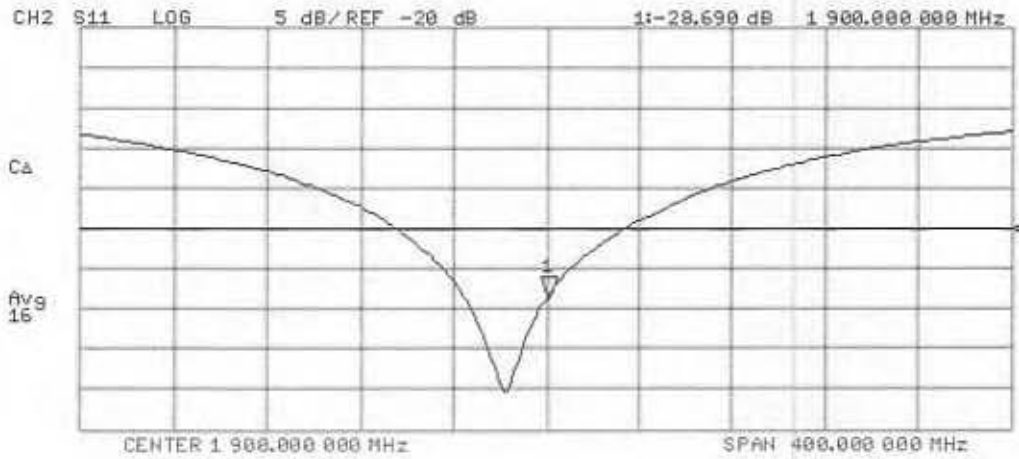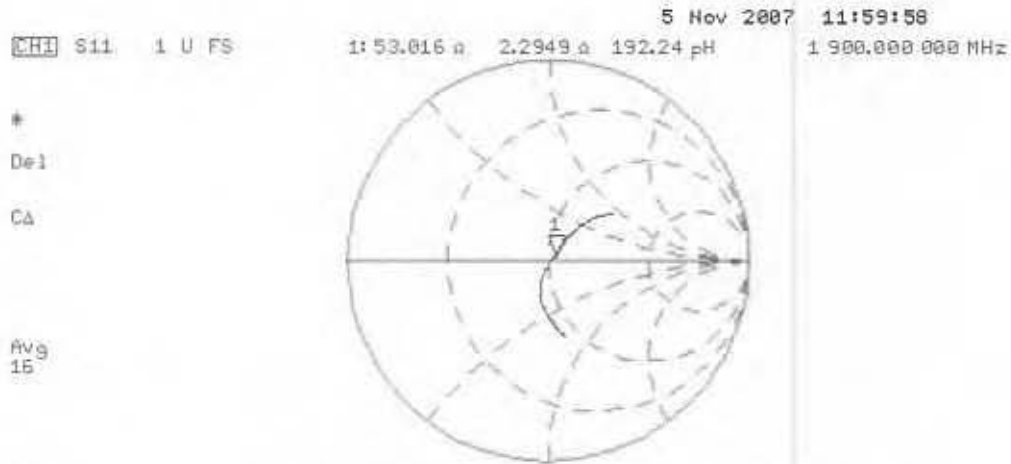

DASY4 Validation Report for Body TSL

Date/Time: 13.11.2007 14:09:19

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d019

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: MSL U10 BB;

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.54$ mho/m; $\epsilon_r = 53.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507 (HF); ConvF(4.48, 4.48, 4.48); Calibrated: 26.10.2007
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 89.5 V/m; Power Drift = -0.006 dB

Peak SAR (extrapolated) = 15.9 W/kg

SAR(1 g) = 9.32 mW/g; SAR(10 g) = 4.99 mW/g

Maximum value of SAR (measured) = 10.6 mW/g

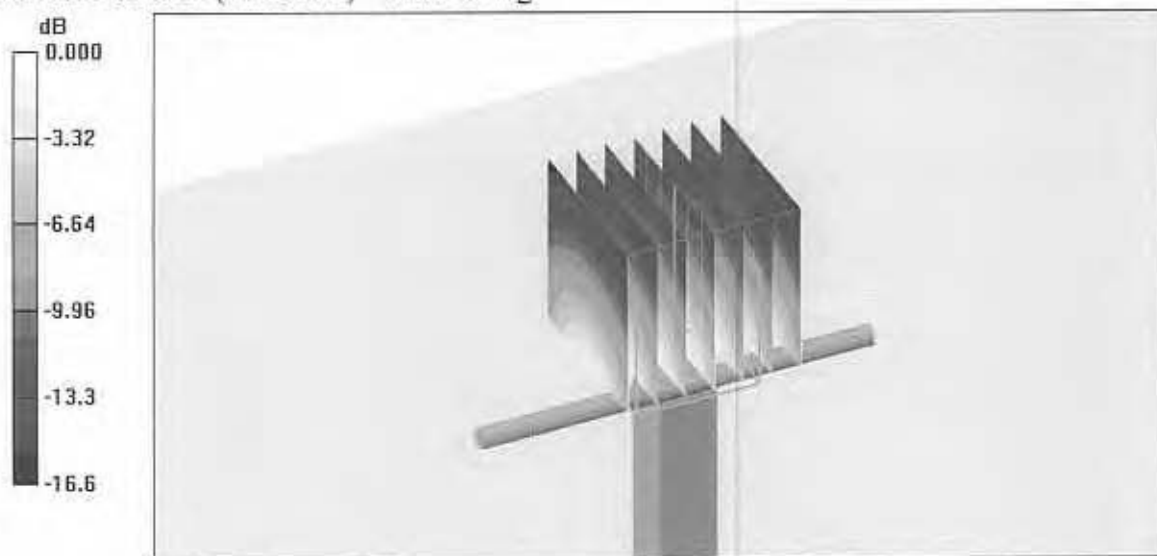

0 dB = 10.6mW/g