

## Annex D

Appendix to Test Report No.: 1-1068/20-04-08



#### Testing Laboratory

CTC advanced GmbH Untertürkheimer Straße 6 – 10 66117 Saarbrücken/Germany Phone: + 49 681 5 98 - 0 Fax: + 49 681 5 98 - 9075 Internet: <u>http://www.ctcadvanced.com</u> e-mail: mail@ctcadvanced.com

#### Accredited Test Laboratory:

The testing laboratory (area of testing) is accredited according to DIN EN ISO/IEC 17025 (2005) by the Deutsche Akkreditierungsstelle GmbH (DAkkS) The accreditation is valid for the scope of testing procedures as stated in the accreditation certificate with the registration number: D-PL-12076-01-01

# Appendix with Calibration data, Phantom certificate and system check information



### 1 Table of contents

1	Tabl	le of contents	2
2	Calil	bration report "Probe ES3DV3"	3
3	Calil	bration report "1900 MHz System validation dipole"	20
4	Calil	bration certificate of Data Acquisition Unit (DAE)	28
5	Cert	tificate of "SAM Twin Phantom V4.0/V4.0C"	29
6	Арр	lication Note System Performance Check	
	6.1	Purpose of system performance check	
	6.2	System Performance check procedure	
	6.3	Uncertainty Budget	
	6.4	Power set-up for validation	
	6.5	Laboratory reflection	
	6.6	Additional system checks	



### 2 Calibration report "Probe ES3DV3"

		and show a second s	
ccredited by the Swiss Accred he Swiss Accreditation Serv fultilateral Agreement for the	ice is one of the signatories	to the EA.	reditation No.: SCS 0108
Sient CTC advance	d GmbH	Certificate No:	ES3-3320_Jan20
CALIBRATION	CERTIFICATE		
	500000 00000		
Object	ES3DV3 - SN:332	0	
Calibration procedure(s)		A CAL-12.v9, QA CAL-23.v5, QA lure for dosimetric E-field probes	CAL-25.v7
Calibration date:	January 20, 2020		
		al standards, which realize the physical units bability are given on the following pages and	
All calibrations have been cond	lucted in the closed laboratory	facility: environment temperature (22 ± 3)°C a	and humidity < 70%.
		facility: environment temperature (22 $\pm$ 3)°C a	and humidity < 70%.
Calibration Equipment used (M		facility: environment temperature (22 ± 3)°C a	and humidity < 70%.
Calibration Equipment used (M Primary Standards	&TE critical for calibration)		
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291	&TE critical for calibration)	Cal Date (Certificate No.)	Scheduled Calibration
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291	8TE oritical for calibration) ID SN: 104778 SN: 103244 SN: 103245	Cal Date (Certificate No ) 03-Apr-19 (No. 217-02892/02593)	Scheduled Calibration Apr-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator	8TE oritical for calibration) ID SN: 104778 3N: 103244 SN: 103245 SN: 105245 SN: 55277 (20x)	Cal Date (Certificate: No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator DAE4	&TE oritical for calibration) ID SN: 104778 3N: 103244 SN: 103245 SN: 55277 (20x) SN: 560	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02593) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 27-Dec-19 (No. DAE4-680_Dec19)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator DAE4	8TE oritical for calibration) ID SN: 104778 3N: 103244 SN: 103245 SN: 105245 SN: 55277 (20x)	Cal Date (Certificate: No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES30V2	8TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 55277 (20x) SN: 560 SN: 3013	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02593) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 27-Dec-19 (No. DAE4-880_Dec19) 31-Dec-19 (No. ES3-3013_Dec19)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES30V2 Secondary Standards	ID         ID           SN: 104778         SN: 103244           SN: 103245         SN: 55277 (20x)           SN: 560         SN: 3013           ID         ID	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 27-Dec-19 (No. DAE4-680_Dec19) 31-Dec-19 (No. ES3-3013_Dec19) Check Date (in house)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Check
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES3DV2 Secondary Standards Power meter E44198	8TE oritical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 85277 (20x) SN: 860 SN: 860 SN: 3013 ID SN: G841293874	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 27-Dec-19 (No. DAE4-680_Dec19) 31-Dec-19 (No. ES3-3013_Dec19) Check Date (in house) 06-Apr-16 (in house check Jun-18)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Scheduled Check In house check: Jun-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES30V2 Secondary Standards Power meter E44198 Power sensor E4412A	8TE ortical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 55277 (20k) SN: 560 SN: 3013 ID SN: GB41293874 SN: MY41499087	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 27-Dec-19 (No. DAE4-080_Dec19) 31-Dec-19 (No. ES3-3013_Dec19) Check Date (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Check In house check: Jun-20 In house check: Jun-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES3DV2 Secondary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A	8TE ortical for calibration) ID SN: 104778 3N: 103244 SN: 103245 SN: 58277 (20x) SN: 660 SN: 3013 ID SN: G841293874 SN: MY41498087 SN: 000110210	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02593) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 27-Dec-19 (No. DAE4-880_Dec19) 31-Dec-19 (No. ES3-3013_Dec19) Check Date (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Check In house check: Jun-20 In house check: Jun-20 In house check: Jun-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES3DV2 Secondary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A RF generator HP 8648C	8TE ortical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 55277 (20k) SN: 560 SN: 3013 ID SN: GB41293874 SN: MY41499087	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 27-Dec-19 (No. DAE4-080_Dec19) 31-Dec-19 (No. ES3-3013_Dec19) Check Date (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Check In house check Jun-20 In house check: Jun-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES30V2 Secondary Standards Power sensor E44198 Power sensor E4412A Power sensor E4412A RF generator HP 8648C	ID         SN: 104778           SN: 104778         SN: 103245           SN: 103245         SN: 103245           SN: 55277 (20x)         SN: 560           SN: 50345         SN: 3013           ID         SN: CB41293874           SN: 000110210         SN: 000110210           SN: US3642U01700         SN: US41090477	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 10-Apr-19 (No. 217-02893) 31-Dec-19 (No. 217-02894) 27-Dec-19 (No. 217-02894) 27-Dec-19 (No. 217-02894) 05-Apr-16 (in house) 06-Apr-16 (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 04-Aug-98 (in house check Jun-18) 04-Aug-98 (in house check Jun-18) 31-Mar-14 (in house check Oct-19)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Chack In house check: Jun-20 In house check: Oct-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES30V2 Secondary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A RF generator HP 8648Q Network Analyzer E8358A	8TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 55277 (20x) SN: 660 SN: 3013 ID SN: G841293874 SN: MY41498087 SN: 000110210 SN: US342U01700 SN: US41080477 Name	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02693) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 27-Dec-19 (No. DAE4-680_Dec19) 31-Dec-19 (No. ES3-3013_Dec19) Check Date (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 04-Aug-96 (in house check Jun-18) 31-Mar-14 (in house check Oct-19) Function	Scheduled Calibration Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Check In house check: Jun-20 In house check: Jun-20 In house check: Jun-20 In house check: Jun-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES3DV2 Secondary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A	ID         SN: 104778           SN: 104778         SN: 103245           SN: 103245         SN: 103245           SN: 55277 (20x)         SN: 560           SN: 50345         SN: 3013           ID         SN: CB41293874           SN: 000110210         SN: 000110210           SN: US3642U01700         SN: US41090477	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 10-Apr-19 (No. 217-02893) 31-Dec-19 (No. 217-02894) 27-Dec-19 (No. 217-02894) 27-Dec-19 (No. 217-02894) 05-Apr-16 (in house) 06-Apr-16 (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 04-Aug-98 (in house check Jun-18) 04-Aug-98 (in house check Jun-18) 31-Mar-14 (in house check Oct-19)	Scheduled Calibration Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Chack In house check: Jun-20 In house check: Oct-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES3DV2 Secondary Standards Power sensor E44198 Power sensor E4419A Power sensor E4412A Power sensor E4412A RF generator HP 8648C Network Analyzer E8358A Calibrated by	8TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 55277 (20x) SN: 660 SN: 3013 ID SN: G841293874 SN: MY41498087 SN: 000110210 SN: US342U01700 SN: US41080477 Name	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02693) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 27-Dec-19 (No. DAE4-680_Dec19) 31-Dec-19 (No. ES3-3013_Dec19) Check Date (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 04-Aug-96 (in house check Jun-18) 31-Mar-14 (in house check Oct-19) Function	Scheduled Calibration Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Chack In house check Jun-20 In house check: Jun-20
Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ES3DV2 Secondary Standards Power sensor E44198 Power sensor E4412A RF generator HP 8648C Network Analyzer E8358A Calibrated by:	BTE critical for calibration)           ID           SN: 104778           3N: 103244           SN: 103245           SN: 860           SN: 3013           ID           SN: 6841293874           SN: 000110210           SN: 000110210           SN: US41080477           Name           Michael Weber           Katja Pokovic	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02593) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 27-Dec-19 (No. DAE4-860_Dec19) 31-Dec-19 (No. ES3-3013_Dec19) Check Date (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 08-Apr-16 (in house check Jun-18) 08-Apr-16 (in house check Jun-18) 31-Mar-14 (in house check Oct-19) Function	Scheduled Calibration Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Chack In house check Jun-20 In house check: Jun-20



#### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



- S Schweizerischer Kalibrierdienst
- C Service suisse d'étalonnage
  - Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

S

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\phi$	o rotation around probe axis
Polarization 9	9 rotation around an axis that is in the plane normal to probe axis (at measurement center),
	i.e., 9 = 0 is normal to probe axis

Connector Angle

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, ", "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from handheld and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016

information used in DASY system to align probe sensor X to the robot coordinate system

- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below *ConvF*).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is
  implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
  in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z; A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diade.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMs, y, z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom
  exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: ES3-3320\_Jan20

Page 2 of 23



ES3DV3 - SN:3320

January 20, 2020

### DASY/EASY - Parameters of Probe: ES3DV3 - SN:3320

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	1.23	1.04	1.13	± 10.1 %
DCP (mV) <sup>8</sup>	103.6	107.4	105.2	

#### **Calibration Results for Modulation Response**

UID	Communication System Name		A dB	B dBõV	С	D dB	VR mV	Max dev.	Max Unc (k=2)						
0	CW	X	0.00	0.00	1.00	0.00	180.9	± 3.3 %	±4.7 %						
	1980	Y	0.00	0.00	1.00	- XORNA	193.1	120110200400	A12.00104						
		Z	0.00	0.00	1.00	1	197.7		l						
10352-	Pulse Waveform (200Hz, 10%)	X	10.78	82.52	22.57	10.00	60.0	±2.1%	±9.6%						
AAA	A CONTRACTOR RECEVED AND A STREET AND A STREET	Y	15.25	88.98	24.03	124522	60.0	100000000	10.25253						
ACTION OF		Z	10.22	80.83	22.01		60.0	1							
10353-	Pulse Waveform (200Hz, 20%)	X	20.00	93.74	24.74	6.99	80.0 80.0	± 3.3 %	± 9.6 %						
AAA	Contract and a second	Y	20.00	93.54	23.BB	26-22-20		CO155521 1952							
		Z	13.95	87.65	22.90	1	80.0	1							
10354-	Pulse Waveform (200Hz, 40%)	X	20.00	95.29	23.36	3.98	95.0	±4.9 %	± 9.6 %						
AAA	0	Y	20.00	94.93	22.65	822.52				832.54		95.0		07005/33	12000000
290500		Z	20.00	94.27	23.02		95.0	_							
10355-	Pulse Waveform (200Hz, 60%)	X	20.00	98.09	22.92	2.22	120.0	±4.9%	± 9.6 %						
AAA	0 C A	Y	20.00	97.84	22.42	1000	120.0	225333425							
		Z	20.00	96.69	22.36		120.0	1							
10387-	QPSK Waveform, 1 MHz	X	0.92	63.99	11.26	0.00	150.0	±25% ±	±2.5 %	±9.6%					
AAA		Y	0.85	63.62	10.50		150.0								
986697		Z	0.86	63.07	10.83		150.0	1							
10388-	QPSK Waveform, 10 MHz	X	2.40	69.02	16.05	0.00	150.0	±1.1%	±9.6 %						
AAA		Y	2.41	69.39	16.26		150.0								
		Z	2.28	68.17	15.58		150.0								
10396-	64-QAM Waveform, 100 kHz	X	3.47	71.45	19.18	3.01	150.0	±0.8 %	± 9.6 %						
AAA		Y	4.08	75.81	21.03		150.0								
	1012-2010 (2010) - MOTO - MINESON	Z	3.55	71.27	18.98		150.0								
10399-	64-QAM Waveform, 40 MHz	X	3.48	67.00	15.67	0.00	150.0	±1.8 %	±9.6 %						
AAA		Y	3.51	67.32	15.80		150.0								
	Construction and a construction of the second	Z	3.54	67.24	15.73		150.0								
10414-	WLAN CCDF, 64-QAM, 40MHz	X	4.87	65.42	15.38	0.00	150.0	± 3.8 %	± 9.6 %						
AAA		Y	4.87	65.75	15.51		150.0		11111000						
		Z	4.98	65.72	15.51		150.0	-							

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>8</sup> Numerical linearization parameter: uncertainty not required. <sup>9</sup> Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: ES3-3320\_Jan20

Page 3 of 23



ES3DV3- SN:3320

January 20, 2020

### DASY/EASY - Parameters of Probe: ES3DV3 - SN:3320

#### Sensor Model Parameters

	C1 fF	C2 fF	α V-1	T1 ms.V <sup>-2</sup>	T2 ms.V <sup>-+</sup>	T3 ms	T4 V <sup>-2</sup>	T5 V-1	Т6
X	58.6	419.57	35.21	29.85	3.99	5.10	0.00	0.69	1.01
Y	50.1	351.97	34.06	28.86	2.69	5.10	1.51	0.31	1.01
Z	61.3	440.64	35.39	33.77	4.41	5.10	0.00	0.77	1.01

#### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	72.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

Certificate No: ES3-3320\_Jan20

Page 4 of 23



ES3DV3- SN:3320

January 20, 2020

### DASY/EASY - Parameters of Probe: ES3DV3 - SN:3320

f (MHz) <sup>c</sup>	Relative Permittivity F	Conductivity (S/m)	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
450	43.5	0.87	7.01	7.01	7.01	0.16	1.40	± 13.3 %
750	41.9	0.89	6.47	6.47	6.47	0.60	1.36	± 12.0 %
850	41.5	0.92	6.18	6.18	6.18	0.64	1.34	± 12.0 %
900	41.5	0.97	6.14	6.14	6,14	0.80	1.15	± 12.0 %
1450	40.5	1.20	5.65	5.65	5.65	0.61	1.36	± 12.0 %
1640	40.2	1,31	5.53	5.53	5.53	0.80	1.20	± 12.0 %
1750	40.1	1.37	5.41	5.41	5.41	0.60	1.44	± 12.0 %
1900	40.0	1.40	5.19	5.19	5.19	0.80	1.24	± 12.0 %
2450	39.2	1.80	4.65	4.65	4.65	0.80	1.26	± 12.0 %

#### Calibration Parameter Determined in Head Tissue Simulating Media

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the CorvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10.25, 40, 50 and 70 MHz for CorvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of CorvF assessed at 6 MHz is ± 90.25, 40, 50 and 70 MHz for CorvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of CorvF assessed at 6 MHz is ± 9 MHz, and CorvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz. <sup>A</sup> At frequencies below 3 GHz, the validity of issue parameters (is and o) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of issue parameters (c and o) is restricted to ± 5%. The uncertainty is the RSS of the CorvF uncertainty for indicated target tissue parameters. <sup>A</sup> At hequencies below 3 GHz, the validity of uncertainty at the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: ES3-3320\_Jan20

Page 5 of 23



ES30V3- SN:3320

January 20, 2020

### DASY/EASY - Parameters of Probe: ES3DV3 - SN:3320

f (MHz) <sup>c</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>0</sup> (mm)	Unc (k=2)
450	56.7	0.94	7.09	7.09	7.09	0.05	1.25	± 13.3 %
750	55.5	0.96	6.36	6.36	6.36	0.78	1.20	± 12.0 %
850	55.2	0.99	6.12	6,12	6.12	0.80	1.15	± 12.0 %
900	55.0	1.05	6.10	6.10	6.10	0.80	1.13	± 12.0 %
1450	54.0	1.30	5.29	5.29	5.29	0.80	1.10	± 12.0 %
1640	53.7	1.42	5.18	5.18	5.18	0.80	1.17	± 12.0 %
1750	53.4	1,49	4.91	4.91	4.91	0.45	1.75	± 12.0 %
1900	53.3	1.52	4.72	4.72	4.72	0.67	1.38	± 12.0 %
2150	53.1	1.66	4.70	4.70	4.70	0.69	1.37	± 12.0 %
2450	52.7	1.95	4.40	4.40	4.40	0.80	1.20	± 12.0 %

#### Calibration Parameter Determined in Body Tissue Simulating Media

<sup>6</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the CorvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for CorvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of CorvF assessed at 8 MHz is 4-9 MHz, and CorvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 100 MHz. <sup>6</sup> At frequencies below 3 GHz, the validity of tissue parameters (is and e) can be relaxed to ± 10% If liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and e) is restricted to ± 5%. The uncertainty is the RSS of the CorvF uncertainty for indicated target tissue parameters. (c and the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: ES3-3320\_Jan20


Page 6 of 23



ES3DV3- \$N:3320

January 20, 2020

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

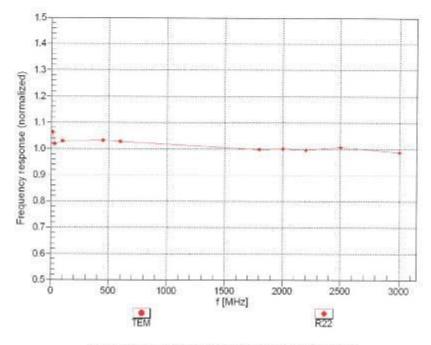

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Certificate No: ES3-3320\_Jan20

Page 7 of 23

ES3DV3-- SN:3320

January 20, 2020

CTC I advanced

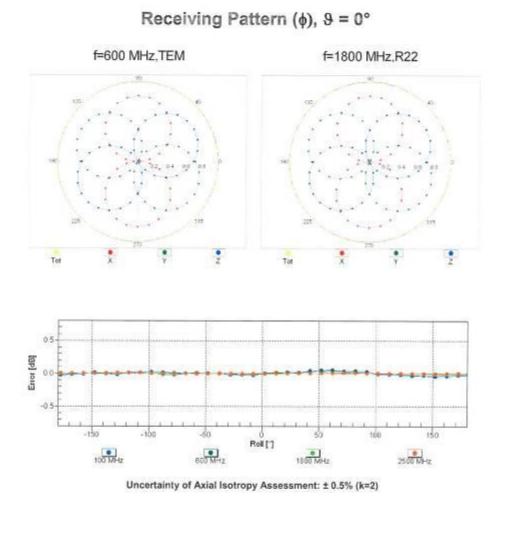


Certificate No: ES3-3320\_Jan20

Page 8 of 23



January 20, 2020

CTC | advanced

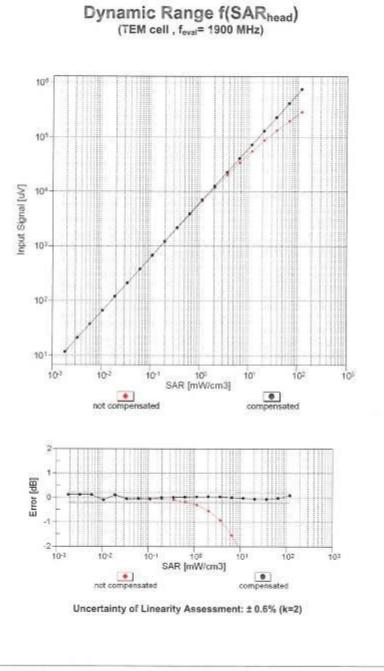


Certificate No: ES3-3320\_Jan20

Page 9 of 23

ES3DV3- SN:3320

January 20, 2020

CTC I advanced

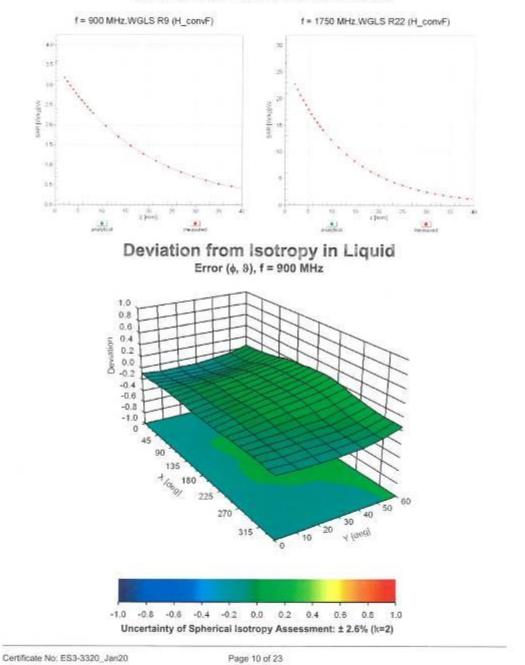

### Conversion Factor Assessment



ES3DV3-- SN:3320

January 20, 2020

#### Appendix: Modulation Calibration Parameters

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> (k=2)
0		CW	CW	0.00	± 4.7 %
10010	CAA	SAR Validation (Square, 100ms, 10ms)	Test	10.00	± 9.6 %
10011	CAB	UMTS-FDD (WCDMA)	WCDMA	2.91	± 9.6 %
10012	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	WLAN	1,87	± 9.6 %
10013	CAB	IEEE 802.11g WIFI 2.4 GHz (DSSS-OFDM, 6 Mbps)	WLAN	9.46	± 9.6 %
10021	DAC	GSM-FDD (TDMA, GMSK)	GSM	9.39	± 9.6 %
10023	DAC	GPRS-FDD (TDMA, GMSK, TN 0)	GSM	9.57	±9.6 %
10024	DAC	GPRS-FDD (TDMA, GMSK, TN 0-1)	GSM	6.56	± 9.6 %
10025	DAC	EDGE-FDD (TDMA, 8PSK, TN 0)	GSM	12.62	±9.6 %
10026	DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1)	GSM	9.55	±9.6 %
10027	DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	GSM	4.80	±9.6 %
10028	DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	GSM	3.55	± 9.6 %
10029	DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	GSM	7.78	± 9.6 %
10030	CAA	IEEE 802.15.1 Bluetooth (GFSK, DH1)	Bluetooth	5.30	±9.6 %
10031	CAA	IEEE 802.15.1 Bluetooth (GFSK, DH3)	Bluetooth	1.87	± 9.6 %
10032	CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	Bluetooth	1.16	±9.6 %
10033	CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH1)	Bluetooth	7.74	±9.6 %
10034	CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH3)	Bluetooth	4.53	± 9.6 %
10035	CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH5)	Bluetooth	3.83	±9.6 %
10036	CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH1)	Bluetooth	8.01	± 9.6 %
10037	CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH3)	Bluetooth	4.77	± 9.6 %
10038	CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH5)	Bluetooth	4.10	± 9.6 %
10039	CAB	CDMA2000 (1xRTT, RC1)	CDMA2000	4.57	± 9.6 %
10042	CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Haifrate)	AMPS	7.78	± 9.6 %
10044	CAA	IS-91/EIA/TIA-553 FDD (FDMA, FM)	AMPS	0.00	± 9.6 %
10048	CAA	DECT (TDD, TDMA/FDM, GFSK, Full Slot, 24)	DECT	13.80	± 9.6 %
10049	CAA	DECT (TDD, TDMA/FDM, GFSK, Double Slot, 12)	DECT	10.79	±9.6 %
10056	CAA	UMTS-TDD (TD-SCDMA, 1.28 Mcps)	TD-SCDMA	11.01	± 9.6 %
10058	DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	GSM	6.52	±9.6 %
10059	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps)	WLAN	2.12	± 9.6 %
10060	CAB	IEEE 802.11b WIFI 2.4 GHz (DSSS, 5.5 Mbps)	WLAN	2.83	±9.6 %
10061	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps)	WLAN	3.60	±9.6 %
10062	CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps)	WLAN	8.68	±9.6.%
10063	CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps)	WLAN	8.63	± 9.6 %
10064	CAC	IEEE 802.11a/h WIFi 5 GHz (OFDM, 12 Mbps)	WLAN	9.09	±9.6 %
10065	CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps)	WLAN	9.00	±9.6 %
10066	CAC	IEEE 802.11a/h WIFI 5 GHz (OFDM, 24 Mbps)	WLAN	9.38	±9.6 %
10067	CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps)	WLAN	10.12	±9.6 %
10068	CAC	IEEE 802.11a/h WIFI 5 GHz (OFDM, 48 Mbps)	WLAN	10.24	±9.6 %
10069	CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps)	WLAN	10.56	±9.6 %
10071	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 9 Mbps)	WLAN	9.83	±9.6%
10072	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 12 Mbps)	WLAN	9.62	±9.6 %
10073	CAB	IEEE 802.11g WIFI 2.4 GHz (DSSS/OFDM, 18 Mbps)	WLAN	9.94	±9.6 %
10074	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 24 Mbps)	WLAN	10.30	±9.6%
10075	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 36 Mbps)	WLAN	10.77	±9.6 %
10076	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 48 Mbps)	WLAN	10.94	±9.6%
10077	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 54 Mbps)	WLAN	11.00	±9.6%
10081	CAB	CDMA2000 (1xRTT, RC3)	CDMA2000	3.97	± 9.6 %
10082	CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Fullrate)	AMPS	4.77	±9.6 %
10090	DAC	GPRS-FDD (TDMA, GMSK, TN 0-4)	GSM	6.56	± 9.6 %
10097	CAB	UMTS-FDD (HSDPA)	WÇDMA	3.98	±9.6 %
10098	CAB	UMTS-FDD (HSUPA, Subtest 2)	WCDMA	3.98	±9.6 %
10099	DAC	EDGE-FDD (TDMA, 8PSK, TN 0-4)	GSM	9.55	± 9.6 %
10100	CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	LTE-FDD	5.67	±9.6 %
10101	CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	LTE-FDD	6.42	±9.6 %
10102	CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	LTE-FDD	6.60	±9.6 %
10103	CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	LTE-TDD	9.29	±9.6 %
10104	CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	LTE-TDD	9.97	±9.6 %
10105	CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	LTE-TDD	10.01	±9.6 %
10108	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	LTE-FDD	5.80	± 9.6 %

Certificate No: ES3-3320\_Jan20

Page 11 of 23



0220	CAC	IEEE 802.11n (HT Mixed, 43.3 Mbps, 16-QAM)	WLAN	8.13	±9.6 %
0221	CAC	IEEE 802.11n (HT Mixed, 72.2 Mbps, 64-QAM)	WLAN	8.27	± 9.6 %
0222	CAC	IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)	WLAN	8.06	± 9.6 %
0223	CAC	IEEE 802.11n (HT Mixed, 90 Mbps, 16-QAM)	WLAN	8.48	±9.6 9
0224	CAC	IEEE 802.11n (HT Mixed, 150 Mbps, 64-QAM)	WLAN	8.08	± 9.6 9
0225	CAB	UMTS-FDD (HSPA+)	WCDMA	5.97	19.69
0226	CAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	LTE-TDD	9.49	± 9.6 %
0227	CAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	LTE-TDD	10.26	±9.6 %
0228	CAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	LTE-TDD	9.22	± 9.6 %
0229	CAD	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	LTE-TDD	9.48	± 9.6 %
0230	CAD	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	LTE-TDD	10.25	± 9.6 %
)232	CAD	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	LTE-TDD	9.19	±9.6%
)233	CAG	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM) LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	LTE-TDD LTE-TDD	9.48	± 9.6 %
1234	CAG	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	LTE-TDD	9.21	± 9.6 %
)235	CAG	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	LTE-TDD	9.48	± 9.6 %
0236	CAG	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	LTE-TDD	10.25	± 9.6 %
0237	CAG	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	LTE-TDD	9.21	± 9.6 %
0238	CAF	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	LTE-TDD	9.48	± 9.6 %
0239	CAF	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	LTE-TDD	10.25	± 9.6 %
0240	CAF	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	LTE-TDD	9.21	± 9.6 %
0241	CAB	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	LTE-TDD	9.82	± 9.6 %
0242	CAB	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	LTE-TDD	9.86	± 9.6 %
0243	CAB	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	LTE-TDD	9.46	±9.6 %
0244	CAD	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	LTE-TDD	10.05	±9.6 %
0245	CAD	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	LTE-TDD	10.06	± 9.6 %
0246	CAD	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	LTE-TDD	9,30	±9.6 %
0247	CAG	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	LTE-TDD	9.91	± 9.6 %
0248	CAG	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	LTE-TDD	10.09	± 9.6 %
249	CAG	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK) LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	LTE-TDD LTE-TDD	9.29 9.81	± 9.6 %
251	CAG	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	LTE-TDD	10.17	± 9.6 %
252	CAG	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	LTE-TDD	9.24	±9.6%
253	CAF	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	LTE-TDD	9.90	± 9.6 %
254	CAF	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	LTE-TDD	10.14	± 9.6 %
255	CAF	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	LTE-TDD	9.20	± 9.6 %
256	CAB	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	LTE-TDD	9.96	± 9.6 %
257	CAB	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-TDD	10.08	± 9.6 %
258	CAB	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	LTE-TDD	9.34	± 9.6 %
259	CAD	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	LTE-TDD	9.98	± 9.6 %
260	CAD	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	LTE-TDD	9.97	± 9.6 %
261	CAD	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	LTE-TDD	9.24	± 9.6 %
262	CAG	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	LTE-TDD	9.83	± 9.6 %
263	CAG	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	LTE-TDD	10.16	± 9.6 %
264	CAG	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	LTE-TDD	9.23	± 9.6 %
265	CAG	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM) LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	LTE-TDD	9.92	± 9.6 %
267	CAG	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	LTE-TDD	9.30	± 9.6 %
268	CAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-TDD	10.06	± 9.6 %
269	CAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-TDD	10.13	± 9.6 %
270	CAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	LTE-TDD	9.58	± 9.6 %
274	CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)	WCDMA	4.87	± 9.6 %
275	CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	WCDMA	3.96	± 9.6 %
277	CAA	PHS (QPSK)	PHS	11.81	± 9.6 %
278	CAA	PHS (QPSK, BW 884MHz, Rolloff 0.5)	PHS	11.81	±9.6 %
279	CAA	PHS (QPSK, BW 884MHz, Rolloff 0.38)	PHS	12.18	± 9.6 %
290	AAB	CDMA2000, RC1, SO55, Full Rate	CDMA2000	3.91	±9.6 %
291	AAB	CDMA2000, RC3, SO55, Full Rate	CDMA2000	3.46	± 9.6 %
292	AAB	CDMA2000, RC3, SO32, Full Rate	CDMA2000	3.39	±9.6 %
293	AAB	CDMA2000, RC3, SO3, Full Rate	CDMA2000	3.50	± 9.6.%
295	AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	CDMA2000	12.49	± 9.6 %
297	AAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	LTE-FDD	5.81	± 9.6 %
298	AAD	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK) LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	LTE-FDD LTE-FDD	5.72 6.39	± 9.6 %

Certificate No: ES3-3320\_Jan20

Page 13 of 23



ES3DV3- SN:3320

January 20, 2020

10451	AAA	W-CDMA (BS Test Model 1, 64 DPCH, Clipping 44%)	WCDMA	7.59	± 9.6 %
10453	AAD	Validation (Square, 10ms, 1ms)	Test	10.00	± 9.6 %
10456	AAB	IEEE 802.11ac WiFi (160MHz, 64-QAM, 99pc duty cycle)	WLAN	8.63	± 9.6 %
10457	AAA	UMTS-FDD (DC-HSDPA)	WCDMA	6.62	± 9.6 %
10458	AAA	CDMA2000 (1xEV-DO, Rev. B, 2 carriers)	CDMA2000	6.55	± 9.6 %
10459	AAA	CDMA2000 (1xEV-DO, Rev. B, 3 carriers)	CDMA2000	8.25	± 9.6 %
10460	AAA	UMTS-FDD (WCDMA, AMR)	WCDMA	2.39	± 9.6 %
10461	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.82	± 9.6 %
10462	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.30	± 9.6 %
10463	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.56	± 9.6 %
10464	AAC	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.82	±9.6 %
10465	AAC	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM, UL	LTE-TDD	8.32	± 9.6 %
10466	AAC	Subframe=2,3,4,7,8,9) LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM, UL	LTE-TDD	8.57	± 9.6 %
10467	AAF	Subframe=2,3,4,7,8,9) LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL	LTE-TDD	7.82	± 9.6 %
10468	AAF	Subframe=2,3,4,7,8,9) LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM, UL	LTE-TDD	8.32	± 9.6 %
10469	AAF	Subframe=2,3,4,7,8,9) LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM, UL	LTE-TDD	8.56	± 9.6 %
	AAF	Subframe=2,3,4,7,8,9)	LTE-TDD		
10470	199.00	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2.3,4,7,8,9)	12136-212/2010	7.82	± 9.6 %
10471	AAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDO	8.32	± 9.6 %
10472	AAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.57	± 9.6 %
10473	AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.82	± 9.6 %
10474	AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.32	± 9.6 %
10475	AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.57	± 9.6 %
10477	AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL	LTE-TDD	8.32	± 9.6 %
10478	AAF	Subframe=2,3,4,7,8,9) LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM, UL	LTE-TDD	B.57	± 9.6 %
10479	AAB	Subframe=2.3,4,7,8,9) LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL	LTE-TDD	7.74	± 9.6 %
10480	AAB	Subframe=2,3,4,7,8,9) LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL	LTE-TDD	8.18	±9.6 %
10481	AAB	Subframe=2,3,4,7,8,9) LTE-TDD (SC-FDMA, 50% RB, 1,4 MHz, 64-QAM, UL	LTE-TDD	8.45	± 9.6 %
10482	AAC	Subframe=2.3,4,7,8,9) LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK, UL	LTE-TDD	7.71	± 9.6 %
		Subframe=2,3,4,7,8,9)		C-SARCA	01.0040.0000
10483	AAC	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.39	± 9.6 %
10484	AAC	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.47	±9.6 %
10485	AAF	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	LTE-TDD	7.59	±9.6 %
10486	AAF	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	LTE-TDD	8.38	± 9.6 %
10487	AAF	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM, UL Subframe=2.3.4,7.8,9)	LTE-TDD	8.60	± 9.6 %
10488	AAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL	LTE-TDD	7.70	±9.6 %
10489	AAF	Subframe=2,3,4,7,8,9) LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL	LTE-TDD	8.31	± 9.6 %
10490	AAF	Subframe=2,3,4,7,8,9) LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM, UL	LTE-TDD	8.54	± 9.6 %
	1.5.5.	Subframe=2,3,4,7,8,9)			

Certificate No: ES3-3320\_Jan20

Page 15 of 23



					-
10534	AAB	IEEE 802.11ac WIFI (40MHz, MCS0, 99pc duty cycle)	WLAN	8.45	± 9.6 %
10535	AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 99pc duty cycle)	WLAN	8.45	± 9.6 %
0536	AAB	IEEE 802.11ac WiFi (40MHz, MCS2, 99pc duty cycle)	WLAN	8.32	± 9.6 %
0537	AAB	IEEE 802.11ac WiFi (40MHz, MCS3, 99pc duty cycle)	WLAN	8.44	± 9.6 %
0538	AAB	IEEE 802.11ac WiFi (40MHz, MCS4, 99pc duty cycle)	WLAN	8.54	± 9.6 %
0540	AAB	IEEE 802.11ac WiFi (40MHz, MCS6, 99pc duty cycle)	WLAN	8.39	± 9.6 %
10541	AAB	IEEE 802.11ac WiFi (40MHz, MCS7, 99pc duty cycle)	WLAN	8.46	± 9.6 %
10542	AAB	IEEE 802.11ac WiFi (40MHz, MCS8, 99pc duty cycle)	WLAN	8.65	± 9.6 %
10543	AAB	IEEE 802.11ac WiFi (40MHz, MCS9, 99pc duty cycle)	WLAN	8.65	±9.6 %
10544	AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)	WLAN	8.47	± 9.6 %
10545	AAB	IEEE 802,11ac WiFi (80MHz, MCS1, 99pc duty cycle)	WLAN	8.55	±9.6 %
10546	AAB	IEEE 802.11ac WiFi (80MHz, MCS2, 99pc duty cycle)	WLAN	8.35	±9.6 %
10547	AAB	IEEE 802.11ac WiFi (80MHz, MCS3, 99pc duty cycle)	WLAN	8.49	±9.6 %
10548	AAB	IEEE 802.11ac WiFi (80MHz, MCS4, 99pc duty cycle)	WLAN	8.37	± 9.6 %
10550	AAB	IEEE 802.11ac WiFi (80MHz, MCS6, 99pc duty cycle)	WLAN	8.38	± 9.6 %
10551	AAB	IEEE 802.11ac WiFi (80MHz, MCS7, 99pc duty cycle)	WLAN	8.50	± 9.6 %
10552	AAB	IEEE 802.11ac WiFi (80MHz, MCS8, 99pc duty cycle)	WLAN	8.42	± 9.6 %
0553	AAB	IEEE 802.11ac WiFi (80MHz, MCS9, 99pc duty cycle)	WLAN	8.45	±9.6 %
0554	AAC	IEEE 802.11ac WiFi (160MHz, MCS0, 99pc duty cycle)	WLAN	8.48	±9.6 %
0555	AAC	IEEE 802.11ac WiFi (160MHz, MCS1, 99pc duty cycle)	WLAN	8.47	± 9.6 %
0556	AAC	IEEE 802.11ac WiFi (160MHz, MCS2, 99pc duty cycle)	WLAN	8.50	± 9.6 %
10557	AAC	IEEE 802.11ac WiFi (160MHz, MCS3, 99pc duty cycle)	WLAN	8.52	± 9.6 %
10558	AAC	IEEE 802.11ac WiFi (160MHz, MCS4, 99pc duty cycle)	WLAN	8.61	±9.6 %
10560	AAC	IEEE 802.11ac WiFi (160MHz, MCS6, 99pc duty cycle)	WLAN	8.73	± 9.6 %
10561	AAC	IEEE 802.11ac WiFi (160MHz, MCS7, 99pc duty cycle)	WLAN	8.56	± 9.6 %
0562	AAC	IEEE 802.11ac WiFi (160MHz, MCS8, 99pc duty cycle)	WLAN	8.69	±9.6 %
0563	AAC	IEEE 802.11ac WiFi (160MHz, MCS9, 99pc duty cycle)	WLAN	8.77	± 9.6 %
0564	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 99pc duty	WLAN	8.25	± 9.6 %
0565	AAA	cycle) IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 99pc duty	WLAN	8.45	± 9.6 %
10566	AAA	cycle) IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 99pc duty	WLAN	8.13	± 9.6 %
		cycle)			
10567	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 99pc duty cycle)	WLAN	8.00	± 9.6 %
10568	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 99pc duty cycle)	WLAN	8.37	± 9.6 %
10569	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 99pc duty cycle)	WLAN	8.10	± 9.6 %
10570	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 99pc duty cycle)	WLAN	8.30	± 9.6 %
0571	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	WLAN	1.99	± 9.6 %
0572	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	WLAN	1.99	± 9.6 %
0573	AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 90pc duty cycle)	WLAN	1.98	± 9.6 %
0574	AAA	IEEE 802.11b WIFI 2.4 GHz (DSSS, 11 Mbps, 90pc duty cycle)	WLAN	1.98	± 9.6 %
0575	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	WLAN	8.59	± 9.6 %
0576	AAA	IÉEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)	WLAN	8.60	±9.6 %
0577	AAA	IÉEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 90pc duty cycle)	WLAN	8.70	±9.6 %
0578	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 90pc duty cycle)	WLAN	8.49	±9.6 %
0579	AAA	IEEE 802.11g WIFI 2.4 GHz (DSSS-OFDM, 24 Mbps, 90pc duty cycle)	WLAN	8.36	± 9.6 %
0580	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 90pc duty cycle)	WLAN	8.76	±9.6 %
0581	AAA	IEEE 802.11g WIFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 90pc duty cycle)	WLAN	8.35	±9.6 %
0582	AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 90pc duty cycle)	WLAN	8.67	±9.6 %
0583	AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)	WLAN	8.59	± 9.6 %
0584	AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle)	WLAN	8.60	± 9.6 %
0585	AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 90pc duty cycle)	WLAN	8.70	± 9.6 %
		the second	1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1		

Certificate No: ES3-3320\_Jan20

Page 17 of 23



10654	AAD	LTE-TDD (OFDMA, 15 MHz, E-TM 3.1, Clipping 44%)	LTE-TDD	6.96	± 9.6 %
0655	AAE	LTE-TDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	LTE-TDD	7.21	± 9.6 %
0658	AAA	Pulse Waveform (200Hz, 10%)	Test	10.00	±9.6 %
0659	AAA	Pulse Waveform (200Hz, 20%)	Test	6.99	±9.6 %
0660	AAA	Pulse Waveform (200Hz, 40%)	Test	3.98	± 9.6 %
0661	AAA	Pulse Waveform (200Hz, 60%)	Test	2.22	±9.6 %
0662	AAA	Pulse Waveform (200Hz, 80%)	Test	0.97	± 9.6 %
0670	AAA	Bluetooth Low Energy	Bluetooth	2.19	±9.6 %
0671	AAA	IEEE 802.11ax (20MHz, MCS0, 90pc duty cycle)	WLAN	9.09	± 9.6 %
0672	AAA	IEEE 802.11ax (20MHz, MCS1, 90pc duty cycle)	WEAN	8.57	± 9.6 %
0673	AAA	IEEE 802.11ax (20MHz, MCS2, 90pc duty cycle)	WLAN	8.78	±9.6 %
0674	AAA	IEEE 802.11ax (20MHz, MCS3, 90pc duty cycle)	WLAN	8.74	± 9.6 %
0675	AAA	IEEE 802.11ax (20MHz, MCS4, 90pc duty cycle)	WLAN	8.90	± 9.6 %
0676	AAA	IEEE 802.11ax (20MHz, MCS5, 90pc duty cycle)		8.77	± 9.6 %
0678	AAA	IEEE 802.11ax (20MHz, MCS6, 90pc duty cycle)	WLAN	8.73	± 9.6 %
0679	AAA	IEEE 802.11ax (20MHz, MCS7, 90pc duty cycle) IEEE 802.11ax (20MHz, MCS8, 90pc duty cycle)	WEAN	8.78	± 9.6 %
0680	AAA	IEEE 802.11ax (20MHz, MCS9, 90pc duty cycle)	WLAN	8.80	19.6 %
0681	AAA	IEEE 802.11ax (20MHz, MCS10, 90pc duty cycle)	WLAN	8.62	± 9.6 %
0682	AAA	IEEE 802.11ax (20MHz, MCS10, 30pc duty cycle)	WLAN	8.83	± 9.6 %
0683	AAA	IEEE 802.11ax (20MHz, MCS0, 99pc duty cycle)	WLAN	8.42	± 9.6 %
0684	AAA	IEEE 802.11ax (20MHz, MCS1, 99pc duty cycle)	WLAN	8.26	19.6 %
0685	AAA	IEEE 802.11ax (20MHz, MCS2, 99pc duty cycle)	WLAN	8.33	± 9.6 %
0686	AAA	IEEE 802.11ax (20MHz, MCS3, 99pc duty cycle)	WLAN	8.28	± 9.6 %
0687	AAA	IEEE 802.11ax (20MHz, MCS4, 99pc duty cycle)	WLAN	8.45	± 9.6 %
0688	AAA	IEEE 802.11ax (20MHz, MCS5, 99pc duty cycle)	WLAN	8.29	± 9.6 %
0689	AAA	IEEE 802.11ax (20MHz, MCS6, 99pc duty cycle)	WLAN	8.55	± 9.6 %
0690	AAA	IEEE 802.11ax (20MHz, MCS7, 99pc duty cycle)	WLAN	8.29	± 9.6 %
0691	AAA	IEEE 802.11ax (20MHz, MCS8, 99pc duty cycle)	WLAN	8.25	± 9.6 %
0692	AAA	IEEE 802.11ax (20MHz, MCS9, 99pc duty cycle)	WLAN	8.29	± 9.6 %
0693	AAA	IEEE 802.11ax (20MHz, MCS10, 99pc duty cycle)	WLAN	8.25	± 9.6 %
0694	AAA	IEEE 802.11ax (20MHz, MCS11, 99pc duty cycle)	WLAN	8.57	± 9.6 %
0695	AAA	IEEE 802.11ax (40MHz, MCS0, 90pc duty cycle)	WLAN	8.78	± 9.6 %
0696	AAA	IEEE 802.11ax (40MHz, MCS1, 90pc duty cycle)	WLAN	8.91	± 9.6 %
0697	AAA	IEEE 802.11ax (40MHz, MCS2, 90pc duty cycle)	WLAN	8.61	±.9.6 %
0698	AAA	IEEE 802.11ax (40MHz, MCS3, 90pc duty cycle)	WLAN	8.89	±9.6 %
0699	AAA	IEEE 802.11ax (40MHz, MCS4, 90pc duty cycle)	WLAN	8.82	± 9.6 %
0700	AAA	IEEE 802.11ax (40MHz, MCS5, 90pc duty cycle)	WLAN	8.73	± 9.6 %
0701	AAA	IEEE 802.11ax (40MHz, MCS6, 90pc duty cycle)	WLAN	8.86	± 9.6 %
0702	AAA	IEEE 802.11ax (40MHz, MCS7, 90pc duty cycle)	WLAN	8.70	± 9.6 %
0703	AAA	IEEE 802.11ax (40MHz, MCS8, 90pc duty cycle) IEEE 802.11ax (40MHz, MCS9, 90pc duty cycle)	WLAN WLAN	8.82 8.56	± 9.6 %
0705	AAA	IEEE 802.11ax (40MHz, MCS9, 90pc duty cycle)	WLAN		± 9.6 %
0706	AAA	IEEE 802.11ax (40MHz, MCS10, 50pc duty cycle)	WLAN	8.69	± 9.6 %
0707	AAA	IEEE 802.11ax (40MHz, MCS0, 99pc duty cycle)	WLAN	8.32	± 9.6 %
0708	AAA	IEEE 802.11ax (40MHz, MCS1, 99pc duty cycle)	WLAN	8.55	±9.6 %
0709	AAA	IEEE 802.11ax (40MHz, MCS2, 99pc duty cycle)	WLAN	8.33	± 9.6 %
0710	AAA	IEEE 802.11ax (40MHz, MCS3, 99pc duty cycle)	WLAN	8.29	± 9.6 %
0711	AAA	IEEE 802.11ax (40MHz, MCS4, 99pc duty cycle)	WLAN	8.39	± 9.6 %
0712	AAA	IEEE 802.11ax (40MHz, MCS5, 99pc duty cycle)	WLAN	8.67	±9.6 %
0713	AAA	IEEE 802.11ax (40MHz, MCS6, 99pc duty cycle)	WLAN	B.33	± 9.6 %
0714	AAA	IEEE 802.11ax (40MHz, MCS7, 99pc duty cycle)	WLAN	8.26	±9.6%
0715	AAA	IEEE 802.11ax (40MHz, MCS8, 99pc duty cycle)	WLAN	8.45	±9.6 %
0716	AAA	IEEE 802.11ax (40MHz, MCS9, 99pc duty cycle)	WLAN	8.30	± 9.6 %
0717	AAA	IEEE 802.11ax (40MHz, MCS10, 99pc duty cycle)	WLAN	8.48	± 9.6 %
0718	AAA	IEEE 802.11ax (40MHz, MCS11, 99pc duty cycle)	WLAN	8.24	±9.6 %
0719	AAA	IEEE 802.11ax (80MHz, MCS0, 90pc duty cycle)	WLAN	8.81	± 9.6 %
0720	AAA	IEEE 802.11ax (80MHz, MCS1, 90pc duty cycle)	WLAN	8.87	±9.6 %
0721	AAA	IEEE 802.11ax (80MHz, MCS2, 90pc duty cycle)	WLAN	8.76	±9.6 %
0722	AAA	IEEE 802.11ax (80MHz, MCS3, 90pc duty cycle)	WLAN	8.55	±9.6%
0723	AAA	IEEE 802.11ax (80MHz, MCS4, 90pc duty cycle)	WLAN	8.70	± 9.6 %
0724	AAA	IEEE 802.11ax (80MHz, MCS5, 90pc duty cycle)	WLAN	8.90	±9.6 %
	AAA	IEEE 802.11ax (80MHz, MCS6, 90pc duty cycle)	WLAN	8.74	± 9.6 %

Certificate No: ES3-3320\_Jan20

Page 19 of 23



ES3DV3- SN:3320

January 20, 2020

	- and the		TDD		1000
10783	AAB	5G NR (CP-OFDM, 100% RB, 5 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.31	±9.6 %
10784	AAB	5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.29	± 9.6 %
10785	AAB	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.40	±9.6 %
10786	AAB	5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.35	± 9.6 %
10787	AAB	5G NR (CP-OFDM, 100% RB, 25 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.44	±9.6 %
10788	AAB	5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.39	± 9.6 %
10789	AAB	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.37	± 9.6 %
10790	AAB	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.39	± 9.6 %
10791	AAB	5G NR (CP-OFDM, 1 RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.83	± 9.6 %
10792	AAB	5G NR (CP-OFDM, 1 RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.92	± 9.6 %
10793	AAB	5G NR (CP-OFDM, 1 RB, 15 MHz, QPSK, 30 kHz)	SG NR FR1 TDD	7.95	± 9.6 %
10794	AAB	5G NR (CP-OFDM, 1 RB, 20 MHz, GPSK, 30 kHz)	5G NR FR1 TDD	7.82	±9.6 %
10795	AAB	5G NR (CP-OFDM, 1 RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.84	± 9.6 %
10796	AAB	5G NR (CP-OFDM, 1 RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.82	± 9.6 %
10797	AAB	5G NR (CP-OFDM, 1 RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.01	± 9.6 %
10798	AAB	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.89	± 9.6 %
10799	AAB	5G NR (CP-OFDM, 1 RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.93	±9.6 %
10801	AAB	5G NR (CP-OFDM, 1 RB, 80 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.89	± 9.6 %
10802	AAB	5G NR (CP-OFDM, 1 RB, 90 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.87	± 9.6 %
10803	AAB	5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7,93	±9.6 %
10805	AAB	5G NR (CP-OFDM, 50% RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	± 9.6 %
10806	AAB	5G NR (CP-OFDM, 50% RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.37	± 9.6 %
10809	AAB	5G NR (CP-OFDM, 50% RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	± 9.6 %
10810	AAB	5G NR (CP-OFDM, 50% RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	± 9.6 %
10812	AAB	5G NR (CP-OFDM, 50% RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.35	± 9.6 %
10817	AAB	5G NR (CP-OFDM, 100% RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.35	± 9.6 %
10818	AAB	5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	± 9.6 %
10819	AAB	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.33	± 9.6 %
10820	AAB	5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.30	± 9.6 %
10821	AAB	5G NR (CP-OFDM, 100% RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.41	±9.6 %
10822	AAB	5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.41	± 9.6 %
10823	AAB	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.36	± 9.6 %
10824	AAB	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1	8.39	± 9.6 %

Certificate No: ES3-3320\_Jan20

Page 21 of 23



ES3DV3- SN:3320

January 20, 2020

			TDD		
10871	AAC	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	5.75	± 9.6 %
10872	AAC	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.52	±9.6 %
10873	AAC	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.61	± 9.6 %
10874	AAC	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.65	± 9.6 %
10875	AAC	5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	7.78	±9.6.3
10876	AAC	5G NR (CP-OFDM, 100% RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	8.39	± 9.6 %
10877	AAC	5G NR (CP-OFDM, 1 RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	7.95	±9.6 %
10878	AAC	5G NR (CP-OFDM, 100% RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	8.41	± 9.6 %
10879	AAC	5G NR (CP-OFDM; 1 RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.12	± 9.6 %
10880	AAC	5G NR (CP-OFDM, 100% RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.38	±9.6 %
10881	AAC	5G NR (DFT-8-OFDM, 1 RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.75	± 9.6 %
10882	AAC	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.96	± 9.6 %
10883	AAC	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.57	± 9.6 %
10884	AAC	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, 160AM, 120 kHz)	5G NR FR2 TDD	6.53	± 9.6 %
10885	AAC	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.61	# 9.6 %
10886	AAC	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.65	±9.6 %
10887	AAC	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	7.78	± 9.6 %
10888	AAC	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	8.35	± 9.6 %
10889	AAC	5G NR (CP-OFDM, 1 RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	8.02	± 9.6 %
10890	AAC	5G NR (CP-OFDM, 100% RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	8.40	± 9.6 %
10891	AAC	5G NR (CP-OFDM, 1 RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.13	± 9.6 %
10892	AAC	5G NR (CP-OFDM, 100% RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.41	± 9.6 %

<sup>6</sup> Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: ES3-3320\_Jan20

Page 23 of 23



### 3 Calibration report "1900 MHz System validation dipole"

	Switzerland	S S	Servizio svizzero di taratura Swiss Calibration Service
ccredited by the Swiss Accreditation he Swiss Accreditation Service i ultilateral Agreement for the rec	is one of the signatorie	s to the EA	creditation No.: SCS 0108
lient CTC advanced (			: D1900V2-5d009_May20
CALIBRATION C	ERTIFICATE		
Dbject	D1900V2 - SN:50	1009	
Calibration procedure(s)	QA CAL-05.v11 Calibration Proce	dure for SAR Validation Sources	between 0.7-3 GHz
Calibration date:	May 08, 2020		
		robability are given on the following pages an y facility: environment temperature (22 ± 3)*(	
VI calibrations have been conduct	ed in the closed laborator	$\gamma$ facility; environment temperature (22 $\pm$ 3)°(	C and humidity < 70%.
U calibrations have been conduct Calibration Equipment used (M&Ts Primary Standards	ed in the closed laborator E critical for calibration)		C and humidity < 70%. Scheduled Calibration
U calibrations have been conduct Calibration Equipment used (M&Ts Primary Standards Power meter NRP	ed in the closed laborator E critical for calibration)	y facility: environment temperature (22 ± 3)°( Cal Date (Certificate No.)	C and humidity < 70%.
Il calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power mater NRP Power sensor NRP-291	ed in the closed laborator E critical for calibration) ID # SN: 104778	y facility: environment temperature (22 ± 3)*( Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101)	C and humidity < 70%. Scheduled Calibration Apr-21
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power mater NRP Power sensor NRP-291 Power sensor NRP-291	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244	ry facility: environment temperature (22 ± 3)*( Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k) SN: 310962 / 06327	v facility: environment temperature (22 ± 3)*( Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03101)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k)	y facility: environment temperature (22 ± 3)*( Cai Date (Certificate No.) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03101) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. 217-03104)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Dec-20
All cellibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Peterence 20 dB Attanuator Pype-N mismatch combination Reference Probe EX3DV4 DAE4	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 8H9394 (20k) SN: 310962 / 06327 SN: 7349 SN: 601	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03101) 31-Mar-20 (No. 217-03104) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. EX3-7349, Dec19) 27-Dec-19 (No. DAE4-601_Dec19)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Dec-20
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power mater NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attanuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Sacondary Standards	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 013245 SN: 013245 SN: 013245 SN: 310962 / 06327 SN: 7349 SN: 601 ID #	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03106) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. DAE4-601_Dec19) 27-Dec-19 (No. DAE4-601_Dec19) Check Date (in house)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 8H9394 (20k) SN: 310962 / 06327 SN: 7349 SN: 601	Cal Date (Certificate No.) 01-Apr-20 (No. 217-0310003101) 01-Apr-20 (No. 217-0310003101) 01-Apr-20 (No. 217-03100) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. 217-03104) 31-Dec-19 (No. DAE4-601_Dec19) 27-Dec-19 (No. DAE4-601_Dec19) Check Date (in house) 30-Oct-14 (in house check Feb-19)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 013245 SN: 013245 SN: 01982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03101) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. DAE4-601_Dec19) 27-Dec-19 (No. DAE4-601_Dec19) Check Date (in house) 30-Oct-14 (in house check Feb-19) 07-Oct-15 (in house check Oct-18)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attanuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power meter E4419B Power sensor HP 8481A	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 103245 SN: 310982 / 06327 SN: 310982 / 06327 SN: 601 ID # SN: GB39512475 SN: US37292783	Cal Date (Certificate No.) 01-Apr-20 (No. 217-0310003101) 01-Apr-20 (No. 217-0310003101) 01-Apr-20 (No. 217-03100) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. 217-03104) 31-Dec-19 (No. DAE4-601_Dec19) 27-Dec-19 (No. DAE4-601_Dec19) Check Date (in house) 30-Oct-14 (in house check Feb-19)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-20
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-05	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 310962 / 06327 SN: 7349 SN: 601 ID # SN: G839512475 SN: US37292783 SN: MY41092317	2 facility: environment temperature (22 ± 3)*( Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03106) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. 247-03104) 31-Dec-19 (No. DAE4-601_Dec19) 27-Dec-19 (No. DAE4-601_Dec19) Check Date (in house) 30-Oct-14 (in house check Feb-19) 07-Oct-15 (in house check Oct-18) 07-Oct-15 (in house check Oct-18)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch containation Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4418B Power sensor HP 6481A Power sensor HP 6481A RF generator R&S SMT-05 Network Analyzer Agitent EB358A	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103244 SN: 103245 SN: 8149394 (20k) SN: 310962 / 06327 SN: 601 ID # SN: 6039512475 SN: 0839512475 SN: 0839512475 SN: 08392512475 SN: 08392512475 SN: 08392512475 SN: 09372	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03100) 31-Mar-20 (No. 217-03104) 31-Mar-20 (No. 217-03104) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. DAT4-601_Dec19) 27-Dec-19 (No. DAE4-601_Dec19) 20-Oct-19 (No. DAE4-601_Dec19) 20-Oct-19 (In house check Feb-19) 07-Oct-15 (In house check Cot-18) 07-Oct-15 (In house check Oct-18) 15-Jun-15 (In house check Oct-18)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch containation Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4418B Power sensor HP 6481A Power sensor HP 6481A RF generator R&S SMT-05 Network Analyzer Agitent EB358A	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 310962 / 06327 SN: 310962 / 06327 SN: 310962 / 06327 SN: 0839512475 SN: 0839512475 SN: US37292783 SN: WY41092317 SN: 100972 SN: US41080477	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03104) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. 217-03104) 31-Mar-14 (in house check Oct-19)	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 310962 / 06327 SN: 7349 SN: 601 ID # SN: 0839512475 SN: 0839512475 SN: US37292783 SN: MY41092317 SN: 100972 SN: US41080477 Name	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03108) 31-Mar-20 (No. 217-03108) 30-Oct-19 (No. DAE4-601_Dec19) Check Date (in house check Feb-19) 07-Oct-15 (in house check Feb-19) 07-Oct-15 (in house check Oct-18) 15-Jun-15 (in house check Oct-19) Function	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attanuator Type-N mismatch combination Reference 20 dB Attanuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Sacondary Standards Power meter E4419B Power sensor HP 6481A RF generator R&S SMT-06 Network Analyzer Agitent EB358A Calibrated by:	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 103245 SN: 103245 SN: 60327 SN: 601 ID # SN: 6039512475 SN: 0839512475 SN: 0839512475 SN: 0839512475 SN: 10327292783 SN: MY41092317 SN: 10972 SN: 10541080477 Name Jeton Kastrati	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100003101) 01-Apr-20 (No. 217-03100 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03100) 31-Mar-20 (No. 217-03104) 31-Mar-20 (No. 217-03104) 31-Mar-19 (No. DAE4-601_Dec19) Check Date (in house) 30-Oct-15 (in house check Feb-19) 07-Oct-15 (in house check Cot-18) 07-Oct-15 (in house check Oct-18) 31-Mar-14 (in house check Oct-19) Function Laboratory Technician	C and humidity < 70%. Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check:



#### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





- S Schweizerischer Kalibrierdienst
  - Service suisse d'étalonnage Servizio svizzero di taratura
  - Swiss Calibration Service

Accreditation No.: SCS 0108

С

s

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

e) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D1900V2-5d009\_May20

Page 2 of 8



#### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	2101/2	The standard Manual Co.
DAST version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.3 ± 6 %	1.40 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.66 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	38.9 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR everaged over 10 cm <sup>3</sup> (10 g) of Head TSL SAR measured	condition 250 mW input power	5.04 W/kg
	2.818.01800.8020	5.04 W/kg 20.3 W/kg ± 16.5 % (k=2)

Body TSL parameters The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.1 ± 6 %	1.51 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

#### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.78 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	39.4 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL SAR measured	condition 250 mW input power	5.16 W/kg

Certificate No: D1900V2-5d009\_May20

Page 3 of 8



#### Appendix (Additional assessments outside the scope of SCS 0108)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.7 Ω + 2.9 jΩ	
Return Loss	- 30.6 dB	

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.3 Ω + 3.8 jΩ				
Return Loss	- 26.5 dB				

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.189 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG	
-----------------	-------	--

Certificate No: D1900V2-5d009\_May20

Page 4 of 8



#### DASY5 Validation Report for Head TSL

Date: 07.05.2020

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d009


Communication System: UID 0 - CW; Frequency: 1900 MHz Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.4 S/m;  $\varepsilon_r$  = 41.3;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(8.6, 8.6, 8.6) @ 1900 MHz; Calibrated; 31.12.2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.12.2019
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

#### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 107.7 V/m; Power Drift = 0.02 dB Peak SAR (extrapolated) = 18.0 W/kg SAR(1 g) = 9.66 W/kg; SAR(10 g) = 5.04 W/kg Smallest distance from peaks to all points 3 dB below = 10 mm Ratio of SAR at M2 to SAR at M1 = 54.3% Maximum value of SAR (measured) = 15.1 W/kg

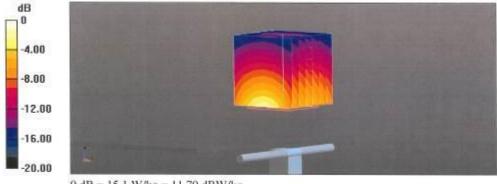


0 dB = 15.1 W/kg = 11.79 dBW/kg

Certificate No: D1900V2-5d009\_May20

Page 5 of 8



Impedance Measurement Plot for Head TSL

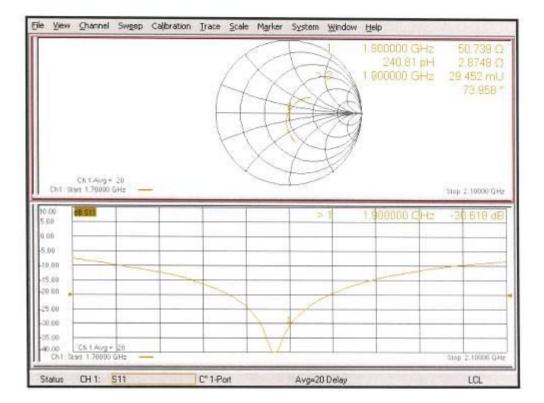

Certificate No: D1900V2-5d009\_May20.

Page 6 of 8



#### DASY5 Validation Report for Body TSL

Date: 08.05.2020

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d009


Communication System: UID 0 - CW; Frequency: 1900 MHz Medium parameters used: f = 1900 MHz;  $\sigma = 1.51$  S/m;  $\epsilon_r = 54.1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(8.42, 8.42, 8.42) @ 1900 MHz; Calibrated: 31.12.2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- · Electronics: DAE4 Sn601; Calibrated: 27.12.2019
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 104.5 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 17.2 W/kg SAR(1 g) = 9.78 W/kg; SAR(10 g) = 5.16 W/kg Smallest distance from peaks to all points 3 dB below = 9 mm Ratio of SAR at M2 to SAR at M1 = 57.8% Maximum value of SAR (measured) = 14.8 W/kg

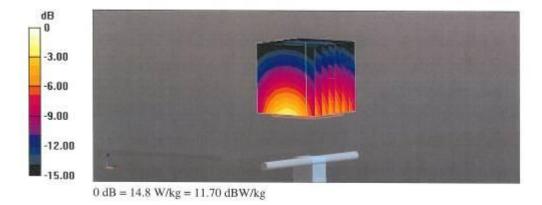


Certificate No: D1900V2-5d009\_May20

Page 7 of 8



Impedance Measurement Plot for Body TSL

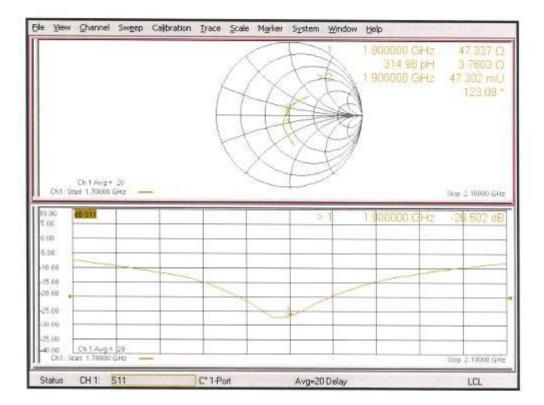

Certificate No: D1900V2-5d009\_May20

Page 8 of 8



### 4 Calibration certificate of Data Acquisition Unit (DAE)

ccredited by the Swiss Accredit he Swiss Accreditation Servi	ce is one of the signatorie	s to the EA	on No.: SCS 0108
Aultilateral Agreement for the			
Client CTC advance	d GmbH	Certificate N	lo: DAE3-413_Jan20
CALIBRATION	CERTIFICATE		
Object	DAE3 - SD 000 D	003 AA - SN: 413	
Calibration procedure(s)	QA CAL-06.v29		
	Calibration proce	dure for the data acquisition ele	ctronics (DAE)
Calibration date:	January 10, 2020		
This calibration certificate docum	nents the traceability to natio entainties with confidence pr	onal standards, which realize the physical ur obability are given on the following pages a	nits of measurements (SI). nd are part of the certificate.
The measurements and the unc	ertainties with confidence pr	obability are given on the following pages a	nd are part of the certificate.
The measurements and the unc	ertainties with confidence pr ucted in the closed laboratory	onal standards, which realize the physical us obability are given on the following pages a y facility: environment temperature (22 ± 3)°	nd are part of the certificate.
The measurements and the unco NI calibrations have been condu Calibration Equipment used (M&	ertainties with confidence pr ucted in the closed laboratory	obability are given on the following pages a	nd are part of the certificate.
The measurements and the uncomposition of the incomposition of the second of the secon	ertainties with confidence pr incled in the closed laboratory .TE oritical for calibration)	obability are given on the following pages a y facility: environment temperature (22 ± 3)°	nd are part of the certificate. C and humidity < 70%
The measurements and the unc M calibrations have been condu Calibration Equipment used (M& Primary Standards Ceithley Multimeter Type 2001	ertainties with confidence pr incled in the closed laboratory .TE oritical for calibration)	obability are given on the following pages a y facility: environment temperature (22 ± 3)° Call Date (Certificate No.)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration
The measurements and the uncount alibration Equipment used (M& <u>trimary Standards</u> eithley Multimeter Type 2001 econdary Standards uto DAE Calibration Unit	ertainties with confidence pr incled in the closed laboratory TE ontical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001	obability are given on the following pages at y facility: environment temperature (22 ± 3)° Cal Date (Certificate No.) 03-Sep-19 (No:25949) Check Date (in house) 09-Jan-20 (in house check)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Sep-20 Scheduled Check In house check: Jan-21
The measurements and the unc	ertainties with confidence pr intend in the closed laboratory TE ontical for calibration) ID # SN: 0810278 ID #	obability are given on the following pages a y facility: environment temperature (22 ± 3)° Cal Date (Certificate No.) 03-Sep-19 (No:25949) Check Date (in house)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Sep-20 Scheduled Check.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit	ertainties with confidence pr incled in the closed laboratory TE ontical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001	obability are given on the following pages at y facility: environment temperature (22 ± 3)° Cal Date (Certificate No.) 03-Sep-19 (No:25949) Check Date (in house) 09-Jan-20 (in house check)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Sep-20 Scheduled Check In house check: Jan-21
The measurements and the unco alibration Equipment used (M& <u>trimary Standards</u> eithley Multimeter Type 2001 econdary Standards uto DAE Calibration Unit alibrator Box V2.1	entainties with confidence pr incred in the closed laboratory ID # SN: 0810278 ID # SE UWS 053 AA 1001 SE UWS 005 AA 1002	obability are given on the following pages al y facility: environment temperature (22 ± 3)° Cal Date (Certificate No.) 03-Sep-19 (No:25949) Check Date (in house) 09-Jan-20 (in house check) 09-Jan-20 (in house check) Function	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Sep-20 Scheduled Check In house check: Jan-21
The measurements and the unce All calibrations have been condu- Calibration Equipment used (M& Primary Standards Secondary Standary	ertainties with confidence pr inteed in the closed laboratory TE critical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001 SE UWS 006 AA 1002	obability are given on the following pages al y facility: environment temperature (22 ± 3)° Cal Date (Certificate No.) 03-Sep-19 (No:25949) Check Date (in house) 09-Jan-20 (in house check) 09-Jan-20 (in house check)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Sep-20 Schedulad Check In house check: Jan-21 In house check: Jan-21 Signature
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit	entainties with confidence pr incred in the closed laboratory ID # SN: 0810278 ID # SE UWS 053 AA 1001 SE UWS 005 AA 1002	obability are given on the following pages al y facility: environment temperature (22 ± 3)° Cal Date (Certificate No.) 03-Sep-19 (No:25949) Check Date (in house) 09-Jan-20 (in house check) 09-Jan-20 (in house check) Function	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Sep-20 Scheduled Check In house check: Jan-21 In house check: Jan-21



#### 5 Certificate of "SAM Twin Phantom V4.0/V4.0C"

### Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

#### Certificate of conformity / First Article Inspection

ltem	SAM Twin Phantom V4.0
Type No	QD 000 P40 BA
Series No	TP-1002 and higher
Manufacturer / Origin	Untersee Composites Hauptstr. 69 CH-8559 Fruthwilen Switzerland

#### Tests

The series production process used allows the limitation to test of first articles. Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series units (called samples).

Test	Requirement	Details	Units tested
Shape	Compliance with the geometry according to the CAD model.	IT'IS CAD File (*)	First article, Samples
Material thickness	Compliant with the requirements according to the standards	2mm +/- 0.2mm in specific areas	First article, Samples
Material parameters	Dielectric parameters for required frequencies	200 MHz – 3 GHz Relative permittivity < 5 Loss tangent < 0.05.	Material sample TP 104-5
Material resistivity	The material has been tested to be compatible with the liquids defined in the standards	Liquid type HSL 1800 and others according to the standard.	Pre-series, First article

#### Standards

- [1] CENELEC EN 50361
- [2] IEEE P1528-200x draft 6.5
- [3] IEC PT 62209 draft 0.9
- (\*) The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of [1] and [3].

#### Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standard [1] and draft standards [2] and [3].

18.11.2001 Date Fin Brubelt 1 lats Schmid & Partner Signature / Stamp Engineering AG Zeughausstrasse 43, CH-8004 Zurich Tel. +41 1 245 97 00, Fax +41 1 245 97 79

Doc No 881 - QD 000 P40 BA - B

Page 1 (1)



#### 6 Application Note System Performance Check

#### 6.1 **Purpose of system performance check**

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check is performed prior to any usage of the system in order to guarantee reproducible results.

The measurement of the Specific Absorption Rate (SAR) is a complicated task and the result depends on the proper functioning of many components and the correct settings of many parameters. Faulty results due to drift, failures or incorrect parameters might not be recognized, since they often look similar in distribution to the correct ones. The Dosimetric Assessment System DASY5 incorporates a system performance check procedure to test the proper functioning of the system. The system performance check uses normal SAR measurements in a simplified setup (the flat section of the SAM Twin Phantom) with a well characterized source (a matched dipole at a specified distance). This setup was selected to give a high sensitivity to all parameters that might fail or vary over time (e.g., probe, liquid parameters, and software settings) and a low sensitivity to external effects inherent in the system (e.g., positioning uncertainty of the device holder). The system performance check does not replace the calibration of the components. The accuracy of the system performance check is not sufficient for calibration purposes. It is possible to calculate the field quite accurately in this simple setup; however, due to the open field situation some factors (e.g., laboratory reflections) cannot be accounted for. Calibrations in the flat phantom are possible with transfer calibration methods, using either temperature probes or calibrated E-field probes. The system performance check also does not test the system performance for arbitrary field situations encountered during real measurements of mobile phones. These checks are performed at SPEAG by testing the components under various conditions (e.g., spherical isotropy measurements in liquid, linearity measurements, temperature variations, etc.), the results of which are used for an error estimation of the system. The system performance check will indicate situations where the system uncertainty is exceeded due to drift or failure.

#### 6.2 System Performance check procedure

#### Preparation

The conductivity should be measured before the validation and the measured liquid parameters must be entered in the software. If the measured values differ from targeted values in the dipole document, the liquid composition should be adjusted. If the validation is performed with slightly different (measured) liquid parameters, the expected SAR will also be different. See the application note about SAR sensitivities for an estimate of possible SAR deviations. Note that the liquid parameters are temperature dependent with approximately - 0.5% decrease in permittivity and + 1% increase in conductivity for a temperature decrease of 1° C. The dipole must be placed beneath the flat phantom section of the Generic Twin Phantom with the correct distance holder in place. The distance holder should touch the phantom surface with a light pressure at the reference marking (little hole) and be oriented parallel to the long side of the phantom. Accurate positioning is not necessary, since the system will search for the peak SAR location, except that the dipole arms should be parallel to the surface. The device holder for mobile phones can be left in place but should be rotated away from the dipole. The forward power into the dipole at the dipole SMA connector should be determined as accurately as possible. The actual dipole input power level can be between 20mW and several watts. The result can later be normalized to any power level. It is strongly recommended to note the actually used power level in the "comment"-window of the measurement file; otherwise you loose this crucial information for later reference.



#### System Performance Check

The DASY5 installation includes predefined files with recommended procedures for measurements and validation. They are read-only document files and destined as fully defined but unmeasured masks, so you must save the finished validation under a different name. The validation document requires the Generic Twin Phantom, so this phantom must be properly installed in your system. (You can create your own measurement procedures by opening a new document or editing an existing document file). Before you start the validation, you just have to tell the system with which components (probe, medium, and device) you are performing the validation; the system will take care of all parameters. After the validation, which will take about 20 minutes, the results of each task are displayed in the document window. Selecting all measured tasks and opening the predefined "validation" graphic format displays all necessary information for validation. A description of the different measurement tasks in the predefined document is given below, together with the information that can be deduced from their results:

- The "reference" and "drift" measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the amplifier output power. If it is too high (above ± 0.1dB) the validation should be repeated; some amplifiers have very high drift during warm-up. A stable amplifier gives drift results in the DASY5 system below ± 0.02 dB.
- The "area scan" measures the SAR above the dipole on a parallel plane to the surface. It is used to locate the approximate location of the peak SAR with 2D spline interpolation. The proposed scan uses large grid spacing for faster measurement; due to the symmetric field the peak detection is reliable. If a finer graphic is desired, the grid spacing can be reduced. Grid spacing and orientation have no influence on the SAR result.
- The zoom scan job measures the field in a volume around the peak SAR value assessed in the previous "area" scan (for more information see the application note on SAR evaluation).

If the validation measurements give reasonable results, the peak 1g and 10g spatial SAR values averaged between the two cubes and normalized to 1W dipole input power give the reference data for comparisons. The next section analyzes the expected uncertainties of these values. Section 6 describes some additional checks for further information or troubleshooting.

#### 6.3 Uncertainty Budget

Please note that in the following Tables, the tolerance of the following uncertainty components depends on the actual equipment and setup at the user location and need to be either assessed or verified on-site by the end user of the DASY5 system:

- RF ambient conditions
- Dipole Axis to Liquid Distance
- Input power and SAR drift measurement
- Liquid permittivity measurement uncertainty
- · Liquid conductivity measurement uncertainty

Note: All errors are given in percent of SAR, so 0.1 dB corresponds to 2.3%. The field error would be half of that. The liquid parameter assessment give the targeted values from the dipole document. All errors are given in percent of SAR, so 0.1dB corresponds to 2.3%. The field error would be half of that.



#### System validation

In the table below, the system validation uncertainty with respect to the analytically assessed SAR value of a dipole source as given in the IEEE1528 standard is given. This uncertainty is smaller than the expected uncertainty for mobile phone measurements due to the simplified setup and the symmetric field distribution.

Uncertainty Budget for System Validation for the 0.3 - 6 GHz range										
Source of	Uncertainty	Probability	Divisor	Ci	Ci	Standard L	Incertainty	$v_i^2$ or		
uncertainty	Value	Distribution		(1g)	(10g)	± %, (1g) ± %, (10g)		V <sub>eff</sub>		
Measurement System										
Probe calibration	± 6.6 %	Normal	1	1	1	± 6.6 %	± 6.6 %	∞		
Axial isotropy	± 4.7 %	Rectangular	√ 3	1	1	± 2.7 %	± 2.7 %	∞		
Hemispherical isotropy	± 9.6 %	Rectangular	√ 3	0	0	± 0.0 %	± 0.0 %	∞		
Boundary effects	± 1.0 %	Rectangular	√ 3	1	1	± 0.6 %	± 0.6 %	∞		
Probe linearity	± 4.7 %	Rectangular	√ 3	1	1	± 2.7 %	± 2.7 %	∞		
System detection limits	± 1.0 %	Rectangular	√ 3	1	1	± 0.6 %	± 0.6 %	∞		
Readout electronics	± 0.3 %	Normal	1	1	1	± 0.3 %	± 0.3 %	8		
Response time	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	∞		
Integration time	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
RF ambient conditions	± 1.0 %	Rectangular	√ 3	1	1	± 0.6 %	± 0.6 %	∞		
Probe positioner	± 0.8 %	Rectangular	√ 3	1	1	± 0.5 %	± 0.5 %	8		
Probe positioning	± 6.7 %	Rectangular	√ 3	1	1	± 3.9 %	± 3.9 %	8		
Max. SAR evaluation	± 2.0 %	Rectangular	√ 3	1	1	± 1.2 %	± 1.2 %	8		
Dipole Related										
Dev. of exp. dipole	± 5.5 %	Rectangular	√ 3	1	1	± 3.2 %	± 3.2 %	8		
Dipole Axis to Liquid Dist.	± 2.0 %	Rectangular	√ 3	1	1	± 1.2 %	± 1.2 %	8		
Input power & SAR drift	± 3.4 %	Rectangular	√ 3	1	1	± 2.0 %	± 2.0 %	8		
Phantom and Set-up										
Phantom uncertainty	± 4.0 %	Rectangular	√ 3	1	1	± 2.3 %	± 2.3 %	8		
SAR correction	± 1.9 %	Rectangular	√ 3	1	0.84	± 1.1 %	± 0.9 %	∞		
Liquid conductivity (meas.)	± 5.0 %	Normal	1	0.78	0.71	± 3.9 %	± 3.6 %	8		
Liquid permittivity (meas.)	± 5.0 %	Normal	1	0.26	0.26		± 1.3 %	∞		
Temp. unc Conductivity	± 1.7 %	Rectangular	√ 3	0.78	0.71	± 0.8 %	± 0.7 %	8		
Temp. unc Permittivity	± 0.3 %	Rectangular	√ 3	0.23	0.26	± 0.0 %	± 0.0 %	8		
Combined Uncertainty						± 10.7 %	± 10.6 %	330		
Expanded Std.						± 21.4 %	± 21.1 %			
Uncertainty						± 21.4 %	± <b>21.1</b> %			

Table 1: Measurement uncertainties of the System Validation with DASY5 (0.3-6GHz). The RF ambient noise uncertainty has been reduced to  $\pm 1.0$ , considering input power levels are  $\geq 250$ mW.



#### Performance check repeatability

The repeatability check of the validation is insensitive to external effects and gives an indication of the variations in the DASY5 measurement system, provided that the same power reading setup is used for all validations. The repeatability estimates for frequencies below ad above 3GHz are given in the following tables:

Repeatability Budget for System Check for the 0.3 - 3 GHz range										
Source of	Uncertainty	Probability	Divisor	Ci	Ci	Standard I	Uncertainty	v <sup>2</sup> or		
uncertainty	Value	Distribution		(1g)	(10g)	± %, (1g) ± %, (10g)		Veff		
Measurement System										
Repeatability of probe cal.	± 1.8 %	Normal	1	1	1	± 1.8 %	± 1.8 %	∞		
Axial isotropy	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	∞		
Hemispherical isotropy	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
Boundary effects	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
Probe linearity	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
System detection limits	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
Modulation response	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
Readout electronics	± 0.0 %	Normal	1	1	1	± 0.0 %	± 0.0 %	8		
Response time	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
Integration time	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	∞		
RF ambient noise	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
RF ambient positioning	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
Probe positioner	± 0.4 %	Rectangular	√ 3	1	1	± 0.2 %	± 0.2 %	8		
Probe positioning	± 2.9 %	Rectangular	√ 3	1	1	± 1.7 %	± 1.7 %	8		
Max. SAR evaluation	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
Dipole Related										
Dev. of experimental dipole	± 0.0 %	Rectangular	√ 3	1	1	± 0.0 %	± 0.0 %	8		
Dipole axis to liquid dist.	± 2.0 %	Rectangular	√ 3	1	1	± 1.2 %	± 1.2 %	8		
Input power & SAR drift	± 3.4 %	Rectangular	√ 3	1	1	± 2.0 %	± 2.0 %	8		
Phantom and Set-up										
Phantom uncertainty	± 4.0 %	Rectangular	√ 3	1	1	± 2.3 %	± 2.3 %	∞		
SAR correction	± 1.9 %	Rectangular	√ 3	1	0.84	± 1.1 %	± 0.9 %	8		
Liquid conductivity (meas.)	± 5.0 %	Normal	1	0.78	0.71	± 3.9 %	± 3.6 %	8		
Liquid permittivity (meas.)	± 5.0 %	Normal	1	0.26	0.26	± 1.3 %	± 1.3 %	8		
Temp. unc Conductivity	± 1.7 %	Rectangular	√ 3	0.78	0.71	± 0.8 %	± 0.7 %	8		
Temp. unc Permittivity	± 0.3 %	Rectangular	√ 3	0.23	0.26	± 0.0 %	± 0.0 %	8		
Combined Uncertainty						± 5.9 %	± 5.7 %			
Expanded Std.						± 11.9 %	± 11.4 %			
Uncertainty										

Table 2: Repeatability of the System Check with DASY5 (0.3-3GHz)



Repeatability Budget for System Check for the 3 - 6 GHz range											
Source of	Und	certainty	Probability	Divisor	Ci	Ci	St	andard I	Unce	ertainty	v <sup>2</sup> or
uncertainty		Value	Distribution		(1g)	(10g)	±'	%, (1g)	± %, (10g)		V <sub>eff</sub>
Measurement System											
Repeatability of probe cal.	±	1.8 %	Normal	1	1	1	±	1.8 %	±	1.8 %	8
Axial isotropy	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	±	0.0 %	8
Hemispherical isotropy	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	±	0.0 %	8
Boundary effects	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	H	0.0 %	8
Probe linearity	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	±	0.0 %	8
System detection limits	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	±	0.0 %	8
Modulation response	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	H	0.0 %	8
Readout electronics	±	0.0 %	Normal	1	1	1	±	0.0 %	±	0.0 %	8
Response time	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	±	0.0 %	8
Integration time	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	H	0.0 %	8
RF ambient noise	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	±	0.0 %	8
RF ambient positioning	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	±	0.0 %	8
Probe positioner	±	0.8 %	Rectangular	√ 3	1	1	±	0.5 %	Ħ	0.5 %	8
Probe positioning	±	6.7 %	Rectangular	√ 3	1	1	±	3.9 %	±	3.9 %	8
Max. SAR evaluation	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	±	0.0 %	8
Dipole Related											
Dev. of experimental dipole	±	0.0 %	Rectangular	√ 3	1	1	±	0.0 %	ŧ	0.0 %	8
Dipole axis to liquid dist.	±	2.0 %	Rectangular	√ 3	1	1	±	1.2 %	±	1.2 %	8
Input power & SAR drift	±	3.4 %	Rectangular	√ 3	1	1	±	2.0 %	±	2.0 %	8
Phantom and Set-up											
Phantom uncertainty	±	4.0 %	Rectangular	√ 3	1	1	±	2.3 %	±	2.3 %	∞
SAR correction	±	1.9 %	Rectangular	√ 3	1	0.84	±	1.1 %	±	0.9 %	8
Liquid conductivity (meas.)	±	5.0 %	Normal	1	0.78	0.71	±	3.9 %		3.6 %	∞
Liquid permittivity (meas.)	±	5.0 %	Normal	1	0.26	0.26	±	1.3 %	_	1.3 %	∞
Temp. unc Conductivity	±	1.7 %	Rectangular	√ 3	0.78	0.71	±	0.8 %		0.7 %	∞
Temp. unc Permittivity	±	0.3 %	Rectangular	√ 3	0.23	0.26	±	0.0 %		0.0 %	∞
Combined Uncertainty							±	6.9 %	±	6.7 %	
Expanded Std.							+	13.8 %		13.4 %	
Uncertainty							<u> </u>	13.0 /0	<u> </u>	13.4 /0	

Table 3: Repeatability of the System Check with DASY5 (3-6GHz)


Note: Worst case probe calibration uncertainty has been applied for all probes used during the measurements.

The expected repeatability deviation is low. Excessive drift (e.g., drift in liquid parameters), partial system failures or incorrect parameter settings (e.g., wrong probe or device settings) will lead to unexpectedly high repeatability deviations. The repeatability gives an indication that the system operates within its initial specifications. Excessive drift, system failure and operator errors are easily detected.



#### 6.4 Power set-up for validation

The uncertainty of the dipole input power is a significant contribution to the absolute uncertainty and the expected deviation in interlaboratory comparisons. The values in Section 2 for a typical and a sophisticated setup are just average values. Refer to the manual of the power meter and the detector head for the evaluation of the uncertainty in your system. The uncertainty also depends on the source matching and the general setup. Below follows the description of a recommended setup and procedures to increase the accuracy of the power reading:

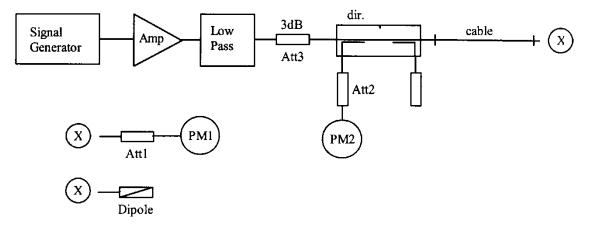

The figure shows the recommended setup. The PM1 (incl. Att1) measures the forward power at the location of the validation dipole connector. The signal generator is adjusted for the desired forward power at the dipole connector and the power meter PM2 is read at that level. After connecting the cable to the dipole, the signal generator is readjusted for the same reading at power meter PM2. If the signal generator does not allow a setting in 0.01dB steps, the remaining difference at PM2 must be noted and considered in the normalization of the validation results. The requirements for the components are:

- The signal generator and amplifier should be stable (after warm-up). The forward power to the dipole should be above 10mW to avoid the influence of measurement noise. If the signal generator can deliver 15dBm or more, an amplifier is not necessary. Some high power amplifiers should not be operated at a level far below their maximum output power level (e.g. a 100W power amplifier operated at 250mW output can be quite noisy). An attenuator between the signal generator and amplifier is recommended to protect the amplifier input.
- The low pass filter after the amplifier reduces the effect of harmonics and noise from the amplifier. For most amplifiers in normal operation the filter is not necessary.
- The attenuator after the amplifier improves the source matching and the accuracy of the power head. (See power meter manual.) It can also be used also to make the amplifier operate at its optimal output level for noise and stability. In a setup without directional coupler, this attenuator should be at least 10dB.
- The directional coupler (recommended <sup>3</sup> 20dB) is used to monitor the forward power and adjust the signal generator output for constant forward power. A medium quality coupler is sufficient because the loads (dipole and power head) are well matched. (If the setup is used for reflective loads, a high quality coupler with respect to directivity and output matching is necessary to avoid additional errors.)
- The power meter PM2 should have a low drift and a resolution of 0.01dBm, but otherwise its accuracy has no impact on the power setting. Calibration is not required.
- The cable between the coupler and dipole must be of high quality, without large attenuation and phase changes when it is moved. Otherwise, the power meter head PM1 should be brought to the location of the dipole for measuring.
- The power meter PM1 and attenuator Att1 must be high quality components. They should be calibrated, preferably together. The attenuator (<sup>3</sup>10dB) improves the accuracy of the power reading. (Some higher power heads come with a built-in calibrated attenuator.) The exact attenuation of the attenuator at the frequency used must be known; many attenuators are up to 0.2dB off from the specified value.
- Use the same power level for the power setup with power meter PM1 as for the actual measurement to avoid linearity and range switching errors in the power meter PM2. If the validation is performed at various power levels, do the power setting procedure at each level.



- The dipole must be connected directly to the cable at location "X". If the power meter has a different connector system, use high quality couplers. Preferably, use the couplers at the attenuator Att1 and calibrate the attenuator with the coupler.
- Always remember: We are measuring power, so 1% is equivalent to 0.04dB.

#### 6.5 Laboratory reflection

In near-field situations, the absorption is predominantly caused by induction effects from the magnetic nearfield. The absorption from reflected fields in the laboratory is negligible. On the other hand, the magnetic field around the dipole depends on the currents and therefore on the feed point impedance. The feed point impedance of the dipole is mainly determined from the proximity of the absorbing phantom, but reflections in the laboratory can change the impedance slightly. A 1% increase in the real part of the feed point impedance will produce approximately a 1% decrease in the SAR for the same forward power. The possible influence of laboratory reflections should be investigated during installation. The validation setup is suitable for this check, since the validation is sensitive to laboratory reflections. The same tests can be performed with a mobile phone, but most phones are less sensitive to reflections due to the shorter distance to the phantom. The fastest way to check for reflection effects is to position the probe in the phantom above the feed point and start a continuous field measurement in the DASY5 multi-meter window. Placing absorbers in front of possible reflectors (e.g. on the ground near the dipole or in front of a metallic robot socket) will reveal their influence immediately. A 10dB absorber (e.g. ferrite tiles or flat absorber mats) is probably sufficient, as the influence of the reflections is small anyway. If you place the absorber too near the dipole, the absorber itself will interact with the reactive near-field. Instead of measuring the SAR, it is also possible to monitor the dipole impedance with a network analyzer for reflection effects. The network analyzer must be calibrated at the SMA connector and the electrical delay (two times the forward delay in the dipole document) must be set in the NWA for comparisons with the reflection data in the dipole document. If the absorber has a significant influence on the results, the absorber should be left in place for validation or measurements. The reference data in the dipole document are produced in a low reflection environment.

#### 6.6 Additional system checks

While the validation gives a good check of the DASY5 system components, it does not include all parameters necessary for real phone measurements (e.g. device modulation or device positioning). For system validation (repeatability) or comparisons between laboratories a reference device can be useful. This can be any mobile phone with a stable output power (preferably a device whose output power can be set through the keyboard). For comparisons, the same device should be sent around, since the SAR variations between samples can be large. Several measurement possibilities in the DASY5 software allow additional tests of the performance of the DASY5 system and components. These tests can be useful to localize component failures:

- The validation can be performed at different power levels to check the noise level or the correct compensation of the diode compression in the probe.
- If a pulsed signal with high peak power levels is fed to the dipole, the performance of the diode compression compensation can be tested. The correct crest factor parameter in the DASY5 software must be set (see manual). The system should give the same SAR output for the same averaged input power.
- The probe isotropy can be checked with a 1D-probe rotation scan above the feed point. The automatic probe alignment procedure must be passed through for accurate probe rotation movements (optional DASY5 feature with a robot-mounted light beam unit). Otherwise the probe tip might move on a small circle during rotation, producing some additional isotropy errors in gradient fields.