

Dipole Verification Plots

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1115

Communication System: CW; Frequency: 750 MHz

Medium parameters used: $f = 750$ MHz; $\sigma = 0.924$ S/m; $\epsilon_r = 41.377$; $\rho = 1000$ kg/m³

Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(9.13, 9.13, 9.13); Calibrated: 2015/4/24;

Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$

Electronics: DAE4 Sn328; Calibrated: 2015/5/22

Phantom: SAM v5.0 TP:1799; Type: QD000P40CD; Serial: TP:1799

Measurement SW: DASY52, Version 52.8 (8)

Test date: 2015-11-18; Ambient Temp: 22.3; Tissue Temp: 23.2

750 MHz System Verification -Head-

Area Scan (5x14x1): Measurement grid: $dx=15$ mm, $dy=15$ mm

Maximum value of SAR (measured) = 2.57 W/kg


Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm

Reference Value = 54.11 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 3.06 W/kg

SAR(1 g) = 2.04 W/kg; SAR(10 g) = 1.34 W/kg

Maximum value of SAR (measured) = 2.59 W/kg

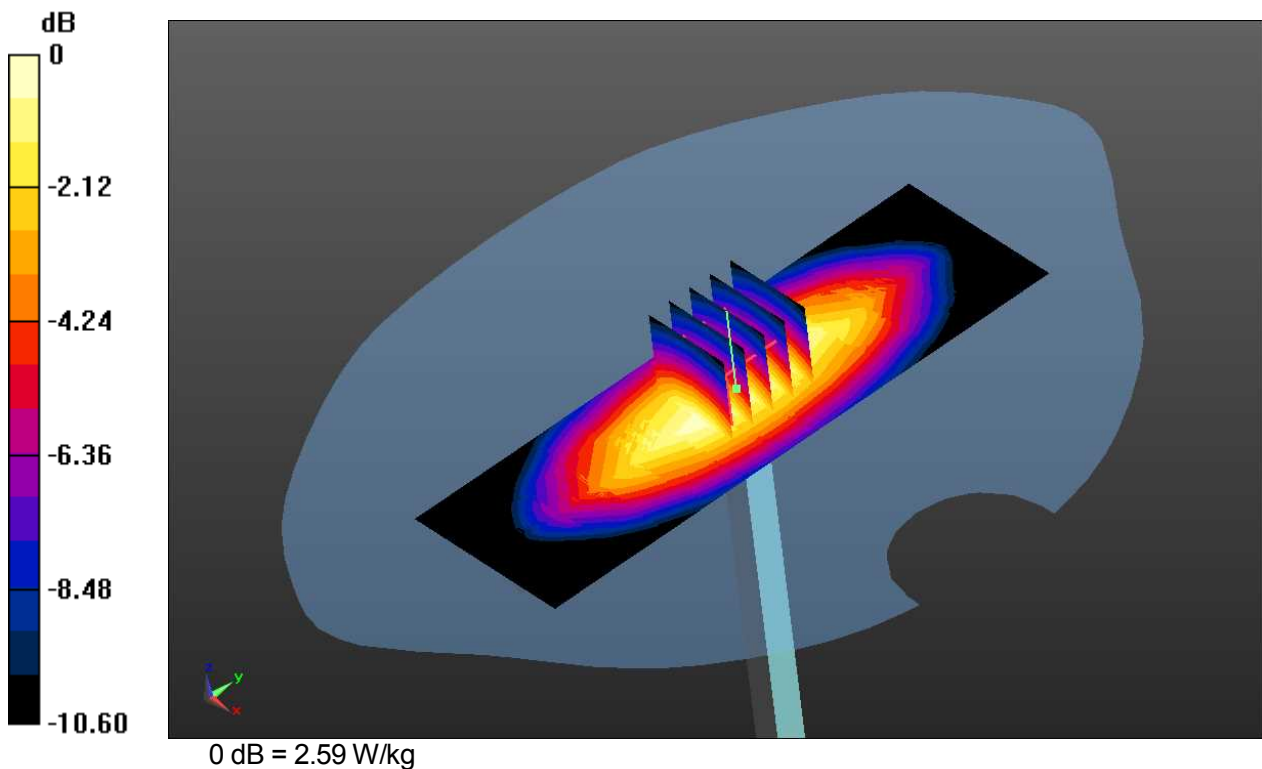

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1115

Communication System: CW; Frequency: 750 MHz
 Medium parameters used: $f = 750$ MHz; $\sigma = 0.924$ S/m; $\epsilon_r = 41.377$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(9.13, 9.13, 9.13); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: SAM v5.0 TP:1799; Type: QD000P40CD; Serial: TP:1799
 Measurement SW: DASY52, Version 52.8 (8)


Test date: 2015-11-18; Ambient Temp: 22.3; Tissue Temp: 23.2

750 MHz System Verification -Head-

Area Scan (5x14x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 2.57 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 54.11 V/m; Power Drift = 0.06 dB
 Peak SAR (extrapolated) = 3.06 W/kg

SAR(1 g) = 2.04 W/kg; SAR(10 g) = 1.34 W/kg
 Maximum value of SAR (measured) = 2.59 W/kg

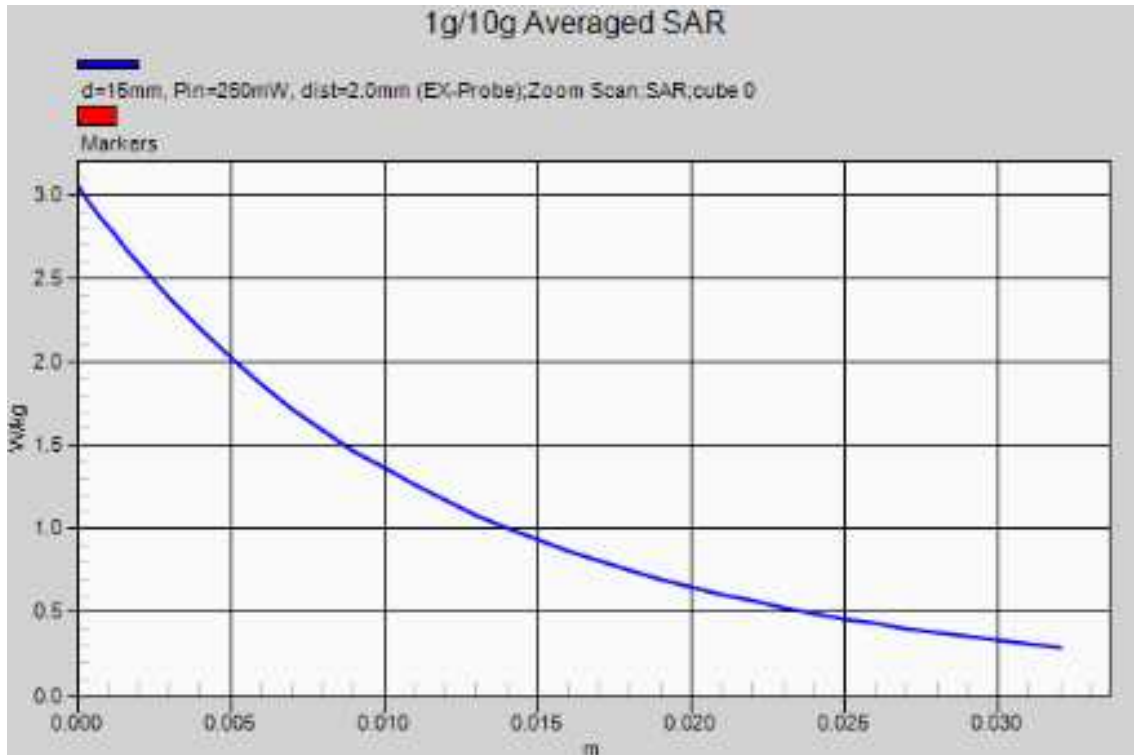

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1115

Communication System: CW; Frequency: 750 MHz
 Medium parameters used: $f = 750$ MHz; $\sigma = 0.983$ S/m; $\epsilon_r = 54.648$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(8.86, 8.86, 8.86); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: ELI v5.0 (20deg probe tilt) TP:1230; Type: QDOVA001BB; Serial: TP:1230
 Measurement SW: DASY52, Version 52.8 (8)


Test date: 2015-11-19; Ambient Temp: 22.4; Tissue Temp: 22.0

750 MHz System Verification -Body-

Area Scan (5x14x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 2.71 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 53.92 V/m; Power Drift = 0.05 dB
 Peak SAR (extrapolated) = 3.21 W/kg

SAR(1 g) = 2.18 W/kg; SAR(10 g) = 1.45 W/kg
 Maximum value of SAR (measured) = 2.74 W/kg

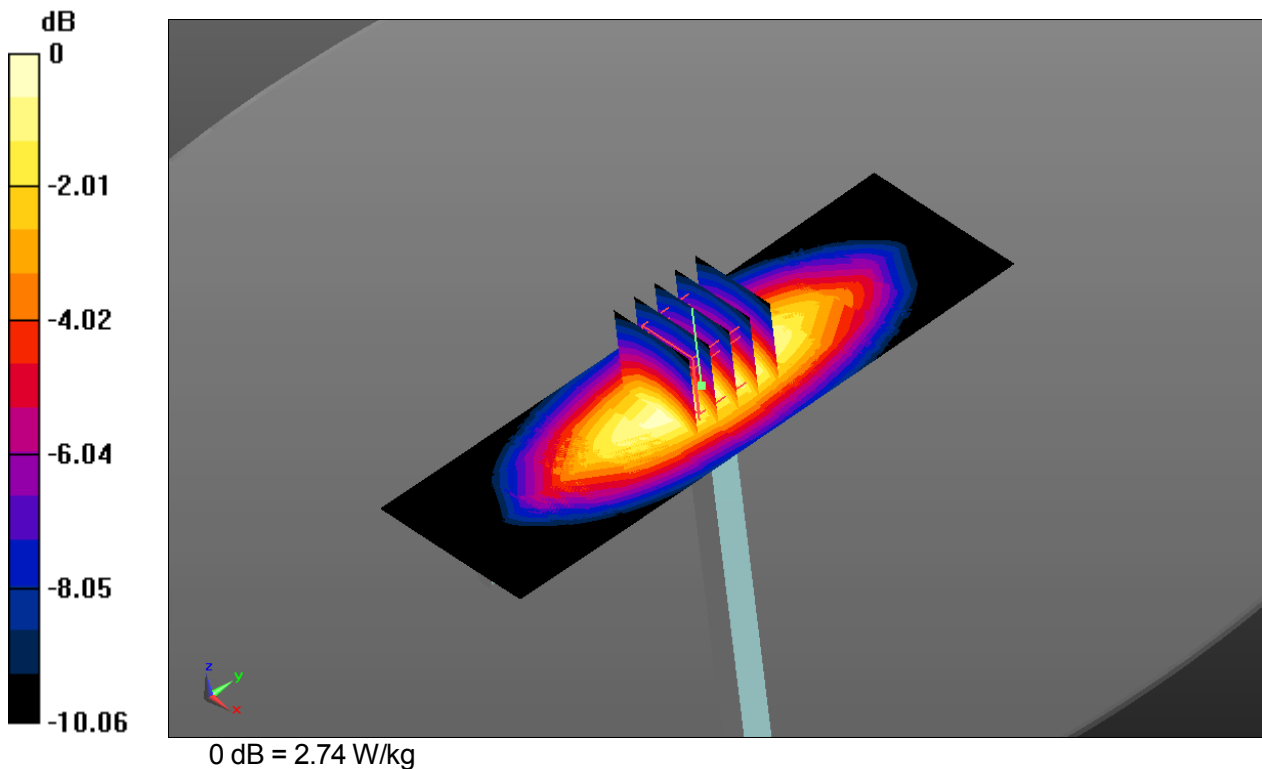

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1115

Communication System: CW; Frequency: 750 MHz
 Medium parameters used: $f = 750$ MHz; $\sigma = 0.983$ S/m; $\epsilon_r = 54.648$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(8.86, 8.86, 8.86); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: ELI v5.0 (20deg probe tilt) TP:1230; Type: QDOVA001BB; Serial: TP:1230
 Measurement SW: DASY52, Version 52.8 (8)


Test date: 2015-11-19; Ambient Temp: 22.4; Tissue Temp: 22.0

750 MHz System Verification -Body-

Area Scan (5x14x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 2.71 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 53.92 V/m; Power Drift = 0.05 dB
 Peak SAR (extrapolated) = 3.21 W/kg

SAR(1 g) = 2.18 W/kg; SAR(10 g) = 1.45 W/kg
 Maximum value of SAR (measured) = 2.74 W/kg

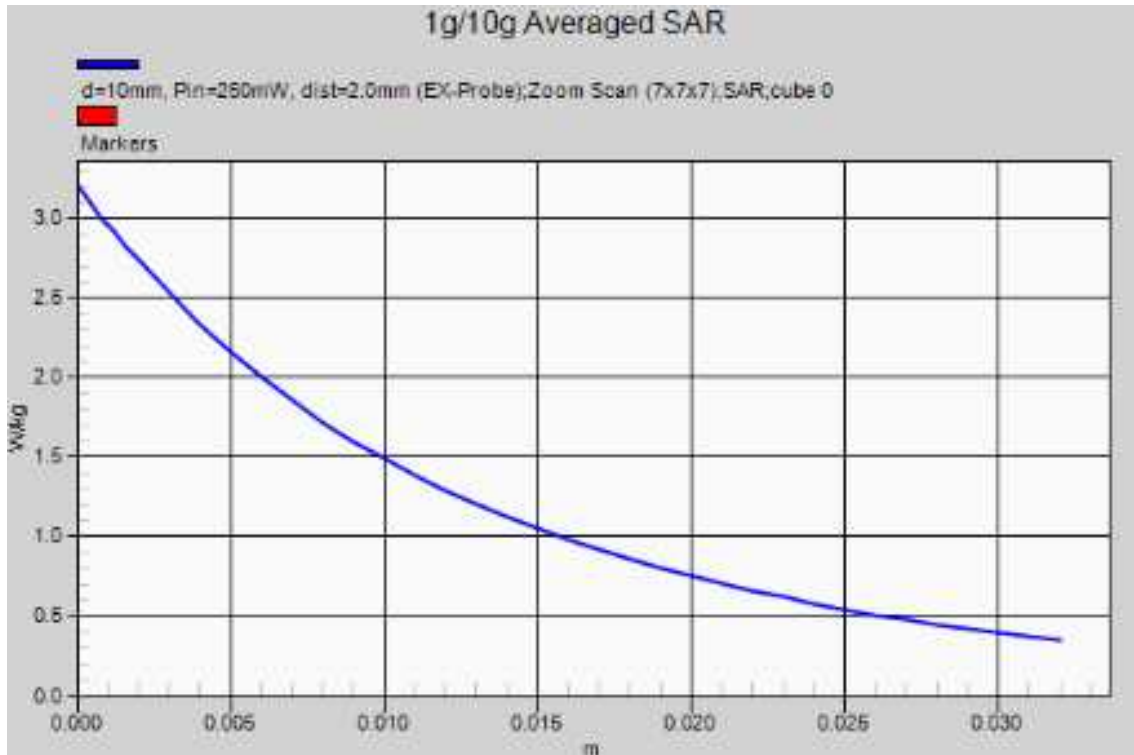

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d104

Communication System: CW; Frequency: 835 MHz
 Medium parameters used: $f = 835$ MHz; $\sigma = 0.908$ S/m; $\epsilon_r = 41.539$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(8.78, 8.78, 8.78); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: SAM v5.0 TP:1799; Type: QD000P40CD; Serial: TP:1799
 Measurement SW: DASY52, Version 52.8 (8)


Test date: 2015-11-16; Ambient Temp: 22.0; Tissue Temp: 22.9

835 MHz System Verification -Head-

Area Scan (5x13x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 2.84 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 57.06 V/m; Power Drift = -0.01 dB
 Peak SAR (extrapolated) = 3.32 W/kg

SAR(1 g) = 2.23 W/kg; SAR(10 g) = 1.46 W/kg
 Maximum value of SAR (measured) = 2.83 W/kg

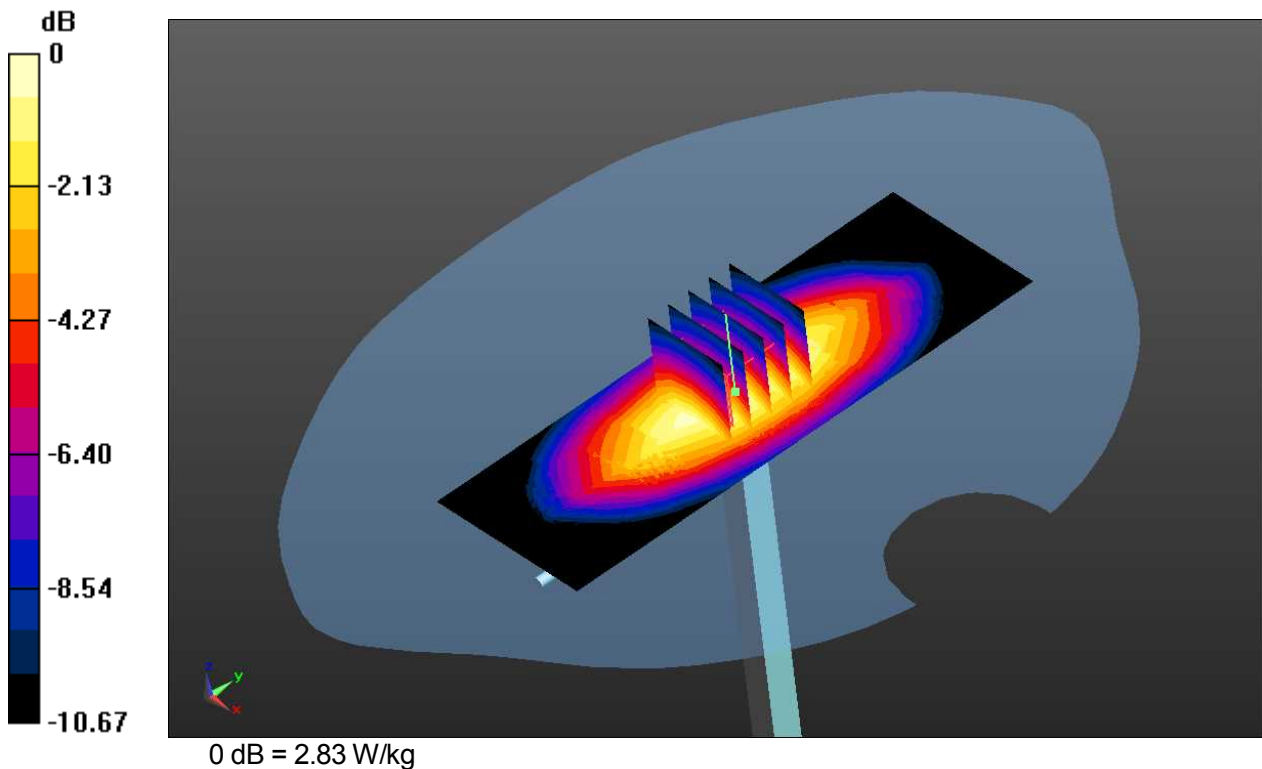

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d104

Communication System: CW; Frequency: 835 MHz
 Medium parameters used: $f = 835$ MHz; $\sigma = 0.908$ S/m; $\epsilon_r = 41.539$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(8.78, 8.78, 8.78); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: SAM v5.0 TP:1799; Type: QD000P40CD; Serial: TP:1799
 Measurement SW: DASY52, Version 52.8 (8)


Test date: 2015-11-16; Ambient Temp: 22.0; Tissue Temp: 22.9

835 MHz System Verification -Head-

Area Scan (5x13x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 2.84 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 57.06 V/m; Power Drift = -0.01 dB
 Peak SAR (extrapolated) = 3.32 W/kg

SAR(1 g) = 2.23 W/kg; SAR(10 g) = 1.46 W/kg
 Maximum value of SAR (measured) = 2.83 W/kg

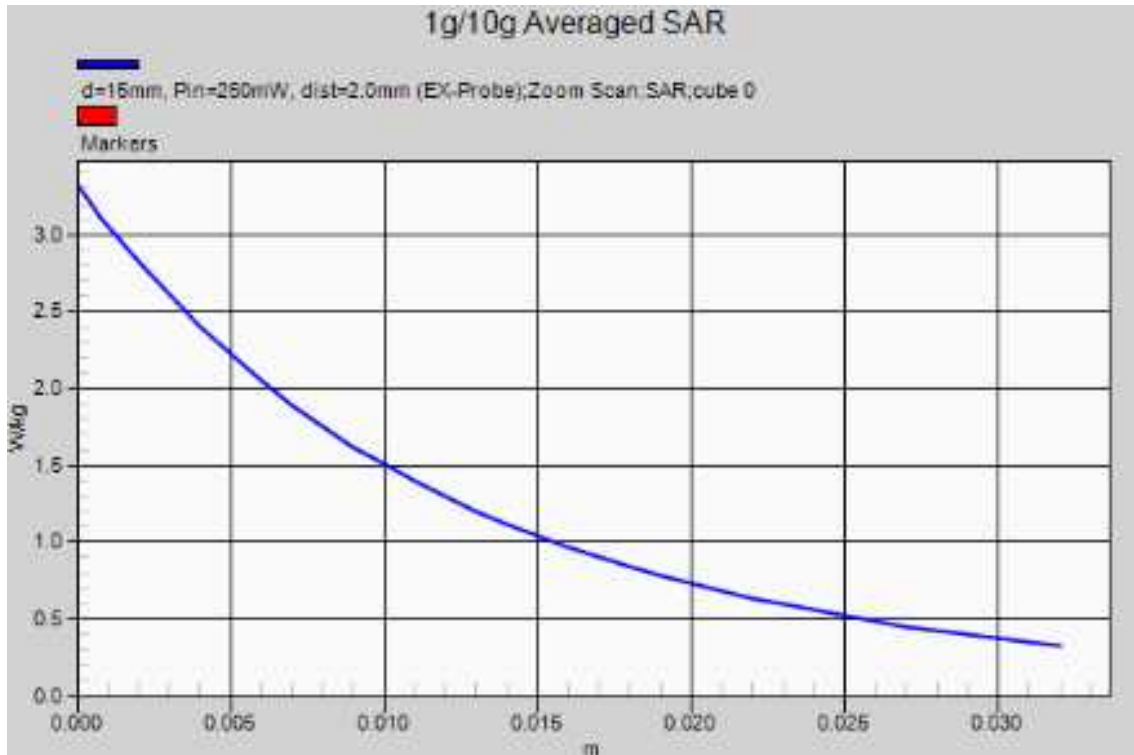

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d104

Communication System: CW; Frequency: 835 MHz
 Medium parameters used: $f = 835$ MHz; $\sigma = 1.008$ S/m; $\epsilon_r = 55.151$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(8.81, 8.81, 8.81); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: ELI v5.0 (20deg probe tilt) TP:1230; Type: QDOVA001BB; Serial: TP:1230
 Measurement SW: DASY52, Version 52.8 (8)


Test date: 2015-11-16; Ambient Temp: 22.9; Tissue Temp: 23.0

835 MHz System Verification -Body-

Area Scan (5x13x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 2.96 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 55.20 V/m; Power Drift = 0.02 dB
 Peak SAR (extrapolated) = 3.43 W/kg

SAR(1 g) = 2.32 W/kg; SAR(10 g) = 1.53 W/kg
 Maximum value of SAR (measured) = 2.94 W/kg

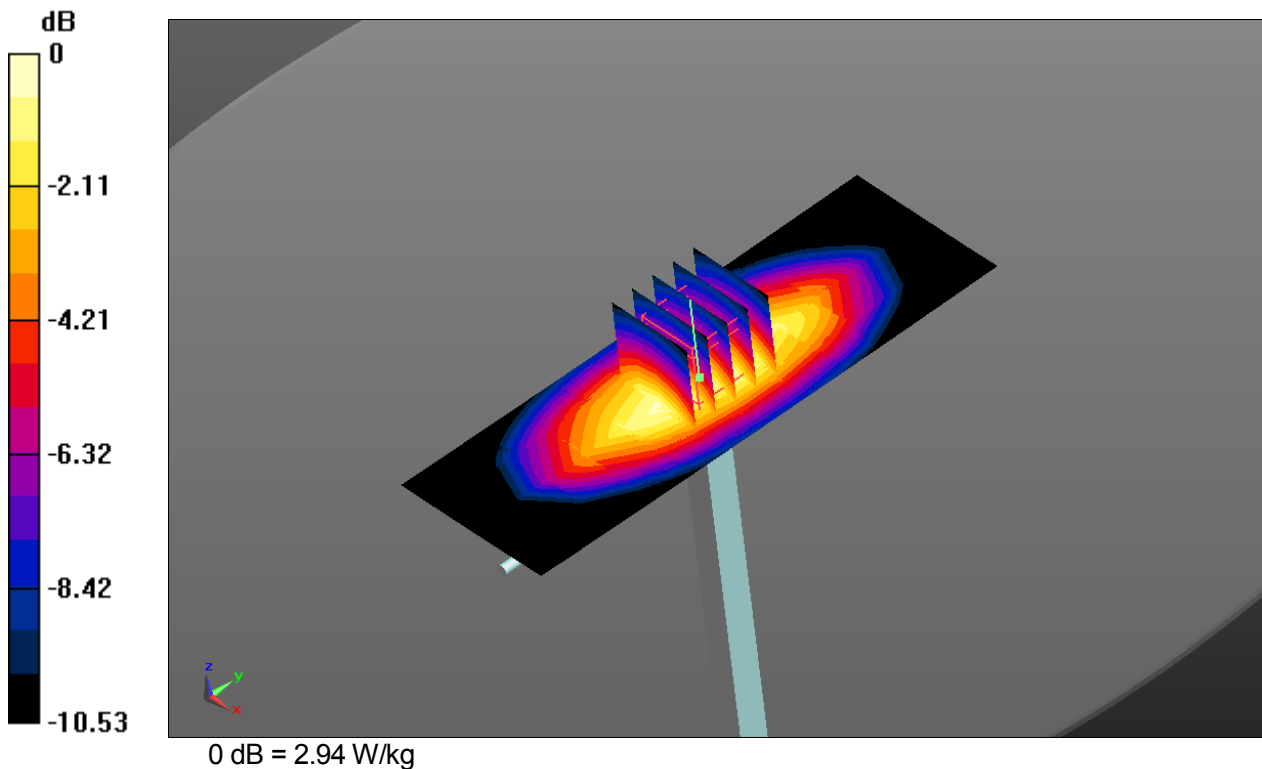

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d104

Communication System: CW; Frequency: 835 MHz
 Medium parameters used: $f = 835$ MHz; $\sigma = 1.008$ S/m; $\epsilon_r = 55.151$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(8.81, 8.81, 8.81); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: ELI v5.0 (20deg probe tilt) TP:1230; Type: QDOVA001BB; Serial: TP:1230
 Measurement SW: DASY52, Version 52.8 (8)


Test date: 2015-11-16; Ambient Temp: 22.9; Tissue Temp: 23.0

835 MHz System Verification -Body-

Area Scan (5x13x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 2.96 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 55.20 V/m; Power Drift = 0.02 dB
 Peak SAR (extrapolated) = 3.43 W/kg

SAR(1 g) = 2.32 W/kg; SAR(10 g) = 1.53 W/kg
 Maximum value of SAR (measured) = 2.94 W/kg

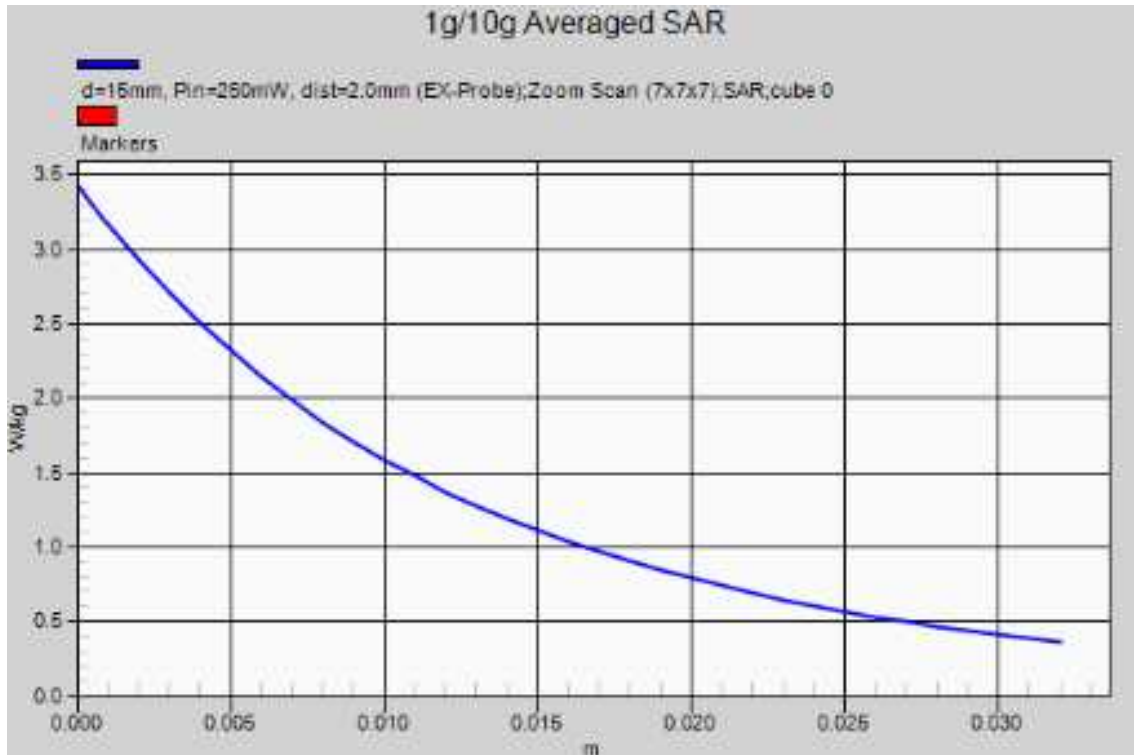

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d129

Communication System: CW; Frequency: 1900 MHz
 Medium parameters used: $f = 1900$ MHz; $\sigma = 1.423$ S/m; $\epsilon_r = 39.349$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(7.29, 7.29, 7.29); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: SAM v5.0 TP:1799; Type: QD000P40CD; Serial: TP:1799
 MEASUREMENT SW: DASY52, VERSION 52.8 (8);


Test date: 2015-11-17; Ambient Temp: 22.2; Tissue Temp: 23.4

1900 MHz System Verification -Head-

Area Scan (5x7x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 14.3 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 101.09 V/m; Power Drift = 0.06 dB
 Peak SAR (extrapolated) = 18.3 W/kg

SAR(1 g) = 9.96 W/kg; SAR(10 g) = 5.18 W/kg
 Maximum value of SAR (measured) = 14.2 W/kg

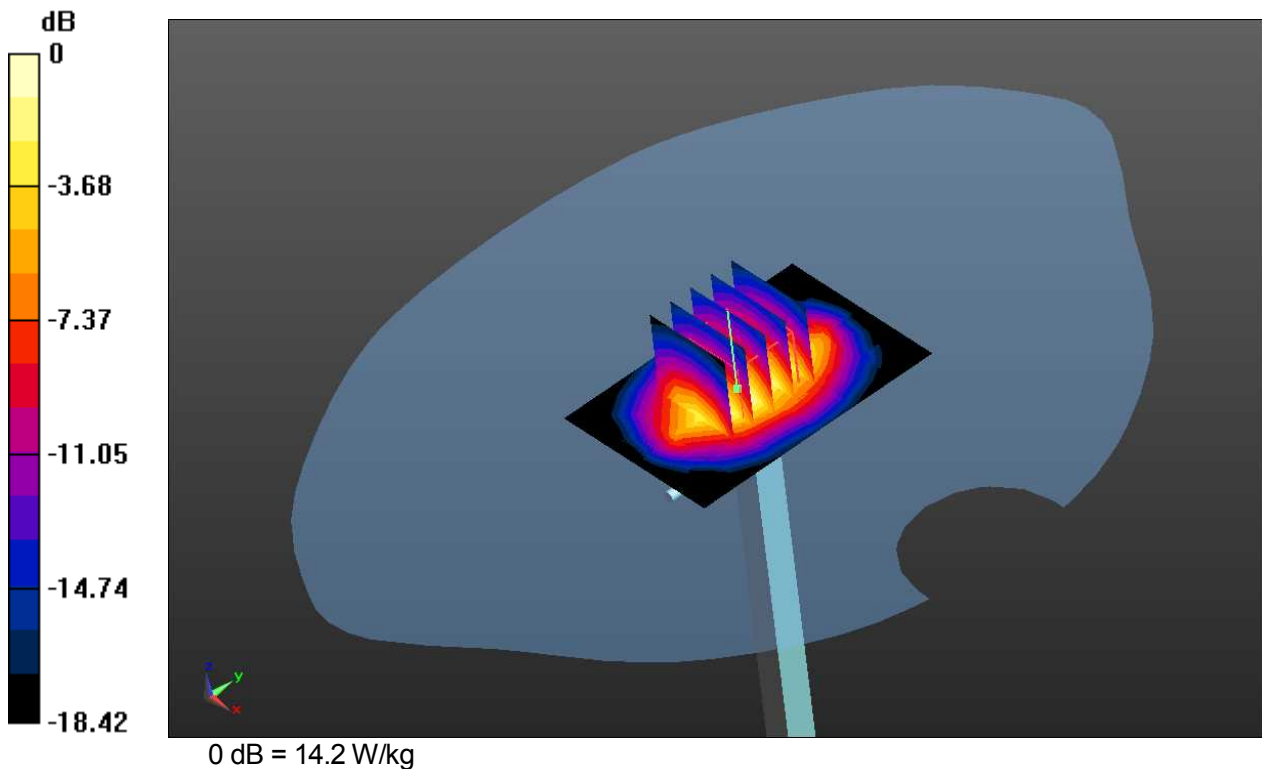

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d129

Communication System: CW; Frequency: 1900 MHz
 Medium parameters used: $f = 1900$ MHz; $\sigma = 1.423$ S/m; $\epsilon_r = 39.349$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(7.29, 7.29, 7.29); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: SAM v5.0 TP:1799; Type: QD000P40CD; Serial: TP:1799
 MEASUREMENT SW: DASY52, VERSION 52.8 (8);


Test date: 2015-11-17; Ambient Temp: 22.2; Tissue Temp: 23.4

1900 MHz System Verification -Head-

Area Scan (5x7x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 14.3 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 101.09 V/m; Power Drift = 0.06 dB
 Peak SAR (extrapolated) = 18.3 W/kg

SAR(1 g) = 9.96 W/kg; SAR(10 g) = 5.18 W/kg
 Maximum value of SAR (measured) = 14.2 W/kg

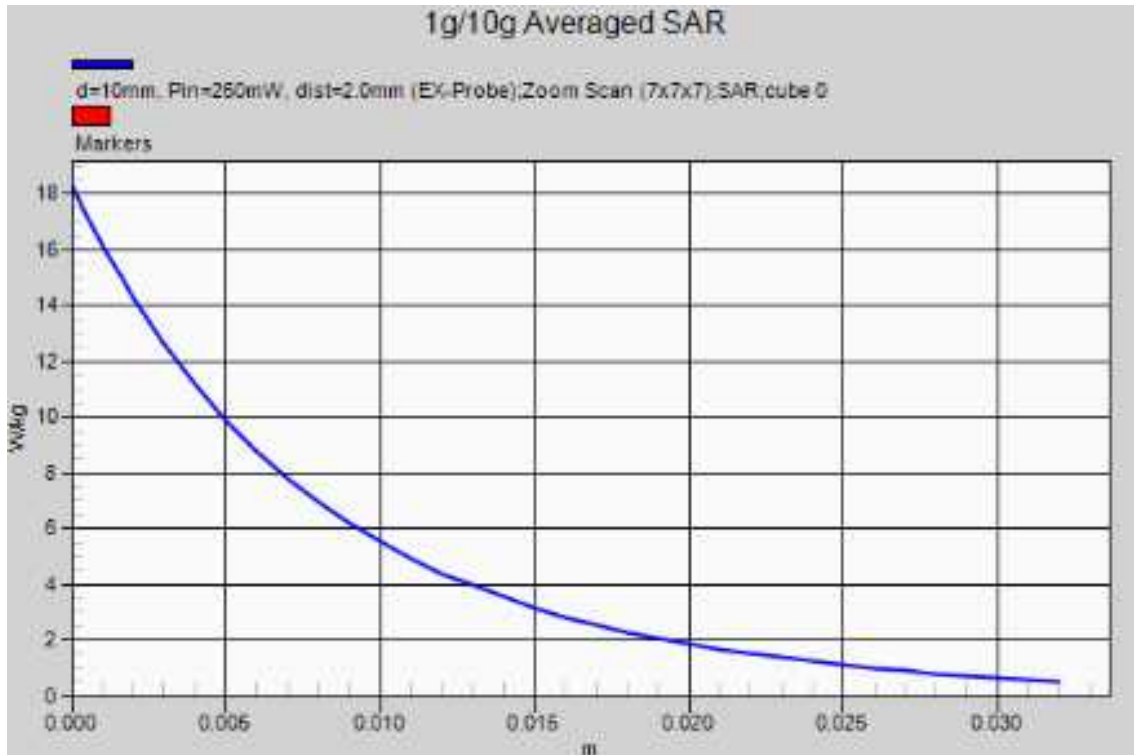

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d129

Communication System: CW; Frequency: 1900 MHz
 Medium parameters used: $f = 1900$ MHz; $\sigma = 1.555$ S/m; $\epsilon_r = 52.679$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(6.99, 6.99, 6.99); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: ELI v5.0 (20deg probe tilt) TP;1230; Type: QDOVA001BB; Serial: TP:1230
 MEASUREMENT SW: DASY52, VERSION 52.8 (8);


Test date: 2015-11-18; Ambient Temp: 23.1; Tissue Temp: 22.3

1900 MHz System Verification -Body-

Area Scan (5x7x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 13.6 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 95.18 V/m; Power Drift = 0.03 dB
 Peak SAR (extrapolated) = 17.1 W/kg

SAR(1 g) = 9.64 W/kg; SAR(10 g) = 5.08 W/kg
 Maximum value of SAR (measured) = 13.4 W/kg

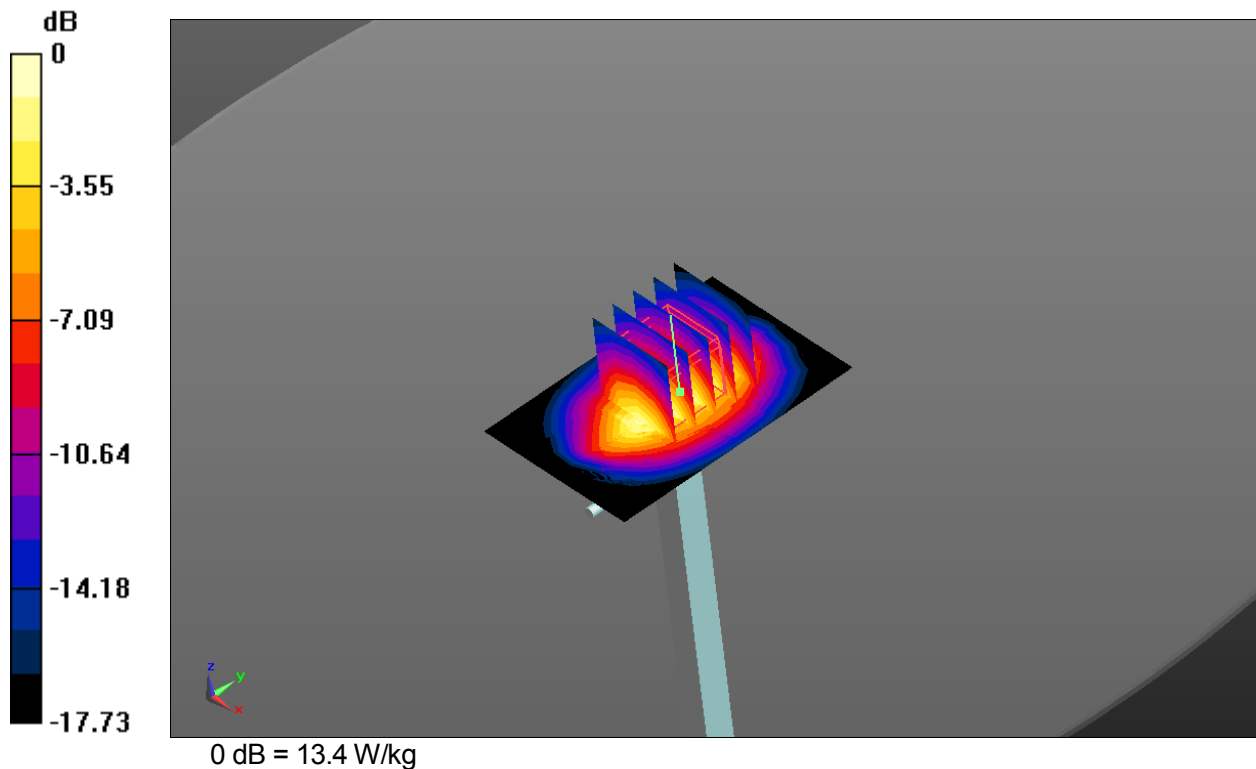

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d129

Communication System: CW; Frequency: 1900 MHz
 Medium parameters used: $f = 1900$ MHz; $\sigma = 1.555$ S/m; $\epsilon_r = 52.679$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(6.99, 6.99, 6.99); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: ELI v5.0 (20deg probe tilt) TP;1230; Type: QDOVA001BB; Serial: TP:1230
 MEASUREMENT SW: DASY52, VERSION 52.8 (8);


Test date: 2015-11-18; Ambient Temp: 23.1; Tissue Temp: 22.3

1900 MHz System Verification -Body-

Area Scan (5x7x1): Measurement grid: $dx=15$ mm, $dy=15$ mm
 Maximum value of SAR (measured) = 13.6 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8$ mm, $dy=8$ mm, $dz=5$ mm
 Reference Value = 95.18 V/m; Power Drift = 0.03 dB
 Peak SAR (extrapolated) = 17.1 W/kg

SAR(1 g) = 9.64 W/kg; SAR(10 g) = 5.08 W/kg
 Maximum value of SAR (measured) = 13.4 W/kg

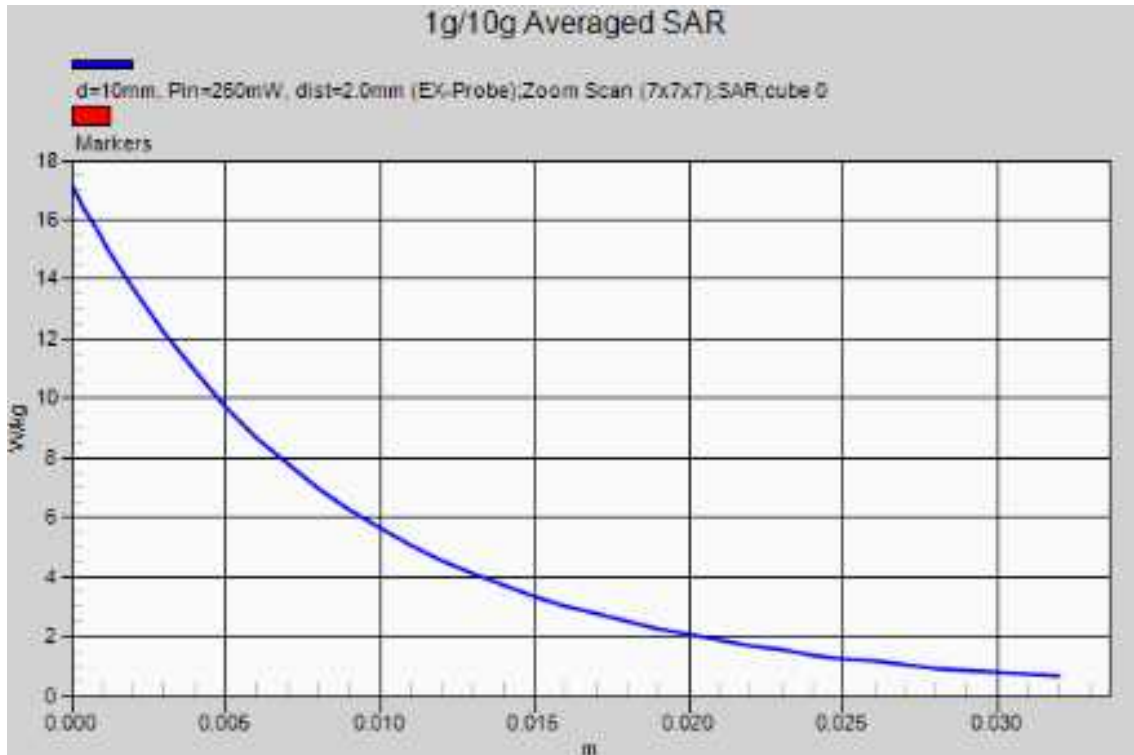

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 765

Communication System: CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.857$ S/m; $\epsilon_r = 40.118$; $\rho = 1000$ kg/m³

Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(6.64, 6.64, 6.64); Calibrated: 2015/4/24;

Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$

Electronics: DAE4 Sn328; Calibrated: 2015/5/22

Phantom: SAM v5.0 TP:1799; Type: QD000P40CD; Serial: TP:1799

MEASUREMENT SW: DASY52, VERSION 52.8 (8);

Test date: 2015-11-19; Ambient Temp: 21.9; Tissue Temp: 21.7

2450 MHz System Verification -Head-

Area Scan (7x10x1): Measurement grid: $dx=10$ mm, $dy=10$ mm

Maximum value of SAR (measured) = 20.2 W/kg


Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 106.0 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 27.9 W/kg

SAR(1 g) = 13 W/kg; SAR(10 g) = 5.93 W/kg

Maximum value of SAR (measured) = 20.1 W/kg

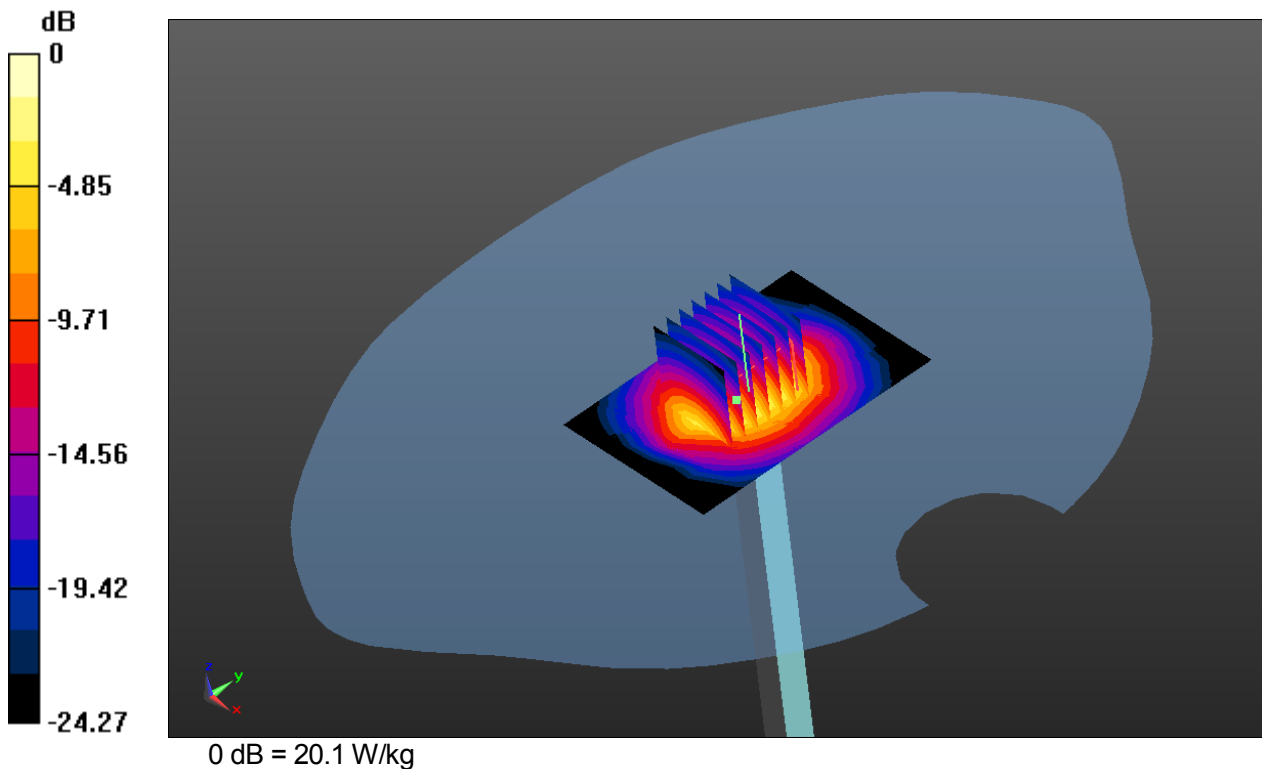

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 765

Communication System: CW; Frequency: 2450 MHz
 Medium parameters used: $f = 2450$ MHz; $\sigma = 1.857$ S/m; $\epsilon_r = 40.118$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(6.64, 6.64, 6.64); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: SAM v5.0 TP:1799; Type: QD000P40CD; Serial: TP:1799
 MEASUREMENT SW: DASY52, VERSION 52.8 (8);


Test date: 2015-11-19; Ambient Temp: 21.9; Tissue Temp: 21.7

2450 MHz System Verification -Head-

Area Scan (7x10x1): Measurement grid: $dx=10$ mm, $dy=10$ mm
 Maximum value of SAR (measured) = 20.2 W/kg

Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm
 Reference Value = 106.0 V/m; Power Drift = 0.01 dB
 Peak SAR (extrapolated) = 27.9 W/kg

SAR(1 g) = 13 W/kg; SAR(10 g) = 5.93 W/kg
 Maximum value of SAR (measured) = 20.1 W/kg

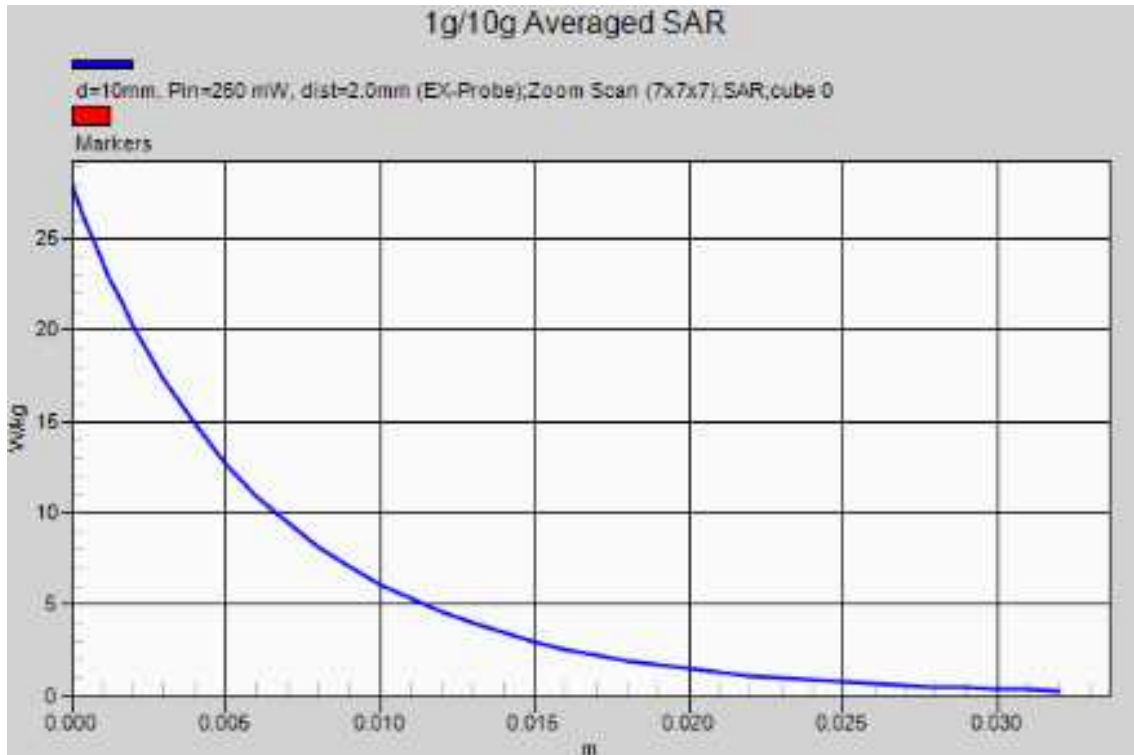

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 765

Communication System: CW; Frequency: 2450 MHz
 Medium parameters used: $f = 2450$ MHz; $\sigma = 2.012$ S/m; $\epsilon_r = 51.375$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(6.73, 6.73, 6.73); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: ELI v5.0 (20deg probe tilt) TP;1230; Type: QDOVA001BB; Serial: TP:1230
 MEASUREMENT SW: DASY52, VERSION 52.8 (8);


Test date: 2015-11-19; Ambient Temp: 23.0; Tissue Temp: 22.4

2450 MHz System Verification -Body-

Area Scan (7x10x1): Measurement grid: $dx=10$ mm, $dy=10$ mm
 Maximum value of SAR (measured) = 18.8 W/kg

Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm
 Reference Value = 100.8 V/m; Power Drift = -0.06 dB
 Peak SAR (extrapolated) = 25.9 W/kg

SAR(1 g) = 12.6 W/kg; SAR(10 g) = 5.89 W/kg
 Maximum value of SAR (measured) = 19.3 W/kg

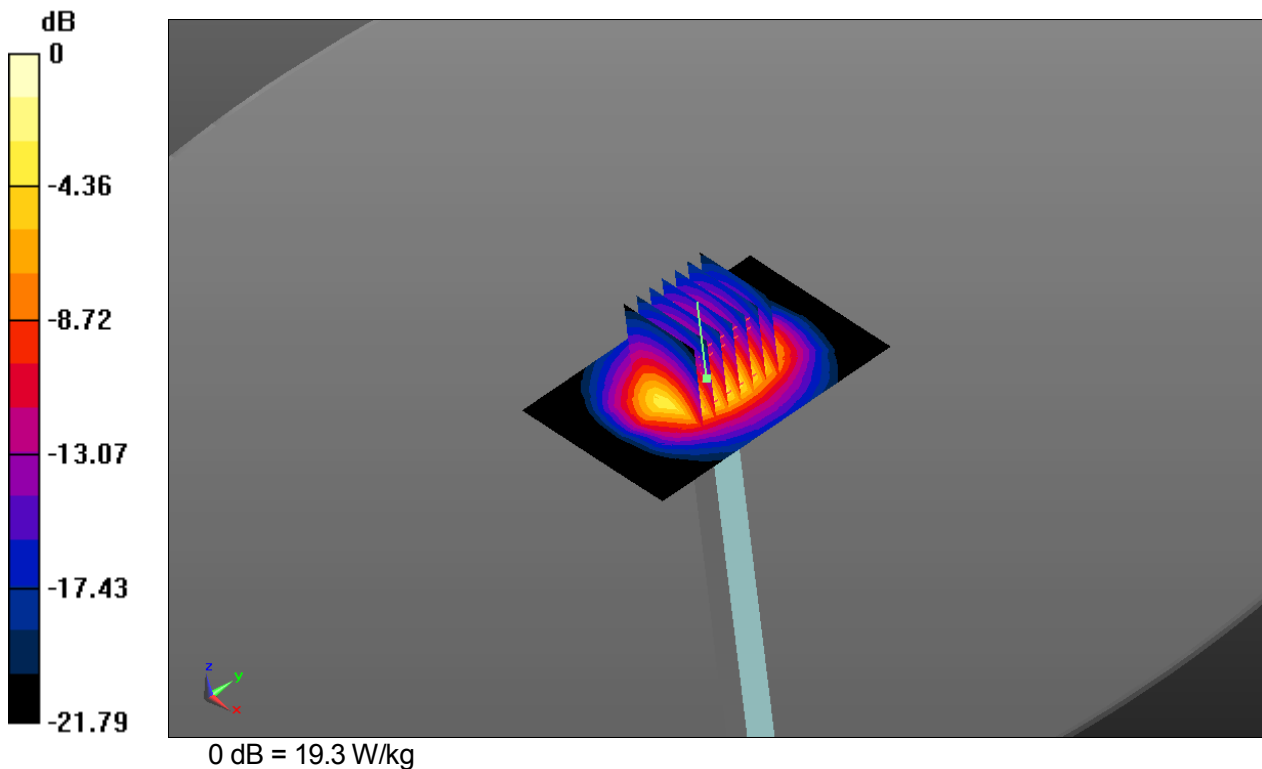

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 765

Communication System: CW; Frequency: 2450 MHz
 Medium parameters used: $f = 2450$ MHz; $\sigma = 2.012$ S/m; $\epsilon_r = 51.375$; $\rho = 1000$ kg/m³
 Phantom section: Flat section

DASY Configuration

Probe: EX3DV4 - SN3745; ConvF(6.73, 6.73, 6.73); Calibrated: 2015/4/24;
 Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
 Electronics: DAE4 Sn328; Calibrated: 2015/5/22
 Phantom: ELI v5.0 (20deg probe tilt) TP;1230; Type: QDOVA001BB; Serial: TP:1230
 MEASUREMENT SW: DASY52, VERSION 52.8 (8);

Test date: 2015-11-19; Ambient Temp: 23.0; Tissue Temp: 22.4

2450 MHz System Verification -Body-

Area Scan (7x10x1): Measurement grid: $dx=10$ mm, $dy=10$ mm
 Maximum value of SAR (measured) = 18.8 W/kg

Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm
 Reference Value = 100.8 V/m; Power Drift = -0.06 dB
 Peak SAR (extrapolated) = 25.9 W/kg

SAR(1 g) = 12.6 W/kg; SAR(10 g) = 5.89 W/kg
 Maximum value of SAR (measured) = 19.3 W/kg

