



Specific Absorption Rate (SAR) Test Report

for

Trimble Navigation Ltd.

on the

PDA

Report Number	: FA8O0405A
Trade Name	: Trimble
Model Name	: Juno SC
FCC ID	: JUP66400
Date of Testing	: Oct. 07, 2008
Date of Report	: Nov. 11, 2008
Date of Review	: Nov. 11, 2008

- The test results refer exclusively to the tested model/sample only.
- Without written approval of SPORTON INTERNATIONAL INC., the test report shall not be reproduced except in full.
- Report Version: Rev. 02

SPORTON INTERNATIONAL INC.

No. 52, Hwa Ya 1st Rd., Hwa Ya Technology Park, Kwei-Shan Hsiang, Tao Yuan Hsien, Taiwan, R.O.C.





Table of Contents

1.		nent of Compliance	
2.	Admiı	nistration Data	
	2.1	Testing Laboratory	
	2.2	Applicant	
	2.3	Manufacturer	
	2.4	Application Details	
3.	Gener	al Information	5
	3.1	Description of Device Under Test (DUT)	5
	3.2	Basic Description of Accessories	
	3.3	Product Photos	6
	3.4	Applied Standards	6
	3.5	Device Category and SAR Limits	6
	3.6	Test Conditions	7
		3.6.1 Ambient Condition	7
		3.6.2 Test Configuration	
		3.6.3 FCC 3G SAR Measurement Procedures	
4.	Speci	fic Absorption Rate (SAR)	
	4.1	Introduction	
	4.2	SAR Definition	
5.	SAR N	Neasurement Setup	
	5.1	DASY4 E-Field Probe System	
	-	5.1.1 ET3DV6 E-Field Probe Specification	
		5.1.2 ET3DV6 E-Field Probe Calibration	
	5.2	DATA Acquisition Electronics (DAE)	
	5.3	Robot	
	5.4	Measurement Server	
	5.5	SAM Twin Phantom	
	5.6	Device Holder for SAM Twin Phantom	
	5.7	Data Storage and Evaluation	
		5.7.1 Data Storage	
		5.7.2 Data Evaluation	
	5.8	Test Equipment List	
6.	Tissu	e Simulating Liquids	
7.		tainty Assessment	
8.		Measurement Evaluation	
0.	8.1	Purpose of System Performance check	23 25
	8.2	System Setup	
	8.3	Validation Results	
0		iption for DUT Testing Position	
9.			
10.		urement Procedures	
	10.1	Spatial Peak SAR Evaluation	
	10.2	Scan Procedures	
		SAR Averaged Methods	
11.		Fest Results	
	11.1	Conducted Power	
	11.2	Test Records for Body SAR Test	
		ences	
		A - System Performance Check Data	
Арр	oendix	B - SAR Measurement Data	
App	pendix	C - Calibration Data	

Appendix D - Product Photos

Appendix E - Test Setup Photos



1. <u>Statement of Compliance</u>

The Specific Absorption Rate (SAR) maximum results found during testing for the Trimble Navigation Ltd. PDA Trimble Juno SC are as follows (with expanded uncertainty 21.9%):

SAR Position	GSM850 SAR (W/kg)	GSM1900 SAR (W/Kg)	WCDMA Band V SAR (W/kg)	WCDMA Band II SAR (W/kg)
Body	0.354	0.246	0.346	0.452

They are in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1999 and had been tested in accordance with the measurement methods and procedures specified in IEEE P1528-2003, and OET Bulletin 65 Supplement C (Edition 01-01).

Approved by

ey Nu Rov Wu

Manager



2. Administration Data

2.1 Testing Laboratory

Company Name :	Sporton International Inc.
Address :	No.52, Hwa-Ya 1 st RD., Hwa Ya Technology Park, Kwei-Shan Hsiang,
	TaoYuan Hsien, Taiwan, R.O.C.
Test Site :	SAR01-HY
Telephone Number :	886-3-327-3456
Fax Number :	886-3-328-4978

2.2 Applicant

Company Name :	Trimble Navigation Ltd.
Address :	935 Stewart Drive, Sunnyvale CA 94088-3642, U.S.A.

2.3 Manufacturer

Company Name :	GOLDTEK Technology Co., Ltd.
Address :	3F., No.3, Ln. 768, Sec. 4, Pateh Rd., Taipei 115, Taiwan, R.O.C.

2.4 Application Details

Date of reception of application:	Oct. 04, 2008
Start of test :	Oct. 07, 2008
End of test :	Oct. 07, 2008



3. General Information

3.1 Description of Device Under Test (DUT)

Product Feature & Specification				
DUT Type :	PDA			
Trade Name :	Trimble			
Model Name :	Juno SC			
FCC ID :	JUP66400			
Tx Frequency :	GSM850 : 824 MHz ~ 849 MHz GSM1900 : 1850 MHz ~1910 MHz WCDMA Band V : 824 MHz ~ 849 MHz WCDMA Band II : 1850 MHz ~ 1910 MHz			
Rx Frequency :	GSM850 : 869 MHz ~ 894 MHz GSM1900 : 1930 MHz ~ 1990 MHz WCDMA Band V : 869 MHz ~ 894 MHz WCDMA Band II : 1930 MHz ~ 1990 MHz			
Maximum Output Power to Antenna :	GSM850 : 31.73 dBm GSM1900 : 28.89 dBm WCDMA Band V : 22.20 dBm WCDMA Band II : 22.69 dBm			
Antenna Type :	Fixed Internal			
HW Version :	1.0			
SW Version :	1.0			
Type of Modulation :	GSM / GPRS : GMSK EDGE : 8PSK WCDMA : QPSK HSDPA : QPSK / 16QAM			
DUT Stage :	Identical Prototype			



3.2	Basic	Description	of Accessories

	Brand Name	Trimble			
AC Adapter	Model Name	3A-161WP05			
	Power Rating	I/P: 100-240Vac, 50-60Hz, 0.6A; O/P: 5Vdc, 2.6A			
	AC Power Cord Type	1.24 meter non-shielded cable with ferrite core			
	Model Name	BA-1405206			
Battery	Power Rating	3.7Vdc, 2600mAh			
	Туре	Li-ion			
USB Cable	Signal Line Type	1.2 meter shielded cable with ferrite core			
LCD Panel	Brand Name	Торру			
LCD Patiel	Model Name	td035sted7			

Remark: Above DUT's information was declared by manufacturer. Please refer to the specifications of manufacturer or User's Manual for more detailed features description.

3.3 Product Photos

Refer to Appendix D.

3.4 <u>Applied Standards</u>

The Specific Absorption Rate (SAR) testing specification, method and procedure for this PDA is in accordance with the following standards:

47 CFR Part 2 (2.1093), IEEE C95.1-1999, IEEE C95.3-2002, IEEE P1528-2003, and OET Bulletin 65 Supplement C (Edition 01-01) KDB 648474 D01 v01r05 KDB 941225 D01 v02

3.5 Device Category and SAR Limits

This device belongs to portable device category because its radiating structure is allowed to be used within 20 centimeters of the body of the user. Limit for General Population/Uncontrolled exposure should be applied for this device, it is 1.6 W/kg as averaged over any 1 gram of tissue.



3.6 Test Conditions

3.6.1 Ambient Condition

Indicht Conulion	
Ambient Temperature	20-24 °C
Humidity	<60%

3.6.2 Test Configuration

The device was controlled by using a base station emulator R&S CMU200. Communication between the device and the emulator was established by air link. The distance between the DUT and the antenna of the emulator is larger than 50 cm and the output power radiated from the emulator antenna is at least 30 dB smaller than the output power of DUT. The DUT was set from the emulator to radiate maximum output power during all tests.

Measurements were performed on the lowest, middle, and highest channel for each testing position. However, measurements were performed only on the middle channel if the SAR is below 3 dB of limit.

For WWAN SAR testing, DUT is in GPRS/EDGE or WCDMA/HSDPA link mode. In GPRS/EDGE link mode, its crest factor is 4, because DUT is GPRS/EDGE class 10 device. In WCDMA/HSDPA link mode, its crest factor is 1.




3.6.3 FCC 3G SAR Measurement Procedures

The DUT was tested according to the requirements of the FCC 3G procedures and the TS 34.121. The DUT's WCDMA and HSDPA function is Release 5 version supporting HSDPA Category 8.

WCDMA Setup Configuration:

- a. The DUT was connected to Base Station referred to the drawing of Setup Configuration.
- b. The RF path losses were compensated into the measurements.
- c. A call was established between DUT and Base Station with following setting
 - i. Data rates: Varied from RMC 12.2Kbps to 384Kbps for each measurement.
 - ii. RMC Test Loop=Loop Mode 1 RLC TM
 - iii. TPC with All Up.
- d. The transmitted maximum output power was recorded.








Mu	ax.Level: A ultiple Sign cr. Code: 0]:	uto al: DPCCH+I / Off	Low noise DPDCH 1	SR1 CC1			Chan./Fi	req.: 4132Slot	CDP/Co Rho Mar
1.0 5 0.8		701	Ų.		7.011	ų.		7011	Appli-
0.6									cation
0.4 0.2 0.0								i 1 	Trigger Ana. Let
0	DPCCH	DPDCH1	DPDCH2	DPDCH3	DPDCH4	DPDCH5	DPDCH6	HS-DPCCH	UE Signa
Curr.	0.221	0.778						cal	Ana.Se
Avg.	0.221	0.778						N/A	BS Signa
Мах.	0.222	0.779							Level
Min.	0.221	0.777							BS Signa
				1		40	_		Settings
	ectMagn I		2.6 %		Stati	10 stic Count		0 Slot Numbe	
I/Q C	origin Offse	et 🛛 🗕	45.97 dB			0.00 %	-	23.36 dBm	Marker

Single DPCCH with only one DPDCH at RMC 12.2Kbps (Symbol Rate 60 Kbps)

Ch. 1 Ch. 2 WCDMA FDE) ^{Band} Co	de Domair		1 - C	Connect Control
WCDMA FDD Connection C	ontrol 📱	PS:	Attached	CS: Co	onnected
-Setup			— TPC Settings/Set	1/Pattern Type	
TPC Step Size Activate Pattern TPC Pattern Setup Test Step Preconditions •Set1 Pattern Type Pattern	5	1 dB Execute Set 1 Manual All 1 11 bin			<u>o</u>
 Set 2 Set 3 Set 4 Set 5 Test Step A Test Step B Test Step C 					
Connection Handover UE Sig	nal BS Sigr	nal Networ	k AF/RF ⊕+	Sync.	1 2

TPC with All " 1" (Continuous transmitting)



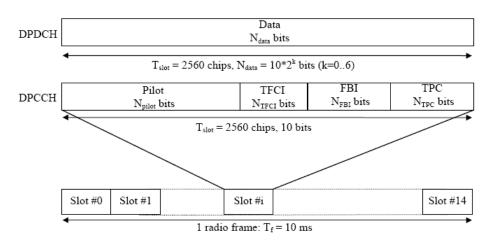

Frame structure for uplink DPDCH/DPCCH

The parameter K in the figure determines the number of bits per uplink DPDCH slot. It is related to the spreading factor SF of the DPDCH as $SF = 256/2^k$. The DPDCH spreading factor may range from 256 down to 4. The spreading factor of the uplink DPCCH is always equal to 256, i.e. there are 10 bits per uplink DPCCH slot.

	Channel Bit Rate (kbps)	Channel Symbol Rate (ksps)	Spreading Factor	Spreading Code Number	Bits/Slot
DPCCH	15	15	256	0	10
	15	15	256	64	10
	30	30	128	32	20
	60	60	64	16	40
DPDCH1	120	120	32	8	80
	240	240	16	4	160
	480	480	8	2	320
	960	960	4	1	640
DPDCHn	960	960	4	1, 2, 3	640

Table 2 DPCCH and DPDCH

There is only one DPCCH per radio link. Data rates, channelization codes and spread factor information for DPCCH and DPDCH_n are indicated in the following Table. Spreading Rate (SF) * Symbol Rate = 3.84 Mcps.



HSDPA Setup Configuration:

- a. The DUT was connected to Base Station referred to the drawing of Setup Configuration.
- b. The RF path losses were compensated into the measurements.
- c. A call was established between DUT and Base Station with following setting:
 - i. Set RMC12.2Kbps with HSDPA mode.
 - ii. RMC Test Loop=Loop Mode 1 RLC TM
 - iii. TPC with All Up
 - iv. Channel Configuration Type=FRC with H-set 1 (QPSK)
 - v. CQI Feedback Cycle=4ms, CQI Repetition Factor=2
 - vi. RV Coding Sequence {0.2.5.6}
 - vii. Gain Factors(β c,and β d) and parameters were set according to each specific sub-test in the following table, C10.1.4, quoted from the TS 34.121.

Table C.10.1.4: β values for transmitter characteristics tests with HS-DPCCH

d. The transmitted maximum output power was recorded.

Sub-test	βα	βd	β _d (SF)	β₀/βd	βHs (Note1, Note 2)	CM (dB) (Note 3)	MPR (dB) (Note 3)
1	2/15	15/15	64	2/15	4/15	0.0	0.0
2	12/15	15/15	64	12/15	24/15	1.0	0.0
	(Note 4)	(Note 4)		(Note 4)			
3	15/15	8/15	64	15/8	30/15	1.5	0.5
4	15/15	4/15	64	15/4	30/15	1.5	0.5
Note 2:	For the HS-I Magnitude (I discontinuity with β_{hs} = 2	DPCCH pow EVM) with H in clause 5. 4/15 * β_c .	er mask requ S-DPCCH te 13.1AA, Δ _{ACF}	$_{\rm s}$ = 30/15 * β_c . irement test in cla st in clause 5.13.1 $_{\rm A}$ and $\Delta_{\rm NACK}$ = 30/1	A, and HSDF 5 with β_{hs} =	PA EVM with pha 30/15 * β_c , and	ase I ∆ _{CQI} = 24/15
Note 3:		MPR is base	ed on the rela	. For all other com tive CM difference r releases.			
Note 4:				for the TFC during a factors for the ref			

Connect WCDMA FDD Band **Receiver Quality** Control WCDMA FDD Connection Control 📄 PS: Established CS: Registered Packet Switched/HSDPA Test Mode/ -Setup ▶ Node-B Settings Circuit Switched Packet Switched Default Settings \checkmark DCH (Dedicated Chn.) Type HSDPA Test Mode ►HSDPA Test Mode Radiobearer Setup RMC 12.2 kbps + HSDPA RMC Test Loop Loop Mode 1 RLC TM ▶ HSDPA HS-DSCH Downlink Physical Channels TPC Settinas Compressed Mode Settings DL Power Control Settings AF/RF ⊕+ Handover UE Signal BS Signal Network Sync. 1 2 Connection

RMC 12.2Kbps with HSDPA function



4. Specific Absorption Rate (SAR)

4.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

4.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density. ρ). The equation description is as below:

$$\mathbf{SAR} = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$\mathbf{SAR} = C \, \frac{\delta T}{\delta t}$$

, where C is the specific head capacity, δT is the temperature rise and δt the exposure duration,

or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\sigma \left| E \right|^2}{\rho}$$

, where σ is the conductivity of the tissue, ρ is the mass density of the tissue and E is the rms electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.



5. SAR Measurement Setup

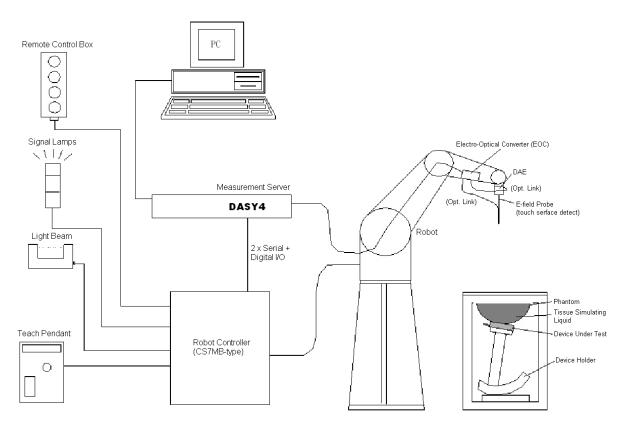


Fig. 5.1 DASY4 System

The DASY4 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- A dosimetric probe equipped with an optical surface detector system
- The electro-optical converter (ECO) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the accuracy of the probe positioning
- A computer operating Windows XP
- DASY4 software
- Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- The SAM twin phantom
- A device holder
- Tissue simulating liquid
- > Dipole for evaluating the proper functioning of the system

Some of the components are described in details in the following sub-sections.



5.1 DASY4 E-Field Probe System

The SAR measurement is conducted with the dosimetric probe ET3DV6 (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency. This probe has a built in optical surface detection system to prevent from collision with phantom.

5.1.1 ET3DV6 E-Field Probe Specification

<ei3dv6></ei3dv6>		
Construction	Symmetrical design with triangular core Built-in optical fiber for surface detection system Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents)	
Frequency	10 MHz to 3 GHz	
Directivity	\pm 0.2 dB in brain tissue (rotation around probe axis) \pm 0.4 dB in brain tissue (rotation perpendicular to probe axis)	
Dynamic Range	5μ W/g to 100mW/g; Linearity: ±0.2dB	
Surface Detection	\pm 0.2 mm repeatability in air and clear liquids on reflecting surface	
Dimensions	Overall length: 330mm Tip length: 16mm Body diameter: 12mm Tip diameter: 6.8mm Distance from probe tip to dipole centers: 2.7mm	Fig. 5.2 Probe Setup on Robot
Application	General dosimetry up to 3GHz Compliance tests for mobile phones and Wireless LAN Fast automatic scanning in arbitrary phantoms	

5.1.2 ET3DV6 E-Field Probe Calibration

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy shall be evaluated and within \pm 0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data are as below:

Sensitivity	X axis : 1.6	X axis : 1.63 μV		is : 1.67 μV	Z axis : 2.18 μV
Diode compression point	X axis : 90) mV	Y az	kis : 93 mV	Z axis : 92 mV
Conversion factor	Frequency (MHz)	X a	xis	Y axis	Z axis
(Head / Body)	800~1000	6.06 /	5.91	6.06 / 5.91	6.06 / 5.91
	1850~2050	5.01 /	4.49	5.01 / 4.49	5.01 / 4.49
Boundary effect	Frequency (MHz)	Alp	oha	Depth	
(Head / Body)	800~1000	0.30 /	0.31	2.80 / 2.98	
	1850~2050	0.59/	0.68	1.96 / 1.95	

NOTE: The probe parameters have been calibrated by the SPEAG.

This report shall not be reproduced except in full, without the written approval of Sporton.



5.2 DATA Acquisition Electronics (DAE)

The data acquisition electronics (DAE3) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE3 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.

5.3 <u>Robot</u>

The DASY4 system uses the high precision robots RX90BL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY4 system, the CS7MB robot controller version from Stäubli is used. The RX robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- ➢ 6-axis controller

5.4 <u>Measurement Server</u>

The DASY4 measurement server is based on a PC/104 CPU board with 166 MHz CPU 32 MB chipset and 64 MB RAM.

Communication with the DAE3 electronic box the 16-bit AD-converter system for optical detection and digital I/O interface.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.



5.5 <u>SAM Twin Phantom</u>

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- ➢ Left head
- ➢ Right head
- ➢ Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

The phantom can be used with the following tissue simulating liquids:

- *Water-sugar based liquid
- *Glycol based liquids



Fig. 5.3 Top View of Twin Phantom



Fig. 5.4 Bottom View of Twin Phantom



5.6 Device Holder for SAM Twin Phantom

The SAR in the Phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source in 5 mm distance, a positioning uncertainty of ± 0.5 mm would produce a SAR uncertainty of $\pm 20\%$. An accurate device position is therefore crucial for accurate and repeatable measurement. The position in which the devices must be measured, are defined by the standards.

The DASY4 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The DASY4 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $\varepsilon_r = 3$ and loss tangent $\delta = 0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



Fig. 5.5 Device Holder



5.7 Data Storage and Evaluation

5.7.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The post-processing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [A/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a non-less media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

5.7.2 Data Evaluation

The DASY4 post-processing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software :

Probe parameters :	- Sensitivity	Norm _{<i>i</i>} , a_{i0} , a_{i1} , a_{i2}
	- Conversion factor	ConvF _i
	- Diode compression point	dcp <i>i</i>
Device parameters :	- Frequency	f
	- Crest factor	cf
Media parameters :	- Conductivity	σ
	- Density	ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY4 components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power.



The formula for each channel can be given as :

$$Vi = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with V_i = compensated signal of channel i (i = x, y, z) U_i = input signal of channel i (i = x, y, z) cf = crest factor of exciting field (DASY parameter) dcp_i = diode compression point (DASY parameter)

From the compensated input signals, the primary field data for each channel can be evaluated :

E-field probes : $E_i = \sqrt{\frac{V_i}{Norm_iConvF}}$ H-field probes : $H_i = \sqrt{V_i} \frac{a_{i0+}a_{i1}f + a_{i2}f^2}{f}$ with V_i = compensated signal of channel i (i = x, y, z) $Norm_i$ = sensor sensitivity of channel i (i = x, y, z) $\mu V/(V/m)2$ for E-field Probes ConvF = sensitivity enhancement in solution a_{ij} = sensor sensitivity factors for H-field probes f = carrier frequency [GHz] E_i = electric field strength of channel i in V/m H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude) :

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with

SAR = local specific absorption rate in mW/g

Etot = total field strength in V/m

 σ = conductivity in [mho/m] or [Siemens/m]

 ρ = equivalent tissue density in g/cm³

* Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or $P_{pwe} = H_{tot}^2 \cdot 37.7$

with P_{pwe} = equivalent power density of a plane wave in mW/cm² E_{tot} = total electric field strength in V/m H_{tot} = total magnetic field strength in A/m



5.8 <u>Test Equipment List</u>

Manufacturer	Nome of Fauinment	Type/Model	Serial Number	Calibration		
Manufacturer	Name of Equipment	Type/Model	Serial Number	Last Cal.	Due Date	
SPEAG	Dosimetric E-Filed Probe	ET3DV6	1787	Aug. 26, 2008	Aug. 25, 2009	
SPEAG	835MHz System Validation Kit	D835V2	499	Mar. 17, 2008	Mar. 16, 2010	
SPEAG	1900MHz System Validation Kit	D1900V2	5d041	Mar. 28, 2008	Mar. 27, 2010	
SPEAG	Data Acquisition Electronics	DAE3	577	Nov. 16, 2007	Nov. 15, 2008	
SPEAG	Device Holder	N/A	N/A	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1477	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1383	NCR	NCR	
Agilent	PNA Series Network Analyzer	E8358A	US40260131	Apr. 02, 2008	Apr. 01, 2009	
Agilent	Wireless Communication Test Set	E5515C	GB46311322	Dec. 22, 2006	Dec. 21, 2008	
R&S	Universal Radio Communication Tester	CMU200	114256	Dec. 11, 2007	Dec. 10, 2008	
Agilent	Dielectric Probe Kit	85070D	US01440205	NCR	NCR	
Agilent	Dual Directional Coupler	778D	50422	NCR	NCR	
AR	Power Amplifier	5S1G4M2	0328767	NCR	NCR	
R&S	Power Meter	NRVD	101394	Oct. 31, 2007	Oct. 30, 2008	
R&S	Power Sensor	NRV-Z1	100130	Oct. 31, 2007	Oct. 30, 2008	

Table 5.1 Test Equipment List



6. <u>Tissue Simulating Liquids</u>

For the measurement of the field distribution inside the SAM phantom with DASY4, the phantom must be filled with around 25 liters of homogeneous tissue simulating liquid. The liquid height from the ear reference point (ERP) of the phantom to the liquid top surface is (head SAR)or from the flat phantom to the liquid top surface (body SAR) is 15.2cm.

The following ingredients for tissue simulating liquid are used:

- ▶ Water: deionized water (pure H₂0), resistivity $\geq 16M \Omega$ as basis for the liquid
- Sugar: refined sugar in crystals, as available in food shops to reduce relative permittivity
- Salt: pure NaCl to increase conductivity
- Cellulose: Hydroxyethyl-cellulose, medium viscosity (75-125 mPa.s, 2% in water, 20°C), CAS#54290-to increase viscosity and to keep sugar in solution.
- Preservative: Preventol D-7 Bayer AG, D-51368 Leverkusen, CAS#55965-84-9- to prevent the spread of bacteria and molds.
- DGMBE: Deithlenglycol-monobuthyl ether (DGMBE), Fluka Chemie GmbH, CAS#112-34-5 – to reduce relative permittivity.

Table 6.1 gives the recipes for one liter of body tissue simulating liquid for frequency band 850MHz and 1900 MHz.

Ingredient	MSL-850	MSL-1900
Water	631.68 g	716.56 g
Cellulose	0 g	0 g
Salt	11.72 g	4.0 g
Preventol D-7	1.2 g	0 g
Sugar	600.0 g	0 g
DGMBE	0 g	300.67 g
Total amount	1 liter (1.3 kg)	1 liter (1.0 kg)
Dielectric Parameters at 22°	f=835 MHz	f= 1900 MHz
	$\varepsilon_{\rm f} = 55.2 \pm 5\%,$	$\varepsilon_{\rm r} = 53.3 \pm 5 \%$,
	σ=0.97±5% S/m	σ= 1.52±5% S/m

Table 6.1 Recipes for Tissue Simulating Liquid

The dielectric parameters of the liquids were verified prior to the SAR evaluation using an Agilent 85070D Dielectric Probe Kit and an Agilent Network Analyzer.



Band	Temperature (°C)	Frequency (MHz)	Conductivity (σ)	Permittivity (ɛ _r)	Measurement Date
		824.2	0.960	56.3	
GSM850	21.5	836.4	0.972	56.3	Oct. 07, 2008
		848.8	0.981	56.1	
		1850.2	1.47	51.2	
GSM1900	21.6	1880.0	1.50	51.1	Oct. 07, 2008
		1909.8	1.53	51.0	
	21.5	826.4	0.962	56.3	
WCDMA Band V		836.4	0.972	56.3	Oct. 07, 2008
		846.6	0.980	56.2	
WCDMA Band II	21.6	1852.4	1.47	51.2	
		1880.0	1.50	51.1	Oct. 07, 2008
		1907.6	1.53	51.0	

Table 6.2 shows the measuring results for muscle simulating liquid.

Table 6.2 Measuring Results for Simulating Liquid

The measuring data are consistent with $\epsilon_r = 55.2 \pm 5\%$ and $\sigma = 0.97 \pm 5\%$ for body GSM850 and WCDMA Band V, and $\epsilon_r = 53.3 \pm 5\%$ and $\sigma = 1.52 \pm 5\%$ for body GSM1900 and WCDMA Band II.



7. <u>Uncertainty Assessment</u>

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table 7.1

Uncertainty Distributions	Normal	Rectangular	Triangular	U-shape
Multiplying factor ^(a)	$_{1/k}(b)$	1/√3	1/√6	1/√2

(a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity

(b) \mathcal{K} is the coverage factor

Table 7.1 Multiplying Factions for Various Distributions

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY4 uncertainty Budget is showed in Table 7.2.



Error Description	Uncertainty Value ± %	Probability Distribution	Divisor	Ci (1g)	Standard Unc. (1g)	vi or Veff
Measurement Equipment						
Probe Calibration	±5.9 %	Normal	1	1	±5.9 %	∞
Axial Isotropy	±4.7 %	Rectangular	$\sqrt{3}$	0.7	±1.9 %	∞
Hemispherical Isotropy	±9.6 %	Rectangular	$\sqrt{3}$	0.7	±3.9 %	∞
Boundary Effects	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Linearity	±4.7 %	Rectangular	$\sqrt{3}$	1	±2.7 %	∞
System Detection Limits	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Readout Electronics	±0.3 %	Normal	1	1	±0.3 %	∞
Response Time	± 0.8 %	Rectangular	$\sqrt{3}$	1	±0.5 %	∞
Integration Time	±2.6 %	Rectangular	$\sqrt{3}$	1	±1.5 %	∞
RF Ambient Noise	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
RF Ambient Reflections	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
Probe Positioner	±0.4 %	Rectangular	$\sqrt{3}$	1	±0.2 %	∞
Probe Positioning	±2.9 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
Max. SAR Eval.	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Test Sample Related						
Device Positioning	±2.9 %	Normal	1	1	±2.9	145
Device Holder	±3.6 %	Normal	1	1	±3.6	5
Power Drift	±5.0 %	Rectangular	$\sqrt{3}$	1	±2.9	∞
Phantom and Setup						
Phantom Uncertainty	±4.0 %	Rectangular	$\sqrt{3}$	1	±2.3	∞
Liquid Conductivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.64	± 1.8	∞
Liquid Conductivity (meas.)	±2.5 %	Normal	1	0.64	±1.6	∞
Liquid Permittivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.6	±1.7	x
Liquid Permittivity (meas.)	±2.5 %	Normal	1	0.6	±1.5	x
Combined Standard Uncertainty					±10.9	387
Coverage Factor for 95 %		K=2				
Expanded uncertainty (Coverage factor = 2)					±21.9	

Table 7.2 Uncertainty Budget of DASY4



8. SAR Measurement Evaluation

Each DASY4 system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY4 software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

8.1 <u>Purpose of System Performance check</u>

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

8.2 System Setup

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave which comes from a signal generator at frequency 835 MHz and 1900 MHz. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

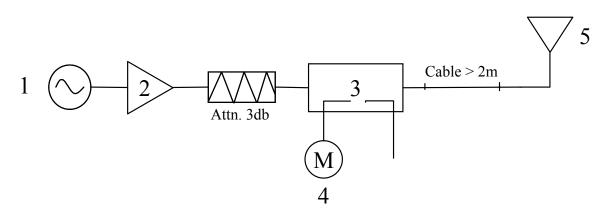


Fig. 8.1 System Setup for System Evaluation



- 1. Signal Generator
- 2. Amplifier
- 3. Directional Coupler
- 4. Power Meter
- 5. 835 MHz or 1900 MHz Dipole

The output power on dipole port must be calibrated to 20dBm (100mW) before dipole is connected.



Fig 8.2 Dipole Setup



8.3 Validation Results

Comparing to the original SAR value provided by SPEAG, the validation data should be within its specification of 10 %. Table 8.1 shows the target SAR and measured SAR after normalized to 1W input power.

Frequency	SAR	Target (W/kg)	Measurement data (W/kg)	Variation	Measurement Date
835MHz	SAR (1g)	9.52	9.80	2.9 %	Oct. 07, 2008
833MITZ	SAR (10g)	6.37	6.49	1.9 %	001.07,2008
1900MHz	SAR (1g)	40.1	40.9	2.0 %	Oct. 07, 2008
T900MHZ	SAR (10g)	21.3	21.5	0.9 %	001.07,2008

Table 8.1 Target and Measurement Data Comparison

The table above indicates the system performance check can meet the variation criterion.



9. Description for DUT Testing Position

This DUT was tested in two different positions. They are body worn with face and body worn with bottom as illustrated below:

- 1) "Body Worn"
 - i) To position the device parallel to the phantom surface.
 - ii) To adjust the phone parallel to the flat phantom.
 - iii) To adjust the distance between the DUT surface and the flat phantom to 1.5 cm.

Remark: Please refer to Appendix E for the test setup photos.



10. Measurement Procedures

The measurement procedures are as follows:

- Linking DUT with base station emulator CMU200 in middle channel
- Setting CMU200 to allow DUT to radiate maximum output power
- Measuring output power through RF cable and power meter
- Placing the DUT in the positions described in the last section
- Setting scan area, grid size and other setting on the DASY4 software
- > Taking data for the middle channel on each testing position
- Finding out the largest SAR result on these testing positions of each band
- Measuring output power and SAR results for the low and high channels in this worst case testing position

According to the IEEE P1528 draft standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- Power reference measurement
- Area scan
- Zoom scan
- Power reference measurement

10.1 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1528-2003 standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY4 software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

Base on the Draft: SCC-34, SC-2, WG-2-Computational Dosimetry, IEEE P1528/D1.2 (Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques), a new algorithm has been implemented. The spatial-peak SAR can be computed over any required mass.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.



The entire evaluation of the spatial peak values is performed within the post-processing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- extraction of the measured data (grid and values) from the Zoom Scan
- calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- generation of a high-resolution mesh within the measured volume
- interpolation of all measured values form the measurement grid to the high-resolution grid
- extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- calculation of the averaged SAR within masses of 1g and 10g

10.2 <u>Scan Procedures</u>

First Area Scan is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an Area Scan is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, Zoom Scan is required. The Zoom Scan measures 5x5x7 points with step size 8, 8 and 5 mm. The Zoom Scan is performed around the highest E-field value to determine the averaged SAR-distribution over 1 g.

10.3 <u>SAR Averaged Methods</u>

In DASY4, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.





11. SAR Test Results

11.1 Conducted Power

Band Mada Channel	GSM 850 (dBm)			GSM 1900 (dBm)			
Mode	128	189	251	512	661	810	
GPRS 8	31.44	31.61	31.73	28.87	28.89	28.59	
GPRS 10	29.87	30.06	30.19	27.28	27.31	27.06	
EGPRS 8	26.51	26.66	26.77	25.74	25.68	25.42	
EGPRS 10	24.52	24.64	24.75	23.65	23.64	23.42	

	Band	W	CDMA Band (dBm)	V	WCDMA Band II (dBm)			
Mode		4132	4182	4233	9262	9400	9538	
12.2k	K	21.92	21.96	21.93	22.10	22.50	22.19	
12.2K+HSDPA	β (2/15)	22.02	21.99	22.04	22.28	22.68	22.30	
	$\beta(12/15)$	22.14	22.20	22.13	22.30	22.69	22.34	
	β (15/8)	20.68	20.75	20.98	21.01	21.44	21.13	
	β (15/4)	19.63	19.54	19.77	19.93	20.38	20.09	



11.2 Test Records for Body SAR Test

Position	Band	Chan.	Freq. (MHz)	Modulation Type	Measured 1g SAR (W/kg)	Limit (W/kg)	Result
Face with 1.5cm Gap	GSM850 (GPRS10)	189	836.4	GMSK	0.228	1.6	Pass
Bottom with 1.5cm Gap	GSM850 (GPRS10)	189	836.4	GMSK	0.290	1.6	Pass
Bottom with 1.5cm Gap	GSM850 (EDGE10)	189	836.4	8PSK	0.085	1.6	Pass
Bottom with 1.5cm Gap	GSM850 (EDGE8)	189	836.4	8PSK	0.068	1.6	Pass
Bottom with 1.5cm Gap	GSM850 (GPRS10)	128	824.2	GMSK	0.282	1.6	Pass
Bottom with 1.5cm Gap	GSM850 (GPRS10)	251	848.8	GMSK	0.354	1.6	Pass
Face with 1.5cm Gap	GSM1900 (GPRS10)	661	1880.0	GMSK	0.132	1.6	Pass
Bottom with 1.5cm Gap	GSM1900 (GPRS10)	661	1880.0	GMSK	0.246	1.6	Pass
Bottom with 1.5cm Gap	GSM1900 (EDGE10)	661	1880.0	8PSK	0.108	1.6	Pass
Bottom with 1.5cm Gap	GSM1900 (EDGE8)	661	1880.0	8PSK	0.086	1.6	Pass
Bottom with 1.5cm Gap	GSM1900 (GPRS10)	512	1850.2	GMSK	0.236	1.6	Pass
Bottom with 1.5cm Gap	GSM1900 (GPRS10)	810	1909.8	GMSK	0.212	1.6	Pass
Face with 1.5cm Gap	WCDMA Band V (RMC12.2K)	4182	836.4	QPSK	0.195	1.6	Pass
Bottom with 1.5cm Gap	WCDMA Band V (RMC12.2K)	4182	836.4	QPSK	0.345	1.6	Pass
Bottom with 1.5cm Gap	WCDMA Band V (HSDPA)	4182	836.4	QPSK	0.277	1.6	Pass
Bottom with 1.5cm Gap	WCDMA Band V (RMC12.2K)	4132	826.4	QPSK	0.260	1.6	Pass
Bottom with 1.5cm Gap	WCDMA Band V (RMC12.2K)	4233	846.6	QPSK	0.346	1.6	Pass
Face with 1.5cm Gap	WCDMA Band II (RMC12.2K)	9400	1880.0	QPSK	0.216	1.6	Pass
Bottom with 1.5cm Gap	WCDMA Band II (RMC12.2K)	9400	1880.0	QPSK	0.452	1.6	Pass
Bottom with 1.5cm Gap	WCDMA Band II (HSDPA)	9400	1880.0	QPSK	0.447	1.6	Pass
Bottom with 1.5cm Gap	WCDMA Band II (RMC12.2K)	9262	1852.4	QPSK	0.376	1.6	Pass
Bottom with 1.5cm Gap	WCDMA Band II (RMC12.2K)	9538	1907.6	QPSK	0.435	1.6	Pass

Remark: Test Engineer : Eric Huang, Jason Wang, Robert Liu, and A-Rod Chen



12.<u>References</u>

- [1] FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2] IEEE Std. P1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", April 21, 2003
- [3] Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 97-01), "Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to RF Emissions", June 2001
- [4] IEEE Std. C95.3-2002, "IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields-RF and Microwave", 2002
- [5] IEEE Std. C95.1-1999, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", 1999
- [6] Robert J. Renka, "Multivariate Interpolation Of Large Sets Of Scattered Data", University of North Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988, pp. 139-148
- [7] DASY4 System Handbook



Appendix A - System Performance Check Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/10/7

System Check_Body_835MHz_20081007

DUT: Dipole 835 MHz


Communication System: CW; Frequency: 835 MHz;Duty Cycle: 1:1 Medium: MSL_850 Medium parameters used: f = 835 MHz; σ = 0.971 mho/m; ϵ_r = 56.3; ρ = 1000 kg/m³ Ambient Temperature : 22.4 °C; Liquid Temperature : 21.5 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Pin=100mW/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.07 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 34.5 V/m; Power Drift = -0.024 dB Peak SAR (extrapolated) = 1.38 W/kg SAR(1 g) = 0.980 mW/g; SAR(10 g) = 0.649 mW/g Maximum value of SAR (measured) = 1.06 mW/g

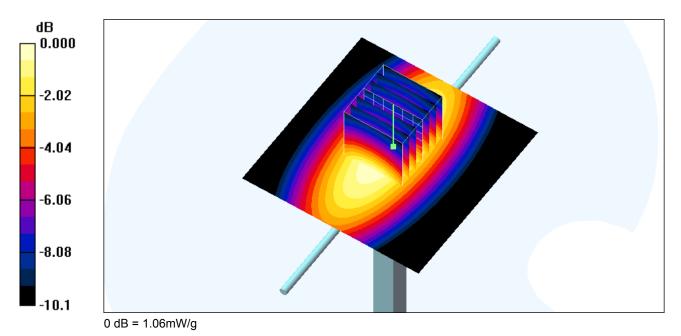



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/10/7

System Check_Body_1900MHz_20081007

DUT: Dipole 1900 MHz


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: MSL_1900 Medium parameters used: f = 1900 MHz; σ = 1.52 mho/m; ϵ_r = 51; ρ = 1000 kg/m³ Ambient Temperature : 22.6 °C; Liquid Temperature : 21.6 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 4.66 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 57.6 V/m; Power Drift = -0.011 dB Peak SAR (extrapolated) = 7.48 W/kg SAR(1 g) = 4.09 mW/g; SAR(10 g) = 2.15 mW/g Maximum value of SAR (measured) = 4.61 mW/g

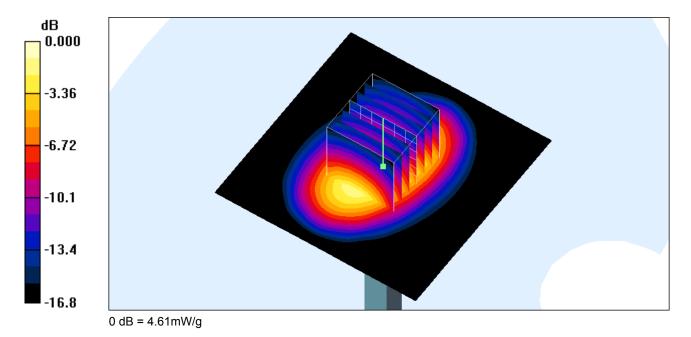



Appendix B - SAR Measurement Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/10/7

Body_GSM850 Ch189_Face with 1.5cm Gap_GPRS10

DUT: 800405


Communication System: GSM850; Frequency: 836.4 MHz;Duty Cycle: 1:4 Medium: MSL_850 Medium parameters used: f = 836.4 MHz; σ = 0.972 mho/m; ϵ_r = 56.3; ρ = 1000 kg/m³ Ambient Temperature : 22.5 °C; Liquid Temperature : 21.4 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch189/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.240 mW/g

Ch189/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 10.7 V/m; Power Drift = 0.161 dB Peak SAR (extrapolated) = 0.270 W/kg SAR(1 g) = 0.228 mW/g; SAR(10 g) = 0.175 mW/g Maximum value of SAR (measured) = 0.240 mW/g

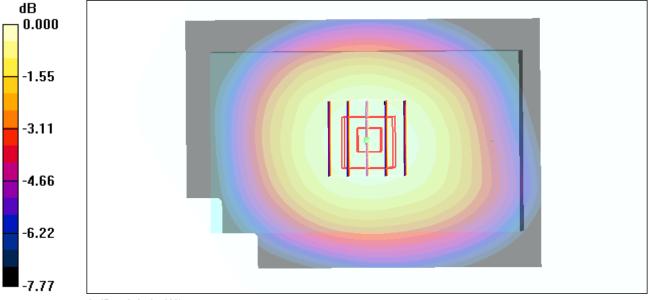

 $^{0 \,} dB = 0.240 \, mW/g$



Date: 2008/10/7

Body_GSM850 Ch251_Bottom with 1.5cm Gap_GPRS10

DUT: 800405


Communication System: GSM850; Frequency: 848.8 MHz;Duty Cycle: 1:8.3 Medium: MSL_850 Medium parameters used: f = 849 MHz; σ = 0.981 mho/m; ϵ_r = 56.1; ρ = 1000 kg/m³ Ambient Temperature : 22.6 °C; Liquid Temperature : 21.5 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch251/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.376 mW/g

Ch251/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 13.1 V/m; Power Drift = -0.003 dB Peak SAR (extrapolated) = 0.447 W/kg SAR(1 g) = 0.354 mW/g; SAR(10 g) = 0.259 mW/g Maximum value of SAR (measured) = 0.375 mW/g

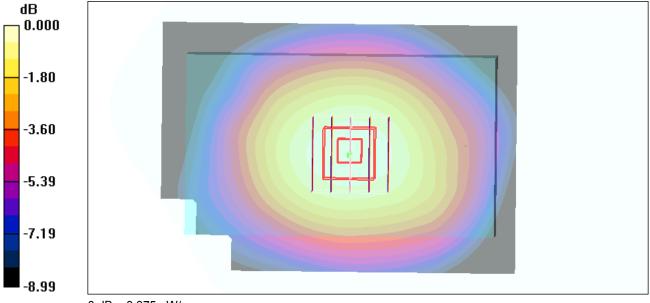

 $0 \, dB = 0.375 mW/g$



Date: 2008/10/7

Body_GSM1900 Ch661_Face with 1.5cm Gap_GPRS10

DUT: 800405

Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:4 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.5 mho/m; ϵ_r = 51.1; ρ = 1000 kg/m³ Ambient Temperature : 22.6 °C; Liquid Temperature : 21.6 °C


DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.145 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 8.82 V/m; Power Drift = -0.186 dB Peak SAR (extrapolated) = 0.232 W/kg SAR(1 g) = 0.132 mW/g; SAR(10 g) = 0.080 mW/g Maximum value of SAR (measured) = 0.141 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 8.82 V/m; Power Drift = -0.186 dB Peak SAR (extrapolated) = 0.199 W/kg SAR(1 g) = 0.120 mW/g; SAR(10 g) = 0.076 mW/g Maximum value of SAR (measured) = 0.126 mW/g

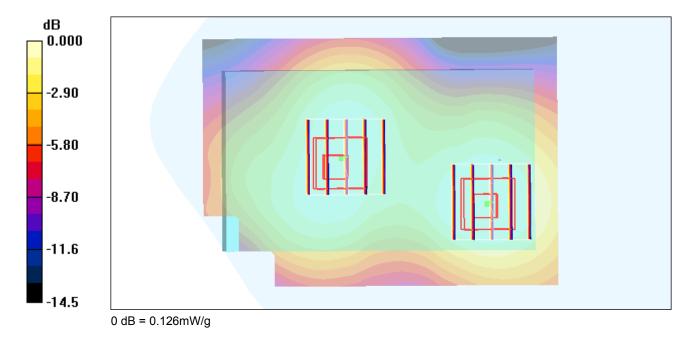



Date: 2008/10/7

Body_GSM1900 Ch661_Bottom with 1.5cm Gap_GPRS10

DUT: 800405


Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:4 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.5 mho/m; ϵ_r = 51.1; ρ = 1000 kg/m³ Ambient Temperature : 22.6 °C; Liquid Temperature : 21.6 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.271 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 13.9 V/m; Power Drift = -0.084 dB Peak SAR (extrapolated) = 0.461 W/kg SAR(1 g) = 0.246 mW/g; SAR(10 g) = 0.141 mW/g Maximum value of SAR (measured) = 0.261 mW/g

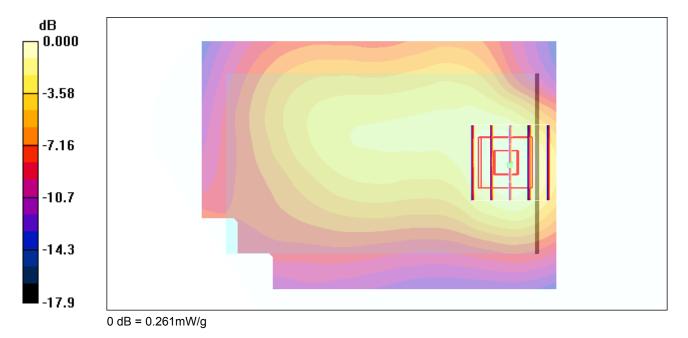



Date: 2008/10/7

Body_WCDMA850 Ch4182_Face with 1.5cm Gap_RMC12.2K

DUT: 800405


Communication System: WCDMA; Frequency: 836.4 MHz;Duty Cycle: 1:1 Medium: MSL_850 Medium parameters used : f = 836.4 MHz; σ = 0.972 mho/m; ϵ_r = 56.3; ρ = 1000 kg/m³ Ambient Temperature : 22.4 °C; Liquid Temperature : 21.5 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch4182/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.204 mW/g

Ch4182/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 10.5 V/m; Power Drift = -0.032 dB Peak SAR (extrapolated) = 0.232 W/kg SAR(1 g) = 0.195 mW/g; SAR(10 g) = 0.150 mW/g Maximum value of SAR (measured) = 0.206 mW/g

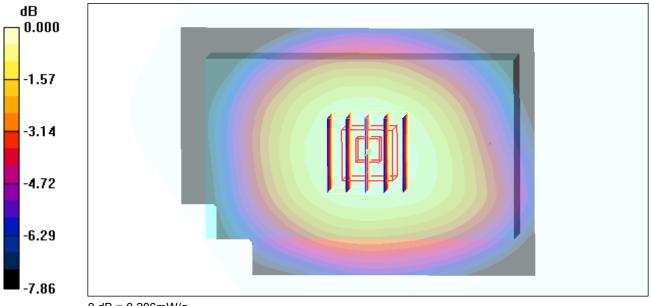

 $0 \, dB = 0.206 \, mW/g$



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab Date: 2008/10/7

Body_WCDMA850 Ch4233_Bottom with 1.5cm Gap_RMC12.2K

DUT: 800405


Communication System: WCDMA; Frequency: 846.6 MHz;Duty Cycle: 1:1 Medium: MSL_850 Medium parameters used: f = 847 MHz; σ = 0.98 mho/m; ϵ_r = 56.2; ρ = 1000 kg/m³ Ambient Temperature : 22.4 °C; Liquid Temperature : 21.5 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch4233/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.359 mW/g

Ch4233/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 11.7 V/m; Power Drift = 0.103 dB Peak SAR (extrapolated) = 0.426 W/kg SAR(1 g) = 0.346 mW/g; SAR(10 g) = 0.256 mW/g Maximum value of SAR (measured) = 0.366 mW/g

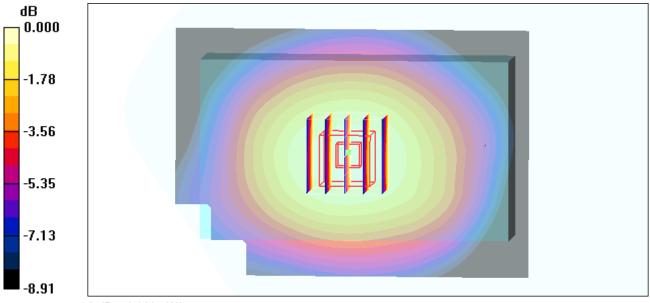

 $0 \, dB = 0.366 mW/g$



Date: 2008/10/7

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Body_WCDMA1900 Ch9400_Face with 1.5cm Gap_RMC12.2K

DUT: 800405

Communication System: WCDMA; Frequency: 1880 MHz;Duty Cycle: 1:1 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.5 mho/m; ϵ_r = 51.1; ρ = 1000 kg/m³ Ambient Temperature : 22.7 °C; Liquid Temperature : 21.6 °C


DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch9400/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.231 mW/g

Ch9400/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 10.5 V/m; Power Drift = -0.071 dB Peak SAR (extrapolated) = 0.382 W/kg SAR(1 g) = 0.216 mW/g; SAR(10 g) = 0.130 mW/g Maximum value of SAR (measured) = 0.227 mW/g

Ch9400/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 10.5 V/m; Power Drift = -0.071 dB Peak SAR (extrapolated) = 0.292 W/kg SAR(1 g) = 0.180 mW/g; SAR(10 g) = 0.114 mW/g Maximum value of SAR (measured) = 0.191 mW/g

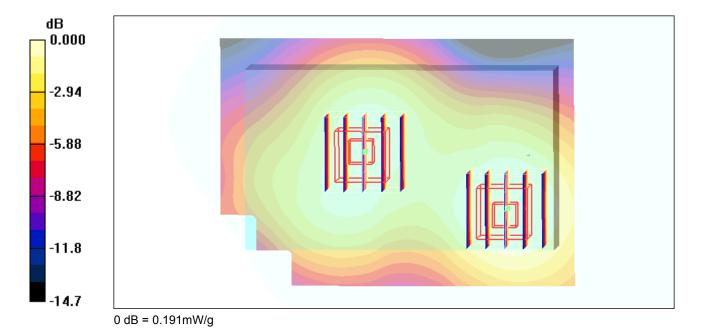



Date: 2008/10/7

Body_WCDMA1900 Ch9400_Bottom with 1.5cm Gap_RMC12.2K

DUT: 800405


Communication System: WCDMA; Frequency: 1880 MHz;Duty Cycle: 1:1 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.5 mho/m; ϵ_r = 51.1; ρ = 1000 kg/m³ Ambient Temperature : 22.7 °C; Liquid Temperature : 21.6 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch9400/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.476 mW/g

Ch9400/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 18.0 V/m; Power Drift = 0.173 dB Peak SAR (extrapolated) = 0.844 W/kg SAR(1 g) = 0.452 mW/g; SAR(10 g) = 0.258 mW/g Maximum value of SAR (measured) = 0.485 mW/g

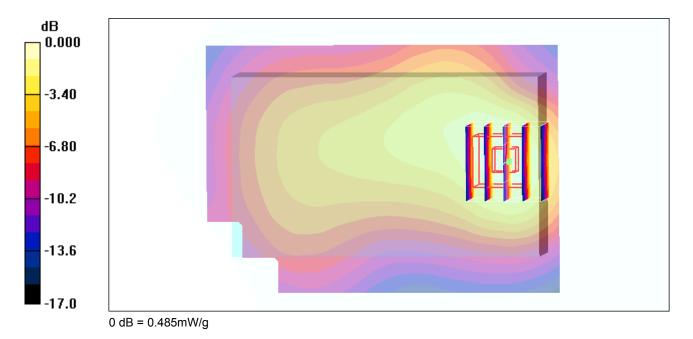



Date: 2008/10/7

Body_GSM850 Ch251_Bottom with 1.5cm Gap_GPRS10_2D

DUT: 800405


Communication System: GSM850; Frequency: 848.8 MHz;Duty Cycle: 1:8.3 Medium: MSL_850 Medium parameters used: f = 849 MHz; σ = 0.981 mho/m; ϵ_r = 56.1; ρ = 1000 kg/m³ Ambient Temperature : 22.6 °C; Liquid Temperature : 21.5 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch251/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.376 mW/g

Ch251/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 13.1 V/m; Power Drift = -0.003 dB Peak SAR (extrapolated) = 0.447 W/kg SAR(1 g) = 0.354 mW/g; SAR(10 g) = 0.259 mW/g Maximum value of SAR (measured) = 0.375 mW/g

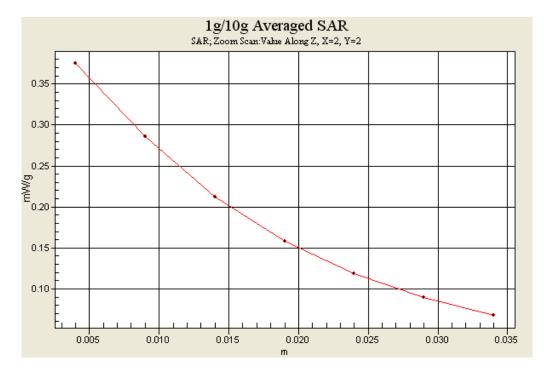



Date: 2008/10/7

Body_GSM1900 Ch661_Bottom with 1.5cm Gap_GPRS10_2D

DUT: 800405


Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:4 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.5 mho/m; ϵ_r = 51.1; ρ = 1000 kg/m³ Ambient Temperature : 22.6 °C; Liquid Temperature : 21.6 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch661/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.271 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 13.9 V/m; Power Drift = -0.084 dB Peak SAR (extrapolated) = 0.461 W/kg SAR(1 g) = 0.246 mW/g; SAR(10 g) = 0.141 mW/g Maximum value of SAR (measured) = 0.261 mW/g

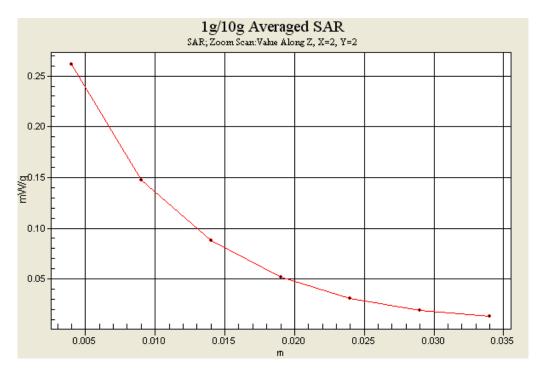



Test Report No : FA8O0405A

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/10/7

Body_WCDMA850 Ch4233_Bottom with 1.5cm Gap_RMC12.2K_2D

DUT: 800405


Communication System: WCDMA; Frequency: 846.6 MHz;Duty Cycle: 1:1 Medium: MSL_850 Medium parameters used: f = 847 MHz; σ = 0.98 mho/m; ϵ_r = 56.2; ρ = 1000 kg/m³ Ambient Temperature : 22.4 °C; Liquid Temperature : 21.5 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.91, 5.91, 5.91); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Left; Type: QD 000 P40 C; Serial: TP-1477
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch4233/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.359 mW/g

Ch4233/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 11.7 V/m; Power Drift = 0.103 dB Peak SAR (extrapolated) = 0.426 W/kg SAR(1 g) = 0.346 mW/g; SAR(10 g) = 0.256 mW/g Maximum value of SAR (measured) = 0.366 mW/g

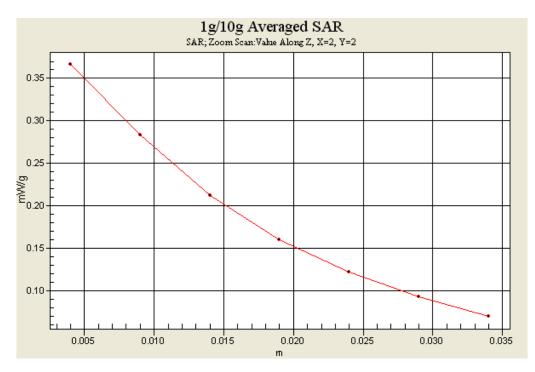



Date: 2008/10/7

Body_WCDMA1900 Ch9400_Bottom with 1.5cm Gap_RMC12.2K_2D

DUT: 800405


Communication System: WCDMA; Frequency: 1880 MHz;Duty Cycle: 1:1 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.5 mho/m; ϵ_r = 51.1; ρ = 1000 kg/m³ Ambient Temperature : 22.7 °C; Liquid Temperature : 21.6 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.49, 4.49, 4.49); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2007/11/16
- Phantom: SAM-Right; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch9400/Area Scan (71x101x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.476 mW/g

Ch9400/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 18.0 V/m; Power Drift = 0.173 dB Peak SAR (extrapolated) = 0.844 W/kg SAR(1 g) = 0.452 mW/g; SAR(10 g) = 0.258 mW/g Maximum value of SAR (measured) = 0.485 mW/g

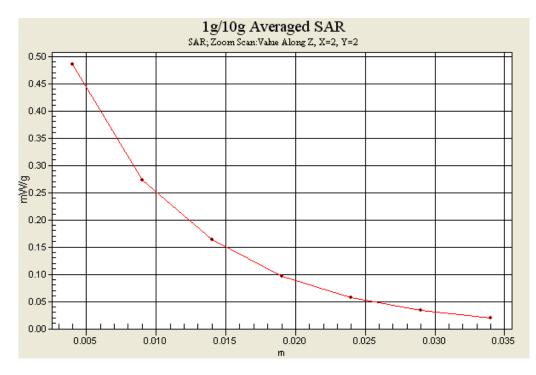



Test Report No : FA8O0405A

2 P

Appendix C – Calibration Data

성영 등 문화 방법 사람이 많은 것이 같아요. 가슴을 걸었다.	e is one of the signatorie	as to the EA	2014 - 19 19 19 19 19 19 19 19 19 19 19 19 19
he Swiss Accreditation Servic			
Iultilateral Agreement for the r			00EN/0 400 Mar 00
Client Sporton (Aude	in)	Certificate No: D	835V2-499_Mar08
CALIBRATION	CERTIFICATE		
Object	D835V2 - SN: 49	99	
Calibration procedure(s)	QA CAL-05.v7		
	Calibration proce	dure for dipole validation kits	
Calibration date:	March 17, 2008		
Condition of the calibrated item	In Tolerance		
The measurements and the unce	rtainties with confidence p	conal standards, which realize the physical units of robability are given on the following pages and are ry facility: environment temperature $(22 \pm 3)^{\circ}$ C and	e part of the certificate.
The measurements and the unce All calibrations have been conduc	rtainties with confidence p	robability are given on the following pages and are	e part of the certificate.
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards	rtainties with confidence p cted in the closed laborator TE critical for calibration}	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.)	a part of the certificate. I humidity < 70%. Scheduled Calibration
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736)	a part of the certificate. d humidity < 70%. <u>Scheduled Calibration</u> Oct-08
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736)	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718)	a part of the certificate. d humidity < 70%. <u>Scheduled Calibration</u> Oct-08
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g)	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736)	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and <u>Cal Date (Calibrated by, Certificate No.)</u> 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08)	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID #	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house)	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # ID # MY41092317	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07)	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # ID # MY41092317 100005	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 04-Aug-99 (SPEAG, in house check Oct-07)	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # ID # MY41092317	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07)	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # MY41092317 100005 US37390585 S4206 Name	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 04-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) Function	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # ID # MY41092317 100005 US37390585 S4206	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00736) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 04-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07)	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by:	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # MY41092317 100005 US37390585 S4206 Name Claudio Leubler	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and <u>Cal Date (Calibrated by, Certificate No.)</u> 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) <u>Check Date (in house)</u> 18-Oct-02 (SPEAG, in house check Oct-07) 04-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) Function Laboratory Technician	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by:	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # MY41092317 100005 US37390585 S4206 Name	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 04-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) Function	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
The measurements and the unce	rtainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # MY41092317 100005 US37390585 S4206 Name Claudio Leubler	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and <u>Cal Date (Calibrated by, Certificate No.)</u> 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) <u>Check Date (in house)</u> 18-Oct-02 (SPEAG, in house check Oct-07) 04-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) Function Laboratory Technician	a part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



WIS, BRP

s

Schweizerischer Kalibrierdienst

- Service suisse d'étalonnage
- С Servizio svizzero di taratura S

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D835V2-499_Mar08

Page 2 of 9

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	(e)
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.5 ± 6 %	0.90 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.29 mW / g
SAR normalized	normalized to 1W	9.16 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	9.16 mW / g ± 17.0 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
	condition 250 mW input power	1.50 mW / g
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured SAR normalized		1.50 mW / g 6.00 mW / g

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D835V2-499_Mar08

Page 3 of 9



Body TSL parameters The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.0 ± 6 %	1.00 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.46 mW / g
SAR normalized	normalized to 1W	9.84 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	9.52 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.63 mW / g
SAR normalized	normalized to 1W	6.52 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	6.37 mW / g ± 16.5 % (k=2)

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D835V2-499_Mar08

Page 4 of 9



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.9 Ω - 2.3 jΩ
Return Loss	- 28.9 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.2 Ω - 3.3 jΩ
Return Loss	- 29.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.392 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	July 10, 2003	

Certificate No: D835V2-499_Mar08

Page 5 of 9





DASY4 Validation Report for Head TSL

Date/Time: 17.03.2008 11:32:45

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:499


Communication System: CW-835; Frequency: 835 MHz; Duty Cycle: 1:1 Medium: HSL 900 MHz; Medium parameters used: f = 835 MHz; σ = 0.9 mho/m; ϵ_r = 41.5; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(6.09, 6.09, 6.09); Calibrated: 01.03.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Unnamed procedure/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 54.9 V/m; Power Drift = -0.005 dB Peak SAR (extrapolated) = 3.34 W/kg SAR(1 g) = 2.29 mW/g; SAR(10 g) = 1.5 mW/g Maximum value of SAR (measured) = 2.58 mW/g

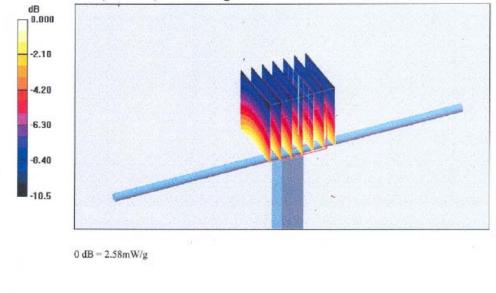


Certificate No: D835V2-499_Mar08

Page 6 of 9

-



Impedance Measurement Plot for Head TSL

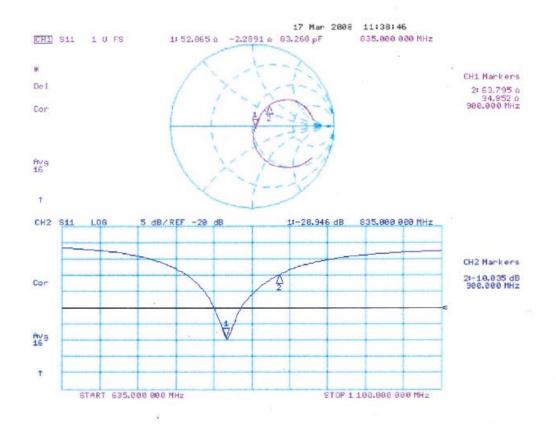

Certificate No: D835V2-499_Mar08

Page 7 of 9





DASY4 Validation Report for Body TSL

Date/Time: 10.03.2008 12:48:36

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:499


Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium: MSL900; Medium parameters used: f = 835 MHz; $\sigma = 1$ mho/m; $\varepsilon_r = 54$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(5.85, 5.85, 5.85); Calibrated: 01.03.2008
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW, d = 15 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 51.8 V/m; Power Drift = 0.036 dB Peak SAR (extrapolated) = 3.59 W/kg SAR(1 g) = 2.46 mW/g; SAR(10 g) = 1.63 mW/g Maximum value of SAR (measured) = 2.64 mW/g

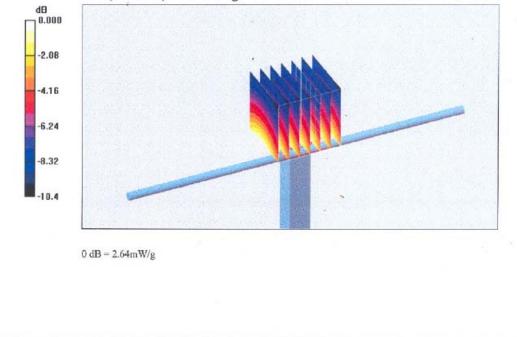


Certificate No: D835V2-499_Mar08

Page 8 of 9



Impedance Measurement Plot for Body TSL

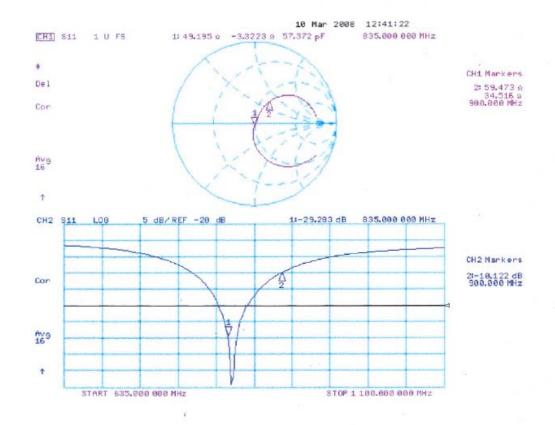

Certificate No: D835V2-499_Mar08

Page 9 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



SWISS

0

Schweizerischer Kalibrierdienst S Service suisse d'étalonnage С

Certificate No: D1900V2-5d041_Mar08

Servizio svizzero di taratura

Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 108

S

Client Sporton (Auden)

Object	D1900V2 - SN: 5	d041	
Calibration procedure(s)	QA CAL-05.v7	dure for dipole validation kits	
	Calibration proce	dure for dipole validation kits	
Calibration date:	March 18, 2008		
Condition of the calibrated item	In Tolerance		
The measurements and the unce	ertainties with confidence p	onal standards, which realize the physical units or robability are given on the following pages and ar y facility: environment temperature (22 ± 3)°C an	e part of the certificate.
Calibration Equipment used (M&		, nong, en nonnen (en person e (ez 2 e), e 2 e	
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
ower meter EPM-442A	GB37480704	04-Oct-07 (METAS, No. 217-00736)	Oct-08
ower sensor HP 8481A	US37292783	04-Oct-07 (METAS, No. 217-00736)	Oct-08
eference 20 dB Attenuator	SN: 5086 (20g)	07-Aug-07 (METAS, No 217-00718)	Aug-08
eference 10 dB Attenuator	SN: 5047.2 (10r)	07-Aug-07 (METAS, No 217-00718)	Aug-08
eference Probe ES3DV2	SN: 3025	01-Mar-08 (SPEAG, No. ES3-3025_Mar08)	Mar-09
	SN 909	2 Car OG COELC No DAEL 000 CarOT	
	1 214 808	3-Sep-08 (SPEAG, No. DAE4-909_Sep07)	Sep-07
AE4	ID#	Check Date (in house)	Sep-07 Scheduled Check
0AE4 Secondary Standards	1		
DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ID #	Check Date (in house)	Scheduled Check In house check: Oct-08
DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	ID # MY41092317	Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07)	Scheduled Check In house check: Oct-08 In house check: Oct-09
DAE4 Secondary Standards Power sensor HP 8481A	ID # MY41092317 100005	Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07)	Scheduled Check In house check: Oct-08 In house check: Oct-09
DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	ID # MY41092317 100005 US37390585 S4206	Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07)	Scheduled Check In house check: Oct-08 In house check: Oct-09 In house check: Oct-08
DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	ID # MY41092317 100005 US37390585 S4206 GB37480704	Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 04-Oct-07 (METAS, No. 217-00736)	Scheduled Check In house check: Oct-08 In house check: Oct-08 Oct-08 Signature
DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Power meter EPM-442A	ID # MY41092317 100005 US37390585 S4206 GB37480704 Name	Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 04-Oct-07 (METAS, No. 217-00736) Function	Scheduled Check In house check: Oct-08 In house check: Oct-08 In house check: Oct-08 Oct-08
DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Power meter EPM-442A Calibrated by:	ID # MY41092317 100005 US37390585 S4206 GB37480704 Name Marcel Fehr	Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 4-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 04-Oct-07 (METAS, No. 217-00/36) Function Laboratory Technician	Scheduled Check In house check: Oct-0 In house check: Oct-0 In house check: Oct-0 Oct-08 Signature



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



SNISS OF NO

S

С

S

Schweizerischer Kalibrierdienst

Service suisse d'étalonnage

Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- · SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D1900V2-5d041_Mar08

Page 2 of 9

. *



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	41.
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.47 mho/m ± 6 %
Head TSL temperature during test	(21.1 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	250 mW input power	10.1 mW/g
SAR normalized	normalized to 1W	40.4 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	39.5 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.20 mW / g
SAR normalized	normalized to 1W	20.8 mW/g
SAR for nominal Head TSL parameters 1	normalized to 1W	20.6 mW / g ± 16.5 % (k=2)

÷

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D1900V2-5d041_Mar08

Page 3 of 9

2 8

Body TSL parameters

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.6 ± 6 %	1.57 mho/m ± 6 %
Body TSL temperature during test	(21.4 ± 0.2) °C	<u></u>	

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.4 mW / g
SAR normalized	normalized to 1W	41.6 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	40.1 mW / g ± 17.0 % (k=2)
	a second bit second	
SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
	condition 250 mW input power	5.44 mW / g
SAR averaged over 10 cm ³ (10 g) of Body TSL SAR measured SAR normalized		5.44 mW / g 21.8 mW / g
SAR measured	250 mW input power	

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D1900V2-5d041_Mar08

Page 4 of 9



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.0 Ω + 5.1 jΩ	
Return Loss	- 24.2 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.0 Ω + 6.1 jΩ	
Return Loss	- 23.6 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.199 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 04, 2003

Certificate No: D1900V2-5d041_Mar08

Page 5 of 9



DASY4 Validation Report for Head TSL

Date/Time: 18.03.2008 12:05:10

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: HSL U10 BB; Medium parameters used: f = 1900 MHz; σ = 1.47 mho/m; ϵ_r = 40.2; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.9, 4.9, 4.9); Calibrated: 01.03.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172


Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 91.7 V/m; Power Drift = 0.013 dB Peak SAR (extrapolated) = 19.1 W/kg SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.2 mW/g Maximum value of SAR (measured) = 11.8 mW/g

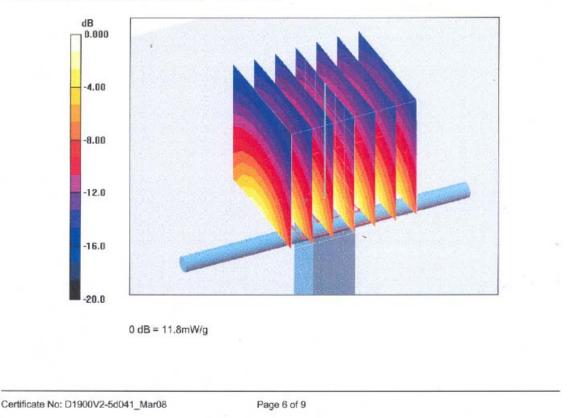



Impedance Measurement Plot for Head TSL

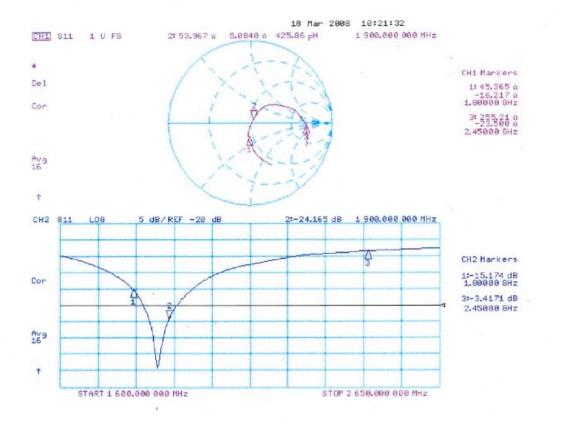

Certificate No: D1900V2-5d041_Mar08

Page 7 of 9



DASY4 Validation Report for Body TSL

Date/Time: 14.03.2008 13:22:24

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: MSL U10 BB; Medium parameters used: f = 1900 MHz; σ = 1.57 mho/m; ϵ_r = 51.7; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.5, 4.5, 4.5); Calibrated: 01.03.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 89.7 V/m; Power Drift = 0.004 dB Peak SAR (extrapolated) = 18.6 W/kg SAR(1 g) = 10.4 mW/g; SAR(10 g) = 5.44 mW/g Maximum value of SAR (measured) = 12.0 mW/g

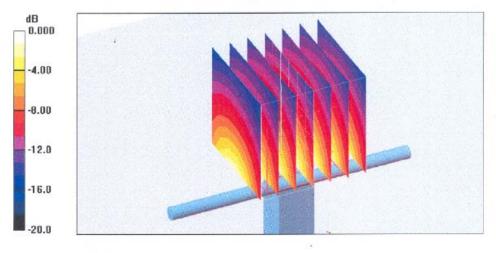


0 dB = 12.0mW/g

Certificate No: D1900V2-5d041_Mar08

Page 8 of 9



Impedance Measurement Plot for Body TSL

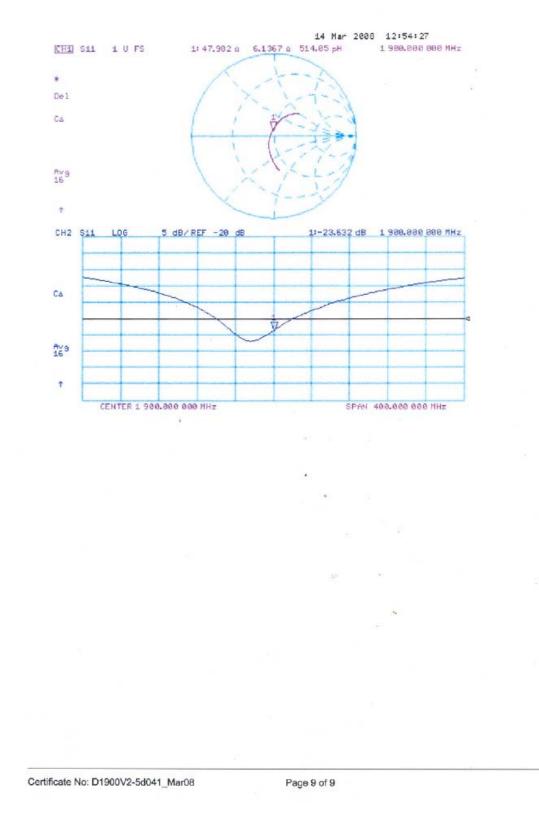



Test Report No : FA8O0405A

Engineering AG Zeughausstrasse 43, 8004 Zurich,	Switzerland	Hac MRA R C C Z Z C R BRATO S	Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
Accredited by the Swiss Accreditation The Swiss Accreditation Service i	이 집에 가지 않는 것이 같은 것이 같이 많이 많이 많이 많이 많이 많이 했다.		No.: SCS 108
Multilateral Agreement for the rec			DAC2 577 No.07
Client Sporton (Auden)			: DAE3-577_Nov07
CALIBRATION CI	ERTIFICATE		
Object	DAE3 - SD 000 D	03 AA - SN: 577	
Calibration procedure(s)	QA CAL-06.v12 Calibration procee	dure for the data acquisition elec	tronics (DAE)
Calibration date:	November 16, 20	07	
Condition of the calibrated item	In Tolerance		
The measurements and the uncerta	ainties with confidence pr	onal standards, which realize the physical uni obability are given on the following pages and y facility: anvironment temperature (22 ± 3)°C	d are part of the certificate.
The measurements and the uncerta	ainties with confidence pr ad in the closed laboratory critical for celibration)	obability are given on the following pages and y facility: environment temperature (22 ± 3)°C	d are part of the certificate. C and humidity < 70%.
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards	ainties with confidence provide in the closed laboratory critical for celibration)	obability are given on the following pages and y facility: environment temperature (22 ± 3)°C Cal Date (Calibrated by, Certificate No.)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702	ainties with confidence provide in the closed laboratory critical for celibration)	obability are given on the following pages and y facility: environment temperature (22 ± 3)°C	d are part of the certificate. C and humidity < 70%.
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001	ainties with confidence provide in the closed laboratory ortical for cellbration)	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (Elcal AG, No: 6467)	d are part of the certificate. C and humidity < 70%. <u>Scheduled Calibration</u> Oct-08
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ainties with confidence provide in the closed laboratory ortifical for calibration) ID # SN: 6295803 SN: 0810278 ID #	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (Elcal AG, No: 6465)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-08 Oct-08
The measurements and the uncerta	ainties with confidence provide in the closed laboratory ortifical for calibration) ID # SN: 6295803 SN: 0810278 ID #	obability are given on the following pages and y facility: environment temperature (22 ± 3)°C Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (Elcal AG, No: 6467) 03-Oct-07 (Elcal AG, No: 6465) Check Date (in house)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Scheduled Check
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ainties with confidence provide in the closed laboratory ortifical for calibration) ID # SN: 6295803 SN: 0810278 ID #	Obability are given on the following pages and y facility: environment temperature (22 ± 3)°C Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (Elcal AG, No: 6467) 03-Oct-07 (Elcal AG, No: 6465) Check Date (in house) 25-Jun-07 (SPEAG, in house check)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Scheduled Check
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ainties with confidence proved in the closed laboratory ortical for celibration) ID # SN: 6295803 SN: 0810278 ID # SE UMS 006 AB 1004	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (Elcal AG, No: 6467) 03-Oct-07 (Elcal AG, No: 6465) Check Date (in house) 25-Jun-07 (SPEAG, in house check)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Scheduled Check
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ainties with confidence proved in the closed laboratory oritical for celibration) ID # SN: 6295803 SN: 0810278 ID # SE UMS 006 AB 1004	obability are given on the following pages and y facility: environment temperature (22 ± 3)°C Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (Elcal AG, No: 6467) 03-Oct-07 (Elcal AG, No: 6465) Check Date (in house) 25-Jun-07 (SPEAG, in house check)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Scheduled Check In house check Jun-08
The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ainties with confidence proved in the closed laboratory ortical for celibration) ID # SN: 6295803 SN: 0810278 ID # SE UMS 006 AB 1004	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (Elcal AG, No: 6467) 03-Oct-07 (Elcal AG, No: 6465) Check Date (in house) 25-Jun-07 (SPEAG, in house check)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Scheduled Check In house check Jun-08

Certificate No: DAE3-577_Nov07

Page 1 of 5



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



SWISS C. Z. Z Pr. BRAT

S

C

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE Connector angle data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a
 result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE3-577_Nov07

Page 2 of 5



DC Voltage Measurement

High Range:	1LSB =	6.1µV,	full range =	-100+300 mV
Low Range:	1LSB =	61nV,	full range =	-1+3mV
DASY measurement	parameters: Aut	o Zero Time: 3	sec; Measuring	time: 3 sec

Calibration Factors	X	Y	Z
High Range	404.432 ± 0.1% (k=2)	403.884 ± 0.1% (k=2)	404.331 ± 0.1% (k=2)
Low Range	3.94218 ± 0.7% (k=2)	3.94771 ± 0.7% (k=2)	3.94526 ± 0.7% (k=2)

Connector Angle

	268 9 + 1 9
Connector Angle to be used in DASY system	208 ° ± 1 °

÷



Appendix

1. DC Voltage Linearity

High Range		Input (µV)	Reading (µV)	Error (%)
Channel X	+ Input	200000	199999.3	0.00
Channel X	+ Input	20000	20005.75	0.03
Channel X	- Input	20000	-19997.67	-0.01
Channel Y	+ input	200000	199999.5	0.00
Channel Y	+ input	20000	20002.82	0.01
Channel Y	- Input	20000	-20004.40	0.02
Channel Z	+ Input	200000	199999.6	0.00
Channel Z	+ Input	20000	20005.54	0.03
Channel Z	- Input	20000	-20001.11	0.01

Low Range		Input (µV)	Reading (µV)	Error (%)
Channel X	+ input	2000	2000.1	0.00
Channel X	+ Input	200	199.12	-0.44
Channel X	- Input	200	-200.64	0.32
Channel Y	+ Input	2000	2000	0.00
Channel Y	+ Input	200	199.96	-0.02
Channel Y	- Input	. 200	-201.00	0.50
Channel Z	+ Input	2000	1999.9	0.00
Channel Z	+ Input	200	199.05	-0.47
Channel Z	- Input	200	-201.08	0.54

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Averaģe Reading (μV)	Low Range Average Reading (µV)
Channel X	200	13.88	12.97
	- 200	-12.40	-14.29
Channel Y	200	-6.32	-6.22
	- 200	5.34	5.31
Channel Z	200	1.08	0.59
	- 200	-1.42	-1.66

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	-	1.14	0.16
Channel Y	200	1.52	-	3.87
Channel Z	200	0.23	0.75	-

Certificate No: DAE3-577_Nov07



4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15969	16269
Channel Y	15848	16148
Channel Z	16203	16661

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input $10 M \Omega$

+	Average (µV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.12	-1.70	1.72	0.50
Channel Y	-2.46	-3.42	-1.39	0.44
Channel Z	-0.78	-2.16	0.00	0.29

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	199.3
Channel Y	0.2001	199.9
Channel Z	0.1999	199.4

8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC)		
Supply (+ Vcc)		+7.9	
Supply (- Vcc)		-7.6	

9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.0	t≓ +6 ·	+14
Supply (- Vcc)	-0.01	-8	-9

Page 5 of 5



Schmid & Partner Engineering AG eughausstrasse 43, 8004 Zuric	y of h, Switzerland	SWISS BC MRA C D Z SWISS C D Z S C D Z S S S S S S S S S S S S S S S S S S S	Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
ccredited by the Swiss Accredita he Swiss Accreditation Service			No.: SCS 108
lient Sporton (Aude			: ET3-1787_Aug08
ALIBRATION		Έ	
Dbject	ET3DV6 - SN:1	787	
Calibration procedure(s)		and QA CAL-23.v3 edure for dosimetric E-field probe	S
Calibration date:	August 26, 2008	3	
Condition of the calibrated item	In Tolerance		
The measurements and the unce	rtainties with confidence	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)°(d are part of the certificate.
he measurements and the unce	rtainties with confidence	probability are given on the following pages an	d are part of the certificate.
he measurements and the unce Il calibrations have been conduc alibration Equipment used (M&T	rtainties with confidence	probability are given on the following pages an	d are part of the certificate.
he measurements and the unce II calibrations have been conduc alibration Equipment used (M& rimary Standards	rtainties with confidence sted in the closed laborat TE critical for calibration)	probability are given on the following pages an ory facility: environment temperature $(22 \pm 3)^{\circ}$	d are part of the certificate C and humidity < 70%.
he measurements and the unce II calibrations have been conduct alibration Equipment used (M& rimary Standards ower meter E4419B	rtainties with confidence sted in the closed laborat TE critical for calibration)	probability are given on the following pages an ory facility: environment temperature (22 ± 3)*(Cal Date (Certificate No.)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration
he measurements and the unce Il calibrations have been conduct alibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A	rtainties with confidence sted in the closed laborat TE critical for calibration) ID # GB41293874	probability are given on the following pages an ory facility: environment temperature (22 ± 3)*(Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Apr-09
he measurements and the unce Il calibrations have been conduct alibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c)	probability are given on the following pages an ory facility: environment temperature (22 ± 3)*(Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Apr-09 Jul-09
he measurements and the unce all calibrations have been conduct calibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A leference 3 dB Attenuator leference 20 dB Attenuator	tainties with confidence ated in the closed laboration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	probability are given on the following pages an ory facility: environment temperature (22 ± 3)*(Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 31-Mar-08 (No. 217-00787)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Apr-09 Jul-09 Apr-09
he measurements and the unce all calibrations have been conduct calibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A tower sensor E4412A telefence 3 dB Attenuator leference 20 dB Attenuator leference 30 dB Attenuator	tainties with confidence ated in the closed laboration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b)	probability are given on the following pages an ory facility: environment temperature (22 ± 3)*(Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 31-Mar-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00866)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09
he measurements and the unce Il calibrations have been conduct alibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A eference 3 dB Attenuator eference 30 dB Attenuator eference 30 dB Attenuator eference Stop ES3DV2	tainties with confidence ated in the closed laboration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	probability are given on the following pages an ory facility: environment temperature (22 ± 3)*(Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 31-Mar-08 (No. 217-00787)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Apr-09 Jul-09 Apr-09
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M&T Primary Standards Prower meter E4419B Prower sensor E4412A Prower sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ID # GB41293874 MY41495277 MY41495277 SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013 SN: 660	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 253-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09 Sep-08
he measurements and the unce all calibrations have been conduct calibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A leference 3 dB Attenuator leference 20 dB Attenuator leference 30 dB Attenuator leference Probe ES3DV2 (AE4 econdary Standards	rtainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID #	probability are given on the following pages an ory facility: environment temperature (22 ± 3)*(Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00786) 2-Jan-08 (No. E3-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07) Check Date (in house)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09 Sep-08 Scheduled Check
he measurements and the unce Il calibrations have been conduct alibration Equipment used (M& rimary Standards ower meter E4419B ower sensor E4412A eference 3 dB Attenuator eference 20 dB Attenuator eference 20 dB Attenuator eference 70 dB Attenuator eference Probe ES3DV2 AE4 econdary Standards F generator HP 8648C	ID # GB41293874 MY41495277 MY41495277 SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013 SN: 660	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 253-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09 Sep-08
he measurements and the unce alibrations have been conduct calibration Equipment used (M& trimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A deference 3 dB Attenuator leference 20 dB Attenuator leference 30 dB Attenuator leference Probe ES3DV2 AE4 econdary Standards /F generator HP 8648C	rtainties with confidence cted in the closed laboration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700 US37390585	probability are given on the following pages an ory facility: environment temperature (22 ± 3)*0 Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 1-Jul-08 (No. 217-00786) 31-Mar-08 (No. 217-00787) 1-Jul-08 (No. 217-00786) 2-Jan-08 (No. 217-00787) 3-Sep-07 (No. DAE4-660_Sep07) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-08
he measurements and the unce alibrations have been conduct calibration Equipment used (M& trimary Standards tower meter E4419B tower sensor E4412A tower sensor E4412A teleference 3 dB Attenuator teleference 20 dB Attenuator teleference 30 dB Attenuator teleference Probe ES3DV2 (AE4 tecondary Standards (F generator HP 8648C tetwork Analyzer HP 8753E	ID # GB41293874 MY41495277 MY41495277 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700 US37390585 Name	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00786) 1-Jul-08 (No. 217-00786) 2-Jan-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 2-Jan-08 (No. ES3-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07) Function	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jan-09 Sep-08 Scheduled Check In house check: Oct-09
The measurements and the unce NI calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	rtainties with confidence cted in the closed laboration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700 US37390585	probability are given on the following pages an ory facility: environment temperature (22 ± 3)*0 Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 1-Jul-08 (No. 217-00786) 31-Mar-08 (No. 217-00787) 1-Jul-08 (No. 217-00786) 2-Jan-08 (No. 217-00787) 3-Sep-07 (No. DAE4-660_Sep07) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-08
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M&T Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Standards RF generator HP 8648C Network Analyzer HP 8753E Calibrated by:	ID # GB41293874 MY41495277 MY41495277 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700 US37390585 Name	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00786) 1-Jul-08 (No. 217-00786) 2-Jan-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 2-Jan-08 (No. ES3-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07) Function	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-08
The measurements and the unce	ID # ID # GB41293874 MY41495277 MY41495277 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700 US37390585 Name Katja Pokovic	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. ES3-3013_Jan08) 3-Sep-07 (No. DAE4-660_Sep07) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07) Function Technical Manager	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-08

Certificate No: ET3-1787_Aug08

Page 1 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



SWISS

0

IBRA

S

C

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary: TSL

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
Polarization φ	φ rotation around probe axis
Polarization 9	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This
 linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of
 the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1787_Aug08

Page 2 of 9



August 26, 2008

Probe ET3DV6

SN:1787

Manufactured: Last calibrated: Recalibrated: May 28, 2003 August 28, 2007 August 26, 2008

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: ET3-1787_Aug08

Page 3 of 9



August 26, 2008

DASY - Parameters of Probe: ET3DV6 SN:1787

Sensitivity in Free Space^A

Diode Compression^B

NormX	1.63 ± 10.1%	μV/(V/m) ²	DCP X	90 mV
NormY	1.67 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	93 mV
NormZ	2.18 ± 10.1%	μ V/(V/m) ²	DCP Z	92 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect

```
TSL
```

900 MHz Typical SAR gradient: 5 % per mm

Sensor Cente	er to Phantom Surface Distance	3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	11.3	7.5
SARbe [%]	With Correction Algorithm	0.8	0.5

TSL 1750 MHz Typical SAR gradient: 10 % per mm

Sensor Cente	r to Phantom Surface Distance	3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	10.1	6.5
SAR _{be} [%]	With Correction Algorithm	0.8	0.6

Sensor Offset

Probe Tip to Sensor Center

2.7 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).

⁸ Numerical linearization parameter: uncertainty not required.

Certificate No: ET3-1787_Aug08

Page 4 of 9



August 26, 2008

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22) 1.5 1.4 1.3 Frequency response (normalized) 1.2 1.1 1.0 0.9 0.8 0.7 0.6 0.5 2000 2500 3000 0 500 1000 1500 f [MHz] --- TEM

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


2

Certificate No: ET3-1787_Aug08


Page 5 of 9



August 26, 2008

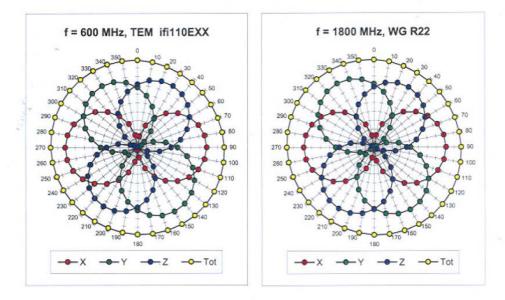

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

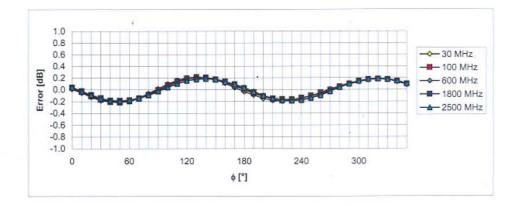


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ET3-1787_Aug08

Page 6 of 9



August 26, 2008

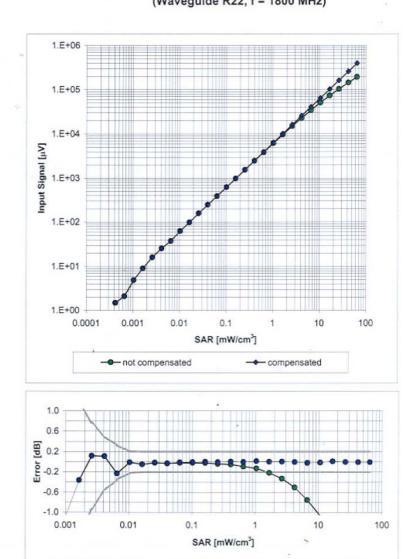

Dynamic Range f(SAR_{head}) (Waveguide R22, f = 1800 MHz)


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: ET3-1787_Aug08

Page 7 of 9



August 26, 2008

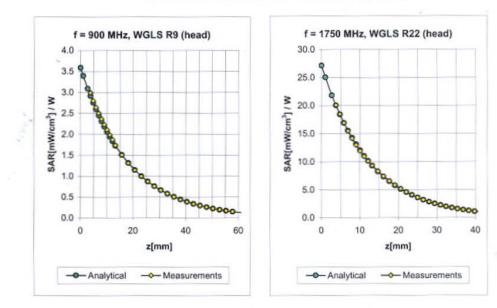

Conversion Factor Assessment

f [MHz]	Validity [MHz] ^c	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.30	2.80	6.06 ± 11.0% (k=2)
1750	± 50 / ± 100	Head	40.1 ± 5%	1.37 ± 5%	0.53	2.11	5.36 ± 11.0% (k=2)
1950	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.59	1.96	5.01 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1,80 ± 5%	0.77	1.57	4.49 ± 11.0% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	$1.05 \pm 5\%$	0.31	2.98	5.91 ± 11.0% (k=2)
1750	± 50 / ± 100	Body	53.4 ± 5%	$1.49 \pm 5\%$	0.60	2.20	4.73 ± 11.0% (k=2)
1950	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.68	1.95	4.49 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.90	1.51	3.79 ± 11.0% (k=2)

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: ET3-1787_Aug08


Page 8 of 9



August 26, 2008



Error (\, \,), f = 900 MHz

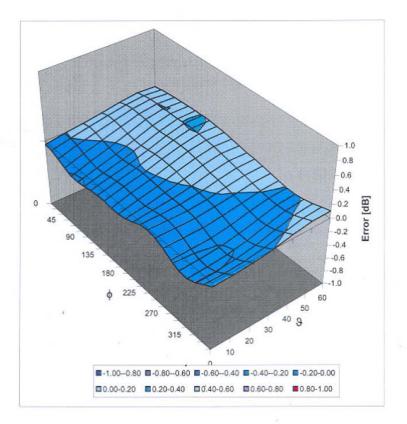


Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ET3-1787_Aug08

Page 9 of 9




Appendix D - Product Photos

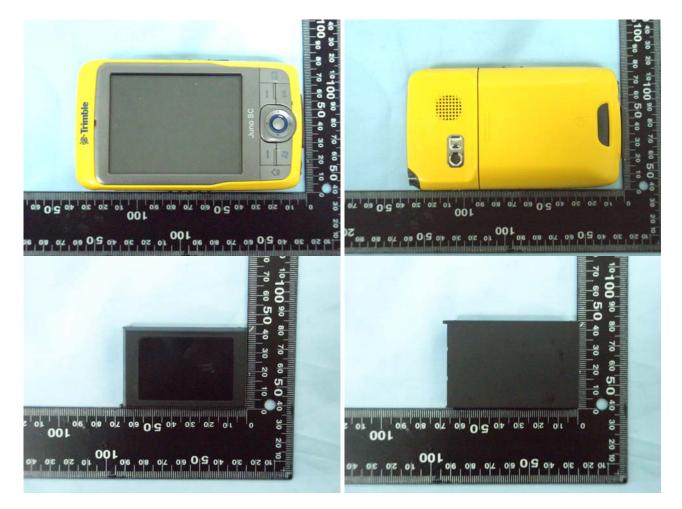




Appendix E - Test Setup Photos

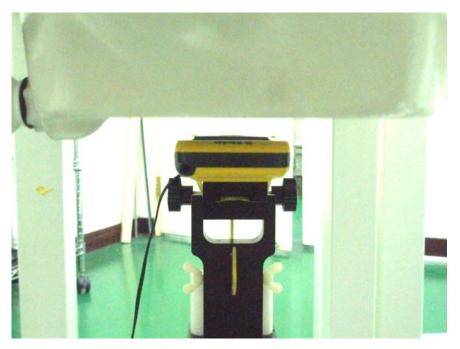

Face with 1.5cm Gap

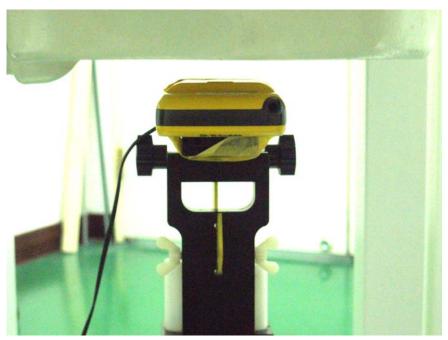

Bottom with 1.5cm Gap