



Calibration Laboratory of  
 Schmid & Partner  
 Engineering AG  
 Zeughausstrasse 43, 8004 Zurich, Switzerland

Client **Auden > Sporton Int. Inc.**

| CALIBRATION CERTIFICATE  |   |   |  |
|--|---|---|--|
| Object(s)  | ET3DV6 - SN:1788  |   |  |
| Calibration procedure(s)   | QA CAL-01.v2<br>Calibration procedure for dosimetric E-field probes |   |  |
| Calibration date:  | August 29, 2003   |   |  |
| Condition of the calibrated item   | In Tolerance (according to the specific calibration document)       |   |  |
| This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.   |   |   |  |
| All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.   |   |   |  |
| Calibration Equipment used (M&TE critical for calibration)   |   |   |  |
| Model Type   | ID #  | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration  |
| RF generator HP 8884C  | US3642U01700  | 4-Aug-99 (SPEAG, in house check Aug-02)   | In house check: Aug-05   |
| Power sensor E4412A  | MY41495277  | 2-Apr-03 (METAS, No 252-0250)             | Apr-04   |
| Power sensor HP 8481A  | MY41092180  | 18-Sep-02 (Agilent, No. 20020918)         | Sep-03   |
| Power meter EPM E4419B   | GB41293874  | 2-Apr-03 (METAS, No 252-0250)             | Apr-04   |
| Network Analyzer HP 8753E  | US37390585  | 18-Oct-01 (Agilent, No. 24BR1033101)      | In house check: Oct 03   |
| Fluke Process Calibrator Type 702  | SN: 6295803   | 3-Sep-01 (ELCAL, No.2360)                 | Sep-03   |
| Calibrated by:   | Name<br>Nico Vetterli   | Function<br>Technician                    | Signature<br> |
| Approved by:   | Name<br>Kajsa Pokovic   | Function<br>Laboratory Director           | Signature<br> |
| Date issued: August 28, 2003   |   |   |  |
| This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed. |   |   |  |

Schmid & Partner Engineering AG

**s p e a g**

Zeughausstrasse 43, 8004 Zurich, Switzerland  
Phone +41 1 245 9700, Fax +41 1 245 9779  
info@speag.com, <http://www.speag.com>

# Probe ET3DV6

SN:1788

Manufactured: May 28, 2003  
Last calibration: August 29, 2003

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1788

August 29, 2003

**DASY - Parameters of Probe: ET3DV6 SN:1788**

Sensitivity in Free Space

Diode Compression

|       |   |       |           |    |
|-------|---|-------|-----------|----|
| NormX | <b>1.68</b> $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP X | <b>95</b> | mV |
| NormY | <b>1.62</b> $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP Y | <b>95</b> | mV |
| NormZ | <b>1.71</b> $\mu\text{V}/(\text{V}/\text{m})^2$ | DCP Z | <b>95</b> | mV |

Sensitivity in Tissue Simulating Liquid

Head                      900 MHz                       $\epsilon_r = 41.5 \pm 5\%$                        $\sigma = 0.97 \pm 5\%$  mho/m

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

|         |                              |                  |             |
|---------|------------------------------|------------------|-------------|
| ConvF X | <b>6.6</b> $\pm 9.5\%$ (k=2) | Boundary effect: |             |
| ConvF Y | <b>6.6</b> $\pm 9.5\%$ (k=2) | Alpha            | <b>0.34</b> |
| ConvF Z | <b>6.6</b> $\pm 9.5\%$ (k=2) | Depth            | <b>2.48</b> |

Head                      1800 MHz                       $\epsilon_r = 40.0 \pm 5\%$                        $\sigma = 1.40 \pm 5\%$  mho/m

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

|         |                              |                  |             |
|---------|------------------------------|------------------|-------------|
| ConvF X | <b>5.3</b> $\pm 9.5\%$ (k=2) | Boundary effect: |             |
| ConvF Y | <b>5.3</b> $\pm 9.5\%$ (k=2) | Alpha            | <b>0.43</b> |
| ConvF Z | <b>5.3</b> $\pm 9.5\%$ (k=2) | Depth            | <b>2.80</b> |

Boundary Effect

Head                      900 MHz                      Typical SAR gradient: 5 % per mm

|                       |                              |      |      |
|-----------------------|------------------------------|------|------|
| Probe Tip to Boundary |                              | 1 mm | 2 mm |
| SAR <sub>be</sub> [%] | Without Correction Algorithm | 8.7  | 5.0  |
| SAR <sub>be</sub> [%] | With Correction Algorithm    | 0.3  | 0.5  |

Head                      1800 MHz                      Typical SAR gradient: 10 % per mm

|                       |                              |      |      |
|-----------------------|------------------------------|------|------|
| Probe Tip to Boundary |                              | 1 mm | 2 mm |
| SAR <sub>be</sub> [%] | Without Correction Algorithm | 12.8 | 8.9  |
| SAR <sub>be</sub> [%] | With Correction Algorithm    | 0.3  | 0.1  |


Sensor Offset

|                            |                  |    |
|----------------------------|------------------|----|
| Probe Tip to Sensor Center | <b>2.7</b>       | mm |
| Optical Surface Detection  | <b>1.6 ± 0.2</b> | mm |

ET3DV6 SN:1788


August 29, 2003

Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$

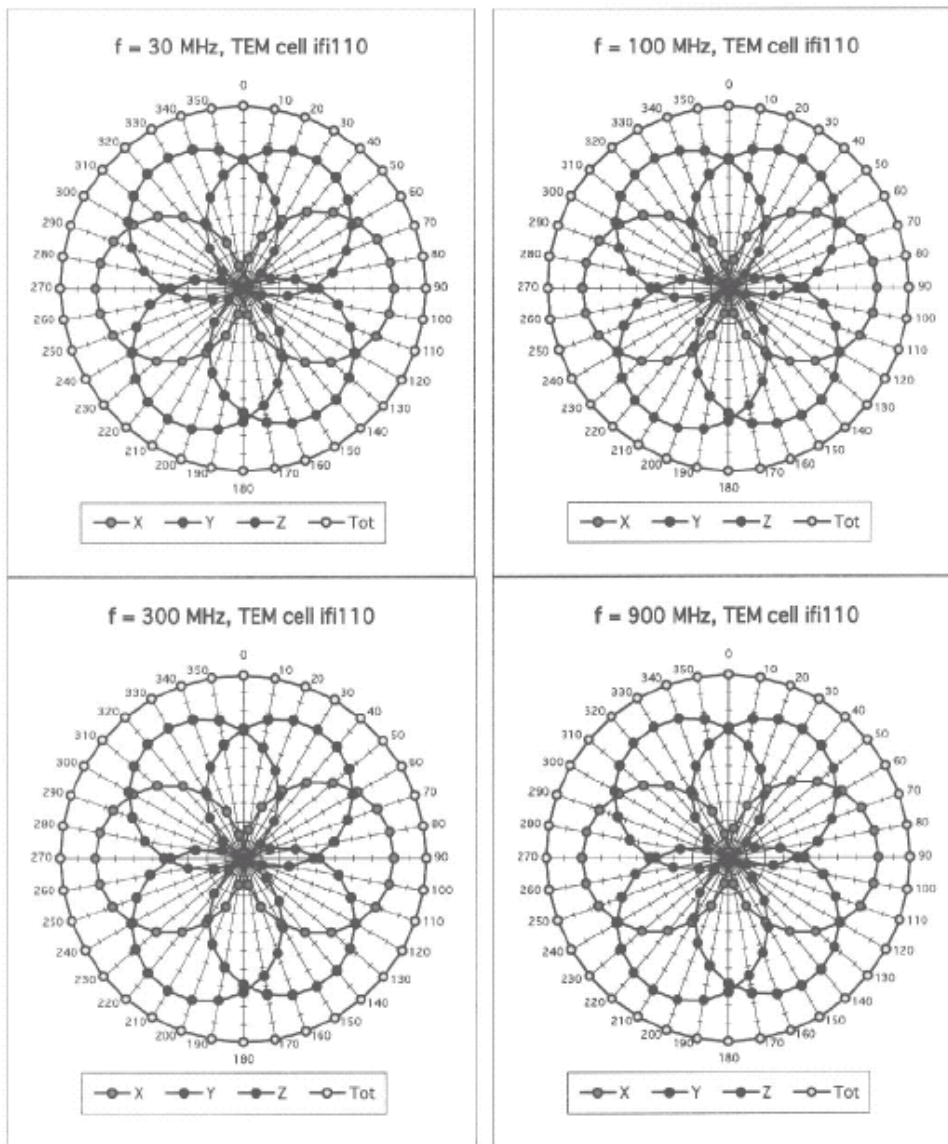


ET3DV6 SN:1788

August 29, 2003

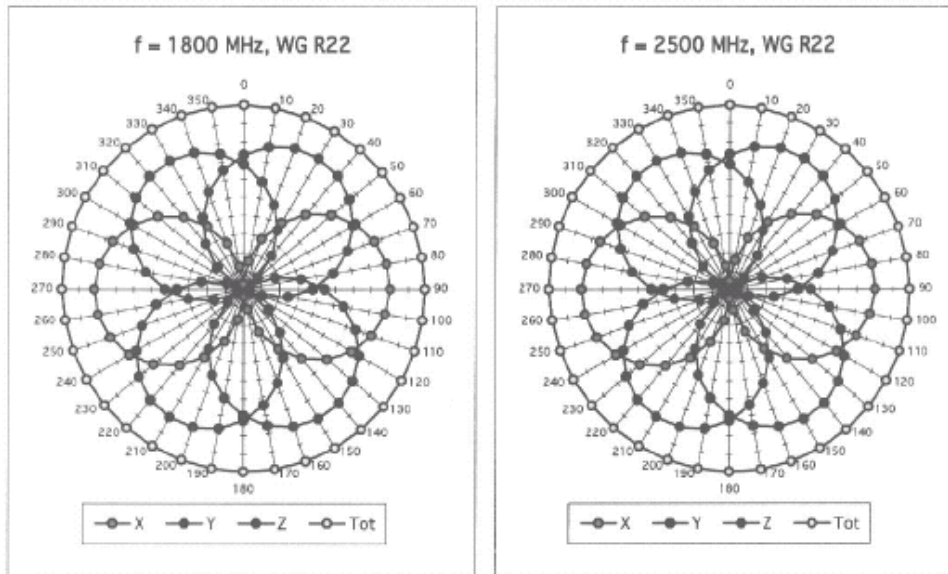

Isotropy Error ( $\phi$ ),  $\theta = 0^\circ$

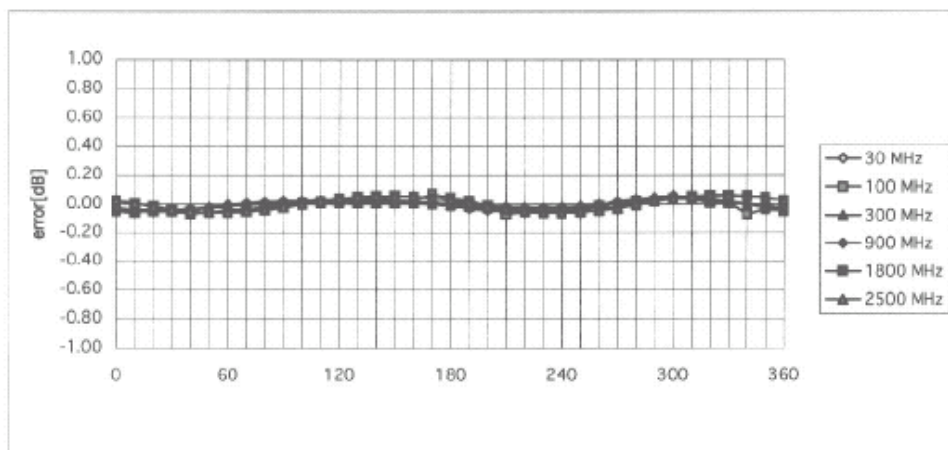


ET3DV6 SN:1788

August 29, 2003

### Frequency Response of E-Field

( TEM-Cell:ifi110, Waveguide R22)


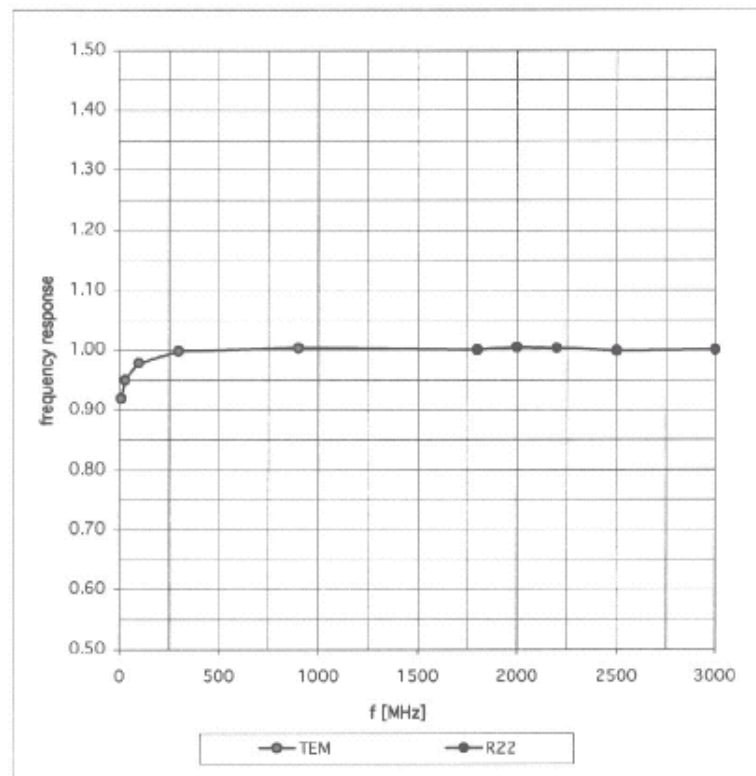


ET3DV6 SN:1788

August 29, 2003

### Dynamic Range f(SAR<sub>brain</sub>)


( Waveguide R22 )

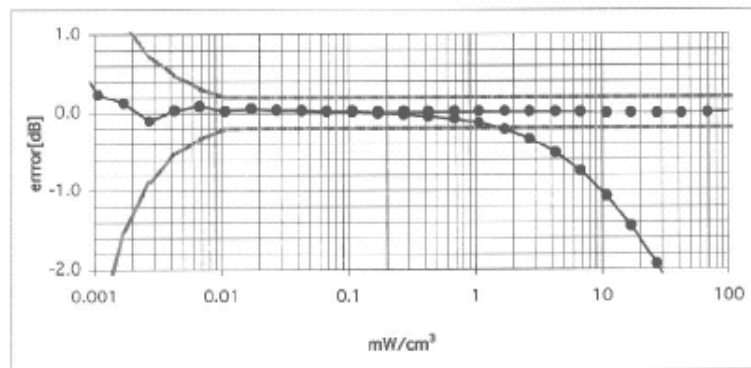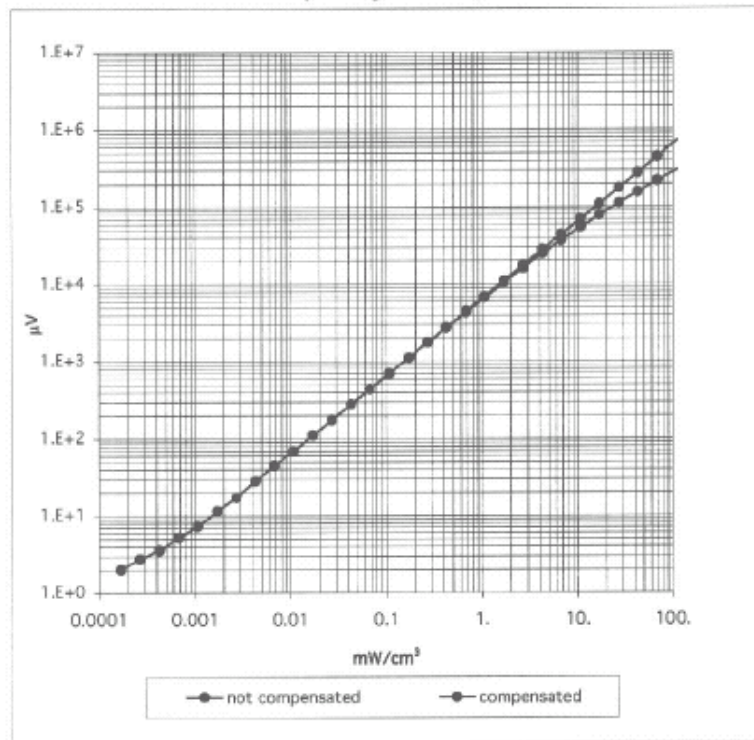

ET3DV6 SN:1788

August 29, 2003

### Conversion Factor Assessment

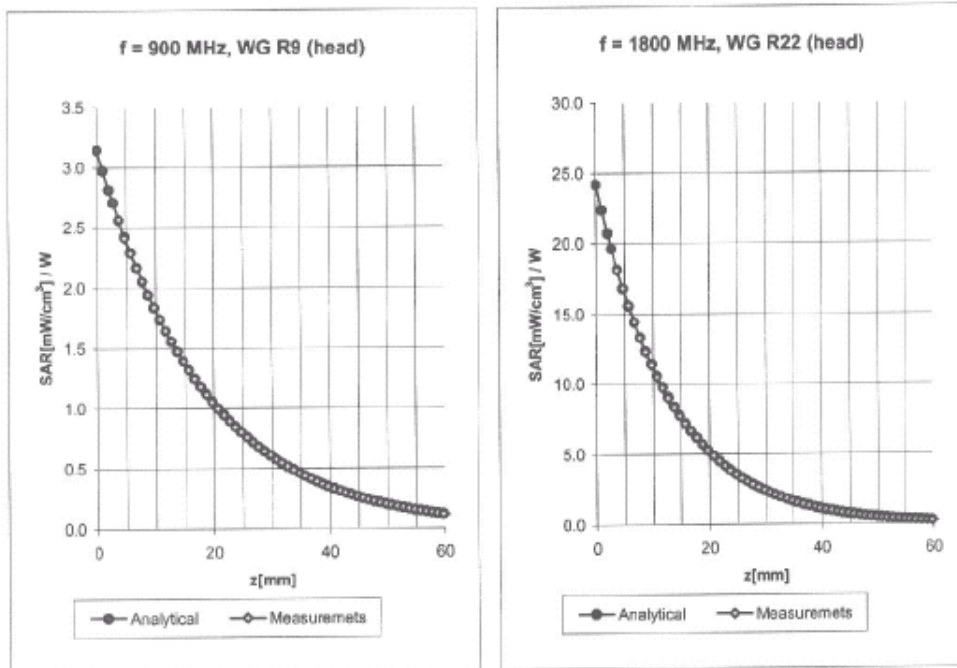

Head                      900 MHz                       $\epsilon_r = 41.5 \pm 5\%$                        $\sigma = 0.97 \pm 5\%$  mho/m

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

|         |                  |                  |      |
|---------|------------------|------------------|------|
| ConvF X | 6.6 ± 9.5% (k=2) | Boundary effect: |      |
| ConvF Y | 6.6 ± 9.5% (k=2) | Alpha            | 0.34 |
| ConvF Z | 6.6 ± 9.5% (k=2) | Depth            | 2.48 |

Head                      1800 MHz                       $\epsilon_r = 40.0 \pm 5\%$                        $\sigma = 1.40 \pm 5\%$  mho/m

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X


|         |                  |                  |      |
|---------|------------------|------------------|------|
| ConvF X | 5.3 ± 9.5% (k=2) | Boundary effect: |      |
| ConvF Y | 5.3 ± 9.5% (k=2) | Alpha            | 0.43 |
| ConvF Z | 5.3 ± 9.5% (k=2) | Depth            | 2.80 |



ET3DV6 SN:1788

August 29, 2003

### Conversion Factor Assessment

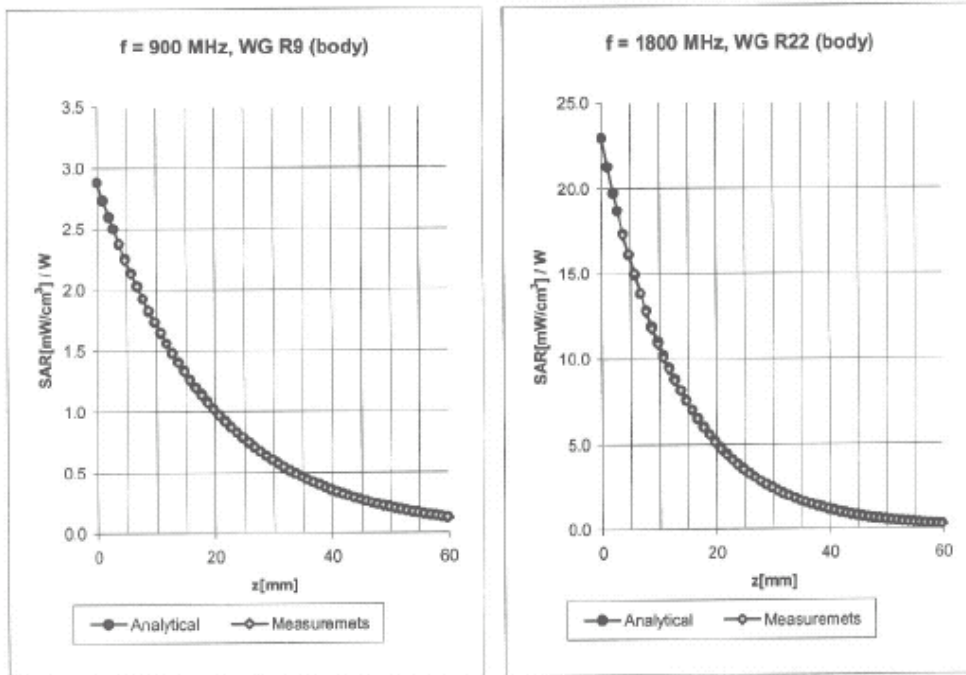

Body                      900 MHz                       $\epsilon_r = 55.0 \pm 5\%$                        $\sigma = 1.05 \pm 5\%$  mho/m

Valid for f=800-1000 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

|         |                  |                  |      |
|---------|------------------|------------------|------|
| ConvF X | 6.5 ± 9.5% (k=2) | Boundary effect: |      |
| ConvF Y | 6.5 ± 9.5% (k=2) | Alpha            | 0.31 |
| ConvF Z | 6.5 ± 9.5% (k=2) | Depth            | 2.92 |

Body                      1800 MHz                       $\epsilon_r = 53.3 \pm 5\%$                        $\sigma = 1.52 \pm 5\%$  mho/m


Valid for f=1710-1910 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

|         |                  |                  |      |
|---------|------------------|------------------|------|
| ConvF X | 5.0 ± 9.5% (k=2) | Boundary effect: |      |
| ConvF Y | 5.0 ± 9.5% (k=2) | Alpha            | 0.51 |
| ConvF Z | 5.0 ± 9.5% (k=2) | Depth            | 2.78 |

ET3DV6 SN:1788

August 29, 2003

### Conversion Factor Assessment

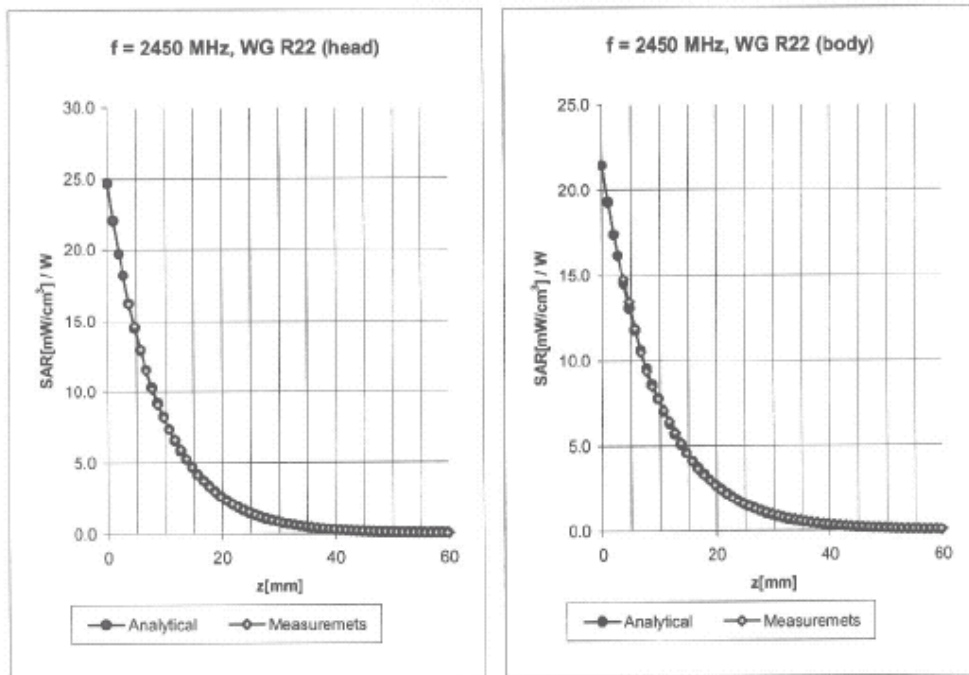

Head                      2450 MHz                       $\epsilon_r = 39.2 \pm 5\%$                        $\sigma = 1.80 \pm 5\%$  mho/m

Valid for f=2400-2500 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

|         |                  |                  |             |
|---------|------------------|------------------|-------------|
| ConvF X | 4.7 ± 8.9% (k=2) | Boundary effect: |             |
| ConvF Y | 4.7 ± 8.9% (k=2) | Alpha            | <b>0.99</b> |
| ConvF Z | 4.7 ± 8.9% (k=2) | Depth            | <b>1.81</b> |

Body                      2450 MHz                       $\epsilon_r = 52.7 \pm 5\%$                        $\sigma = 1.95 \pm 5\%$  mho/m

Valid for f=2400-2500 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C


|         |                  |                  |             |
|---------|------------------|------------------|-------------|
| ConvF X | 4.5 ± 8.9% (k=2) | Boundary effect: |             |
| ConvF Y | 4.5 ± 8.9% (k=2) | Alpha            | <b>1.01</b> |
| ConvF Z | 4.5 ± 8.9% (k=2) | Depth            | <b>1.74</b> |

ET3DV6 SN:1788

August 29, 2003

### Deviation from Isotropy in HSL

Error ( $\theta, \phi$ ),  $f = 900$  MHz

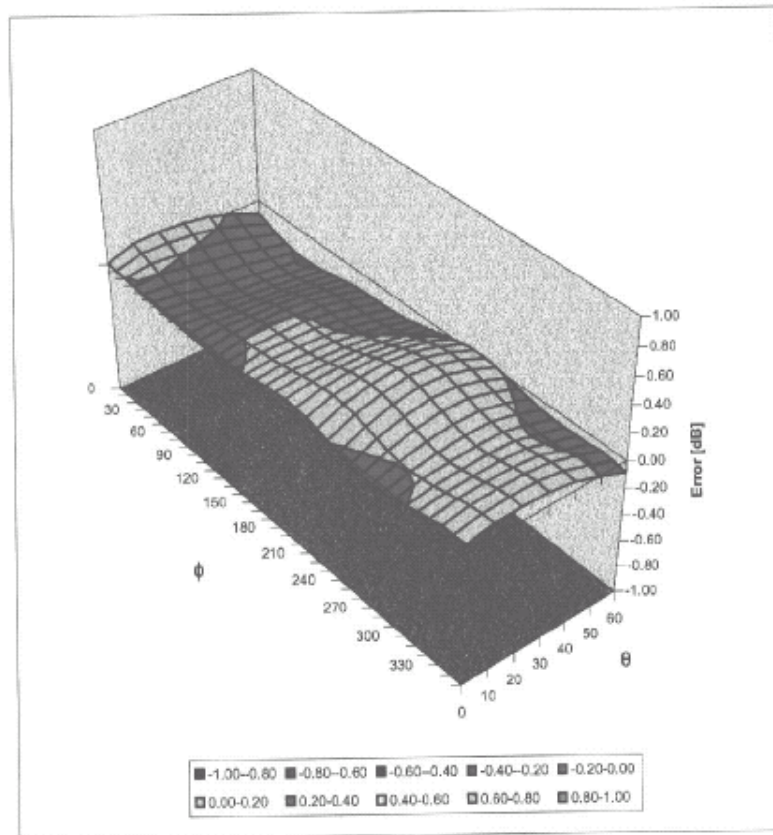

Client **Sproton Int. (Auden)**

## CALIBRATION CERTIFICATE

Object(s) **D835V2 - SN:499**

Calibration procedure(s) **QA CAL-05.v2  
Calibration procedure for dipole validation kits**

Calibration date: **February 12, 2004**



Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

| Model Type                | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration  |
|---------------------------|------------|---|------------------------|
| Power meter EPM E442      | GB37480704 | 6-Nov-03 (METAS, No. 252-0254)            | Nov-04                 |
| Power sensor HP 8481A     | US37292783 | 6-Nov-03 (METAS, No. 252-0254)            | Nov-04                 |
| Power sensor HP 8481A     | MY41092317 | 18-Oct-02 (Agilent, No. 20021018)         | Oct-04                 |
| RF generator R&S SML-03   | 100698     | 27-Mar-2002 (R&S, No. 20-92389)           | In house check: Mar-05 |
| Network Analyzer HP 8753E | US37390585 | 18-Oct-01 (SPEAG, in house check Nov-03)  | In house check: Oct 05 |

|                | Name           | Function            | Signature   |
|----------------|----------------|---------------------|---|
| Calibrated by: | Judith Mueller | Technician          |  |
| Approved by:   | Katja Pokovic  | Laboratory Director |  |

Date issued: February 18, 2004

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

# DASY

## Dipole Validation Kit

Type: D835V2

Serial: 499

Manufactured: July 10, 2003

Calibrated: February 12, 2004

## 1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **head simulating solution** of the following electrical parameters at 835 MHz:

|                        |                   |           |
|------------------------|-------------------|-----------|
| Relative Dielectricity | <b>42.1</b>       | $\pm 5\%$ |
| Conductivity           | <b>0.89 mho/m</b> | $\pm 5\%$ |

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.3 at 835 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was  $250 \text{ mW} \pm 3 \%$ . The results are normalized to 1W input power.

## 2. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over  $1 \text{ cm}^3$  (1 g) of tissue: **9.96 mW/g**  $\pm 16.8 \%$  (k=2)<sup>1</sup>

averaged over  $10 \text{ cm}^3$  (10 g) of tissue: **6.48 mW/g**  $\pm 16.2 \%$  (k=2)<sup>1</sup>

### 3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

|                      |                 |                                       |
|----------------------|-----------------|---------------------------------------|
| Electrical delay:    | <b>1.382 ns</b> | (one direction)                       |
| Transmission factor: | <b>0.985</b>    | (voltage transmission, one direction) |

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

|                                 |                                |
|---------------------------------|--------------------------------|
| Feedpoint impedance at 835 MHz: | $\text{Re}\{Z\} = 51.2 \Omega$ |
|                                 | $\text{Im}\{Z\} = -1.7 \Omega$ |
| Return Loss at 835 MHz          | <b>-33.9 dB</b>                |

### 4. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **body simulating solution** of the following electrical parameters at 835 MHz:

|                        |                   |           |
|------------------------|-------------------|-----------|
| Relative Dielectricity | <b>55.5</b>       | $\pm 5\%$ |
| Conductivity           | <b>0.99 mho/m</b> | $\pm 5\%$ |

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.13 at 835 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was 250 mW  $\pm 3\%$ . The results are normalized to 1W input