

SAR Data Report 02091901

Start : 19-Sep-02 09:38:29 am  
End : 19-Sep-02 09:43:50 am  
Code Version : 4.08  
Robot Version: 4.08

Product Data:

Type : Validation  
Frequency : 836.49 MHz  
Transmit Pwr : 0.250 W  
Antenna Type : Dipole  
Antenna Posn. : Validation

Measurement Data:

Phantom Name : SAM FLAT  
Phantom Type : Uniphantom  
Tissue Type : Brain  
Tissue Dielectric : 40.190  
Tissue Conductivity : 0.930  
Tissue Density : 1.000  
Robot Name : CRS

Probe Data:

Probe Name : PCT002  
Probe Type : E Fld Triangle  
Frequency : 835 MHz  
Tissue Type : Brain  
Calibrated Dielectric : 40.700  
Calibrated Conductivity : 0.890  
Calibrated Density : 1.000  
Probe Offset : 2.400 mm  
Conversion Factor : 5.800  
Probe Sensitivity : 3.597 3.474 3.049 mV/(mW/cm^2)  
Amplifier Gains : 20.00 20.00 20.00

Sample:

Rate: 6000 Samples/Sec  
Count: 100 Samples  
NIDAQ Gain: 5

Comments:

835 MHz Validation  
  
CF=1; Amb. Temp= 22.5 'C; Liq. Temp=22.1 'C

Area Scan - Max Peak SAR Value at x=3.0 y=-3.0 = 2.12 W/kg

Zoom Scan - Max Peak SAR Value at x=3.0 y=-4.0 z=0.0 = 3.61 W/kg


Max 1g SAR at x=4.0 y=-3.0 z=0.0 = 2.28 W/kg

Max 10g SAR at x=3.0 y=-2.0 z=0.0 = 1.41 W/kg

Validation Results at 0.25 W:

Peak Nominal = 3.5, Error: 2.39 %  
1g Nominal = 2.4, Error: -3.85 %  
10g Nominal = 1.6, Error: -8.90 %

SAR - Z Axis  
at Hotspot x:3.0 y:-4.0

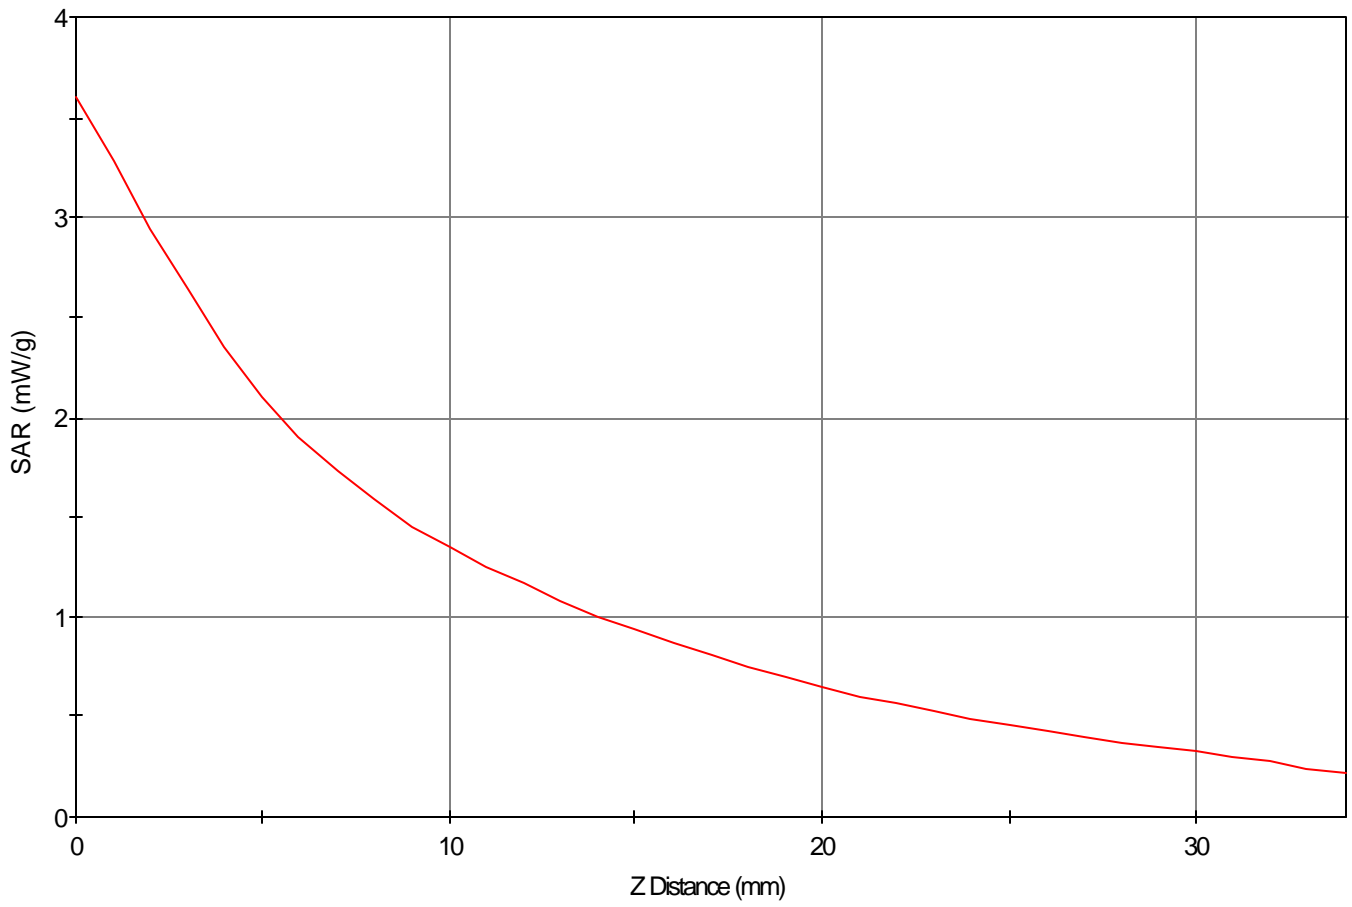

### 1g SAR Values

