

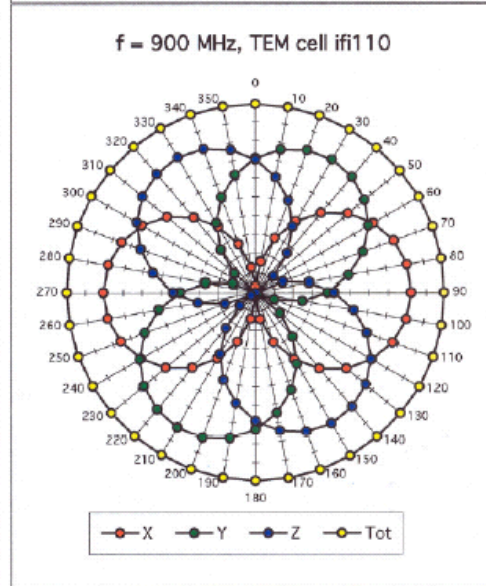
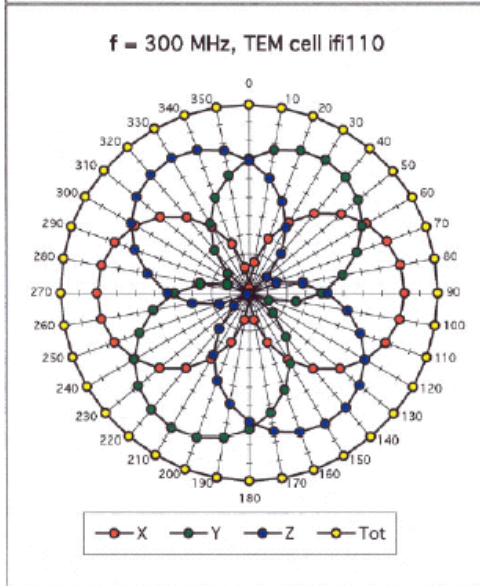


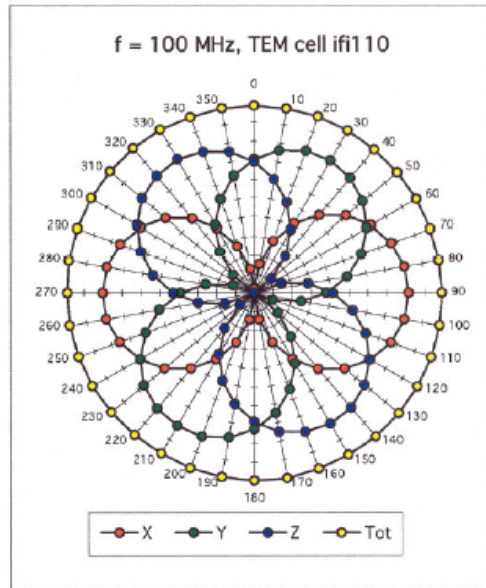

ET3DV6 SN:1788

August 29, 2003



Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$

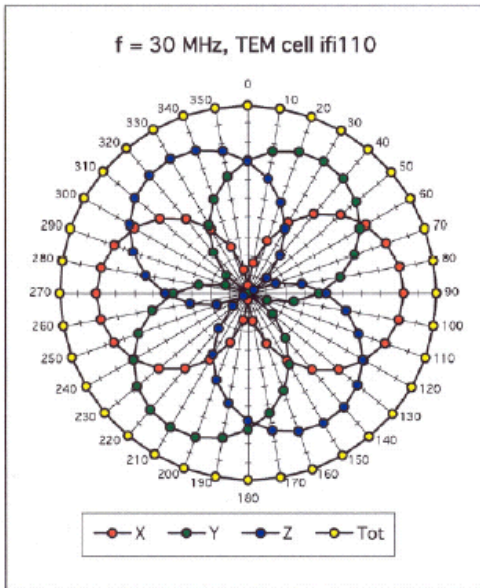




ET3DV6 SN:1788

August 29, 2003

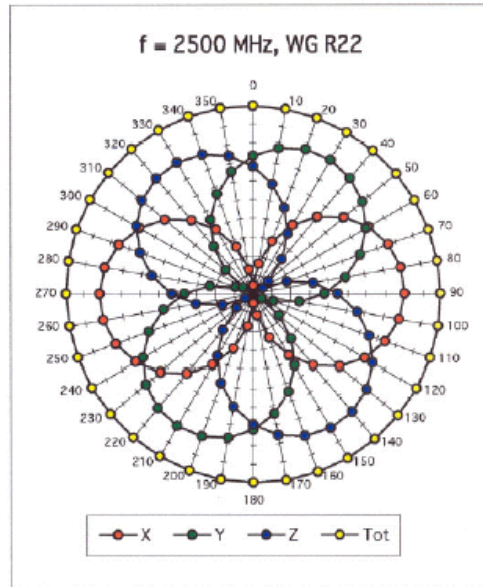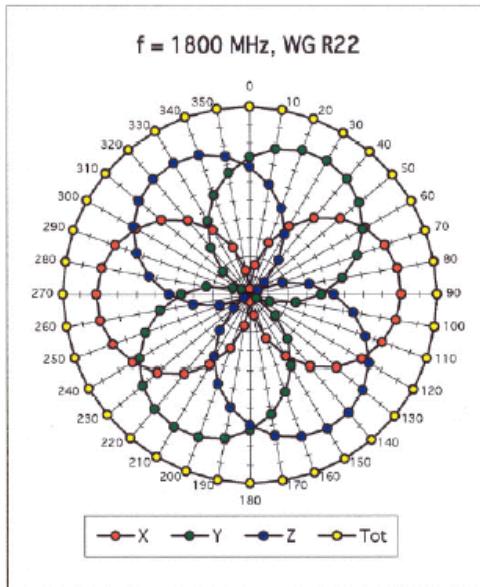

Isotropy Error ( $\phi$ ),  $\theta = 0^\circ$

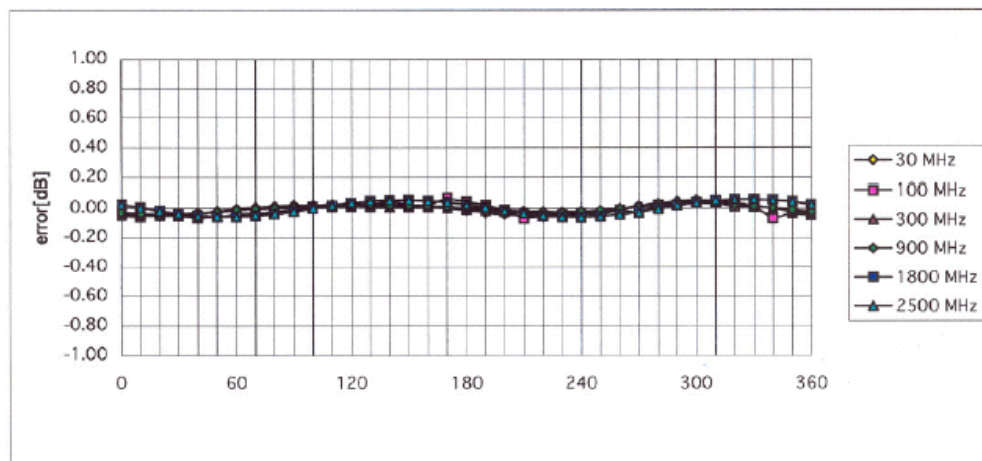




ET3DV6 SN:1788

August 29, 2003

### Frequency Response of E-Field

( TEM-Cell:ifi110, Waveguide R22)

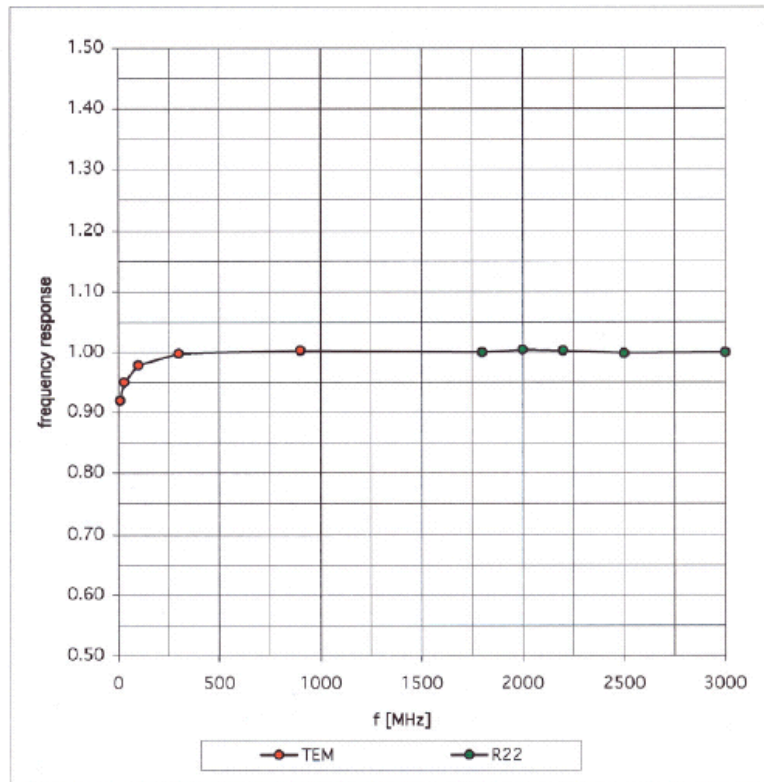





ET3DV6 SN:1788

August 29, 2003

### Dynamic Range f(SAR<sub>brain</sub>)

( Waveguide R22 )

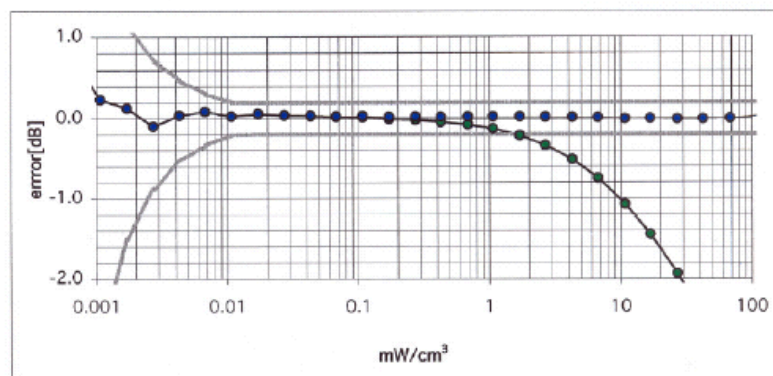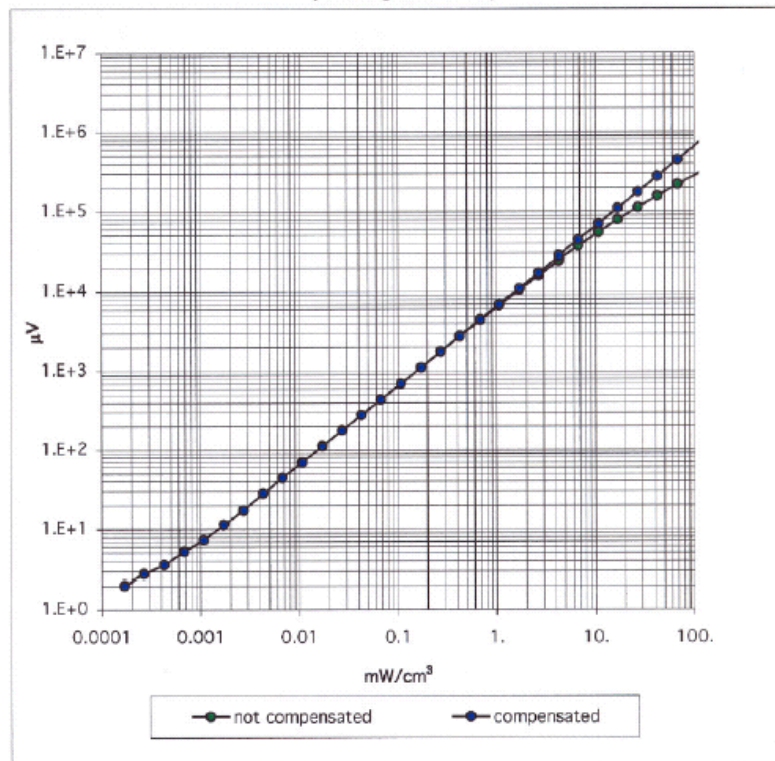






ET3DV6 SN:1788

August 29, 2003

### Conversion Factor Assessment

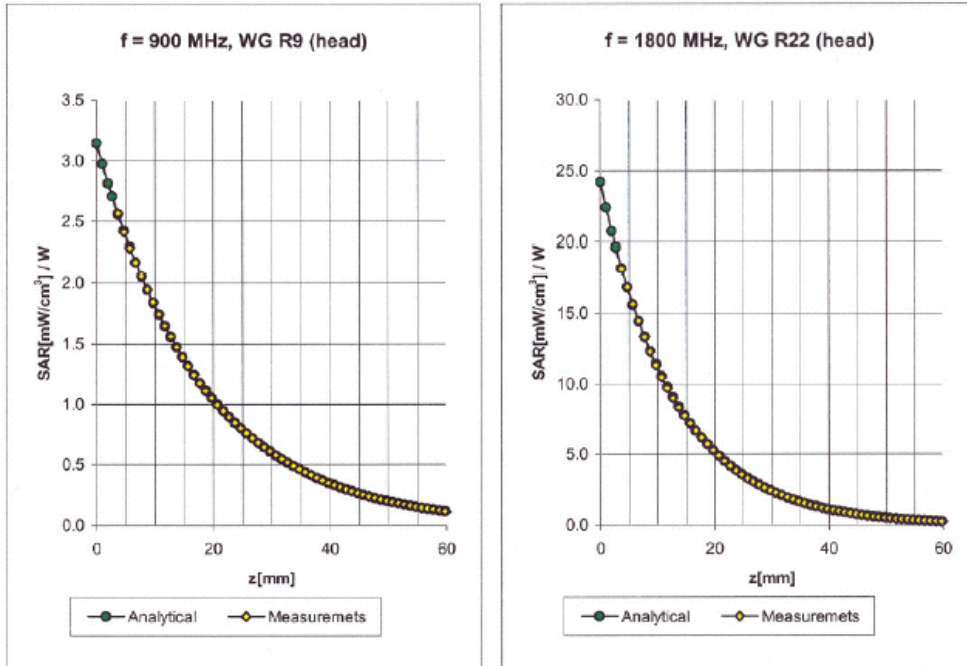

Head                      900 MHz                       $\epsilon_r = 41.5 \pm 5\%$                        $\sigma = 0.97 \pm 5\%$  mho/m

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	<b>6.6</b> $\pm 9.5\%$ (k=2)	Boundary effect:	
ConvF Y	<b>6.6</b> $\pm 9.5\%$ (k=2)	Alpha	<b>0.34</b>
ConvF Z	<b>6.6</b> $\pm 9.5\%$ (k=2)	Depth	<b>2.48</b>

Head                      1800 MHz                       $\epsilon_r = 40.0 \pm 5\%$                        $\sigma = 1.40 \pm 5\%$  mho/m

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X


ConvF X	<b>5.3</b> $\pm 9.5\%$ (k=2)	Boundary effect:	
ConvF Y	<b>5.3</b> $\pm 9.5\%$ (k=2)	Alpha	<b>0.43</b>
ConvF Z	<b>5.3</b> $\pm 9.5\%$ (k=2)	Depth	<b>2.80</b>



ET3DV6 SN:1788

August 29, 2003

### Conversion Factor Assessment

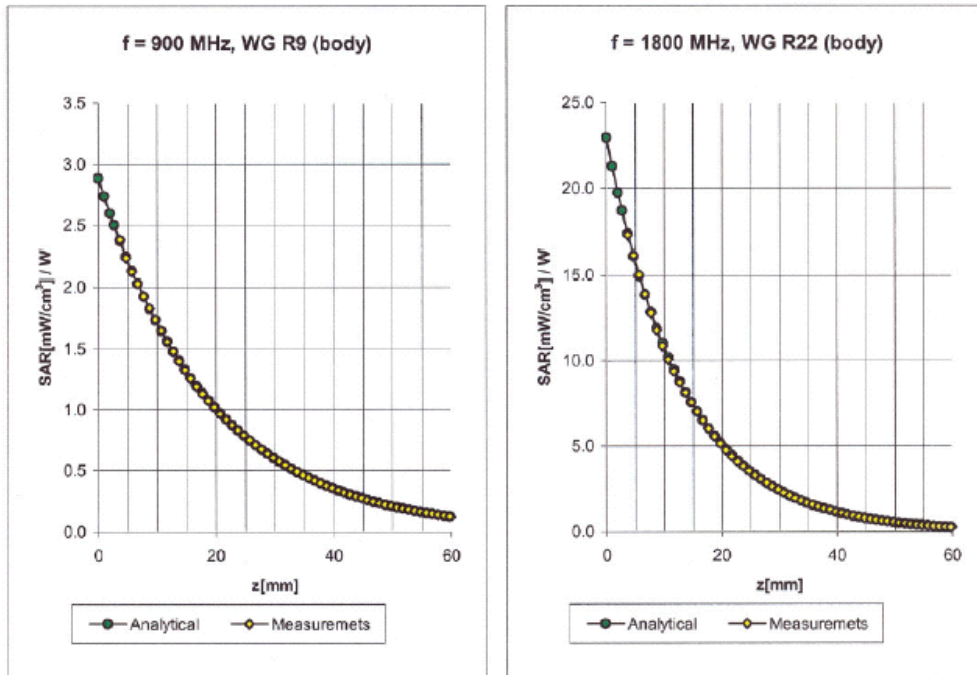

Body                      900 MHz                       $\epsilon_r = 55.0 \pm 5\%$                        $\sigma = 1.05 \pm 5\%$  mho/m

Valid for f=800-1000 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X	<b>6.5</b> $\pm 9.5\%$ (k=2)	Boundary effect:	
ConvF Y	<b>6.5</b> $\pm 9.5\%$ (k=2)	Alpha	<b>0.31</b>
ConvF Z	<b>6.5</b> $\pm 9.5\%$ (k=2)	Depth	<b>2.92</b>

Body                      1800 MHz                       $\epsilon_r = 53.3 \pm 5\%$                        $\sigma = 1.52 \pm 5\%$  mho/m

Valid for f=1710-1910 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C


ConvF X	<b>5.0</b> $\pm 9.5\%$ (k=2)	Boundary effect:	
ConvF Y	<b>5.0</b> $\pm 9.5\%$ (k=2)	Alpha	<b>0.51</b>
ConvF Z	<b>5.0</b> $\pm 9.5\%$ (k=2)	Depth	<b>2.78</b>



ET3DV6 SN:1788

August 29, 2003

### Conversion Factor Assessment

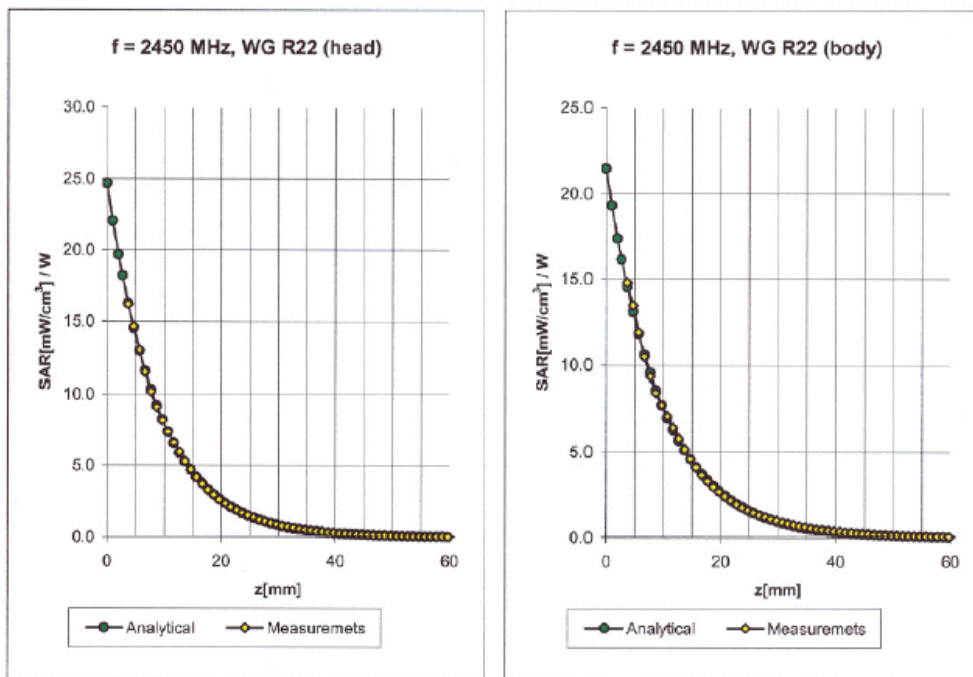

Head                      2450 MHz                       $\epsilon_r = 39.2 \pm 5\%$                        $\sigma = 1.80 \pm 5\%$  mho/m

Valid for f=2400-2500 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	4.7 ± 8.9% (k=2)	Boundary effect:	
ConvF Y	4.7 ± 8.9% (k=2)	Alpha	<b>0.99</b>
ConvF Z	4.7 ± 8.9% (k=2)	Depth	<b>1.81</b>

Body                      2450 MHz                       $\epsilon_r = 52.7 \pm 5\%$                        $\sigma = 1.95 \pm 5\%$  mho/m

Valid for f=2400-2500 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X	4.5 ± 8.9% (k=2)	Boundary effect:	
ConvF Y	4.5 ± 8.9% (k=2)	Alpha	<b>1.01</b>
ConvF Z	4.5 ± 8.9% (k=2)	Depth	<b>1.74</b>




ET3DV6 SN:1788

August 29, 2003

### Deviation from Isotropy in HSL

Error ( $\theta, \phi$ ),  $f = 900$  MHz

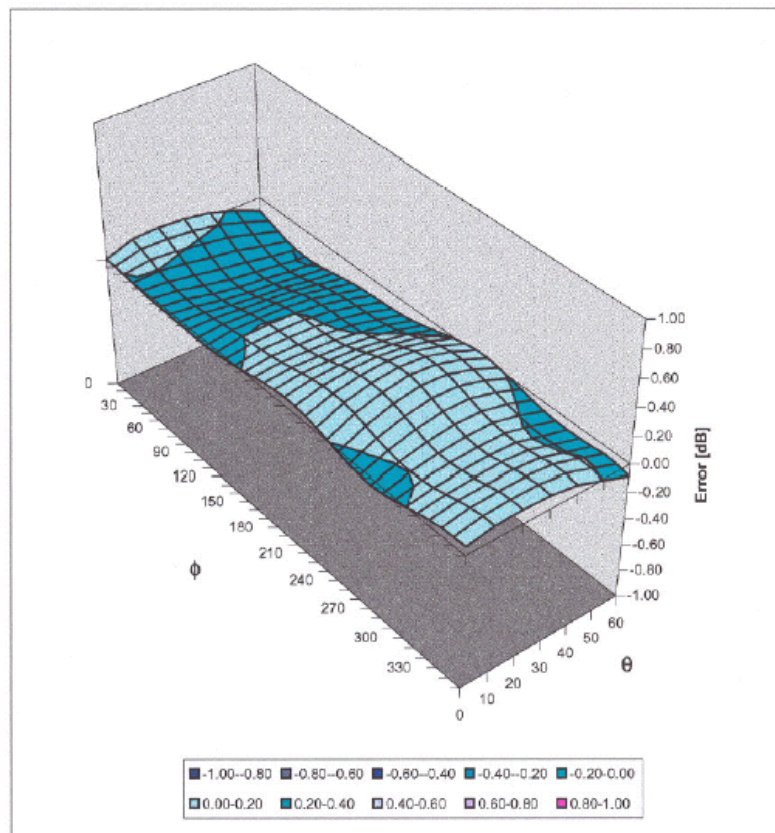





Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland

Client **Sporton (Auden)**

CALIBRATION CERTIFICATE			
Object(s)	DAE3 – SD 000 D03 AA – SN:577		
Calibration procedure(s)	QA CAL-06.v4 Calibration procedure for the data acquisition unit (DAE)		
Calibration date:	21.11.2003		
Condition of the calibrated item	In Tolerance (according to the specific calibration document)		
This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.			
All calibrations have been conducted in the closed laboratory facility environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.			
Calibration Equipment used (M&TE critical for calibration)			
Model Type	ID #	Cal Date	Scheduled Calibration
Fluke Process Calibrator Type 702	SN. 6295803	8-Sep-03	Sep-05
Calibrated by:	Name Philipp Storchenegger	Function Technician	Signature 
Approved by:	Name Fin Bomholt	Function R&D Director	Signature 
Date issued 21.11.2003			
This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.			



DAE3 SN: 577

DATE: 21.11.2003

**1. Cal Lab. Incoming Inspection & Pre Test**

<b>Modification Status</b>	Note Status here → → → →	BC
<b>Visual Inspection</b>	Note anomalies.....	None
	.....	.....
<b>Pre Test</b>	<b>Indication</b>	<b>Yes/No</b>
<b>Probe Touch</b>	Function	Yes
<b>Probe Collision</b>	Function	Yes
<b>Probe Touch&amp;Collision</b>	Function	Yes

**2. DC Voltage Measurement**

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1µV, full range = 400 mV  
 Low Range: 1LSB = 61nV, full range = 4 mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
<b>High Range</b>	404.434	403.889	404.352
<b>Low Range</b>	3.94303	3.94784	3.9501
<b>Connector Angle</b> to be used in DASY System	127 °		

High Range	Input	Reading in µV	% Error
<b>Channel X + Input</b>	200mV	200000.6	0.00
	20mV	20000.9	0.00
<b>Channel X - Input</b>	20mV	-19992.7	-0.04
<b>Channel Y + Input</b>	200mV	200000.6	0.00
	20mV	19999.1	0.00
<b>Channel Y - Input</b>	20mV	-19994.7	-0.03
<b>Channel Z + Input</b>	200mV	199999.8	0.00
	20mV	19998.1	-0.01
<b>Channel Z - Input</b>	20mV	-19999.2	0.00

Low Range	Input	Reading in µV	% Error
<b>Channel X + Input</b>	2mV	1999.94	0.00
	0.2mV	199.08	-0.46
<b>Channel X - Input</b>	0.2mV	-200.24	0.12
<b>Channel Y + Input</b>	2mV	1999.98	0.00
	0.2mV	199.50	-0.25
<b>Channel Y - Input</b>	0.2mV	-200.80	0.40
<b>Channel Z + Input</b>	2mV	1999.98	0.00
	0.2mV	199.11	-0.44
<b>Channel Z - Input</b>	0.2mV	-201.12	0.56



DAE3 SN: 577

DATE: 21.11.2003

**3. Common mode sensitivity**

DASY measurement parameters:

Auto Zero Time: 3 sec,

Measuring time: 3 sec

High/Low Range

in $\mu\text{V}$	Common mode Input Voltage	High Range Reading	Low Range Reading
Channel X	200mV	12.00	11.9
	- 200mV	-10.76	-12.44
Channel Y	200mV	-8.55	-8.51
	- 200mV	7.58	6.67
Channel Z	200mV	-0.86	-0.58
	- 200mV	-0.85	-0.77

**4. Channel separation**

DASY measurement parameters:

Auto Zero Time: 3 sec,

Measuring time: 3 sec

High Range

in $\mu\text{V}$	Input Voltage	Channel X	Channel Y	Channel Z
Channel X	200mV	-	1.96	0.28
Channel Y	200mV	0.66	-	3.59
Channel Z	200mV	-0.89	-0.11	-

**5.1 AD-Converter Values with Input Voltage set to 2.0 VDC**

in Zero Low	Low Range Max - Min	Max.	Min
Channel X	17	16137	16120
Channel Y	27	16767	16740
Channel Z	8	15103	15077

**5.2 AD-Converter Values with inputs shorted**

in LSB	Low Range	High Range
Channel X	16134	15955
Channel Y	16740	15960
Channel Z	15093	16252

**6. Input Offset Measurement**





DAE3 SN: 577

DATE: 21.11.2003

DASY measurement parameters:

Auto Zero Time: 3 sec, Measuring time: 3 sec  
Number of measurements: 100, Low Range

Input 10MΩ

in μV	Average	min. Offset	max. Offset	Std. Deviation
Channel X	-0.64	-1.84	0.71	0.49
Channel Y	-1.77	-3.93	0.94	0.58
Channel Z	-2.21	-3.14	-0.81	0.34

Input shorted

in μV	Average	min. Offset	max. Offset	Std. Deviation
Channel X	0.12	-1.34	1.45	0.69
Channel Y	-0.69	-1.39	0.30	0.26
Channel Z	-0.94	-1.58	-0.30	0.23

**7. Input Offset Current**

Nominal Input circuitry offset current on all channels: <25fA

**8. Input Resistance**

In MOhm	Calibrating	Measuring
Channel X	0.2000	197.1
Channel Y	0.1999	200.3
Channel Z	0.2001	198.3

**9. Low Battery Alarm Voltage**

in V	Alarm Level
Supply (+ Vcc)	7.58
Supply (- Vcc)	-7.65

**10. Power Consumption**

in mA	Switched off	Stand by	Transmitting
Supply (+ Vcc)	0.00	5.65	13.7
Supply (- Vcc)	-0.01	-7.69	-8.97