

APPENDIX C (DIPOLE VALIDATION)

Test Laboratory: HCT CO., LTD.
 Ambient Temperature 21.3 °C
 Test Date Jul. 17, 2012

DUT: HAC-Dipole 835 MHz; Type: D835V3; Serial: 1024

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1
 Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³
 Phantom section: E Dipole Section ; Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184


DASY4 Configuration:
 - Probe: ER3DV6 - SN2343; ConvF(1, 1, 1); Calibrated: 2012-05-22
 - Sensor-Surface: (Fix Surface)
 - Electronics: DAE3 Sn466; Calibrated: 2012-02-21
 - Phantom: HAC Test Arch; Type: SD HAC P01 BA

E Scan 10mm above CD 835 MHz/Hearing Aid Compatibility Test (41x361x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 164.6 V/m
 Probe Modulation Factor = 1.00
 Device Reference Point: 0.000, 0.000, 354.7 mm
 Reference Value = 129.2 V/m; Power Drift = 0.014 dB
Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m

Grid 1 154.8 M4	Grid 2 164.6 M4	Grid 3 162.1 M4
Grid 4 77.5 M4	Grid 5 85.1 M4	Grid 6 84.7 M4
Grid 7 148.5 M4	Grid 8 162.7 M4	Grid 9 161.7 M4

Cursor:
 Total = 164.6 V/m
 E Category: M4
 Location: -1, -78.5, 365.8 mm

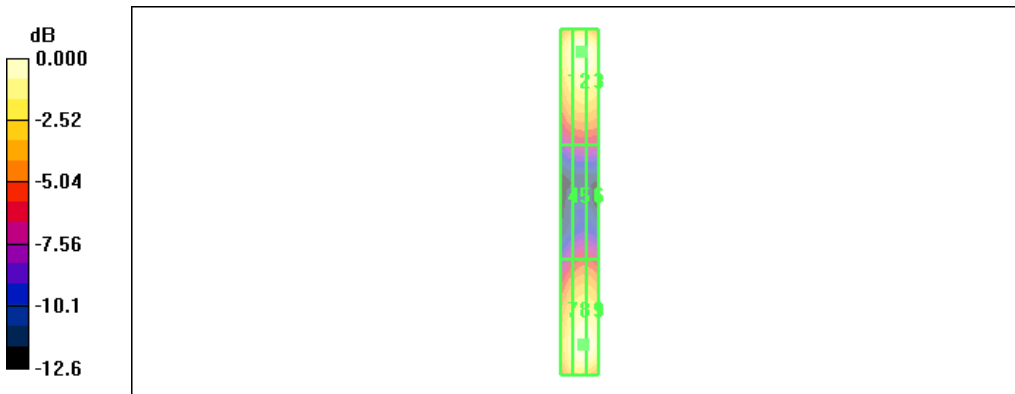

0 dB = 164.6V/m

Test Laboratory: HCT CO., LTD.

Ambient Temperature 21.3 °C

Test Date Jul. 17, 2012

DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: 1019

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³

Phantom section: E Dipole Section ; Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

DASY4 Configuration:

- Probe: ER3DV6 - SN2343; ConvF(1, 1, 1); Calibrated: 2012-05-22
- Sensor-Surface: (Fix Surface)
- Electronics: DAE3 Sn466; Calibrated: 2012-02-21
- Phantom: HAC Test Arch; Type: SD HAC P01 BA

E Scan 10mm above CD 1880 MHz/Hearing Aid Compatibility Test (41x181x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 143.7 V/m

Probe Modulation Factor = 1.00

Device Reference Point: 0.000, 0.000, 354.7 mm

Reference Value = 169.4 V/m; Power Drift = 0.014 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak E-field in V/m


Grid 1	Grid 2	Grid 3
132.7 M2	140.8 M2	138.9 M2
Grid 4	Grid 5	Grid 6
89.0 M3	96.9 M3	96.8 M3
Grid 7	Grid 8	Grid 9
131.4 M2	143.7 M2	142.9 M2

Cursor:

Total = 143.7 V/m

E Category: M2

Location: -2, 33.5, 365.8 mm

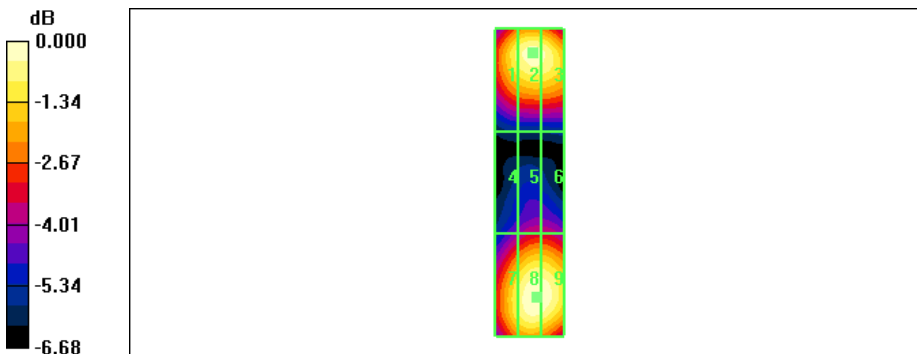

0 dB = 143.7V/m

Test Laboratory: HCT CO., LTD.
 Ambient Temperature: 21.3 °C
 Test Date: Jul. 17, 2012

DUT: HAC–Dipole 835 MHz; Type: D835V3; Serial:1024

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1
 Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom section: H Dipole Section ; Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

- DASY4 Configuration:
- Probe: H3DV6 – SN6101; ; Calibrated: 2012-05-22
 - Sensor–Surface: (Fix Surface)
 - Electronics: DAE3 Sn466; Calibrated: 2012-02-21
 - Phantom: HAC Test Arch; Type: SD HAC P01 BA


H Scan 10mm above CD 835 MHz/Hearing Aid Compatibility Test (41x361x1): Measurement grid: dx=5mm, dy=5mm
 Maximum value of peak Total field = 0.451 A/m
 Probe Modulation Factor = 1.00
 Device Reference Point: 0.000, 0.000, 354.7 mm
 Reference Value = 0.562 A/m; Power Drift = -0.015 dB
Hearing Aid Near–Field Category: M4 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.359 M4	0.388 M4	0.381 M4
Grid 4	Grid 5	Grid 6
0.412 M4	0.451 M4	0.444 M4
Grid 7	Grid 8	Grid 9
0.368 M4	0.407 M4	0.400 M4

Cursor:

Total = 0.451 A/m
 H Category: M4
 Location: -1.5, 2, 366.6 mm

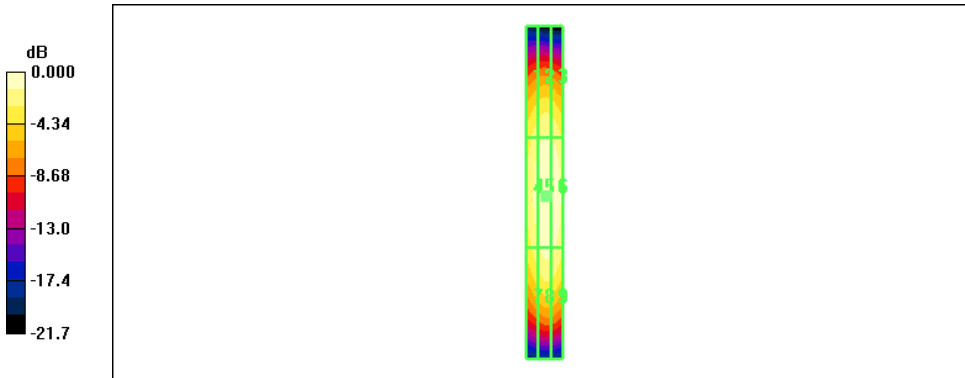

0 dB = 0.451 A/m

Test Laboratory: HCT CO., LTD.
 Ambient Temperature 21.3 °C
 Test Date Jul. 17, 2012

DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: 1019

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1
 Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1$ kg/m³
 Phantom section: H Dipole Section ; Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

DASY4 Configuration:
 - Probe: H3DV6 - SN6101; ; Calibrated: 2012-05-22
 - Sensor-Surface: (Fix Surface)
 - Electronics: DAE3 Sn466; Calibrated: 2012-02-21
 - Phantom: HAC Test Arch; Type: SD HAC P01 BA

H Scan 10mm above CD 1880 MHz/Hearing Aid Compatibility Test (41x181x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.475 A/m
 Probe Modulation Factor = 1.00
 Device Reference Point: 0.000, 0.000, 354.7 mm
 Reference Value = 0.566 A/m; Power Drift = 0.040 dB


Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.392 M2	0.423 M2	0.417 M2
Grid 4	Grid 5	Grid 6
0.442 M2	0.475 M2	0.470 M2
Grid 7	Grid 8	Grid 9
0.409 M2	0.442 M2	0.437 M2

Cursor:

Total = 0.475 A/m
 H Category: M2
 Location: -1.5, 1.5, 366.6 mm

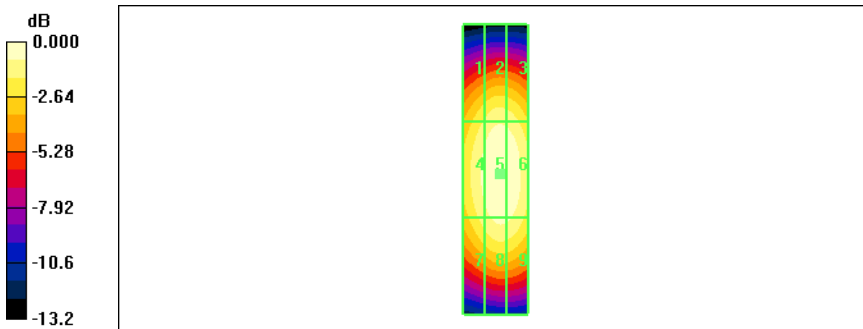

0 dB = 0.475A/m