

Date(s) of Evaluation Jan 28-30, 2013

01312014K66-1264 Test Report Issue Date Description of Test(s) Feb 5, 2014 Specific Absorption Rate

Test Report Serial No.

Test Report Revision No. Rev. 1.1 (Revised Issue) RF Exposure Category

ilac-MRA



Test Lab Certificate No. 2470.01 Gen. Pop. / Uncontrolled

## **APPENDIX D - SAR TEST SETUP & DUT PHOTOGRAPHS**

Applicant:	Y	aesu Musen Co., Ltd	FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):	FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro			oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 38 of 52



Date(s) of Evaluation
Jan 28-30, 2013

<u>Test Report Serial No.</u> 01312014K66-1264

Description of Test(s)

Rev. 1.1 (Revised Issue)

RF Exposure Category
Gen. Pop. / Uncontrolled

Test Report Revision No.





Set-Up - Body Configuration

Applicant:	ant: Yaesu Musen Co., Ltd		FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):		FTA-550, FTA-750	DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be reproduced		oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 39 of 52	




Date(s) of Evaluation
Jan 28-30, 2013

Test Report Serial No. 01312014K66-1264

RF Exposure Category Description of Test(s) Gen. Pop. / Uncontrolled Specific Absorption Rate





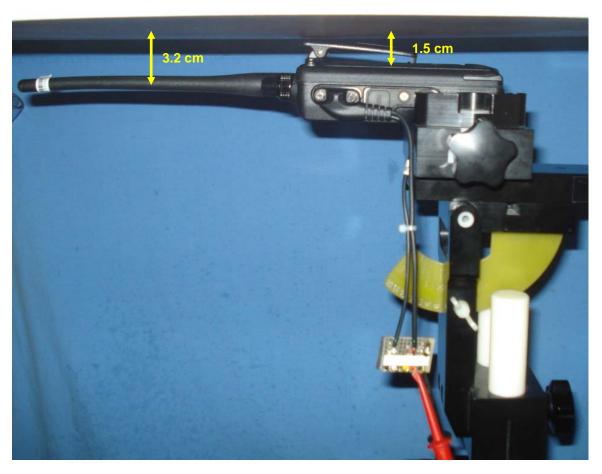

**DUT** in Body Configuration

Applicant:	Y	aesu Musen Co., Ltd	FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):	FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro			oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 40 of 52



Date(s) of Evaluation
Jan 28-30, 2013

Test Report Issue Date

Test Report Serial No. 01312014K66-1264


Rev. 1.1 (Revised Issue) Description of Test(s) RF Exposure Category

Test Report Revision No.

ilac-MR/



Feb 5, 2014 Specific Absorption Rate Gen. Pop. / Uncontrolled

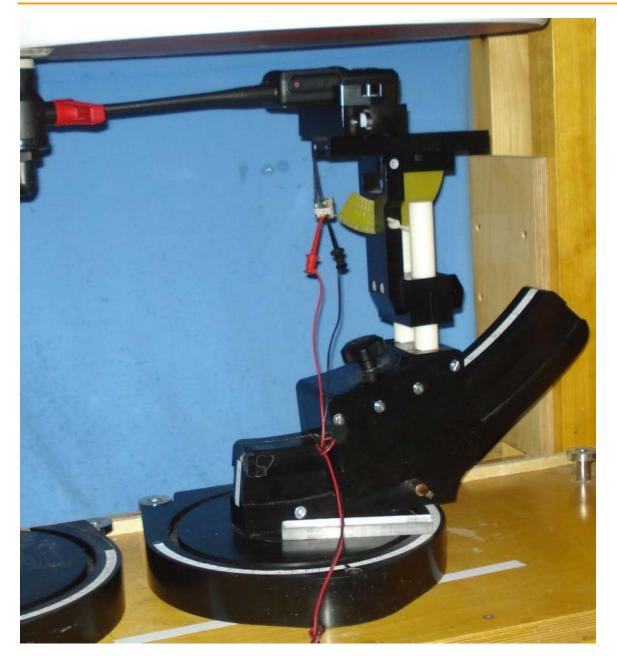

Set-Up - Face Configuration

Applicant:	Y	aesu Musen Co., Ltd	FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):		FTA-550, FTA-750	DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro			oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 41 of 52



Date(s) of Evaluation
Jan 28-30, 2013

<u>Test Report Serial No.</u> 01312014K66-1264

Description of Test(s)


Specific Absorption Rate

RF Exposure Category
Gen. Pop. / Uncontrolled

Test Report Revision No.

Rev. 1.1 (Revised Issue)



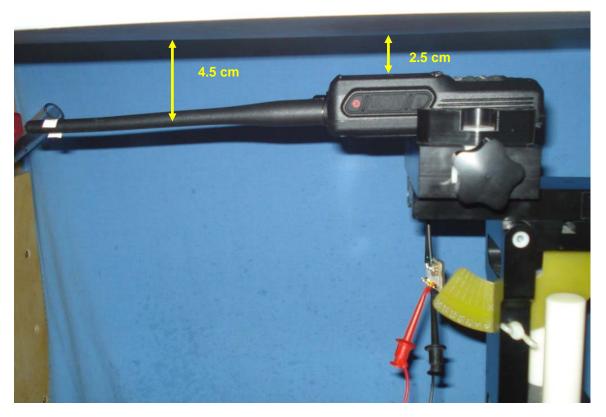

**DUT** in Face Configuration

Applicant:	nt: Yaesu Musen Co., Ltd		FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):		FTA-550, FTA-750	DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro			oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 42 of 52



Date(s) of Evaluation
Jan 28-30, 2013

<u>Test Report Serial No.</u> 01312014K66-1264

Description of Test(s)
Specific Absorption Rate

Test Report Revision No.
Rev. 1.1 (Revised Issue)

RF Exposure Category
Gen. Pop. / Uncontrolled





DUT in Face Configuration Showing Audio Cables

Applicant:	Y	aesu Musen Co., Ltd	FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):	FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro			oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 43 of 52



Date(s) of Evaluation
Jan 28-30, 2013
Test Report Issue Date

Feb 5, 2014

Test Report Serial No.
01312014K66-1264

Description of Test(s)
Specific Absorption Rate

Test Report Revision No.
Rev. 1.1 (Revised Issue)
RF Exposure Category
Gen. Pop. / Uncontrolled



## **DUT PHOTOGRAPHS**

Applicant:	Y	aesu Musen Co., Ltd	FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):	FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro-			oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 44 of 52




Date(s) of Evaluation						
Jan 28-30, 2013						
To at Daniel Laure Date						

Description of Test(s) Feb 5, 2014 Specific Absorption Rate

Test Report Serial No.

01312014K66-1264

Test Report Revision No. Rev. 1.1 (Revised Issue) RF Exposure Category





FTA-750 Front View

Applicant:	Applicant: Yaesu Musen Co., Ltd		FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):	Model(s): FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro-		oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 45 of 52	



Date(s) of Evaluation
Jan 28-30, 2013

<u>Test Report Serial No.</u> 01312014K66-1264

Description of Test(s)
Specific Absorption Rate

Test Report Revision No. Rev. 1.1 (Revised Issue)

RF Exposure Category
Gen. Pop. / Uncontrolled





FTA-750 Back View

Applicant:	Applicant: Yaesu Musen Co., Ltd		FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):	Model(s): FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio 118-137 MI		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro		oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 46 of 52	



Date(s) of Evaluation							
Jan 28-30, 2013							

<u>Test Report Serial No.</u> 01312014K66-1264

Description of Test(s)

Specific Absorption Rate

Rev. 1.1 (Revised Issue)

RF Exposure Category

Gen. Pop. / Uncontrolled

Test Report Revision No.





FTA-750 Back View w/o Battery

Applicant: Yaesu Musen Co., Ltd		FCC ID:	K6650013X20	IC:	511B-50013X20		
Model(s):	Model(s): FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio 11		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro-		oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 47 of 52	



Date(s) of Evaluation
Jan 28-30, 2013

<u>Test Report Serial No.</u> 01312014K66-1264

Description of Test(s)

Specific Absorption Rate

Rev. 1.1 (Revised Issue)

RF Exposure Category
Gen. Pop. / Uncontrolled

Test Report Revision No.





FTA-750 Top View



FTA-750 Bottom View

Applicant: Yaesu Musen Co., Ltd		FCC ID:	K6650013X20	IC:	511B-50013X20		
Model(s):	Model(s): FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro-		oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 48 of 52	



Date(s) of Evaluation
Jan 28-30, 2013
Test Report Issue Date

Feb 5, 2014

01312014K66-1264

Description of Test(s)

Specific Absorption Rate

Test Report Serial No.

Test Report Revision No.
Rev. 1.1 (Revised Issue)

RF Exposure Category
Gen. Pop. / Uncontrolled



## **APPENDIX E - DIPOLE CALIBRATION**

Applicant:	Applicant: Yaesu Musen Co., Ltd		FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):	Model(s): FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be repro		oduced in whole or	in part without the prior	written pern	nission of Celltech Labs Inc.	Page 49 of 52	

## Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S wiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Celltech

Certificate No: D300V3-1009\_Apr12

Accreditation No.: SCS 108

## CALIBRATION CERTIFICATE

Object D300V3 - SN: 1009

Calibration procedure(s) QA CAL-15.v6

Calibration procedure for dipole validation kits below 700 MHz

Calibration date: April 17, 2012

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

1	1		
Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	29-Mar-12 (No. 217-01508)	Apr-13
Power sensor E4412A	MY41498087	29-Mar-12 (No. 217-01508)	Apr-13
Reference 3 dB Attenuator	SN: S5054 (3c)	27-Mar-12 (No. 217-01531)	Apr-13
Reference 20 dB Attenuator	SN: S5086 (20b)	27-Mar-12 (No. 217-01529)	Apr-13
Type-N mismatch combination	SN: 5047.2 / 06327	27-Mar-12 (No. 217-01533)	Apr-13
Reference Probe ET3DV6	SN: 1507	30-Dec-11 (No. ET3-1507_Dec11)	Dec-12
DAE4	SN: 900	11-Apr-12 (No. DAE4-900_Apr12)	Apr-13
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-11)	In house check: Oct-12
	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	4 / /
			1
Approved by:	Katja Pokovic	Technical Manager	mi.
			106 hige

Issued: April 27, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D300V3-1009\_Apr12

# Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

## **Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### **Additional Documentation:**

d) DASY4/5 System Handbook

#### **Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D300V3-1009\_Apr12 Page 2 of 6

## **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.1	
Extrapolation	Advanced Extrapolation		
Phantom	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm	
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dx, $dy$ , $dz = 5 mm$		
Frequency	300 MHz ± 1 MHz		

Head TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	45.3	0.87 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	44.9 ± 6 %	0.89 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

## **SAR** result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	398 mW input power	1.17 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	2.88 mW /g ± 18.1 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	398 mW input power	0.770 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	1.90 mW /g ± 17.6 % (k=2)

Certificate No: D300V3-1009\_Apr12 Page 3 of 6

#### **Appendix**

#### **Antenna Parameters with Head TSL**

Impedance, transformed to feed point	57.8 Ω - 2.9 jΩ
Return Loss	- 22.2 dB

## **General Antenna Parameters and Design**

· · · · · · · · · · · · · · · · · · ·	
Electrical Delay (one direction)	1.748 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	February 26, 2009

Certificate No: D300V3-1009\_Apr12 Page 4 of 6

#### **DASY5 Validation Report for Head TSL**

Date: 17.04.2012

Test Laboratory: SPEAG

#### DUT: Dipole 300 MHz; Type: D300V3; Serial: D300V3 - SN: 1009

Communication System: CW; Frequency: 300 MHz

Medium parameters used: f = 300 MHz;  $\sigma = 0.89 \text{ mho/m}$ ;  $\varepsilon_r = 44.9$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

## DASY52 Configuration:

• Probe: ET3DV6 - SN1507; ConvF(6.59, 6.59, 6.59); Calibrated: 30.12.2011;

Sensor-Surface: 4mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn900; Calibrated: 11.04.2012

Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1003

• DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

## Dipole Calibration for Head Tissue/d=15mm, Pin=398mW/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 37.838 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 1.974 mW/g

SAR(1 g) = 1.17 mW/g; SAR(10 g) = 0.770 mW/g


Maximum value of SAR (measured) = 1.24 mW/g

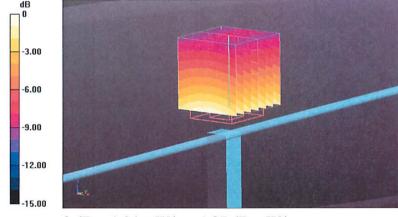

0 dB = 1.24 mW/g = 1.87 dB mW/g

Certificate No: D300V3-1009\_Apr12

## Impedance Measurement Plot for Head TSL

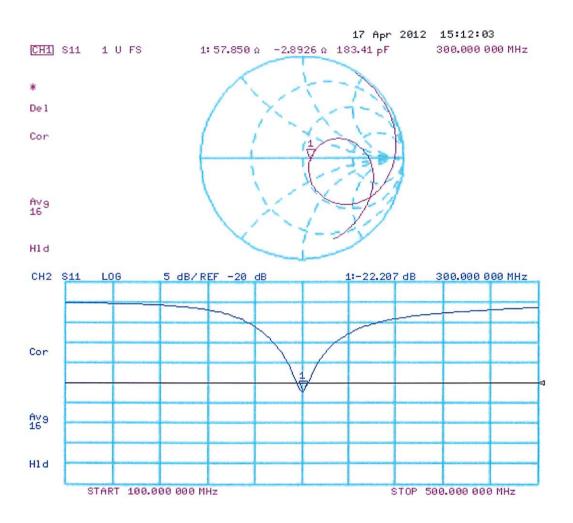



#### <u>Date:</u> May 16, 2013

Revision No. Rev. 1.0



#### **450 MHz Dipole Extended Calibration**

Dipole: D300V3
Serial Number: 1009

Last Calibrated: Apr. 27, 2012 (Head)
Jan. 8, 2013 (Body)

Antenna Parameters with Head TSL						
Impedance Real (ohms)  Deviation from cal Impedance Imaginary (ohms)  Deviation from cal (dB)  Return Loss Deviation from Cal						
Last Calibration	57.8	-	-2.9	-	-22.2	-
Extended Cal May 16, 2013	54.0	3.8	-7.5	4.6	-21.8	1.8%

Antenna Parameters with Body TSL						
	Impedance Real (ohms)	Deviation from cal (ohms)	Impedance Imaginary (ohms)	Deviation from cal (ohms)	Return Loss (dB)	Deviation from Cal (%)
Last Calibration	57.1	-	-5.9	-	-21.3	-

## Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client Celltech

Accreditation No.: SCS 108

Certificate No: D300V3-1009 Jan13

## **CALIBRATION CERTIFICATE**

Object D300V3 - SN: 1009

Calibration procedure(s) QA CAL-15.v7

Calibration procedure for dipole validation kits below 700 MHz

Calibration date: January 08, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	29-Mar-12 (No. 217-01508)	Apr-13
Power sensor E4412A	MY41498087	29-Mar-12 (No. 217-01508)	Apr-13
Reference 3 dB Attenuator	SN: S5054 (3c)	27-Mar-12 (No. 217-01531)	Apr-13
Reference 20 dB Attenuator	SN: S5086 (20b)	27-Mar-12 (No. 217-01529)	Apr-13
Type-N mismatch combination	SN: 5047.3 / 06327	27-Mar-12 (No. 217-01533)	Apr-13
Reference Probe ET3DV6	SN: 1507	28-Dec-12 (No. ET3-1507_Dec12)	Dec-13
DAE4	SN: 654	18-Apr-12 (No. DAE4-654_Apr12)	Apr-13
	33		
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-12)	In house check: Oct-13
	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	_7 , 1
Approved by:	Katja Pokovic	Technical Manager	
			Do offer

Issued: January 8, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D300V3-1009\_Jan13

## **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





C

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF

N/A

sensitivity in TSL / NORM x,y,z not applicable or not measured

## Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### **Additional Documentation:**

d) DASY4/5 System Handbook

#### **Methods Applied and Interpretation of Parameters:**

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D300V3-1009\_Jan13 Page 2 of 6

## **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.4
Extrapolation	Advanced Extrapolation	
Phantom	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, $dy$ , $dz = 5 mm$	
Frequency	300 MHz ± 1 MHz	

## **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	58.2	0.92 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	57.6 ± 6 %	0.91 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

## **SAR result with Body TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	0.717 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	2.89 W/kg ± 18.1 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	0.483 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	1.94 W/kg ± 17.6 % (k=2)

Certificate No: D300V3-1009\_Jan13 Page 3 of 6

#### **Appendix**

## **Antenna Parameters with Body TSL**

Impedance, transformed to feed point	57.1 Ω - 5.9 jΩ
Return Loss	- 21.3 dB

## **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.748 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	February 26, 2009

Certificate No: D300V3-1009\_Jan13 Page 4 of 6

## **DASY5 Validation Report for Body TSL**

Date: 08.01.2013

Test Laboratory: SPEAG, Zürich, Switzerland

DUT: Dipole 300 MHz; Type: D300V3; Serial: D300V3 - SN: 1009

Communication System: CW; Frequency: 300 MHz

Medium parameters used: f = 300 MHz;  $\sigma = 0.91 \text{ S/m}$ ;  $\varepsilon_r = 57.6$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY52 Configuration:

• Probe: ET3DV6 - SN1507; ConvF(7.08, 7.08, 7.08); Calibrated: 28.12.2012;

• Sensor-Surface: 4mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn654; Calibrated: 18.04.2012

Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1003

DASY52 52.8.4(1052); SEMCAD X 14.6.8(7028)

## Dipole Calibration for Body Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 29.820 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 1.11 W/kg

SAR(1 g) = 0.717 W/kg; SAR(10 g) = 0.483 W/kg


Maximum value of SAR (measured) = 0.763 W/kg

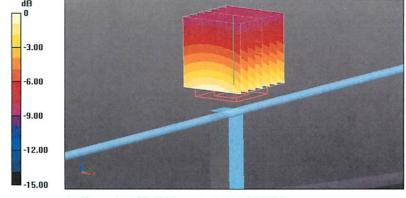

0 dB = 0.763 W/kg = -1.17 dBW/kg

Certificate No: D300V3-1009\_Jan13 Page 5 of 6

## Impedance Measurement Plot for Body TSL

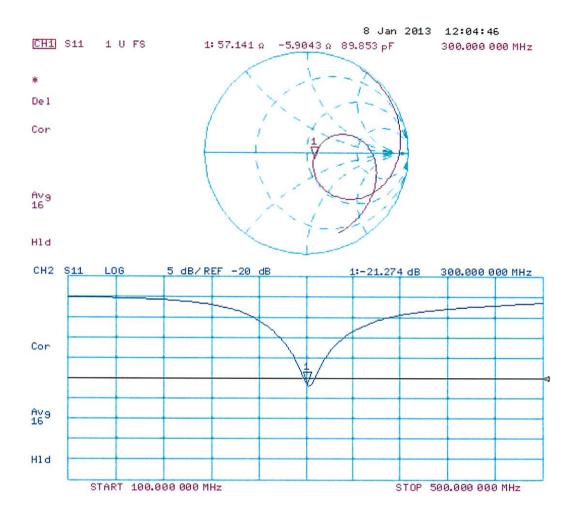



Date(s) of Evaluation
Jan 28-30, 2013
Test Report Issue Date

Feb 5, 2014

01312014K66-1264

Description of Test(s)

Specific Absorption Rate

Test Report Serial No.

Test Report Revision No.
Rev. 1.1 (Revised Issue)

RF Exposure Category
Gen. Pop. / Uncontrolled



## **APPENDIX F - PROBE CALIBRATION**

Applicant:	Yaesu Musen Co., Ltd		FCC ID:	K6650013X20 IC:		511B-50013X20	
Model(s):	FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech L	abs Inc.	This document is not to be reproduced in whole or in part without the prior written permission of Celltech Labs Inc.				Page 50 of 52	

#### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Celltech

Certificate No: ET3-1590\_Apr13

S

C

S

Accreditation No.: SCS 108

## **CALIBRATION CERTIFICATE**

Object ET3DV6 - SN:1590

Calibration procedure(s) QA CAL-01.v8, QA CAL-12.v7, QA CAL-23.v4, QA CAL-25.v4

Calibration procedure for dosimetric E-field probes

Calibration date: April 24, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	04-Apr-13 (No. 217-01733)	Apr-14
Power sensor E4412A	MY41498087	04-Apr-13 (No. 217-01733)	Apr-14
Reference 3 dB Attenuator	SN: S5054 (3c)	04-Apr-13 (No. 217-01737)	Apr-14
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-13 (No. 217-01735)	Apr-14
Reference 30 dB Attenuator	SN: S5129 (30b)	04-Apr-13 (No. 217-01738)	Apr-14
Reference Probe ES3DV2	SN: 3013	28-Dec-12 (No. ES3-3013_Dec12)	Dec-13
DAE4	SN: 660	31-Jan-13 (No. DAE4-660_Jan13)	Jan-14
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-15
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-12)	In house check: Oct-13

Name Function Signature
Calibrated by: Claudio Leubler Laboratory Technician

Approved by: Katja Pokovic Technical Manager

Issued: April 27, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## **Calibration Laboratory of**

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid NORMx,y,z sensitivity in free space

ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty\_cycle) of the RF signal modulation dependent linearization parameters

Polarization  $\varphi$   $\varphi$  rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center).

i.e., 9 = 0 is normal to probe axis

#### Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### **Methods Applied and Interpretation of Parameters:**

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
   NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

ET3DV6 - SN:1590

# Probe ET3DV6

SN:1590

Calibrated:

Manufactured: March 19, 2001 April 24, 2013

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m) <sup>2</sup> ) <sup>A</sup>	1.73	1.85	1.61	± 10.1 %
DCP (mV) <sup>B</sup>	94.7	99.4	88.0	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc <sup>±</sup> (k=2)
0	CW	Х	0.0	0.0	1.0	0.00	186.7	±2.7 %
		Υ	0.0	0.0	1.0		151.0	
		Z	0.0	0.0	1.0		171.2	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

A The uncertainties of NormX,Y,Z do not affect the E2-field uncertainty inside TSL (see Pages 5 and 6).

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the

## Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
450	43.5	0.87	7.53	7.53	7.53	0.21	2.23	± 13.4 %
750	41.9	0.89	7.24	7.24	7.24	0.25	3.00	± 12.0 %
835	41.5	0.90	6.84	6.84	6.84	0.26	3.00	± 12.0 %
900	41.5	0.97	6.68	6.68	6.68	0.28	3.00	± 12.0 %

<sup>&</sup>lt;sup>C</sup> Frequency validity of  $\pm$  100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to  $\pm$  50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

F At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to

At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## Calibration Parameter Determined in Body Tissue Simulating Media


			_					
f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
450	56.7	0.94	7.98	7.98	7.98	0.13	2.14	± 13.4 %
750	55.5	0.96	6.84	6.84	6.84	0.31	2.49	± 12.0 %
835	55.2	0.97	6.67	6.67	6.67	0.29	2.67	± 12.0 %
900	55.0	1.05	6.63	6.63	6.63	0.26	3.00	± 12.0 %

<sup>&</sup>lt;sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

FAt frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if fluid compensation formula is applied to

At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to  $\pm$  10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to  $\pm$  5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

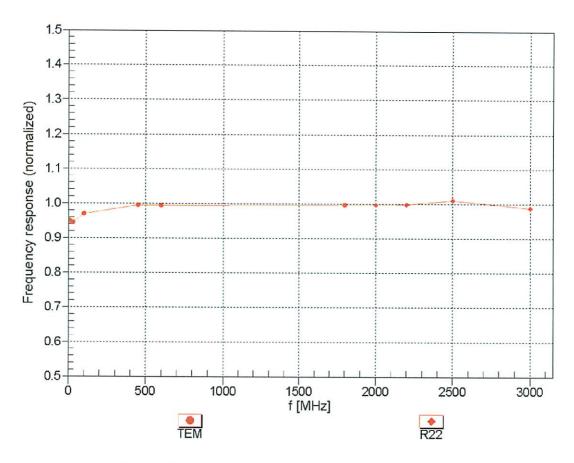



Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


# Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$



f=1800 MHz,R22

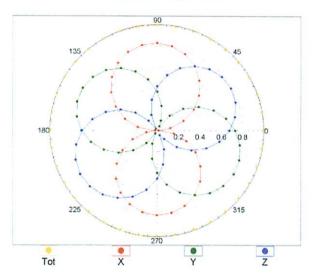





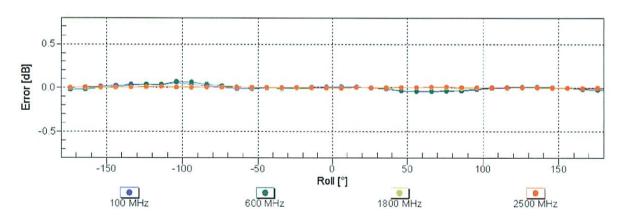

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


## Dynamic Range f(SAR<sub>head</sub>) (TEM cell , f = 900 MHz)

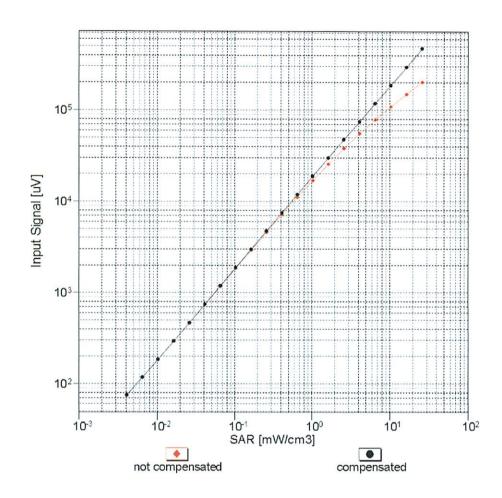

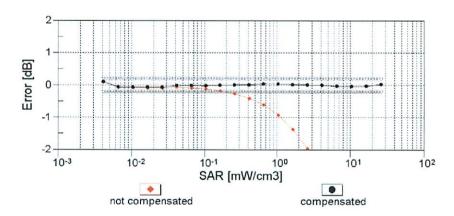


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

## **Conversion Factor Assessment**

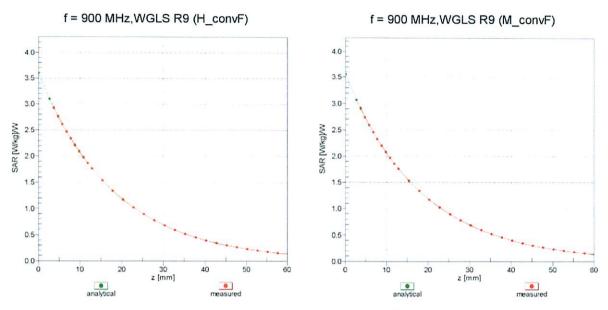

# Deviation from Isotropy in Liquid

Error  $(\phi, \vartheta)$ , f = 900 MHz

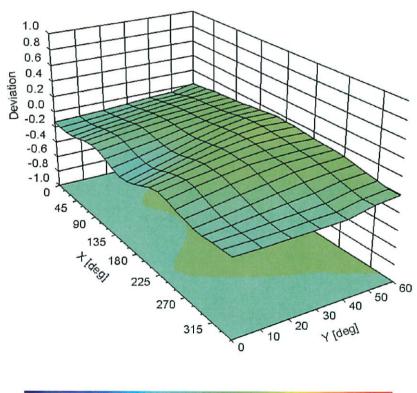

#### **Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	6
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	6.8 mm
Probe Tip to Sensor X Calibration Point	2.7 mm
Probe Tip to Sensor Y Calibration Point	2.7 mm
Probe Tip to Sensor Z Calibration Point	2.7 mm
Recommended Measurement Distance from Surface	4 mm

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

## **Additional Conversion Factors**

for Dosimetric E-Field Probe

Type:	ET3DV6
Serial Number:	1590
Place of Assessment:	Zurich
Date of Assessment:	April 29, 2013
Probe Calibration Date:	April 24, 2013

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 450, 835 and 900 MHz.

Assessed by:

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

## Dosimetric E-Field Probe ET3DV6 SN:1590

Conversion factor (± standard deviation)

$$150 \pm 50 \text{ MHz}$$

$$9.31 \pm 10\%$$

$$\varepsilon_r = 52.3 \pm 5\%$$

$$\sigma = 0.76 \pm 5\%$$
 mho/m

(head tissue)

$$300 \pm 50 \text{ MHz}$$

$$8.36 \pm 9\%$$

$$\varepsilon_r = 45.3 \pm 5\%$$

$$\sigma = 0.87 \pm 5\%$$
 mho/m

(head tissue)

$$150 \pm 50 \text{ MHz}$$

$$8.65 \pm 10\%$$

$$\varepsilon_r = 61.9 \pm 5\%$$

$$\sigma = 0.80 \pm 5\% \text{ mho/m}$$

(body tissue)

$$300 \pm 50 \text{ MHz}$$

ConvF 
$$8.41 \pm 9\%$$

$$\varepsilon_r = 58.2 \pm 5\%$$

$$\sigma = 0.92 \pm 5\%$$
 mho/m

(body tissue)

#### **Important Note:**

For numerically assessed probe conversion factors, parameters Alpha and Delta in the DASY software must have the following entries: Alpha = 0 and Delta = 1.

Please see also DASY Manual.



Date(s) of Evaluation			
Jan 28-30, 2013			

t Report Issue Date

Feb 5, 2014

Description of Test(s)

Specific Absorption Rate

Test Report Revision No.
Rev. 1.1 (Revised Issue)

RF Exposure Category
Gen. Pop. / Uncontrolled



## **APPENDIX G - ELI PHANTOM CERTIFICATE OF CONFORMITY**

Test Report Serial No.

01312014K66-1264

Applicant:	plicant: Yaesu Musen Co., Ltd		FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):	s): FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be reproduced in whole or in part without the prior written permission of Celltech Labs Inc.					Page 51 of 52		

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

#### **Certificate of Conformity / First Article Inspection**

Item	Oval Flat Phantom ELI 5.0
Type No	QD OVA 002 A
Series No	1108 and higher
Manufacturer	Untersee Composites
	Knebelstrasse 8, CH-8268 Mannenbach, Switzerland

#### Tests

Complete tests were made on the prototype units QD OVA 001 A, pre-series units QD OVA 001 B as well as on some series units QD OVA 001 B. Some tests are made on all series units QD OVA 002 A.

Test	Requirement	Details	Units tested
Shape	Internal dimensions, depth and sagging are compatible with standards	Bottom elliptical 600 x 400 mm, Depth 190 mm, dimension compliant with [1] for f > 375 MHz	Prototypes
Material thickness	Bottom: 2.0mm +/- 0.2mm	dimension compliant with [3] for f > 800 MHz	all
Material parameters	rel. permittivity 2 – 5, loss tangent ≤ 0.05, at f ≤ 6 GHz	rel. permittivity 3.5 +/- 0.5 loss tangent ≤ 0.05	Material samples
Material resistivity	Compatibility with tissue simulating liquids .	Compatible with SPEAG liquids. **	Phantoms, Material sample
Sagging	Sagging of the flat section in tolerance when filled with tissue simulating liquid.	within tolerance for filling height up to 155 mm	Prototypes, samples

Note: Compatibility restrictions apply certain liquid components mentioned in the standard, containing e.g. DGBE, DGMHE or Triton X-100. Observe technical note on material compatibility.

#### **Standards**

- [1] OET Bulletin 65, Supplement C, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", Edition 01-01
- [2] IEEE 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques, December 2003
- [3] IEC 62209–1 ed1.0, "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices Human models, instrumentation, and procedures Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", 2005-02-18
- [4] IEC 62209–2 ed1.0, "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices Human models, instrumentation, and procedures Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", 2010-03-30

#### Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of **body-worn** SAR measurements and system performance checks as specified in [1-4] and further standards.

Date

25.7.2011

Signature / Stamp

Speak a G Schmid & Partner-Engineering AG Zeughavestrasse 43, 8004 Zorich, Switzerland Phone 441 44/245 8708, 484 44 44 45 8779 info@speag.com, http://www.speag.com



Date(s) of Evaluation			
Jan 28-30, 2013			
T (D () D (			

Test Report Issue Date Description of Test(s)

Feb 5, 2014 Specific Absorption Rate

Test Report Revision No.
Rev. 1.1 (Revised Issue)

RF Exposure Category
Gen. Pop. / Uncontrolled



## APPENDIX H – KDB INQUIRY RE: 150MHZ SPC – TRACKING NUMBER 802841

Test Report Serial No.

01312014K66-1264

Applicant:	Y	aesu Musen Co., Ltd	FCC ID:	K6650013X20	IC:	511B-50013X20	
Model(s):	odel(s): FTA-550, FTA-750		DUT Type:	VHF Digital Mobile Radio		118-137 MHz	
2013 Celltech Labs Inc. This document is not to be reproduced in whole or in part without the prior written permission of Celltech Labs Inc.					Page 52 of 52		

#### **Ben Hewson**

From: oetech@fccsun27w.fcc.gov Sent: December-05-13 12:19 PM

To: Ben Hewson

Subject: Response to Inquiry to FCC (Tracking Number 802841)



#### Office of Engineering and Technology

П

#### Inquiry on 12/03/2013:

#### **Inquiry:**

We have a confined loop antenna on order from SPEAG, where we have received confirmation that it will not be anticipated for delivery until January 31, 2014.

Pursuant to instructions from Kwok's presentation in October at the TCB Council workshop in Baltimore, we are submitting this KDB for permission to have an extension to continue to utlize the provisions of KDB 865664 for system validations below 300MHz, during this period.

#### **FCC response on 12/05/2013**

You may apply the interim 150 MHz SAR system verification procedures in KDB 865664 D01 v01r01 (May 28, 2013 version) for the SAR testing required; however, you need to identify the FCC ID of the devices you will be applying the procedures. All tests must be completed before 02/15/2014. Reconfirmation through this KDB inquiry is required for any further changes.

A copy of this KDB inquiry must be provided to the TCB for review and approval of the specific FCC ID identified in this KDB. The TCB is required to confirm all conditions are satisfied.

#### **Attachment Details:**

Do not reply to this message. Please select the <u>Reply to an Inquiry Response</u> link from the OET Inquiry System to add any additional information pertaining to this inquiry.