

Contents

1. Description of Equipment Under Test (EUT)	3
2. Other Accessories	4
3. Introduction	4
4. SAR Definition	4
5. SAR Measurement Setup	5
6. System Components	6
6.1 DASY4 E-Field Probe System	6
6.1.1 ET3DV6 E-Field Probe Specification	7
6.1.2 ET3DV6 E-Field Probe Calibration	8
6.2 Data Acquisition Electronic (DAE) System.....	8
6.3 Robot.....	9
6.4 Measurement Server.....	9
6.5 Device Holder for Transmitters	9
6.6 Phantom-TWIN SAM V4.0	10
6.7 Data Storage and Evaluation	10
6.7.1 Data Storage	10
6.7.2 Data Evaluation	11
7. Test Equipment List	13
8. Tissue Simulating Liquids	14
8.1 Liquid Confirmation	15
8.1.1 Parameters.....	15
8.1.2 Liquid Depth	16
9. Measurement Process	16
9.1 Device and Test Conditions.....	16
9.2 System Performance Check	17
9.2.1 Symmetric Dipoles for System Validation	17
9.2.2 Validation.....	17
9.3 Dosimetric Assessment Setup	18
9.3.1 Handset Test Position - Head Position.....	18
9.3.2 Handset Test Position - Body Worn.....	19
9.3.3 Measurement Procedures.....	20
9.4 Spatial Peak SAR Evaluation.....	20
10. Measurement Uncertainty	21
11. SAR Test Results Summary	23
10.1 450MHz SAR Test Results-GMRS Face SAR -2.5 cm Spacing	23
10.2 450MHz SAR Test Results-FRS Face SAR -2.5 cm Spacing	24
10.3 450MHz SAR Test Results-GMRS Body SAR W /Belt-clip	25
10.4 450MHz SAR Test Results-FRS Body SAR W /Belt-clip	26
10.5 450MHz SAR Test Results-GMRS Body SAR W /Belt-clip -1.5cm Spacing.....	27
10.6 450MHz SAR Test Results-FRS Body SAR W /Belt-clip -1.5cm Spacing	28
11.7 ANSI/IEEE C95.1 – 1992 RF Exposure Limit.....	29
12. Conclusion	29
13. References	30
Appendix A - System Performance Check	31
Appendix B - SAR Measurement Data	34
Appendix C - Dipole Calibration	48
Appendix D - Probe Calibration	57
Appendix E - Data Acquisition Electronic (DAE) Calibration	62

1. Description of Equipment Under Test (EUT)

Applicant :

Giant Electronics Ltd.

7/F., Elite Industrial Bldg., 135-137 Hoi Bun Road, Kwun Tong, Kowloon, Hong Kong

EUT Type :	FRS & GMRS Two-Way Radio
Trade Name :	Motorola
Model Name :	FV500
FCC ID :	K7GFV500
Test Device :	Production Unit
Tx Frequency :	462.5500 - 462.7250 MHz (GMRS) 467.5625 – 467.7125 MHz (FRS)
Max. RF Output Power :	0.28 W ERP GMRS 0.10 W ERP FRS
Max. SAR Measurement :	0.250 W/kg GMRS Body SAR (50% Duty Cycle) 0.378 W/kg GMRS Face SAR (50% Duty Cycle) 0.086 W/kg FRS Body SAR (50% Duty Cycle) 0.151 W/kg FRS Face SAR (50% Duty Cycle)
Antenna Type :	Fixed Type
Device Category :	Portable
RF Exposure Environment :	General Population / Uncontrolled
Battery Option :	Standard
Application Type :	Certification

This wireless portable device has been shown to be capable of compliance for localized specific absorption rate (SAR) for uncontrolled environment / general population exposure limits specified in ANSI/IEEE Std. C95.1-1992 and had been tested in accordance with the measurement procedures specified in IEEE Std. 1528-2003.



Figure 1. EUT Photo

2. Other Accessories

There is another handset and Belt-clip will be an accessory with this two-way radio.



Figure 2. EUT Photo With two-way radio

3. Introduction

The A Test Lab Techno. Corp. RF Testing Laboratory has performed measurements of the maximum potential exposure to the user of **Giant Electronics Ltd. Trade Name : Motorola Model(s) : FV500**. The test procedures, as described in American National Standards, Institute C95.1 – 1992 [1] , FCC OET Bulletin65-1997 were employed and they specify the maximum exposure limit of 1.6mW/g as averaged over any 1 gram of tissue for portable devices being used within 20cm of the used in the uncontrolled environment. A description of the product and operating configuration, detailed summary of the test results, methodology and procedures used in the equipment used are included within this test report.

.*

4. SAR Definition

Specific Absorption Rate (SAR) is defined as the time derivative (rate) of the incremental energy (dw) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density (ρ). It is also defined as the rate of RF energy absorption per unit mass at a point in an absorbing body (see Figure 2).

$$SAR = \frac{d}{dt} \left(\frac{dw}{dm} \right) = \frac{d}{dt} \left(\frac{dw}{\rho dv} \right)$$

Figure 3. SAR Mathematical Equation

SAR is expressed in units of Watts per kilogram (W/kg)

$$SAR = \frac{\sigma E^2}{\rho}$$

Where :

σ = conductivity of the tissue (S/m)

ρ = mass density of the tissue (kg/m³)

E = RMS electric field strength (V/m)

*** Note :**

The primary factors that control rate of energy absorption were found to be the wavelength of the incident field in relations to the dimensions and geometry of the irradiated organism, the orientation of the organism in relation to the polarity of field vectors, the presence of reflecting surfaces, and whether conductive contact is made by the organism with a ground plane [2]

5. SAR Measurement Setup

These measurements were performed with the automated near-field scanning system DASY4 from Schmid & Partner Engineering AG (SPEAG). The system is based on a high precision robot (working range greater than 0.9m) which positions the probes with a positional repeatability of better than ± 0.025 mm. Special E- and H-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines (length = 300mm) to the data acquisition unit.

A cell controller system contains the power supply, robot controller, teach pendant (Joystick), and remote control, is used to drive the robot motors. The Measurement Server is based on a PC/104 CPU board with a 166MHz low-power Pentium, 32MB chipdisk and 64MB RAM. The necessary circuits for communication with either the DAE3 electronic box as well as the 16-bit AD-converter system for optical detection and digital I/O interface are contained on the DASY4 I/O-board, which is directly connected to the PC/104 bus of the CPU board. The PC consists of the Intel Pentium 4 2.4GHz computer with Windows2000 system and SAR Measurement Software DASY4, Post Processor SEMCAD, monitor, mouse, and keyboard. The Staubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection...etc. is connected to the Electro-optical converter (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the Measurement Server.

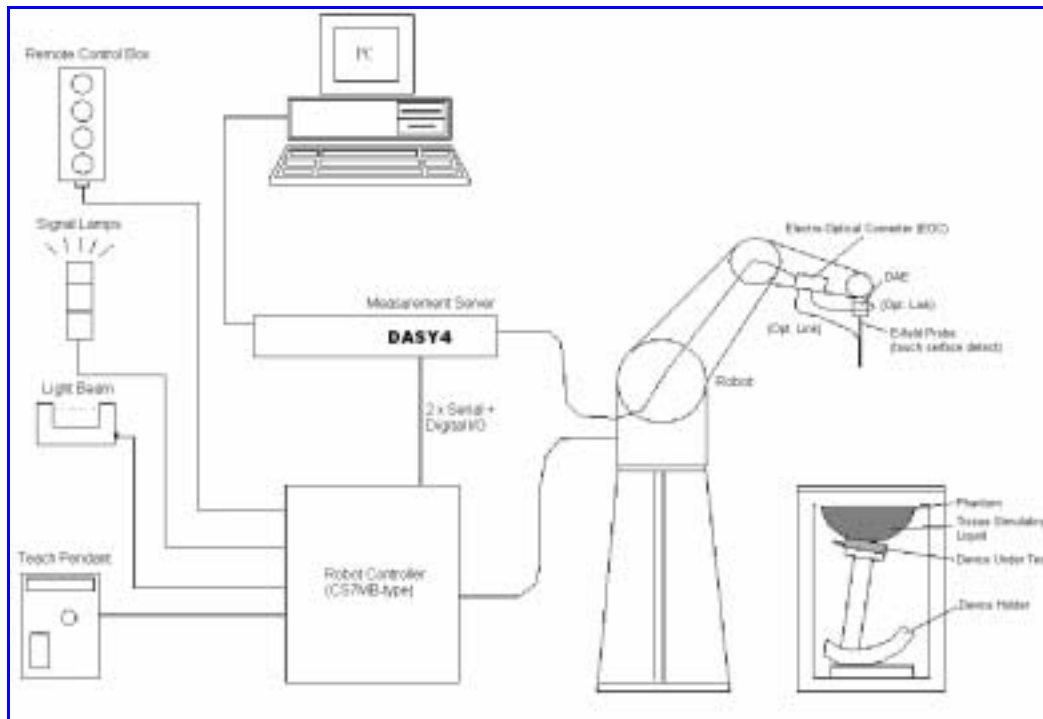


Figure 4. SAR Lab Test Measurement Setup

The DAE3 consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer. The system is described in detail in [3] .

6. System Components

6.1 DASY4 E-Field Probe System

The SAR measurements were conducted with the dosimetric probe ET3DV6 (manufactured by SPEAG), designed in the classical triangular configuration [3] and optimized for dosimetric evaluation. The probes is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multi-fiber line ending at the front of the probe tip. It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection

increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY4 software reads the reflection during a software approach and looks for the maximum using a 2nd order fitting. The approach is stopped when reaching the maximum.

6.1.1 ET3DV6 E-Field Probe Specification

Construction	Symmetrical design with triangular core Built-in optical fiber for surface detection System (ET3DV6 only) Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.q., glycol)
Calibration	In air from 10 MHz to 2.5 GHz In brain and muscle simulating tissue at frequencies of 450MHz, 900MHz, 1.8GHz and 2.45GHz (accuracy ±8%) Calibration for other liquids and frequencies upon request
Frequency	10 MHz to > 6 GHz; Linearity: ±0.2 dB (30 MHz to 3 GHz)
Directivity	± 0.2 dB in brain tissue (rotation around probe axis) ± 0.4 dB in brain tissue (rotation normal probe axis)
Dynamic Range	5 μ W/g to > 100mW/g; Linearity: ±0.2dB
Surface Detection	± 0.2 mm repeatability in air and clear liquids over diffuse reflecting surface(ET3DV6 only)
Dimensions	Overall length: 330mm Tip length: 16mm Body diameter: 12mm Tip diameter: 6.8mm Distance from probe tip to dipole centers: 2.7mm
Application	General dosimetry up to 3GHz Compliance tests of mobile phones Fast automatic scanning in arbitrary phantoms



Figure 5. ET3DV6 E-field Probe



Figure 6. Probe setup on robot

6.1.2 ET3DV6 E-Field Probe Calibration

Each probe is calibrated according to a dosimetric assessment procedure described in [4] with accuracy better than ± 10%. The spherical isotropy was evaluated with the procedure described in [5] and found to be better than ± 0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested.

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies bellow 1GHz, and in a wave guide above 1GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$SAR = C \frac{\Delta T}{\Delta t}$$

Where :

- Δ t** = Exposure time (30 seconds),
- C** = Heat capacity of tissue (brain or muscle),
- Δ T** = Temperature increase due to RF exposure.

Or

$$SAR = \frac{|E|^2 \sigma}{\rho}$$

Where :

- σ** = Simulated tissue conductivity,
- ρ** = Tissue density (kg/m³).

6.2 Data Acquisition Electronic (DAE) System

Cell Controller

- Processor : Intel Pentium 4
- Clock Speed : 2.4GHz
- Operating System : Windows 2000 Professional

Data Converter

- Features : Signal Amplifier, multiplexer, A/D converter, and control logic
- Software : DASY4 v4.4 (Build 3) & SEMCAD v1.8 (Build 180)
- Connecting Lines : Optical downlink for data and status info
 Optical uplink for commands and clock

6.3 Robot

Positioner : Stäubli Unimation Corp. Robot Model: RX90L
Repeatability : ± 0.025 mm
No. of Axis : 6

6.4 Measurement Server

Processor : PC/104 with a 166MHz low-power Pentium
I/O-board : Link to DAE3
16-bit A/D converter for surface detection system
Digital I/O interface
Serial link to robot
Direct emergency stop output for robot

6.5 Device Holder for Transmitters

In combination with the SAM Twin Phantom V4.0, the Mounting Device (POM) enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation points is the ear opening. The devices can be easily, accurately, and repeat ably positioned according to the IEEE SCC34-SC2 and CENELEC specifications. The device holder can be locked at different phantom locations (left head, right head, and flat phantom).

*** Note :** A simulating human hand is not used due to the complex anatomical and geometrical structure of the hand that may produced infinite number of configurations [6] . To produce the worst-case condition (the hand absorbs antenna output power), the hand is omitted during the tests.

Larger DUT cannot be tested using this device holder. Instead a support of bigger polystyrene cubes and thin polystyrene plates is used to position the DUT in all relevant positions to find and measure spots with maximum SAR values. Therefore those devices are normally only tested at the flat part of the SAM.



Figure 7. Device Holder

6.6 Phantom - SAM v4.0

The shell corresponds to the specifications of the Specific Anthropomorphic Mannequin (SAM) phantom defined in IEEE 1528-2003, CENELEC 50361 and IEC 62209. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents evaporation of the liquid. Reference markings on the phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points with the robot.



Figure 8. SAM Twin Phantom

Shell Thickness	2 ± 0.2 mm
Filling Volume	Approx. 25 liters
Dimensions	810×1000×500 mm (H×L×W)

Table 1. Specification of SAM v4.0

6.7 Data Storage and Evaluation

6.7.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The postprocessing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

6.7.2 Data Evaluation

The DASYS4 postprocessing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software :

- Probe parameters :**
- Sensitivity Normi, ai0, ai1, ai2
 - Conversion factor ConvFi
 - Diode compression point dcp_i
- Device parameters :**
- Frequency f
 - Crest factor cf
- Media parameters :**
- Conductivity
 - Density

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASYS components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as :

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

- with
- V_i = compensated signal of channel i ($i = x, y, z$)
 - U_i = input signal of channel i ($i = x, y, z$)
 - cf = crest factor of exciting field (DASY parameter)
 - dcp_i = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated :

E-field probes :

$$E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$$

H-field probes :

$$H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}f + a_{i2}f^2}{f}$$

with V_i = compensated signal of channel i ($i = x, y, z$)
 $Norm_i$ = sensor sensitivity of channel i ($i = x, y, z$)
 $\mu V/(V/m)^2$ for E-field Probes
 $ConvF$ = sensitivity enhancement in solution
 a_{ij} = sensor sensitivity factors for H-field probes
 f = carrier frequency [GHz]
 E_i = electric field strength of channel i in V/m
 Hi = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude) :

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with SAR = local specific absorption rate in mW/g
 E_{tot} = total field strength in V/m
 σ = conductivity in [mho/m] or [Siemens/m]
 ρ = equivalent tissue density in g/cm^3

*** Note :** that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770} \quad \text{or} \quad P_{pwe} = \frac{H_{tot}^2}{37.7}$$

with P_{pwe} = equivalent power density of a plane wave in mW/cm^2
 E_{tot} = total electric field strength in V/m
 H_{tot} = total magnetic field strength in A/m

7. Test Equipment List

Manufacturer	Name of Equipment	Type/Model	Serial Number	Calibration	
				Last Cal.	Due Date
SPEAG	Dosimetric E-Filed Probe	ET3DV6	1531	Jan. 17, 2005	Jan. 17, 2006
SPEAG	450MHz System Validation Kit	D450V2	1021	Feb.01, 2005	Feb.01, 2007
SPEAG	Data Acquisition Electronics	DAE3	393	Jan. 8, 2004	Jan. 8, 2005
SPEAG	Device Holder	N/A	N/A	NCR	NCR
SPEAG	Phantom	SAM V4.0	1009	NCR	NCR
SPEAG	Robot	Staubli RX90L	F00/589B1/A/01	NCR	NCR
SPEAG	Software	DASY4 V4.4 Build 3	N/A	NCR	NCR
SPEAG	Software	SEMCAD V1.8 Build 130	N/A	NCR	NCR
SPEAG	Measurement Server	SE UMS 001 BA	1021	NCR	NCR
Agilent	Wireless Communication Test Set	8960(E5515C)	GB41450409	Jan.31,2005	Jan.31,2007
Agilent	S-Parameter Network Analyzer	8720ES	US39172472	May 18, 2004	May 18, 2005
Agilent	Dielectric Probe Kit	85070C	US99360094	NCR	NCR
Agilent	Power Meter	E4418C	GB40206143	May 18, 2004	May 17, 2005
Agilent	Power Sensor	8481H	3318A0779	July 3, 2004	July 3, 2005
Agilent	Signal Generator	8648C	3847A05201	July 13, 2004	July 13, 2005
Agilent	Dual Directional Coupler	778D	50334	NCR	NCR
Mini-Circuits	Power Amplifier	ZHL-42W-SMA	D111103#5	NCR	NCR

Table 2. Test Equipment List

8. Tissue Simulating Liquids

The Head and Muscle mixtures consist of a viscous gel using hydroxethylcellullose (HEC) gelling agent and saline solution. Preservation with a bacteriacide is added and visual inspection is made to ensure air bubbles are not trapped during the mixing process. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the tissue.

The dielectric parameters of the liquids were verified prior to the SAR evaluation using an 85070C Dielectric Probe Kit and an 8720ES Network Analyzer.

INGREDIENT	FREQUENCY	
	HSL450 – Head (400-500MHz)	MSL450- Muscle (400-500MHz)
Water	38.91 %	46.21 %
HEC	0.25 %	0.18 %
Sugar	56.93 %	51.17 %
Preventol	0.12 %	0.08 %
Salt	3.79 %	2.34 %
Glycol monobutyl	0 %	0 %
Dielectric Parameters at 22°	f = 450 MHz $\epsilon_r = 43.5, \sigma = 0.87 \text{ S/m}$	f = 450 MHz $\epsilon_r = 56.7, \sigma = 0.94 \text{ S/m}$

Table 3. Recipes for Head & Muscle Tissue Simulating Liquids

IEEE SCC-34/SC-2 in 1528 recommended Tissue Dielectric Parameters

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in 1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in human head. Other head and body tissue parameters that have not been specified in 1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equation and extrapolated according to the head parameter specified in 1528.

Target Frequency	Head		Body	
(MHz)	ϵ_r	σ (S/m)	ϵ_r	σ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800 - 2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00
(ϵ_r = relative permittivity, σ = conductivity and ρ = 1000 kg/m ³)				

Table 4. Tissue dielectric parameters for head and body phantoms

8.1 Liquid Confirmation

8.1.1 Parameters

Liquid Verify								
Ambient Temperature : 22±2 ; Relative Humidity : < 60 %								
Liquid Tyep	Frequency	Temp ()	Parameters	Target Value	Measured Value	Deviation (%)	Limit (%)	Measured Date
4 MHz Body	450MHz	22.1	r	56.7	55.97	-0.48 %	±5 %	Feb. 04, 2005
				0.94	0.983	4.57 %	±5 %	

Table 5. Measured Tissue dielectric parameters for head and body phantoms

8.1.2 Liquid Depth

The liquid level was during measurement 15cm \pm 0.5cm.

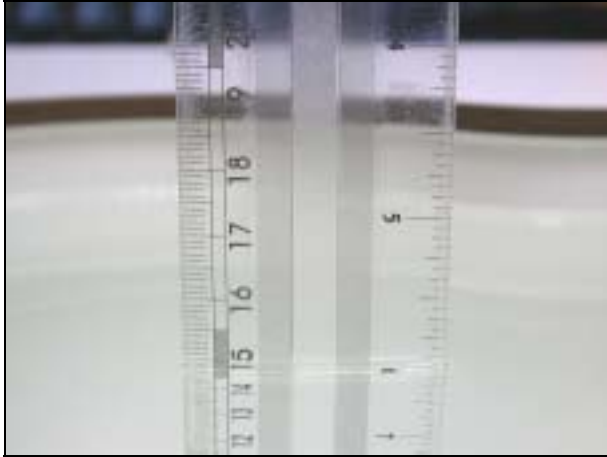


Figure 9. Head-Tissue-Simulating-Liquid 450MHz

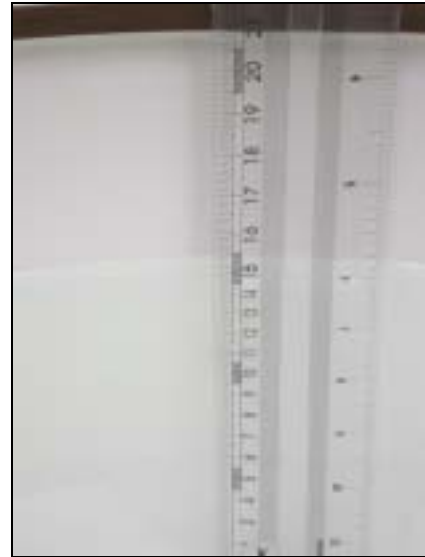


Figure 10. Muscle-Tissue-Simulating-Liquid 450MHz

9. Measurement Process

9.1 Device and Test Conditions

The Test Device was provided by **Giant Electronics Ltd.** for this evaluation. The spatial peak SAR values were assessed for the lowest, middle and highest channels defined by GMRS (Ch4=462.637MHz, Ch15=462.55MHz, Ch22=462.75MHz)/ FRS (Ch8=467.563MHz, Ch11=467.637MHz, Ch14=467.712MHz) systems. The device was put in operation using the **Agilent 8960 wireless Communication Test Set**. The antenna(s), battery and accessories shall be those specified by the manufacturer. The battery shall be fully charged before each measurement and there shall be no external connections.

9.2 System Performance Check

9.2.1 Symmetric Dipoles for System Validation

Construction	Symmetrical dipole with 1/4 balun enables measurement of feed point impedance with NWA matched for use near flat phantoms filled with brain simulating solutions Includes distance holder and tripod adaptor Calibration Calibrated SAR value for specified position and input power at the flat phantom in brain simulating solutions.
Frequency	450, 900, 1800, 2450MHz
Return Loss	> 20 dB at specified validation position
Power Capability	> 100 W (f < 1GHz); > 40 W (f > 1GHz)
Options	Dipoles for other frequencies or solutions and other calibration conditions are available upon request
Dimensions	D450V2 : dipole length 270 mm; overall height 330 mm D900V2 : dipole length 149 mm; overall height 330 mm D1800V2 : dipole length 72 mm; overall height 300 mm D2450V2 : dipole length 51.5 mm; overall height 300 mm



Figure 11. Validation Kit

9.2.2 Validation

Prior to the assessment, the system validation kit was used to test whether the system was operating within its specifications of ± 10%. The validation was performed at 450MHz.

Validation kit		Mixture Type		SAR _{1g} [mW/g]	SAR _{10g} [mW/g]	Date of Calibration	
D450V2-SN265		Head		5.025	3.3	Feb 01, 2005	
		Body		5.35	3.475		
Frequency (MHz)	Power (dBm)	SAR _{1g} (mW/g)	SAR _{10g} (mW/g)	Drift (dB)	Difference percentage		Date
					1g	10g	
450 (Head)	250mW	2.12	1.33	0.0	5.5 %	0.8 %	Feb .04 ,2005
	Normalize to 1 Watt	5.3	3.325				
450 (Body)	250mW	2.12	1.32	0.0	-0.9	-5.0	Feb .04 ,2005
	Normalize to 1 Watt	5.3	3.3				

9.3 Dosimetric Assessment Setup

9.3.1 Handset Test Position - Head Position

A handset should be initially positioned with the earpiece region pressed against the ear spacer of a head phantom. For the SCC-34/SC-2 head phantom, the device should be positioned parallel to the “N-F” line defined along the base of the ear spacer that contains the “ear reference point”. For interim head phantoms, the device should be positioned parallel to the cheek for maximum RF energy coupling. The “test device reference point” is aligned to the “ear reference point” on the head phantom and the “vertical centerline” is aligned to the “phantom reference plane”. This is called the “initial ear position”. While maintaining these three alignments, the body of the handset is gradually adjusted to each of the following positions for evaluating SAR :

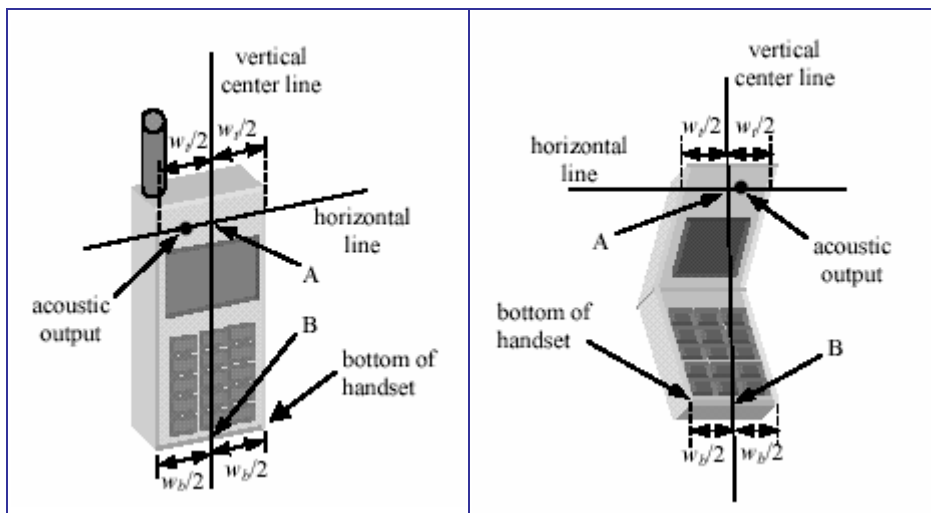


Figure 12. Handset vertical and horizontal Reference Lines - Fixed Case & Clam Shell

- 1) “Cheek/Touch Position” — the device is brought toward the mouth of the head phantom by pivoting against the “ear reference point” or along the “N-F” line for the SCC-34/SC-2 head phantom. This test position is established:
 - i) When any point on the display, keypad or mouthpiece portions of the handset is in contact with the phantom.
 - ii) (Or) when any portion of a foldout, sliding or similar keypad cover opened to its intended self-adjusting normal use position is in contact with the cheek or mouth of the phantom.
 For existing head phantoms — when the handset loses contact with the phantom at the pivoting point, rotation should continue until the device touch the cheek of the phantom or breaks its last contact from the ear spacer.

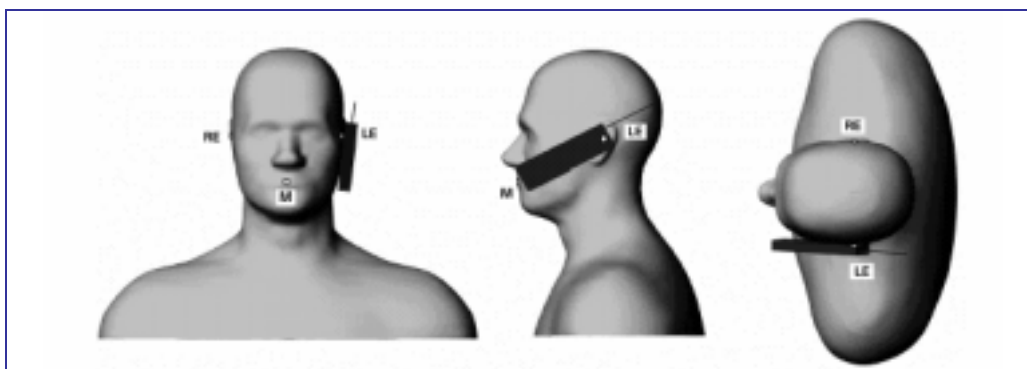


Figure 13. Phone Position 1, Cheek or Touch Position

- 2) "Ear/Tilt Position" — With the handset aligned in the "Cheek/Touch Position":
- i) If the earpiece of the handset is not in full contact with the phantom's ear spacer (in the "Cheek/Touch position") and the peak SAR location for the "Cheek/Touch" position is located at the ear spacer region or corresponds to the earpiece region of the handset, the device should be returned to the "initial ear position" by rotation it away from the mouth until the earpiece is in full contact with the ear spacer.
 - ii) (Otherwise) the handset should be moved (translated) away from the cheek perpendicular to the line passes through both "ear reference points" (note: one of these ear reference points may not physically exist on a split head model) for approximate 2-3cm. While it is in this position, the handset is tilted away from the mouth with respect to the "test device reference point" by 15°. After the tilt, it is then moved (translated) back toward the head perpendicular to the line passes through both "ear reference points" until the device touches the phantom or the ear spacer. If the antenna touches the head first, the positioning process should be repeated with a tilt angle less than 15° so that the device and its antenna would touch the phantom simultaneously. This test position may require a device holder or positioner to achieve the translation and tilting with acceptable positioning repeatability.

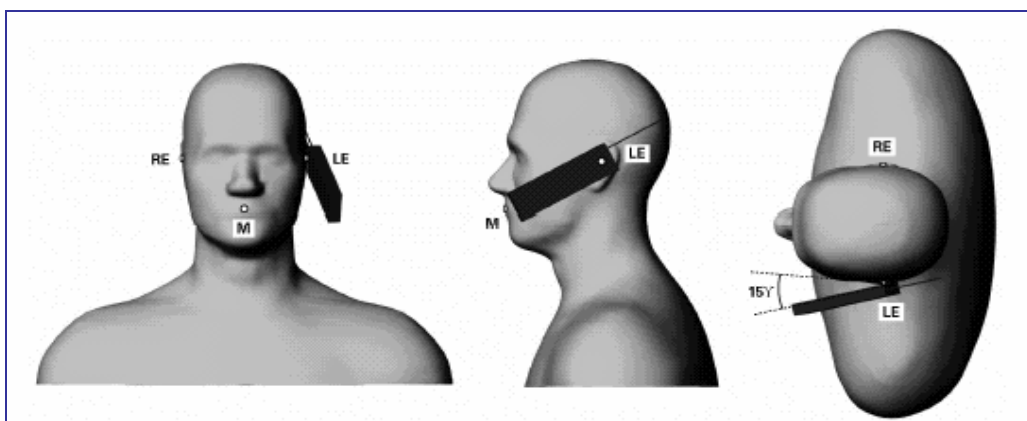


Figure 14. Phone Position 2, Tilted Position

9.3.2 Handset Test Position – Body-Worn

Body-Worn Configuration

Body-worn operating configurations should be tested with the belt-clips and holsters attached to the device and positioned against a flat phantom in normal use configurations. Devices with a headset output should be tested with a headset connected to the device.

Body-worn accessories may not always be supplied or available as options for some devices that are intended to be authorized for body-worn use. A separation distance of 1.5 cm between the back of the device and a flat phantom is recommended for testing body-worn SAR compliance under such circumstances.

For this test :

The EUT is placed into the holster/belt clip and the holster is positioned against the surface of the phantom in a normal operating position.

Since this EUT doesn't supply any body-worn accessory to the end user, a distance of 1.5 cm was tested to confirm the necessary "minimum SAR separation distance".

(* **Note** : this distance includes the 2 mm phantom shell thickness.)

9.3.3 Measurement Procedures

The evaluation was performed with the following procedures :

Surface Check : A surface check job gathers data used with optical surface detection. It determines the distance from the phantom surface where the reflection from the optical detector has its peak. Any following measurement jobs using optical surface detection will then rely on this value. The surface check performs its search a specified number of times, so that the repeatability can be verified.

Reference : The reference job measures the field at a specified reference position, at 4 mm from the selected section's grid reference point.

Area Scan : The area scan is used as a fast scan in two dimensions to find the area of high field values, before doing a finer measurement around the hot spot. The sophisticated interpolation routines can find the maximum locations even in relatively coarse grids. When an area scan has measured all reachable points, it computes the field maxima found in the scanned area, within a range of the global maximum. Any following zoom scan within the same procedure will then perform fine scans around these maxima. The area covered the entire dimension of the EUT and the horizontal grid spacing was 15 mm x 15 mm.

Zoom Scan : Zoom scans are used to assess the highest averaged SAR for cubic averaging volumes with 1 g and 10 g of simulated tissue. The zoom scan measures 5 x 5 x 7 points in a 32 x 32 x 30 mm cube whose base faces are centered around the maxima returned from a preceding area scan within the same procedure.

Drift : The drift job measures the field at the same location as the most recent reference job within the same procedure, with the same settings. The drift measurement gives the field difference in dB from the last reference measurement. Several drift measurements are possible for each reference measurement. This allows monitoring of the power drift of the device in the batch process. If the value changed by more than 5%, the evaluation was repeated.

9.4 Spatial Peak SAR Evaluation

The DASY4 software includes all numerical procedures necessary to evaluate the spatial peak SAR values. Based on the Draft: SCC-34, SC-2, WG-2 - Computational Dosimetry, IEEE P1529/D0.0 (Draft Recommended Practice for Determining the Spatial-Peak Specific Absorption Rate (SAR) Associated with the Use of Wireless Handsets - Computational Techniques), a new algorithm has been implemented. The spatial-peak SAR can be computed over any required mass.

The base for the evaluation is a "cube" measurement in a volume of (32x32x30)mm³ (5x5x7 points). The

measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan. If the 10g cube or both cubes are not entirely inside the measured volumes, the system issues a warning regarding the evaluated spatial peak values within the Postprocessing engine (SEMCAD). This means that if the measured volume is shifted, higher values might be possible. To get the correct values you can use a finer measurement grid for the area scan. In complicated field distributions, a large grid spacing for the area scan might miss some details and give an incorrectly interpolated peak location.

The entire evaluation of the spatial peak values is performed within the Postprocessing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into three stages:

Interpolation and Extrapolation

The probe is calibrated at the center of the dipole sensors which is located 1 to 2.7mm away from the probe tip. During measurements, the probe stops shortly above the phantom surface, depending on the probe and the surface detecting system. Both distances are included as parameters in the probe configuration file. The software always knows exactly how far away the measured point is from the surface. As the probe cannot directly measure at the surface, the values between the deepest measured point and the surface must be extrapolated.

In DASY4, the choice of the coordinate system defining the location of the measurement points has no influence on the uncertainty of the interpolation, Maxima Search and SAR extrapolation routines. The interpolation, Maxima Search and extrapolation routines are all based on the modified Quadratic Shepard's method [7].

10. Measurement Uncertainty

Measurement uncertainties in SAR measurements are difficult to quantify due to several variables including biological, physiological, and environmental. However, we estimate the measurement uncertainties in SAR to be less than $\pm 27\%$ [8] .

According to ANSI/IEEE C95.3 [9] , the overall uncertainties are difficult to assess and will vary with the type of meter and usage situation. However, accuracy's of ± 1 to 3 dB can be expected in practice, with greater uncertainties in near-field situations and at higher frequencies (shorter wavelengths), or areas where large reflecting objects are present. Under optimum measurement conditions, SAR measurement uncertainties of at least ± 2 dB can be expected.

According to CENELEC [10] , typical worst-case uncertainty of field measurements is ± 5 dB. For well-defined modulation characteristics the uncertainty can be reduced to ± 3 dB.

Source of Uncertainty	Uncertainty Value	Probability Distribution	Divisor	C_j	Standard Uncertainty $\pm 1\%$ (1-g)	V_j or V_{eff}
Type-A	0.9 %	Normal	1	1	0.9	9
Measurement System						
Probe Calibration	7 %	Normal	2	1	3.5	
Axial Isotropy	0.2dB	Rectangular	$\sqrt{3}$	$\sqrt{0.5}$	1.9	
Hemispherical Isotropy	9.6 %	Rectangular	$\sqrt{3}$	$\sqrt{0.5}$	3.9	
Spatial Resolution	0 %	Rectangular	$\sqrt{3}$	1	0	
Boundary Effect	11.0 %	Rectangular	$\sqrt{3}$	1	6.4	
Linearity	0.2dB	Rectangular	$\sqrt{3}$	1	2.7	
Detection Limit	1.0 %	Rectangular	$\sqrt{3}$	1	0.6	
Readout Electronics	1.0 %	Normal	1	1	1.0	
RF Ambient Conditions	3.0 %	Rectangular	$\sqrt{3}$	1	1.73	
Probe Positioner Mech. Const.	0.4 %	Rectangular	$\sqrt{3}$	1	0.2	
Probe Positioning	0.35 %	Rectangular	$\sqrt{3}$	1	0.2	
Extrapolation and Integration	3.9 %	Rectangular	$\sqrt{3}$	1	2.3	
Test sample Related						
Test sample Positioning	4.7 %	Normal	1	1	4.7	5
Device Holder Uncertainty	6.1 %	Normal	1	1	6.1	5
Drift of Output Power	5.0 %	Rectangular	$\sqrt{3}$	1	2.9	
Phantom and Setup						
Phantom Uncertainty (Including temperature effects)	4.0%	Rectangular	$\sqrt{3}$	1	2.3	
Liquid Conductivity (target)	5.0%	Rectangular	$\sqrt{3}$	0.6	1.7	
Liquid Conductivity (meas.)	10.0%	Rectangular	$\sqrt{3}$	0.6	3.4	
Liquid Permittivity (target)	5.0%	Rectangular	$\sqrt{3}$	0.6	1.7	
Liquid Permittivity (meas.)	5.0%	Rectangular	$\sqrt{3}$	0.6	1.7	
Combined standard uncertainty		RSS			13.5	88.7
Expanded uncertainty (Coverage factor = 2)		Normal (k=2)			27	

Table 6. Uncertainty Budget of DASY

11. SAR Test Results Summary

11.1 GMRS Face SAR -1.5CM Spacing-

Ambient :

Temperature () : 22 ± 2 Relative HUMIDITY (%) : < 60

Liquid :

Mixture Type : HSL450 Liquid Temperature () : 22.1
 Depth of liquid (cm) : 15

Measurement :

Crest Factor : 1 Probe S/N : 1530

Frequency		Moduction	Battery	Accessory	SAR _{1g} [mW/g]		Power Drift	Remark	Amb. Temp	Liq. Temp
MHz	Ch.				Duty Cycle					
					100%	50%				
462.5500	15	FM	Moto	N/A	0.733	0.367	-0.5	-	22.1	22.2
462.6375	4	FM	Moto	N/A	0.755	0.378	-0.5	-	22.2	22.1
462.7250	22	FM	Moto	N/A	0.694	0.347	-0.5	-	22.1	22.2
ANSI / IEEE C95.1 1992 - Safety Limit Spatial Peak Uncontrolled Exposure/General Population					Brain 1.6 W/kg (mW/g) Averaged over 1 gram					

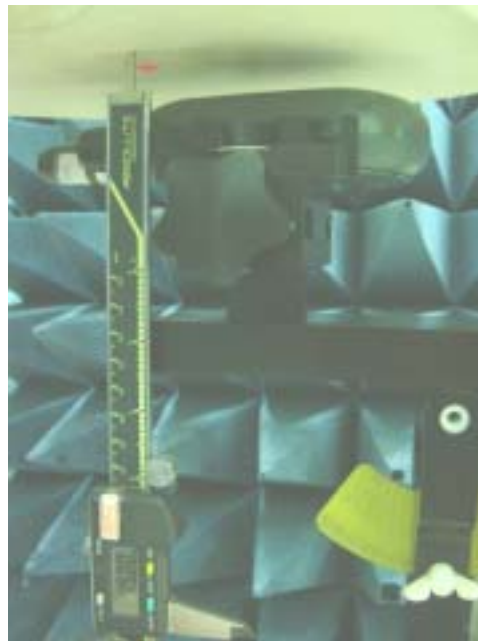


Figure 11.1 SAR Test Setup
 -----Face Position-----

11.2 FRS Face SAR -1.5 cm Spacing-

Ambient :		Temperature () :	<u>22 ± 2</u>	Relative HUMIDITY (%) :	<u>< 60</u>
Liquid :		Mixture Type :	<u>HSL450</u>	Liquid Temperature () :	<u>22.1</u>
				Depth of liquid (cm) :	<u>15</u>
Measurement :		Crest Factor :	<u>1</u>	Probe S/N :	<u>1530</u>

Frequency		Moduction	Battery	Accessory	SAR _{1g} [mW/g]		Power Drift	Remark	Amb. Temp	Liq. Temp
MHz	Ch.				Duty Cycle					
					100%	50%				
467.5625	8	FM	Moto	N/A	0.295	0.148	-0.3	-	22.2	22.0
467.6375	11	FM	Moto	N/A	0.274	0.137	-0.5	-	22.2	22.1
467.7125	14	FM	Moto	N/A	0.302	0.151	-0.6	-	22.2	22.1
ANSI / IEEE C95.1 1992 - Safety Limit Spatial Peak Uncontrolled Exposure/General Population					Brain 1.6 W/kg (mW/g) Averaged over 1 gram					

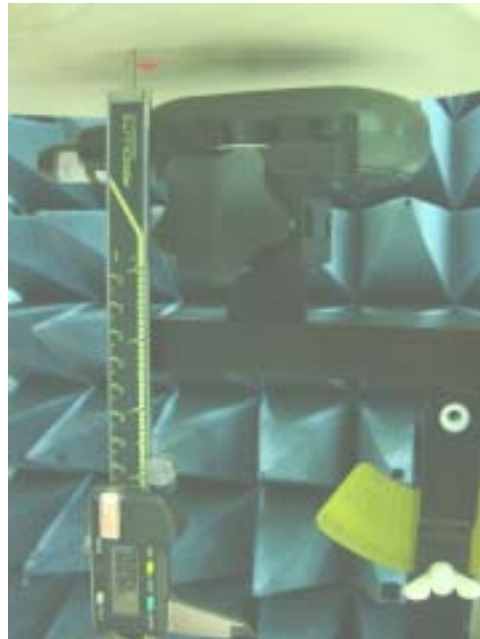


Figure 11.2 SAR Test Setup
 -----Face Position-----

11.3 GMRS Body SAR W /Belt –clip

Ambient :			
Temperature () :	<u>22 ± 2</u>	Relative HUMIDITY (%) :	<u>< 60</u>
Liquid :			
Mixture Type :	<u>HSL450</u>	Liquid Temperature () :	<u>22.1</u>
		Depth of liquid (cm) :	<u>15</u>
Measurement :			
Crest Factor :	<u>1</u>	Probe S/N :	<u>1530</u>

Frequency		Moduction	Battery	Accessory	SAR _{1g} [mW/g]		Power Drift	Remark	Amb. Temp	Liq. Temp
MHz	Ch.				Duty Cycle					
					100%	50%				
462.5500	15	FM	Moto	Headset	0.499	0.250	-0.4	-	22.2	22.1
462.6375	4	FM	Moto	Headset	0.490	0.245	-0.5	-	22.1	22.2
462.7250	22	FM	Moto	Headset	0.396	0.198	-0.4	-	22.2	22.2
ANSI / IEEE C95.1 1992 - Safety Limit Spatial Peak Uncontrolled Exposure/General Population					Brain 1.6 W/kg (mW/g) Averaged over 1 gram					

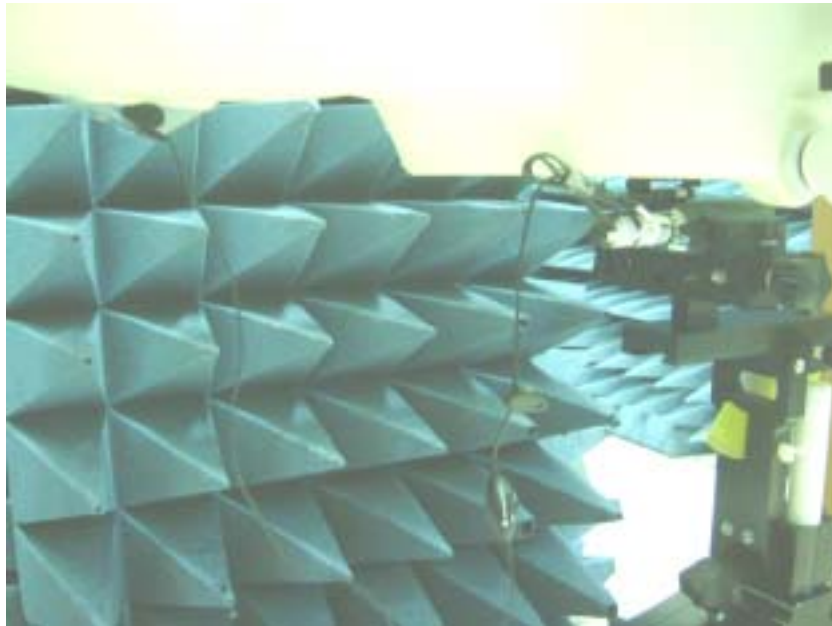


Figure 11.3 SAR Test Setup
 -----w / Belt Clip-----

11.4 FRS Body SAR w /Belt – clip

Ambient :

Temperature () : 22 ± 2 Relative HUMIDITY (%) : < 60


Liquid :

Mixture Type : HSL450 Liquid Temperature () : 22.1
 Depth of liquid (cm) : 15

Measurement :

Crest Factor : 1 Probe S/N : 1530

Frequency		Moduction	Battery	Accessory	SAR _{1g} [mW/g]		Power Drift	Remark	Amb. Temp	Liq. Temp
MHz	Ch.				Duty Cycle					
					100%	50%				
467.5625	8	FM	Moto	Headset	0.172	0.086	-0.3	-	22.0	22.2
467.6375	11	FM	Moto	Headset	0.132	0.066	-0.4	-	22.0	22.2
467.7125	14	FM	Moto	Headset	0.152	0.076	-0.4	-	22.2	22.2
ANSI / IEEE C95.1 1992 - Safety Limit Spatial Peak Uncontrolled Exposure/General Population					Brain 1.6 W/kg (mW/g) Averaged over 1 gram					

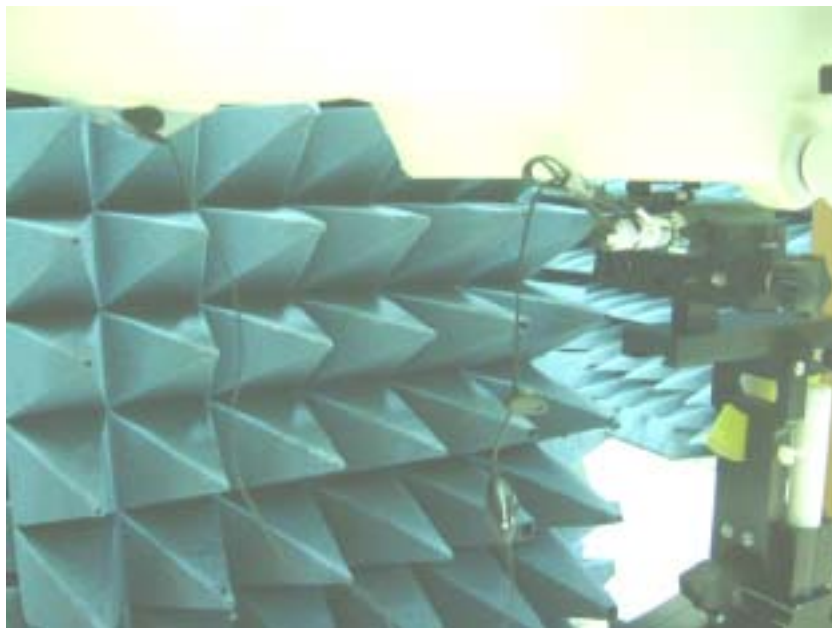

**Figure 11.4 Body SAR Test Setup
 -----w / Belt Clip-----**

11.5 GMRS Body SAR w/out Belt-clip -1.5 cm Spacing

Ambient :					
Temperature () :	<u>22 ± 2</u>	Relative HUMIDITY (%) :	<u>< 60</u>		
Liquid :					
Mixture Type :	<u>HSL450</u>	Liquid Temperature () :	<u>22.1</u>		
		Depth of liquid (cm) :	<u>15</u>		
Measurement :					
Crest Factor :	<u>1</u>	Probe S/N :	<u>1530</u>		

Frequency		Moduction	Battery	Accessory	SAR _{1g} [mW/g]		Power Drift	Remark	Amb. Temp	Liq. Temp	
MHz	Ch.				Duty Cycle						
462.6375	4	FM	Moto	N/A	0.662	0.331	-0.7	-	22.2	22.1	
ANSI / IEEE C95.1 1992 - Safety Limit Spatial Peak Uncontrolled Exposure/General Population					Brain 1.6 W/kg (mW/g) Averaged over 1 gram						



Figure 11.5 Body SAR Test Setup
 -----w / out Belt Clip-----

11.6 FRS Body SAR w/out Belt-clip -1.5 cm Spacing

Ambient :	Temperature () :	<u>22 ± 2</u>	Relative HUMIDITY (%) :	<u>< 60</u>
Liquid :	Mixture Type :	<u>HSL450</u>	Liquid Temperature () :	<u>22.1</u>
			Depth of liquid (cm) :	<u>15</u>
Measurement :	Crest Factor :	<u>1</u>	Probe S/N :	<u>1530</u>

Frequency		Moduction	Battery	Accessory	SAR _{1g} [mW/g]		Power Drift	Remark	Amb. Temp	Liq. Temp
MHz	Ch.				Duty Cycle					
467.6375	11	FM	Moto	N/A	0.266	0.133	-0.4	-	22.2	22.2
ANSI / IEEE C95.1 1992 - Safety Limit Spatial Peak Uncontrolled Exposure/General Population					Brain 1.6 W/kg (mW/g) Averaged over 1 gram					



**Figure 11.6 Body SAR Test Setup
 -----w / out Belt Clip-----**

11.7 ANSI/IEEE C95.1 – 1992 RF Exposure Limit

Human Exposure	Population Uncontrolled Exposure (W/kg) or (mW/g)	Occupational Controlled Exposure (W/kg) or (mW/g)
Spatial Peak SAR* (Brain)	1.60	8.00
Spatial Peak SAR** (Whole Body)	0.08	0.40
Spatial Peak SAR*** (Hands / Feet / Ankle / Wrist)	4.00	20.00

Table 7. Safety Limits for Partial Body Exposure

Notes :

- * The Spatial Peak value of the SAR averaged over any 1 gram of tissue.
(defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.
- ** The Spatial Average value of the SAR averaged over the whole – body.
- *** The Spatial Peak value of the SAR averaged over any 10 grams of tissue.
(defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

Population / Uncontrolled Environments : are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure.

Occupational / Controlled Environments : are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation).

12. Conclusion

The SAR test values found for the portable mobile phone **Giant Electronics Ltd. Trade Name : Motorola Model(s) : FV500**, are below the maximum recommended level of 1.6 W/kg (mW/g).

13. References

- [1] ANSI/IEEE C95.1-1991, "American National Standard safety levels with respect to human exposure to radio frequency electromagnetic fields, 300KHz to 100GHz", New York: IEEE, Aug. 1992.
- [2] NCRP, National Council on Radiation Protection and Measurements, "Biological Effects and Exposure Criteria for Radio frequency Electromagnetic Fields", NCRP report NO. 86, 1986.
- [3] T. Schmid, O. Egger, and N. Kuster, "Automatic E-field scanning system for dosimetric assessments", IEEE Transactions on Microwave Theory and Techniques, vol. 44, pp, 105-113, Jan. 1996.
- [4] K. Pokovič, T. Schmid, and N. Kuster, "Robust setup for precise calibration of E-field probes in tissue simulating liquids at mobile communications frequency", in ICECOM'97, Dubrovnik, October 15-17, 1997, pp.120-124.
- [5] K. Pokovič, T. Schmid, and N. Kuster, "E-field probe with improved isotropy in brain simulating liquids", in Proceedings of the ELMAR, Zadar, Croatia, 23-25 June, 1996, pp.172-175.
- [6] N. Kuster, and Q. Balzano, "Energy absorption mechanism by biological bodies in the near field of dipole antennas above 300MHz", IEEE Transaction on Vehicular Technology, vol. 41, no. 1, Feb. 1992, pp. 17-23.
- [7] Robert J. Renka, "Multivariate Interpolation Of Large Sets Of Scattered Data", University of North Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988 , pp. 139-148.
- [8] N. Kuster, R. Kastle, T. Schmid, "Dosimetric evaluation of mobile communications equipment with known precision", IEEE Transaction on Communications, vol. E80-B, no. 5, May 1997, pp. 645-652.
- [9] ANSI/IEEE C95.3-1991, "IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields – RF and Microwave", New York: IEEE, Aug. 1992.
- [10] CENELEC CLC/SC111B, European Prestandard (prENV 50166-2), Human Exposure to Electromagnetic Fields High-frequency: 10KHz-300GHz, Jan. 1995.

Appendix A – System Performance Check

Date/Time: 02/04/05 08:23:07

Test Laboratory: A Test Lab Techno Corp.

System Performance Check at 450MHz_Head

DUT: Dipole 450 MHz; Type: D450V2; Serial: D450V2 - SN:1021

Communication System: CW; Frequency: 450 MHz; Duty Cycle: 1:1

Medium: Head 450MHz Medium parameters used: $f = 450 \text{ MHz}$; $s = 0.83 \text{ mho/m}$; $\epsilon_r = 45.6$;

Conductivity = 1000 kg/m^3 ; Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.27, 7.27, 7.27); Calibrated: 1/17/2005

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009

- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (61x181x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (interpolated) = 2.33 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 53.1 V/m ; Power Drift = -0.0 dB

Peak SAR (extrapolated) = 3.77 W/kg

SAR(1 g) = 2.12 mW/g ; SAR(10 g) = 1.33 mW/g

Maximum value of SAR (measured) = 2.28 mW/g

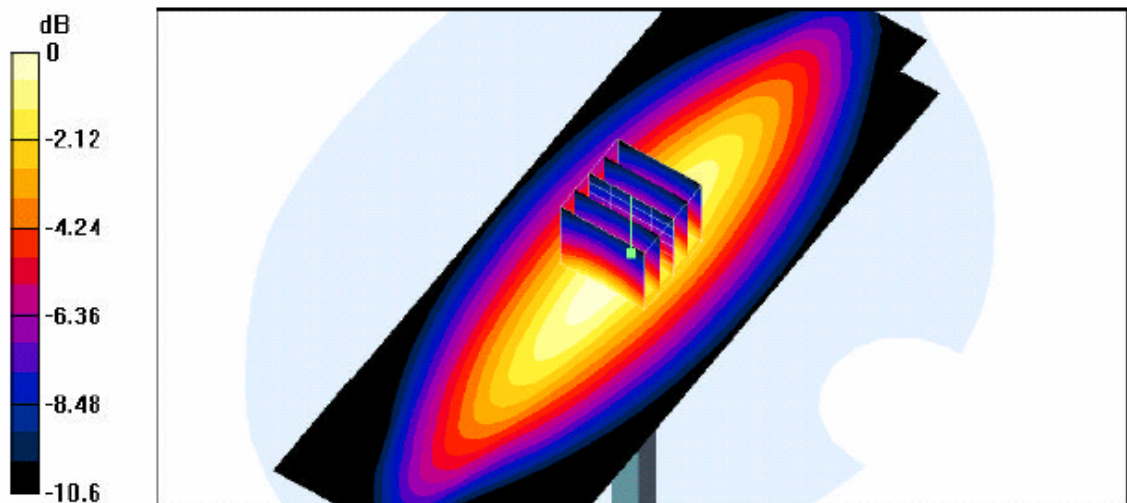

0 dB = 2.28 mW/g

Head-Tissue-Simulating-Liquid 450MHz (2005/02/04)

Date/Time: 02/04/05 09:30:47

Test Laboratory: A Test Lab Techno Corp.

System Performance Check at 450MHz_Body_

DUT: Dipole 450 MHz; Type: D450V2; Serial: D450V2 - SN:1021

Communication System: CW; Frequency: 450 MHz; Duty Cycle: 1:1

Medium: Body 450MHz Medium parameters used: $f = 450$ MHz; $s = 0.973$ mho/m; $\epsilon_r = 56.6$;

Conductivity = 1000 kg/m³; Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.19, 7.19, 7.19); Calibrated: 1/17/2005
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (61x181x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 2.26 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 48.8 V/m; Power Drift = -0.0 dB

Peak SAR (extrapolated) = 3.81 W/kg


SAR(1 g) = 2.12 mW/g; SAR(10 g) = 1.32 mW/g

Maximum value of SAR (measured) = 2.26 mW/g

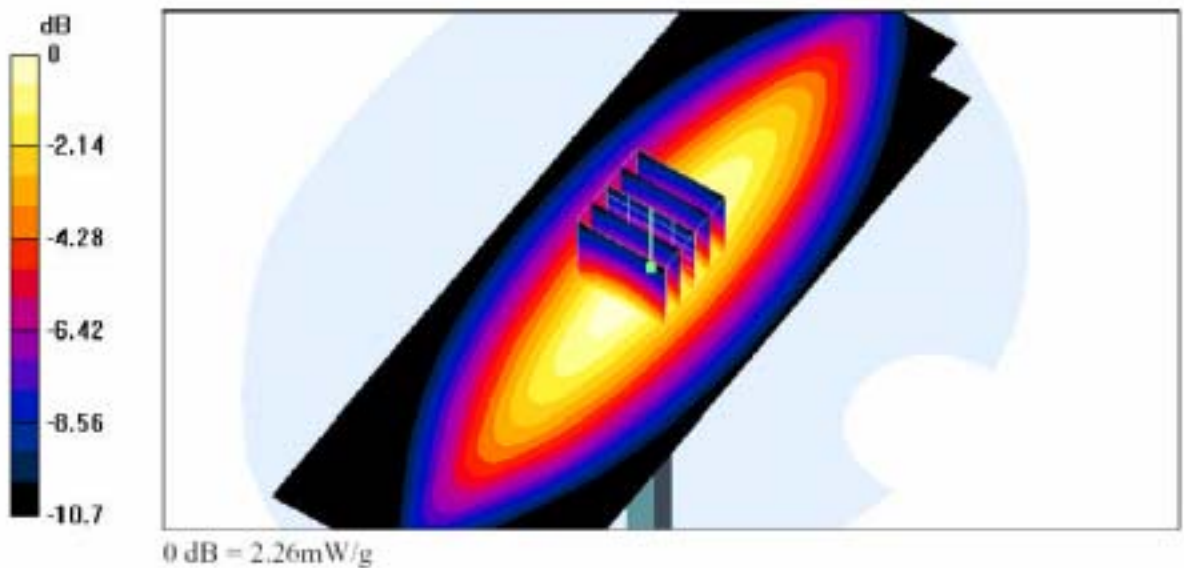


Muscle-Tissue-Simulating-Liquid 450MHz (2005/02/04)

Z-axis Plot of System Performance Check

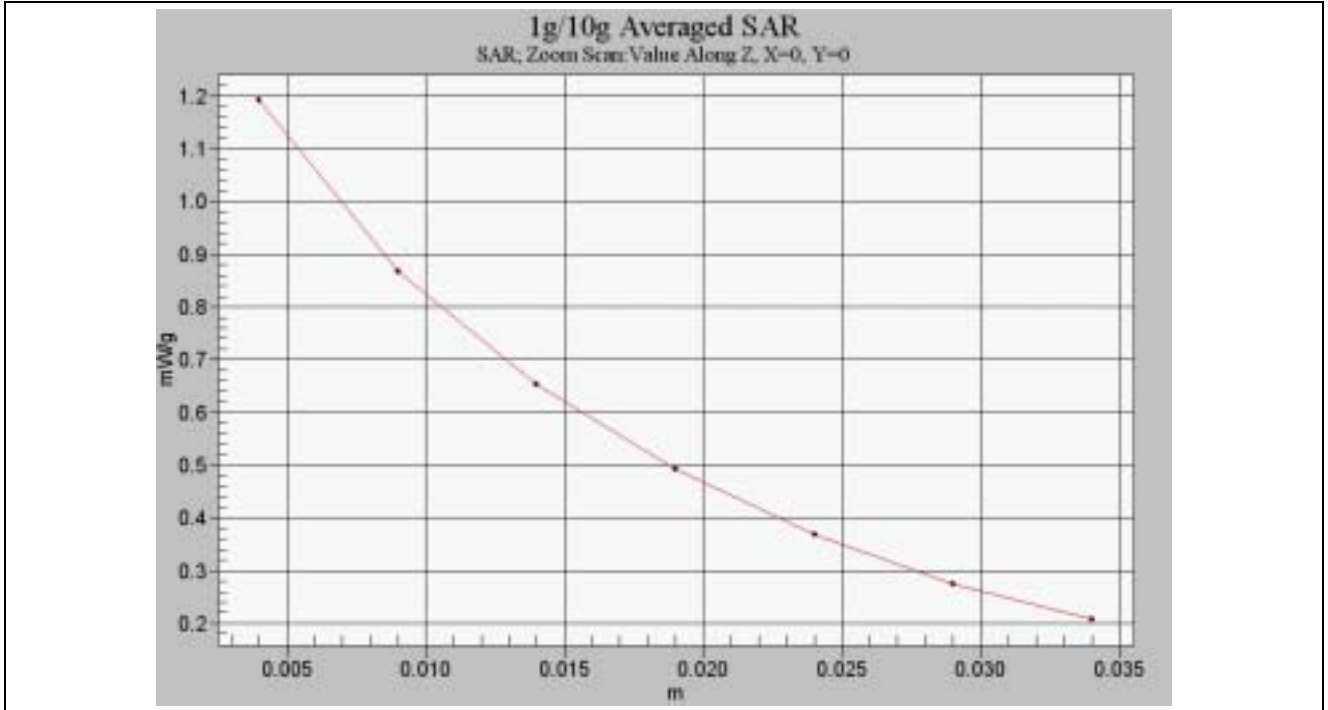

Head-Tissue-Simulating-Liquid 450MHz (2005/02/04)

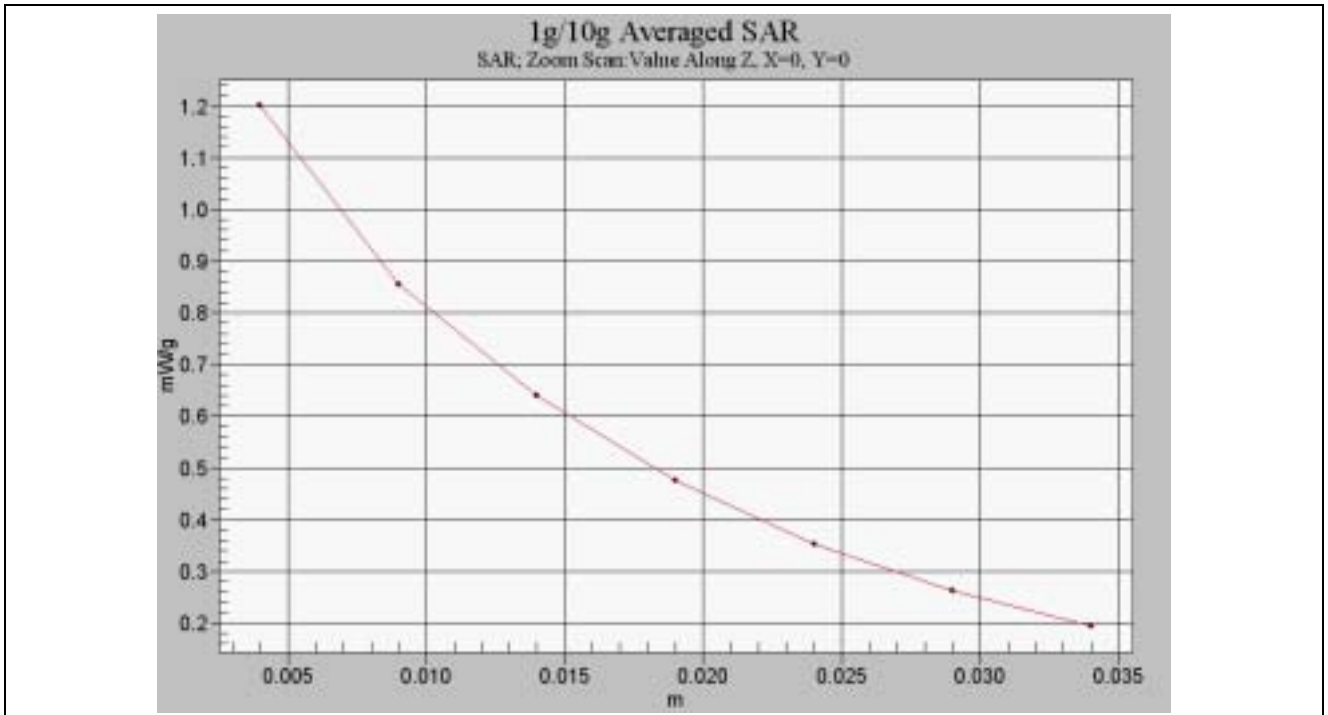

Muscle-Tissue-Simulating-Liquid 450MHz (2005/02/04)

Appendix B – SAR Measurement Data

Date/Time: 02/04/05 11:48:34

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_GMRS CH15_20050204_Brain_15mm_

DUT: FV 500; Type: Two way radio;

Communication System: GMRS; Frequency: 462.55 MHz;Duty Cycle: 1:1

Medium: Head 450MHz Medium parameters used (interpolated): f = 462.55 MHz; $\sigma = 0.84$ mho/m; $\epsilon_r = 45.4$;

Conductivity = 1000 kg/m³

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; CorrF(7.27, 7.27, 7.27); Calibrated: 1/17/2005
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x131x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.789 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 31.7 V/m; Power Drift = -0.5 dB

Peak SAR (extrapolated) = 1.14 W/kg

SAR(1 g) = 0.733 mW/g; SAR(10 g) = 0.509 mW/g

Maximum value of SAR (measured) = 0.773 mW/g

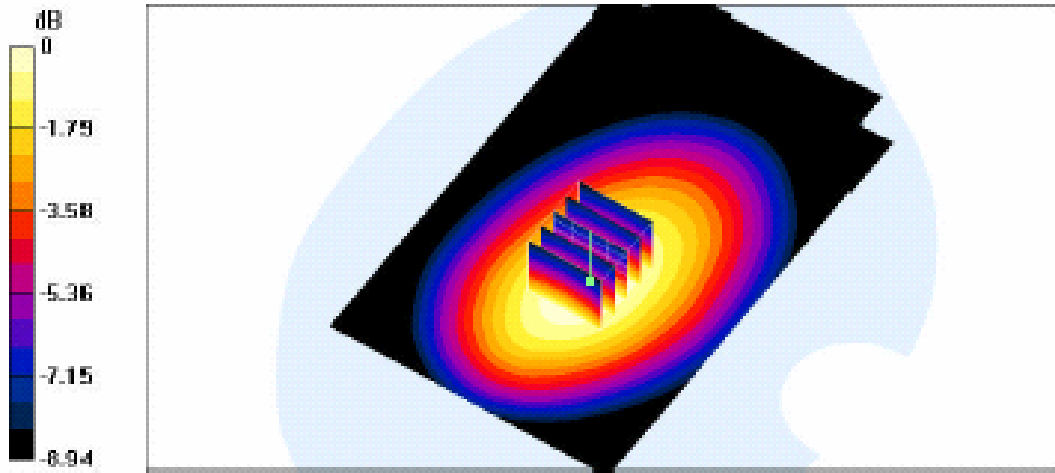

SAR Test Result for GMRS Face SAR -1.5 cm Spacing-Channel 15

Date/Time: 02/04/05 12:43:47

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_GMRS CH4_20050204_Brain_15mm_

DUT: FV 500; Type: Two way radio;

Communication System: GMRS; Frequency: 462.637 MHz; Duty Cycle: 1:1
Medium: Head 450MHz Medium parameters used (interpolated): $f = 462.637$ MHz; $s = 0.84$ mho/m; $\epsilon_r = 45.4$;

Conductivity = 1000 kg/m^3
Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; CorrF(7.27, 7.27, 7.27); Calibrated: 1/17/2005
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 1.30


Flat/Area Scan (81x131x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.819 mW/g

Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 31.7 V/m; Power Drift = -0.5 dB
Peak SAR (extrapolated) = 1.15 W/kg
SAR(1 g) = 0.755 mW/g; SAR(10 g) = 0.529 mW/g

Maximum value of SAR (measured) = 0.795 mW/g

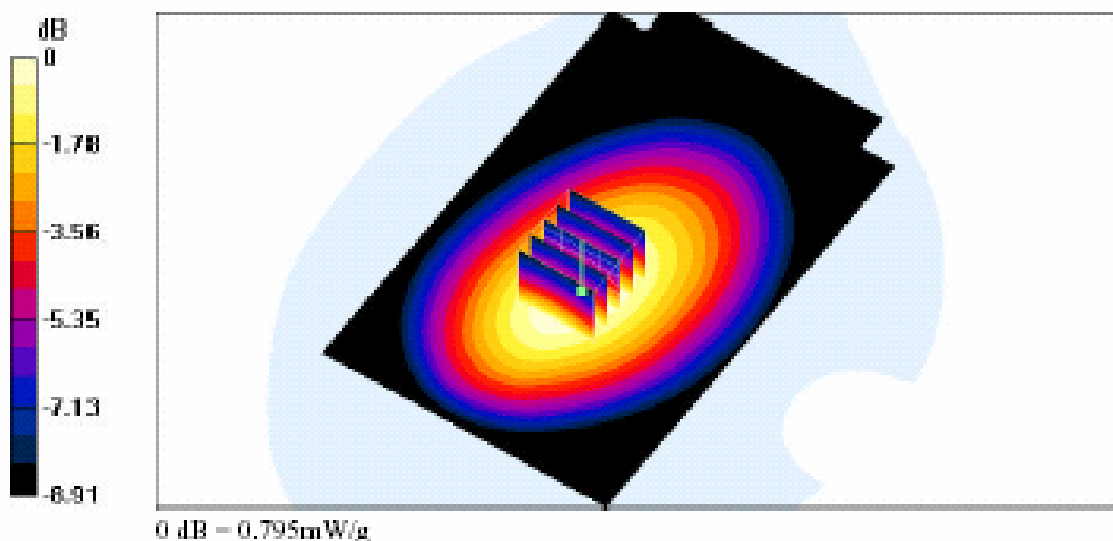

SAR Test Result for GMRS Face SAR -1.5 cm Spacing-Channel 4

Date/Time: 02/04/05 10:32:05

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_GMRS CH22_20050204_Brain_15mm_

DUT: FV 500; Type: Two way radio;

Communication System: GMRS; Frequency: 462.75 MHz;Duty Cycle: 1:1

Medium: Head 450MHz Medium parameters used (interpolated): $f = 462.75$ MHz; $s = 0.84$ mho/m; $\epsilon_r = 45.4$;

Conductivity = 1000 kg/m^3

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.27, 7.27, 7.27); Calibrated: 1/17/2005
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.763 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 30.2 V/m; Power Drift = -0.5 dB

Peak SAR (extrapolated) = 1.06 W/kg

SAR(1 g) = 0.694 mW/g; SAR(10 g) = 0.488 mW/g

Maximum value of SAR (measured) = 0.727 mW/g

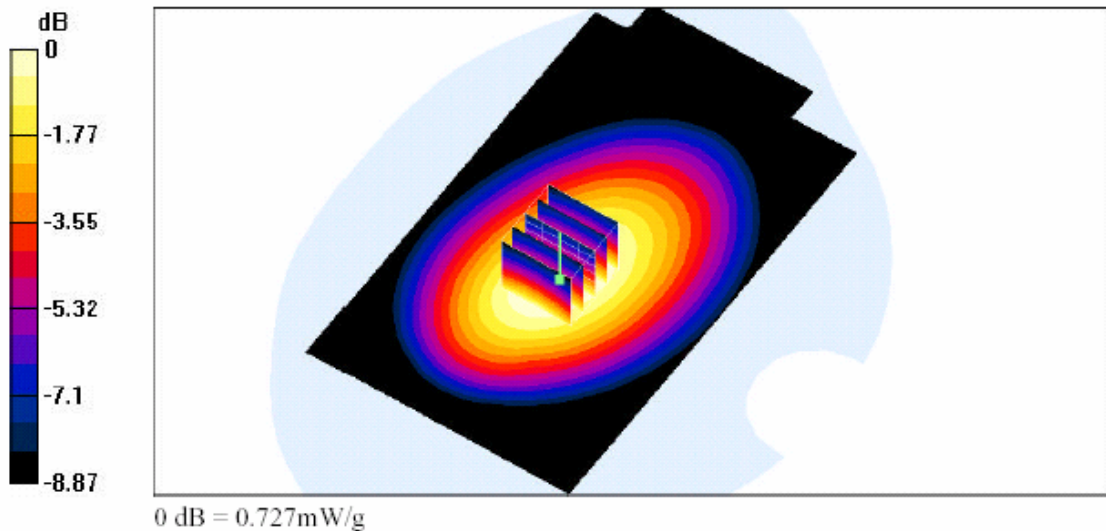

SAR Test Result for GMRS Face SAR -1.5 cm Spacing-Channel 22

Date/Time: 02/04/05 13:26:05

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_FRS CH8_20050204_Brain_15mm_

DUT: FV 500; Type: Two way radio;

Communication System: FRS; Frequency: 467.563 MHz;Duty Cycle: 1:1

Medium: Head 450MHz Medium parameters used (interpolated): $f = 467.563$ MHz; $s = 0.844$ mho/m; $\epsilon_p = 45.3$;

Conductivity = 1000 kg/m^3

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.27, 7.27, 7.27); Calibrated: 1/17/2005

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009

- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.318 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 19.1 V/m; Power Drift = -0.3 dB

Peak SAR (extrapolated) = 0.462 W/kg

SAR(1 g) = 0.295 mW/g; SAR(10 g) = 0.205 mW/g

Maximum value of SAR (measured) = 0.310 mW/g

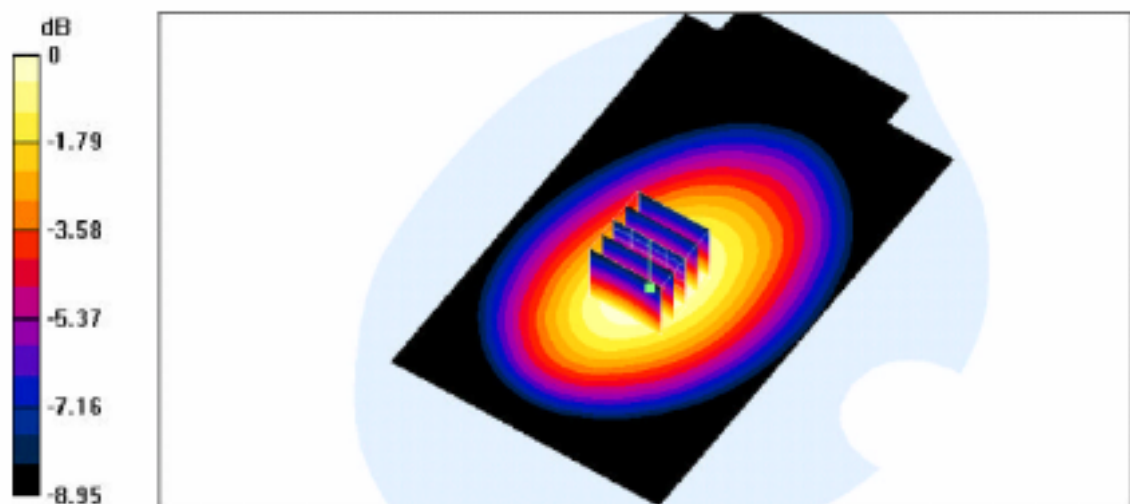

0 dB = 0.310mW/g

SAR Test Result for FRS Face SAR -1.5 cm Spacing-Channel 8

Date/Time: 02/04/05 14:18:48

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_FRS CH11_20050204_Brain_15mm_

DUT: FV 500; Type: Two way radio;

Communication System: FRS; Frequency: 467.637 MHz; Duty Cycle: 1:1

Medium: Head 450MHz Medium parameters used (interpolated): $f = 467.637 \text{ MHz}$; $s = 0.844 \text{ mho/m}$; $\epsilon_r = 45.3$;

Conductivity = 1000 kg/m^3

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.27, 7.27, 7.27); Calibrated: 1/17/2005

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009

- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.301 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 18.6 V/m; Power Drift = -0.5 dB

Peak SAR (extrapolated) = 0.424 W/kg

SAR(1 g) = 0.274 mW/g; SAR(10 g) = 0.191 mW/g

Maximum value of SAR (measured) = 0.287 mW/g

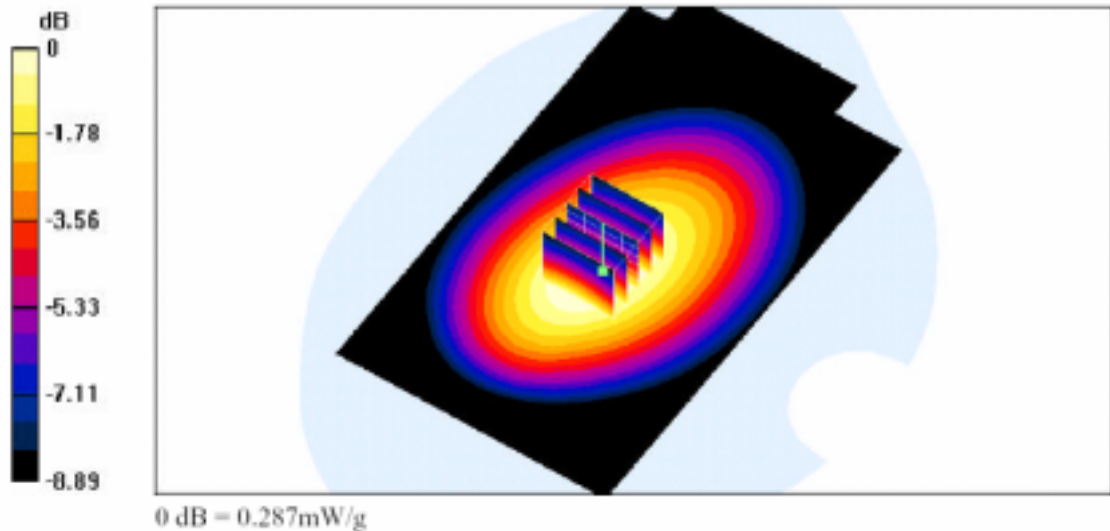

SAR Test Result for FRS Face SAR -1.5 cm Spacing-Channel 11

Date/Time: 02/04/05 15:11:08

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_FRS CH14_20050204_Brain_15mm_

DUT: FV 500; Type: Two way radio;

Communication System: FRS; Frequency: 467.712 MHz;Duty Cycle: 1:1

Medium: Head 450MHz Medium parameters used (interpolated): $f = 467.712$ MHz; $s = 0.845$ mho/m; $\epsilon_r = 45.3$;

Conductivity = 1000 kg/m^3

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.27, 7.27, 7.27); Calibrated: 1/17/2005
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.337 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 19.2 V/m; Power Drift = -0.6 dB

Peak SAR (extrapolated) = 0.462 W/kg

SAR(1 g) = 0.302 mW/g; SAR(10 g) = 0.213 mW/g

Maximum value of SAR (measured) = 0.315 mW/g

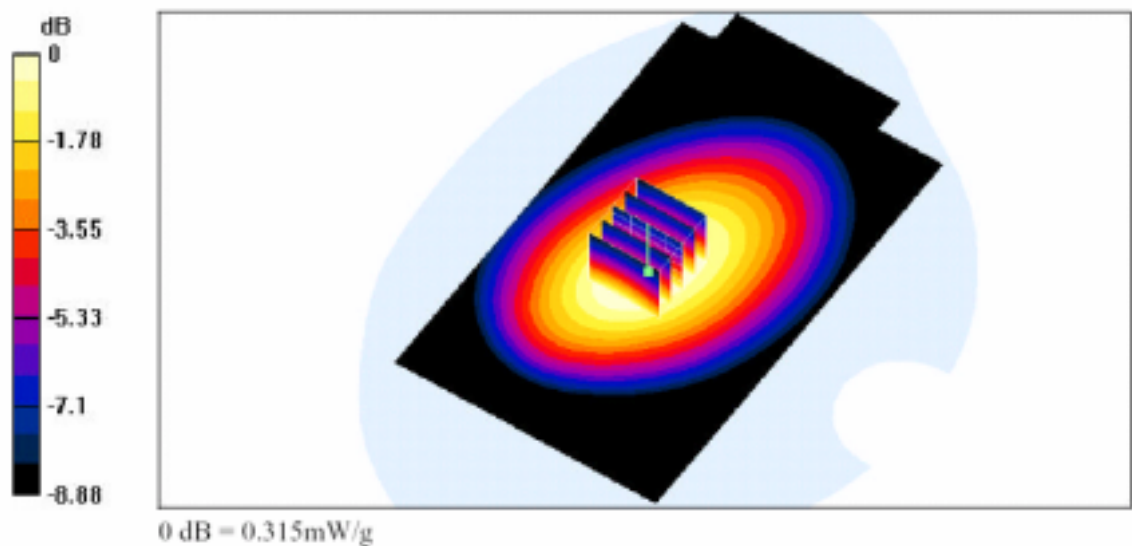

SAR Test Result for FRS Face SAR -1.5 cm Spacing-Channel 14

Date/Time: 02/04/05 15:58:46

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_GMRS CH15_20050204_muscle_Headset_

DUT: FV 500; Type: Two way radio;

Communication System: GMRS; Frequency: 462.55 MHz;Duty Cycle: 1:1

Medium: Body 450MHz Medium parameters used (interpolated): $f = 462.55$ MHz; $s = 0.983$ mho/m; $\epsilon_r = 56.4$;

Conductivity = 1000 kg/m^3

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.19, 7.19, 7.19); Calibrated: 1/17/2005
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.547 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 23.3 V/m; Power Drift = -0.4 dB

Peak SAR (extrapolated) = 0.774 W/kg

SAR(1 g) = 0.499 mW/g; SAR(10 g) = 0.349 mW/g

Maximum value of SAR (measured) = 0.523 mW/g

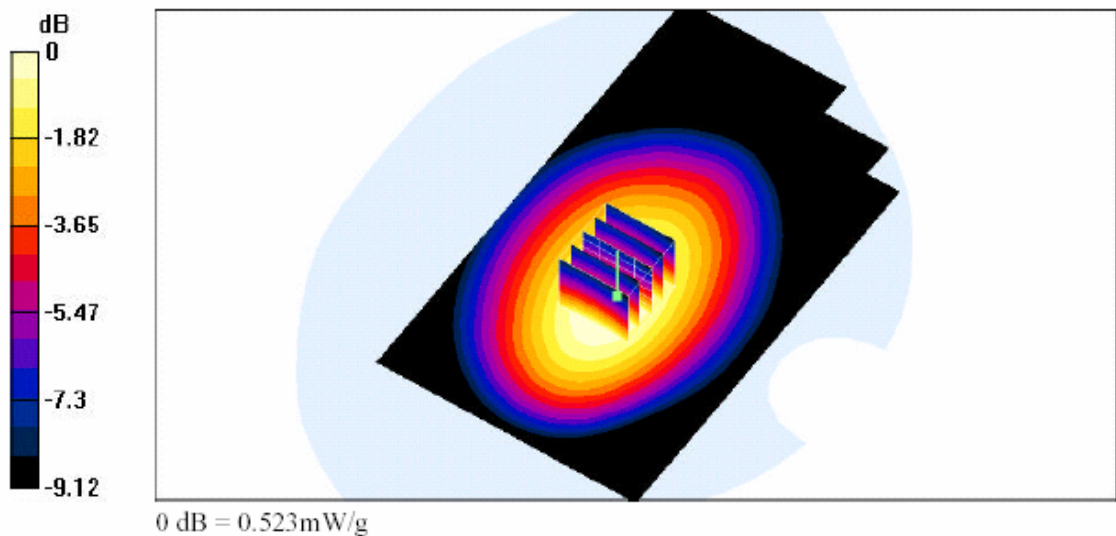

SAR Test Result for GMRS Body SAR w / Belt -clip Channel 15

Date/Time: 02/04/05 16:49:14

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_GMRS CH4_20050204_muscle_Headset_

DUT: FV 500; Type: Two way radio;

Communication System: GMRS; Frequency: 462.637 MHz;Duty Cycle: 1:1

Medium: Body 450MHz Medium parameters used (interpolated): $f = 462.637$ MHz; $s = 0.983$ mho/m; $\epsilon_r = 56.4$;

Conductivity – 1000 kg/m^3

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.19, 7.19, 7.19); Calibrated: 1/17/2005

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009

- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) – 0.520 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value – 22.8 V/m; Power Drift – -0.5 dB

Peak SAR (extrapolated) – 0.763 W/kg

SAR(1 g) – 0.490 mW/g; SAR(10 g) – 0.342 mW/g

Maximum value of SAR (measured) – 0.513 mW/g

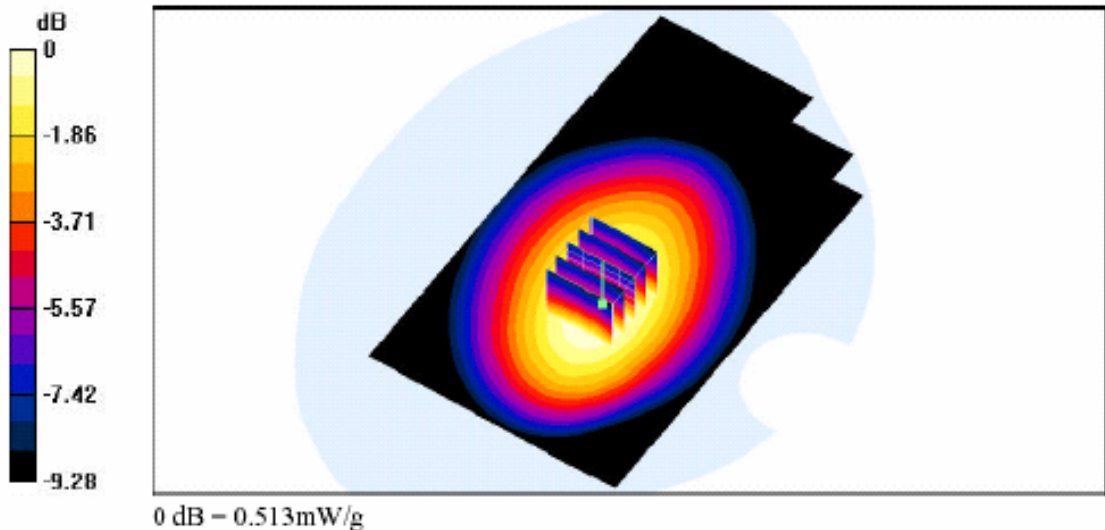

SAR Test Result for GMRS Body SAR w / Belt –clip Channel 4

Date/Time: 02/04/05 17:22:39

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_GMRS CH22_20050204_muscle_Headset_

DUT: FV 500; Type: Two way radio;

Communication System: GMRS; Frequency: 462.75 MHz;Duty Cycle: 1:1
Medium: Body 450MHz Medium parameters used (interpolated): $f = 462.75$ MHz; $s = 0.984$ mho/m; $\epsilon_r = 56.4$;

Conductivity – 1000 kg/m^3
Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.19, 7.19, 7.19); Calibrated: 1/17/2005
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) – 0.436 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value – 20.6 V/m; Power Drift – -0.4 dB

Peak SAR (extrapolated) – 0.612 W/kg

SAR(1 g) – 0.396 mW/g; SAR(10 g) – 0.279 mW/g

Maximum value of SAR (measured) – 0.415 mW/g

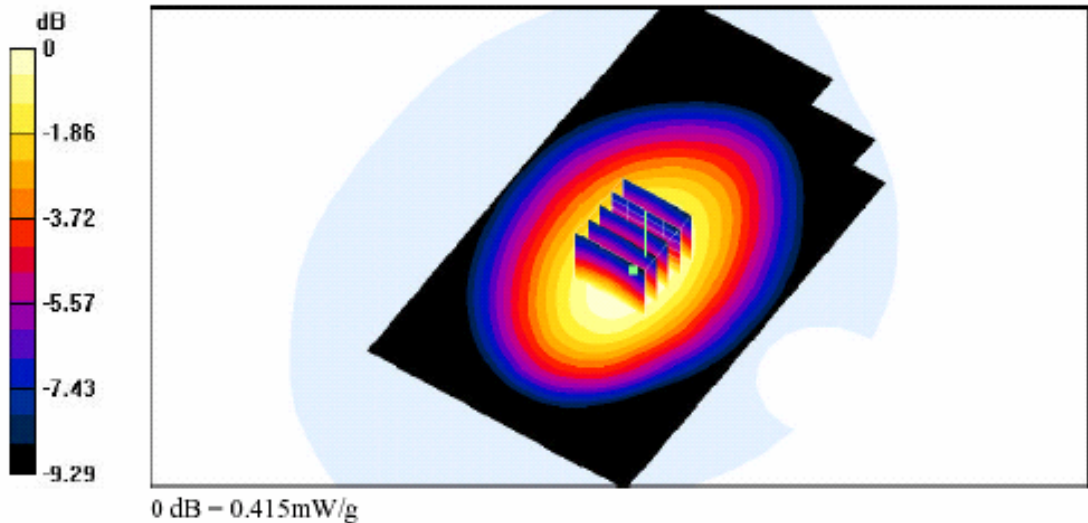

SAR Test Result for GMRS Body SAR w / Belt –clip Channel 22

Date/Time: 02/04/05 18:37:46

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_FRS CH8_20050204_muscle_Headset_

DUT: FV 500; Type: Two way radio;

Communication System: FRS; Frequency: 467.563 MHz;Duty Cycle: 1:1

Medium: Body 450MHz Medium parameters used (interpolated): $f = 467.563$ MHz; $s = 0.987$ mho/m; $\epsilon_r = 56.3$;

Conductivity – 1000 kg/m^3

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.19, 7.19, 7.19); Calibrated: 1/17/2005

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009

- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) – 0.185 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value – 13.2 V/m; Power Drift – -0.3 dB

Peak SAR (extrapolated) – 0.262 W/kg

SAR(1 g) – 0.172 mW/g; SAR(10 g) – 0.120 mW/g

Maximum value of SAR (measured) – 0.179 mW/g

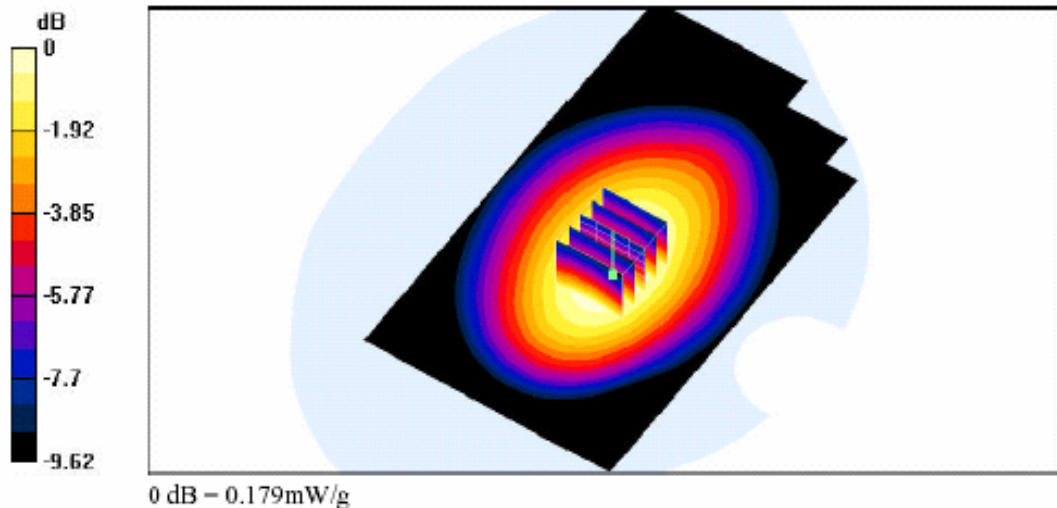

SAR Test Result for FRS Body SAR w / Belt –clip Channel 8

Date/Time: 02/04/05 19:20:30

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_FRS CH11_20050204_muscle_Headset_

DUT: FV 500; Type: Two way radio;

Communication System: FRS; Frequency: 467.637 MHz; Duty Cycle: 1:1

Medium: Body 450MHz Medium parameters used (interpolated): $f = 467.637$ MHz; $s = 0.987$ mho/m; $\epsilon_r = 56.3$;

Conductivity = 1000 kg/m^3

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.19, 7.19, 7.19); Calibrated: 1/17/2005
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.143 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 11.6 V/m; Power Drift = -0.4 dB

Peak SAR (extrapolated) = 0.208 W/kg

SAR(1 g) = 0.132 mW/g; SAR(10 g) = 0.091 mW/g

Maximum value of SAR (measured) = 0.140 mW/g

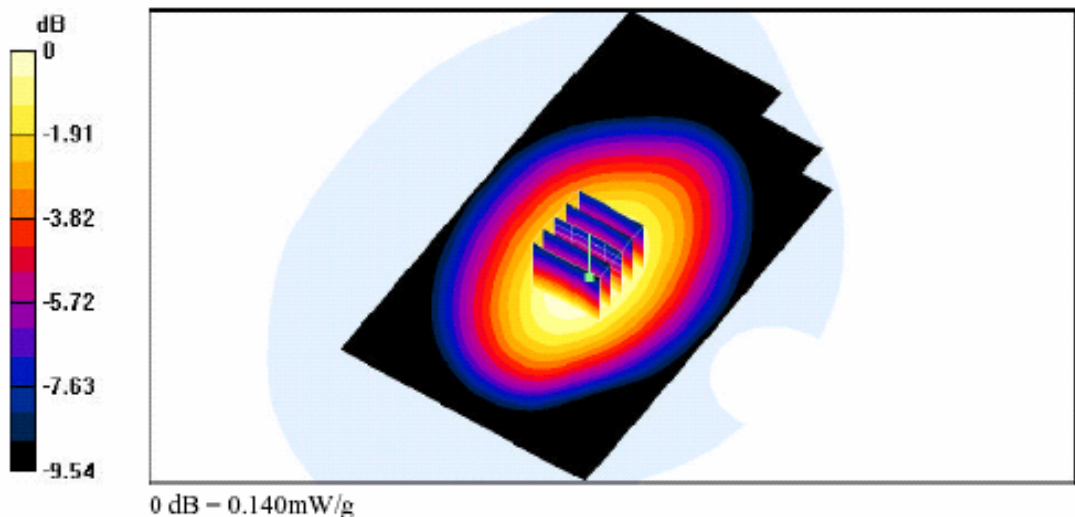

SAR Test Result for FRS Body SAR w / Belt –clip Channel 11

Date/Time: 02/04/05 20:23:28

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_FRS CH14_20050204_muscle_Headset_

DUT: FV 500; Type: Two way radio;

Communication System: FRS; Frequency: 467.712 MHz;Duty Cycle: 1:1

Medium: Body 450MHz Medium parameters used (interpolated): $f = 467.712$ MHz; $s = 0.988$ mho/m; $\epsilon_r = 56.3$;

Conductivity - 1000 kg/m^3

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.19, 7.19, 7.19); Calibrated: 1/17/2005
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) - 0.166 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value - 12.7 V/m; Power Drift - -0.4 dB

Peak SAR (extrapolated) - 0.237 W/kg

SAR(1 g) - 0.152 mW/g; SAR(10 g) - 0.106 mW/g

Maximum value of SAR (measured) - 0.159 mW/g

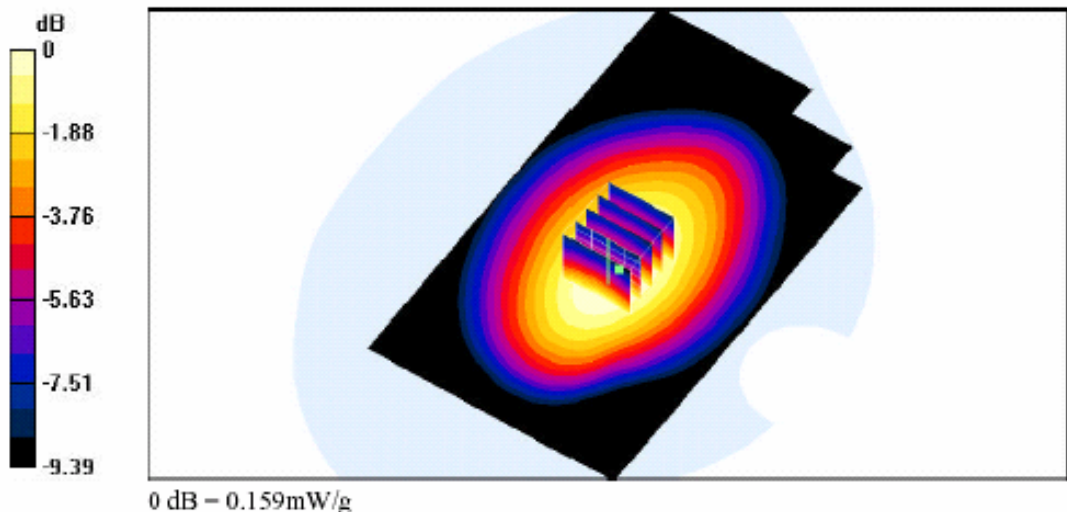

SAR Test Result for FRS Body SAR w / Belt -clip Channel 14

Date/Time: 02/04/05 21:13:21

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_GMRS CH4_20050204_muscle_15mm_

DUT: FV 500; Type: Two way radio;

Communication System: GMRS; Frequency: 462.637 MHz;Duty Cycle: 1:1

Medium: Body 450MHz Medium parameters used (interpolated): $f = 462.637$ MHz; $s = 0.983$ mho/m; $\epsilon_r = 56.4$;

Conductivity – 1000 kg/m^3

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.19, 7.19, 7.19); Calibrated: 1/17/2005

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009

- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) – 0.734 mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value – 26.3 V/m; Power Drift – -0.7 dB

Peak SAR (extrapolated) – 1.01 W/kg

SAR(1 g) – 0.662 mW/g; SAR(10 g) – 0.465 mW/g

Maximum value of SAR (measured) – 0.693 mW/g

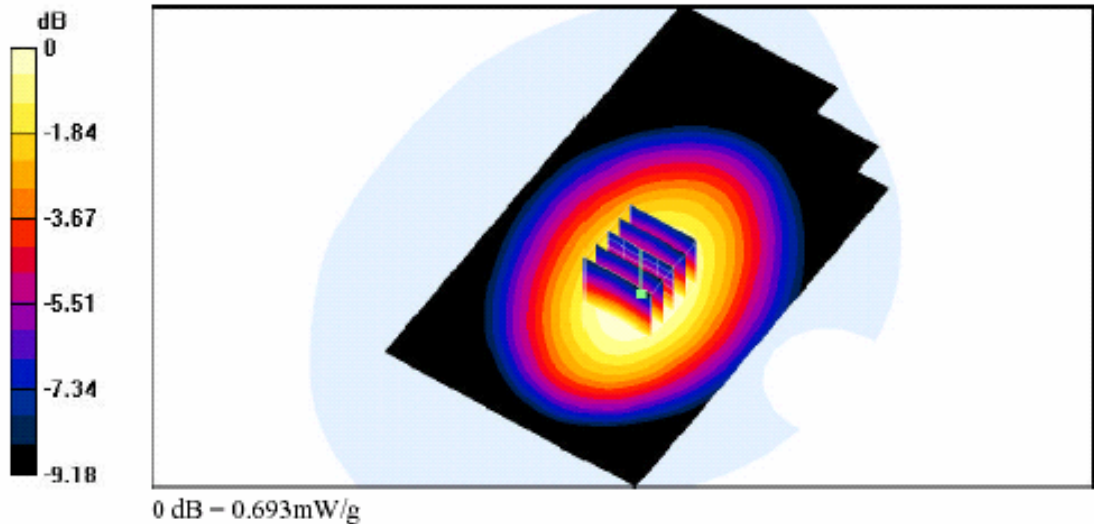

SAR Test Result for GMRS Body SAR w / out Belt –clip -1.5cm Channel 4

Date/Time: 02/04/05 22:05:08

Test Laboratory: A Test Lab Techno Corp.

05-0037-S_FV 500_Flat_FRS CH11_20050204_muscle_15mm_

DUT: FV 500; Type: Two way radio;

Communication System: FRS; Frequency: 467.637 MHz; Duty Cycle: 1:1

Medium: Body 450MHz Medium parameters used (interpolated): $f = 467.637$ MHz; $s = 0.987$ mho/m; $\epsilon_r = 56.3$;

Conductivity $= 1000$ kg/m³

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530-LF; ConvF(7.19, 7.19, 7.19); Calibrated: 1/17/2005

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009

- Measurement SW: DASY4, V4.4 Build 3; Postprocessing SW: SEMCAD, V1.8 Build 130

Flat/Area Scan (81x141x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) $= 0.290$ mW/g


Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value $= 16$ V/m; Power Drift $= -0.4$ dB

Peak SAR (extrapolated) $= 0.413$ W/kg

SAR(1 g) $= 0.266$ mW/g; SAR(10 g) $= 0.186$ mW/g

Maximum value of SAR (measured) $= 0.276$ mW/g

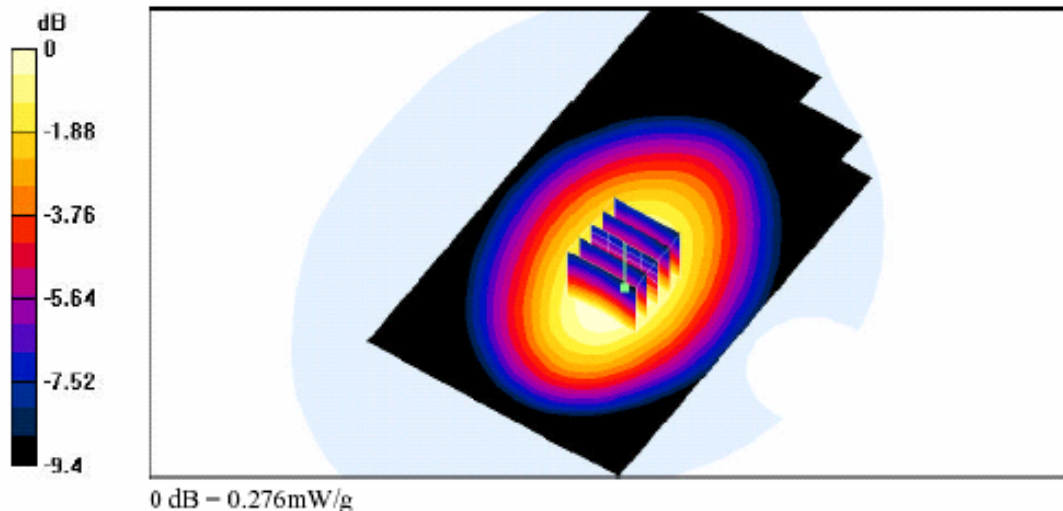

SAR Test Result for FRS Body SAR w / out Belt -clip -1.5cm Channel 11

Appendix C – Dipole Calibration

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8064 Zurich, Switzerland

S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Auden**

Certificate No: **D450V2-1021_Feb05**

CALIBRATION CERTIFICATE

Object:	D450V2 - SN: 1021
Calibration procedure(s):	QA CAL-15.v4 Calibration Procedure for dipole validation kits below 800 MHz
Calibration date:	February 1, 2005
Condition of the calibrated item:	In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 75%.

Calibration Equipment used (M&E critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	G041293874	5-May-04 (METAS, No. 251-00388)	May-05
Power sensor E4412A	MY41495277	5-May-04 (METAS, No. 251-00388)	May-05
Reference 3 dB Attenuator	SN: 55054 (3c)	10-Aug-04 (METAS, No. 251-00403)	Aug-05
Reference 20 dB Attenuator	SN: 55086 (20c)	3-May-04 (METAS, No. 251-00389)	May-05
Reference Probe ET3DV6	SN 1507	26-Oct-04 (SPEAG, No. ET3-1507_Oct04)	Oct-05
DAE4	SN: 901	29-Jun-04 (SPEAG, No. DAE4-901_Jun04)	Jun-05

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092180	18-Sep-02 (SPEAG, in house check Oct-03)	In house check: Oct-05
RF generator HP 8648C	US3642U01700	4-Aug-05 (SPEAG, in house check Dec-03)	In house check: Dec-05
Network Analyzer HP 8733E	US37300585	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov-05

Calibrated by: **Nico Vetterli**
Name: Nico Vetterli
Function: Laboratory Technician

Approved by: **Kolja Pokovic**
Name: Kolja Pokovic
Function: Technical Manager

Signature: *Nico Vetterli*
Kolja Pokovic

Issued: February 1, 2005

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D450V2-1021_Feb05

Page 1 of 9

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
S Service suisse d'étalonnage
C Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- d) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.3
Extrapolation	Advanced Extrapolation	
Phantom	Flat Phantom V4.4	Shell thickness: 6 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Area Scan resolution	dx, dy = 15 mm	
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.87 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	45.1 ± 6 %	0.87 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	398 mW input power	2.01 mW / g
SAR normalized	normalized to 1W	5.06 mW / g
SAR for nominal Head TSL parameters [†]	normalized to 1W	5.13 mW / g ± 18.1 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	398 mW input power	1.32 mW / g
SAR normalized	normalized to 1W	3.32 mW / g
SAR for nominal Head TSL parameters [†]	normalized to 1W	3.36 mW / g ± 17.6 % (k=2)

[†] Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	56.7	0.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.6 ± 6 %	0.96 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm ² (1 g) of Body TSL	condition	
SAR measured	398 mW input power	2.14 mW / g
SAR normalized	normalized to 1W	5.36 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	5.26 mW / g ± 18.1 % (k=2)

SAR averaged over 10 cm ² (10 g) of Body TSL	condition	
SAR measured	398 mW input power	1.39 mW / g
SAR normalized	normalized to 1W	3.49 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	3.43 mW / g ± 17.6 % (k=2)

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	55.4 Ω - 6.5 j Ω
Return Loss	- 21.9 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	52.6 Ω - 8.3 j Ω
Return Loss	- 21.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	0.993 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	February 4, 2004

DASY4 Validation Report for Head TSL

Date/Time: 02/01/05 11:33:32

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz; Type: D450V2; Serial: D450V2 - SN:1021
Program Name: Unnamed Program


Communication System: CW; Frequency: 450 MHz; Duty Cycle: 1:1
Medium: HSL450 Medium parameters used: $f = 450$ MHz; $\sigma = 0.87$ mho/m; $\epsilon_r = 45.1$; $\rho = 1000$ kg/m³
Phantom section: Flat Section
Measurement Standard: DASY4 (High Precision Assessment)


DASY4 Configuration:

- Probe: ET3DA6 - SN1507; ConvF(6.94, 6.94, 6.94); Calibrated: 10/26/2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAB4 Sr901; Calibrated: 6/29/2004
- Phantom: Flat Phantom 4.4; Type: Flat Phantom 4.4; Serial: TP:1002
- Measurement SW: DASY4, V4.4 Build 13; Postprocessing SW: SEMCAD, V1.8 Build 136

d=15mm, Pin=398mW/Area Scan (71x181x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 2.11 mW/g

d=15mm, Pin=398mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 51.1 V/m; Power Drift = -0.1 dB
Peak SAR (extrapolated) = 3.23 W/kg
SAR(1 g) = 2.01 mW/g; SAR(10 g) = 1.32 mW/g
Maximum value of SAR (measured) = 2.15 mW/g

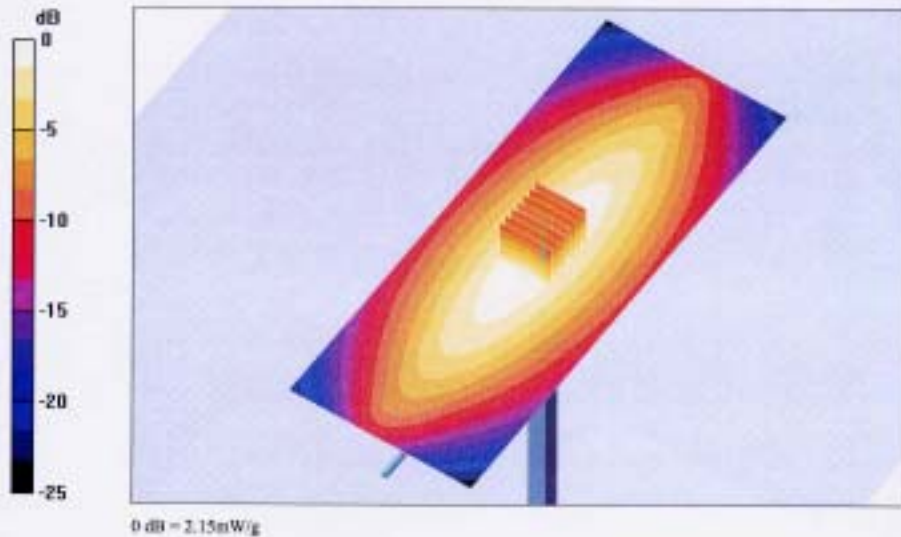

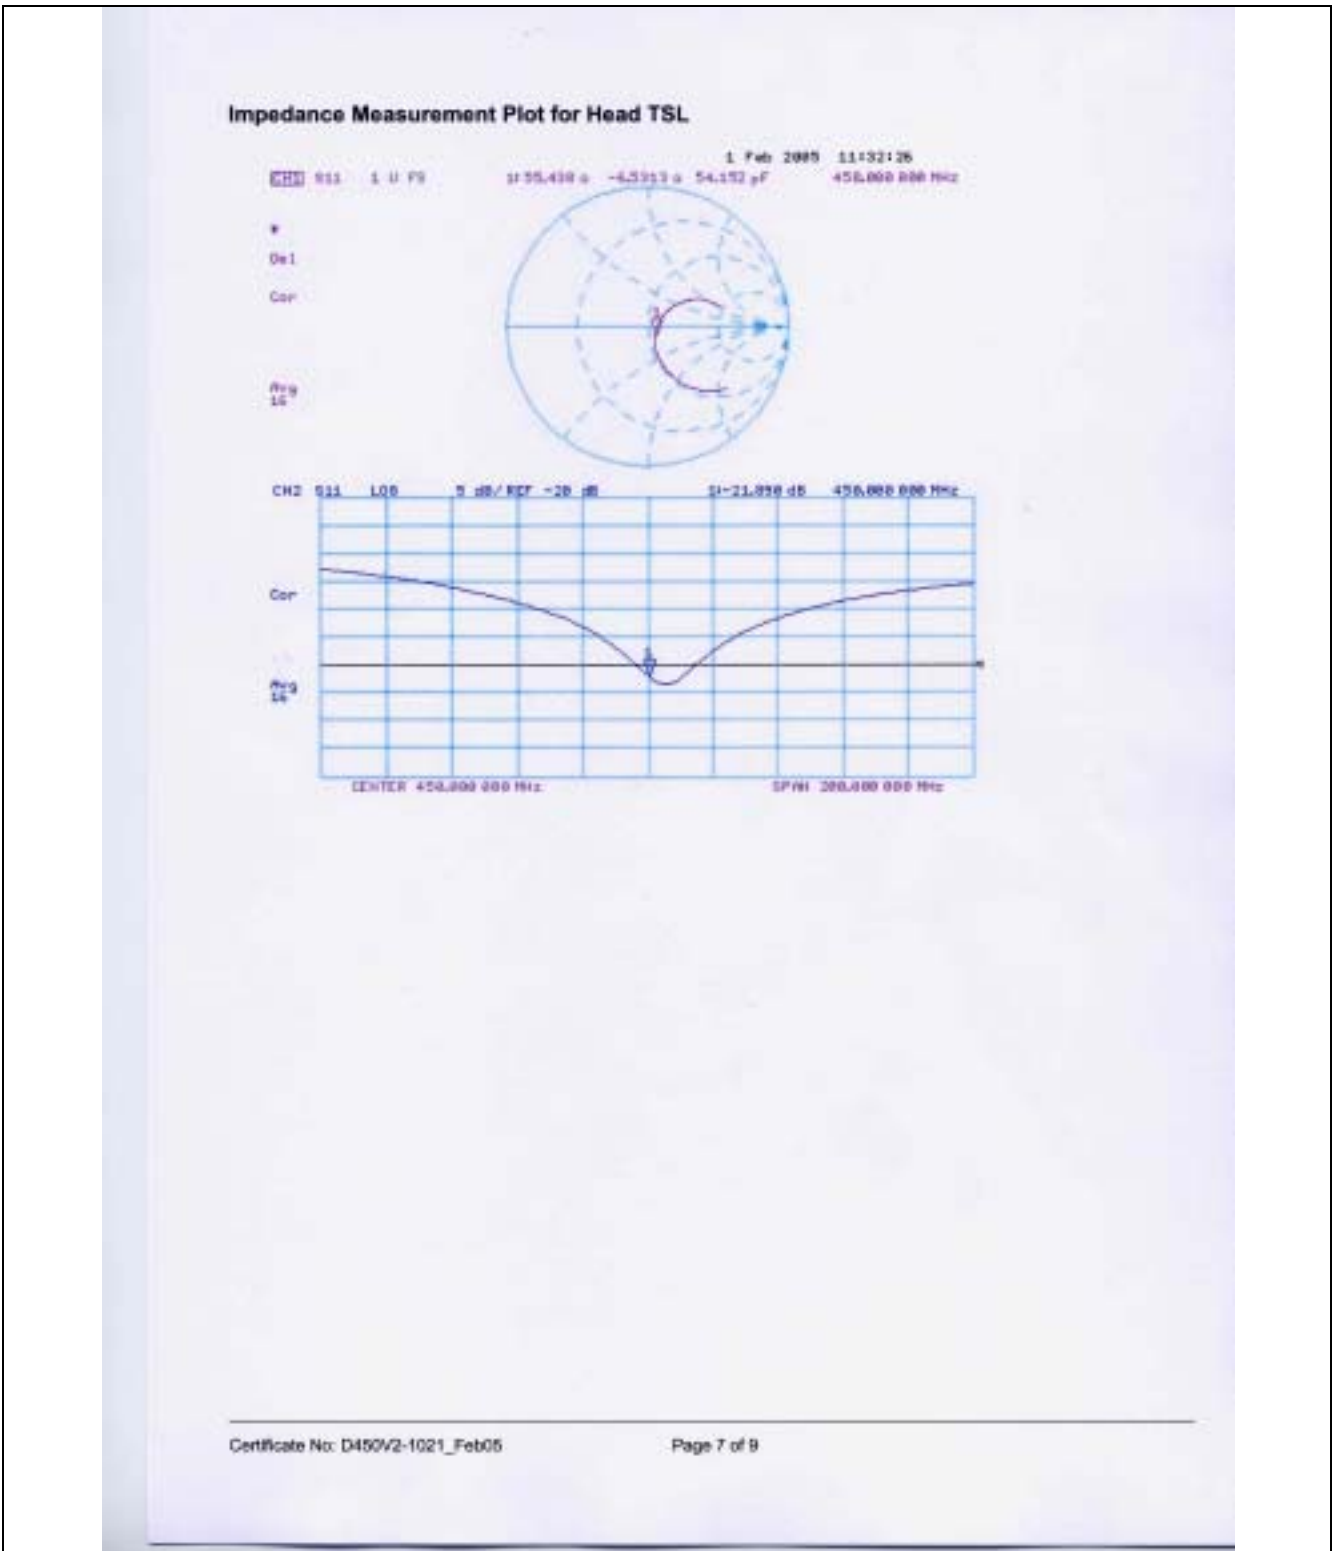

DASY4 Validation Report for Body TSL

Date/Time: 02/01/05 15:02:01

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz; Type: D450V2; Serial: D450V2 - SN:1021
Program Name: System Performance Check at 450 MHz

Communication System: CW; Frequency: 450 MHz; Duty Cycle: 1:1

Medium: MSL450 Medium parameters used: $f = 450$ MHz; $\sigma = 0.96$ mho/m; $\epsilon_r = 55.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507; ConvP[6.84, 6.84, 6.84]; Calibrated: 10/26/2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAB4 Sr901; Calibrated: 6/29/2004
- Phantom: Flat Phantom 4.4; Type: Flat Phantom 4.4; Serial: TP:1002
- Measurement SW: DASY4, V4.4 Build 13; Postprocessing SW: SEMCAD, V1.8 Build 136

d=15mm, Pin=398mW/Area Scan (61x161x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (interpolated) = 2.24 mW/g


d=15mm, Pin=398mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Reference Value = 48.8 V/m; Power Drift = -0.0 dB

Peak SAR (extrapolated) = 3.54 W/kg

SAR(1 g) = 2.14 mW/g; SAR(10 g) = 1.39 mW/g

Maximum value of SAR (measured) = 2.28 mW/g

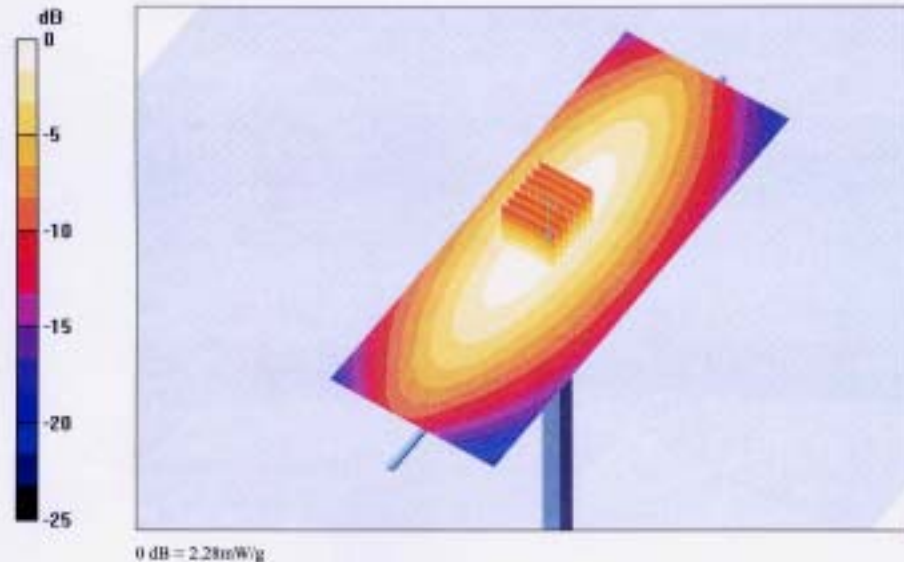

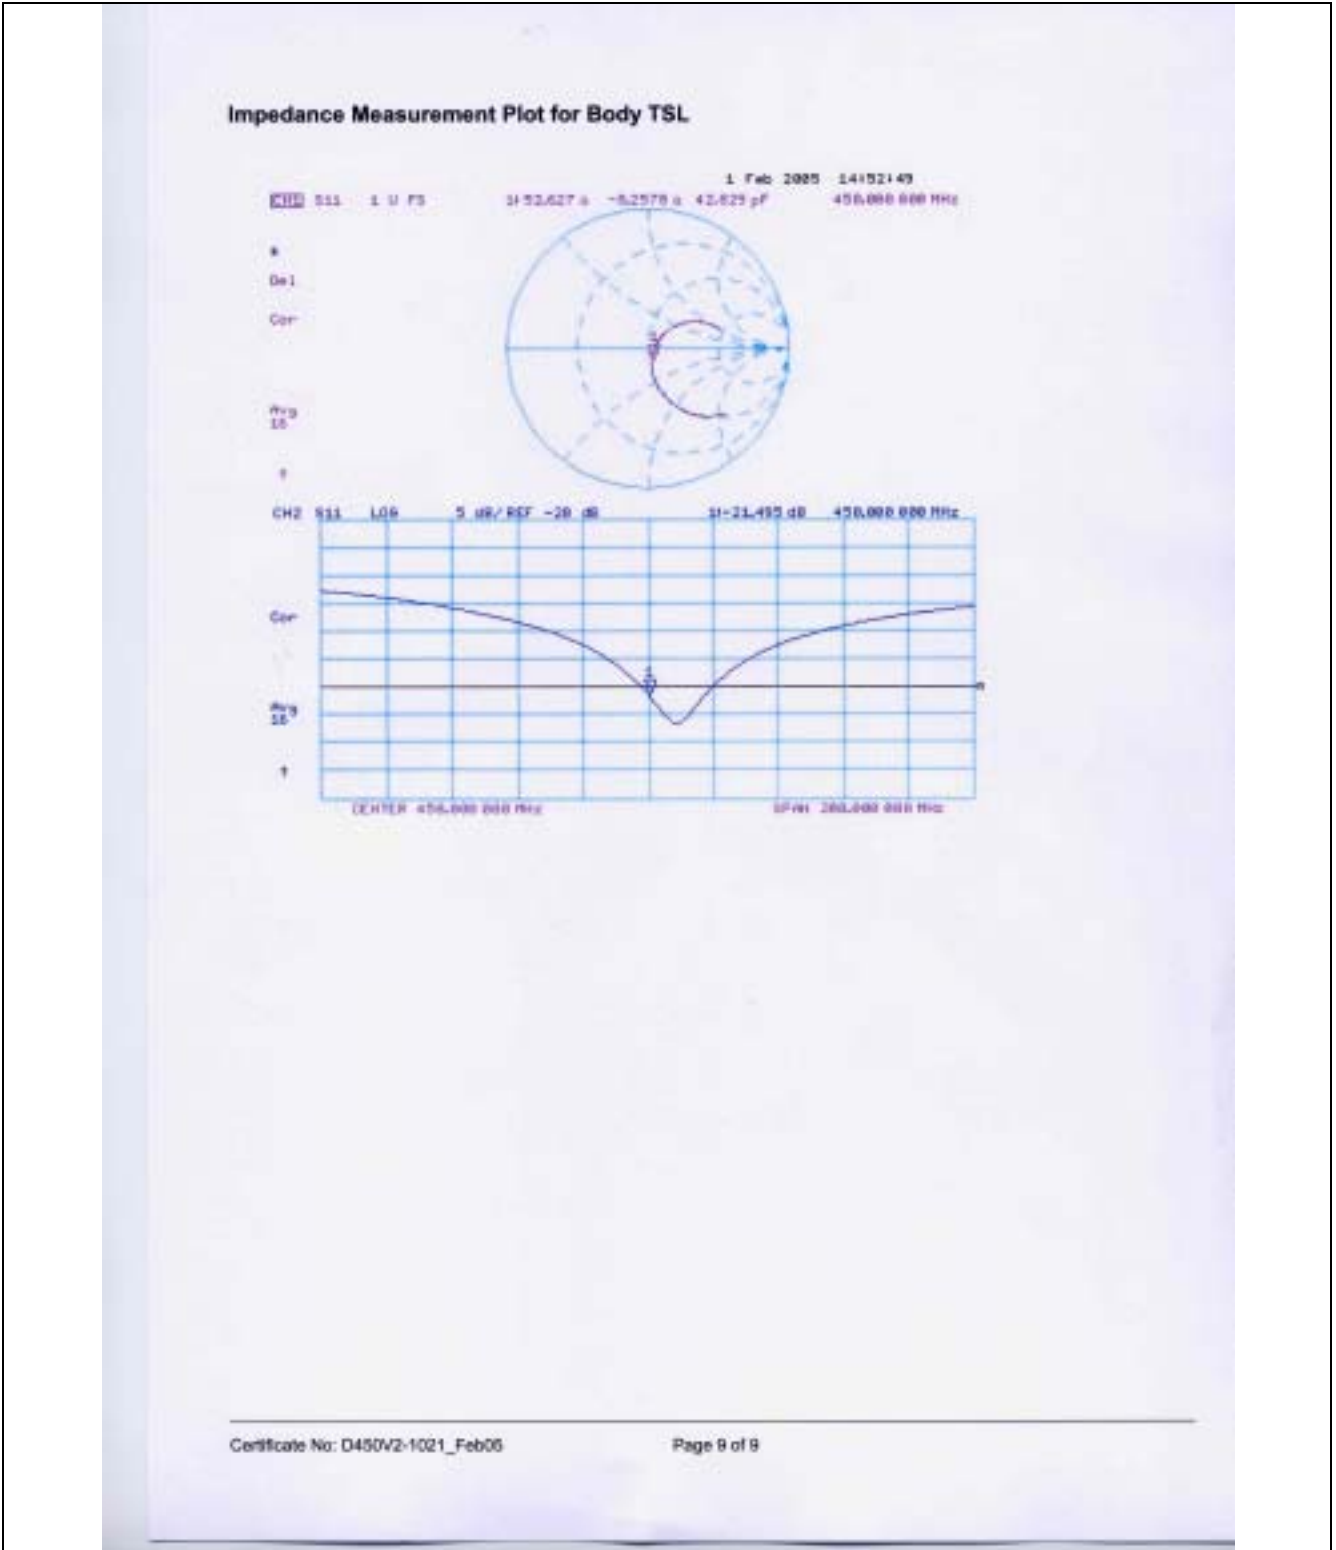

Appendix D – Probe Calibration

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland

S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client: **Auden**

Certificate No: **ET3-1530_Jan05**

CALIBRATION CERTIFICATE

Object: **ET3DV6 - SN:1530 (Additional Conversion Factors)**

Calibration procedure(s): **QA CAL-12 v4
Calibration procedure for dosimetric E-field probes**

Calibration date: **January 17, 2004**

Condition of the calibrated item: **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 0.1°C and humidity < 70%).

Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E44198	0841203874	5-May-04 (METAS, No. 251-00368)	May-05
Power sensor E4412A	MY141495277	5-May-04 (METAS, No. 251-00368)	May-05
Reference 3 dB Attenuator	SN: 55054 (3c)	10-Aug-04 (METAS, No. 251-00433)	Aug-05
Reference 20 dB Attenuator	SN: 55088 (30c)	3-May-04 (METAS, No. 251-00369)	May-05
Reference 30 dB Attenuator	SN: 55129 (30c)	10-Aug-04 (METAS, No. 251-00404)	Aug-05
Reference Probe ESSDV2	SN: 3013	7-Jan-05 (SPEAG, No. ESS-3013_Jan05)	Jan-06
DAE4	SN: 617	29-Sep-04 (SPEAG, No. DAE4-617_Sep04)	Sep-05

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY11062190	18-Sep-02 (SPEAG, in house check Oct-03)	In house check: Oct-05
HP generator HP 8648C	US38425J01700	4-Aug-09 (SPEAG, in house check Dec-03)	In house check: Dec-05
Network Analyzer HP 8753E	US37300686	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov-05

Calibrated by:

Name: **Kolja Pokovic** Function: **Technical Manager**

Signature: *[Signature]*

Approved by:

Name: **F. Borchert** Function: **R&D Director**


Signature: *[Signature]*

Issued: January 18, 2005

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ET3-1530_Jan05

Page 1 of 5

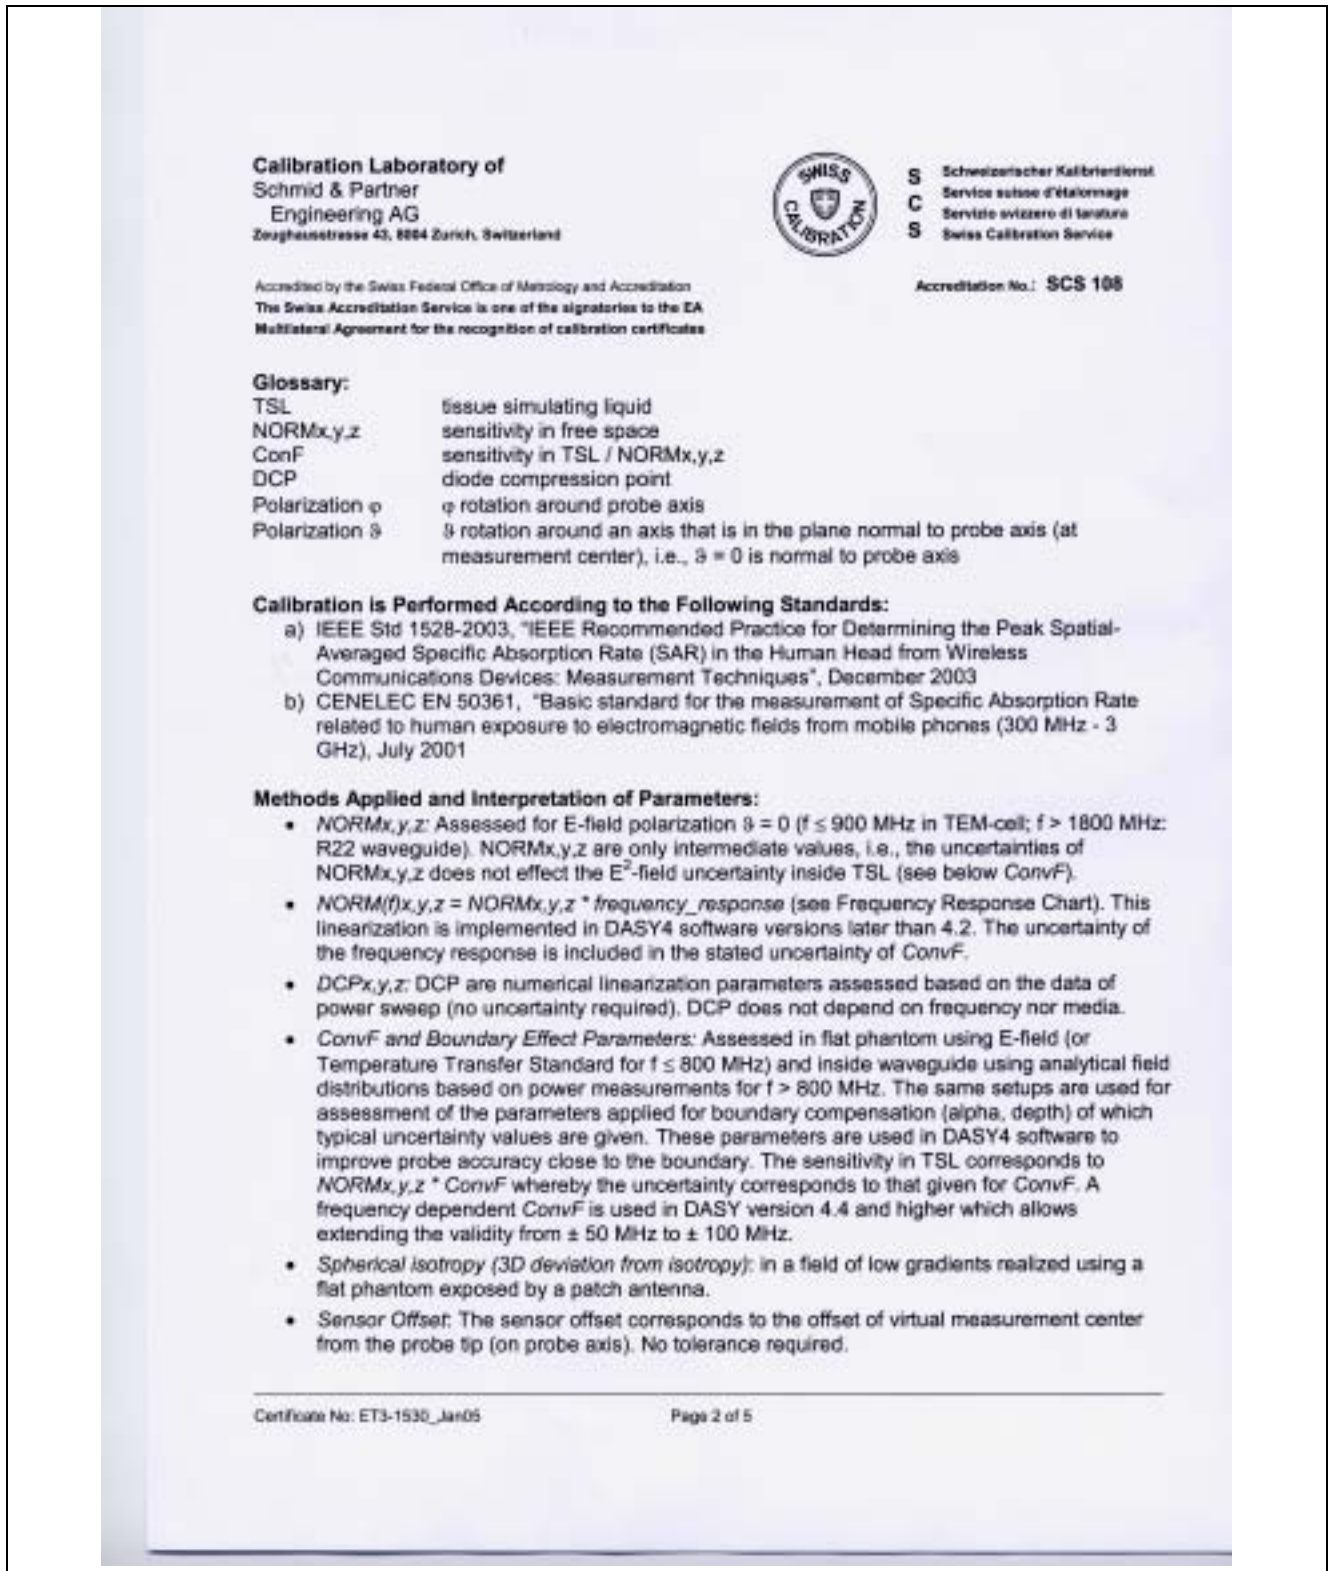

ET3DV6 SN:1530

January 17, 2005

Probe ET3DV6

SN:1530

Additional Conversion Factors

Manufactured:	July 15, 2000
Last calibrated:	September 1, 2004
Recalibrated:	January 17, 2005

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1530

January 17, 2005

DASY - Parameters of Probe: ET3DV6 SN:1530

Sensitivity in Free Space^A

NormX	1.44 ± 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$
NormY	1.47 ± 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	1.45 ± 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$

Diode Compression^B

DCP X	95 mV
DCP Y	95 mV
DCP Z	95 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 5.

Sensor Offset

Probe Tip to Sensor Center **2.7 mm**

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.



^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 5).

^B Numerical linearization parameter; uncertainty not required.

ET3DV6 SN:1530

January 17, 2005

Conversion Factor Assessment

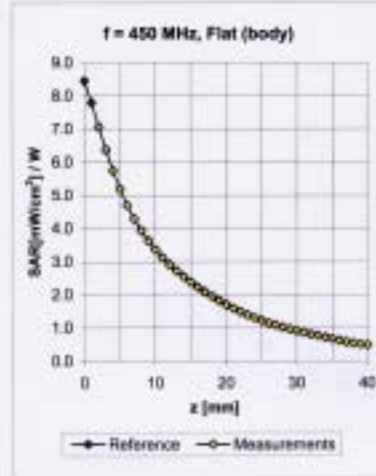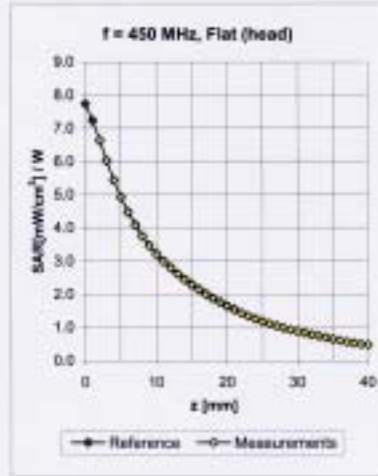

f [MHz]	Validity [MHz] ²	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
450	± 50 / ± 100	Head	43.5 ± 5%	0.87 ± 5%	0.17	2.00	7.27 ± 13.3% (k=2)
450	± 50 / ± 100	Body	56.7 ± 5%	0.94 ± 5%	0.14	1.82	7.19 ± 13.3% (k=2)

² The validity of ± 100 MHz only applies for DASV ≥ 4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Appendix E – Data Acquisition Electronic (DAE) Calibration

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland

Client **Auden**

CALIBRATION CERTIFICATE			
Object(s)	DAE3 – SD 000 D03 AA – SN:393		
Calibration procedure(s)	QA CAL-06.v5a Calibration procedure for the data acquisition unit (DAE)		
Calibration date:	08.01.2004		
Condition of the calibrated item	In Tolerance (according to the specific calibration document)		
<small>This calibration statement documents traceability of M&E used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.</small>			
<small>All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.</small>			
<small>Calibration Equipment used (M&E critical for calibration)</small>			
Model Type	ID #	Cal Date	Scheduled Calibration
Fuke Process Calibrator Type 762	SN: 6295803	8-Sep-03	Sep-04
Calibrated by:	Name Philipp Storchegger	Function Technician	Signature 
Approved by:	Name Fin Borcholt	Function R&D Director	Signature 
Date issued: 08.01.2004			
<small>This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.</small>			

DAE3 SN: 393

DATE: 08.01.2004

1. Cal Lab. Incoming Inspection & Pre Test

Modification Status	Note Status here → → → →	BC
Visual Inspection	Note anomalies.....	None
Pre Test	Indication	Yes/No
Probe Touch	Function	Yes
Probe Collision	Function	Yes
Probe Touch&Collision	Function	Yes

2. DC Voltage Measurement

A/D - Converter Resolution nominal
 High Range: 1LSB = 6.1µV , full range = 400 mV
 Low Range: 1LSB = 61nV , full range = 4 mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	403.989	404.251	404.118
Low Range	3.96967	3.95088	3.95250
Connector Angle to be used in DASY System	15 °		

High Range	Input	Reading in µV	% Error
Channel X + Input	200mV	199999.5	0.00
	20mV	19999.8	0.00
Channel X - Input	20mV	-19992.4	-0.04
Channel Y + Input	200mV	200000.2	0.00
	20mV	19996.1	-0.02
Channel Y - Input	20mV	-19992.5	-0.04
Channel Z + Input	200mV	200000.0	0.00
	20mV	20001.4	0.01
Channel Z - Input	20mV	-19998.8	-0.01

Low Range	Input	Reading in µV	% Error
Channel X + Input	2mV	1999.91	0.00
	0.2mV	199.98	-0.01
Channel X - Input	0.2mV	-200.39	0.19
Channel Y + Input	2mV	1999.94	0.00
	0.2mV	199.28	-0.36
Channel Y - Input	0.2mV	-200.58	0.29
Channel Z + Input	2mV	2000.03	0.00
	0.2mV	199.19	-0.41
Channel Z - Input	0.2mV	-201.21	0.61

Page 2 of 4

DAE3 SN: 393

DATE: 08.01.2004

3. Common mode sensitivity

DASY measurement parameters:

Auto Zero Time: 3 sec, Measuring time: 3 sec
 High/Low Range

in μ V	Common mode Input Voltage	High Range Reading	Low Range Reading
Channel X	200mV	12.68	10.78
	- 200mV	-9.74	-11.02
Channel Y	200mV	9.71	9.34
	- 200mV	-10.96	-11.04
Channel Z	200mV	2.62	2.78
	- 200mV	-4.70	-4.90

4. Channel separation

DASY measurement parameters:

Auto Zero Time: 3 sec, Measuring time: 3 sec
 High Range

in μ V	Input Voltage	Channel X	Channel Y	Channel Z
Channel X	200mV	-	2.53	0.76
Channel Y	200mV	0.56	-	5.50
Channel Z	200mV	-1.26	-0.03	-

5.1 AD-Converter Values with Input Voltage set to 2.0 mVDC

in Zero Low	Low Range Max - Min	Max.	Min
Channel X	10	16338	16328
Channel Y	8	16574	16566
Channel Z	14	16503	16489

5.2 AD-Converter Values with inputs shorted

in LSB	Low Range	High Range
Channel X	16353	16146
Channel Y	16546	16009
Channel Z	16495	16442

DAE3 SN: 393

DATE: 08.01.2004

6. Input Offset Measurement

DASY measurement parameters:

Auto Zero Time: 3 sec, Measuring time: 3 sec
 Number of measurements: 100, Low Range

Input 10MΩ

in μV	Average	min. Offset	max. Offset	Std. Deviation
Channel X	1.27	0.41	1.94	0.27
Channel Y	-1.15	-2.03	-0.01	0.32
Channel Z	-0.17	-2.91	1.44	0.42

Input shorted

in μV	Average	min. Offset	max. Offset	Std. Deviation
Channel X	0.14	-0.33	0.69	0.18
Channel Y	-0.77	-1.88	-0.17	0.22
Channel Z	-0.87	-2.76	0.98	0.38

7. Input Offset Current

Nominal input circuitry offset current on all channels: <25fA

8. Input Resistance

in MOhm	Calibrating	Measuring
Channel X	0.1999	198.3
Channel Y	0.2001	198.4
Channel Z	0.1998	198.6

9. Low Battery Alarm Voltage

in V	Alarm Level
Supply (+ Vcc)	8.01
Supply (- Vcc)	-7.74

10. Power Consumption

in mA	Switched off	Stand by	Transmitting
Supply (+ Vcc)	0.00	5.43	13.8
Supply (- Vcc)	-0.01	-7.60	-8.79