

	ADT CORP.
D5: 5GHz SYSTEM VALIDATION DIPOLE SN: 1019	

## Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

ADT (Auden)

Object(s)	D5GHzV2 - S	N:1019	
Calibration procedure(s)	QA CAL-05.v Calibration pr	2 ocedure for dipole validation kits	
Calibration date:	February 23,	2004	
Condition of the calibrated item	In Tolerance	(according to the specific calibration	document)
17025 international standard.  All calibrations have been conductions.	cted in the closed laborat	E used in the calibration procedures and conformity of love the calibration procedures and love the calibrat	
17025 international standard.  All calibrations have been conduct  Calibration Equipment used (M&	eted in the closed laborat	ory facility: environment temperature 22 +/- 2 degrees	Celsius and humidity < 75%.
17025 international standard.  All calibrations have been conduct  Calibration Equipment used (M&  Model Type	cted in the closed laborat	ory facility: environment temperature 22 +/- 2 degrees  Cal Date (Calibrated by, Certificate No.)	Celsius and humidity < 75%.  Scheduled Calibration
17025 international standard.  All calibrations have been conduct  Calibration Equipment used (M&  Model Type  Power meter EPM E4419B	cted in the closed laborat TE critical for calibration)	Cal Date (Calibrated by, Certificate No.) 2-Apr-03 (METAS, No 252-0250)	Celsius and humidity < 75%.
17025 international standard.  All calibrations have been conduct  Calibration Equipment used (M&  Model Type  Power meter EPM E4419B  Power sensor E4412A	rited in the closed laboration)  ID #  GB41293874	Cal Date (Calibrated by, Certificate No.)  2-Apr-03 (METAS, No 252-0250)  2-Apr-03 (METAS, No 252-0250)	Celsius and humidity < 75%.  Scheduled Calibration  Apr-04
17025 international standard.  All calibrations have been conduct Calibration Equipment used (M&  Model Type Power meter EPM E4419B Power sensor E4412A Power sensor HP 8481A	rted in the closed laboration)  ID #  GB41293874  MY41495277	Cal Date (Calibrated by, Certificate No.) 2-Apr-03 (METAS, No 252-0250)	Celsius and humidity < 75%.  Scheduled Calibration  Apr-04  Apr-04
17025 international standard.  All calibrations have been conduct Calibration Equipment used (M&  Model Type Power meter EPM E4419B Power sensor E4412A Power sensor HP 8481A RF generator R&S SMT06	ID # GB41293874 MY41495277 MY41092317	Cal Date (Calibrated by, Certificate No.) 2-Apr-03 (METAS, No 252-0250) 2-Apr-03 (METAS, No 252-0250) 18-Oct-02 (Agilent, No. 20021018)	Celsius and humidity < 75%.  Scheduled Calibration  Apr-04  Apr-04  Oct-04
17025 international standard.  All calibrations have been conductor.  Calibration Equipment used (M& Model Type  Power meter EPM E4419B  Power sensor E4412A  Power sensor HP 8481A  RF generator R&S SMT06	ID # GB41293874 MY41495277 MY41092317 100058	Cal Date (Calibrated by, Certificate No.)  2-Apr-03 (METAS, No 252-0250)  2-Apr-03 (METAS, No 252-0250)  18-Oct-02 (Agilent, No. 20021018)  23-May-01 (SPEAG, in house check May-03)	Scheduled Calibration Apr-04 Apr-04 Oct-04 In house check: May-05
17025 international standard.	TE critical for calibration)  ID #  GB41293874  MY41495277  MY41092317 100058 US37390585	Cal Date (Calibrated by, Certificate No.)  2-Apr-03 (METAS, No 252-0250)  2-Apr-03 (METAS, No 252-0250)  18-Oct-02 (Agilent, No. 20021018)  23-May-01 (SPEAG, in house check Nov-03)	Scheduled Calibration  Apr-04  Apr-04  Oct-04  In house check: May-05  In house check: Oct 05

Date issued: February 26, 2004

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed,

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

# DASY

## Dipole Validation Kit

Type: D5GHzV2

Serial: 1019

Manufactured:

February 5, 2004

Calibrated:

February 23, 2004

## 1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **head simulating solution** of the following electrical parameters:

Frequency:	5200 MHz	
Relative Dielectricity	36.3	± 5%
Conductivity	1 57 h a /	L 50/

Conductivity 4.57 mho/m 
$$\pm$$
 5%

Relative Dielectricity 35.4 
$$\pm 5\%$$
  
Conductivity 5.20 mho/m  $\pm 5\%$ 

The DASY4 System with a dosimetric E-field probe EX3DV3 - SN:3503 was used for the measurements. The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. Special 8x8x8 fine cube was chosen for cube integration (dx=dy=4.3mm, dz=3mm). Distance between probe sensors and phantom surface was set to 2.5 mm. The dipole input power (forward power) was 250 mW  $\pm$  3 %. The results are normalized to 1W input power.

#### 2. SAR Measurement with DASY System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figures supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured at **5200 MHz** (**Head Tissue**) with the dosimetric probe EX3DV3 SN:3503 and applying the <u>advanced extrapolation</u> are:

averaged over 1 cm<sup>3</sup> (1 g) of tissue: **86.0 mW/g** 
$$\pm$$
 20.3 % (k=2)<sup>1</sup>

averaged over 10 cm<sup>3</sup> (10 g) of tissue: **24.1 mW/g** 
$$\pm$$
 19.8 % (k=2)<sup>1</sup>

The resulting averaged SAR-values measured at 5800 MHz (Head Tissue) with the dosimetric probe EX3DV3 SN:3503 and applying the advanced extrapolation are:

averaged over 1 cm<sup>3</sup> (1 g) of tissue: **86.8 mW/g** 
$$\pm$$
 20.3 % (k=2)<sup>2</sup>

averaged over 10 cm<sup>3</sup> (10 g) of tissue: **24.4 mW/g** 
$$\pm$$
 19.8 % (k=2)<sup>2</sup>

<sup>&</sup>lt;sup>1</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR\_1g=76.5 mW/g, SAR\_10g=21.6 mW/g and SAR\_peak=310.3 mW/g.

<sup>&</sup>lt;sup>2</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR\_1g=78.0 mW/g, SAR 10g=21.9 mW/g and SAR peak=340.9 mW/g.

## 3. Dipole Transformation Parameters

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint (please refer to the graphics attached to this document). The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay: 1. 200 ns (one direction)

Transmission factor: 0.974 (voltage transmission, one direction)

#### 4. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **body simulating solution** of the following electrical parameters:

Frequency: 5200 MHz

Relative Dielectricity 49.7  $\pm 5\%$ Conductivity 5.18 mho/m  $\pm 5\%$ 

Frequency: 5800 MHz

Relative Dielectricity 48.5  $\pm 5\%$ Conductivity 6.01 mho/m  $\pm 5\%$ 

The DASY3 System with a dosimetric E-field probe EX3DV3 - SN:3503 was used for the measurements. The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 8x8x8 fine cube was chosen for cube integration (dx=dy=4.3mm, dz=3mm). Distance between probe sensors and phantom surface was set to 2.5 mm. The dipole input power (forward power) was 250 mW  $\pm$  3 %. The results are normalized to 1W input power.

## 5. SAR Measurement with DASY System

Standard SAR-measurements were performed according to the measurement conditions described in section 4. The results (see figures supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured at **5200 MHz (Body Tissue)** with the dosimetric probe EX3DV3 SN:3503 and applying the <u>advanced extrapolation</u> are:

averaged over 1 cm<sup>3</sup> (1 g) of tissue: 77.6 mW/g  $\pm$  20.3 % (k=2)<sup>3</sup>

averaged over 10 cm<sup>3</sup> (10 g) of tissue: **21.8 mW/g**  $\pm$  19.8 % (k=2)<sup>3</sup>

The resulting averaged SAR-values measured at 5800 MHz (Body Tissue) with the dosimetric probe EX3DV3 SN:3503 and applying the <u>advanced extrapolation</u> are:

averaged over 1 cm<sup>3</sup> (1 g) of tissue:  $75.6 \text{ mW/g} \pm 20.3 \% (k=2)^4$ 

averaged over 10 cm<sup>3</sup> (10 g) of tissue: **21.0 mW/g**  $\pm$  19.8 % (k=2)<sup>4</sup>

## 6. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

## 7. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Small end caps have been added to the dipole arms in order to increase frequency bandwidth at the position as explained in Sections 1 and 4.

## 8. Power Test

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

<sup>&</sup>lt;sup>3</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR\_1g=71.8 mW/g, SAR\_10g=20.1 mW/g and SAR\_peak=284.7 mW/g.

<sup>&</sup>lt;sup>4</sup> Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR\_1g=74.1 mW/g, SAR 10g=20.5 mW/g and SAR peak=324.7 mW/g.

Date/Time: 02/20/04 16:13:30

Test Laboratory: SPEAG, Zurich, Switzerland

## DUT: Dipole 5GHz; Serial: D5GHzV2 - SN:1019

Communication System: CW-5GHz; Duty Cycle: 1:1; Medium: HSL5800

Medium parameters used: f = 5200 MHz;  $\sigma = 4.57 \text{ mho/m}$ ;  $\varepsilon_r = 36.3$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Medium parameters used: f = 5800 MHz;  $\sigma = 5.2 \text{ mho/m}$ ;  $\varepsilon_r = 35.4$ ;  $\rho = 1000 \text{ kg/m}^3$ 

## **DASY4** Configuration:

 Probe: EX3DV3 - SN3503; ConvF(5.7, 5.7, 5.7) ConvF(5, 5, 5); Calibrated: 6/27/2003

- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE4 600; Calibrated: 9/30/2003
- Phantom: SAM with CRP TP:1312; Phantom section: Flat Section
- Measurement SW: DASY4, V4.2 Build 30; Postprocessing SW: SEMCAD, V1.8 Build 98

d=10mm, Pin=250mW, f=5200 MHz/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 96.8 V/m

Power Drift = 0.0 dB

Maximum value of SAR = 39.6 mW/g

## d=10mm, Pin=250mW, f=5800 MHz 2/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Peak SAR (extrapolated) = 90.4 W/kg


SAR(1 g) = 21.7 mW/g; SAR(10 g) = 6.09 mW/g

## d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:


Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Peak SAR (extrapolated) = 83.1 W/kg

SAR(1 g) = 21.5 mW/g; SAR(10 g) = 6.03 mW/g

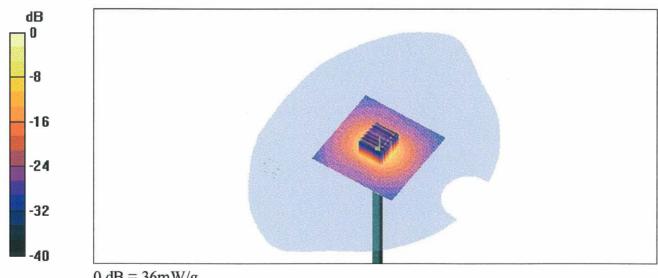

0 dB = 36 mW/g

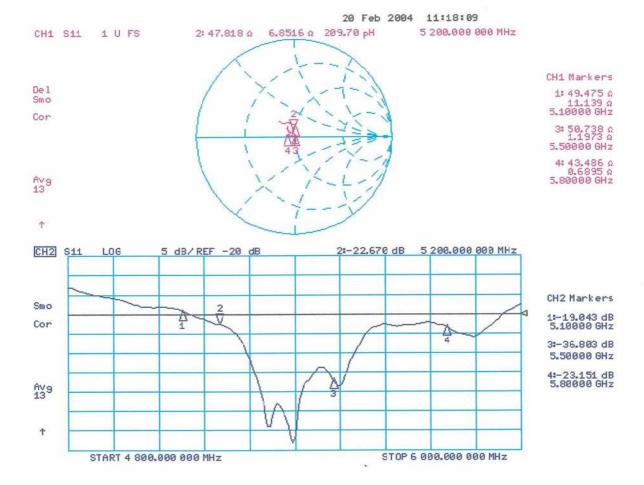

Date/Time: 02/23/04 18:22:03

Test Laboratory: SPEAG, Zurich, Switzerland

## DUT: Dipole 5GHz; Serial: D5GHzV2 - SN:1019

Communication System: CW-5GHz; Duty Cycle: 1:1; Medium: MSL5800

Medium parameters used: f = 5200 MHz;  $\sigma = 5.18 \text{ mho/m}$ ;  $\varepsilon_r = 49.7$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Medium parameters used: f = 5800 MHz;  $\sigma = 6.01 \text{ mho/m}$ ;  $\varepsilon_r = 48.5$ ;  $\rho = 1000 \text{ kg/m}^3$ 

## DASY4 Configuration:

- Probe: EX3DV3 SN3503; ConvF(5, 5, 5) ConvF(4.6, 4.6, 4.6); Calibrated: 6/27/2003
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE4 600; Calibrated: 9/30/2003
- Phantom: SAM with CRP TP:1312; Phantom section: Flat Section
- Measurement SW: DASY4, V4.2 Build 34; Postprocessing SW: SEMCAD, V1.8 Build 105

## d=10mm, Pin=250mW, f=5200 MHz/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 79.9 V/m; Power Drift = -0.002 dB Maximum value of SAR (interpolated) = 35.3 mW/g

## d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Peak SAR (extrapolated) = 75.2 W/kg


SAR(1 g) = 18.9 mW/g; SAR(10 g) = 5.25 mW/g

## d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Peak SAR (extrapolated) = 69.2 W/kg

SAR(1 g) = 19.4 mW/g; SAR(10 g) = 5.45 mW/g

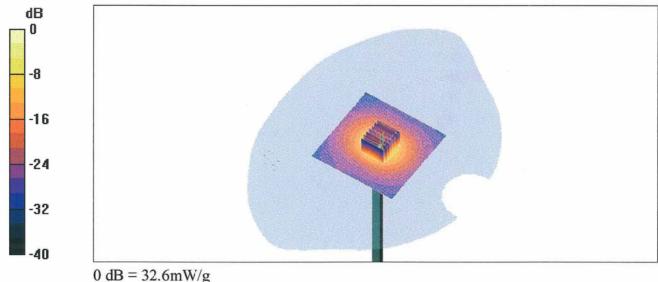

#### 23 Feb 2004 12:04:44

