

SAR COMPLIANCE TESTING OF SONY MODEL CM-Z200
CELLULAR TELEPHONE

FINAL TECHNICAL REPORT

July 20, 1998

Submitted to: Dr. Yoshiro Fukuoka
Wireless Telecommunications Company
Sony Electronics Inc.
16450 West Bernardo Drive/MZ7315
San Diego, CA 92127-1804

Submitted by: Om P. Gandhi
Professor and Chairman
University of Utah
Electrical Engineering Department
50 S Central Campus Dr., Rm. 3280
Salt Lake City, UT 84112-9206

SAR COMPLIANCE TESTING OF SONY MODEL CM-Z200 CELLULAR TELEPHONE

I. Introduction

The U.S. Federal Communications Commission (FCC) has adopted limits of human exposure to RF emissions from mobile and portable devices that are regulated by the FCC [1]. The FCC has also recently issued Supplement C (Edition 97-01) to OET Bulletin 65 defining both the measurement and the computational procedures that should be followed for evaluating compliance of mobile and portable devices with FCC limits for human exposure to radiofrequency emissions [2].

For Sony Model CM-Z200 Cellular Telephone (FCC ID# L5ACMZ200DM), we have used the experimental measurement techniques to determine the SAR distributions from which the peak 1-g SARs are obtained, as recommended in [2], both when the antenna is fully extended (completely pulled out) or left retracted. Also as recommended in [2], the telephone is placed against the left ear with the antenna located towards the front of the head. This allows a longer portion of the antenna to be in close proximity to the head resulting in higher SARs allowing thereby the worst case determination of absorbed energy in the user's head [3]. Also as recommended in [2], the handset is tested without the model of a hand to determine once again the worst case SAR distribution.

II. The Sony Model CM-Z200 Cellular Telephone

The Sony Model CM-Z200 Cellular Telephone is a dual mode telephone that can be operated in the AMPS or the CDMA mode. It works in the frequency band 825-849 MHz for transmission frequencies. Since the radiated power is considerably higher in the AMPS mode up to 600 mW and is lower by a factor of 2-3 in the CDMA mode, we decided to determine the SAR distributions for the higher power output of 600 mW. Prior to SAR testing, we measured the power fed to the antenna by tapping it off with an I/O connector of 15 pins and a coaxial RF output port connected to the base of the telephone. By using the software provided, we could adjust the power output until it was 600 mW CW as

measured with the Hewlett Packard (HP) Model 436A Power Meter with HP Model 8481 H Power Sensor. The SAR measurements were conducted with the antenna pulled out or left retracted at the low-frequency end (channel 991, frequency 824 MHz), midband (channel 383, frequency 836.5 MHz) and high-frequency end (channel 799, frequency 849 MHz), each for the power fed to the antenna adjusted, as indicated above, to a measured power amplifier output of 600 mW.

III. The Tissue-Simulant Model

For measurements of SAR distributions, we have used the Utah Experimental Model that is described in detail in Appendix A [4]. This model uses a lossy outer shell of the following approximate dimensions:

Axial length from chin to top of the head = 26 cm
Distance from location of the ear canal to top of the head = 14.7 cm
Width from side to side = 16.5 cm

These dimensions are typical for adult human beings. The shell thickness of the head and neck model is approximately 4-7 mm, which is typical of the human skull thickness. The thickness for the ear region is, however, considerably less and is only about 3 mm.

This experimental model shown in Fig. 1 has, in the past, been used for comparison of the measured peak 1-g SARs with those obtained with the Utah FDTD Code for ten wireless telephones, five at 835 MHz and five for PCS (1900 MHz) frequencies [see Table 6 of Appendix A]. The numerical SARs were obtained using the anatomically-based, 15-tissue Utah model of the head and neck with a resolution of $1.974 \times 1.974 \times 3.0$ mm that has been described in the scientific literature through numerous publications (see e.g. references 3, 5). The measured and calculated 1-g SARs for these ten telephones, including some research test samples from diverse manufacturers using a variety of radiating antennas for different source-based time-averaged powers are compared in Table 1 (taken from Table 6 of Appendix A). Even though widely different peak 1-g SARs from 0.13 to 5.41 W/kg are obtained because of the variety of antennas and handsets,

agreement between the calculated and the measured data is excellent and generally within ± 25 percent.

These tests validate the Utah Experimental Phantom Model as being capable of giving peak 1-g SARs that are in good agreement with the SARs obtained with the realistic, anatomically-based model of the human head and neck both at 835 and 1900 MHz.

The head and neck and the upper part of the torso of the model are filled with a liquid with measured electrical properties (dielectric constant and conductivity) close to the average properties of the brain for white and gray matters at 835 MHz which is close to the midband transmission frequency for this telephone. A composition suggested by Hartsgrove et al. [6] consists of 40.4% water, 56.0% sugar, 2.5 percent salt (NaCl) and 1.0% HEC. As measured in our laboratory using the HP Model 85070B Dielectric Probe in conjunction with HP Model 8720C Network Analyzer (50 MHz-20 GHz), this composition gives a measured $\epsilon_r = 41.1 \pm 1.4$ and $\sigma = 1.06 \pm 0.05$ S/m. From reference 7, we obtained the desired dielectric properties to simulate the brain tissue at 835 MHz to be $\epsilon_r = 45.3$ and $\sigma = 0.92$ S/m. Thus the measured properties for the brain-simulant fluid used for experimental SAR measurements are close to the desired values. To the extent that the conductivity σ is slightly higher and the permittivity ϵ_r is somewhat lower than the desired values for the brain tissue, it should help in avoiding underestimating the SAR [2].

IV. The E-Field Probe

The non-perturbing implantable E-field probe used in the setup was originally developed by Bassen et al. [8] and is now manufactured by L3/Narda Microwave Corporation, Hauppauge, New York as Model 8021 E-field probe. In this probe, three orthogonal miniature dipoles are placed on a triangular beam substrate. Each dipole is loaded with a small Schottky diode and connected to the external circuitry by high resistance ($2 \text{ M}\Omega \pm 40\%$) leads to reduce secondary pickups. The entire structure is then encapsulated with a low dielectric constant insulating material. The probe thus constructed

has a very small (4 mm) diameter, which results in a relatively small perturbation of the internal electric field.

Test for Square Law Region

It is necessary to operate the E-field probe in the square law region for each of the diodes so that the sum of the dc voltage outputs from the three dipoles is proportional to the square of the internal electric field ($|E_i|^2$). Fortunately, the personal wireless devices induce SARs that are generally less than 5-6 W/kg even for closest locations of the head [3]. For compliance testing, it is, therefore, necessary that the E-field probe be checked for square law behavior for SARs up to such values that are likely to be encountered. Such a test may be conducted using a canonical lossy body such as a rectangular box or a sphere irradiated by a dipole. By varying the radiated power of the dipole, the output of the probe should increase linearly with the applied power for each of the test locations.

Shown in Figs. 2a, 2b are the results of the tests performed to check the square law behavior of the E-field probe used in our setup at 840 and 1900 MHz, respectively. For these measurements, we have used a rectangular box of dimensions $30 \times 15 \times 50$ cm that was irradiated by the corresponding half wave dipoles with different amounts of radiated powers from 200-800 mW. Since the dc voltage outputs of the probe are fairly similar when normalized to a radiated power of 100 mW, the square law behavior is demonstrated and an output voltage that is proportional to $|E_i|^2$ is obtained within ± 3 percent.

Test for Isotropy of the Probe

Another important characteristic of the probe that affects the measurement accuracy is its isotropy. Since the orientation of the induced electric field is generally unknown, the E-field probe should be relatively isotropic in its response to the orientation of the E-field. Shown in Figs. 3a, 3b are the test results of the E-field probe used in our setup at 840 and 1900 MHz, respectively. The previously described box phantom of dimensions $30 \times 15 \times 50$ cm along x, y and z dimensions, respectively, was also used for these measurements. This phantom was filled to a depth of 15 cm with brain-simulant materials (Table 2). The

E-field probe was rotated around its axis from 0 to 360° in incremental steps of 60°. An isotropy of less than ± 0.23 dB ($\pm 5.5\%$) was observed for this E-field probe both at 840 and 1900 MHz.

Calibration of the E-Field Probe

Since the voltage output of the E-field probe is proportional to the square of the internal electric field ($|E_i|^2$), the SAR, given by $\sigma|E_i|^2/\rho$ is, therefore, proportional to the voltage output of the E-field probe by a proportionality constant C . The constant C is defined as the calibration factor, and is frequency and material dependent. It is measured to calibrate the probe at the various frequencies of interest using the appropriate tissue-simulating materials for the respective frequencies.

Canonical geometries such as waveguides, rectangular slabs and layered or homogeneous spheres have, in the past, been used for the calibration of the implantable E-field probe [9-11]. Since the Finite Difference Time Domain (FDTD) has been carefully validated to solve electromagnetic problems for a variety of geometries [12, 13], we were able to calibrate the Narda E-field probe by comparing the measured variations of the probe voltage ($\approx |E_i|^2$) against the FDTD-calculated variations of SARs for a box phantom of dimensions $30 \times 15 \times 50$ cm used previously for the data given in Figs. 2 and 3, respectively. For these measurements, we placed the nominal half-wave dipoles of lengths 178 mm and 77 mm at 840 and 1900 MHz, respectively, at several distances d (see inserts of Figs. 4a, 4b, and 5a, 5b) from the outer surface of the acrylic ($\epsilon_r = 2.56$) box of thickness 6.55 mm. Shown in Figs. 4a, 4b and 5a, 5b are the comparisons between the experimentally measured and FDTD-calculated variations of the SAR distributions for this box phantom. Since there are excellent agreements between the calculated SARs and the measured variations of the voltage output of the E-field probe for four different separations d of the half wave dipoles at each of the two frequencies, it is possible to calculate the calibration factors at the respective frequencies. For the Narda Model 8021 E-field probe

used in our setup, the calibration factors are determined to be 0.49 and 0.84 (mW/kg)/ μ V at 840 and 1900 MHz, respectively.

V. Experimental Results: Canonical Problems

To further validate the system, it has been used to measure the peak 1-g SAR for the above-mentioned box phantom and a glass sphere model of thickness 5 mm, external diameter = 223 mm and assumed dielectric constant $\epsilon_r = 4.0$. This sphere model is once again filled with the corresponding brain-simulant fluids of compositions given in Table 2. Shown in Figs. 6a, 6b and 7a, 7b are the measured and FDTD-calculated SAR distributions inside the sphere for various separations d between the dipole and the sphere (see insert for Figs. 6, 7). Comparison of the measured and FDTD-calculated peak 1-g SARs for both phantom geometries are given in Tables 3 and 4, respectively. As can be seen, the agreement between experimental measurement and numerical simulation is excellent and generally within ± 10 percent for both rectangular and spherical phantoms.

VI. Measurement Uncertainty: Test Runs With Cellular Telephones

The automated setup shown in Fig. 2 of Appendix A has been used for the testing of ten personal wireless devices including some research test samples, five each at 835 and 1900 MHz, respectively. Given in Table 1 is the comparison of the numerical and measured peak 1-g SARs for these devices using our experimental phantom model and the FDTD-based numerical procedure used for calculations of SAR distributions for an anatomically-based model of the head of an adult male [4]. The measured and calculated SARs for the ten telephones which have quite different operational modes (TDMA, CDMA, etc.) and antenna structures (helical, monopole, or helix-monopole) vary from 0.13 to 5.41 W/kg. Even though widely different peak 1-g SARs are obtained because of the variety of antennas and handsets, agreement between the calculated and the measured data is excellent and generally within $\pm 25\%$. This is particularly remarkable since an MRI-

derived, 16-tissue anatomically-based model of the adult human head is used for FDTD calculations and a relatively simplistic two tissue phantom model is used for experimental peak 1-g SAR measurements.

We estimate the uncertainty of our measuring system to be ± 12.5 percent. As seen in Table 1, an agreement within ± 25 percent is obtained for the peak 1-g SARs calculated using the Utah FDTD Code and the Utah Experimental Phantom Model for ten assorted wireless devices using a variety of antennas and handset dimensions. Since both the numerical and experimental methods are completely independent methods, and each is prone to its own set of errors, an uncertainty of ± 12.5 percent can be ascribed to each of the methods.

VII. The Measured SAR Distributions for Sony Model CM-Z200 Telephone

As suggested in Supplement C (Edition 97-01) to the FCC OET Bulletin 65 [2], the SAR measurements are conducted with the Sony Model CM-Z200 Cellular Telephone pressed against the model of the head such that the center of the ear piece is aligned against the location of the ear canal. Furthermore, the handset is oriented such that the center line of the body of the handset is in the plane passing through the two ear canals and the tip of the mouth.

For two possible configurations of the antenna i.e. completely pulled out or left retracted, respectively, the regions of the maximum SARs were located in the first instance by searching coarser regions of dimensions 4.8×8.0 cm close to the antenna and the central region of the handset where it is in contact with the cheek. For this cellular telephone, the highest SARs were measured for the upper region of the ear that is close to the base of the antenna.

After having identified the regions of the highest SARs for both configurations of the antenna, these regions were measured with a finer resolution of 2.0 mm with the Sony

Cellular Telephone radiating maximum power (600 mW) at low frequency end (channel 991, frequency 824 MHz), midband (channel 383, frequency 836.5 MHz) and high-frequency end (channel 799, frequency 849 MHz), respectively. We give in Tables 5-10 the detailed SAR distributions that have been measured for the highest SAR region of the model of the head for the Sony Model CM-Z200 Cellular Telephone. From these measurements, the peak 1-g SARs are calculated and are summarized in Table 11. The peak SARs have been measured to vary from 0.69 to 1.29 W/kg for different configurations of the antenna (pulled out or retracted) at various frequencies i.e. low end, midband and high end of the transmission frequencies. Several of these measurements were taken repeatedly two, or four times and found to give consistent 1-g SARs that were identical within ± 1 percent.

VIII. Comparison of the Data With FCC 96-326 Guidelines

According to the FCC 96-326 Guidelines [1], the peak SAR for any 1-g of tissue should not exceed 1.6 W/kg. We have determined the peak 1-g SARs for the Sony Model CM-Z200 Cellular Telephone to vary between 0.69 and 1.29 W/kg depending on the frequency and configuration of the antenna whether it was pulled out or left retracted, respectively. All of these values are lower than 1.6 W/kg suggested in the FCC 96-326 Guidelines [1].

REFERENCES

1. Federal Communications Commission, "Guidelines for Evaluating the Environmental Effects of Radiofrequency Radiation," FCC 96-326, August 1, 1996.
2. K. Chan, R. F. Cleveland, Jr., and D. L. Means, "Evaluating Compliance With FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields," Supplement C (Edition 97-01) to OET Bulletin 65, December, 1997. Available from Office of Engineering and Technology, Federal Communications Commission, Washington D.C., 20554.
3. O. P. Gandhi, G. Lazzi and C. M. Furse, "Electromagnetic Absorption in the Human Head and Neck for Mobile Telephones at 835 and 1900 MHz," *IEEE Transactions on Microwave Theory and Techniques*, Vol. 44, pp. 1884-1897, 1996.
4. Q. Yu, M. Aronsson, D. Wu, and O. P. Gandhi, "An Automated SAR Measurement System for Compliance Testing of Personal Wireless Devices," submitted to *IEEE Transactions on Electromagnetic Compatibility*, March 1998 (attached as Appendix A).
5. O. P. Gandhi, "FDTD in Bioelectromagnetics: Safety Assessment and Medical Applications," Chapter 4 in *Advances in Computational Electrodynamics I: The FDTD Method*, edited by A. Taflove, Artech House Inc., Dedham, MA, 1998.
6. G. Hartsgrove, A. Kraszewski, and A. Surowiec, "Simulated Biological Materials for Electromagnetic Radiation Absorption Studies," *Bioelectromagnetics*, Vol. 8, pp. 29-36, 1987.
7. C. Gabriel, "Compilation of the Dielectric Properties of Body Tissues at RF and Microwave Frequencies," Technical Report AL/OE-TR-1996-0037, Armstrong Laboratory, Air Force Materiel Command, Brooks Air Force Base, Texas 78235, June 1996.
8. H. I. Bassen and G. S. Smith, "Electric Field Probes -- A Review," *IEEE Trans. Antennas Propagation*, Vol. 34, pp. 710-718, September 1983.
9. D. Hill, "Waveguide Techniques for the Calibration of Miniature Electric Field Probes for Use in Microwave Bioeffects Studies," *IEEE Trans. Microwave Theory Tech.*, Vol. 30, pp. 92-94, 1982.
10. N. Kuster and Q. Balzano, "Energy Absorption Mechanism by Biological Bodies in the Near Field of Dipole Antennas Above 300 MHz," *IEEE Trans. Veh. Technology*, Vol. 41, pp. 17-23, 1992.
11. M. A. Stuchly, S. S. Stuchly, and A. Kraszewski, "Implantable Electric Field Probes -- Some Performance Characteristics," *IEEE Trans. Biomed. Eng.*, Vol. 31, pp. 526-531, 1984.
12. A. Taflove, K. R. Umashankar, T. G. Jurgens, "Validation of FDTD Modeling of the Radar Cross Section of Three-Dimensional Structures Spanning Up to Nine Wavelengths," *IEEE Trans. Antennas and Propagation*, pp. 662-666, 1985.

13. C. M. Furse, Q. Yu, and O. P. Gandhi, "Validation of the Finite-Difference Time-Domain Method for Near-Field Bioelectromagnetic Simulations," *Microwave and Optical Technology Letters*, Vol. 16, pp. 341-345, 1997.

Table 1. Comparison of the experimentally measured and FDTD-calculated peak 1-g SARs for ten wireless telephones, five each at 835 and 1900 MHz, respectively.

	Time-Averaged Radiated Power mW	Using Experimental Model W/kg	Numerical Method W/kg
Cellular Telephones at 835 MHz			
Telephone A	600	4.02	3.90
Telephone B	600	5.41	4.55
Telephone C	600	4.48	3.52
Telephone D	600	3.21	2.80
Telephone E	600	0.54	0.53
PCS Telephones at 1900 MHz			
Telephone A	125	1.48	1.47
Telephone B	125	0.13	0.15
Telephone C	125	0.65	0.81
Telephone D	125	1.32	1.56
Telephone E	99.3	1.41	1.25

Table 2. Compositions used for brain-equivalent materials.

840 MHz		1900 MHz	
Water	40.4%	Water	60.0%
Sugar	56.0%	Sugar	18.0%
Salt (NaCl)	2.5%	PEP	20.0%
HEC	1.0%	Salt (NaCl)	0.4%
		TX 151	1.6%
$\epsilon_r = 41.1 \pm 1.4$		$\epsilon_r = 45.5 \pm 1.7$	
$\sigma = 1.06 \pm 0.05 \text{ S/m}$		$\sigma = 1.31 \pm 0.06 \text{ S/m}$	

Table 3. Box phantom: Comparison of the measured and FDTD-calculated peak 1-g SARs for four spacings each at 840 and 1900 MHz, radiated power normalized to 0.5 W.

Frequency (MHz)	Distance (mm) Between $\lambda/2$ Dipole and the Box	SAR (W/kg)		Difference (%)
		Measured	FDTD	
840	17.5	4.58	4.20	+8.3
840	22.5	3.53	3.65	-3.4
840	27.5	2.69	3.00	-10.2
840	33.0	1.95	2.24	-12.9
1900	16.5	7.45	7.46	-0.1
1900	21.5	4.24	4.18	+1.4
1900	26.5	2.71	2.91	-7.9
1900	31.5	1.77	1.75	+1.1

Table 4. Sphere phantom: Comparison of the measured and FDTD-calculated peak 1-g SARs for three spacings each at 840 and 1900 MHz, radiated power normalized to 0.5 W.

Frequency (MHz)	Distance (mm) Between $\lambda/2$ Dipole and the Box	SAR (W/kg)		Difference (%)
		Measured	FDTD	
840	5	6.78	6.77	+0.23
840	15	3.41	3.27	+4.22
840	25	1.85	1.68	+9.51
1900	5	17.45	18.01	-3.21
1900	15	4.96	5.05	-1.81
1900	25	1.69	1.77	-4.73

Table 5. **Sony Model CM-Z200 Cellular Telephone at Low End Radiation Frequency (Channel 991, 824.04 MHz). Antenna pulled out.** The SAR distribution (in W/kg) measured with a step size of 2 mm for the highest SAR region of the head.

a. At depth of 1 mm

1.096	0.925	0.768	0.723	0.688
1.285	1.230	1.160	1.074	0.886
1.309	1.301	1.288	1.268	1.228
1.355	1.403	1.351	1.272	1.259
1.378	1.417	1.390	1.326	1.314

b. At depth of 3 mm

1.049	0.975	0.873	0.831	0.798
1.147	1.129	1.099	1.065	0.954
1.141	1.143	1.143	1.140	1.123
1.165	1.207	1.168	1.110	1.101
1.184	1.215	1.192	1.143	1.133

c. At depth of 5 mm

0.945	0.952	0.902	0.865	0.840
0.967	0.978	0.981	0.989	0.947
0.940	0.950	0.960	0.969	0.971
0.945	0.980	0.954	0.916	0.912
0.960	0.983	0.965	0.931	0.923

d. At depth of 7 mm

0.841	0.904	0.895	0.866	0.849
0.812	0.843	0.868	0.904	0.910
0.773	0.788	0.805	0.822	0.836
0.766	0.795	0.780	0.757	0.756
0.778	0.796	0.782	0.760	0.755

e. At depth of 9 mm

0.738	0.831	0.852	0.833	0.827
0.683	0.722	0.759	0.808	0.844
0.642	0.659	0.679	0.698	0.719
0.631	0.654	0.647	0.633	0.634
0.639	0.653	0.643	0.630	0.627

Table 6. **Sony Model CM-Z200 Cellular Telephone at Low End Radiation Frequency (Channel 991, 824.04 MHz). Antenna retracted.**
 The SAR distribution (in W/kg) measured with a step size of 2 mm for the highest SAR region of the head.

a. At depth of 1 mm

0.800	1.850	0.871	0.902	0.891
0.951	1.993	1.002	0.989	0.967
0.981	1.032	1.038	1.028	0.998
1.025	1.050	1.053	1.028	0.984
1.000	1.034	1.023	1.023	0.970

b. At depth of 3 mm

0.884	0.938	0.965	1.000	0.994
1.032	1.079	1.093	1.087	1.068
1.067	1.124	1.134	1.128	1.098
1.115	1.145	1.151	1.129	1.088
1.096	1.134	1.127	1.126	1.072

c. At depth of 5 mm

0.780	0.827	0.853	0.885	0.884
0.895	0.936	0.952	0.955	0.941
0.927	0.976	0.990	0.988	0.964
0.969	0.997	1.005	0.990	0.959
0.960	0.994	0.992	0.990	0.948

d. At depth of 7 mm

0.687	0.727	0.752	0.782	0.784
0.777	0.813	0.829	0.840	0.828
0.807	0.849	0.864	0.865	0.846
0.843	0.868	0.877	0.869	0.846
0.841	0.872	0.872	0.871	0.838

e. At depth of 9 mm

0.605	0.640	0.662	0.691	0.694
0.677	0.709	0.725	0.741	0.729
0.705	0.741	0.755	0.759	0.744
0.738	0.759	0.769	0.764	0.746
0.739	0.767	0.768	0.769	0.744

Table 7. **Sony Model CM-Z200 Cellular Telephone at Midband Radiation Frequency (Channel 383, 836.49 MHz). Antenna pulled out.** The SAR distribution (in W/kg) measured with a step size of 2 mm for the highest SAR region of the head. _

a. At depth of 1 mm

1.217	1.199	1.141	1.018	0.846
1.282	1.282	1.263	1.240	1.217
1.334	1.378	1.328	1.248	1.236
1.350	1.399	1.371	1.307	1.260
1.291	1.317	1.328	1.289	1.267

b. At depth of 3 mm

1.243	1.255	1.233	1.162	1.050
1.271	1.283	1.279	1.272	1.265
1.307	1.349	1.308	1.240	1.227
1.322	1.363	1.336	1.281	1.238
1.287	1.306	1.309	1.269	1.246

c. At depth of 5 mm

1.052	1.087	1.101	1.088	1.048
1.044	1.064	1.074	1.083	1.089
1.060	1.093	1.067	1.021	1.011
1.072	1.099	1.078	1.039	1.008
1.063	1.072	1.069	1.035	1.015

d. At depth of 7 mm

0.887	0.937	0.973	0.998	1.010
0.858	0.882	0.900	0.918	0.935
0.859	0.886	0.871	0.842	0.834
0.869	0.886	0.871	0.845	0.822
0.877	0.880	0.873	0.846	0.828

e. At depth of 9 mm

0.748	0.803	0.850	0.894	0.936
0.711	0.736	0.757	0.780	0.800
0.705	0.727	0.720	0.701	0.697
0.712	0.725	0.714	0.697	0.681
0.729	0.729	0.722	0.700	0.686

Table 8. **Sony Model CM-Z200 Cellular Telephone at Midband Radiation Frequency (Channel 383, 836.49 MHz). Antenna retracted.** The SAR distribution (in W/kg) measured with a step size of 2 mm for the highest SAR region of the head. -

a. At depth of 1 mm

1.269	1.387	1.449	1.511	1.521
1.431	1.530	1.587	1.620	1.582
1.565	1.670	1.727	1.722	1.647
1.600	1.720	1.739	1.748	1.692
1.695	1.776	1.802	1.779	1.730

b. At depth of 3 mm

1.305	1.424	1.499	1.563	1.580
1.455	1.550	1.602	1.650	1.622
1.566	1.669	1.724	1.727	1.664
1.600	1.712	1.739	1.752	1.709
1.692	1.775	1.803	1.788	1.742

c. At depth of 5 mm

1.168	1.272	1.349	1.407	1.426
1.290	1.369	1.411	1.465	1.449
1.369	1.456	1.503	1.512	1.468
1.398	1.489	1.519	1.533	1.507
1.477	1.550	1.576	1.570	1.532

d. At depth of 7 mm

1.038	1.130	1.206	1.258	1.277
1.141	1.206	1.241	1.296	1.289
1.198	1.271	1.311	1.323	1.292
1.222	1.296	1.327	1.342	1.328
1.293	1.354	1.379	1.378	1.348

e. At depth of 9 mm

0.917	0.997	1.068	1.116	1.134
1.008	1.061	1.092	1.142	1.142
1.051	1.113	1.148	1.160	1.137
1.073	1.134	1.163	1.178	1.172
1.138	1.189	1.211	1.213	1.190

Table 9. **Sony Model CM-Z200 Cellular Telephone at High End Radiation Frequency (Channel 799, 848.97 MHz). Antenna pulled out.** The SAR distribution (in W/kg) measured with a step size of 2 mm for the highest SAR region of the head.

a. At depth of 1 mm

0.887	0.881	0.838	0.752	0.634
0.952	0.945	0.939	0.918	0.905
0.987	1.028	0.992	0.936	0.930
1.014	1.048	1.028	0.982	0.951
0.962	1.025	1.037	1.007	0.994

b. At depth of 3 mm

0.835	0.848	0.833	0.788	0.719
0.868	0.871	0.874	0.867	0.866
0.890	0.925	0.899	0.854	0.851
0.913	0.939	0.923	0.885	0.859
0.885	0.932	0.940	0.911	0.898

c. At depth of 5 mm

0.709	0.737	0.746	0.738	0.717
0.715	0.725	0.735	0.741	0.748
0.724	0.752	0.736	0.705	0.704
0.740	0.759	0.747	0.720	0.701
0.736	0.765	0.769	0.745	0.733

d. At depth of 7 mm

0.601	0.636	0.662	0.679	0.691
0.588	0.602	0.617	0.630	0.644
0.588	0.610	0.602	0.582	0.582
0.601	0.613	0.605	0.587	0.573
0.612	0.628	0.629	0.610	0.599

e. At depth of 9 mm

0.508	0.545	0.579	0.609	0.642
0.488	0.503	0.520	0.536	0.552
0.483	0.502	0.498	0.486	0.487
0.493	0.502	0.497	0.485	0.475
0.514	0.520	0.520	0.505	0.497

Table 10. **Sony Model CM-Z200 Cellular Telephone at High-End Radiation Frequency (Channel 799, 848.97 MHz). Antenna retracted.** The SAR distribution (in W/kg) measured with a step size of 2 mm for the highest SAR region of the head.

a. At depth of 1 mm

1.402	1.510	1.560	1.615	1.571
1.548	1.660	1.708	1.698	1.621
1.601	1.709	1.742	1.733	1.677
1.685	1.744	1.760	1.731	1.671
1.648	1.721	1.722	1.732	1.661

b. At depth of 3 mm

1.333	1.429	1.478	1.529	1.500
1.450	1.548	1.594	1.593	1.533
1.495	1.592	1.625	1.621	1.579
1.569	1.625	1.645	1.626	1.577
1.545	1.614	1.620	1.632	1.571

c. At depth of 5 mm

1.179	1.258	1.302	1.347	1.332
1.264	1.345	1.386	1.392	1.350
1.301	1.381	1.412	1.413	1.384
1.362	1.411	1.433	1.423	1.386
1.351	1.411	1.420	1.433	1.385

d. At depth of 7 mm

1.040	1.105	1.144	1.185	1.178
1.103	1.169	1.205	1.215	1.186
1.133	1.200	1.227	1.231	1.213
1.184	1.226	1.249	1.245	1.218
1.183	1.235	1.245	1.258	1.221


e. At depth of 9 mm

0.916	0.971	1.004	1.041	1.039
0.965	1.020	1.051	1.063	1.043
0.991	1.047	1.071	1.077	1.066
1.036	1.071	1.093	1.093	1.072
1.040	1.085	1.096	1.109	1.080

Table 11. Summary of the measured peak 1-g SARs for the Sony Model CM-Z200 Cellular Telephone for a power amplifier output of 600 mW fed to the antenna. The numbers in parentheses indicate the number of times the measurements were repeated.

Antenna	Low End Channel 991, 824.04 MHz W/kg	Midband Channel 383, 836.49 MHz W/kg	High End Channel 799, 848.97 MHz W/kg
Pulled out	0.91	0.91	0.69 (2)
Retracted	0.77 (2)	1.28 (4)	1.29

a.

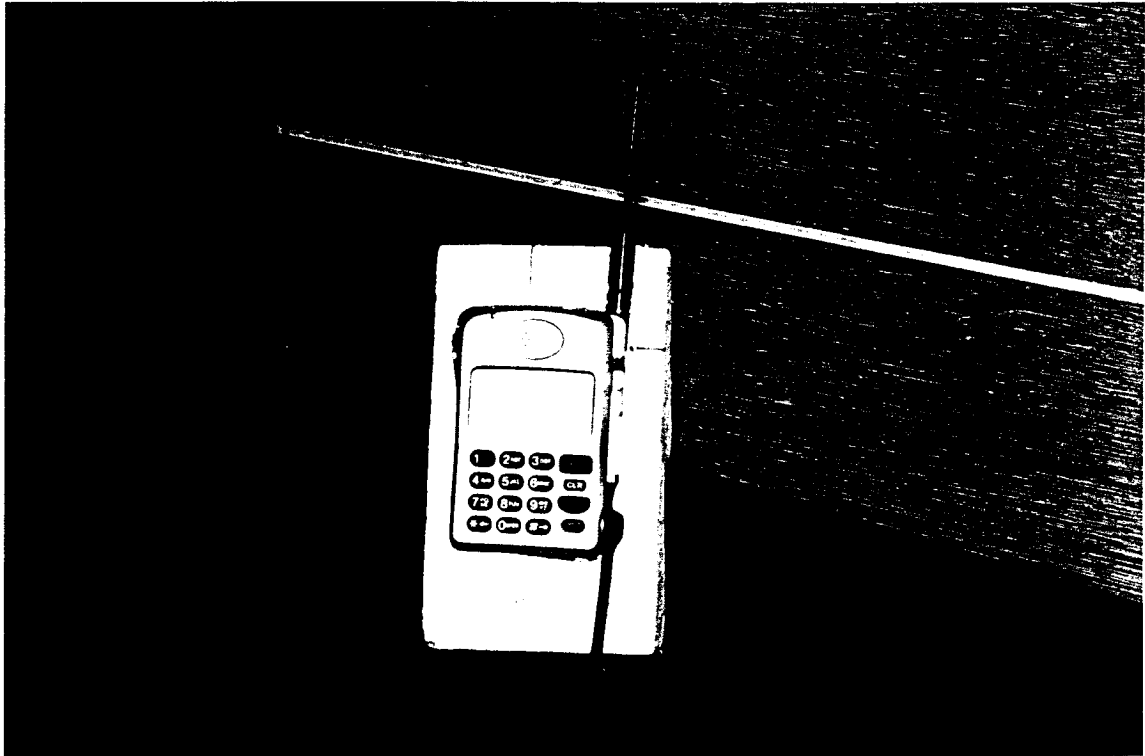

b.

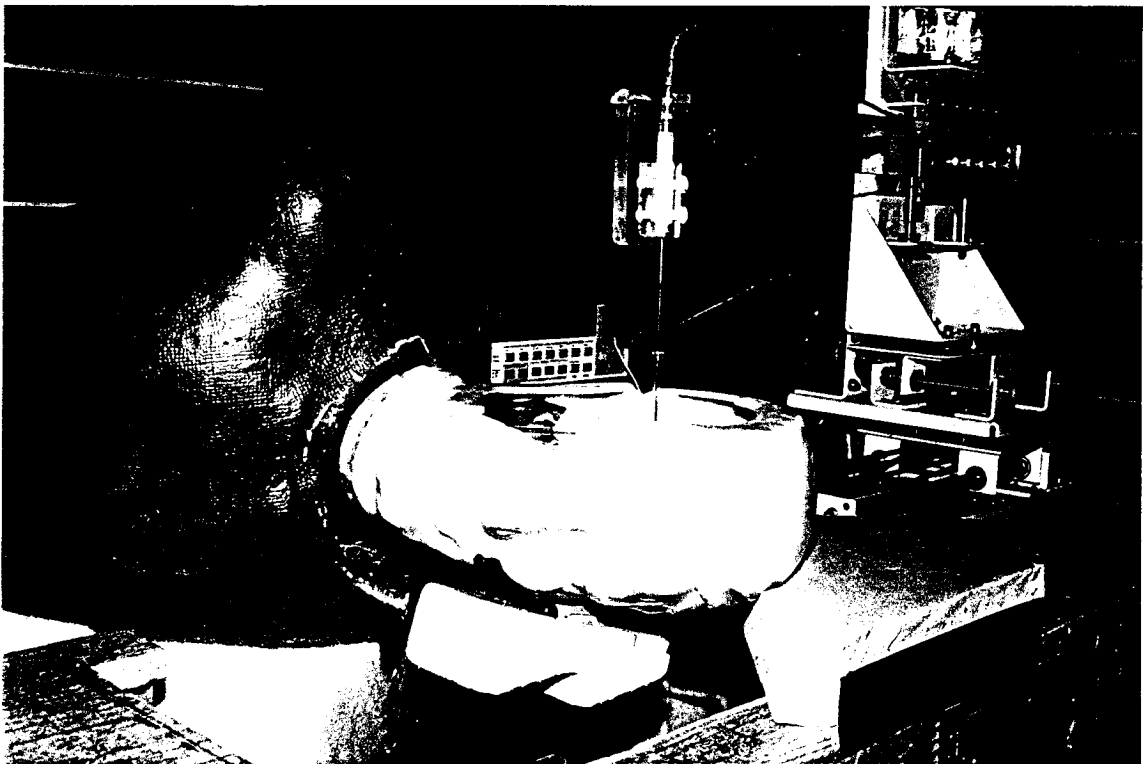


Fig. 1 a. The closeup of Sony Model CM-Z200 Cellular Telephone, and
b. The phantom model used for measurement of the SAR distribution for CM-Z200 Cellular Telephone.

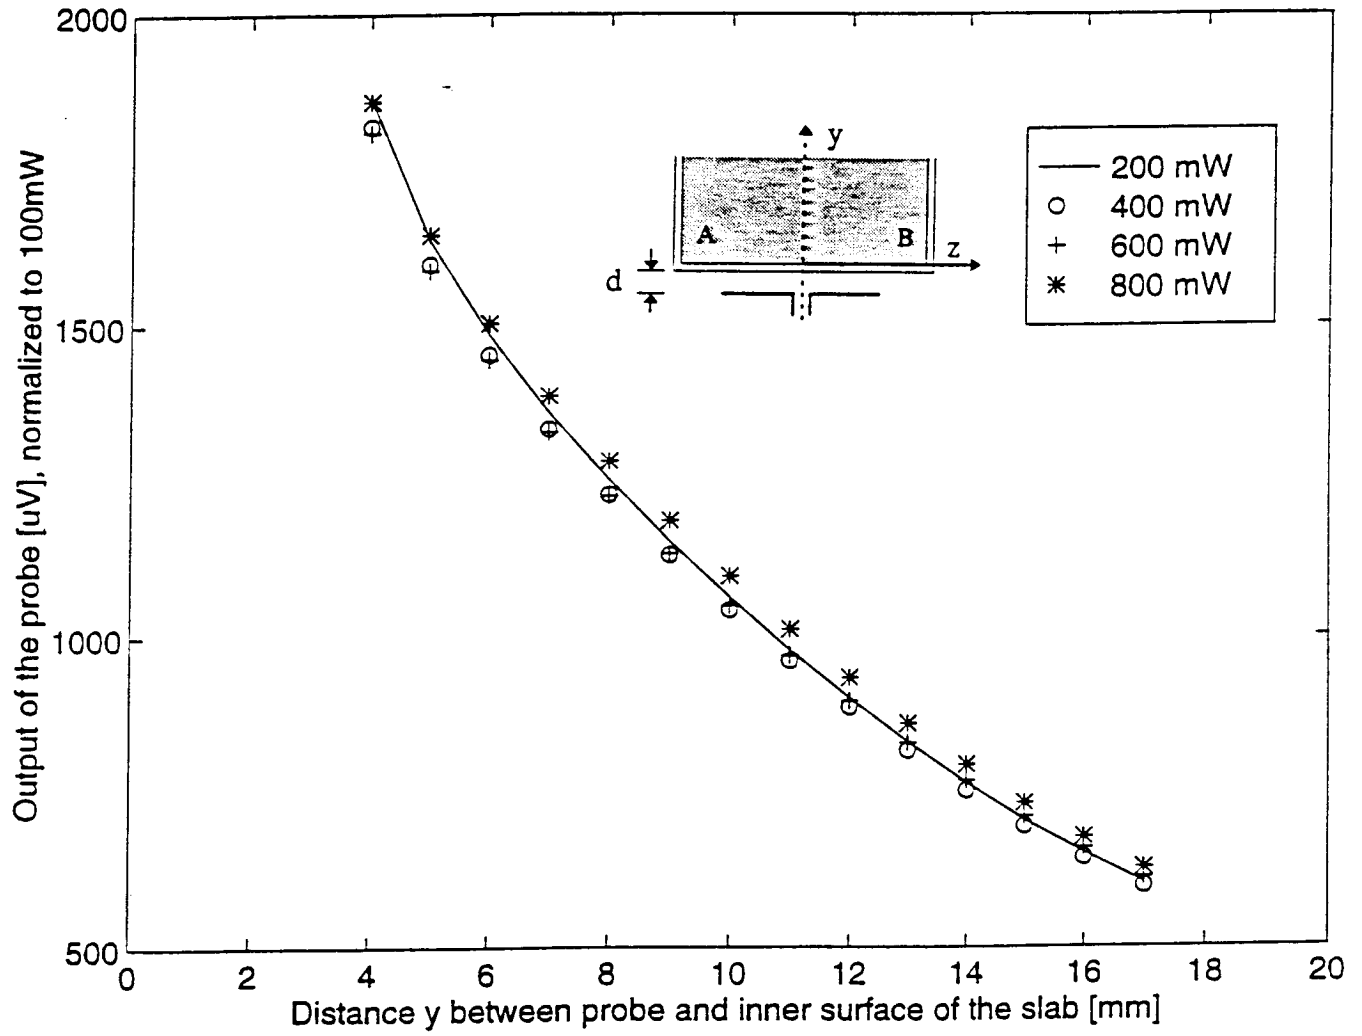


Fig. 2a. Test for square-law behavior at 840 MHz: Variation of the output voltage (proportional to $|E_i|^2$) for different radiated powers normalized to 0.1 W.

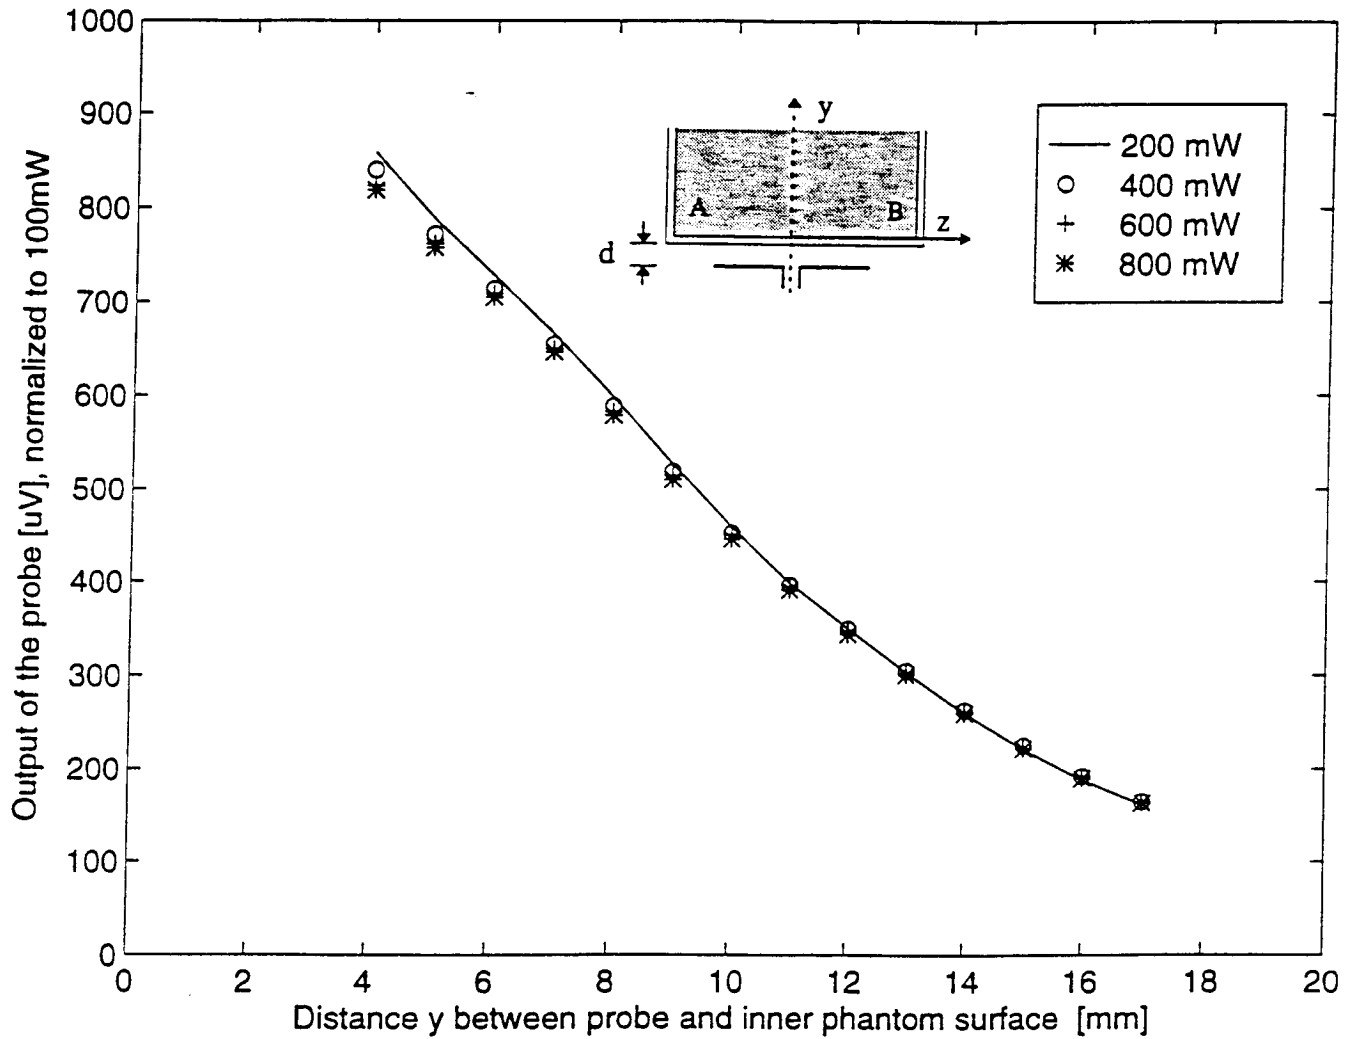


Fig. 2b. Test for square-law behavior at 1900 MHz: Variation of the output voltage (proportional to $|E_1|^2$) for different radiated powers normalized to 0.1 W.

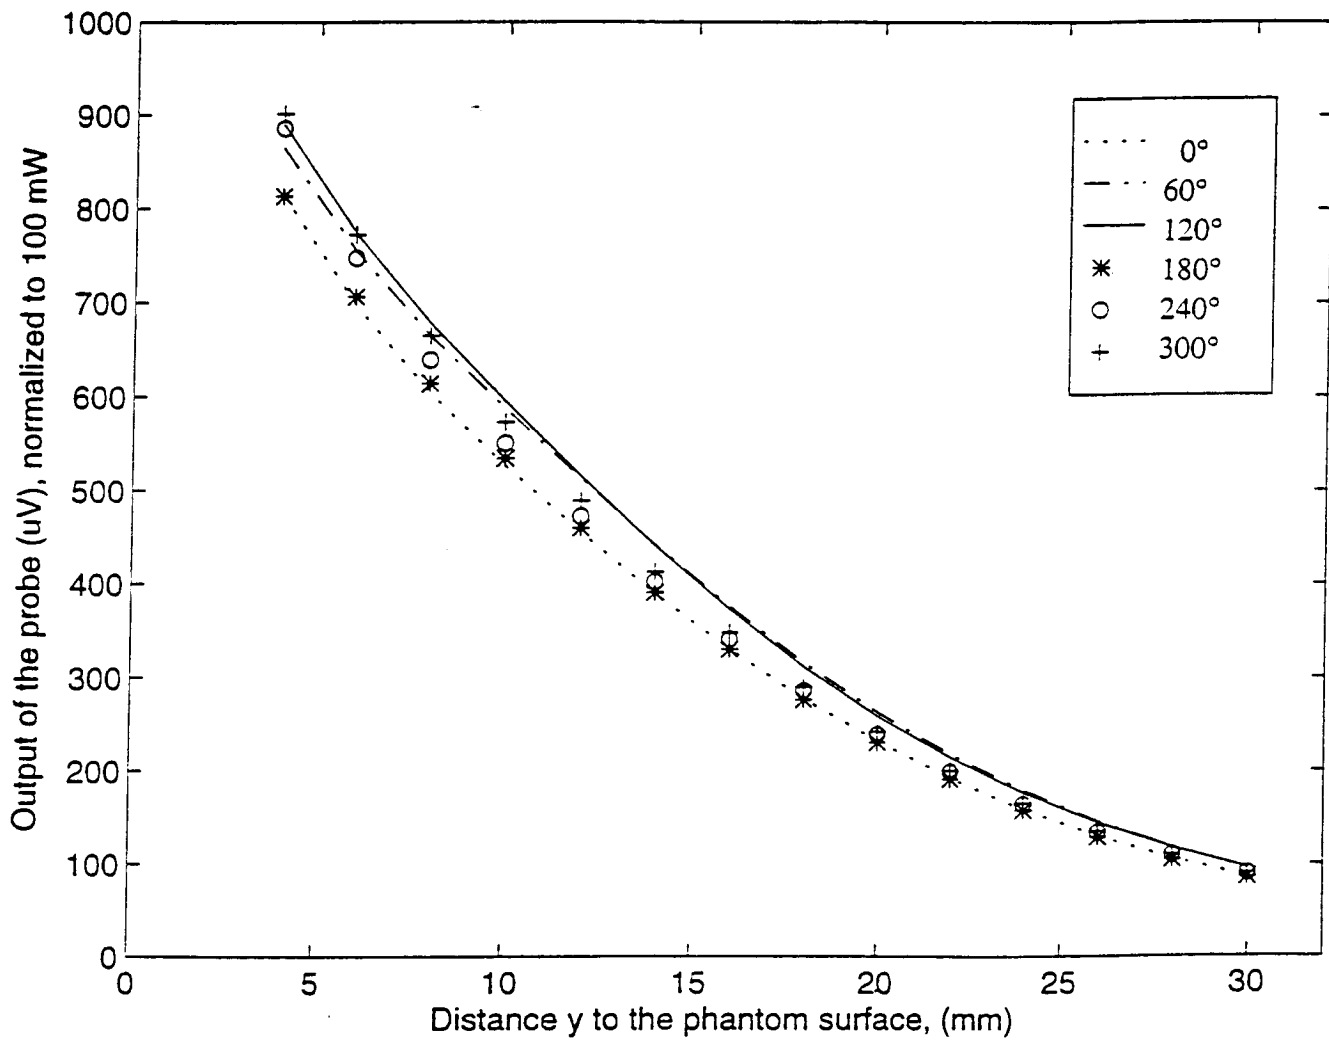


Fig. 3a. Test for isotropy: The model shown in Fig. 1 was used with nominal half wavelength dipole radiator of length 178 mm at 840 MHz.

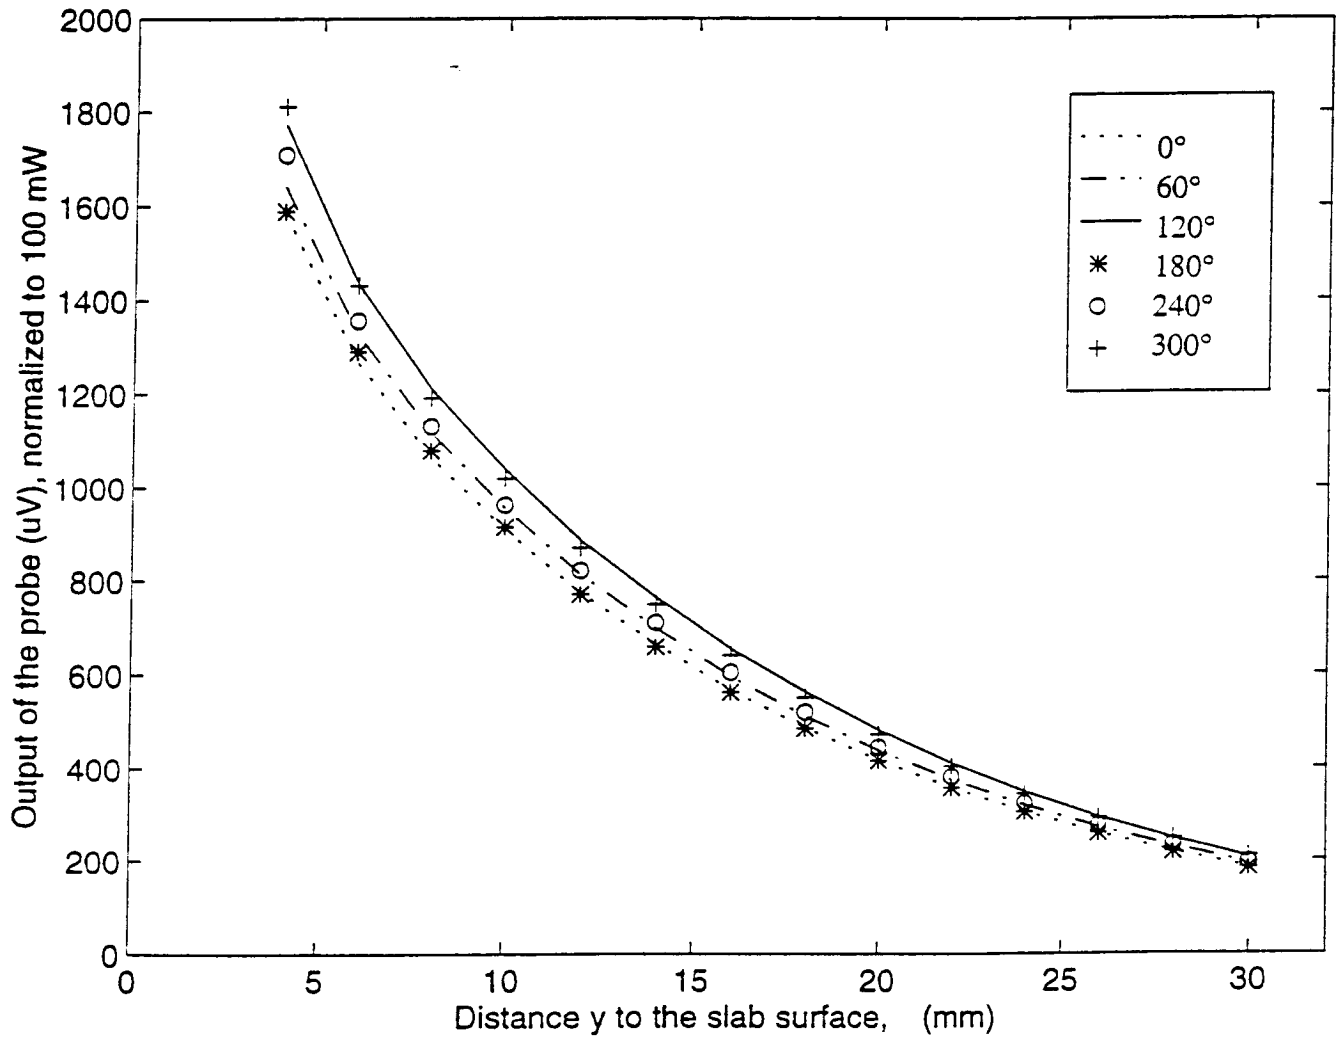


Fig. 3b. Test for isotropy: The model shown in Fig. 1 was used with nominal half wavelength dipole radiator of length 77 mm at 1900 MHz.

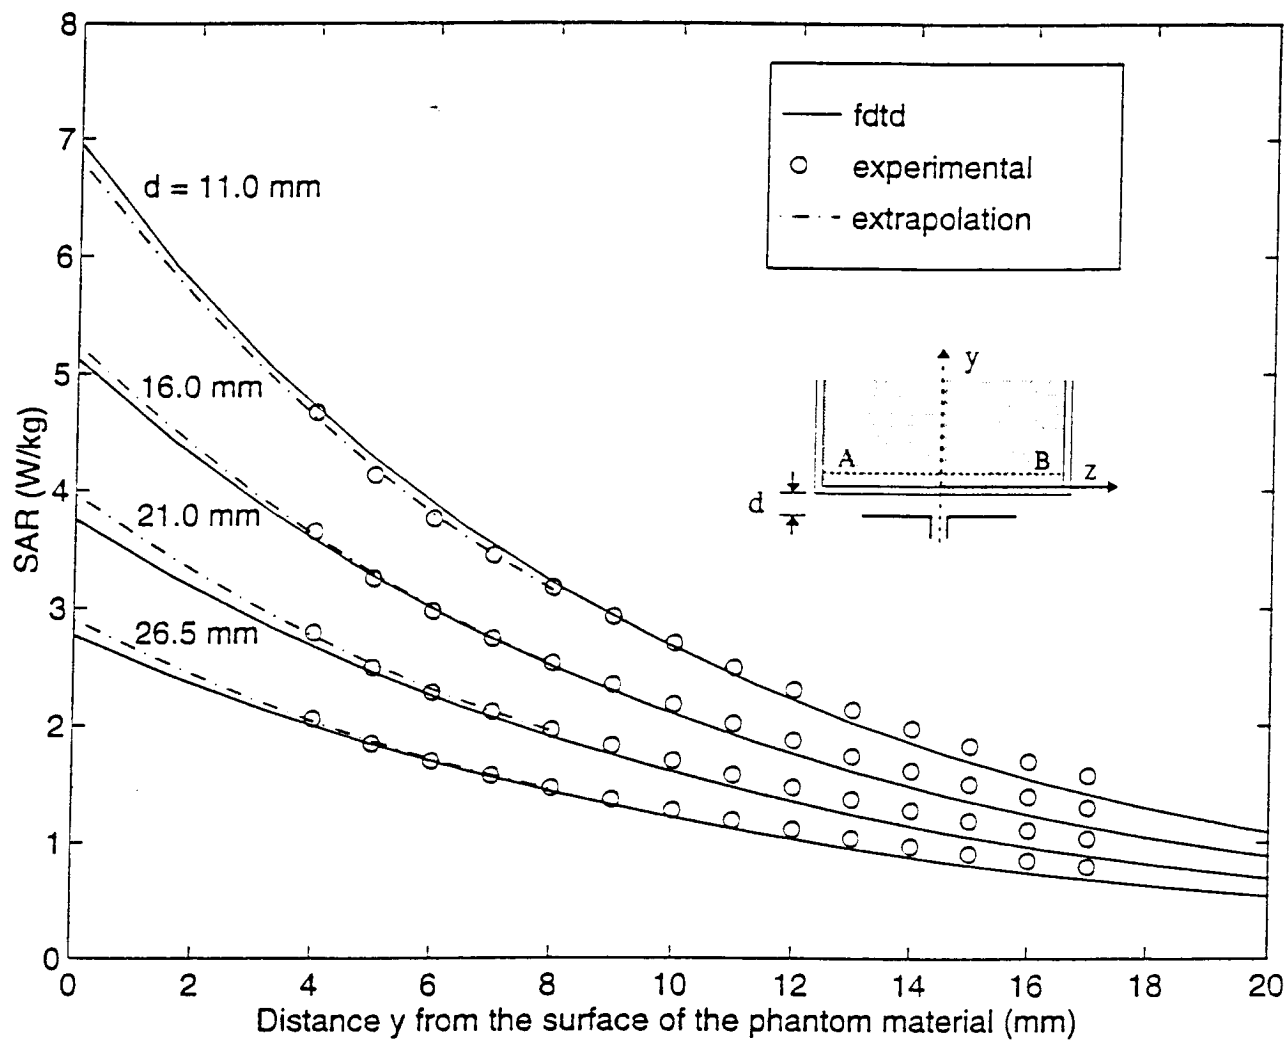


Fig. 4a. Comparison of the calculated and measured SAR variations for a box phantom of dimensions $30 \times 15 \times 50$ cm; 840 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 840 MHz = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

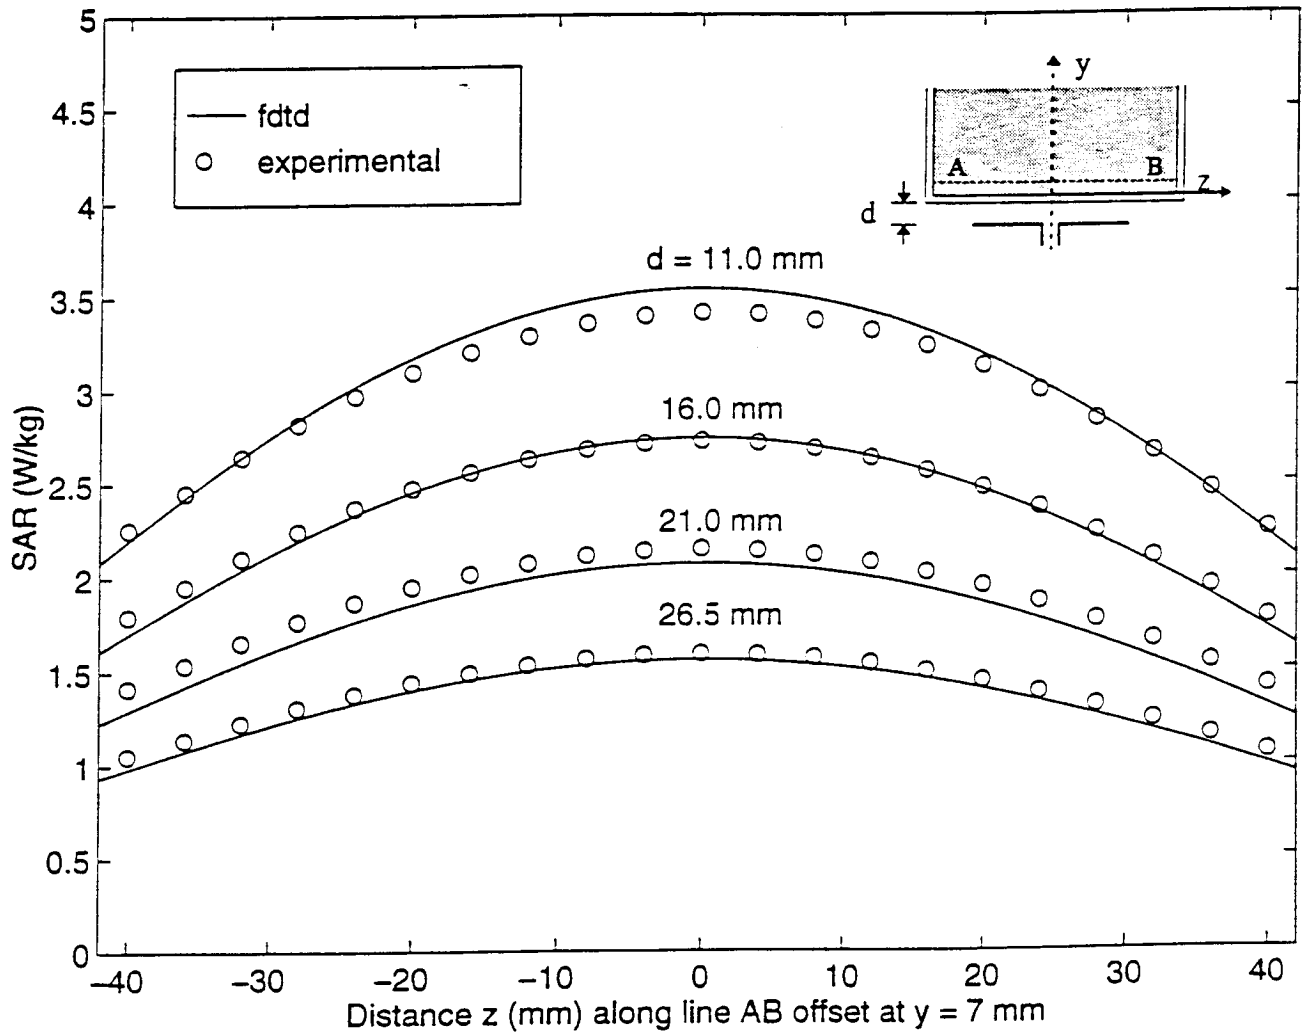


Fig. 4b. Comparison of the calculated and measured SAR variations for a box phantom of dimensions $30 \times 15 \times 50$ cm for a line AB parallel to the z axis at a distance $y = 7$ mm from the surface of the phantom material; 840 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 840 MHz = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

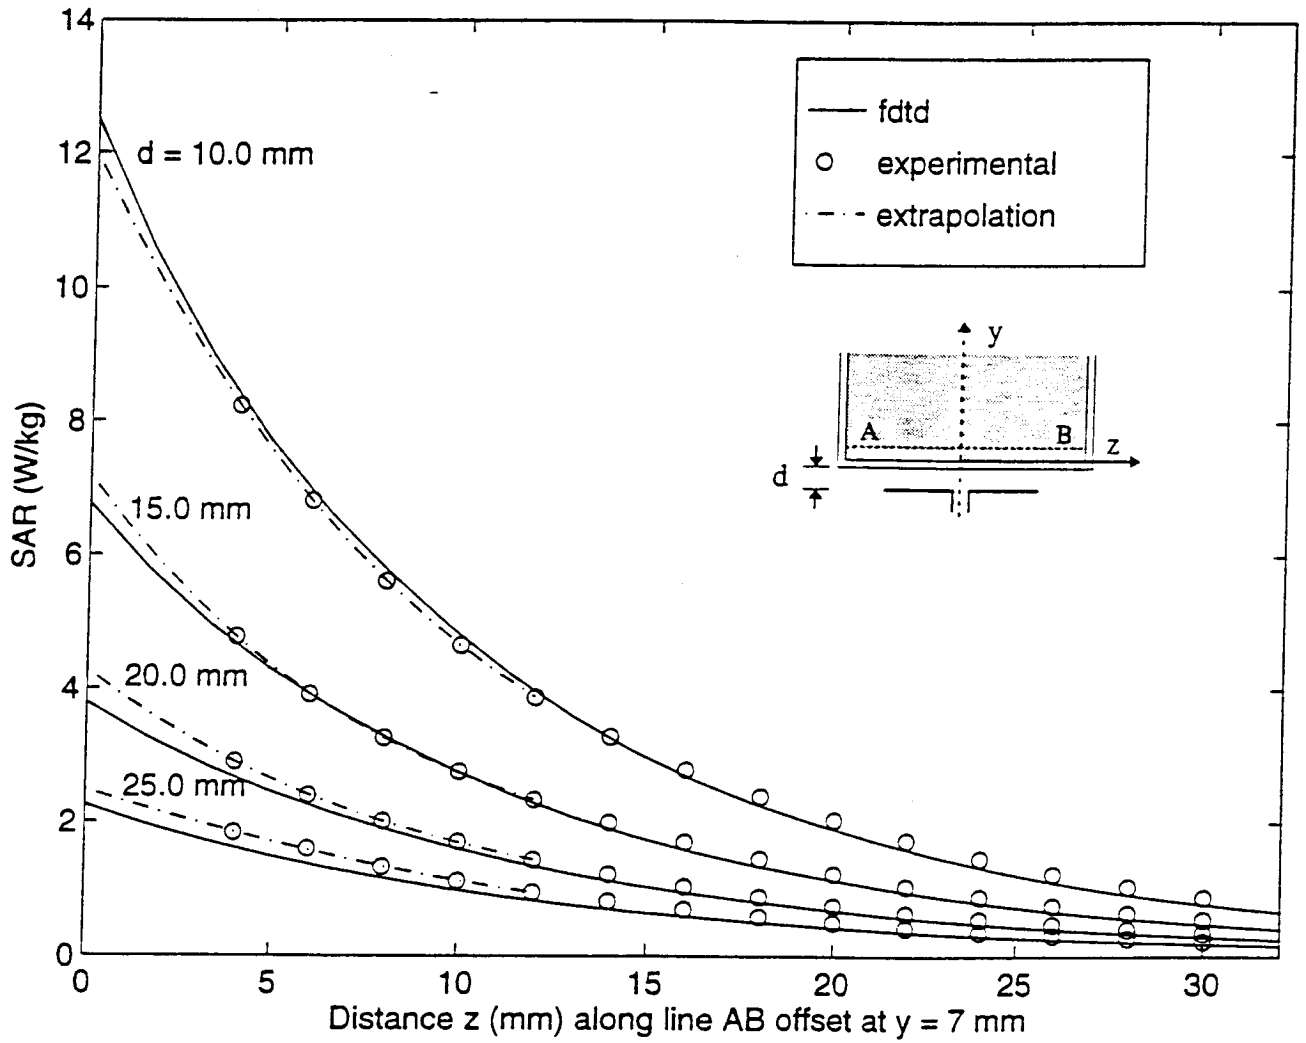


Fig. 5a. Comparison of the calculated and measured SAR variations for a box phantom of dimensions $30 \times 15 \times 50$ cm; 1900 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 1900 MHz = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.

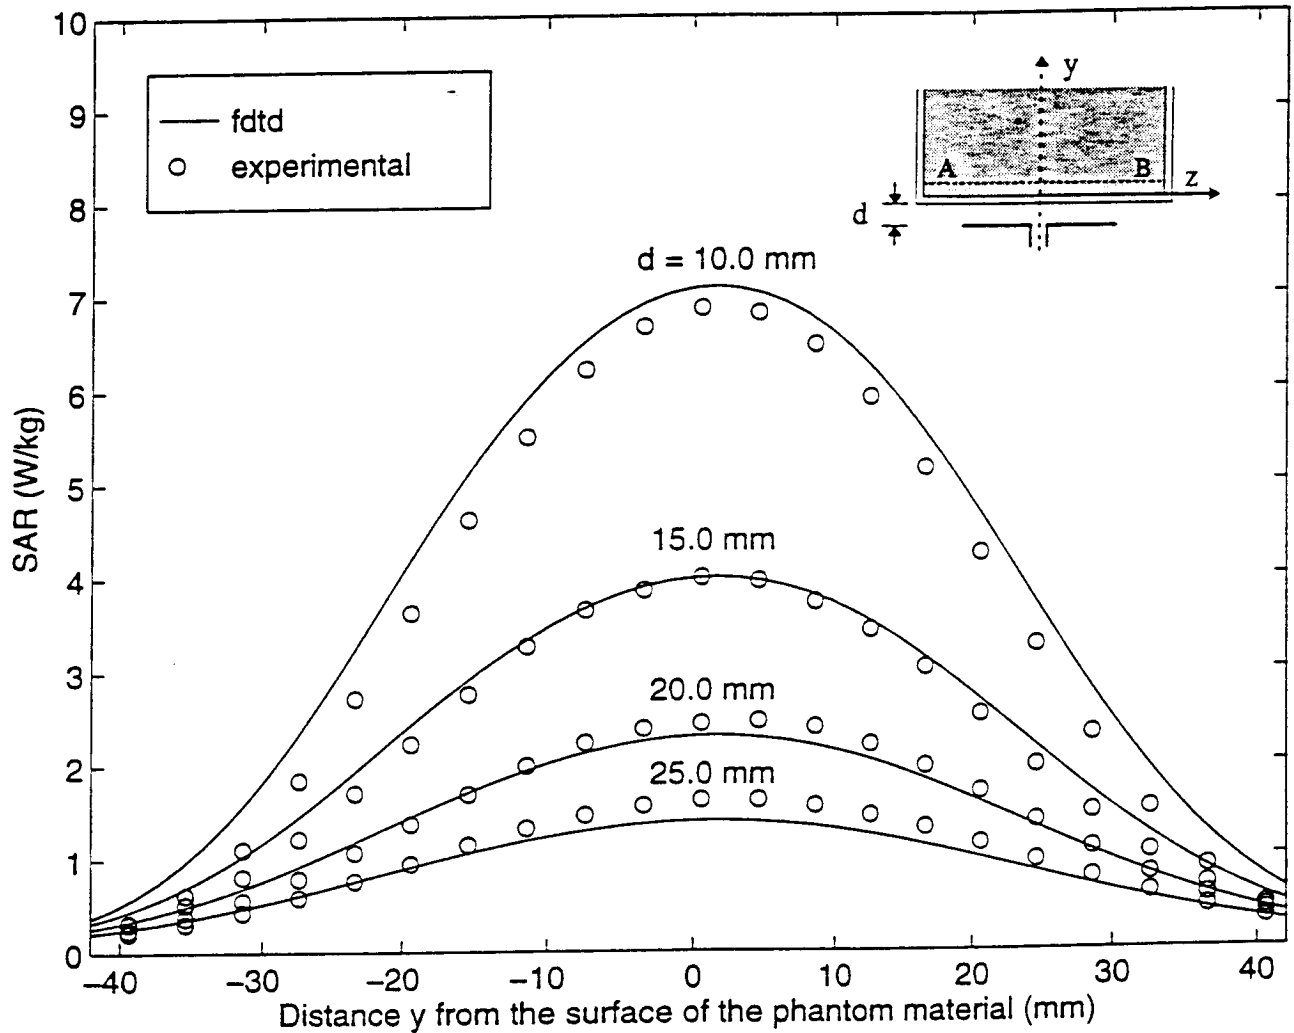


Fig. 5b. Comparison of the calculated and measured SAR variations for a box phantom of dimensions $30 \times 15 \times 50$ cm for a line AB parallel to the z axis at a distance $y = 7$ mm from the surface of the phantom material; 1900 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 1900 MHz = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.

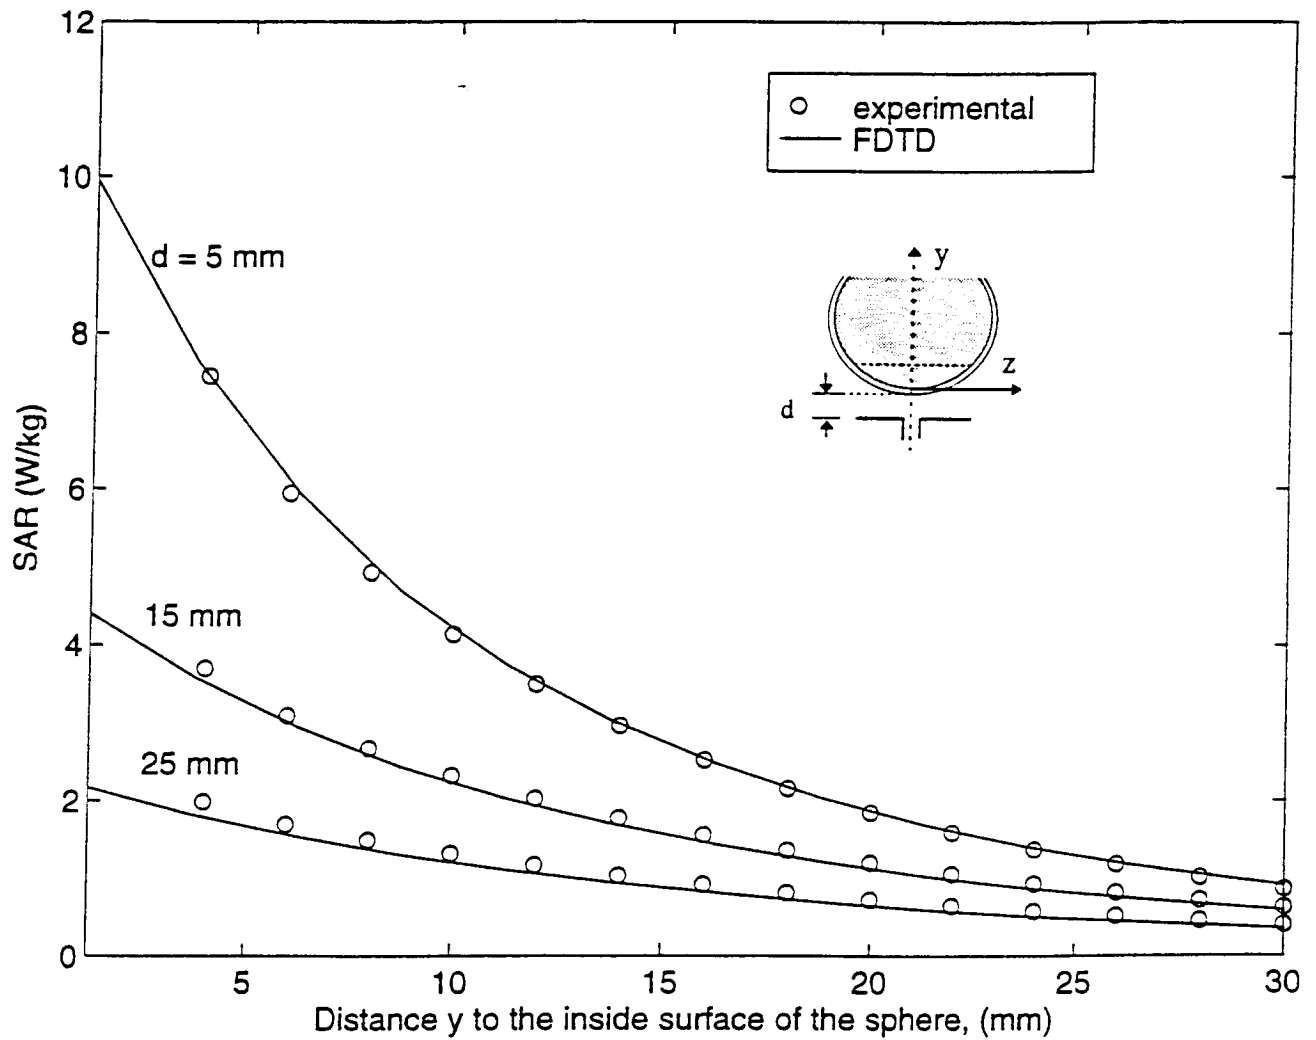


Fig. 6a. Comparison of measured and FDTD-calculated SAR variations at 840 MHz for a glass sphere model of outer diameter 22.3 cm and thickness 5 mm. SARs normalized to a radiated power of 0.5 W. Calibration factor = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

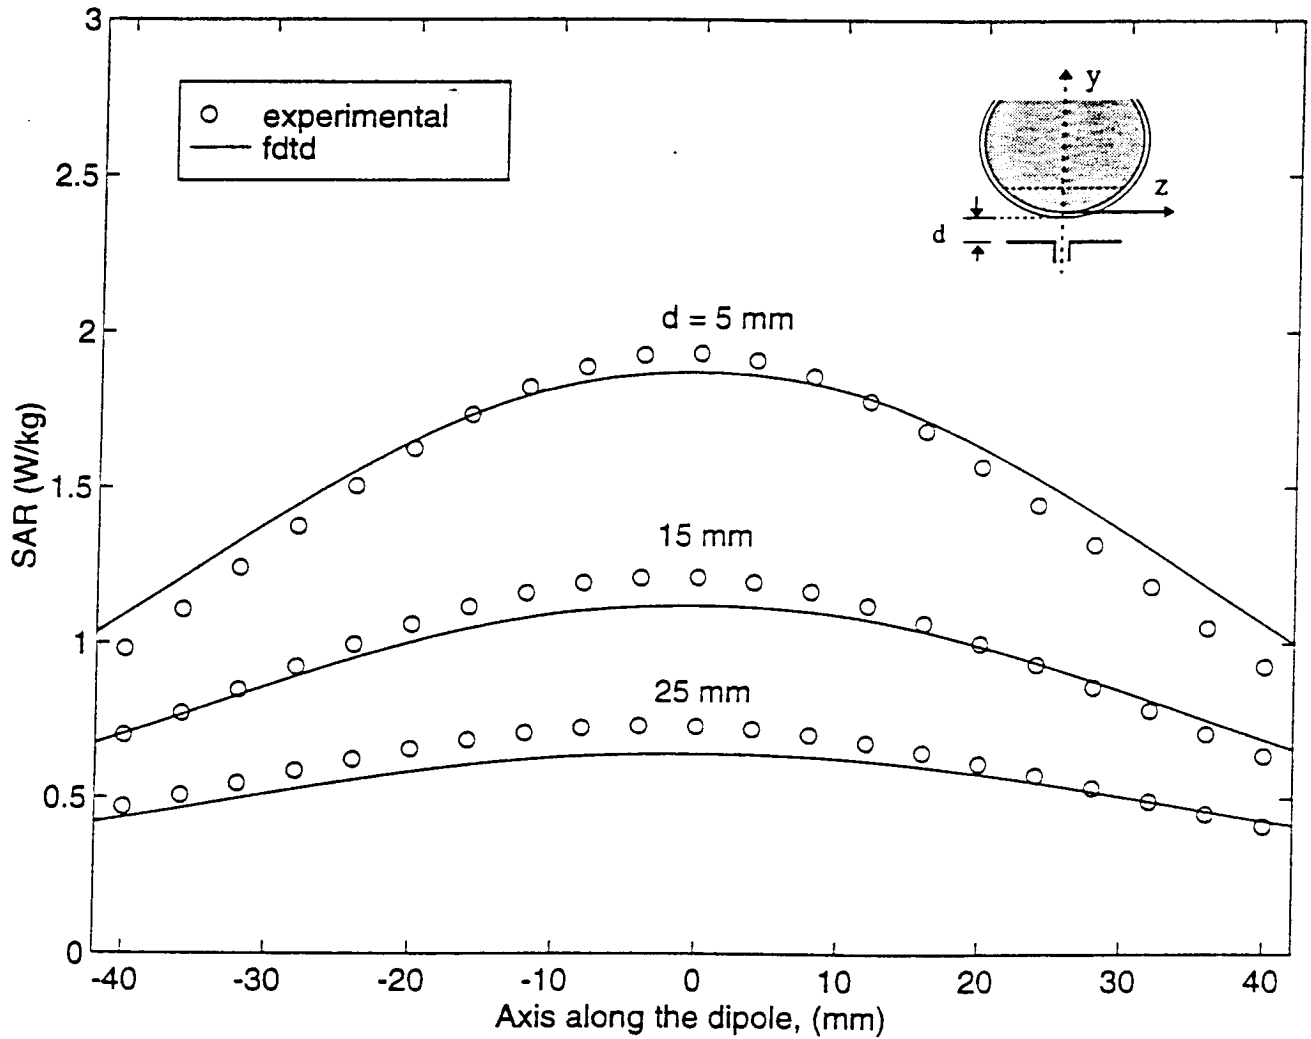


Fig. 6b. Comparison of calculated and measured SAR variations at 840 MHz for a plane at a distance of 20 mm from the lowest point on the inside of the sphere. SARs normalized to a radiated power of 0.5 W. Calibration factor = $0.49 \text{ (mW/kg)/}\mu\text{V}$. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06 \text{ S/m}$.

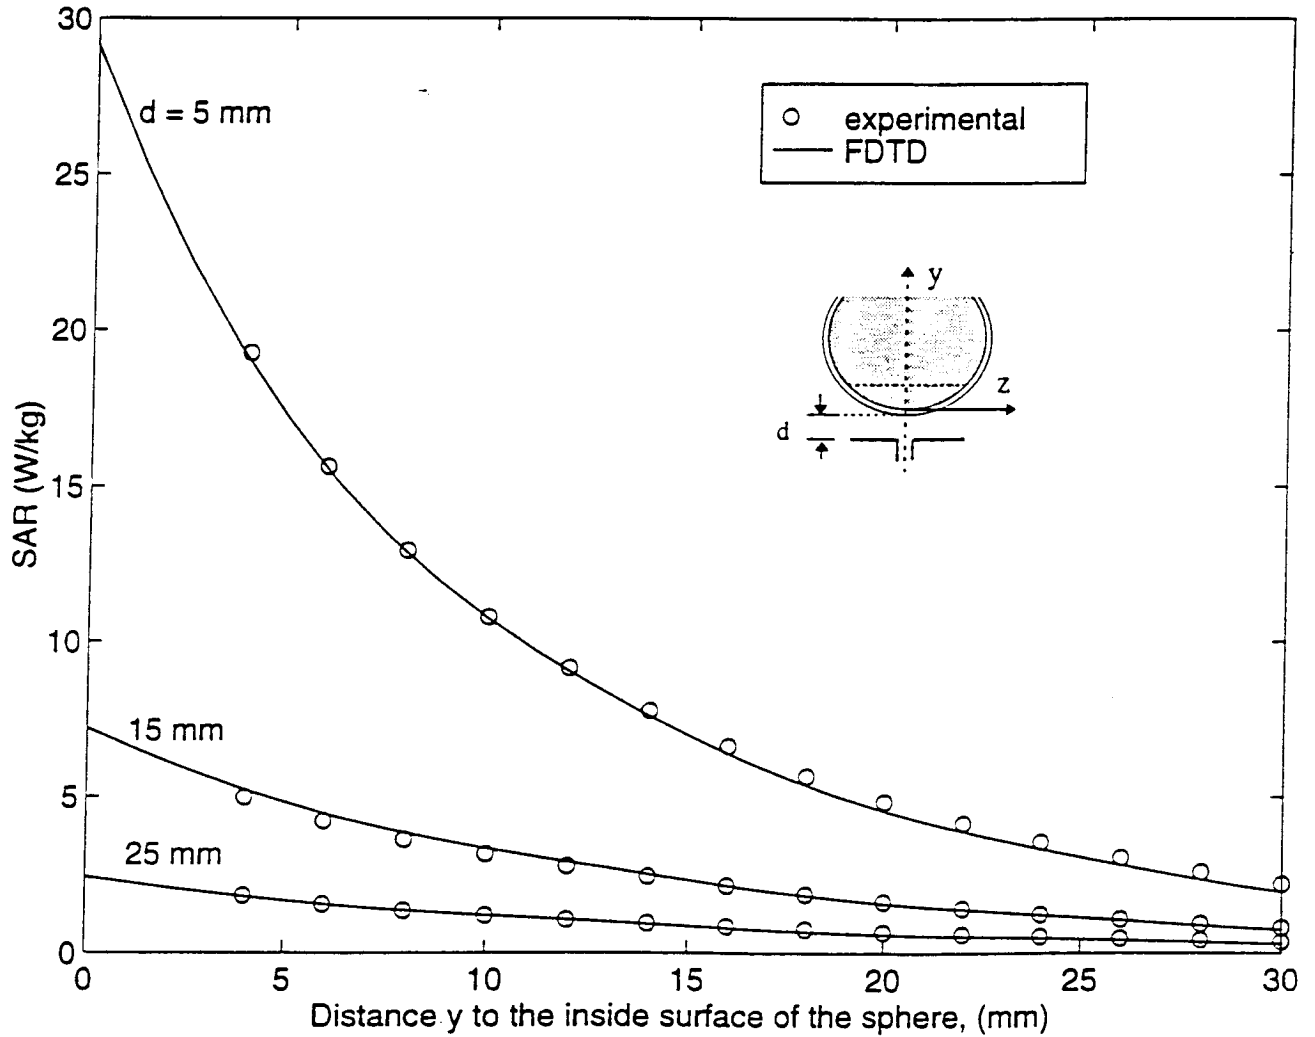


Fig. 7a. Comparison of measured and FDTD-calculated SAR variations at 1900 MHz for a glass sphere model of outer diameter 22.3 cm and thickness 5 mm. SARs normalized to a radiated power of 0.5 W. Calibration factor = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.

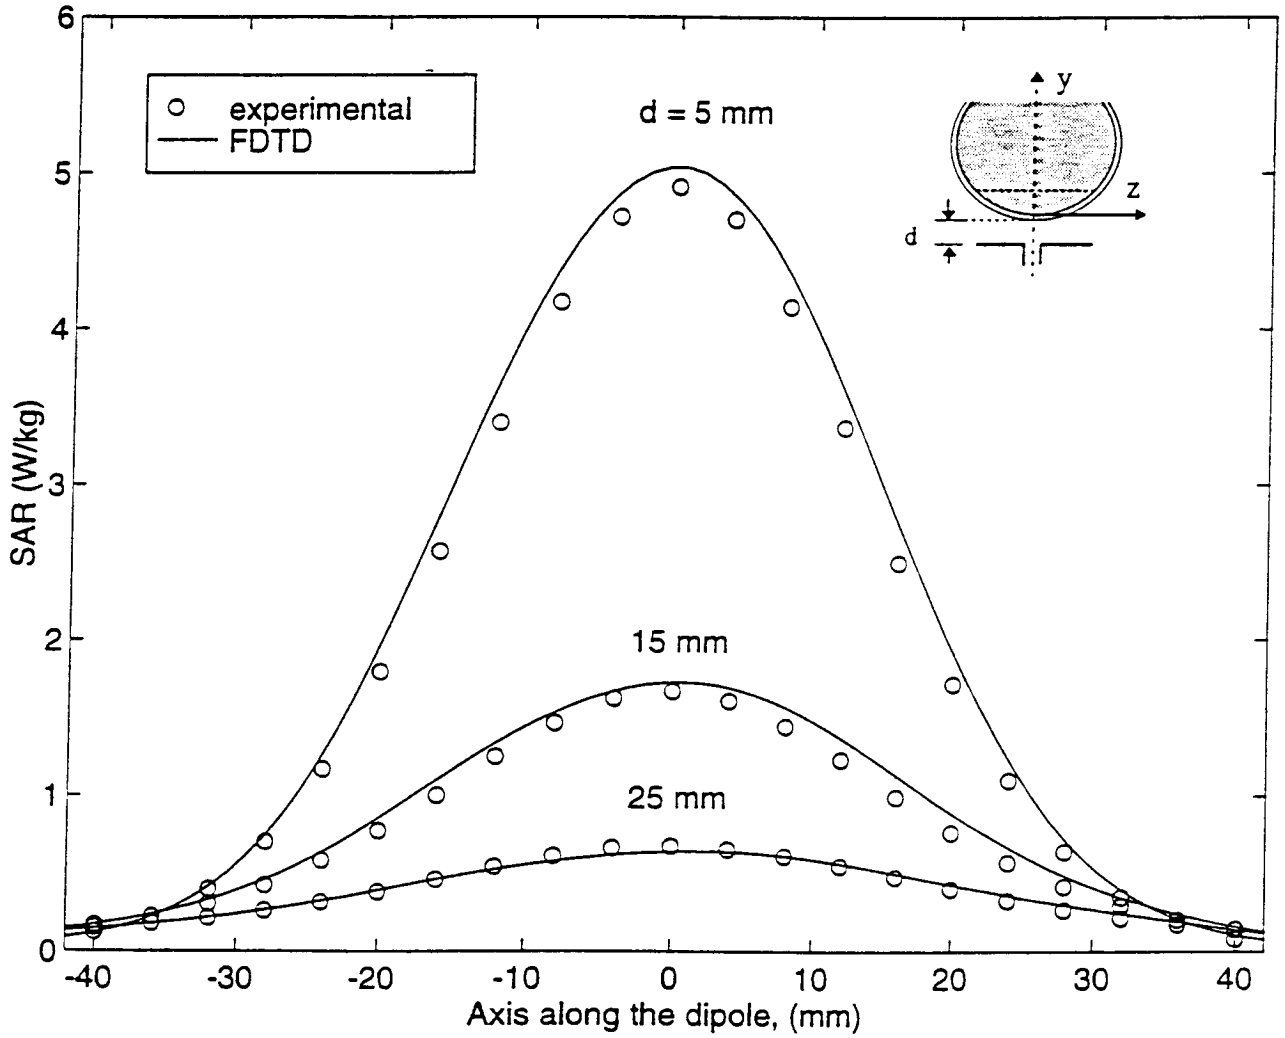


Fig. 7b. Comparison of calculated and measured SAR variations at 1900 MHz for a plane at a distance of 20 mm from the lowest point on the inside of the sphere. SARs normalized to a radiated power of 0.5 W. Calibration factor = $0.84 \text{ (mW/kg)/}\mu\text{V}$. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31 \text{ S/m}$.

An Automated SAR Measurement System for Compliance Testing of Personal Wireless Devices

Q. Yu, M. Aronsson, D. Wu, and O.P. Gandhi

Department of Electrical Engineering
University of Utah
Salt Lake City, Utah 84112

Abstract

An automated SAR measurement system has been developed for compliance testing of personal wireless devices. The setup uses a 3-D stepper motor system to move a Narda Model 8021 E-field probe to measure the SAR distribution inside a head-shaped tissue-simulant phantom near the radiating device. The head and neck part of the model is made of an outer shell of 5-7 mm thickness of epoxy laced with KCl solution for losses. This and the upper part of the torso are filled with a liquid with measured electrical properties (dielectric constant and conductivity) that are close to those for the brain at the center frequencies of interest (840 and 1900 MHz). The implantable E-field probe is calibrated against FDTD-calculated SAR variations for a slab model at AMPS (840 MHz) and PCS (1900 MHz) frequencies and is checked to have good isotropic characteristics (± 0.23 dB) and a wide dynamic range (1 mW/kg - 10 W/kg). The system is validated using a 223 mm diameter sphere model. Several commercial telephones with different types of antennas have been measured for 1-g SAR using the system, and excellent agreement (within ± 1 dB) with numerical results has been obtained.

I. Introduction

The use of cellular telephones and mobile wireless communication systems has increased dramatically during the past few years. Meanwhile, there is public concern for safety of RF exposure from these devices. Since the RF exposure is quantified by the mass-normalized rate of electromagnetic energy absorption or the Specific Absorption Rate (SAR), the U.S. Federal Communications Commission (FCC) requires that the SAR values of new personal wireless devices must meet the prescribed RF safety guidelines [1]. Furthermore, since electromagnetic energy absorbed by the human head depends to a large extent on the antenna used for the personal wireless devices [2], knowledge of SAR distributions in the human head can also help the industry to design better antennas to improve the performance of the wireless transceivers. In this regard we should note that 30-65 percent of the power radiated by the helix-monopole antennas used today is wasted by absorption in the human head and hand [2] and this could be reduced greatly.

Recent dosimetric studies on the RF exposure to the human body from personal wireless devices have been carried out by both numerical simulation [3-5] and experimental measurements [6, 7]. Numerical methods using millimeter resolution anatomically based human body models and CAD files could simulate the human body and the cellular phones in much more detail, respectively, thus providing highly accurate information about the electromagnetic coupling of the radiating device to the human body [8], but they generally require increasing computational resources (memory and computation time) for just one test condition of the device [8]. To alleviate this problem, use of the expanding grid FDTD method [9] together with the use of the truncated models of the head [10] has resulted in savings of memory requirements by factors in excess of

20 making it possible to compute the high resolution SAR distributions using workstations instead of parallel computers [11]. Nevertheless, if a device is to be tested for several orientations relative to the head, an easy, fast experimental procedure with validated accuracy and repeatability is of interest. The difficulties encountered by the experimental techniques lie mainly in two aspects: the construction of a validated phantom model that could accurately simulate electromagnetic coupling to the human head at least in the context of peak 1-g SAR for compliance testing required by FCC [1], and a miniature E-field probe which has a wide dynamic range and good isotropy and is calibrated properly at the AMPS (840 MHz) and PCS (1900 MHz) frequencies. In this paper, we will present an automated SAR measurement system developed for compliance testing at both 840 and 1900 MHz. The system is fully automated by a 3D stepper motor system controlled by a computer, with a miniature implantable E-field probe that is used to determine spatial SAR variations. The head and neck part of the phantom model is made of an outer shell of 5-7 mm thickness of epoxy laced with KCl solution for losses. This and the upper part of the torso are filled with a liquid with measured electrical properties (dielectric constant and conductivity) close to the average properties of the brain for white and gray matters at the center frequency of interest. Ten commercial telephones, five each at 840 and 1900 MHz, with different types of antennas have been measured for peak 1-g SARs using this system. Agreement with the FDTD-calculated values using the anatomically-based model of a male adult is within ± 1 dB.

II. Experimental Setup and Measurements

A. The Specific Absorption Rate (SAR)

The RF exposure to human body from wireless devices can be quantified by the Specific Absorption Rate (SAR) which measures the rate at which electromagnetic energy is absorbed by the exposed tissues. It can be expressed as follows[12]:

$$\text{SAR} = \sigma |E_i|^2 / \rho \quad (1)$$

where σ is the conductivity of the tissue, ρ is the mass density and E_i is the *rms* value of the internal electric field. The unit of SAR is Watts per kilogram (W/kg).

Since the SAR is proportional to the square of the local electric field, it can be determined by measuring the electric field inside the exposed tissue-simulant volume. Two SAR values are required for compliance testing [1]: the whole body average SAR, which is the ratio of the total power absorbed by the exposed body to its mass, should be below 0.08 W/kg, and the spatial peak SAR, as averaged over any of 1-g of tissue, which should not exceed 1.6 W/kg. Since most mobile telephones have an output power below 1 W, the whole body average SAR is well below the limit of 0.08 W/kg. The peak 1-g SAR, however, may exceed the safety limit for devices even with fairly low output power [2]. This therefore, needs to be accurately measured for compliance testing.

B. The Experimental Setup

The diagram of the experimental setup is shown in Fig. 1. A commercial Narda Model 8021 E-field probe is mounted on a computer-controlled 3D stepper motor system (Arrick Robotics MD-2A) to determine the SAR distributions inside the phantom tissue.

The positioning repeatability of the stepper motor system is within ± 0.1 mm. Outputs from the three channels of the E-field probe are dc voltages, the sum of which is proportional to $|E_i|^2$ as well as SAR through Eq. (1). The dc voltages are read by three HP 34401A multimeters and sent to the computer via GPIB interface. The setup is properly grounded to reduce noise due to EMI.

The internal surface of the phantom is pre-scanned with a high resolution (2x2 mm) so that the computer knows how far it can move the probe in the vertical direction (z) at each horizontal position (x, y) without breaking the probe. A special program is written to scan the phantom surface. Before scanning, a thin copper film is first tightly taped to the internal surface of the phantom, then a metal rod with the same shape and diameter as the E-field probe is moved by the stepper motor system on the programmed path to detect the surface, when the metal rod's tip touches the surface, an electrical signal is sent to the computer, the computer stops the stepper motor and records the position (x, y, z). Since the positions of the stepper motor system and the phantom are relatively stable, pre-scanning of the phantom surface is needed only once for each phantom model.

The compliance testing procedure includes two steps: a coarser sampling with a step size of 8.0 mm is done in the first instance to locate the peak SAR region. The coarser scan area is 4.8 cm x 8.0 cm, with each sampling close to the phantom surface. The peak SAR region is then sampled with a finer step size of 2.0 mm on a 3D grid over a 1 cm³ volume cube, a total of 5 x 5 x 5 points are measured. The fine scan data are processed by the computer to give the peak 1-g SAR. The whole testing procedure takes about 20 minutes with coarser and finer sampling steps taking about 10 minutes each, so

the measurement can be finished within the battery charge life of most personal wireless devices.

C. The Phantom Model

As shown in Fig. 2, the phantom model used in the setup has dimensions similar to the upper parts of the human body. The head and neck part of the model is made of an outer shell of 5-7 mm thickness of epoxy laced with KCl solution for losses. This and the upper part of the torso are filled with a liquid with measured electrical properties (dielectric constant and conductivity) close to the average properties of the brain for white and gray matters at the center frequency of interest. Table 1 shows the desired tissue properties [13] and the measured electrical properties of the skull- and brain-simulant materials at 840 and 1900 MHz. The head and neck region of the phantom is filled with brain simulating liquid materials of compositions given in Table 2. The model also has shoulders and chest, which are filled with a semi-solid composition of water, salt, polyethylene powder, and a gelling agent TX151 that simulates the dielectric properties equivalent to those of two-thirds muscle. The same material is used to fill a thin surgical rubber glove to create the shape of the hand. As shown in Fig. 2, the “hand “ thus created is used to hold the cellular telephone which is positioned against the phantom head along the line connecting the ear canal and the mouth of the phantom. This is done in order to load the handset similar to the dielectric loading provided by the hand in actual use of a hand-held wireless device.

Two different fluids of compositions given in Table 2 are used to simulate the average dielectric properties of the brain at 840 and 1900 MHz. The clear fluid used at

840 MHz is a composition of water, sugar, salt, and a gelling agent HEC proposed by Hartsgrave et al [14]. Even without salt, this composition has an electrical conductivity $\sigma = 1.65$ S/m which is considerably higher than $\sigma = 1.29$ S/m needed to simulate the average properties for the brain at 1900 MHz [13]. Thus we have developed another liquid brain simulating material for SAR measurements at 1900 MHz. The composition of this material is also given in Table 2. The dielectric properties of this material were measured using a HP 85070B dielectric probe measurement system and are given in Table 2. The brain-simulant composition for use at 1900 MHz has shown a very good long term stability (Table 3) when it is properly sealed after measurements to minimize the vaporization of water.

D. The E-field Probe

The non-perturbing implantable E-field probe used in the setup was originally developed by Bassen et al [15] and is now manufactured by L3/Narda Microwave Corporation, Hauppauge, New York as Model 8021 E-field probe. In the probe, three orthogonal miniature dipoles are placed on a triangular beam substrate. Each dipole is loaded with a small Schottky diode and connected to the external circuitry by high resistance ($2 \text{ M}\Omega \pm 40\%$) leads to reduce secondary pickups. The entire structure is then encapsulated with a low dielectric constant insulating material. The probe thus constructed has a very small (4 mm) diameter, which results in a relatively small perturbation of the internal electric field.

Test for Square Law Region

It is necessary to operate the E-field probe in the square law region for each of the diodes so that the sum of the dc voltage outputs from the three dipoles is proportional to the square of the internal electric field ($|E_i|^2$). Fortunately the personal wireless devices induce SARs that are generally less than 5-6 W/kg even for closest locations of the head [2]. For compliance testing it is therefore necessary that the E-field probe be checked for square law behavior for SARs up to such values that are likely to be encountered. Such a test may be conducted using a canonical lossy body such as a rectangular box or a sphere irradiated by a dipole. By varying the radiated power of the dipole, the output of the probe should increase linearly with the applied power for each of the test locations.

Shown in Figs. 3a, 3b are the results of the tests performed to check the square law behavior of the E-field probe used in our setup at 840 and 1900 MHz, respectively. For these measurements we have used a rectangular box of dimensions 30 x 15 x 50 cm that was irradiated by the corresponding half wave dipoles with different amounts of radiated powers from 200-800 mW. Since the dc voltage outputs of the probe are fairly similar when normalized to a radiated power of 100 mW, the square law behavior is demonstrated and an output voltage that is proportional to $|E_i|^2$ is obtained within ± 3 percent.

Test for Isotropy of the probe

Another important characteristic of the probe that affects the measurement accuracy is its isotropy. Since the orientation of the induced electric field is generally unknown, the E-field probe should be relatively isotropic in its response to the orientation

of the E-field. Shown in Figs. 4a, 4b are the test results of the E-field probe used in our setup at 840 and 1900 MHz, respectively. The previously described box phantom of dimensions 30 x 15 x 50 cm along x, y and z dimensions, respectively, was also used for these measurements. This phantom was filled to a depth of 15 cm with brain-simulant materials (Table 2). The E-field probe was rotated around its axis from 0 to 360° in incremental steps of 60°. An isotropy of less than ± 0.23 dB ($\pm 5.5\%$) was observed for this E-field probe both at 840 and 1900 MHz.

Calibration of the E-field Probe

Since the voltage output of the E-field probe is proportional to the square of the internal electric field ($|E_i|^2$), from the definition of SAR (Eq. 1), the SAR is therefore proportional to the voltage output of the E-field probe by a proportionality constant C. The constant C is defined as the calibration factor, and is frequency and material dependent. It is measured to calibrate the probe at the various frequencies of interest using the appropriate tissue-simulating materials for the respective frequencies.

Canonical geometries such as waveguides, rectangular slabs and layered or homogeneous spheres have in the past been used for the calibration of the implantable E-field probe [16-18]. Since the Finite Difference Time Domain (FDTD) has been carefully validated to solve electromagnetic problems for a variety of geometries [19, 20], we were able to calibrate the Narda E-field probe by comparing the measured variations of the probe voltage ($\approx |E_i|^2$) against the FDTD-calculated variations of SARs for a box phantom of dimensions 30 x 15 x 50 cm used previously for the data given in Figs. 3 and 4, respectively. For these measurements we placed the nominal half-wave dipoles of lengths

178 mm and 77 mm at 840 and 1900 MHz, respectively, at several distances d (see inserts of Figs. 5a, 5b and 6a, 6b) from the outer surface of the acrylic ($\epsilon_r = 2.56$) box of thickness 6.55 mm. Shown in Figs. 5a, 5b and 6a, 6b are the comparisons between the experimentally measured and FDTD-calculated variations of the SAR distributions for this box phantom. Since there are excellent agreements between the calculated SARs and the measured variations of the voltage output of the E-field probe for four different separations d of the half wave dipoles at each of the two frequencies, it is possible to calculate the calibration factors at the respective frequencies. For the Narda Model 8021 E-field probe used in our setup, the calibration factors are determined to be 0.49 and 0.84 (mW/kg)/ μ V at 840 and 1900 MHz, respectively

III. Experimental Results: Canonical Problems

To further validate the system, it has been used to measure the peak 1-g SAR for the above-mentioned box phantom and a glass sphere model of thickness 5 mm, external diameter = 223 mm and dielectric constant $\epsilon_r = 4.0$. This sphere model is once again filled with the corresponding brain-simulant fluids of compositions given in Table 2. Shown in Figs. 7a, 7b and 8a, 8b are the measured and FDTD-calculated SAR distributions inside the sphere for various separations d between the dipole and the sphere (see insert for Figs. 7, 8). Comparison of the measured and FDTD-calculated peak 1-g SARs for both phantom geometries are given in Table 4 and 5, respectively. As can be seen, the agreement between experimental measurement and numerical simulation is excellent and generally within ± 10 percent for both rectangular and spherical phantoms.

Since the dipole sensors of the Narda Model 8021 E-field probe used for SAR measurements are recessed about 4 mm from the tip of the probe, it is necessary to use an extrapolation subroutine to obtain the SARs at the internal surface for both of these phantoms as these are generally the highest and contribute the most to the peak 1-g SAR. A second order polynomial obtained by using the least mean square error method to fit the measured data was used to extrapolate the SARs to the phantom surface in our measurements. As shown in Figs. 5a, 6a, the results are satisfactory compared to the FDTD simulations.

IV. SAR Measurements for Cellular Telephones

The automated setup shown in Fig. 2 has been used for the testing of ten commercial personal wireless devices five each at 835 and 1900 MHz, respectively. Given in Table 6 is the comparison of the numerical and measured peak 1-g SARs for these devices using our experimental phantom model and the FDTD-based numerical procedure used for calculations of SAR distributions for an anatomically-based model of the head of an adult male. The measured and calculated SARs for the ten telephones which have quite different operational modes (TDMA, CDMA, etc.) and antenna structures (helical, monopole, or helix-monopole) vary from 0.13 to 5.41 W/kg. Even though widely different peak 1 g SARs are obtained because of the variety of antennas and handsets, agreement between the calculated and the measured data is excellent and generally within $\pm 20\%$ (± 1 dB). This is particularly remarkable since an MRI-derived, 16-tissue anatomically-based model of the adult human head is used for FDTD calculations and a relatively simplistic two tissue phantom model is used for experimental

peak 1-g SAR measurements. It is interesting to note that even though the dielectric properties of the external shell (Fig. 2) are not as high as for human skull (see Table 1), the peak 1-g SARs obtained with this experimental phantom model are quite accurate.

V. Conclusions

An automated SAR measurement system has been developed with a dynamic range (1mW/kg to 10W/kg) suitable for the compliance testing of personal wireless devices. With a miniature Narda E-field probe, the system provides accurate measurements at 840 MHz as well as 1900 MHz. Besides the peak 1-g SAR, the system also gives the SAR distributions for any radiating device, thus providing information for better antenna design.

The E-field probe is a crucial part of the system. The accuracy of measurement can be further improved by using probes with still smaller size, better isotropy and less sensor offset from the tip. The dielectric properties of the various tissues for a heterogeneous phantom have been well established and recognized, however, since the SAR measurements are very sensitive to the geometric shape and size of the phantom model, it would be desirable to standardize the phantom model for consistent and comparable testing results. Before a phantom model can be considered to be acceptable, it should be validated, as in Table 6, for accuracy relative to realistic anatomically-based models of the human body.

Acknowledgment

The authors gratefully acknowledge many helpful discussions and the FDTD calculations provided by Drs. Gianluca Lazzi and Adam Tinniswood.

References

1. FCC 96-326, "Guidelines for evaluating the environmental effects of radio frequency radiation," August 1, 1996, Federal Communications Commission, Washington, DC, 20554.
2. O. P. Gandhi, G. Lazzi, and C. M. Furse, "Electromagnetic absorption in the human head and neck for mobile telephones at 835 and 1900 MHz," *IEEE Trans. Microwave Theory Tech.*, Vol. 44, pp. 1884-1897, 1996.
3. P. J. Dimbylow and S. M. Mann, "SAR calculations in an anatomically based realistic model of the head for mobile communication transceivers at 900 MHz and 1.8 GHz," *Physics in Medicine and Biology*, Vol. 39, pp. 1537-1553, 1994.
4. O. P. Gandhi and J. Y. Chen, "Electromagnetic absorption in the human head from experimental 6-GHz transceivers," *IEEE Trans. Electromag. Compat.*, Vol. 37, pp. 547-558, 1995.
5. M. A. Jensen and Y. Rahmat-Samii, "EM interaction in handset antennas and a human in personal communications," *Proc. IEEE*, Vol. 83, pp. 7-17, 1995.
6. Q. Balzano, O. Garay, and T. J. Manning, Jr., "Electromagnetic energy exposure of simulated users of portable cellular telephones," *IEEE Trans. Veh. Technol.*, Vol. 44, pp. 390-403, 1995.
7. T. Schmid, O. Egger, and N. Kuster, "Automated E-field scanning system for dosimetric assessments," *IEEE Trans. Microwave Theory Tech.*, Vol. 44, pp. 105-113, 1996.
8. A. D. Tinniswood, C. M. Furse and O. P. Gandhi, "Computations of SAR distributions for two anatomically-based models of the human head using CAD files of commercial telephones and the parallelized FDTD code," *IEEE Trans. Antennas Propagat.*, Vol. 46, 1998.
9. B. Q. Gao and O. P. Gandhi, "An expanding-grid algorithm for the finite-difference time-domain method," *IEEE Trans. Electromag. Compat.*, Vol. 34, pp. 277-283, 1992.
10. G. Lazzi and O. P. Gandhi, "Realistically tilted and truncated anatomically-based models of the human head for dosimetry of mobile telephones," *IEEE Trans. on Electromag. Compat.*, vol. 39, pp. 55-61, 1997.
11. A. Tinniswood, G. Lazzi and O. P. Gandhi, "The use of the expanding grid FDTD method for simulation of CAD-derived personal wireless devices," Submitted to *IEEE Trans. Microwave Theory Tech.*

12. M. A. Stuchly and S. S. Stuchly, "Experimental radio and microwave dosimetry," in *Handbook of Biological Effects of Electromagnetic Fields*, second edition, edited by C. Polk and E. Postow, CRC Press, Boca Raton, Florida, pp. 295-336, 1996.
13. C. Gabriel, "Compilation of the Dielectric properties of body tissues at RF and microwave frequencies," U.S. Air Force Armstrong Laboratory, Report AL/OE-TR-1996-0037, Brooks Air Force Base, Texas, 78235, June 1996.
14. G. Hartsgrave, A. Kraszewski and A. Surowiec, "Simulated biological materials for electromagnetic absorption studies," *Bioelectromagnetics*, Vol. 8, pp. 29-36, 1987.
15. H. I. Bassen and G. S. Smith, "Electric field probes — a review," *IEEE Trans. Antennas Propagat.*, Vol. 3, pp710-718, Sept., 1983.
16. D. Hill, "Waveguide techniques for the calibration of miniature electric field probes for use in microwave bioeffects studies," *IEEE Trans. Theory Tech.*, Vol. 30, pp. 92-94, 1982.
17. N. Kuster and Q. Balzano, "Energy absorption mechanism by biological bodies in the near field of dipole antennas above 300 MHz," *IEEE Trans. Veh. Technol.*, Vol. 41, pp. 17-23, 1992.
18. M. A. Stuchly, S. S. Stuchly, and A. Kraszewski, "Implantable electric field probes — some performance characteristics," *IEEE Trans. Biomed. Eng.*, Vol. 31, pp. 526-531, 1984.
19. A. Taflove, K. R. Umashankar, T. G. Jurgens, "Validation of FDTD modeling of the radar cross section of three-dimensional structures spanning up to nine wavelengths," *IEEE Trans. Antennas and Propagat.*, pp. 662-666, 1985.
20. C. M. Furse, Q. Yu and O. P. Gandhi, "Validation of the Finite-Difference Time-Domain method for near-field bioelectromagnetic simulations," *Microwave and Optical Technology Letters*, Vol. 16, pp.341-345, 1997.

Figure Captions

Figure 1: Block diagram of the experimental setup of the automated SAR measurement system.

Figure 2: Phantom model used in the automated SAR measurement system.

Figure 3a: Test for square-law behavior at 840 MHz: Variation of the output voltage (proportional to $|E_i|^2$) for different radiated powers normalized to 0.1 W.

Figure 3b: Test for square-law behavior at 1900 MHz: Variation of the output voltage (proportional to $|E_i|^2$) for different radiated powers normalized to 0.1 W.

Figure 4a: Test for isotropy: The model shown in Figure 2 was used with nominal half wavelength dipole radiator of length 178 mm at 840 MHz.

Figure 4b: Test for isotropy: The model shown in Figure 2 was used with nominal half wavelength dipole radiator of length 77 mm at 1900 MHz.

Figure 5a: Comparison of the calculated and measured SAR variations for a box phantom of dimensions 30 x 15 x 50 cm; 840 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 840 MHz = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

Figure 5b: Comparison of the calculated and measured SAR variations for a box phantom of dimensions 30 x 15 x 50 cm for a line AB parallel to the z axis at a distance $y = 7$ mm from the surface of the phantom material; 840 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 840 MHz = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

Figure 6a: Comparison of the calculated and measured SAR variations for a box phantom of dimensions 30 x 15 x 50 cm; 1900 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 1900 MHz = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.

Figure 6b: Comparison of the calculated and measured SAR variations for a box phantom of dimensions 30 x 15 x 50 cm for a line AB parallel to the z axis at a distance $y = 7$ mm from the surface of the phantom material; 1900 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 1900 MHz = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.

Figure 7a: Comparison of measured and FDTD-calculated SAR variations at 840 MHz for a glass sphere model of outer diameter 22.3 cm and thickness 5 mm. SARs normalized to a radiated power of 0.5 W. Calibration factor = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

Figure 7b: Comparison of calculated and measured SAR variations at 840 MHz for a plane at a distance of 20 mm from the lowest point on the inside of the sphere. SARs normalized to a radiated power of 0.5 W. Calibration factor = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

Figure 8a: Comparison of measured and FDTD-calculated SAR variations at 1900 MHz for a glass sphere model of outer diameter 22.3 cm and thickness 5 mm. SARs normalized to a radiated power of 0.5 W. Calibration factor = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.

Figure 8b: Comparison of calculated and measured SAR variations at 1900 MHz for a plane at a distance of 20 mm from the lowest point on the inside of the sphere. SARs normalized to a radiated power of 0.5 W. Calibration factor = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.

Table Captions

Table 1: The desired tissue properties and the measured electrical properties of the tissue-simulant materials for the phantom model.

Table 2: Composition used for brain equivalent materials.

Table 3: Long term stability of the phantom material at 1900 MHz.

Table 4: Box phantom: Comparison of the measured and FDTD-calculated peak 1-g SARs for four spacings each at 840 and 1900 MHz, radiated power normalized to 0.5 W.

Table 5: Sphere phantom: Comparison of the measured and FDTD-calculated peak 1-g SARs for three spacings each at 840 and 1900 MHz, radiated power normalized to 0.5 W.

Table 6: Comparison of the experimentally measured and FDTD-calculated peak 1-g SARs for ten commercial wireless devices, five each at 835 and 1900 MHz, respectively.

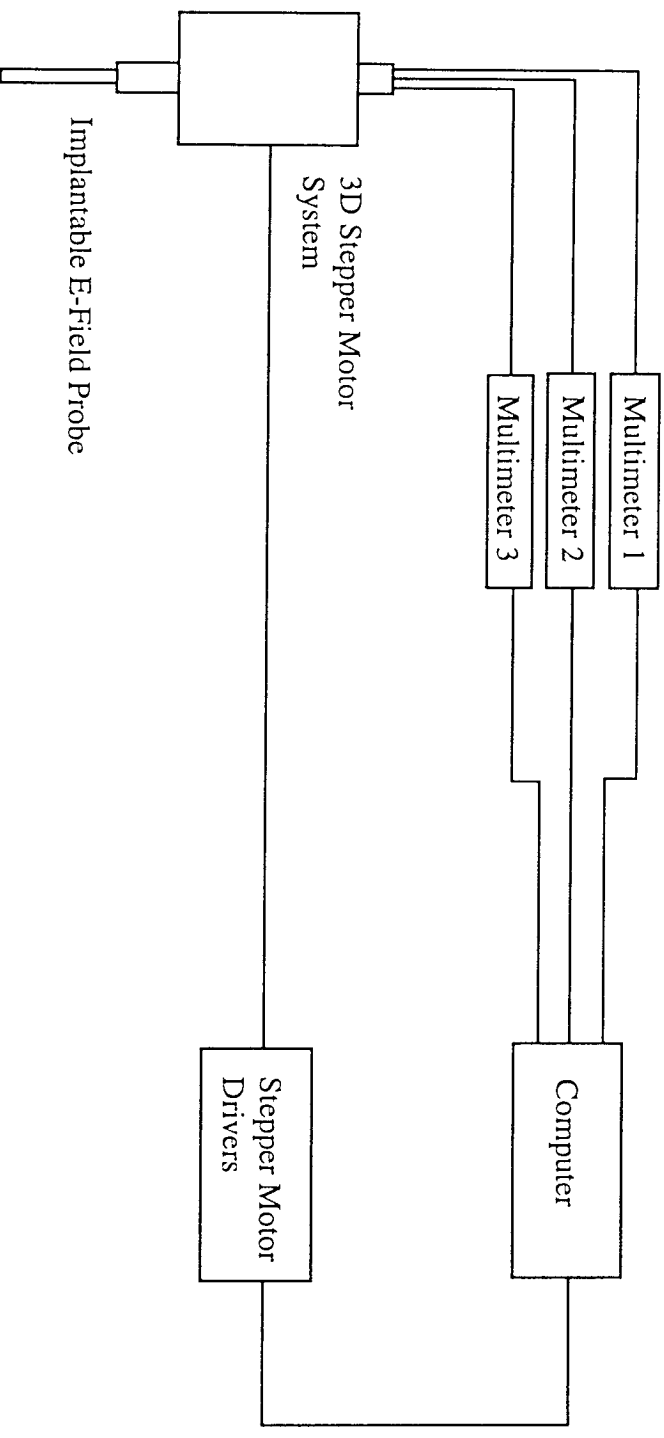


Figure 1 Block diagram of the experimental setup of the automated SAR measurement system

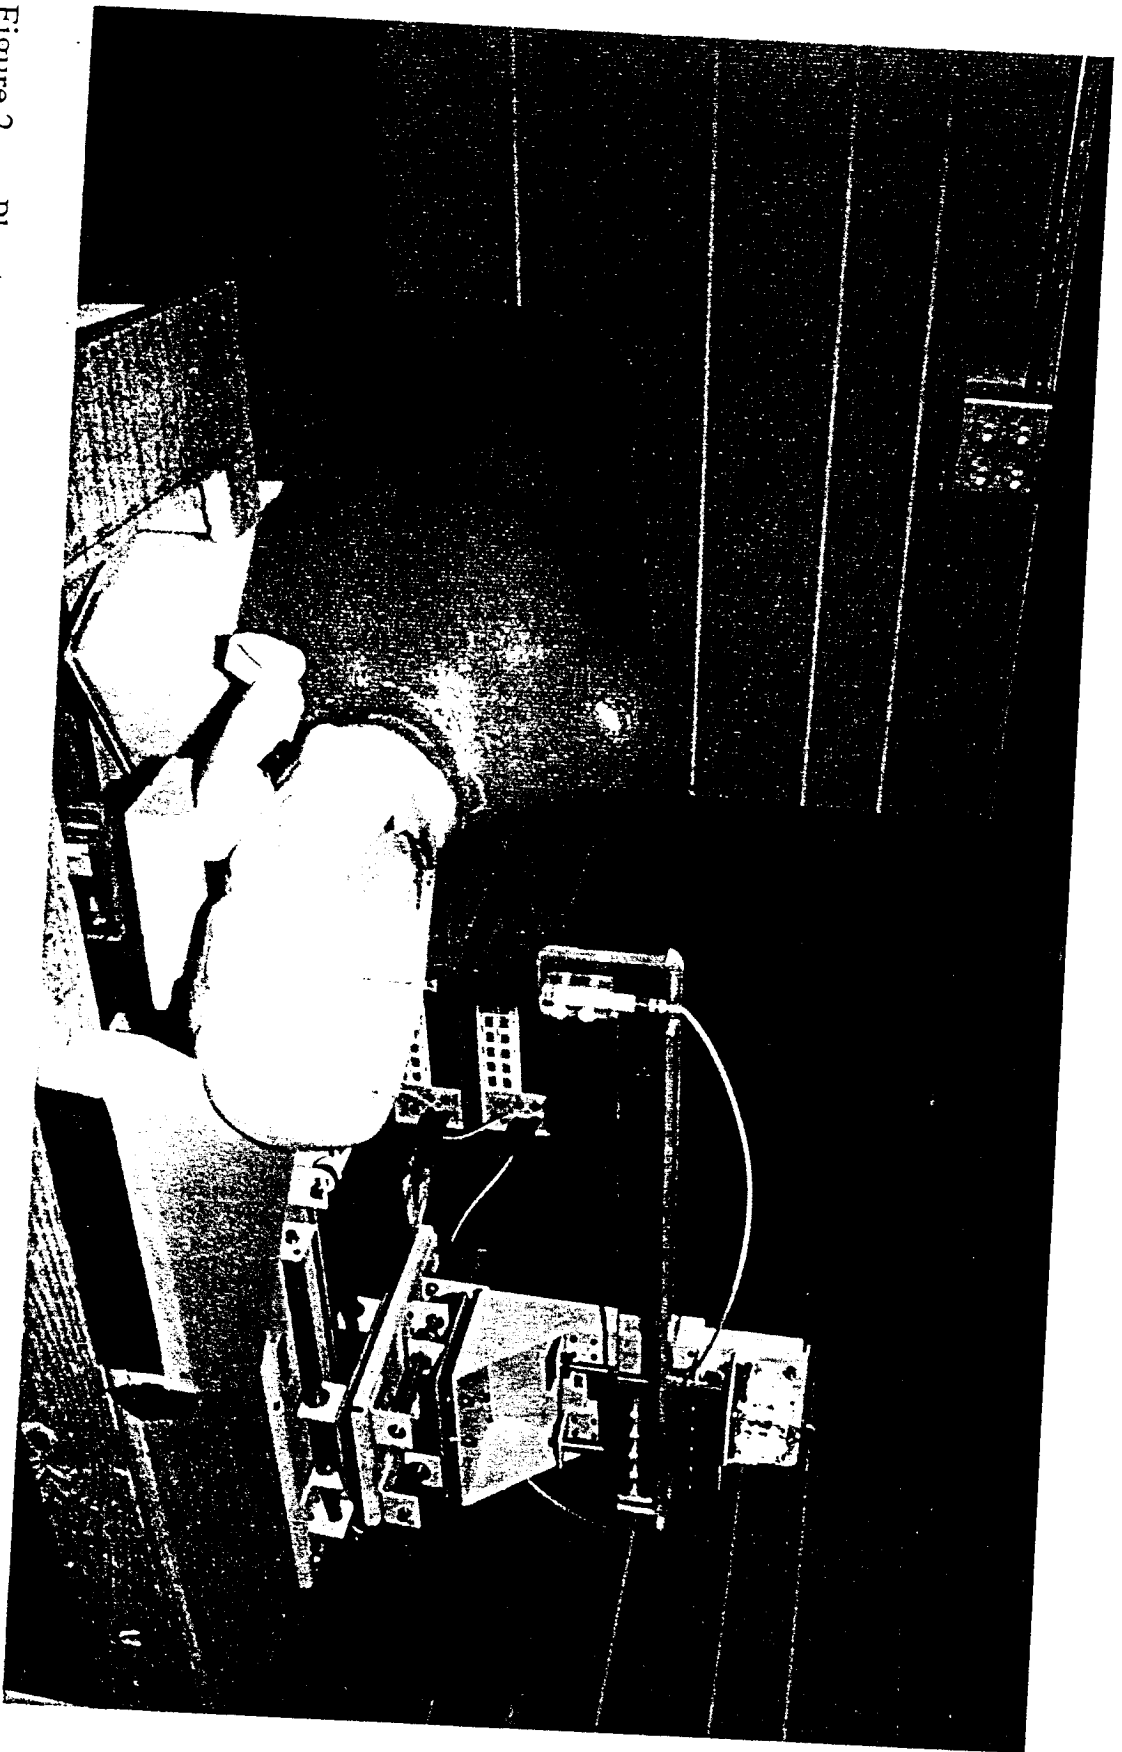


Figure 2 Phantom model used in the automated SAR measurement system.

Table 1 The desired tissue properties and the measured electrical properties of the tissue-simulant materials used for the phantom model.

	Desired*		Measured	
	ϵ_r	σ (S/m)	ϵ_r	σ (S/m)
	840 MHz			
Brain	45.3	0.92	41.1 ± 1.4	1.06 ± 0.05
Skull	17.4	0.25	7.4	0.16
	1900 MHz			
Brain	43.2	1.29	45.5 ± 1.7	1.31 ± 0.06
Skull	16.4	0.45	7.4	0.34

*From C. Gabriel [13]

Table 2 Compositions used for brain-equivalent materials

840 MHz		1900 MHz	
Water	40.4%	Water	60.0%
Sugar	56.0%	Sugar	18.0%
Salt (NaCl)	2.5%	PEP	20.0%
HEC	1.0%	Salt (NaCl)	0.4%
		TX 151	1.6%
$\epsilon_r = 41.1 \pm 1.4$		$\epsilon_r = 45.5 \pm 1.7$	
$\sigma = 1.06 \pm 0.05$ S/m		$\sigma = 1.31 \pm 0.06$ S/m	

Table 3 Long Term Stability of the phantom material at 1900 MHz

Day	ϵ_r	σ (S/m)
1	46.2 ± 1.1	1.35 ± 0.03
7	44.9 ± 1.7	1.29 ± 0.06
15	44.2 ± 1.8	1.25 ± 0.05

Table 4 Box phantom: Comparison of the measured and FDTD-calculated peak 1-g SARs for four spacings each at 840 and 1900 MHz, radiated power normalized to 0.5 W.

Frequency (MHz)	Distance (mm) between $\lambda/2$ dipole and the Box	SAR (W/kg) Measured	SAR (W/kg) FDTD	Difference (%)
840	17.5	4.58	4.20	+8.3
840	22.5	3.53	3.65	-3.4
840	27.5	2.69	3.00	-10.2
840	33.0	1.95	2.24	-12.9
1900	16.5	7.45	7.46	-0.1
1900	21.5	4.24	4.18	+1.4
1900	26.5	2.71	2.91	-7.9
1900	31.5	1.77	1.75	+1.1

Table 5 Sphere phantom: Comparison of the measured and FDTD-calculated peak 1-g SARs for three spacings each at 840 and 1900 MHz, radiated power normalized to 0.5 W.

Frequency (MHz)	Distance (mm) between $\lambda/2$ dipole and the Box	SAR (W/kg) Measured	FDTD	Difference (%)
840	5	6.78	6.77	+0.23
840	15	3.41	3.27	+4.22
840	25	1.85	1.68	+9.51
1900	5	17.45	18.01	-3.21
1900	15	4.96	5.05	-1.81
1900	25	1.69	1.77	-4.73

Table 6. Comparison of the experimentally measured and FDTD-calculated peak 1-g SARs for ten commercial wireless devices, five each at 835 and 1900 MHz, respectively.

	Time-Averaged Radiated Power mW	Experimental Method W/kg	Numerical Method W/kg
Cellular Telephones at 835 MHz			
Telephone A	600	4.02	3.90
Telephone B	600	5.41	4.55
Telephone C	600	4.48	3.52
Telephone D	600	3.21	2.80
Telephone E	600	0.54	0.53
PCS Telephones at 1900 MHz			
Telephone A	125	1.48	1.47
Telephone B	125	0.13	0.15
Telephone C	125	0.65	0.81
Telephone D	125	1.32	1.56
Telephone E	99.3	1.41	1.25

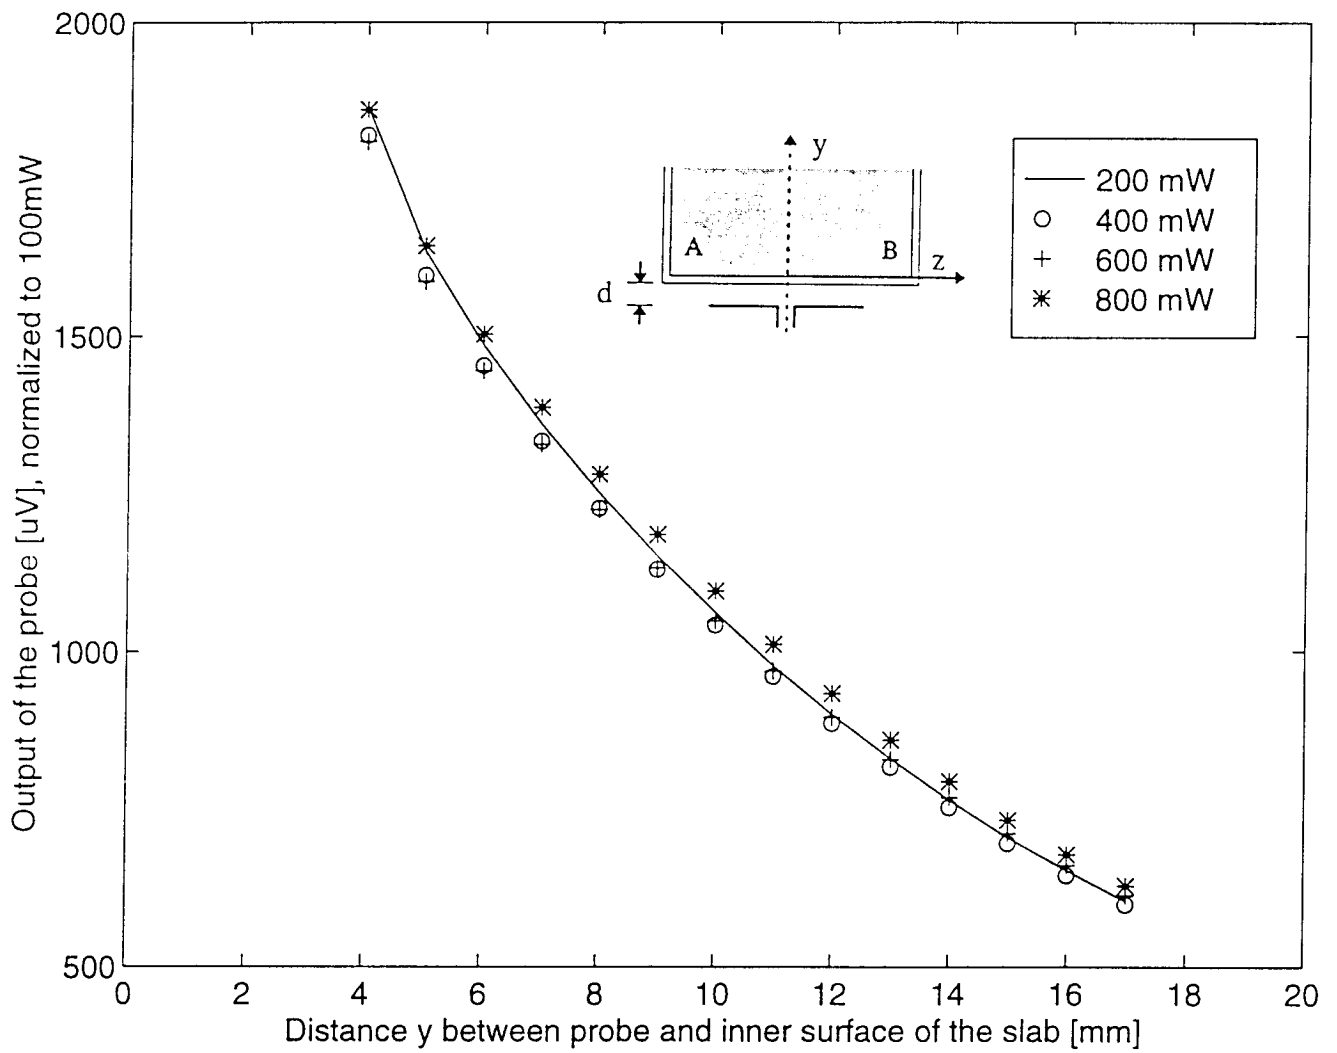


Figure 3a: Test for square-law behavior at 840 MHz: Variation of the output voltage (proportional to $|E_i|^2$) for different radiated powers normalized to 0.1 W.

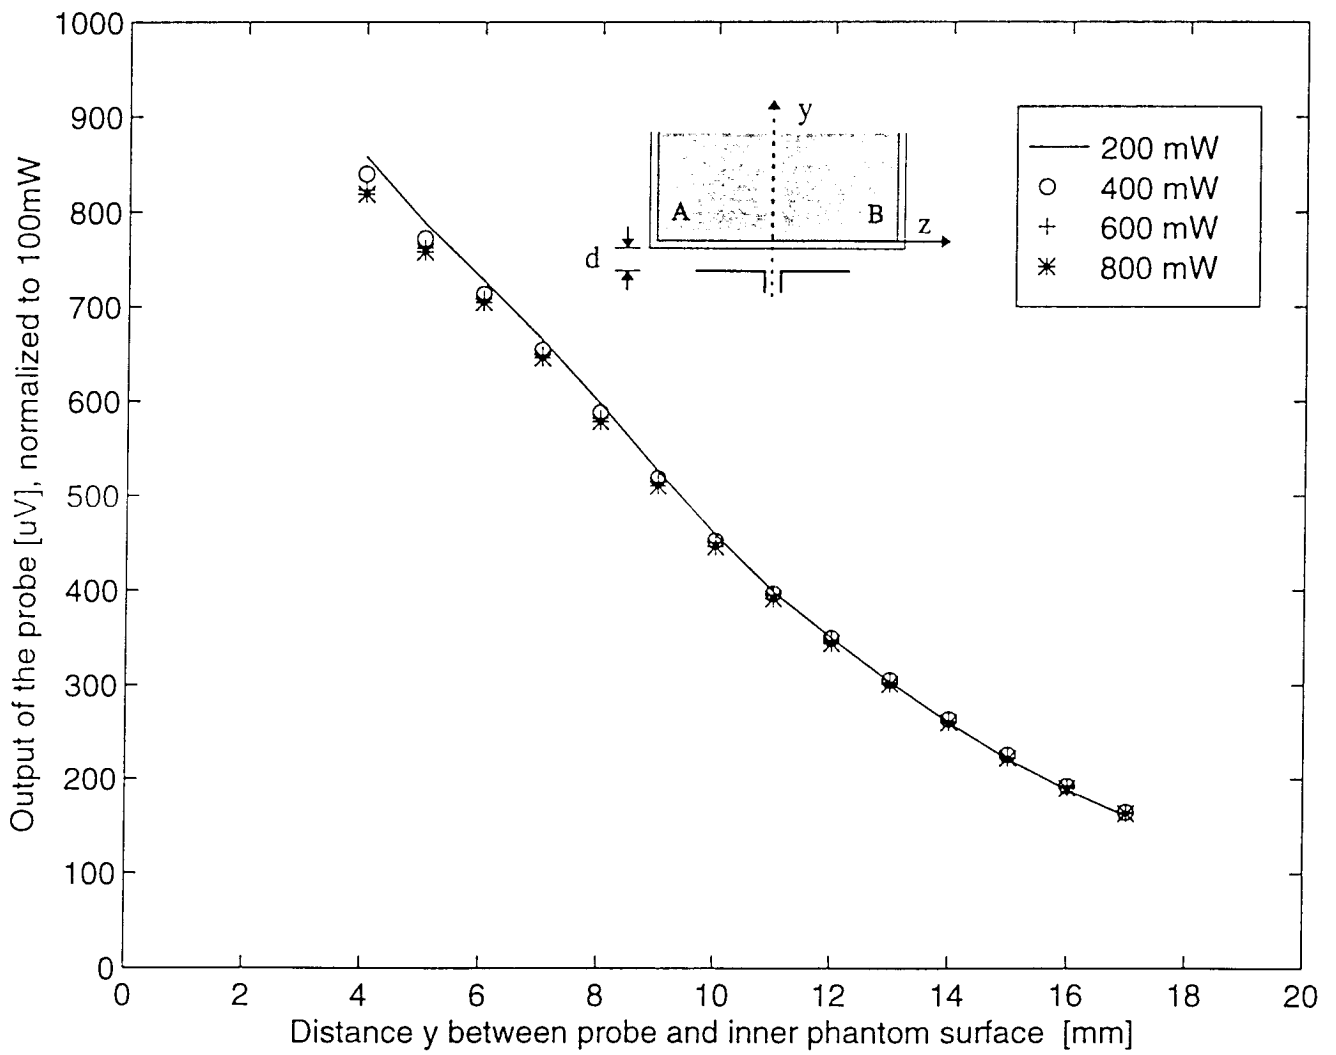


Figure 3b: Test for square-law behavior at 1900 MHz: Variation of the output voltage (proportional to $|E_i|^2$) for different radiated powers normalized to 0.1 W.

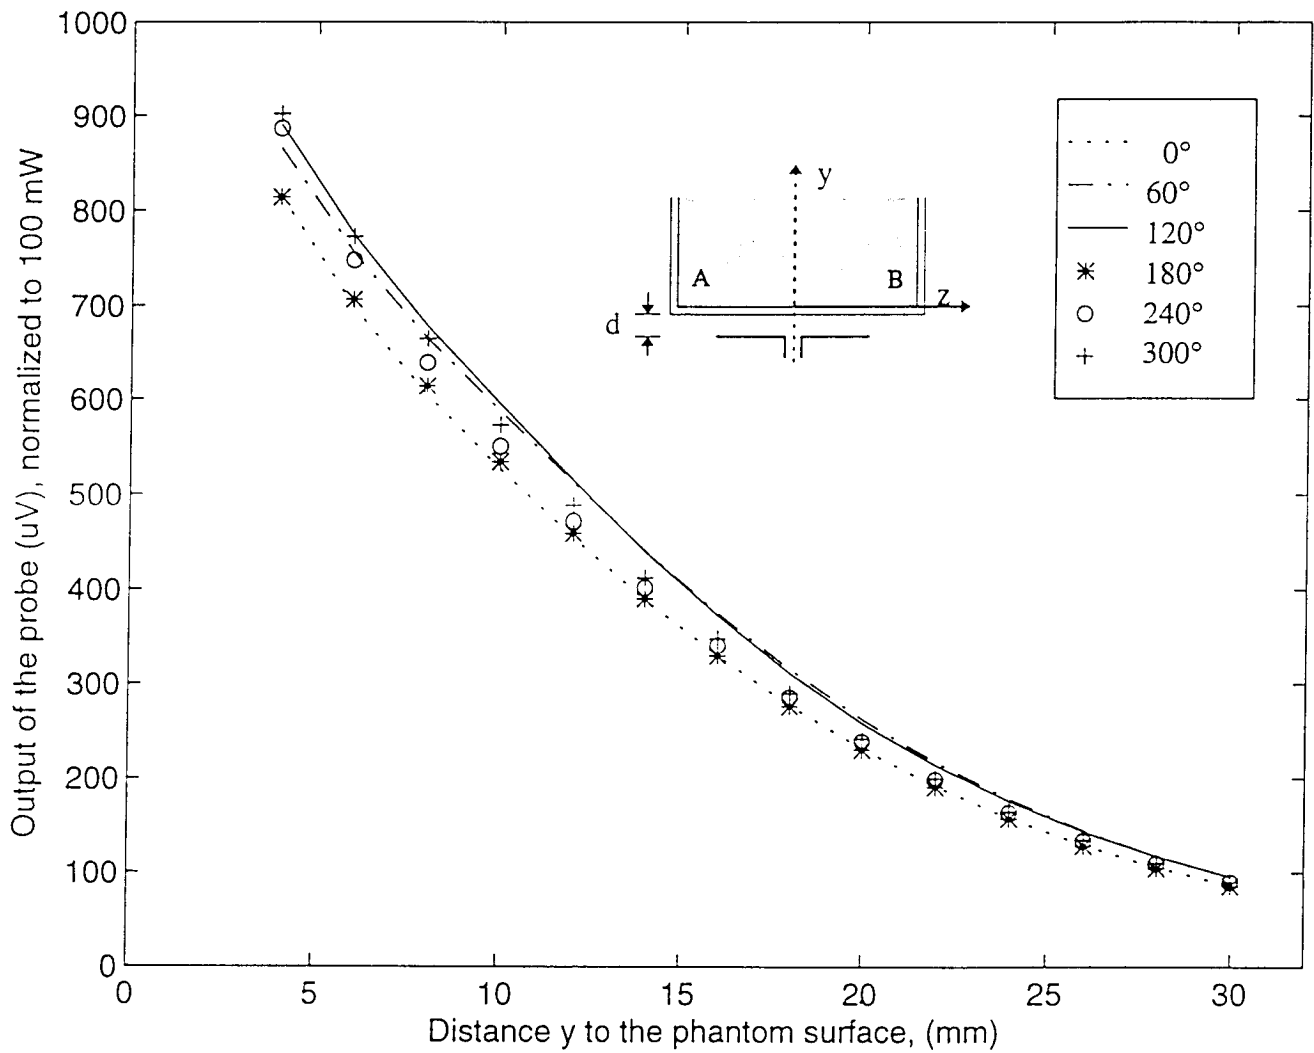


Figure 4a: Test for isotropy: The model shown in Figure 2 was used with nominal half wavelength dipole radiator of length 178 mm at 840 MHz.

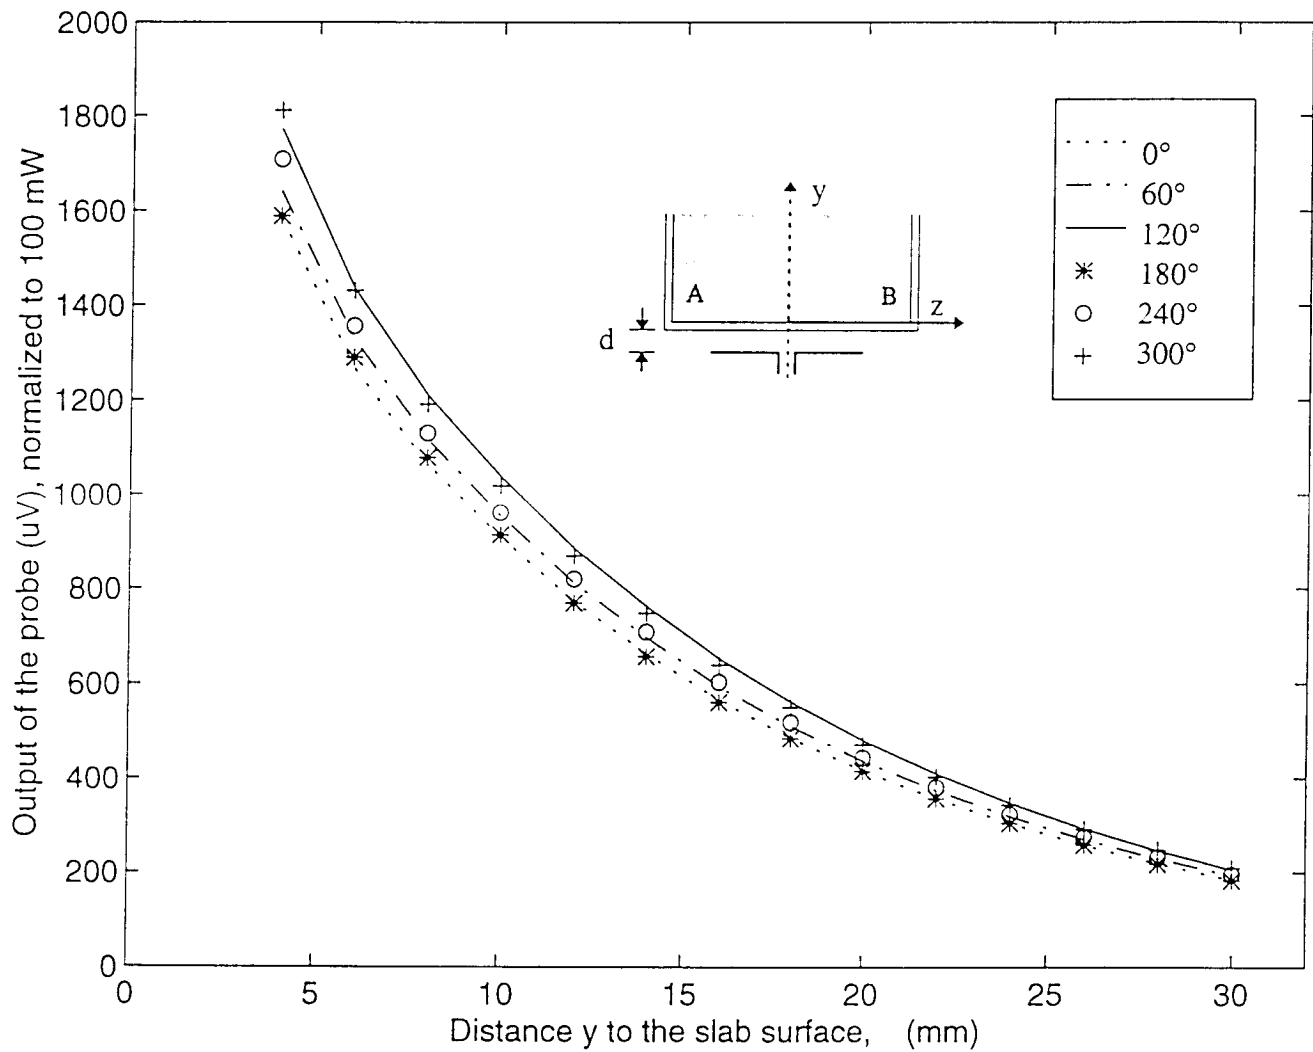


Figure 4b: Test for isotropy: The model shown in Figure 2 was used with nominal half wavelength dipole radiator of length 77 mm at 1900 MHz.

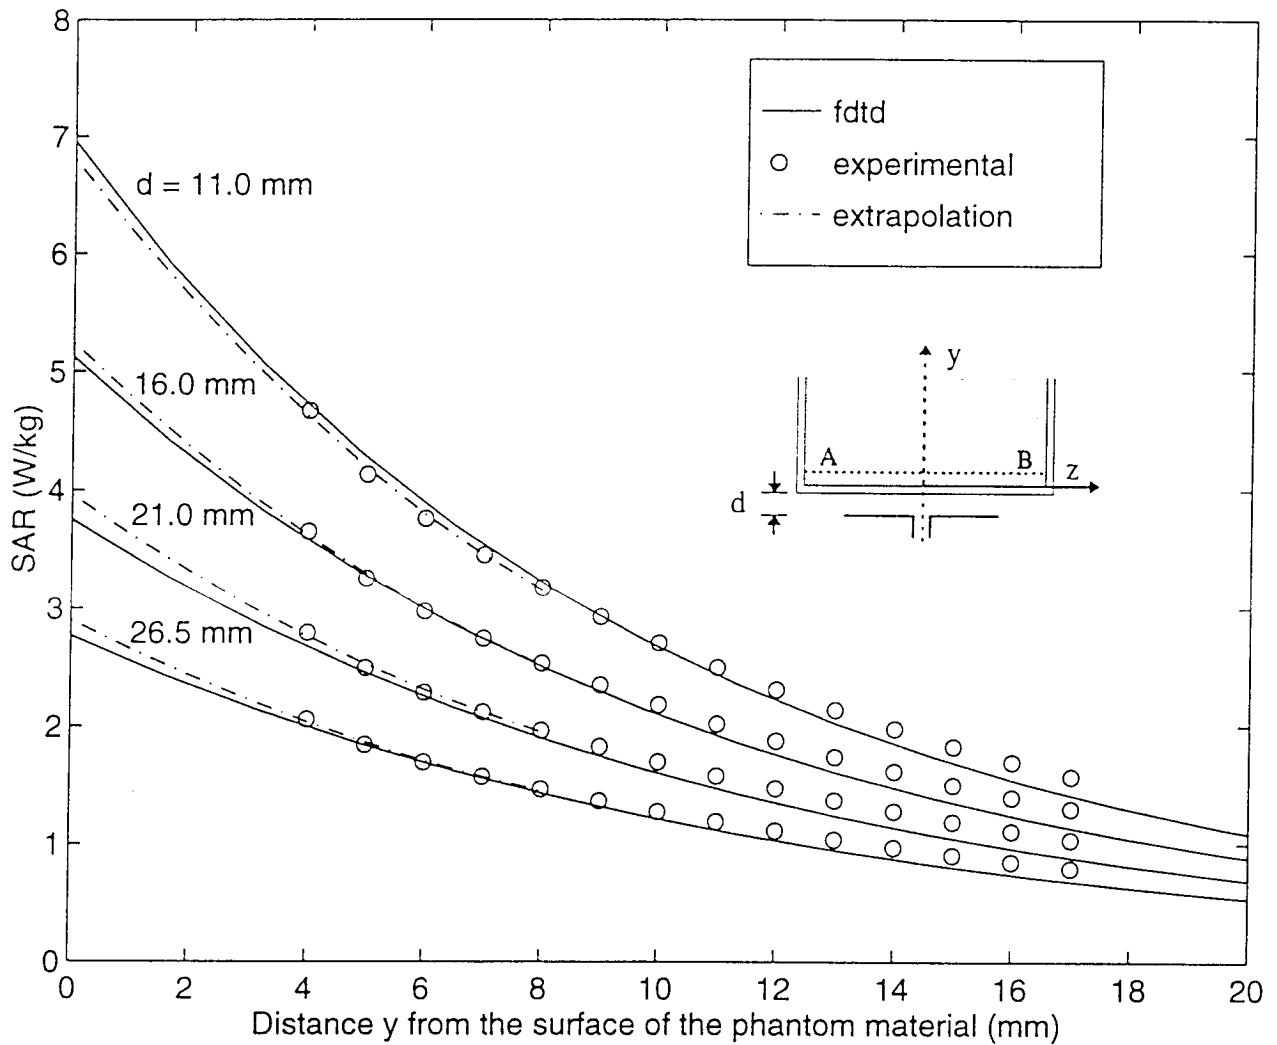


Figure 5a: Comparison of the calculated and measured SAR variations for a box phantom of dimensions 30 x 15 x 50 cm; 840 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 840 MHz = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

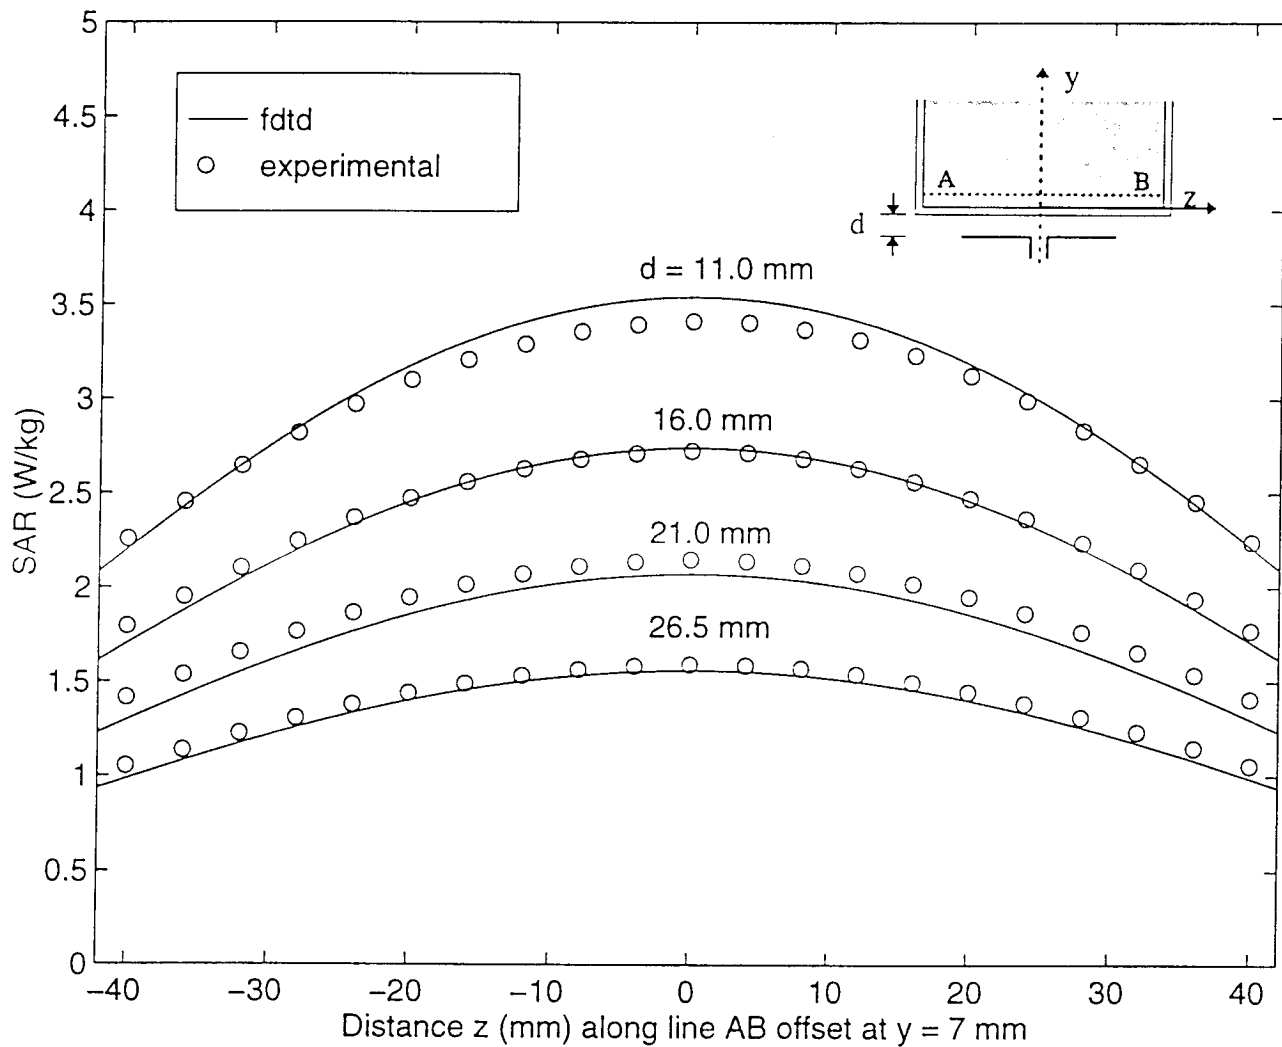


Figure 5b: Comparison of the calculated and measured SAR variations for a box phantom of dimensions 30 x 15 x 50 cm for a line AB parallel to the z axis at a distance $y = 7$ mm from the surface of the phantom material; 840 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 840 MHz = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

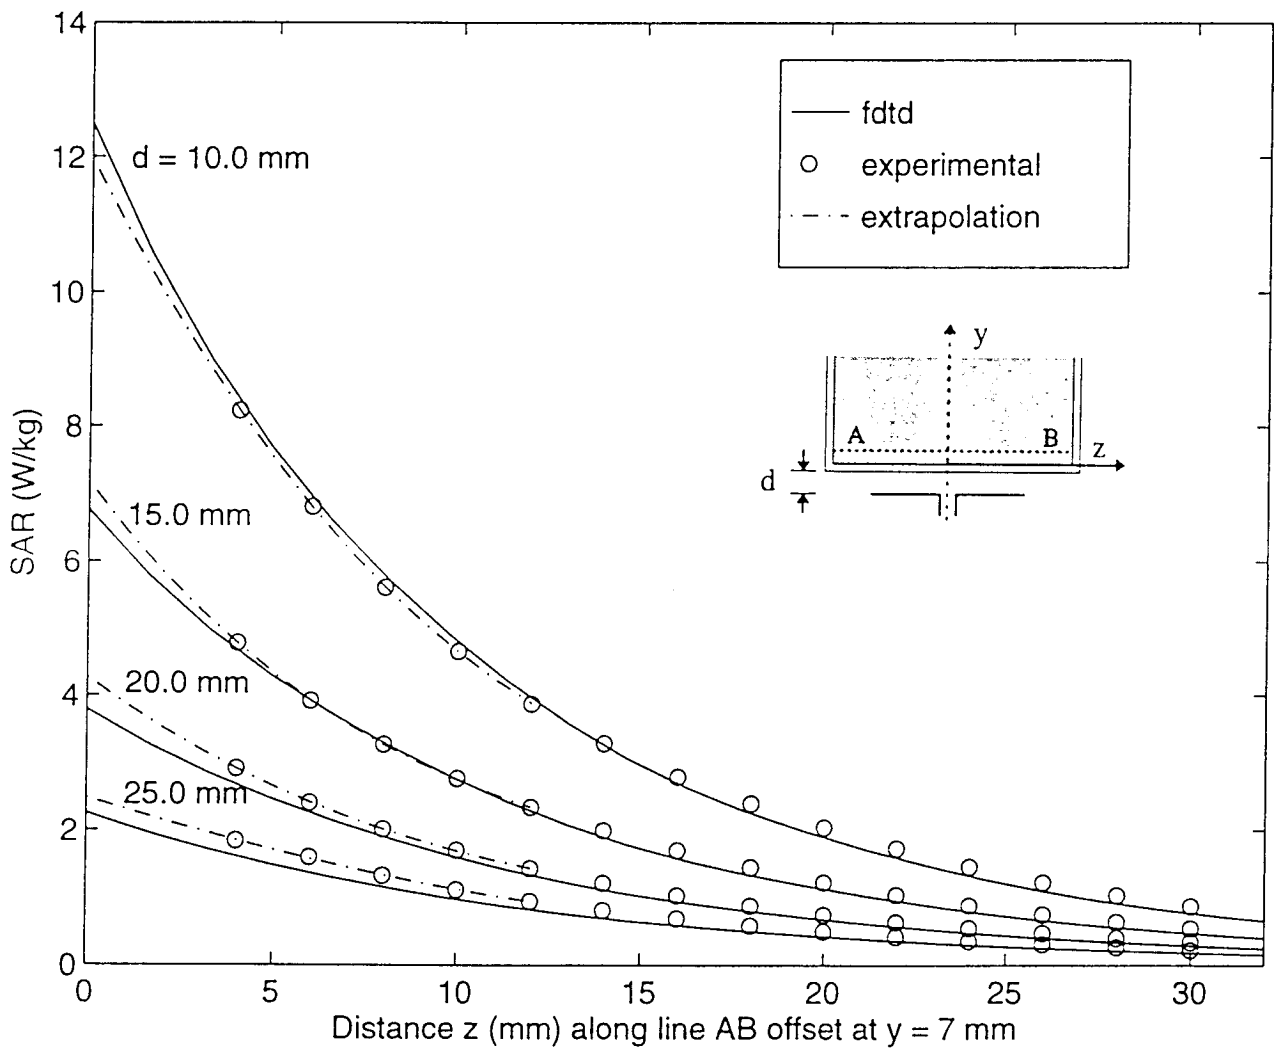


Figure 6a: Comparison of the calculated and measured SAR variations for a box phantom of dimensions 30 x 15 x 50 cm; 1900 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 1900 MHz = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.

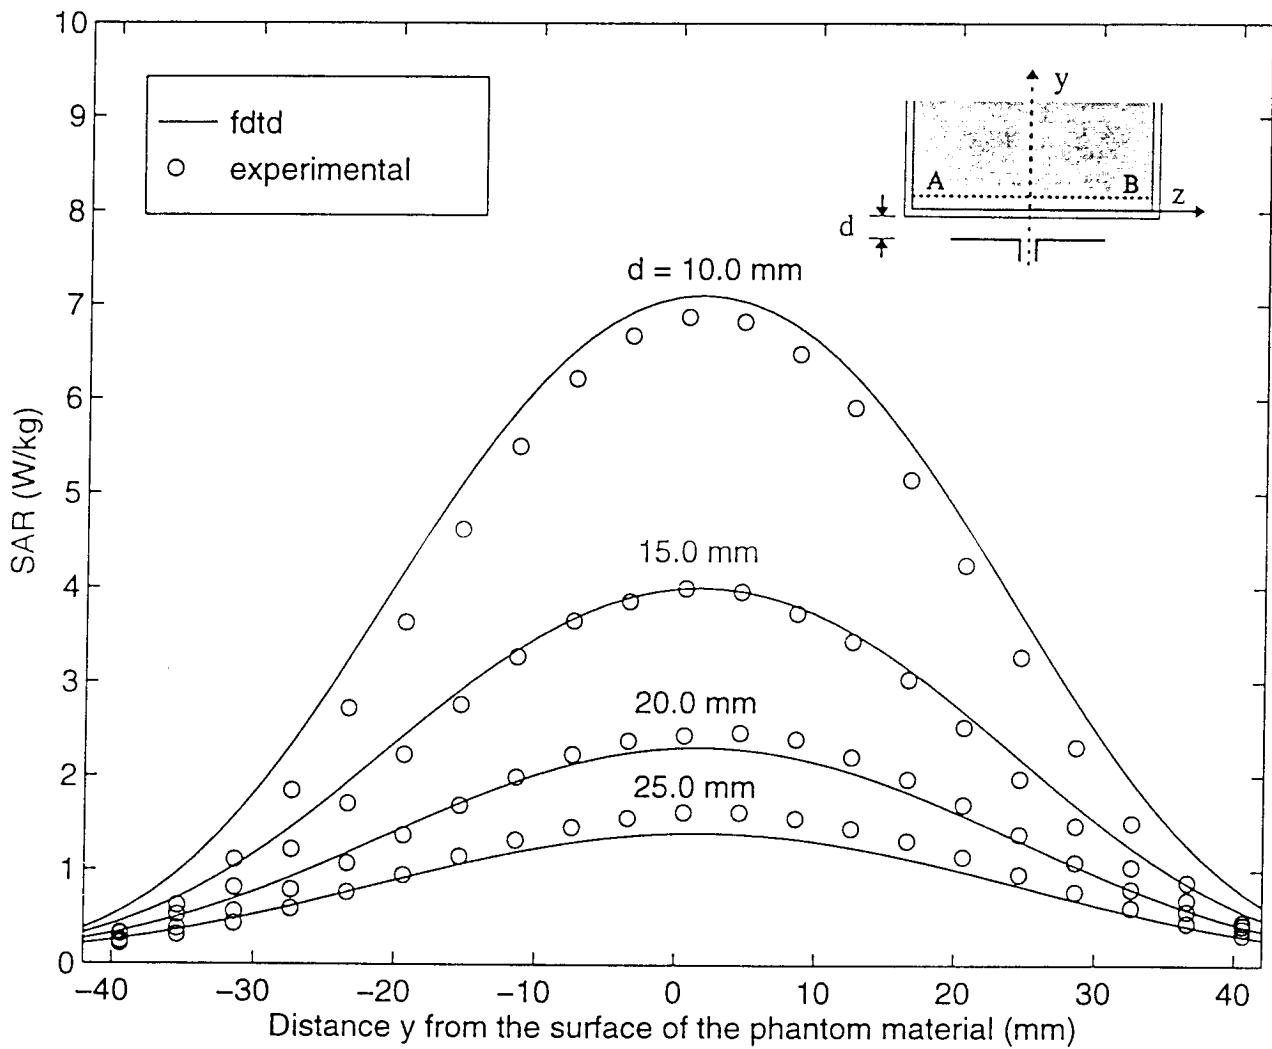


Figure 6b: Comparison of the calculated and measured SAR variations for a box phantom of dimensions 30 x 15 x 50 cm for a line AB parallel to the z axis at a distance $y = 7$ mm from the surface of the phantom material; 1900 MHz; $\lambda/2$ dipole antenna; 0.5 W radiated power. Calibration factor for the Narda Model 8021 probe at 1900 MHz = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.

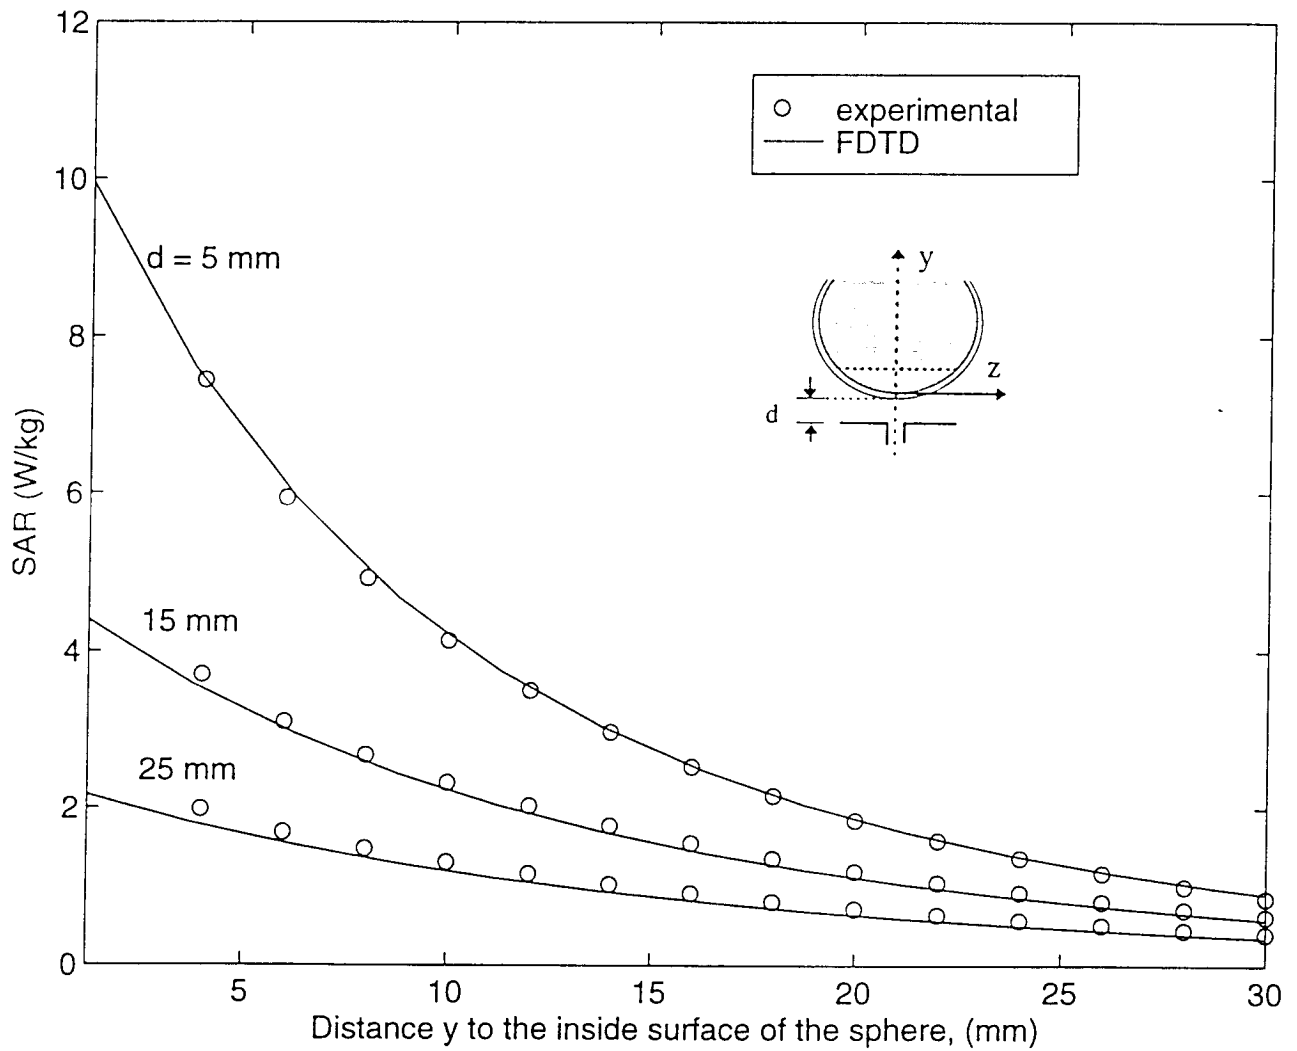


Figure 7a: Comparison of measured and FDTD-calculated SAR variations at 840 MHz for a glass sphere model of outer diameter 22.3 cm and thickness 5 mm. SARs normalized to a radiated power of 0.5 W. Calibration factor = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

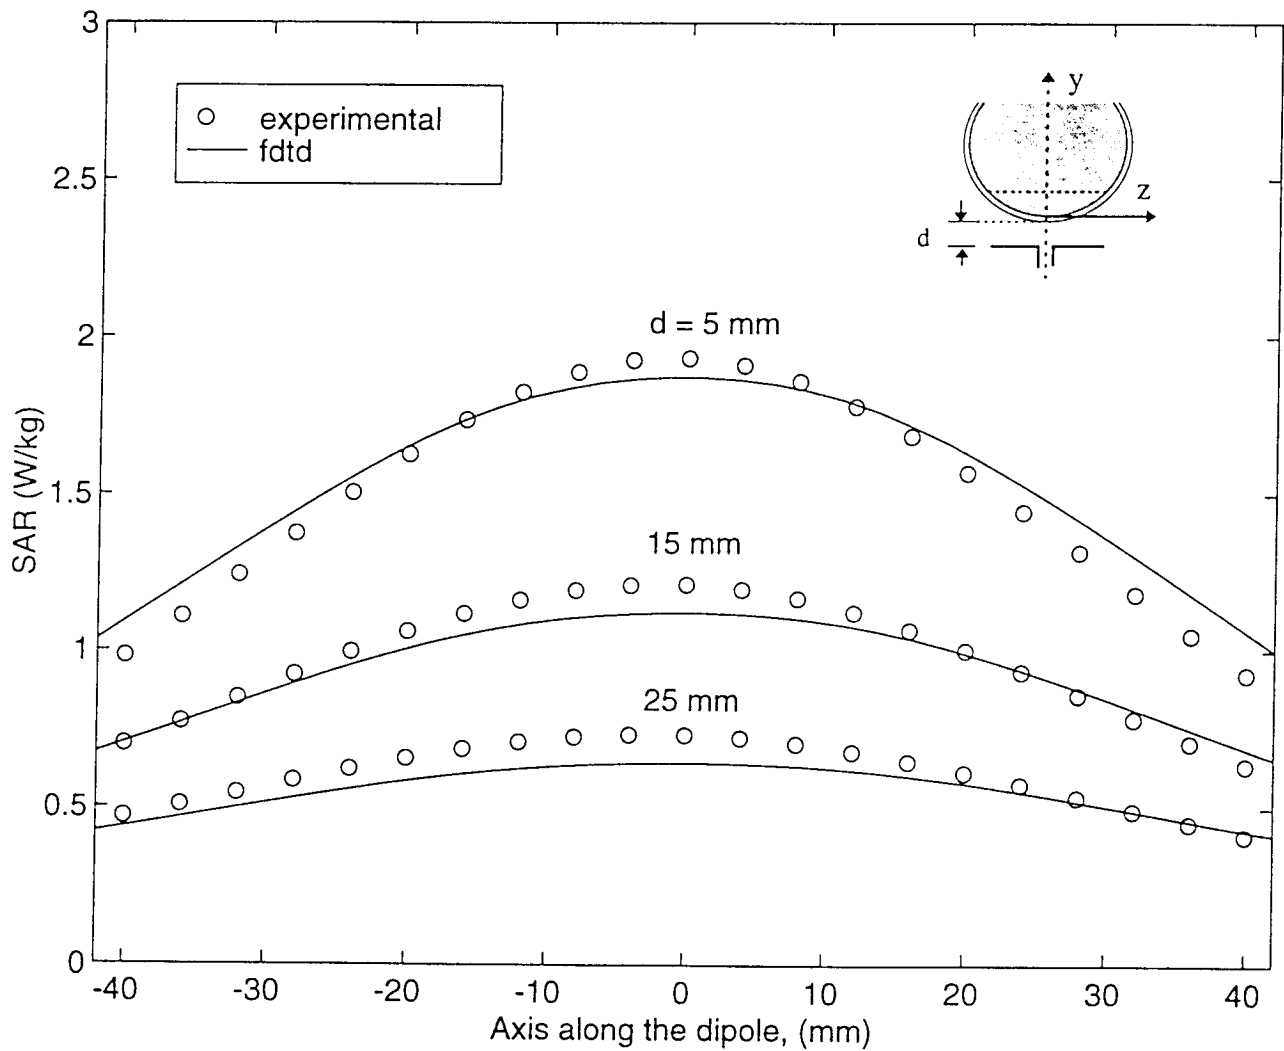


Figure 7b: Comparison of calculated and measured SAR variations at 840 MHz for a plane at a distance of 20 mm from the lowest point on the inside of the sphere. SARs normalized to a radiated power of 0.5 W. Calibration factor = 0.49 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 41.1$, $\sigma = 1.06$ S/m.

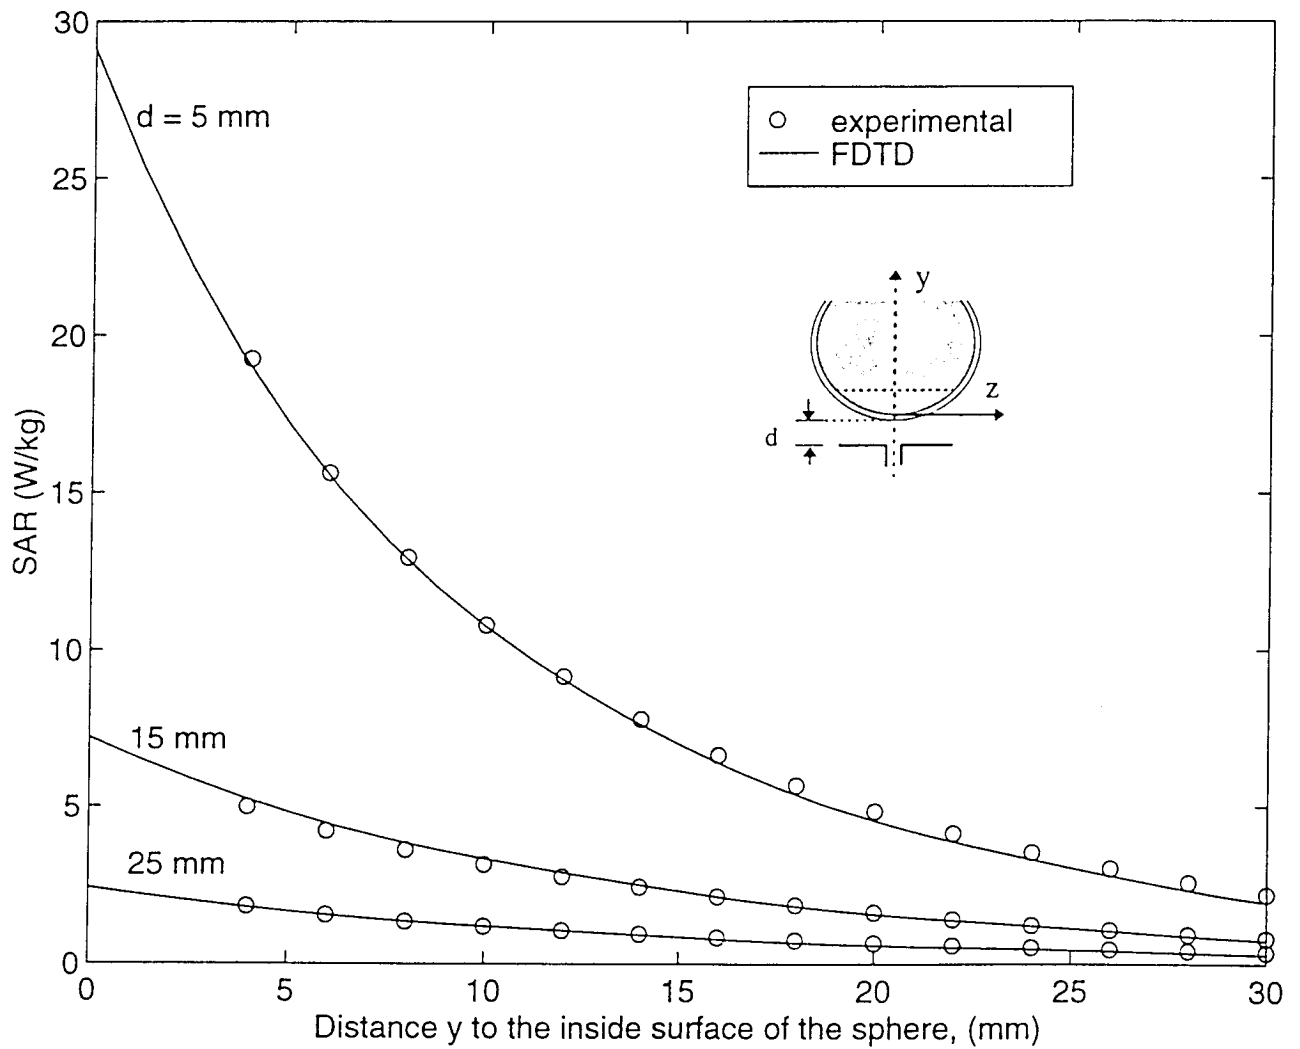


Figure 8a: Comparison of measured and FDTD-calculated SAR variations at 1900 MHz for a glass sphere model of outer diameter 22.3 cm and thickness 5 mm. SARs normalized to a radiated power of 0.5 W. Calibration factor = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.

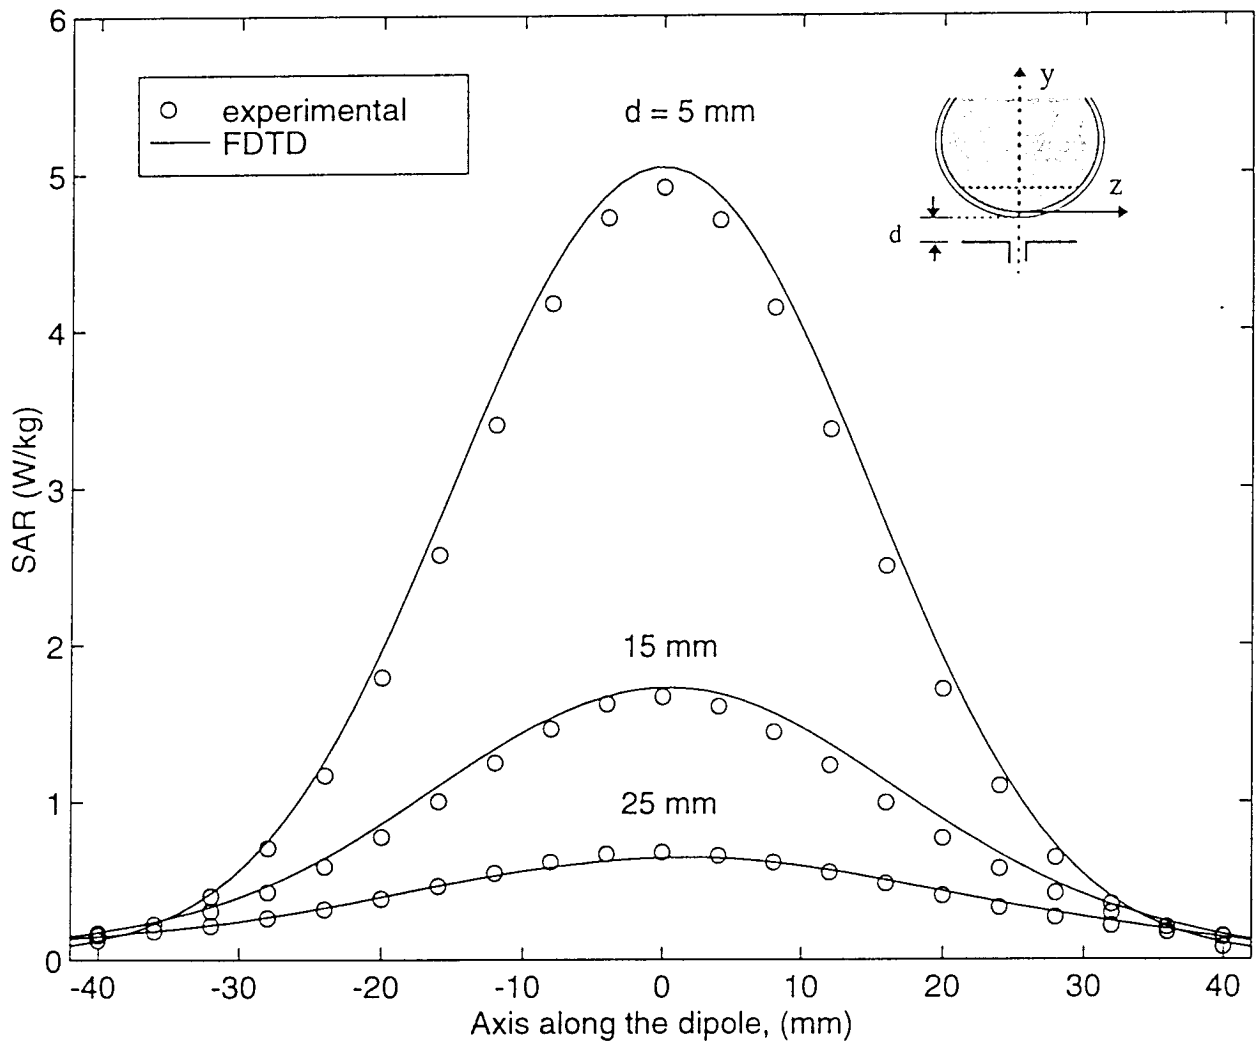


Figure 8b: Comparison of calculated and measured SAR variations at 1900 MHz for a plane at a distance of 20 mm from the lowest point on the inside of the sphere. SARs normalized to a radiated power of 0.5 W. Calibration factor = 0.84 (mW/kg)/ μ V. Measured for the phantom material $\epsilon_r = 45.5$, $\sigma = 1.31$ S/m.