
Testing Services™	Appendix for the BlackBerry SAR Report	® Smartphone Model R	CK71CW	Page 1(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

APPENDIX D: PROBE & DIPOLE CALIBRATION DATA

	ates of Test uly 23-August 12	2,2009 RTS -	•1765-0907-30	FCC ID: L6ARCK70CW
Calibration Labor Schmid & Partner Engineering AG Zeughausstrasse 43, 8004	ANNUE 12 12 12		C Service suiss	ner Kalibrierdienst e d'étalonnage ero di taratura tion Service
	reditation Service (SAS) ervice is one of the signatori the recognition of calibration	es to the EA	Accreditation No.: SCS 10	8
	festing Services)		Certificate No: ET3-1642	_Jan09
CALIBRATIO	N CERTIFICAT	E		
Object	ET3DV6 - SN:1	642		
Calibration procedure(s)	a company of the second s	and QA CAL-23.v3 edure for dosimetric E-fit	eld probes	
Calibration date:	January 12, 200	9		
Condition of the calibrated i	tem In Tolerance			
The measurements and the All calibrations have been of Calibration Equipment used	uncertainties with confidence	tional standards, which realize the probability are given on the follow ory facility: environment temperate	ing pages and are part of the o ure (22 ± 3)°C and humidity < 1	rentificate.
The measurements and the All calibrations have been of	uncertainties with confidence conducted in the closed laborat	probability are given on the follow	ing pages and are part of the o ure (22 ± 3)°C and humidity < 1	vertificate.
The measurements and the All calibrations have been of Calibration Equipment used Primary Standards Power meter E44198 Power sensor E4412A	Incertainties with confidence conducted in the closed laborat (M&TE critical for calibration) ID # GB41293874 MY41495277	probability are given on the follow ory facility: environment temperatu Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788)	ing pages and are part of the o ure (22 ± 3)°C and humidity < 1 Schedule Apr-09 Apr-09 Apr-09	rentificate.
The measurements and the All calibrations have been of Calibration Equipment used Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A	I uncertainties with confidence conducted in the closed laborat (M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788)	ing pages and are part of the o ure (22 ± 3)°C and humidity < Schedule Apr-09 Apr-09 Apr-09	rentificate.
The measurements and the All calibrations have been of Calibration Equipment used Primary Standards Power meter E44198 Power sensor E4412A	Incertainties with confidence conducted in the closed laborat (M&TE critical for calibration) ID # GB41293874 MY41495277 MY41496087 SN: S5054 (3c)	probability are given on the follow ory facility: environment temperatu Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788)	ing pages and are part of the o ure (22 ± 3)°C and humidity < 1 Schedule Apr-09 Apr-09 Apr-09	rentificate.
The measurements and the All calibrations have been of Calibration Equipment used Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuato Reference 30 dB Attenuato	ID uncertainties with confidence conducted in the closed laborat (M&TE critical for calibration) ID # GB41293874 MY41495277 MY41496087 SN: S5054 (3c) r SN: S5058 (2b) r SN: S5129 (30b)	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00787) 1-Jul-08 (No. 217-00866)	ing pages and are part of the of ure (22 ± 3)°C and humidity < 1 Schedule Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09	rentificate.
The measurements and the All calibrations have been of Calibration Equipment used Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	Incertainties with confidence conducted in the closed laborat (M&TE critical for calibration) ID # GB41293874 MY41495277 MY41496087 SN: S5054 (3c) r SN: S5086 (20b)	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-09 (No. ES3-3013_Jan	ing pages and are part of the of ure (22 ± 3)*C and humidity < 1 Schedule Apr-09 Apr-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09 Jul-09	rentificate.
The measurements and the All calibrations have been of Calibration Equipment used Primary Standards Power metar E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuato Reference 20 dB Attenuato Reference Probe ES3DV2 DAE4	uncertainties with confidence conducted in the closed laborat (M&TE critical for calibration) ID # GB41293874 MY41495087 MY41496087 SN: \$5054 (3c) SN: \$50586 (20b) SN: \$5129 (30b) SN: 3013 SN: 660	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00786) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00866) 2-Jan-09 (No. ES3-3013_Jan 9-Sep-08 (No. DAE4-660_Se	ing pages and are part of the o ure (22 ± 3)°C and humidity < 1 Schedule Apr-09 Apr-09 Jul-09 Apr-09 Jul-09 09) Jan-10 p08) Sep-09	ertificate. 10%. d Calibration
The measurements and the All calibrations have been of Calibration Equipment used Primary Standards Power sensor E44128 Power sensor E4412A Reference 3 dB Attenuato Reference 30 dB Attenuato Reference 20 dB Attenuato	uncertainties with confidence conducted in the closed laborat (M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) r SN: S5054 (3c) r SN: S5058 (20b) r SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-09 (No. ES3-3013_Jan	ing pages and are part of the of ure (22 ± 3)*C and humidity < 1 Schedule Apr-09 Apr-09 Apr-09 Jul-09 09) Jan-10 p08) Sep-09 Schedule t-07) In house	ertificate. 10%. d Calibration
The measurements and the All calibrations have been of Calibration Equipment used Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuato Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	uncertainties with confidence conducted in the closed laborat (M&TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) r SN: S5054 (3c) r SN: S5058 (20b) r SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 1-Jul-08 (No. 217-00788) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00787) 2-Jan-09 (No. ES3-3013_Jan 9-Sep-08 (No. DAE4-660_Se Check Date (in house) 4-Aug-99 (in house check Oc	ing pages and are part of the of ure (22 ± 3)°C and humidity < 1 Schedule Apr-09 Apr-09 Jul-09 Apr-09 Jul-09 Schedule (-07) Schedule (-07) Schedule (-07) Schedule (-07) Schedule (-07) Schedule (-07) Schedule (-07) Schedule (-07) Schedule (-07) Schedule (-08) Schedule (-08) Schedule	d Check check: Oct-09 check: Oct-09
The measurements and the All calibrations have been of Calibration Equipment used Primary Standards Power metar E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuato Reference 20 dB Attenuato Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753	uncertainties with confidence inducted in the closed laborat (M&TE critical for calibration)	probability are given on the follow ory facility: environment temperatu 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00786) 1-Jul-08 (No. 217-00787) 1-Jul-08 (No. 217-00866) 2-Jan-09 (No. ES3-3013_Jan 9-Sep-08 (No. DAE4-660_Se Check Date (in house) 4-Aug-99 (in house check Oc 18-Oct-01 (in house check Oc Function	ing pages and are part of the of ure (22 ± 3)°C and humidity < 1 Schedule Apr-09 Apr-09 Jul-09 Apr-09 Jul-09 09) Jan-10 p08) Sep-09 Schedule t-07) In house Signature 2er	d Check check: Oct-09 check: Oct-09



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst S Service suisse d'étalonnage С

Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary.

Glossary.	
TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
Polarization ϕ	o rotation around probe axis
Polarization 9	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held b) devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx, y, z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of • power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx, y, z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from \pm 50 MHz to \pm 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1642_Jan09

Page 2 of 9

Testing Services™	Document Appendix for the BlackBerry SAR Report	y® Smartphone Model I	RCK71CW	Page 4(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

January 12, 2009

Probe ET3DV6

SN:1642

Manufactured: Last calibrated: Recalibrated: November 7, 2001 January 18, 2008 January 12, 2009

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: ET3-1642_Jan09

Page 3 of 9

January 12, 2009

DASY - Parameters of Probe: ET3DV6 SN:1642

Sen	sitivity in Fr	ree Spac	e'		Diode	Compression
	NormX	1.6	58 ± 10.1%	μV/(V/m) ²	DCP X	91 mV
	NormY	1.8	38 ± 10.1%	μV/(V/m) ²	DCP Y	93 mV
	NormZ	1.6	56 ± 10.1%	μ V/(V/m) ²	DCP Z	93 mV
Sen	sitivity in Ti	issue Sin	nulating Li	quid (Conver	sion Factor	s)
Please	e see Page 8.					
Boui	ndary Effec	t				
TSL		900 MHz	Typical S/	AR gradient: 5 %	per mm	
	Sensor Cen	ter to Phanti	om Surface D	istance	3.7 mm	4.7 mm
	SAR _{be} [%]	Withou	t Correction A	lgorithm	- 10.1	5.8
	SAR _{be} [%]	With C	orrection Algo	rithm	0.9	0.5
TSL	1	810 MHz	Typical SA	R gradient: 10 %	per mm	
	Sensor Cent	ter to Phant	om Surface D	stance	3.7 mm	4.7 mm
	SAR _{be} [%]	Withou	t Correction A	Jgorithm	12.6	8.1
	SAR _{be} [%]	With C	orrection Algo	rithm	0.9	0.6
Sens	sor Offset					
	Probe Tip to	Sensor Cer	nter		2.7 mm	
The	anasted or -	antalaturat	-	ent is stated as	the standard	un acadalata af
						mal distribution
corre	sponds to a	coverage	probability	of approximatel	y 95%.	
The un	certainties of Norm	nX,Y,Z do not a	flect the E ² -field	uncertainty inside TSL	(see Page 8).	
			rtainty not require			

Certificate No: ET3-1642_Jan09


Page 4 of 9

Testing Services™	Document Appendix for the BlackBerry SAR Report	® Smartphone Model 1	RCK71CW	Page 6(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

January 12, 2009

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

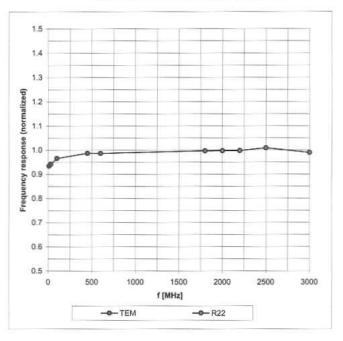


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: ET3-1642_Jan09


Page 5 of 9

Testing Services™	Appendix for the BlackBerr SAR Report	y® Smartphone Model 1	RCK71CW	Page 7(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

January 12, 2009

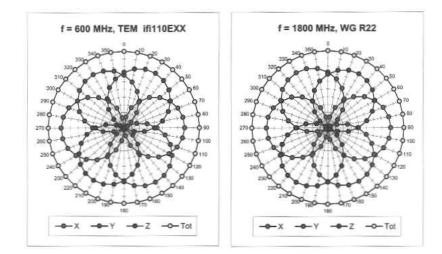

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

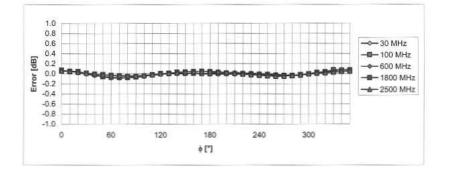


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ET3-1642_Jan09

Page 6 of 9

Testing Services™	Appendix for the BlackBerry SAR Report	® Smartphone Model R	CK71CW	Page 8(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

January 12, 2009

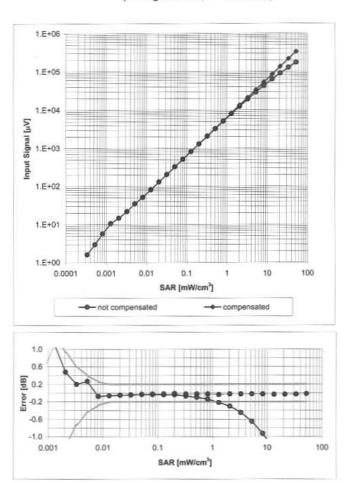






Certificate No: ET3-1642_Jan09

Page 7 of 9

Testing Services™	Document Appendix for the BlackBerry SAR Report	® Smartphone Model R	CK71CW	Page 9(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

January 12, 2009

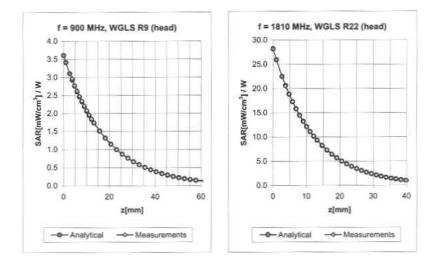

Conversion Factor Assessment

f [MHz]	Validity [MHz] ^C	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.40	2.33	6.06 ± 11.0% (k=2)
1810	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.54	2.62	5.14 ± 11.0% (k=2)
1950	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.67	2.35	4.88 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	0.90	1.74	4.54 ± 11.0% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.37	2.77	5.99 ± 11.0% (k=2)
1810	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.85	2.33	4.71 ± 11.0% (k=2)
1950	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.60	2.30	4.61 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.90	1.89	4.02 ± 11.0% (k=2)

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: ET3-1642_Jan09


Page 8 of 9

Testing Services™	Appendix for the BlackBerry SAR Report	® Smartphone Model R	CK71CW	Page 10(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

January 12, 2009

Deviation from Isotropy in HSL

Error (\, \,), f = 900 MHz

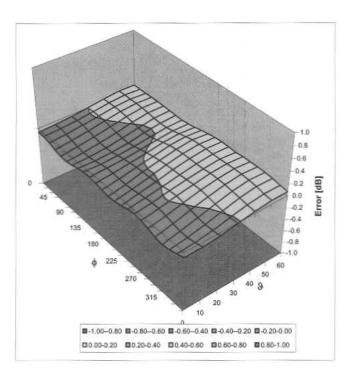


Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ET3-1642_Jan09

Page 9 of 9

Paul Hacquoil	Dates of Test July 23-August 12,	2009 Test Report No RTS-1765-0	907-30	FCC ID: L6ARCK70	CW
Calibration Labor Schmid & Partner Engineering AG Zeughausstrasse 43, 8004	-	BC MEA	C Service sui Servizio sv	scher Kalibrierdienst sse d'étalonnage izzero di taratura pration Service	
The Swiss Accreditation	Accreditation Service (SAS) Service is one of the signatorie r the recognition of calibration	s to the EA	tion No.: SCS	108	
Client RTS (RIM	Testing Services)	Certificate	No: D835V2	-446_Jan09	
CALIBRATIO	N CERTIFICATE				
Object	D835V2 - SN: 44	6			
Calibration procedure(s)	QA CAL-05.v7 Calibration proce	dure for dipole validation kits			
Calibration date:	January 05, 2009		LA CELER		
Condition of the calibrated	item In Tolerance				
This calibration certificate The measurements and th All calibrations have been Calibration Equipment use Primary Standards	documents the traceability to nati e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration)	onal standards, which realize the physical robability are given on the following pages y facility: environment temperature (22 ± 3 Cal Date (Certificate No.)	and are part of the second sec	e certificate. < 70%. uled Calibration	
This calibration certificate The measurements and th All calibrations have been Calibration Equipment use Primary Standards Power meter EPM-442A Power sensor HP 8481A	documents the traceability to nati e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration) ID # GB37480704 US37292783	robability are given on the following pages y facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898)	and are part of the and humidity	e certificate. < 70%. uled Calibration	
This calibration certificate The measurements and th All calibrations have been Calibration Equipment use Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuati	documents the traceability to nati e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration) ID # GB37480704 US37282783 or SN: 5086 (20g)	Cal Date (Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 01-Jul-08 (No. 217-00864)	and are part of th 3)*C and humidity Schedu Oct-09 Oct-09 Jul-09	e certificate. < 70%. uled Calibration	
This calibration certificate The measurements and th All calibrations have been Calibration Equipment use Primary Standards Power meter EPM-442A Power sensor HP 8481A	documents the traceability to nati e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration) ID # GB37480704 US37282783 or SN: 5086 (20g) tion SN: 5047.2 / 06327	robability are given on the following pages y facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898)	and are part of th 3)°C and humidity Schedi Oct-09 Oct-09	e certificate. < 70%. uled Calibration	
This calibration certificate The measurements and th All calibrations have been Calibration Equipment use Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenueth Type-N mismatch combina	documents the traceability to nati e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration) ID # GB37480704 US37282783 or SN: 5086 (20g) tion SN: 5047.2 / 06327	Cal Date (Certificate No.) 08-Oct-06 (No. 217-00898) 08-Oct-08 (No. 217-00898) 01-Jul-08 (No. 217-00864) 01-Jul-08 (No. 217-00867)	and are part of th 3)*C and humidity Schedi Oct-09 Oct-09 Jul-09 Jul-09	e certificate. < 70%. uled Calibration	
This calibration certificate The measurements and th All calibrations have been Calibration Equipment use <u>Primary Standards</u> Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuat Type-N mismatch combina Reference Probe ES3DV2	documents the traceability to nati e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration) ID # GB37480704 US37292783 ar SN: 5086 (20g) tion SN: 5047.2 / 06327 SN: 3025	Cal Date (Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 01-Jul-08 (No. 217-00664) 01-Jul-08 (No. 217-00867) 28-Apr-08 (No. ES3-3025_Apr08)	and are part of th 3)*C and humidity Schedi Oct-09 Jul-09 Jul-09 Mar-09	e certificate. < 70%. uled Calibration	
This calibration certificate The measurements and th All calibrations have been Calibration Equipment use Primary Standards Power meter EPM-442A Power sensor HP 9481A Reference 20 dB Attenuat Type-N mismatch combina Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A	documents the traceability to nati e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration) ID # GB37480704 US37282783 or SN: 5086 (20g) tion SN: 5047.2 / 06327 SN: 3025 SN: 3025 SN: 3025 SN: 601 ID #	coabbility are given on the following pages y facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 01-Jul-08 (No. 217-00898) 01-Jul-08 (No. 217-00864) 01-Jul-08 (No. 217-00867) 28-Apr-08 (No. ES3-3025_Apr08) 14-Mar-08 (No. DAE4-601_Mar08) Check Date (in house) 18-Oct-02 (in house check Oct-07)	and are part of th 3)*C and humidity Schedu Oct-09 Jul-09 Jul-09 Jul-09 Mar-09 Mar-09 Schedu In hous	e certificate. < 70%. uled Calibration	
This calibration certificate The measurements and th All calibrations have been Calibration Equipment use Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuah Type-N mismatch combina Reference Probe ES3DV2 DAE4 Secondary Standards	documents the traceability to nation e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration) ID # GB37480704 US37292783 or SN: 5086 (20g) tion SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 3 100005	robability are given on the following pages y facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 01-Jul-08 (No. 217-00864) 01-Jul-08 (No. 217-00867) 28-Apr-08 (No. ES3-3025_Apr08) 14-Mar-08 (No. DAE4-601_Mar08) Check Date (in house)	and are part of the 3)*C and humidity Oct-09 Oct-09 Jul-09 Jul-09 Jul-09 Mar-09 Schedu In hous In hous	e certificate. < 70%. uled Calibration	
This calibration certificate. The measurements and the All calibrations have been Calibration Equipment use Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenual Type-N mismatch combina Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 9481A RF generator R&S SMT-00 Network Analyzer HP 8753	documents the traceability to nati e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration) ID # GB37480704 US37292783 or SN: 5086 (20g) tion SN: 5086 (20g) SN: 5086 (20g) SN: 5086 (20g) SN: 5086 (20g) ID # ID # ID # ID # ID # ID # ID # ID #	robability are given on the following pages y facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 01-Jul-08 (No. 217-00864) 01-Jul-08 (No. 217-00867) 28-Apr-08 (No. ES3-3025_Apr08) 14-Mar-08 (No. DAE4-601_Mar08) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08) Function	and are part of the 3)*C and humidity Oct-09 Oct-09 Jul-09 Jul-09 Jul-09 Mar-09 Schedu In hous In hous	e certificate. < 70%. uled Calibration uled Check ue check: Oct-09 ie check: Oct-09 ie check: Oct-09	
This calibration certificate The measurements and th All calibrations have been Calibration Equipment use Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenueth Type-N mismatch combina Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	documents the traceability to nati e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration) ID # GB37480704 US37292783 or SN: 5086 (20g) tion SN: 5047.2 / 06327 SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 5 US37390585 S4206	Cal Date (Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 01-Jul-08 (No. 217-00898) 01-Jul-08 (No. 217-00897) 28-Apr-08 (No. 253-00567) 28-Apr-08 (No. DAE4-601_Mar08) Check Date (in house) Check Date (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07)	and are part of th 3)*C and humidity Schedi Oct-09 Jul-09 Jul-09 Apr-09 Mar-09 Schedi In hous In hous In hous	e certificate. < 70%. uled Calibration uled Check ue check: Oct-09 ie check: Oct-09 ie check: Oct-09	
This calibration certificate. The measurements and the All calibrations have been Calibration Equipment use Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenual Type-N mismatch combina Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 9481A RF generator R&S SMT-00 Network Analyzer HP 8753	documents the traceability to nati e uncertainties with confidence p conducted in the closed laborator d (M&TE critical for calibration) ID # GB37480704 US37292783 or SN: 5086 (20g) tion SN: 5086 (20g) SN: 5086 (20g) SN: 5086 (20g) SN: 5086 (20g) ID # ID # ID # ID # ID # ID # ID # ID #	robability are given on the following pages y facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 01-Jul-08 (No. 217-00864) 01-Jul-08 (No. 217-00867) 28-Apr-08 (No. ES3-3025_Apr08) 14-Mar-08 (No. DAE4-601_Mar08) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08) Function	and are part of th 3)*C and humidity Schedi Oct-09 Jul-09 Jul-09 Apr-09 Mar-09 Schedi In hous In hous In hous	e certificate. < 70%. uled Calibration uled Check ue check: Oct-09 ie check: Oct-09 ie check: Oct-09	



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst

C Service suisse d'étalonnage

Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D835V2-446_Jan09

Page 2 of 6

Testing Services™	Document Appendix for the BlackBerry SAR Report	y® Smartphone Model I	RCK71CW	Page 13(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.3 ± 6 %	0.91 mho/m ± 6 %
Head TSL temperature during test	(21.5±0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.40 mW / g
SAR normalized	normalized to 1W	9.60 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	9.50 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.58 mW / g
SAR normalized	normalized to 1W	6.32 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	6.27 mW /g ± 16.5 % (k=2)

1 Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D835V2-446_Jan09

Page 3 of 6

Testing Services™	Document Appendix for the BlackBerry SAR Report	v® Smartphone Model I	RCK71CW	Page 14(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.8 Ω - 6.9 jΩ	
Return Loss	- 23.3 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.385 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	October 24, 2001	

Certificate No: D835V2-446_Jan09

Page 4 of 6

Testing Services™	Appendix for the BlackBerry SAR Report	® Smartphone Model R	CK71CW	Page 15(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

DASY5 Validation Report for Head TSL

Date/Time: 05.01.2009 10:38:06

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:446


Communication System: CW-835; Frequency: 835 MHz; Duty Cycle: 1:1 Medium: HSL 900 MHz Medium parameters used: f = 835 MHz; σ = 0.91 mho/m; ε_r = 41.1; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC)

DASY5 Configuration:

- Probe: ES3DV2 SN3025; ConvF(5.97, 5.97, 5.97); Calibrated: 28.04.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 14.03.2008
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.4 Build 45

Pin=250mW; dip=15mm; dist=3.4mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 55.7 V/m; Power Drift = 0.024 dBPeak SAR (extrapolated) = 3.54 W/kgSAR(1 g) = 2.4 mW/g; SAR(10 g) = 1.58 mW/gMaximum value of SAR (measured) = 2.7 mW/g




 $0 \, dB = 2.7 mW/g$

Certificate No: D835V2-446_Jan09

Page 5 of 6

Testing Services [™]	Document Appendix for the BlackBerry SAR Report	® Smartphone Model F	RCK71CW	Page 16(28)
Author Data	Dates of Test	Test Report No	FCC ID:	
Jean-Paul Hacquoil	July 23-August 12, 2009	RTS-1765-0907-30	L6ARCK70	CW

Impedance Measurement Plot for Head TSL

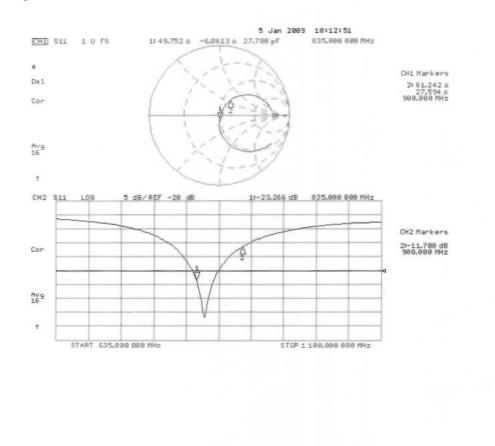

Certificate No: D835V2-446_Jan09

Page 6 of 6