
Testing Services™	Appendix D for the BlackBerr SAR Report	Page 1(30)
Author Data	Dates of Test	IC ID
Andrew Becker	June 10 – June 26, 2010	2503A-RCL20CW

# APPENDIX D: PROBE & DIPOLE CALIBRATION DATA



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





s Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Accreditation No.: SCS 108

#### Certificate No: ES3-3225 Dec09 RTS (RIM Testing Services) CALIBRATION CERTIFICATE AND THE PROPERTY OF THE PARTY O Object ES3DV3 - SN:3225 QA CAL-01.v6, QA CAL-23.v3 and QA CAL-25.v2 Calibration procedure(s) Calibration procedure for dosimetric E-field probes A Company of the comp all places are all the second December 11, 2009 Calibration date: This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards Cal Date (Certificate No.) Scheduled Calibration Power meter E4419B GB41293874 1-Apr-09 (No. 217-01030) Apr-10 Power sensor E4412A MY41495277 1-Apr-09 (No. 217-01030) Apr-10 Power sensor E4412A MY41498087 1-Apr-09 (No. 217-01030) Apr-10 Reference 3 dB Attenuator SN: S5054 (3c) 31-Mar-09 (No. 217-01026) Mar-10 Reference 20 dB Attenuator SN: S5086 (20b) 31-Mar-09 (No. 217-01028) Mar-10 Reference 30 dB Attenuator SN: S5129 (30b) 31-Mar-09 (No. 217-01027) Mar-10 Reference Probe ES3DV2 SN: 3013 2-Jan-09 (No. ES3-3013 Jan09) Jan-10 DAE4 SN: 660 29-Sep-09 (No. DAE4-660\_Sep09) Sep-10 Secondary Standards ID# Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 18-Oct-01 (in house check Oct-09) In house check: Oct10 Name Function Calibrated by: Claudio Leubler Laboratory Technician Approved by: Katja Pokovic Technical Manager Issued: December 11, 2009 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ES3-3225 Dec09

Page 1 of 11

	Testing Services™	Appendix D for th SAR Report	ne BlackBerr	ry® Smartphone Mod	lel RCL22CW	Page 3(30)
Author Data		Dates of Test		Test Report No	FCC ID:	IC ID
Andrew Recker		June 10 – June 26	2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

# Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty\_cycle) of the RF signal A, B, C modulation dependent linearization parameters

Polarization φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- EC 62209-1, \*Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
   NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is
  implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
  in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z; Bx,y,z; Cx,y,z, VRx,y,z: A, B, C are numerical linearization parameters assessed based on the data of
  power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
  maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ES3-3225\_Dec09 Page 2 of 11

Testing Services™	Appendix D for the BlackBerr SAR Report	ry® Smartphone Mod	lel RCL22CW	Page <b>4(30)</b>
Author Data	Dates of Test	IC ID		
Andrew Becker	June 10 – June 26, 2010	2503A-RCL20CW		

# Probe ES3DV3

SN:3225

Manufactured: September 1, 2009 Calibrated: December 11, 2009

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Testing Services™	Appendix D for the BlackBer SAR Report	ry® Smartphone Moo	lel RCL22CW	Page <b>5(30)</b>
Author Data	Dates of Test	IC ID		
Andrew Becker	June 10 – June 26, 2010	2503A-RCL20CW		

# DASY - Parameters of Probe: ES3DV3 SN:3225

# **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m) <sup>2</sup> ) <sup>A</sup>	1.26	1.22	1.32	± 10.1%
DCP (mV) <sup>B</sup>	92.3	94.8	92.7	

#### **Modulation Calibration Parameters**

UID	Communication System Name	PAR		A dB	B dBuV	С	VR mV	Unc <sup>E</sup> (k=2)
10000	cw	0.00	×	0.00	0.00	1.00	300.0	± 1.5%
			Y	0.00	0.00	1.00	300.0	
			z	0.00	0.00	1.00	300.0	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: ES3-3225\_Dec09

 $<sup>^{\</sup>rm h}$  The uncertainties of NormX, Y,Z do not affect the  $\hat{E^{\rm h}}$ -field uncertainty inside TSL (see Pages 5 and 6).

<sup>&</sup>lt;sup>B</sup> Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the maximum deviation from linear response applying recatangular distribution and is expressed for the square of the field value.

Testing Services™	Appendix D for the BlackBer SAR Report	ry® Smartphone Moo	lel RCL22CW	Page <b>6(30)</b>
Author Data	Dates of Test	IC ID		
Andrew Becker	June 10 – June 26, 2010	2503A-RCL20CW		

# DASY - Parameters of Probe: ES3DV3 SN:3225

# Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz]	Validity [MHz] <sup>C</sup>	Permittivity	Conductivity	ConvF X Co	nvFY Co	nvF Z	Alpha	Depth Unc (k=2)
900	±50/±100	41.5 ± 5%	0.97 ± 5%	6.12	6.12	6.12	0.99	1.07 ± 11.0%
1810	±50/±100	40.0 ± 5%	1.40 ± 5%	5.14	5.14	5.14	0.46	1.60 ± 11.0%
1950	±50/±100	$40.0 \pm 5\%$	1.40 ± 5%	4.96	4.96	4.96	0.47	1.57 ± 11.0%
2450	±50/±100	39.2 ± 5%	1.80 ± 5%	4.53	4.53	4.53	0.41	1.89 ± 11.0%

<sup>&</sup>lt;sup>C</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Testing Services™	Appendix D for the BlackE SAR Report	Berry® Smartphone Moo	del RCL22CW	Page <b>7(30)</b>
Author Data	Dates of Test	IC ID		
Andrew Becker	June 10 – June 26, 2010	2503A-RCL20CW		

# DASY - Parameters of Probe: ES3DV3 SN:3225

# Calibration Parameter Determined in Body Tissue Simulating Media


f [MHz]	Validity [MHz] <sup>C</sup>	Permittivity	Conductivity	ConvF X C	ConvF Y C	onvF Z	Alpha	Depth Unc (k=2
900	± 50 / ± 100	55.0 ± 5%	$1.05 \pm 5\%$	5.97	5.97	5.97	0.98	1.12 ± 11.0%
1810	±50/±100	$53.3 \pm 5\%$	1.52 ± 5%	4.90	4.90	4.90	0.35	2.07 ± 11.0%
1950	±50/±100	53.3 ± 5%	1.52 ± 5%	4.83	4.83	4.83	0.32	2.45 ± 11.0%
2450	± 50 / ± 100	52.7 ± 5%	$1.95 \pm 5\%$	4.32	4.32	4.32	0.74	1.27 ± 11.0%

<sup>&</sup>lt;sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Testing Services™	Appendix D for the BlackBerr SAR Report	Page <b>8(30)</b>
Author Data	Dates of Test	IC ID
Andrew Becker	June 10 – June 26, 2010	2503A-RCL20CW

# Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

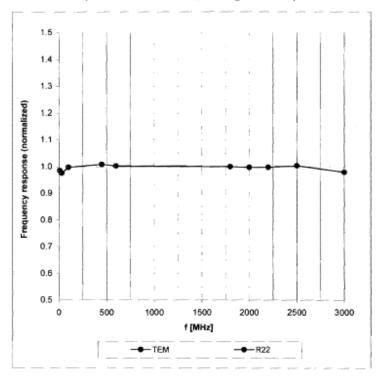


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Testing Services™	Appendix D for the BlackBo SAR Report	erry® Smartphone Moo	lel RCL22CW	Page <b>9(30)</b>
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker   June 10 – June 26, 2010   RTS-2068-1007-18   L6ARCL20CW				2503A-RCL20CW

# Receiving Pattern ( $\phi$ ), $\vartheta$ = 0°

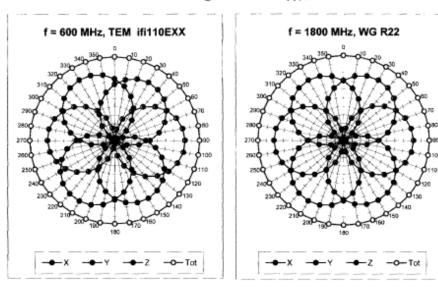

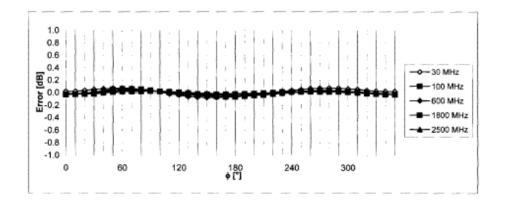


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Testing Services™	Appendix D for the BlackBerr SAR Report	Page 10(30)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

# Dynamic Range f(SAR<sub>head</sub>)


(Waveguide R22, f = 1800 MHz)

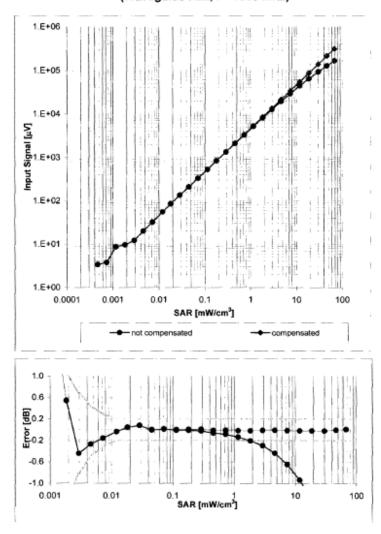


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RCL22CW SAR Report			Page 11(30)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW


# **Conversion Factor Assessment**





# Deviation from Isotropy in HSL

Error (φ, θ), f = 900 MHz

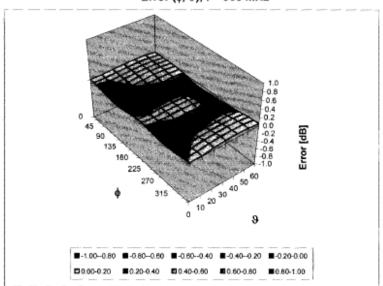

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Testing Services™	Appendix D for the BlackBerr SAR Report	Page 12(30)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

# Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4.0 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

Testing Services™	Appendix D for the BlackBerr SAR Report	Page 13(30)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S wiss Calibration Service

Accreditation No.: SCS 108


Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client RTS ( RIM Testing Services) Certificate No: D835V2-446\_Jan09

#### CALIBRATION CERTIFICATE D835V2 - SN: 446 Object QA CAL-05.v7 Calibration procedure(s) Calibration procedure for dipole validation kits January 05, 2009 Calibration date: Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID# Cal Date (Certificate No.) Scheduled Calibration GB37480704 Power meter EPM-442A 08-Oct-08 (No. 217-00898) Oct-09 11537292783 Power sensor HP 8481A 08-Oct-08 (No. 217-00898) Oct-09 Reference 20 dB Attenuator SN: 5086 (20g) 01-Jul-08 (No. 217-00864) Jul-09 Type-N mismatch combination SN: 5047.2 / 06327 01-Jul-08 (No. 217-00867) Jul-09 Reference Probe E\$3DV2 SN: 3025 28-Apr-08 (No. ES3-3025\_Apr08) Apr-09 DAE4 SN: 601 14-Mar-08 (No. DAE4-601\_Mar08) Mar-09 ID# Secondary Standards Check Date (in house) Scheduled Check Power sensor HP 8481A MY41092317 18-Oct-02 (in house check Oct-07) In house check: Oct-09 RF generator R&S SMT-06 100005 4-Aug-99 (in house check Oct-07) In house check: Oct-09 Network Analyzer HP 8753E US37390585 S4206 18-Oct-01 (in house check Oct-08) In house check: Oct-09 Name Function Calibrated by: Jeton Kastrati Laboratory Technician Approved by: Katja Pokovic Technical Manager Issued: January 7, 2009 This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: D835V2-446\_Jan09

Page 1 of 6



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S wiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- EC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D835V2-446_Jan09	Page 2 of 6	
Jerundate No. Dossyz-440_sanos	Page 2 of 6	

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RCL22CW SAR Report			Page 15(30)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	<b>June 10 – June 26, 2010</b>	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.3 ± 6 %	0.91 mho/m ± 6 %
Head TSL temperature during test	(21.5 ± 0.2) °C	and a	

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.40 mW/g
SAR normalized	normalized to 1W	9.60 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	9.50 mW/g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.58 mW/g
SAR normalized	normalized to 1W	6.32 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	6.27 mW /g ± 16.5 % (k=2)

Certificate No: D835V2-446\_Jan09

<sup>&</sup>lt;sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RCL22CW SAR Report			Page 16(30)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

#### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.8 Ω - 6.9 jΩ	
Return Loss	- 23.3 dB	

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.385 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	October 24, 2001

Certificate No: D835V2-446\_Jan09

Page 4 of 6

Testing Services™			Page <b>17(30)</b>	
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

# **DASY5 Validation Report for Head TSL**

Date/Time: 05.01.2009 10:38:06

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:446

Communication System: CW-835; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL 900 MHz

Medium parameters used: f = 835 MHz;  $\sigma = 0.91$  mho/m;  $\varepsilon_r = 41.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC)

#### DASY5 Configuration:

- Probe: ES3DV2 SN3025; ConvF(5.97, 5.97, 5.97); Calibrated: 28.04.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics; DAE4 Sn601; Calibrated: 14.03.2008
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.4 Build 45

Pin=250mW; dip=15mm; dist=3.4mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm,


dy=5mm, dz=5mm

Reference Value = 55.7 V/m; Power Drift = 0.024 dB

Peak SAR (extrapolated) = 3.54 W/kg

SAR(1 g) = 2.4 mW/g; SAR(10 g) = 1.58 mW/g

Maximum value of SAR (measured) = 2.7 mW/g




0 dB = 2.7 mW/g

Certificate No: D835V2-446\_Jan09

Page 5 of 6

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RCL22CW		Page <b>18(30)</b>	
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

# Impedance Measurement Plot for Head TSL

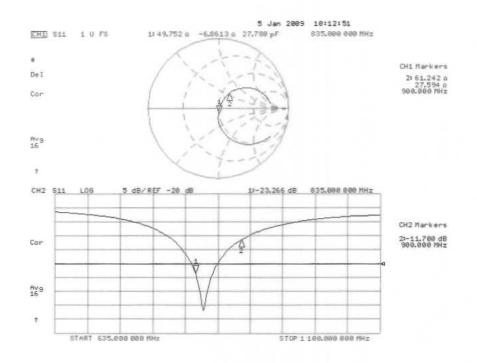

Certificate No: D835V2-446\_Jan09

Page 6 of 6

Testing Services™	Appendix D for the BlackBe SAR Report	rry® Smartphone Moo	lel RCL22CW	Page 19(30)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Certificate No: D1900V2-545-Jan09

Accreditation No.: SCS 108

Constitution of the Consti			Certificate No: D1900V2-545-Jan09	
CALIBRATION (	ERTIFICATE			
Object	D1900V2 - SN: 545			
Calibration procedure(s)	QA CAL-05.v7 Calibration procedure for dipole validation kits			
Calibration date:	January 06, 2009			
Condition of the calibrated item	In Tolerance	The second second	E 13 C 10 C	
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES30V2	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025	Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 01-Jul-08 (No. 217-00864) 01-Jul-08 (No. 217-00867)	Scheduled Calibration Oct-09 Oct-09 Jul-09 Jul-09	
		28-Apr-08 (No. ES3-3025_Apr08)	Apr-09	
DAE4	SN: 601	28-Apr-08 (No. ES3-3025_Apr08) 14-Mar-08 (No. DAE4-601_Mar08)	Apr-09 Mar-09	
DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	SN: 601 ID # MY41092317 100005 US37390585 S4206		Mar-09 Scheduled Check In house check: Oct-09 In house check: Oct-09	
Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	ID # MY41092317 100005 US37390585 S4206 Name	14-Mar-08 (No. DAE4-601_Mar-08)  Check Date (in house)  18-Oct-02 (in house check Oct-07)  4-Aug-99 (in house check Oct-07)  18-Oct-01 (in house check Oct-08)  Function	Mar-09	
Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	ID # MY41092317 100005 US37390585 S4206	14-Mar-08 (No. DAE4-601_Mar-08)  Check Date (in house)  18-Oct-02 (in house check Oct-07)  4-Aug-99 (in house check Oct-07)  18-Oct-01 (in house check Oct-08)	Mar-09 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09	
Secondary Standards Power sensor HP 6481A RF generator R&S SMT-06	ID # MY41092317 100005 US37390585 S4206 Name	14-Mar-08 (No. DAE4-601_Mar-08)  Check Date (in house)  18-Oct-02 (in house check Oct-07)  4-Aug-99 (in house check Oct-07)  18-Oct-01 (in house check Oct-08)  Function	Mar-09 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09	
Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by:	ID # MY41092317 100005 US37390585 S4206 Name Jeton Kastrati	14-Mar-08 (No. DAE4-601_Mar-08)  Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08)  Function Laboratory Technician	Mar-09 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09	

Certificate No: D1900V2-545\_Jan09

Page 1 of 6

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RCL22CW SAR Report  Page 20(30)		Page <b>20(30)</b>	
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

Calibration Laboratory of Schmid & Partner

Engineering AG Zeughavsstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Katibrierdienst
C Service suisse d'étalonnage
Servicio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D1900V2-545 Jan09

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RCL22CW SAR Report		Page <b>21(30)</b>	
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY5	V5.0
Advanced Extrapolation	
Modular Flat Phantom V5.0	
10 mm	with Spacer
dx, dy, dz = 5 mm	
1900 MHz ± 1 MHz	
	Advanced Extrapolation  Modular Flat Phantom V5.0  10 mm  dx, dy, dz = 5 mm

# Head TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.2 ± 6 %	1.47 mho/m ± 6 %
Head TSL temperature during test	(21.0 ± 0.2) °C	_	mpen.

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	condition	
SAR measured	250 mW input power	10.2 mW / g
SAR normalized	normalized to 1W	40.8 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	39.5 mW/g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.29 mW / g
SAR normalized	normalized to 1W	21.2 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	20.8 mW / g ± 16.5 % (k=2)

Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Testing Services™	Appendix D for the BlackBer SAR Report	ry® Smartphone Moo	lel RCL22CW	Page 22(30)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

Appendix.

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	$49.9 \Omega + 1.9 j\Omega$
Return Loss	- 34.4 dB

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.197 ns
Total Control of the	(12/17/1/28)

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	November 15, 2001

Testing Services™	Appendix D for the BlackBer SAR Report	rry® Smartphone Moo	lel RCL22CW	Page 23(30)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

#### **DASY5 Validation Report for Head TSL**

Date/Time: 06.01.2009 13:17:58

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:545

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB

Medium parameters used: f = 1900 MHz;  $\sigma = 1.47$  mho/m;  $\varepsilon_r = 39.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC)

#### DASY5 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.9, 4.9, 4.9); Calibrated: 28.04.2008.
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 14.03.2008
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.4 Build 45

# Pin = 250 mW; dip = 10 mm, scan at 3.4mm/Zoom Scan (dist=3.4mm, probe 0deg)


(7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 92.5 V/m; Power Drift = 0.037 dB

Peak SAR (extrapolated) = 19 W/kg

SAR(1 g) = 10.2 mW/g; SAR(10 g) = 5.29 mW/g


Maximum value of SAR (measured) = 12 mW/g



0~dB=12mW/g

Testing Services™	Appendix D for the BlackBerr SAR Report	Page 24(30)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

#### Impedance Measurement Plot for Head TSL

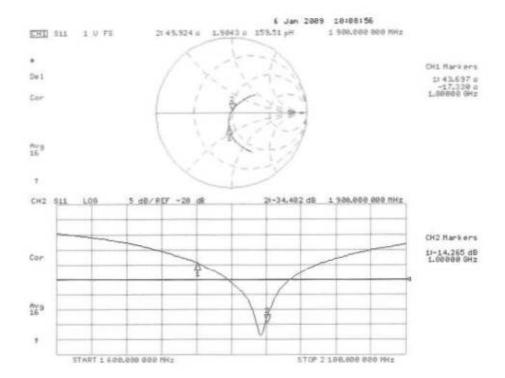

Testing Services™	Appendix D for the BlackBer SAR Report	ry® Smartphone Moo	lel RCL22CW	Page <b>25(30)</b>
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

Calibration Laboratory of Schmid & Partner Engineering AG





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage С Servizio svizzero di taratura s Swiss Calibration Service

Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

RTS (RIM Testing Services) Client

Certificate No: D2450V2-747\_Nov09

Accreditation No.: SCS 108

#### CALIBRATION CERTIFICA D2450V2 - SN: 747 Object QA CAL-05.V7 Calibration procedure(s) Calibration procedure for dipole validation kits Calibration date: November 11, 2009 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards Cal Date (Certificate No.) Scheduled Calibration Power meter EPM-442A GB37480704 06-Oct-09 (No. 217-01086) Oct-10 Power sensor HP 8481A US37292783 06-Oct-09 (No. 217-01086) Oct-10 Reference 20 dB Attenuator SN: 5086 (20g) 31-Mar-09 (No. 217-01025) Mar-10 Type-N mismatch combination SN: 5047.2 / 06327 31-Mar-09 (No. 217-01029) Mar-10 Reference Probe ES3DV3 SN: 3205 26-Jun-09 (No. ES3-3205\_Jun09) Jun-10 DAE4 SN: 601 07-Mar-09 (No. DAE4-601\_Mar09) Mar-10 Secondary Standards ID# Check Date (in house) Scheduled Check Power sensor HP 8481A MY41092317 18-Oct-02 (in house check Oct-09) In house check: Oct-11 RF generator R&S SMT-06 100005 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 S4206 18-Oct-01 (in house check Oct-09) In house check: Oct-10 Name Function Calibrated by: Approved by: Issued: November 16, 2009 This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: D2450V2-747\_Nov09 Page 1 of 6

Testing Services™	Appendix D for the BlackBer SAR Report	ry® Smartphone Moo	lel RCL22CW	Page <b>26(30)</b>
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst

C Service suisse d'étalonnage Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D2450V2-747\_Nov09 Page 2 of 6

Testing Services™	Appendix D for the BlackBerr SAR Report	ry® Smartphone Mod	lel RCL22CW	Page <b>27(30)</b>
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

#### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

# **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mha/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.1 ± 6 %	1.78 mho/m ± 6 %
Head TSL temperature during test	(21.3 ± 0.2) °C		

#### SAR result with Head TSL

SAR averaged over 1 cm3 (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.3 mW / g
SAR normalized	normalized to 1W	53.2 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	53.4 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.23 mW / g
SAR normalized	normalized to 1W	24.9 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.9 mW /g ± 16.5 % (k=2)

Certificate No: D2450V2-747\_Nov09

Testing Services™	Appendix D for the BlackBerr SAR Report	ry® Smartphone Mod	lel RCL22CW	Page <b>28(30)</b>
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

#### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.9 Ω + 0.9 jΩ
Return Loss	- 33.9 dB

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.161 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	December 01, 2003

Certificate No: D2450V2-747\_Nov09

Testing Services™	Appendix D for the BlackBer SAR Report	ry® Smartphone Mod	lel RCL22CW	Page <b>29(30)</b>
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW

### **DASY5 Validation Report for Head TSL**

Date/Time: 11.11.2009 15:04:10

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:747

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U11 BB

Medium parameters used: f = 2450 MHz;  $\sigma = 1.79 \text{ mho/m}$ ;  $\varepsilon_r = 39.2$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 26.06.2009

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 07.03.2009

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

#### Head/d=10mm, Pin=250 mW, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.3 V/m; Power Drift = 0.067 dB

Peak SAR (extrapolated) = 27 W/kg

SAR(1 g) = 13.3 mW/g; SAR(10 g) = 6.23 mW/g

Maximum value of SAR (measured) = 17.1 mW/g

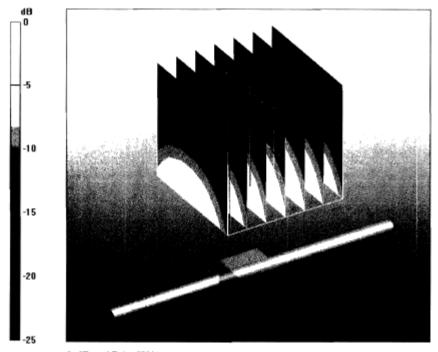

0 dB = 17.1 mW/g

Certificate No: D2450V2-747\_Nov09

Page 5 of 6

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RCL22CW SAR Report			Page 30(30)	
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID	
Andrew Becker	June 10 – June 26, 2010	RTS-2068-1007-18	L6ARCL20CW	2503A-RCL20CW	

# Impedance Measurement Plot for Head TSL

