Testing Services™	Annex B to Hearing Aid Report for the BlackBer	Page 1(25)		
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W

# Annex B: Probe and dipole description and calibration certificates

B.1 Probe, measurement chain description, specification and calibration certificate

Testing Services™		Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW				
Author Data	Dates of Test					
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W		

DASY Dosimetric Assessment System by Schmid & Partner Engineering AG



Applications	ER3DV6 ISOTROPIC E-FIELD PROBE FOR GENERAL NEAR-FIELD MEASUREMENTS				
Support & Downloads	-				
Products	🖂 Download Produ	<u>ct Flyer</u> (PDF, 192kB)			
• DASY4 Packages					
• EASY4	Construction	One dipole parallel, two dipoles normal to probe axis			
Probes     ET3DV6 - Isotropic Dos-Probe     ES3DV3 - Isotropic Dos-Probe     EV3DV4 - Isotropic Dos-Probe		Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., glycolether)			
EX3DV4 - Isotropic Dos-Probe ET1DV3 - D-Probe	Calibration	In air from 100 MHz to 3.0 GHz (absolute accuracy ±6.0%, k=2)			
EUV3 - Universal Vector E-Probe H3DV6 - Isotropic H-Probe	Frequency	100 MHz to > 6 GHz; Linearity: $\pm$ 0.2 dB (100 MHz to 3 GHz)			
HUV4 - Universal Vector H-Probe T1V3 - Temp-Probe DP1 - Dummy-Probe	Directivity	± 0.2 dB in air (rotation around probe axis) ± 0.4 dB in air (rotation normal to probe axis)			
Data Acquisition System	Dynamic Range	2 V/m to > 1000 V/m; Linearity: ± 0.2 dB			
• Software • Phantoms • Robots	Dimensions	Overall length: 330 mm (Tip: 16 mm) Tip diameter: 8 mm (Body: 12 mm) Distance from probe tip to dipole centers: 2.5 mm			
<ul> <li>Validation Kits &amp; Calibration Dipoles</li> <li>Hearing Aid Compatibility (HAC) Ext</li> <li>Tissue Simulating Liquids</li> </ul>	Application	General near-field measurements up to 6 GHz Field component measurements Fast automatic scanning in phantoms			
SPEAG Home					

http://www.dasy4.com/er3.htm

Testing Services™		Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW				
Author Data	Dates of Test					
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W		

DASY Dosimetric Assessment System by Schmid & Partner Engineering AG

DASY Schmid & Partner Engineering AG News Sales Contact		
Applications	H3DV6 3-DIMENSIO	NAL H-FIELD PROBE FOR SMALL BAND
Support & Downloads	-	
Products	Download Product Fl	<u>yer</u> (PDF, 192kB)
DASV4 Packages		
EASY4     Probes     ET3DV6 - Isotropic Dos-Probe     ES3DV3 - Isotropic Dos-Probe     EX3DV4 - Isotropic Dos-Probe	Construction	Three concentric loop sensors with 3.8 mm loop diameters Resistively loaded detector diodes for linear response Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., glycolether)
ET1DV3 - D-Probe ER3DV6 - Isotropic E-Probe	Frequency	200 MHz to 3 GHz (absolute accuracy ± 6.0%, k=2); Output linearized
EUV3 - Universal Vector E-Probe	Directivity	± 0.25 dB (spherical isotropy error)
HUV4 - Universal Vector H-Probe	Dynamic Range	10 mA/m to 2 A/m at 1 GHz
T1V3 - Temp-Probe DP1 - Dummy-Probe	E-Field Interference	< 10% at 3 GHz (for plane wave)
Data Acquisition System     Software	Dimensions	Overall length: 330 mm (Tip: 40 mm) Tip diameter: 6 mm (Body: 12 mm) Distance from probe tip to dipole centers: 3 mm
Phantoms     Robots     Validation Kits & Calibration Dipoles     Hearing Aid Compatibility (HAC) Ext     Tissue Simulating Liquids	Application	General magnetic near-field measurements up to 3 GHz Field component measurements Surface current measurements Measurements in air or liquids Low interaction with the measured field
SPEAG Home		

http://www.dasy4.com/h3d.htm


Testing Services™		Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW			
Author Data	Dates of Test				
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W	

All measurements were performed to the nearest element point as per the C63.19 standard. Offset distances were entered in the DASY4 software so that the measurement was to the nearest element.

Figures 1 and 2, provided by the manufacturer, illustrate detail of the probe tip and its dimensions.

**ER3DV6** E-Field probe: The distances from the probe tip to the closest points on the dipole sensors are 1.45mm for X and Y and 1.25mm for Z. From the probe tip to the center of the sensors is 2.5mm.

**H3DV6** H-Field probe: The distance from the probe tip to the closest point of the X, Y and Z loop sensors is 1.1mm. From the probe tip to the center of the sensor is 3.00mm.

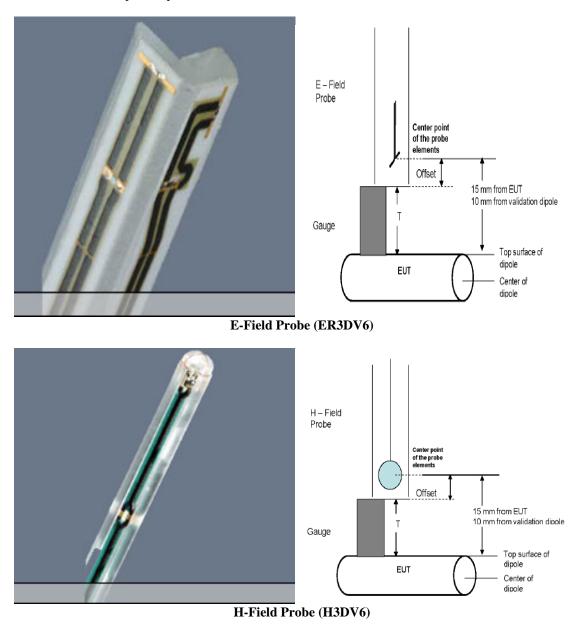

This report shall <u>NOT</u> be reproduced except in full without the written consent of RIM Testing Services Copyright 2005-2010, RIM Testing Services, A division of Research In Motion Limited

Testing Services™	Annex B to Hearing Aid Report for the BlackBerr			Page 5(25)
Author Data	Dates of Test			
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W

The following information is from the system manufacturer user manual describing the process chain:

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$
(20.1)

with	$V_i$	= compensated signal of channel i	(i = x, y, z)
	$U_i$	= input signal of channel i	(i = x, y, z)
	cf	= crest factor of exciting field	(DASY parameter)
	$dcp_i$	= diode compression point	(DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

	$\mathrm{E-field probes}$ :	$E_i = \sqrt{\frac{V_i}{Norm_i \cdot C}}$	onvF
	$\mathbf{H}-\mathbf{fieldprobes}$ :	$H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}f}{f}$	$f + a_{i2}f^2$
with	= compensated signal of $\alpha$ = sensor sensitivity of cha $\mu V/(V/m)^2$ for E-field = sensitivity enhancement = sensor sensitivity factor = carrier frequency [GHz] = electric field strength of = magnetic field strength	nnel i l Probes t in solution rs for H-field probes f channel i in V/m	$\begin{array}{l} (i=x,y,z) \\ (i=x,y,z) \end{array}$

The RSS value of the field components gives the total field strength (Hermitian magnitude):


$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$
(20.2)

The measurement / integration time per point is > 500 ms, as per the system manufacturer:

The time response of the field probes has been assessed by exposing the probe to a well-controlled field producing signals larger than HAC E- and H-fields of class M4. The signal response time is evaluated as the time required by the system to reach 90% of the expected final value after an on/off switch of the power source with an integration time of 500 ms and a probe response time of <5 ms. In the current implementation, DASY4 waits longer than 100 ms after having reached the grid point before starting a measurement, i.e., the response time uncertainty is negligible.

If the device under test does not emit a CW signal, the integration time applied to measure the electric field at a specific point may introduce additional uncertainties due to the discretization. The tolerances for the different systems had the worst-case of 2.6%.

				el RDB/1UW
	Dates of Test	Report No	71 1005 57	FCC ID
Attayi	April 12-20, 2	2010 R15-26	571-1005-57	L6ARDB70UW
<b>Calibration Laborato</b> Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zuri		BOC MEA P. BRAND	S Schweizerischer C Service suisse d Servizio svizzero S Swiss Calibration	étalonnage di taratura
Accredited by the Swiss Accredit The Swiss Accreditation Servic Multilateral Agreement for the	ce is one of the signatorie recognition of calibration	es to the EA a certificates	itation No.: SCS 108	
Client RTS (RIM Tes	ting Services)	Certific	ate No: ER3-2286_J	an10
CALIBRATION	CERTIFICAT	E		
Object	FR3DVA SN-2	286		
	C100200 50112		Stanfallan - Nabrani - Julia - Da	8 - 1 (9889-14) -
Calibration procedure(s)		ind QA CAL-25.v2 edure for E-field probes optim	tized for close near	field
	evaluations in a	A H H West		
Calibration date:				
This calibration certificate docur The measurements and the unc	January 8, 2010		cal units of measurements ges and are part of the cert	(SI). ficate.
This calibration certificate docur The measurements and the unc	January 8, 2010	tional standards, which realize the physi probability are given on the following pag	cal units of measurements ges and are part of the cert	(SI). ficate.
This calibration certificate docur The measurements and the unc All calibrations have been cond Calibration Equipment used (M& Primary Standards	January 8, 2010 ments the traceability to na pertainties with confidence ucted in the closed laborate STE critical for calibration) ID #	tional standards, which realize the physi probability are given on the following pag pry facility: environment temperature (22 Cal Date (Certificate No.)	cal units of measurements ges and are part of the cert ± 3)°C and humidity < 709 Scheduled C	(SI). ficate. 6.
This calibration certificate docur The measurements and the unc All calibrations have been cond Calibration Equipment used (Ma	January 8, 2010 ments the traceability to na pertainties with confidence ucted in the closed laboration STE critical for calibration)	tional standards, which realize the physio probability are given on the following page pry facility: environment temperature (22	cal units of measurements ges and are part of the cert ± 3)°C and humidity < 70%	(SI). ficate. 6.
This calibration certificate docur The measurements and the unc All calibrations have been cond Calibration Equipment used (M& Primary Standards Power meter E4419B	January 8, 2010 ments the traceability to na vertaintiles with confidence i ucted in the closed laborato &TE critical for calibration) ID # GB41293874	tional standards, which realize the physis probability are given on the following pag pry facility: environment temperature (22 <u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030)	cal units of measurements ges and are part of the cert ± 3)°C and humidity < 70% Scheduled C Apr-10	(SI). ficate. 6.
This calibration certificate docur The measurements and the unc All calibrations have been cond Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	January 8, 2010 ments the traceability to na pertainties with confidence ucted in the closed laboration) ID # GB41293874 MY41495277 MY41495277 MY41498087 SN: S5054 (3c)	tional standards, which realize the physio probability are given on the following pay ory facility: environment temperature (22 <u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026)	cal units of measurements ges and are part of the cert ± 3)*C and humidity < 709 Scheduled C Apr-10 Apr-10 Apr-10 Mar-10	(SI). ficate. 6.
This calibration certificate docur The measurements and the unc All calibrations have been condi Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	January 8, 2010 ments the traceability to na pertainties with confidence ucted in the closed laborate STE critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: S5054 (3c) SN: S5086 (20b)	tional standards, which realize the physi probability are given on the following pag pry facility: environment temperature (22 <u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028)	cal units of measurements ges and are part of the cert ± 3)*C and humidity < 70% Scheduled C Apr-10 Apr-10 Mar-10 Mar-10 Mar-10	(SI). ficate. 6.
This calibration certificate docur The measurements and the unc All calibrations have been cond Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	January 8, 2010	tional standards, which realize the physis probability are given on the following pag ory facility: environment temperature (22 <u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01027)	cal units of measurements ges and are part of the cert ± 3)°C and humidity < 709 Scheduled C Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Mar-10	(SI). ficate. 6.
This calibration certificate docur The measurements and the unc All calibrations have been condi Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	January 8, 2010 ments the traceability to na pertainties with confidence ucted in the closed laborate STE critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: S5054 (3c) SN: S5086 (20b)	tional standards, which realize the physi probability are given on the following pag pry facility: environment temperature (22 <u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028)	cal units of measurements ges and are part of the cert ± 3)*C and humidity < 70% Scheduled C Apr-10 Apr-10 Mar-10 Mar-10 Mar-10	(SI). ficate. 6.
This calibration certificate docur The measurements and the unc All calibrations have been cond Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator	January 8, 2010	tional standards, which realize the physio probability are given on the following pay pry facility: environment temperature (22 <u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 3-Oct-09 (No. ER3-2328_Oct09)	cal units of measurements tes and are part of the cert ± 3)°C and humidity < 70% Scheduled C Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Oct-10	(SI). ficate. 6. alibration
This calibration certificate docur The measurements and the unc All calibrations have been condi Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 70 dB Attenuator Reference Probe ER3DV6 DAE4	January 8, 2010 ments the traceability to na certainties with confidence ucted in the closed laborate STE critical for calibration) ID # GB41293874 MY41495277 MY41495277 MY41496087 SN: S5054 (3c) SN: S5056 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 2328 SN: 789	tional standards, which realize the physio probability are given on the following page ory facility: environment temperature (22 <u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01027) 31-Oct-09 (No. 217-01027) 3-Oct-09 (No. DAE4-789_Dec09)	cal units of measurements ges and are part of the cert ± 3)*C and humidity < 709 Scheduled C Apr-10 Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Oct-10 Dec-10	(SI). ficate. 6. alibration
This calibration certificate docur The measurements and the unc All calibrations have been condi Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ER3DV6 DAE4 Secondary Standards	January 8, 2010	tional standards, which realize the physis probability are given on the following pag- bry facility: environment temperature (22 <u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 3-Oct-09 (No. DAE4-789_Dec09) 23-Dec-09 (No. DAE4-789_Dec09)	cal units of measurements tes and are part of the cert ± 3)*C and humidity < 70% Scheduled C Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Oct-10 Dec-10 Scheduled C	(SI). ficate. 6. alibration
This calibration certificate docur The measurements and the unc All calibrations have been cond Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ER3DV6 DAE4 Secondary Standards RF generator HP 8648C	January 8, 2010	tional standards, which realize the physis probability are given on the following pag ory facility: environment temperature (22 <u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01027) 31-Mar-09 (No. 217-01027) 31-Oct-09 (No. ER3-2328_Oct09) 23-Dec-09 (No. DAE4-789_Dec09) <u>Check Date (in house)</u> 4-Aug-99 (in house check Oct-09)	cal units of measurements ges and are part of the cert ± 3)°C and humidity < 709 Scheduled C Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Oct-10 Dec-10 Scheduled C In house che	(SI). ficate. 6. alibration
This calibration certificate docur The measurements and the unc All calibrations have been cond Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ER3DV6 DAE4 Secondary Standards RF generator HP 8648C	January 8, 2010 ments the traceability to na pertainties with confidence ucted in the closed laboratu BTE critical for calibration) ID # GB41293874 MY41495277 MY41495277 MY41495087 SN: S5054 (3c) SN: S5056 (20b) SN: S5056 (20b) SN: S5129 SN: S5129 SN: 789 ID # US3642U01700 US37390585	tional standards, which realize the physio probability are given on the following pay pay facility: environment temperature (22 <u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01027) 3-Oct-09 (No. ER3-2328_Oct09) 23-Dec-09 (No. DAE4-789_Dec09) <u>Check Date (in house)</u> 4-Aug-99 (in house check Oct-09) 18-Oct-01 (in house check Oct-09)	cal units of measurements ges and are part of the cert ± 3)°C and humidity < 709 Scheduled C Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Oct-10 Dec-10 Scheduled C In house che In house che	(SI). ficate. 6. alibration
This calibration certificate docur The measurements and the unc All calibrations have been condi Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 7 ob ER3DV6 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	January 8, 2010	tional standards, which realize the physio probability are given on the following pay boy facility: environment temperature (22 Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 3-Oct-09 (No. ER3-2328, Oct09) 23-Dec-09 (No. ER3-2328, Oct09) 23-Dec-09 (No. ER3-2328, Oct09) 23-Dec-09 (in bouse check Oct-09) Check Date (in house check Oct-09) 18-Oct-01 (in house check Oct-09) Function	cal units of measurements ges and are part of the cert ± 3)°C and humidity < 709 Scheduled C Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Oct-10 Dec-10 Scheduled C In house che In house che	(SI). ficate. 6. alibration



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glos	sary:	
NOR	Mx,y,z	sensitivity in free space
DCP		diode compression point
CF		crest factor (1/duty_cycle) of the RF signal
A, B,	С	modulation dependent linearization parameters
Polar	ization φ	φ rotation around probe axis
Polar	ization 9	$\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Conn	ector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

# Calibration is Performed According to the Following Standards:

 a) IEEE Std 1309-2005, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", December 2005.

### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization ∂ = 0 for XY sensors and ∂ = 90 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart).
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z; Bx,y,z; Cx,y,z, VRx,y,z: A, B, C are numerical linearization parameters assessed based on the data of
  power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
  maximum calibration range expressed in RMS voltage across the diode.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Page 2 of 10

Testing Services™		Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW				
Author Data	Dates of Test	Report No	FCC ID			
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W		

January 8, 2010

# Probe ER3DV6


# SN:2286

Manufactured: Last calibrated: Recalibrated: September 18, 2002 January 8, 2009 January 8, 2010

Calibrated for DASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: ER3-2286\_Jan10

Page 3 of 10



# January 8, 2010

# DASY - Parameters of Probe: ER3DV6 SN:2286

# **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)$	2.23	1.50	1.54	± 10.1%
DCP (mV) <sup>A</sup>	94.9	94.8	95.7	

# **Modulation Calibration Parameters**

UID	Communication System Name	PAR		A dB	B dBuV	с	VR mV	Unc <sup>e</sup> (k=2)
10000	cw	0.00	x	0.00	0.00	1.00	300	± 1.5 %
			Y	0.00	0.00	1.00	300	
			z	0.00	0.00	1.00	300	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A numerical linearization parameter: uncertainty not required

<sup>6</sup> Uncertainty is determined using the maximum deviation from linear response applying recatangular distribution and is expressed for the square of the field value


Certificate No: ER3-2286\_Jan10

Page 4 of 10

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW			
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010 RTS-2671-1005-57 L6ARDB70UW			W

January 8, 2010

# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide R22)

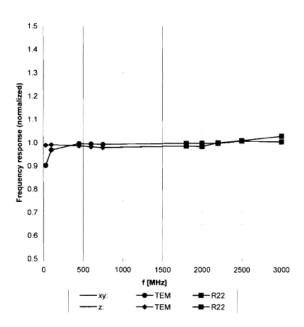


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: ER3-2286\_Jan10

Page 5 of 10


Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW			
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010 RTS-2671-1005-57 L6ARDB70UW			

January 8, 2010

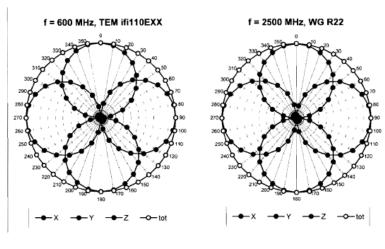

Receiving Pattern ( $\phi$ ),  $\vartheta$  = 0°

Receiving Pattern ( $\phi$ ),  $\vartheta$  = 90°

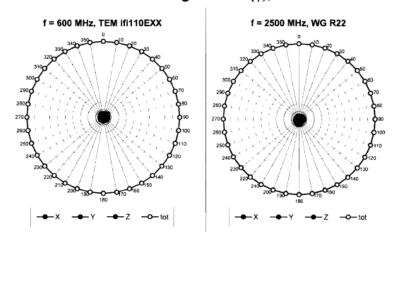


Certificate No: ER3-2286\_Jan10

Page 6 of 10


Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW			
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010 RTS-2671-1005-57 L6ARDB70UW			W

January 8, 2010

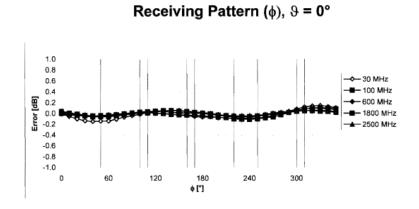

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

# Receiving Pattern ( $\phi$ ), $\vartheta$ = 90°

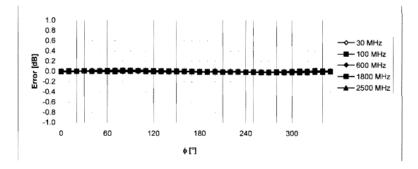


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ER3-2286\_Jan10

Page 7 of 10

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW			Page 13(25)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010 RTS-2671-1005-57 L6ARDB70UW			W

January 8, 2010

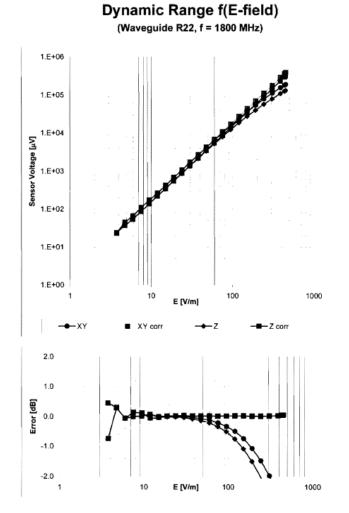




```
Certificate No: ER3-2286_Jan10
```

Page 8 of 10

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW			Page 14(25)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010 RTS-2671-1005-57 L6ARDB70UW			

January 8, 2010

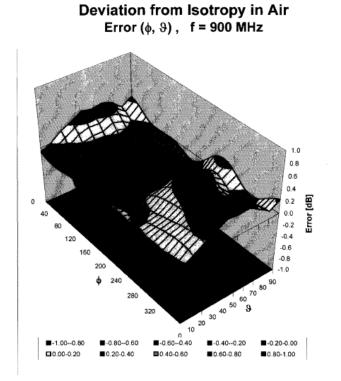

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ER3-2286\_Jan10

Page 9 of 10

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW			
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010 RTS-2671-1005-57 L6ARDB70UW			

January 8, 2010


# **Other Probe Parameters**

Sensor Arrangement	Rectangular
Connector Angle (°)	-9.5
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	8.0 mm
Probe Tip to Sensor X Calibration Point	2.5 mm
Probe Tip to Sensor Y Calibration Point	2.5 mm
Probe Tip to Sensor Z Calibration Point	2.5 mm

Certificate No: ER3-2286\_Jan10

Page 10 of 10

Test Serv			ompatibility RF Emi B Smartphone mode		Page 16(25
thor Data aoud Attayi	Dates of Test April 12-20		eport No RTS-2671-1005-57	FCC ID L6ARDB70U	IW
Schmid & F Engineer			ISS Schweizerischer Kalib C Service suisse d'étalor C Servizio svizzero di tar S Swiss Calibration Serv	inage atura	
The Swiss Acc Multilateral Agr	e Swiss Accreditation Service (SAS) editation Service is one of the sign eement for the recognition of calibi	ration certificates	Accreditation No.: SCS 108		
Client RT	S (RIM Testing Services)	the state of the second se	Certificate No: H3-6105_Nov09	an the state of the second	
CALIBR	ATION CERTIFIC	ATE			
Object	H3DV6 - SN	:6105	ann ann ann a	uch	
Calibration proc		C. S. S. S. S. K. K. S.	s optimized for close near field		
Calibration date	November 1	3, 2009			
1			the physical units of measurements (SI). owing pages and are part of the certificate.		
All calibrations	have been conducted in the closed la	boratory facility: environment temper	ature (22 ± 3)°C and humidity < 70%.		
Calibration Equ	ipment used (M&TE critical for calibra	tion)			
Primary Standa	rds ID #	Cal Date (Certificate No.)	Scheduled Calibrat	ion	
Power meter E Power sensor E		1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030)	Apr-10		
Power sensor E		1-Apr-09 (No. 217-01030)	Apr-10 Apr-10		
Reference 3 dE					
Reference 20 d	B Attenuator SN: S5086 (20)				
Reference 30 d					
Reference Prot DAE4	e H3DV6 SN: 6182 SN: 789	3-Oct-09 (No. H3-6182_O 19-Dec-08 (No. DAE4-789			
Secondary Star	ndards ID #	Check Date (in house)	Scheduled Check		
RF generator H Network Analyz		) 4-Aug-99 (in house check 18-Oct-01 (in house check			
Calibrated by:	Name Kalja Pokovic	Function Technical Ma	nager Signature	¢.	
Approved by:	Niels Kuster	Quality Mana		5	
This calibration	certificate shall not be reproduced ex	cept in full without written approval o	f the laboratory.	13, 2009	
Certificate No:	H3-6105_Nov09	Page 1 of 10			



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



NIS

s

С

s

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

## Glossary:

NORMx,y,z	sensitivity in free space
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization o	φ rotation around probe axis
Polarization 9	9 rotation around an axis that is in the plane normal to probe axis (at measurement center),
	i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards: a) IEEE Std 1309-2005, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz\*, December 2005.

### Methods Applied and Interpretation of Parameters:

- NORMx, y, z: Assessed for E-field polarization  $\vartheta = 0$  for XY sensors and  $\vartheta = 90$  for Z sensor (f  $\leq 900$  MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- X, Y,Z(f)\_a0a1a2= X, Y,Z\_a0a1a2\* frequency\_response (see Frequency Response Chart).
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW ٠ signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z; Bx,y,z; Cx,y,z, VRx,y,z: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required
- Connector Angle: The angle is assessed using the information gained by determining the X\_a0a1a2 (no uncertainty required).

Certificate No: H3-6105\_Nov09

Page 2 of 10

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDB71UW			Page 18(25)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010 RTS-2671-1005-57 L6ARDB70UW			W

November 13, 2009

# Probe H3DV6

# SN:6105


Manufactured: Last calibrated: Recalibrated: January 5, 2002 November 10, 2008 November 13, 2009

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: H3-6105\_Nov09

Page 3 of 10



## November 13, 2009

# DASY - Parameters of Probe: H3DV6 SN:6105

## **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (A/m / √(µV)) a0	2.89E-3	2.67E-3	3.00E-3	± 5.1%
Norm (A/m / √(μV)) a1	6.03E-5	3.03E-5	-9.91E-5	± 5.1%
Norm (A/m / √(μV)) a2	-1.23E-5	3.46E-6	1.02E-5	± 5.1%
DCP (mV) <sup>A</sup>	89.5	84.4	83.4	

# **Modulation Calibration Parameters**

UID	Communication System Name	PAR		A dB	B dBuV	с	VR mV	Unc <sup>E</sup> (k=2)
10000	cw	0.00	x	0.00	0.00	1.00	300	± 1.5%
			Y	0.00	0.00	1.00	300	
			z	0.00	0.00	1.00	300	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A numerical linearization parameter: uncertainty not required

<sup>E</sup> Uncertainty is determined using the maximum deviation from linear response applying recatangular distribution and is expressed for the square of the field value.

Certificate No: H3-6105\_Nov09


Page 4 of 10

Testing Services™	Annex B to Hearing Aid Report for the BlackBer			Page <b>20(25)</b>
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W

# November 13, 2009

# **Frequency Response of H-Field**

(TEM-Cell:ifi110 EXX, Waveguide R22)




Uncertainty of Frequency Response of H-field: ± 6.3% (k=2)

Certificate No: H3-6105\_Nov09

Page 5 of 10


Testing Services™	Annex B to Hearing Aid Report for the BlackBer			Page 21(25)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W

November 13, 2009

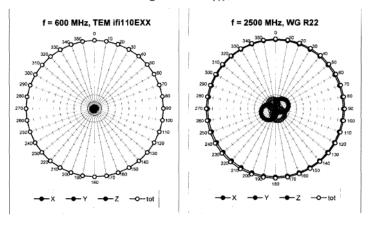

# Receiving Pattern ( $\phi$ ), $\vartheta$ = 90°

Receiving Pattern ( $\phi$ ),  $\vartheta = 0^{\circ}$ 

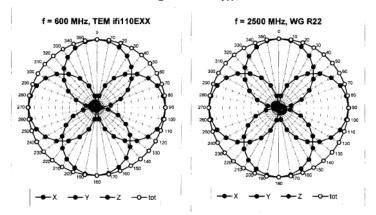

Certificate No: H3-6105\_Nov09

Page 6 of 10


Testing Services™	Annex B to Hearing Aid Report for the BlackBerr			Page <b>22(25)</b>
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W

November 13, 2009

Receiving Pattern ( $\phi$ ),  $\vartheta = 90^{\circ}$ 1.0 0.8 0.6 0.4 0.2 0.0 **13330** -0.2 Error [dB] -750 MHz 网络说会会会说的 - 1800 MHz 4-2500 MHz -0.4 -0.6 -0.8 -1.0 19 7 13 25 31 1 ¢["]

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)



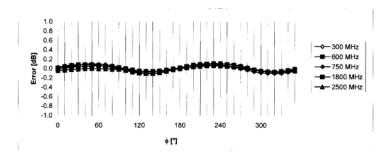


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: H3-6105\_Nov09

Page 7 of 10

Testing Services™		id Compatibility RF Emi erry® Smartphone mode		Page 23(25)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W

November 13, 2009

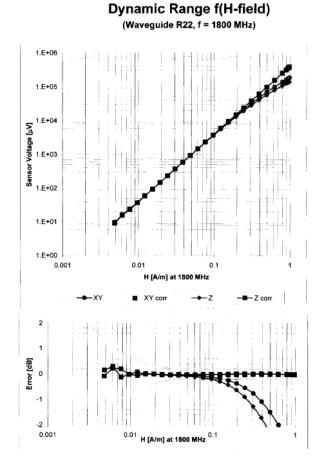


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Certificate No: H3-6105\_Nov09

Page 8 of 10

Testing Services™	Document Annex B to Hearing Aid Report for the BlackBer			Page <b>24(25)</b>
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W

November 13, 2009



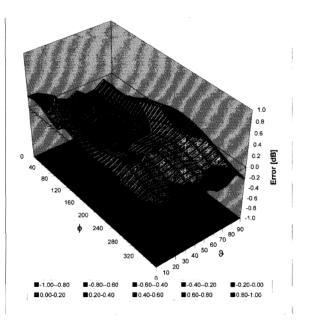

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: H3-6105\_Nov09

Page 9 of 10

Testing Services™	Annex B to Hearing Aid Report for the BlackBerr			Page <b>25(25)</b>
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	April 12-20, 2010	RTS-2671-1005-57	L6ARDB70U	W

### November 13, 2009

# **Other Probe Parameters**

Sensor Arrangement	Rectangular
Connector Angle (°)	-243.0
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	20 mm
Tip Diameter	6.0 mm
Probe Tip to Sensor X Calibration Point	3 mm
Probe Tip to Sensor Y Calibration Point	3 mm
Probe Tip to Sensor Z Calibration Point	3 mm

Certificate No: H3-6105\_Nov09

Page 10 of 10
---------------