Testing Services™	Annex B to Hearing Aid Report for the BlackBer			Page 1(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05,	RTS-2579-1107-18	L6ARDD70U	W
	May 13-16, 2011			

#### Annex B: Probe and dipole description and calibration certificates

# B.1 Probe, measurement chain description, specification and calibration certificate

Testing Services <sup>™</sup>		Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW		Page 2(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

DASY Dosimetric Assessment System by Schmid & Partner Engineering AG

	<u>I</u>
	PIC E-FIELD PROBE FOR GENERAL NEAR-FIELD
Download Produce	<u>ct Flyer</u> (PDF, 192kB)
Construction	One dipole parallel, two dipoles normal to probe axis Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., glycolether)
Calibration	In air from 100 MHz to 3.0 GHz (absolute accuracy ±6.0%, k=2)
Frequency	100 MHz to > 6 GHz; Linearity: $\pm$ 0.2 dB (100 MHz to 3 GHz)
Directivity	± 0.2 dB in air (rotation around probe axis) ± 0.4 dB in air (rotation normal to probe axis)
Dynamic Range	2 V/m to > 1000 V/m; Linearity: ± 0.2 dB
Dimensions	Overall length: 330 mm (Tip: 16 mm) Tip diameter: 8 mm (Body: 12 mm) Distance from probe tip to dipole centers: 2.5 mm
Application	General near-field measurements up to 6 GHz Field component measurements Fast automatic scanning in phantoms
	MEASUREMENTS Download Produ Construction Calibration Frequency Directivity Dynamic Range Dimensions

http://www.dasy4.com/er3.htm

Testing Services™	Annex B to Hearing Aid Report for the BlackBer			Page 3(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05 , May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

DASY Dosimetric Assessment System by Schmid & Partner Engineering AG

DASY Schmid & Partner Engineering AG News Sales Contact		
Applications	H3DV6 3-DIMENSIO	NAL H-FIELD PROBE FOR SMALL BAND
Support & Downloads		
Products	Download Product Fl	<u>yer</u> (PDF, 192kB)
• DASV4 Packages		
EASY4     Probes     ET3DV6 - Isotropic Dos-Probe     ES3DV3 - Isotropic Dos-Probe     EX3DV4 - Isotropic Dos-Probe	Construction	Three concentric loop sensors with 3.8 mm loop diameters Resistively loaded detector diodes for linear response Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., glycolether)
ET1DV3 - D-Probe ER3DV6 - Isotropic E-Probe	Frequency	200 MHz to 3 GHz (absolute accuracy ± 6.0%, k=2); Output linearized
EUV3 - Universal Vector E-Probe	Directivity	± 0.25 dB (spherical isotropy error)
HUV4 - Universal Vector H-Probe	Dynamic Range	10 mA/m to 2 A/m at 1 GHz
T1V3 - Temp-Probe DP1 - Dummy-Probe	E-Field Interference	< 10% at 3 GHz (for plane wave)
Data Acquisition System     Software	Dimensions	Overall length: 330 mm (Tip: 40 mm) Tip diameter: 6 mm (Body: 12 mm) Distance from probe tip to dipole centers: 3 mm
Phantoms     Robots     Validation Kits & Calibration Dipoles     Hearing Aid Compatibility (HAC) Ext     Tissue Simulating Liquids  SPEAG Home	Application	General magnetic near-field measurements up to 3 GHz Field component measurements Surface current measurements Measurements in air or liquids Low interaction with the measured field


Testing Services™	Annex B to Hearing Aid Report for the BlackBerr			Page 4(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05 , May 13-16, 2011	RTS-2579-1107-18	L6ARDD70UW	

All measurements were performed to the nearest element point as per the C63.19 standard. Offset distances were entered in the DASY5 software so that the measurement was to the nearest element.


Figures 1 and 2, provided by the manufacturer, illustrate detail of the probe tip and its dimensions.

**ER3DV6** E-Field probe: The distances from the probe tip to the closest points on the dipole sensors are 1.45mm for X and Y and 1.25mm for Z. From the probe tip to the center of the sensors is 2.5mm.

**H3DV6** H-Field probe: The distance from the probe tip to the closest point of the X, Y and Z loop sensors is 1.1mm. From the probe tip to the center of the sensor is 3.00mm.

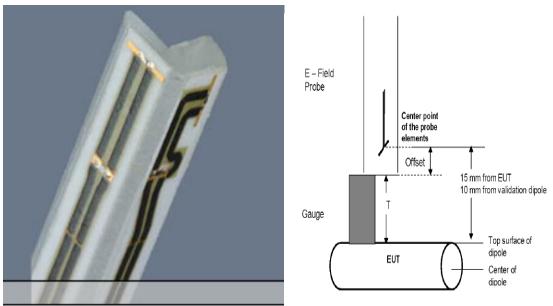

E-Field Probe (ER3DV6)

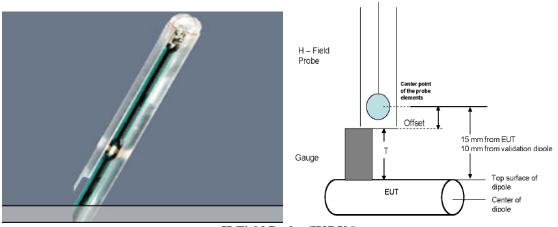

H-Field Probe (H3DV6)

Testing Services™	Document Annex B to Hearing Aid Report for the BlackBer			Page <b>5(24)</b>
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

The following information is from the system manufacturer user manual describing the process chain:

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$
(20.1)

with	$V_i$	= compensated signal of channel i	(i = x, y, z)
	$U_i$	= input signal of channel i	(i = x, y, z)
	cf	= crest factor of exciting field	(DASY parameter)
	$dcp_i$	= diode compression point	(DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

	$\mathrm{E-field probes}$ :	$E_i = \sqrt{\frac{V_i}{Norm_i \cdot C}}$	lonvF
	$\mathbf{H}-\mathbf{fieldprobes}$ :	$H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}}{j}$	$\frac{f + a_{i2}f^2}{f}$
with	= compensated signal of $c$ = sensor sensitivity of cha $\mu V/(V/m)^2$ for E-field = sensitivity enhancement = sensor sensitivity factor = carrier frequency [GHz] = electric field strength of = magnetic field strength	nnel i l Probes t in solution rs for H-field probes f channel i in V/m	$\begin{array}{l} (i=x,y,z) \\ (i=x,y,z) \end{array}$

The RSS value of the field components gives the total field strength (Hermitian magnitude):


$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$
(20.2)

The measurement / integration time per point is > 500 ms, as per the system manufacturer:

The time response of the field probes has been assessed by exposing the probe to a well-controlled field producing signals larger than HAC E- and H-fields of class M4. The signal response time is evaluated as the time required by the system to reach 90% of the expected final value after an on/off switch of the power source with an integration time of 500 ms and a probe response time of <5 ms. In the current implementation, DASY4 waits longer than 100 ms after having reached the grid point before starting a measurement, i.e., the response time uncertainty is negligible.

If the device under test does not emit a CW signal, the integration time applied to measure the electric field at a specific point may introduce additional uncertainties due to the discretization. The tolerances for the different systems had the worst-case of 2.6%.

Ind       Date of Test       Mar. 222-23, Apr. 05, May 13-16, 2011       Rtport No       Rtport No       Rtport No         Calibration Laboratory of Schmid & Partner Engineering AG Zeuphausstrase 43, 804 Zurich, Switzerland       Image: Schwidzerland Schwidzerland       Image: Schwidzerland Schwidzerl	Services <sup>™</sup>	•	Hearing Aid Compa he BlackBerry® Sma		el RDD71UW	6(24
Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzertand       Service suisse d'étalonnage Servizio svitzero di taratura Swiss Calibration Service         Accredited by the Swiss Accreditation Service (SAS)       Accreditation Service is one of the sejnatories to the EA Multilateral Agreement for the recognition of calibration certificates       Accreditation Service is one of the sejnatories to the EA Multilateral Agreement for the recognition of calibration certificates         Client       RTS (RIM Testing Services)       Certificate No: ER-2286_Jan11         Object       ER3DV6 - SN:2286         Calibration procedure(s)       OA CAL-02.V6, OA CAL-25.V3 Calibration procedure for E-field probes optimized for close near field evaluations in air         Calibration date:       January 14, 2011         The taibration schemet swith confidence probability are given on the following pages and are part of the certificate.         Al calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.         Calibration Equipment used (M&TE critical for calibration)         Priver meter E44198       10/10 (2470-1108)         Power sensor E4412A       MY41498087         Ord-Apr-10 (No. 2170-1108)       Apr-11         Power sensor E4412A       MY41498087       01-Apr-10 (No. 2170-1108)       Apr-11         Power sensor E4412A       MY41498087       01-Apr-10 (No. 2170-1108)       Apr-11         Power sensor	Attayi		Apr. 05 , RTS-2	579-1107-18	FCC ID L6ARDD70U	JW
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates         Client       RTS (RIM Testing Services)         Certificate No: ER-2286_Jan11         CALIBRATION CERTIFICATE         Object       ER3DV6 - SN:2286         Calibration procedure(s)       OA CAL-02.v6, QA CAL-25.v8 Calibration procedure for E-field probes optimized for close near field evaluations in air         Calibration date:       January 14, 2011         The calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The resurrements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.         All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.         Calibration Equipment used (M&TE critical for calibration)         Priver sensor E4412A       MY41493087         Ot-oper field 01-Apr-10 (No.217-01138)       Apr-11         Power meter E44198       GB41203874       01-Apr-10 (No.217-01138)       Apr-11         Power sensor E4412A       MY41493087       01-Apr-10 (No.217-01138)       Apr-11         Power meter E44198       GB41203874       01-Apr-10 (No.217-01138)       Apr-11         Power meter E4412A       MY41493087       01-Apr-10 (No.217-01138)       Apr-11	Schmid & Partner Engineering AG		BOC MALA	C Service suisse d'étalo Servizio svizzero di ta	ennage Iratura	
Client       RTS (RIM Testing Services)         Centration No. ER-2286_Jan11             Collect       ER3DV6 - SN:2286             Calibration procedure(s)       QA CAL-02.v6, QA CAL-25.v6         Calibration procedure for E-field probes optimized for close near field evaluations in air             Calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).    The calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).    The calibration shave been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.	The Swiss Accreditation Service is	s one of the signatories to	the EA	ion No.: SCS 108		
Object         ER3DV6 - SN:2286           Calibration procedure(s)         QA CAL-02.v6, QA CAL-25.v3 Calibration procedure for E-field probes optimized for close near field evaluations in air           Calibration date:         January 14, 2011           This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.           All calibration Equipment used (M&TE critical for calibration)           Primary Standards         ID         Cal Date (Certificate No.)         Scheduled Calibration           Power sensor E4412A         MY41495277         01-Apr-10 (No. 217-01136)         Apr-11           Power sensor E4412A         MY41495277         01-Apr-10 (No. 217-01136)         Apr-11           Power sensor E4412A         MY41495277         01-Apr-10 (No. 217-01136)         Apr-11           Power sensor E4412A         MY4149507         01-Apr-10 (No. 217-01136)         Apr-11           Power sensor E4412A         MY4149507 <th></th> <th>and and an an and the line of the second sec</th> <th></th> <th>No: ER-2286_Jan11</th> <th>Stra Ga</th> <th></th>		and and an an and the line of the second sec		No: ER-2286_Jan11	Stra Ga	
Calibration procedure(s)       QA CAL-02.v6, QA CAL-25.v3 Calibration procedure for E-field probes optimized for close near field evaluations in air         Calibration date:       January 14, 2011         This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).         The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.         All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.	CALIBRATION C	RTIFICATE				
Calibration procedure for E-field probes optimized for close near field evaluations in air         Calibration date:       January 14, 2011         This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).         The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.         All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.	Object	ER3DV6 - SN:2286			- 1 .	
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).         The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.         All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.	Calibration procedure(s)	Calibration procedu		ed for close near field		
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.         All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.	Calibration date:	January 14, 2011			<u>N.</u>	
Primary Standards         ID         Cal Date (Certificate No.)         Scheduled Calibration           Power meter E4419B         GB41293874         01-Apr-10 (No. 217-01136)         Apr-11           Power sensor E4412A         MY41495277         01-Apr-10 (No. 217-01136)         Apr-11           Power sensor E4412A         MY41496087         01-Apr-10 (No. 217-01136)         Apr-11           Reference 3 dB Attenuator         SN: S5054 (3c)         30-Mar-10 (No. 217-01159)         Mar-11           Reference 20 dB Attenuator         SN: S5086 (20b)         30-Mar-10 (No. 217-01161)         Mar-11	The measurements and the uncerta	inties with confidence proba	ability are given on the following pages	and are part of the certificate	h.	
Power meter E4419B         GB41293874         01-Apr-10 (No. 217-01136)         Apr-11           Power sensor E4412A         MY41495277         01-Apr-10 (No. 217-01136)         Apr-11           Power sensor E4412A         MY41498087         01-Apr-10 (No. 217-01136)         Apr-11           Power sensor E4412A         MY41498087         01-Apr-10 (No. 217-01136)         Apr-11           Reference 3 dB Attenuator         SN: S5054 (3c)         30-Mar-10 (No. 217-01159)         Mar-11           Reference 20 dB Attenuator         SN: S5086 (20b)         30-Mar-10 (No. 217-01161)         Mar-11	Calibration Equipment used (M&TE	critical for calibration)				
Power sensor E4412A         MY41495277         01-Apr-10 (No. 217-01136)         Apr-11           Power sensor E4412A         MY41498087         01-Apr-10 (No. 217-01136)         Apr-11           Reference 3 dB Attenuator         SN: S5054 (3c)         30-Mar-10 (No. 217-01159)         Mar-11           Reference 20 dB Attenuator         SN: S5086 (20b)         30-Mar-10 (No. 217-01161)         Mar-11	Primary Standards 1	D	Cal Date (Certificate No.)	Scheduled Calibrati	on	
Power sensor E4412A         MY41498087         01-Apr-10 (No. 217-01136)         Apr-11           Reference 3 dB Attenuator         SN: S5054 (3c)         30-Mar-10 (No. 217-01159)         Mar-11           Reference 20 dB Attenuator         SN: S5086 (20b)         30-Mar-10 (No. 217-01161)         Mar-11	Power meter E4419B (	B41293874	01-Apr-10 (No. 217-01136)	Apr-11		
Reference 3 dB Attenuator         SN: S5054 (3c)         30-Mar-10 (No. 217-01159)         Mar-11           Reference 20 dB Attenuator         SN: S5086 (20b)         30-Mar-10 (No. 217-01161)         Mar-11						
Reference 20 dB Attenuator         SN: S5086 (20b)         30-Mar-10 (No. 217-01161)         Mar-11						
Reference Probe ER3DV6         SN: 2328         4-Oct-10 (No. ER3-2328_Oct10)         Oct-11						
DAE4 SN: 789 31-Aug-10 (No. DAE4-789_Aug10) Aug-11	DAE4	in: 789	31-Aug-10 (No. DAE4-789_Aug10	0) Aug-11		
Secondary Standards ID Charle Date (is house) Setendariant Charle	Socondary Standarda	0	Chook Data (in house)	Schodulad ChrI-		
Secondary Standards         ID         Check Date (in house)         Scheduled Check           RF generator HP 8648C         US3642U01700         4-Aug-99 (in house check Oct-09)         In house check: Oct-11					-11	
Network Analyzer HP 8753E US37390585 18-Oct-01 (in house check Oct-10) In house check. Oct-11						
Name         Function         Signature           Calibrated by:         Marcel Fehr         Laboratory Technician	Calibrated by:	and here a many trace of the second s	and the second sec	Signature		
	Approved by:	Katja Pokovic	Technical Manager	R	EL.	
				Issued: January 1	5 2011	
	This calibration certificate shall not	e reproduced except in full	without written approval of the laborat		5, 2011	



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

s

С

s

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

olooda ji	
NORMx,y,z	sensitivity in free space
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization 9	9 rotation around an axis that is in the plane normal to probe axis (at measurement center),
	i.e., $9 = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

#### Calibration is Performed According to the Following Standards:

 IEEE Std 1309-2005, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", December 2005.

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 for XY sensors and 9 = 90 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart).
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z; Bx,y,z; Cx,y,z, VRx,y,z: A, B, C are numerical linearization parameters assessed based on the data of
  power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
  maximum calibration range expressed in RMS voltage across the diode.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: ER-2286\_Jan11

Page 2 of 10

Testing Services <sup>™</sup>	Annex B to Hearing Aid Report for the BlackBe			Page 8(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

ER3DV6 - SN:2286

January 14, 2011

# Probe ER3DV6

# SN:2286

Manufactured: September 18, 2002 Calibrated: January 14, 2011

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: ER-2286\_Jan11

Page 3 of 10

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW			Page 9(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05 , May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

ER3DV6- SN:2286

January 14, 2011

#### DASY/EASY - Parameters of Probe: ER3DV6 - SN:2286

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)$	2.23	1.48	1.51	± 10.1 %
DCP (mV) <sup>B</sup>	97.6	98.4	97.6	

#### **Modulation Calibration Parameters**

UID	Communication System Name	PAR		A dB	B dB	C dB	VR mV	Unc <sup>E</sup> (k=2)
10000	CW	0.00	Х	0.00	0.00	1.00	179.3	±3.0 %
			Y	0.00	0.00	1.00	145.0	
			Z	0.00	0.00	1.00	180.1	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>8</sup> Numerical linearization parameter: uncertainty not required. <sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: ER-2286\_Jan11


Page 4 of 10

Testing Services™	Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW		Page 10(24)	
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

ER3DV6-- SN:2286

January 14, 2011

# Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

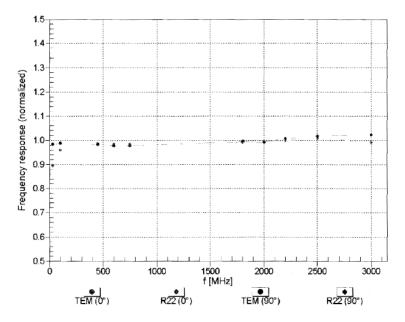

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: ER-2286\_Jan11


Page 5 of 10

Testing Services™	Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW			Page 11(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

ER3DV6-- SN:2286

January 14, 2011

# Fe600 MHz,TEM,0° f=2500 MHz,R22,0° 135

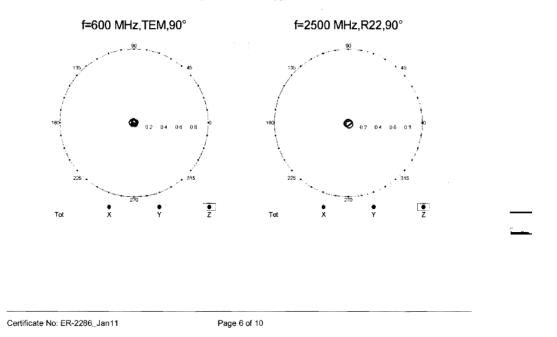


Testing Services <sup>**</sup>	Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW			Page 12(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, RTS-2579-1107-18 L6ARDD70UV May 13-16, 2011			W

ER3DV6- SN:2286


January 14, 2011

Receiving Pattern ( $\phi$ ),  $\vartheta = 0^{\circ}$ 

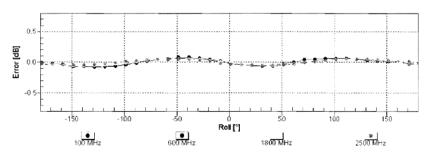

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Receiving Pattern ( $\phi$ ),  $\vartheta = 90^{\circ}$ 

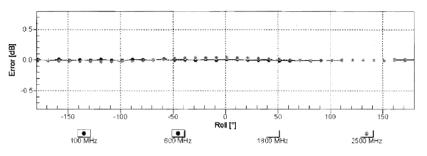

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Certificate No: ER-2286\_Jan11

Page 7 of 10

Testing Services™	Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW			Page 13(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

ER3DV6-- SN:2286

January 14, 2011

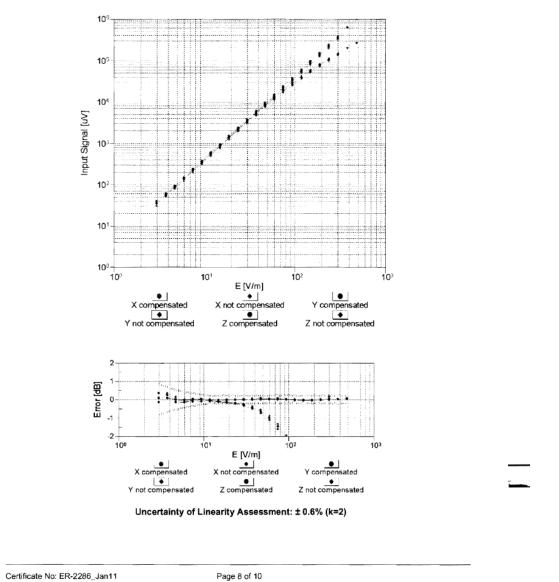


## Dynamic Range f(E-field) (TEM cell , f = 900 MHz)

Testing Services™	Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW			Page 14(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

ER3DV6- SN:2286

January 14, 2011

#### Deviation from Isotropy in Air Error (\, \,), f = 900 MHz

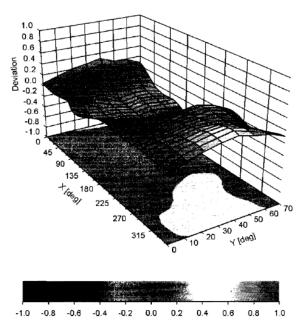

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ER-2286\_Jan11

Page 9 of 10



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW Page

Author Data	Dates of Test	Report No	FCC ID
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70UW

Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



SWISS S Schweizer C Service su Service su Swiss Call

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilataral Agreement for the recognition of calibration certificates

Client Rill


Certificate No: H3-6105\_Nov10

H3DV6 - SN:6105
QA CAL-03.v5, QA CAL-25.v2 Calibration procedure for H-field probes optimized for close near field evaluations in air
November 18, 2010
nts the traceability to national standards, which realize the physical units of measurements (St), aunties with confidence probability are given on the following pages and are part of the cartificate.
ed in the closed laboratory facility; environment temperature (22 $\pm$ 3)°C and humidity < 70%
E critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E44198	GB41293874	10-Apr-10 (No. 217-01136)	Apr-11
Power sensor E4412A	MY41495277	10-Apr-10 (No. 217-01136)	Apr-11
Power sensor E4412A	MY41498087	10-Apr-10 (No. 217-01136)	Apr-11
Reference 3 dB Attenuator	SN: S5054 (3c)	30-Mar-10 (No. 217-01159)	Mar-11
Reference 20 dB Allenuator	SN: \$5086 (20b)	3D-Mar-10 (No. 217-01161)	Mar-11
Reference 30 dB Altenuator	SN: S5129 (30b)	30-Mar-10 (No. 217-01160)	Mar-11
Reference Probe H3OV6	SN: 6182	4-Oct-10 (No. H3-6182_Oct10)	Oct-11
DAE4	<u>SN: 769</u>	31-Aug-10 (No. DAE4-789_Aug10)	Aug-11
Secondary Standarda	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-10)	In house check. Oct-11

Calibrated by:	Name Jeoin Késini	Function <b>Laboratory Technician</b>	Signature
Conternet by			fela
Approved by:	Katja Pokovic	Technical Manager	Lela
			Issued: November 19, 2010
This calibration certificat	e shall not be reproduced except in full	without written approval of the laborato	ry

Certificate No: H3-6105\_Nov10



Page

Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



- SHISS C C Z R JOR NT
- S Schweizerischer Kalibrierdienst
- C Service sulsse d'étalonnage
- S Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

NORMx.y.z	sensitivity in free space
DCP	diode compression point
ÇF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization o	o rotation around probe axis
Polarization 3	9 rotation around an axis that is in the plane normal to probe axis (at measurement center),
	i.e., $9 = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

#### Calibration is Performed According to the Following Standards:

 a) IEEE Std 1309-2005, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", December 2005.

#### Methods Applied and Interpretation of Parameters:

- NORMx.y.z: Assessed for E-field polarization 9 = 0 for XY sensors and 9 = 90 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz; R22 waveguide).
- X, Y,Z(f)\_a0a1a2= X, Y,Z\_a0a1a2\* frequency\_response (see Frequency Response Chart).
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z: Bx,y,z; Cx,y,z, VRx,y,z: A, B, C are numerical linearization parameters assessed based on the data of
  power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
  maximum calibration range expressed in RMS voltage across the diode.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the X\_a0a1a2 (no uncertainty required).

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW			Page 17(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

H3DV6 - SN:6105

November 16, 2010

# Probe H3DV6

# SN:6105

Manufactured: January 5, 2002 Calibrated: November 18, 2010

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Testing Services™	Annex B to Hearing Aid Report for the BlackBe			Page 18(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

H30V6- SN:6105

November 18, 2010

#### DASY/EASY - Parameters of Probe: H3DV6 - SN:6105

#### **Basic Calibration Parameters**

		Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (A/m / √(mV))	a0	2.94E-003	2.71E-003	3.01E-003	± 5.1 %
Norm (A/m / √(mV))	a1	2.83E-005	2.25E-005	-8.45E-005	± 5.1 %
Norm (A/m / $\sqrt{(mV)}$ )	a2	-1.08E-005	2.19E-006	5.51E-005	±5.1%
DCP (mV) <sup>e</sup>		90.4	91.6	92.6	

#### **Modulation Calibration Parameters**

ŪID	Communication System Name	PAR	ļ	A dB	BdB	C dB	VR mV	Unc <sup>E</sup> (k=2)
10000	CW	0.00	X	Q.00	0.00	1.00	211.2	+2.96 %
			Y	0.00	0.00	1.00	233.0	
			z	0.00	0.00	1.00	239.4	

<sup>E</sup> Numerical linearization parameter, uncertainty not required <sup>E</sup> Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.


The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW			Page 19(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

H3DV6- SN:6105

November 18, 2010

# Frequency Response of H-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

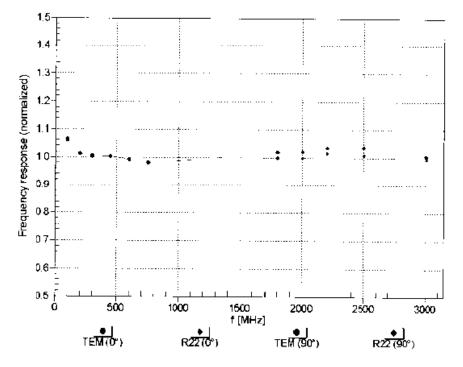

Uncertainty of Frequency Response of H-field: ± 6.3% (k=2)


Certificate No: H3-6105 Nov10


Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW			Page <b>20(24)</b>
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05 , May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

H3DV6-- SN:6105


November 18, 2010

## Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

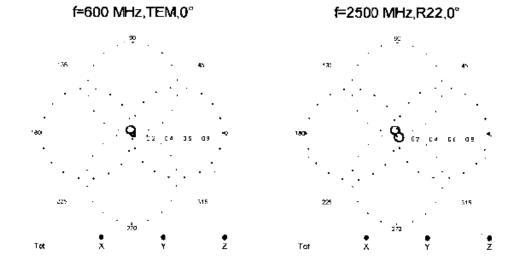



f=2500 MHz,R22,90°




Testing Services™	Annex B to Hearing Aid Report for the BlackBerr			Page 21(24)
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05 , May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

H3DV6- SN:6105


November 18, 2010


## Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

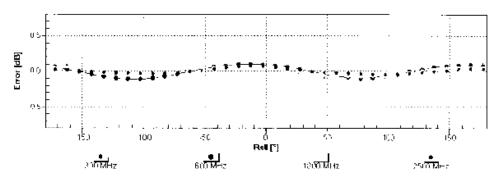

Uncertainty of Axiał Isotropy Assessment: ± 0.5% (k=2)

## Receiving Pattern ( $\phi$ ), $\vartheta$ = 90°

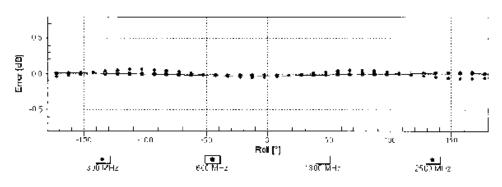




- -

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW			Page <b>22(24)</b>
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, May 13-16, 2011	RTS-2579-1107-18	L6ARDD70U	W

H3DV6- SN:6105

November 18, 2010

#### Dynamic Range f(H-field) (TEM cell, f = 900 MHz)

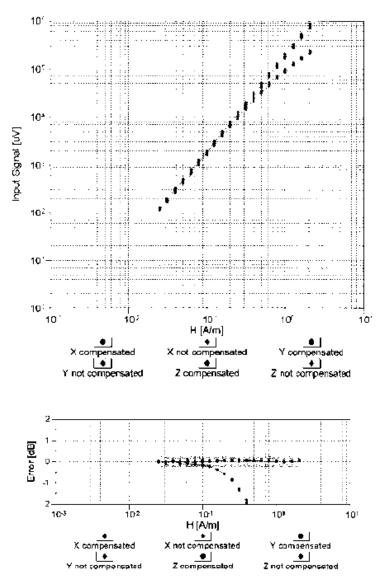


Uncertainty of Linearity Assessment: ±0.6% (k=2)


Page 8 of 10

Testing Services™		Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDD71UW		
Author Data	Dates of Test	Report No	FCC ID	
Daoud Attayi	Mar. 22-23, Apr. 05, RTS-2579-1107-18 L6ARDD70U			W
	May 13-16, 2011			

H3DV6- \$N:6105

November 18, 2010




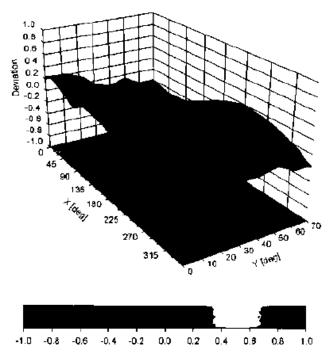

Uncertainty of Spherical Isotropy Assessment: ± 2.5% (k=2)

Certificate No: H3-6105\_Nov10

Page 9 of 10



H3DV6-- SN:6105

November 18, 2010

#### DASY/EASY - Parameters of Probe: H3DV6 - SN:6105

#### Other Probe Parameters

Sensor Arrangement	Rectangular
Connector Angle (*)	-62.8
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	
Probe Body Diameter	
Tip Length	20 mm
Tip Diameter	
Probe Tip to Sensor X Calibration Point	
Probe Tip to Sensor Y Calibration Point	
Probe Tip to Sensor Z Calibration Point	3 mm