| Testing<br>Services™ | Appendix D for the BlackB<br>SAR Report | Serry® Smartphone Mod | el RDD71UW | Page <b>1(36)</b> |
|----------------------|---|-----------------------|------------|-------------------|
| Author Data          | Dates of Test                           | Test Report No        | FCC ID:    | IC ID             |
| Andrew Becker        | Apr 13 – June 16, 2011                  | RTS-2579-1106-34      | L6ARDD70UW | 2503A-RDD70UW     |

### APPENDIX D: PROBE & DIPOLE CALIBRATION DATA



## Calibration Laboratory of

Schmid & Partner Engineering AG





Schweizerlscher Kalibrierdienst Service suisse d'étalonnage С Servizio svizzero di taratura S Swiss Calibration Service

Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

RTS (RIM Testing Services) Client

Certificate No: ES3-3225\_Jan11

Accreditation No.: SCS 108

#### CALIBRATION CERTIFICATE ES3DV3 - SN:3225 Object QA CAL-01.v7, QA CAL-23.v4 and QA CAL-25.v3 Calibration procedure(s) Calibration procedure for dosimetric E-field probes Calibration date: January 13, 2011 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI), The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%, Calibration Equipment used (M&TE critical for calibration) Primary Standards ID# Cal Date (Certificate No.) Scheduled Calibration Power meter E4419B GB41293874 1-Apr-10 (No. 217-01136) Apr-11 Power sensor E4412A MY41495277 1-Apr-10 (No. 217-01136) Apr-11 MY41498087 Power sensor E4412A 1-Apr-10 (No. 217-01136) Apr-11 Reference 3 dB Attenuator SN: S5054 (3c) 30-Mar-10 (No. 217-01159) Reference 20 dB Attenuator SN: S5086 (20b) 30-Mar-10 (No. 217-01161) Mar-11 Reference 30 dB Attenuator SN: S5129 (30b) 30-Mar-10 (No. 217-01160) Mar-11 Reference Probe ES3DV2 SN: 3013 29-Dec-10 (No. ES3-3013\_Dec10) Dec-11 DAE4 SN: 660 20-Apr-10 (No. DAE4-660\_Apr10) Apr-11 ID# Check Date (in house) Secondary Standards Scheduled Check US3642U01700 RF generator HP 8648C 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 18-Oct-01 (in house check Oct-10) In house check: Oct-11 Function Signature Calibrated by: Approved by: Technical Manager Issued: January 15, 2011 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ES3-3225\_ Jan11

Page 1 of 11

| Testing Services™ | Appendix D for the Black<br>SAR Report | kBerry® Smartphone Mo | odel RDD71UW | Page 3(36)    |
|-------------------|--|-----------------------|--------------|---------------|
| Author Data       | Dates of Test                          | Test Report No        | FCC ID:      | IC ID         |
| Andrew Becker     | Apr 13 – June 16, 2011                 | RTS-2579-1106-34      | L6ARDD70UW   | 2503A-RDD70UW |

## Calibration Laboratory of





С

Schweizerischer Kalibrierdienst s

Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

tissue simulating liquid TSL NORMx,y,z sensitivity in free space sensitivity in TSL / NORMx,v,z ConvF DCP diode compression point

CF crest factor (1/duty\_cycle) of the RF signal A, B, C modulation dependent linearization parameters

Polarization e φ rotation around probe axis

9 rotation around an axis that is in the plane normal to probe axis (at measurement center), Polarization 9

i.e., 9 = 0 is normal to probe axis

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices; Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E2-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z; Bx,y,z; Cx,y,z, VRx,y,z; A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f 

  800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

| Codificate No: ES2 2225 Jan11 | Page 7 of 11 |
|-------------------------------|--------------|

| Testing<br>Services™ | Appendix D for the BlackB<br>SAR Report | serry® Smartphone Mod | lel RDD71UW | Page <b>4(36)</b> |
|----------------------|---|-----------------------|-------------|-------------------|
| Author Data          | Dates of Test                           | Test Report No        | FCC ID:     | IC ID             |
| Andrew Becker        | Apr 13 – June 16, 2011                  | RTS-2579-1106-34      | L6ARDD70UW  | 2503A-RDD70UW     |

# Probe ES3DV3

SN:3225

Manufactured: September 1, 2009 Last calibrated: December 11, 2009 Recalibrated: January 13, 2011

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

| Testing Services™ | Appendix D for the Black<br>SAR Report | Berry® Smartphone Mo | del RDD71UW | Page <b>5(36)</b> |
|-------------------|--|----------------------|-------------|-------------------|
| Author Data       | Dates of Test                          | Test Report No       | FCC ID:     | IC ID             |
| Andrew Becker     | Apr 13 – June 16, 2011                 | RTS-2579-1106-34     | L6ARDD70UW  | 2503A-RDD70UW     |

### DASY/EASY - Parameters of Probe: ES3DV3 SN:3225

#### **Basic Calibration Parameters**

|  | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|--|----------|----------|----------|-----------|
| Norm (µV/(V/m) <sup>2</sup> ) <sup>A</sup> | 1.26     | 1.21     | 1.31     | ± 10.1%   |
| DCP (mV) <sup>8</sup>                      | 102.1    | 100.8    | 99.1     |           |

#### **Modulation Calibration Parameters**

| UID   | Communication System Name | PAR  |   | A<br>dB | B<br>dBuV | С    | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-------|---------------------------|------|---|---------|-----------|------|----------|---------------------------|
| 10000 | cw                        | 0.00 | × | 0.00    | 0.00      | 1.00 | 149.8    | ± 2.6 %                   |
|       |                           |      | Υ | 0.00    | 0.00      | 1.00 | 148.1    |                           |
|       |                           |      | Z | 0.00    | 0.00      | 1.00 | 110.7    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: ES3-3225\_Jan11

<sup>&</sup>lt;sup>a</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>&</sup>lt;sup>8</sup> Numerical linearization parameter, uncertainty not required.

<sup>&</sup>lt;sup>6</sup> Uncertainty is determined using the maximum deviation from linear response applying recatangular distribution and is expressed for the square of the field value.

| Testing<br>Services™ | Appendix D for the BlackB<br>SAR Report | erry® Smartphone Mod | lel RDD71UW | Page <b>6(36)</b> |
|----------------------|---|----------------------|-------------|-------------------|
| Author Data          | Dates of Test                           | Test Report No       | FCC ID:     | IC ID             |
| Andrew Becker        | Apr 13 – June 16, 2011                  | RTS-2579-1106-34     | L6ARDD70UW  | 2503A-RDD70UW     |

ES3DV3 SN:3225

January 13, 2011

## DASY/EASY - Parameters of Probe: ES3DV3 SN:3225

### Calibration Parameter Determined in Head Tissue Simulating Media

| f [MHz] | Validity [MHz] <sup>C</sup> | Permittivity   | Conductivity   | ConvF X Co | nvFY Cor | vF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|----------------|----------------|------------|----------|------|-------|-----------------|
| 750     | ±50/±100                    | $41.9 \pm 5\%$ | $0.89 \pm 5\%$ | 6.47       | 6.47     | 6.47 | 0.89  | 1.08 ± 11.0%    |
| 900     | ± 50 / ± 100                | 41.5 ± 5%      | 0.97 ± 5%      | 6.11       | 6.11     | 6.11 | 0.81  | 1.10 ± 11.0%    |
| 1810    | ± 50 / ± 100                | 40.0 ± 5%      | $1.40 \pm 5\%$ | 5.26       | 5.26     | 5.26 | 0.37  | 1.68 ± 11.0%    |
| 1950    | ±50/±100                    | $40.0\pm5\%$   | $1.40 \pm 5\%$ | 4.98       | 4.98     | 4.98 | 0.48  | 1.51 ± 11.0%    |
| 2450    | ±50/±100                    | 39.2 ± 5%      | 1.80 ± 5%      | 4.60       | 4.60     | 4.60 | 0.52  | 1.54 ± 11.0%    |
| 2600    | $\pm 50 / \pm 100$          | $39.0\pm5\%$   | 1.96 ± 5%      | 4.52       | 4.52     | 4.52 | 0.53  | 1.58 ± 11.0%    |

<sup>&</sup>lt;sup>C</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

| Testing<br>Services™ | Appendix D for the Black! SAR Report | Berry® Smartphone Mod | lel RDD71UW | Page <b>7(36)</b> |
|----------------------|--------------------------------------|-----------------------|-------------|-------------------|
| Author Data          | Dates of Test                        | Test Report No        | FCC ID:     | IC ID             |
| Andrew Becker        | Apr 13 – June 16, 2011               | RTS-2579-1106-34      | L6ARDD70UW  | 2503A-RDD70UW     |

ES3DV3 SN:3225

January 13, 2011

### DASY/EASY - Parameters of Probe: ES3DV3 SN:3225

### Calibration Parameter Determined in Body Tissue Simulating Media


| f [MHz] | Validity [MHz] <sup>C</sup> | Permittivity   | Conductivity   | ConvF X Co | nvFY_C | onvF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|----------------|----------------|------------|--------|--------|-------|-----------------|
| 750     | ±50/±100                    | $55.5 \pm 5\%$ | $0.96 \pm 5\%$ | 6.30       | 6.30   | 6.30   | 0.76  | 1.17 ± 11.0%    |
| 900     | ±50/±100                    | $55.0\pm5\%$   | 1.05 ± 5%      | 6.12       | 6.12   | 6.12   | 0.72  | 1.20 ± 11.0%    |
| 1810    | ±50/±100                    | 53.3 ± 5%      | 1.52 ± 5%      | 4.88       | 4.88   | 4.88   | 0.26  | 2.70 ± 11.0%    |
| 1950    | ±50/±100                    | $53.3 \pm 5\%$ | 1.52 ± 5%      | 4.89       | 4.89   | 4.89   | 0.33  | 2.28 ± 11.0%    |
| 2450    | ± 50 / ± 100                | 52.7 ± 5%      | $1.95 \pm 5\%$ | 4.43       | 4.43   | 4.43   | 0.99  | 1.04 ± 11.0%    |
| 2600    | ±50/±100                    | 52.5 ± 5%      | 2.16 ± 5%      | 4.29       | 4.29   | 4.29   | 0.99  | 1.05 ± 11.0%    |

The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

| Testing Services | Appendix D for the Black<br>SAR Report | xBerry® Smartphone Mo | odel RDD71UW | Page <b>8(36)</b> |
|------------------|--|-----------------------|--------------|-------------------|
| Author Data      | Dates of Test                          | Test Report No        | FCC ID:      | IC ID             |
| Andrew Becker    | Apr 13 – June 16, 2011                 | RTS-2579-1106-34      | L6ARDD70UW   | 2503A-RDD70UW     |

## Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

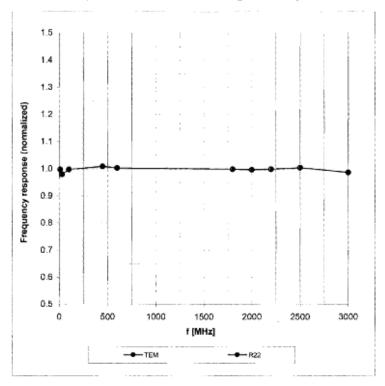


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

| Testing<br>Services™ |                        |                  | Page <b>9(36)</b> |               |
|----------------------|------------------------|------------------|-------------------|---------------|
| Author Data          | Dates of Test          | Test Report No   | FCC ID:           | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW        | 2503A-RDD70UW |

## Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

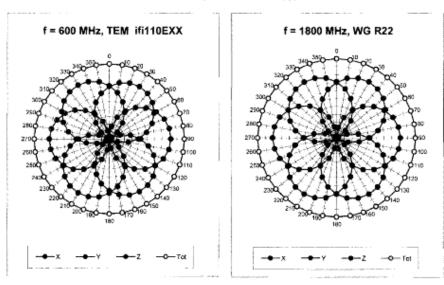

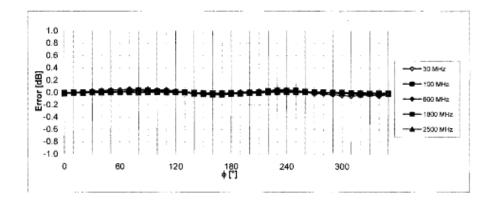



Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

| Testing Services™ | Appendix D for the BlackBerry® Smartphone Model RDD71UW SAR Report |                  |            | Page<br>10(36) |
|-------------------|--|------------------|------------|----------------|
| Author Data       | Dates of Test  | Test Report No   | FCC ID:    | IC ID          |
| Andrew Becker     | Apr 13 – June 16, 2011   | RTS-2579-1106-34 | L6ARDD70UW | 2503A-RDD70UW  |

## Dynamic Range f(SAR<sub>head</sub>)

(TEM cell, f = 900 MHz)

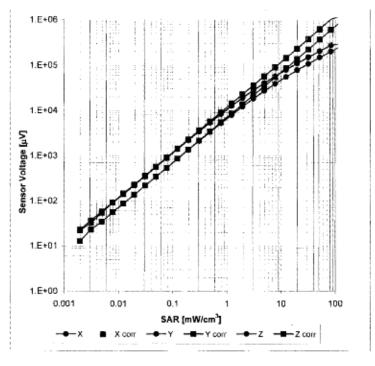


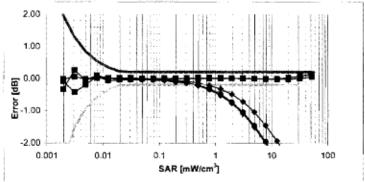


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

| Testing<br>Services™ |                               |                  |            | Page 11(36)   |
|----------------------|-------------------------------|------------------|------------|---------------|
| Author Data          | Dates of Test                 | Test Report No   | FCC ID:    | IC ID         |
| Andrew Becker        | <b>Apr 13 – June 16, 2011</b> | RTS-2579-1106-34 | L6ARDD70UW | 2503A-RDD70UW |


## **Conversion Factor Assessment**





## Deviation from Isotropy in HSL

Error (\$\phi\$, \$\text{3}), f = 900 MHz

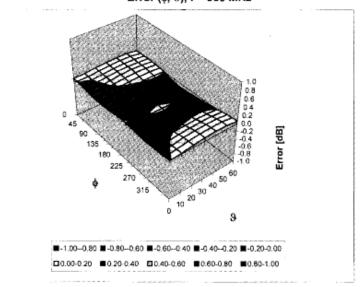

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)


Certificate No: ES3-3225\_Jan11

Page 10 of 11

| Testing Services™ |                        |                  | Page 12(36) |               |
|-------------------|------------------------|------------------|-------------|---------------|
| Author Data       | Dates of Test          | Test Report No   | FCC ID:     | IC ID         |
| Andrew Becker     | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW  | 2503A-RDD70UW |

### Other Probe Parameters

| Sensor Arrangement                            | Triangular     |
|---|----------------|
| Connector Angle (°)                           | Not applicable |
| Mechanical Surface Detection Mode             | enabled        |
| Optical Surface Detection Mode                | disabled       |
| Probe Overall Length                          | 337 mm         |
| Probe Body Diameter                           | 10 mm          |
| Tip Length                                    | 10 mm          |
| Tip Diameter                                  | 4 mm           |
| Probe Tip to Sensor X Calibration Point       | 2 mm           |
| Probe Tip to Sensor Y Calibration Point       | 2 mm           |
| Probe Tip to Sensor Z Calibration Point       | 2 mm           |
| Recommended Measurement Distance from Surface | 3 mm           |



#### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kallbrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client RTS (RIM Testing Services) Certificate No: D835V2-446\_Jan11

#### CALIBRATION CERTIFICATE D835V2 - SN: 446 Object Calibration procedure(s) QA CAL-05.v8 Calibration procedure for dipole validation kits Calibration date: January 21, 2011 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70% Calibration Equipment used (M&TE critical for calibration) Primary Standards ID# Cal Date (Certificate No.) Scheduled Calibration Power meter EPM-442A GB37480704 06-Oct-10 (No. 217-01266) Oct-11 Power sensor HP 8481A US37292783 06-Oct-10 (No. 217-01266) Oct-11 Reference 20 dB Attenuator SN: 5086 (20g) 30-Mar-10 (No. 217-01158) Mar-11 Type-N mismatch combination SN: 5047.2 / 06327 30-Mar-10 (No. 217-01162) Mar-11 Reference Probe ES3DV3 SN: 3205 30-Apr-10 (No. ES3-3205\_Apr10) Apr-11 DAE4 SN: 601 10-Jun-10 (No. DAE4-601\_Jun10) Jun-11 Secondary Standards ID# Check Date (in house) Scheduled Check Power sensor HP 8481A MY41092317 18-Oct-02 (in house check Oct-09) In house check: Oct-11 RF generator R&S SMT-06 100005 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 S4206 18-Oct-01 (in house check Oct-10) In house check: Oct-11 Name Function Calibrated by: Approved by: Issued: January 21, 2011 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D835V2-446\_Jan11

Page 1 of 6

| Testing Services™ | Appendix D for the Black SAR Report | Berry® Smartphone Mo | del RDD71UW | Page <b>14(36)</b> |
|-------------------|-------------------------------------|----------------------|-------------|--------------------|
| Author Data       | Dates of Test                       | Test Report No       | FCC ID:     | IC ID              |
| Andrew Becker     | Apr 13 – June 16, 2011              | RTS-2579-1106-34     | L6ARDD70UW  | 2503A-RDD70UW      |

#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Service suisse d etatonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossarv:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

| Certificate No: D835V2-446_Jan11 | Page 2 of 6 |  |
|----------------------------------|-------------|--|

| Testing Services™ |                        |                  |            | Page<br>15(36) |
|-------------------|------------------------|------------------|------------|----------------|
| Author Data       | Dates of Test          | Test Report No   | FCC ID:    | IC ID          |
| Andrew Becker     | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW | 2503A-RDD70UW  |

### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

| DASY Version                 | DASY5                     | V52.6       |
|------------------------------|---------------------------|-------------|
| Extrapolation                | Advanced Extrapolation    |             |
| Phantom                      | Modular Flat Phantom V4.9 |             |
| Distance Dipole Center - TSL | 15 mm                     | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm         |             |
| Frequency                    | 835 MHz ± 1 MHz           |             |

### Head TSL parameters

The following parameters and calculations were applied.

|                                  | Temperature     | Permittivity | Conductivity     |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters      | 22.0 °C         | 41.5         | 0.90 mho/m       |
| Measured Head TSL parameters     | (22.0 ± 0.2) °C | 41.3 ± 6 %   | 0.89 mho/m ± 6 % |
| Head TSL temperature during test | (21.8 ± 0.2) °C |              |                  |

#### SAR result with Head TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                           |
|---|--------------------|---------------------------|
| SAR measured  | 250 mW input power | 2.39 mW / g               |
| SAR normalized  | normalized to 1W   | 9.56 mW / g               |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 9.63 mW /g ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                           |
|---|--------------------|---------------------------|
| SAR measured  | 250 mW input power | 1.56 mW / g               |
| SAR normalized  | normalized to 1W   | 6.24 mW / g               |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 6.27 mW /g ± 16.5 % (k=2) |

| Testing<br>Services™ |                        |                  | Page<br>16(36) |               |
|----------------------|------------------------|------------------|----------------|---------------|
| Author Data          | Dates of Test          | Test Report No   | FCC ID:        | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW     | 2503A-RDD70UW |

#### Appendix

### Antenna Parameters with Head TSL

| Impedance, transformed to feed point | 49.6 Ω - 7.7 jΩ |
|--------------------------------------|-----------------|
| Return Loss                          | - 22.2 dB       |

### General Antenna Parameters and Design

| Electrical Delay (one direction) | 1.386 ns |
|----------------------------------|----------|
|                                  |          |

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

| Manufactured by | SPEAG            |
|-----------------|------------------|
| Manufactured on | October 24, 2001 |

Certificate No: D835V2-446\_Jan11

| Testing<br>Services™ | Appendix D for the BlackE<br>SAR Report | Berry® Smartphone Mod | lel RDD71UW | Page <b>17(36)</b> |
|----------------------|---|-----------------------|-------------|--------------------|
| Author Data          | Dates of Test                           | Test Report No        | FCC ID:     | IC ID              |
| Andrew Becker        | Apr 13 – June 16, 2011                  | RTS-2579-1106-34      | L6ARDD70UW  | 2503A-RDD70UW      |

#### **DASY5 Validation Report for Head TSL**

Date/Time: 21.01.2011 10:18:05

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:446

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL900

Medium parameters used: f = 835 MHz;  $\sigma = 0.89$  mho/m;  $\varepsilon_r = 41.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY5 Configuration:

Probe: ES3DV3 - SN3205; ConvF(6.03, 6.03, 6.03); Calibrated: 30.04.2010

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 10.06.2010

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

Measurement SW: DASY52, V52.6.1 Build (408)

Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)


#### Pin=250 mW /d=15mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement

grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.426 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 3.600 W/kg

SAR(1 g) = 2.39 mW/g; SAR(10 g) = 1.56 mW/gMaximum value of SAR (measured) = 2.790 mW/g

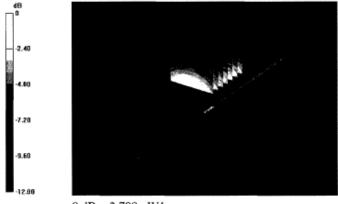



0 dB = 2.790 mW/g

Certificate No: D835V2-446\_Jan11

| Testing<br>Services™ |                               |                | Page 18(36) |       |
|----------------------|-------------------------------|----------------|-------------|-------|
| Author Data          | Dates of Test                 | Test Report No | FCC ID:     | IC ID |
| Andrew Becker        | <b>Apr 13 – June 16, 2011</b> | T              |             |       |

### Impedance Measurement Plot for Head TSL

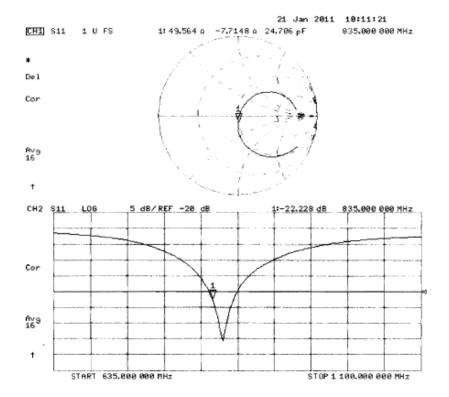



#### Calibration Laboratory of Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage С Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Certificate No: D1800V2-2d020 Jan11 Client RTS (RIM Testing Services)

#### CALIBRATION CERTIFICATE D1800V2 - SN: 2d020 Object QA CAL-05.v8 Calibration procedure(s) Calibration procedure for dipole validation kits January 13, 2011 Calibration date: This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID# Cal Date (Certificate No.) Scheduled Calibration GB37480704 06-Oct-10 (No. 217-01266) Power meter EPM-442A Oct-11 Power sensor HP 8481A US37292783 06-Oct-10 (No. 217-01266) Oct-11 Reference 20 dB Attenuator SN: 5086 (20g) 30-Mar-10 (No. 217-01158) Mar-11 Type-N mismatch combination SN: 5047.2 / 06327 30-Mar-10 (No. 217-01162) Mar-11 SN: 3205 Reference Probe ES3DV3 30-Apr-10 (No. ES3-3205\_Apr10) Apr-11 SN: 601 10-Jun-10 (No. DAE4-601\_Jun10) Jun-11 Secondary Standards ID# Check Date (in house) Scheduled Check Power sensor HP 8481A MY41092317 18-Oct-02 (in house check Oct-09) In house check: Oct-11 RF generator R&S SMT-06 100005 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 S4206 18-Oct-01 (in house check Oct-10) In house check: Oct-11 Name Function Signature Calibrated by: Approved by: Katia Pokovic Issued: January 13, 2011 This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: D1800V2-2d020\_Jan11

Page 1 of 6

| Testing<br>Services™ | Appendix D for the BlackBerry® Smartphone Model RDD71UW SAR Report |                  | Page <b>20(36)</b> |               |
|----------------------|--|------------------|--------------------|---------------|
| Author Data          | Dates of Test  | Test Report No   | FCC ID:            | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011   | RTS-2579-1106-34 | L6ARDD70UW         | 2503A-RDD70UW |

#### Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

| Certificate No: D1800V2-2d020_Jan11 | Page 2 of 6 |  |
|-------------------------------------|-------------|--|

| Testing<br>Services™ |                        |                  | Page <b>21</b> (36) |               |
|----------------------|------------------------|------------------|---------------------|---------------|
| Author Data          | Dates of Test          | Test Report No   | FCC ID:             | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW          | 2503A-RDD70UW |

#### Measurement Conditions

DASY system configuration, as far as not given on page 1.

| DASY5                     | V52.6   |
|---------------------------|---|
| Advanced Extrapolation    |   |
| Modular Flat Phantom V5.0 |   |
| 10 mm                     | with Spacer   |
| dx, dy, dz = 5 mm         |   |
| 1800 MHz ± 1 MHz          |   |
|                           | Advanced Extrapolation  Modular Flat Phantom V5.0  10 mm  dx, dy, dz = 5 mm |

### Head TSL parameters

The following parameters and calculations were applied.

|                                  | Temperature     | Permittivity | Conductivity     |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters      | 22.0 °C         | 40.0         | 1.40 mho/m       |
| Measured Head TSL parameters     | (22.0 ± 0.2) °C | 38.6 ± 6 %   | 1.38 mho/m ± 6 % |
| Head TSL temperature during test | (21.3 ± 0.2) °C |              | ****             |

### SAR result with Head TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                           |
|---|--------------------|---------------------------|
| SAR measured  | 250 mW input power | 9.78 mW / g               |
| SAR normalized  | normalized to 1W   | 39.1 mW / g               |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 39.2 mW /g ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                           |
|---|--------------------|---------------------------|
| SAR measured  | 250 mW input power | 5.13 mW / g               |
| SAR normalized  | normalized to 1W   | 20.5 mW / g               |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 20.5 mW /g ± 16.5 % (k=2) |

| Testing<br>Services™ |                        |                  | Page <b>22(36)</b> |               |
|----------------------|------------------------|------------------|--------------------|---------------|
| Author Data          | Dates of Test          | Test Report No   | FCC ID:            | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW         | 2503A-RDD70UW |

#### Appendix

#### Antenna Parameters with Head TSL

| Impedance, transformed to feed point | 46.5 Ω - 7.3 jΩ |
|--------------------------------------|-----------------|
| Return Loss                          | - 21.5 dB       |

### General Antenna Parameters and Design

| Electrical Delay (one direction) | 1.216 ns |
|----------------------------------|----------|
|                                  |          |

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

| Manufactured by | SPEAG              |
|-----------------|--------------------|
| Manufactured on | September 07, 2001 |

| Testing<br>Services™ |                        |                  | Page 23(36) |               |
|----------------------|------------------------|------------------|-------------|---------------|
| Author Data          | Dates of Test          | Test Report No   | FCC ID:     | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW  | 2503A-RDD70UW |

#### DASY5 Validation Report for Head TSL

Date/Time: 13.01.2011 12:34:12

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN:2d020

Communication System: CW; Frequency: 1800 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: f = 1800 MHz;  $\sigma = 1.38 \text{ mho/m}$ ;  $\varepsilon_r = 38.7$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY5 Configuration:

Probe: ES3DV3 - SN3205; ConvF(5.05, 5.05, 5.05); Calibrated: 30.04.2010

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 10.06.2010

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

Measurement SW: DASY52, V52.6.1 Build (408)

Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)

#### Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement


grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 96.654 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 17.902 W/kg

SAR(1 g) = 9.78 mW/g; SAR(10 g) = 5.13 mW/g

Maximum value of SAR (measured) = 12.051 mW/g

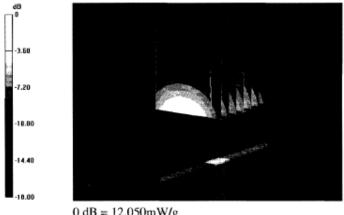


0 dB = 12.050 mW/g

Certificate No: D1800V2-2d020\_Jan11

| Testing<br>Services™ |                        |                  | Page <b>24(36)</b> |               |
|----------------------|------------------------|------------------|--------------------|---------------|
| Author Data          | Dates of Test          | Test Report No   | FCC ID:            | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW         | 2503A-RDD70UW |

### Impedance Measurement Plot for Head TSL

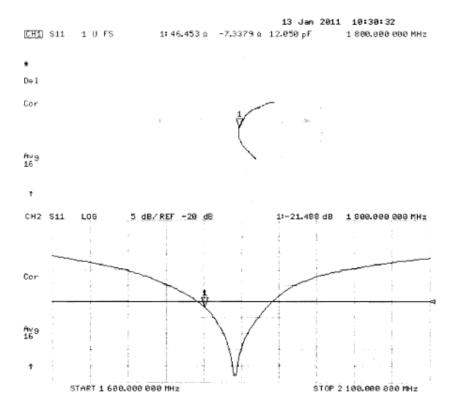

| Testing<br>Services™ |                        |                  |            | Page <b>25</b> (36) |
|----------------------|------------------------|------------------|------------|---------------------|
| Author Data          | Dates of Test          | Test Report No   | FCC ID:    | IC ID               |
| Andrew Becker        | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW | 2503A-RDD70UW       |

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage С Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

RTS (RIM Testing Services)

Certificate No: D1900V2-545\_Jan11

Accreditation No.: SCS 108

#### CALIBRATION CERTIFICATE D1900V2 - SN: 545 Object Calibration procedure(s) QA CAL-05.v8 Calibration procedure for dipole validation kits January 13, 2011 Calibration date: This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID# Cal Date (Certificate No.) Scheduled Calibration Power meter EPM-442A GB37480704 06-Oct-10 (No. 217-01266) Oct-11 Power sensor HP 8481A US37292783 06-Oct-10 (No. 217-01266) Oct-11 SN: 5086 (20g) 30-Mar-10 (No. 217-01158) Reference 20 dB Attenuator Mar-11 SN: 5047.2 / 06327 Type-N mismatch combination 30-Mar-10 (No. 217-01162) Mar-11 Reference Probe ES3DV3 SN: 3205 30-Apr-10 (No. ES3-3205\_Apr10) Apr-11 DAE4 SN: 601 10-Jun-10 (No. DAE4-601\_Jun10) Jun-11 ID# Secondary Standards Check Date (in house) Scheduled Check Power sensor HP 8481A MY41092317 18-Oct-02 (in house check Oct-09) In house check: Oct-11 RF generator R&S SMT-06 100005 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 S4206 18-Oct-01 (in house check Oct-10) In house check: Oct-11 Function Calibrated by: Laboratory Technician and the second second second Approved by: Issued: January 14, 2011 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D1900V2-545\_Jan11

Page 1 of 6

| Testing<br>Services™ |                        |                  | Page <b>26(36)</b> |               |
|----------------------|------------------------|------------------|--------------------|---------------|
| Author Data          | Dates of Test          | Test Report No   | FCC ID:            | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW         | 2503A-RDD70UW |

#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





C

Schweizerischer Kalibrierdienst s

Service suisse d'étalonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

N/A

sensitivity in TSL / NORM x,y,z not applicable or not measured

ConvF

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET). "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

| Certificate No: D1900V2-545_Jan11 | Page 2 of 6 |  |  |
|-----------------------------------|-------------|--|--|

| Testing<br>Services™ |                        |                  | Page <b>27</b> (36) |               |
|----------------------|------------------------|------------------|---------------------|---------------|
| Author Data          | Dates of Test          | Test Report No   | FCC ID:             | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011 | RTS-2579-1106-34 | L6ARDD70UW          | 2503A-RDD70UW |

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

| DASY Version                 | DASY5                     | V52.6       |
|------------------------------|---------------------------|-------------|
| Extrapolation                | Advanced Extrapolation    |             |
| Phantom                      | Modular Flat Phantom V5.0 |             |
| Distance Dipole Center - TSL | 10 mm                     | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm         |             |
| Frequency                    | 1900 MHz ± 1 MHz          |             |

Head TSL parameters
The following parameters and calculations were applied.

|                                  | Temperature     | Permittivity | Conductivity     |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters      | 22.0 °C         | 40.0         | 1.40 mho/m       |
| Measured Head TSL parameters     | (22.0 ± 0.2) °C | 38.5 ± 6 %   | 1.43 mho/m ± 6 % |
| Head TSL temperature during test | (21.2 ± 0.2) °C |              |                  |

### SAR result with Head TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                           |
|---|--------------------|---------------------------|
| SAR measured  | 250 mW input power | 10.2 mW / g               |
| SAR normalized  | normalized to 1W   | 40.8 mW / g               |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 40.0 mW /g ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                          |
|---|--------------------|--------------------------|
| SAR measured  | 250 mW input power | 5.26 mW / g              |
| SAR normalized  | normalized to 1W   | 21.0 mW / g              |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 20.8 mW/g ± 16.5 % (k=2) |

| Testing<br>Services™ | Appendix D for the Black<br>SAR Report | Berry® Smartphone Mo | del RDD71UW | Page <b>28(36)</b> |
|----------------------|--|----------------------|-------------|--------------------|
| Author Data          | Dates of Test                          | Test Report No       | FCC ID:     | IC ID              |
| Andrew Becker        | Apr 13 – June 16, 2011                 | RTS-2579-1106-34     | L6ARDD70UW  | 2503A-RDD70UW      |

#### Appendix

#### Antenna Parameters with Head TSL

| Impedance, transformed to feed point | $50.8 \Omega + 1.8 j\Omega$ |
|--------------------------------------|-----------------------------|
| Return Loss                          | - 34.4 dB                   |

#### General Antenna Parameters and Design

| Electrical Delay (one direction) | 1.199 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

| Manufactured by | SPEAG             |
|-----------------|-------------------|
| Manufactured on | November 15, 2001 |

| Testing<br>Services™ | Appendix D for the BlackE<br>SAR Report | Berry® Smartphone Mod | lel RDD71UW | Page <b>29(36)</b> |
|----------------------|---|-----------------------|-------------|--------------------|
| Author Data          | Dates of Test                           | Test Report No        | FCC ID:     | IC ID              |
| Andrew Becker        | Apr 13 – June 16, 2011                  | RTS-2579-1106-34      | L6ARDD70UW  | 2503A-RDD70UW      |

#### **DASY5 Validation Report for Head TSL**

Date/Time: 13.01.2011 14:52:49

Test Laboratory: SPEAG, Zurich, Switzerland

### DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:545

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: f = 1900 MHz;  $\sigma = 1.43 \text{ mho/m}$ ;  $\varepsilon_r = 38.6$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

#### DASY5 Configuration:

Probe: ES3DV3 - SN3205; ConvF(5.09, 5.09, 5.09); Calibrated: 30.04.2010

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 10.06.2010

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

Measurement SW: DASY52, V52.6.1 Build (408)

Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)


#### Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement

grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.053 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 18.648 W/kg

SAR(1 g) = 10.2 mW/g; SAR(10 g) = 5.26 mW/gMaximum value of SAR (measured) = 12.743 mW/g

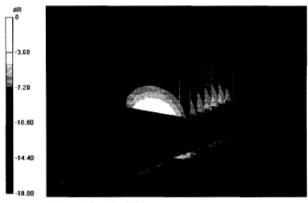


0 dB = 12.740 mW/g

Certificate No: D1900V2-545\_Jan11 Page 5 of 6

| Testing<br>Services™ | Appendix D for the BlackB<br>SAR Report | Page 30(36)      |            |               |
|----------------------|---|------------------|------------|---------------|
| Author Data          | Dates of Test                           | Test Report No   | FCC ID:    | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011                  | RTS-2579-1106-34 | L6ARDD70UW | 2503A-RDD70UW |

### Impedance Measurement Plot for Head TSL

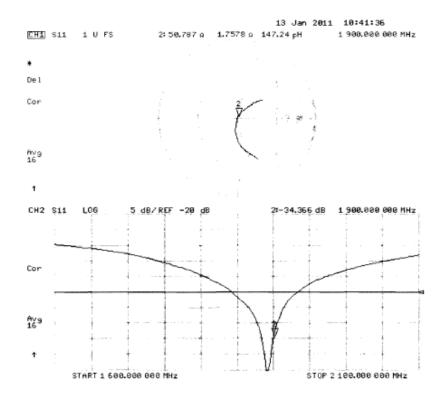

| Testing<br>Services™ | Appendix D for the Black SAR Report | Berry® Smartphone Mo | del RDD71UW | Page 31(36)   |
|----------------------|-------------------------------------|----------------------|-------------|---------------|
| Author Data          | Dates of Test                       | Test Report No       | FCC ID:     | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011              | RTS-2579-1106-34     | L6ARDD70UW  | 2503A-RDD70UW |

Calibration Laboratory of Schmid & Partner Engineering AG





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage С Servizio svizzero di taratura s Swiss Calibration Service

Accreditation No.: SCS 108

Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

RTS (RIM Testing Services) Certificate No: D2450V2-747\_Nov09 Client

#### CALIBRATION CERTIFICA D2450V2 - SN: 747 Object QA CAL-05.V7 Calibration procedure(s) Calibration procedure for dipole validation kits Calibration date: November 11, 2009 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards Cal Date (Certificate No.) Scheduled Calibration Power meter EPM-442A GB37480704 06-Oct-09 (No. 217-01086) Oct-10 Power sensor HP 8481A US37292783 06-Oct-09 (No. 217-01086) Oct-10 Reference 20 dB Attenuator SN: 5086 (20g) 31-Mar-09 (No. 217-01025) Mar-10 Type-N mismatch combination SN: 5047.2 / 06327 31-Mar-09 (No. 217-01029) Mar-10 Reference Probe ES3DV3 SN: 3205 26-Jun-09 (No. ES3-3205\_Jun09) Jun-10 DAE4 SN: 601 07-Mar-09 (No. DAE4-601\_Mar09) Mar-10 Secondary Standards ID# Check Date (in house) Scheduled Check Power sensor HP 8481A MY41092317 18-Oct-02 (in house check Oct-09) In house check: Oct-11 RF generator R&S SMT-06 100005 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 S4206 18-Oct-01 (in house check Oct-09) In house check: Oct-10 Name Function Calibrated by: Approved by: Issued: November 16, 2009 This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: D2450V2-747\_Nov09 Page 1 of 6

| Testing Services™ | Appendix D for the Black<br>SAR Report | Berry® Smartphone Mo | del RDD71UW | Page 32(36)   |
|-------------------|--|----------------------|-------------|---------------|
| Author Data       | Dates of Test                          | Test Report No       | FCC ID:     | IC ID         |
| Andrew Becker     | Apr 13 – June 16, 2011                 | RTS-2579-1106-34     | L6ARDD70UW  | 2503A-RDD70UW |

#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst

C Service suisse d'étalonnage Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D2450V2-747\_Nov09 Page 2 of 6

| Testing<br>Services™ | Appendix D for the Black<br>SAR Report | Berry® Smartphone Mo | del RDD71UW | Page 33(36)   |
|----------------------|--|----------------------|-------------|---------------|
| Author Data          | Dates of Test                          | Test Report No       | FCC ID:     | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011                 | RTS-2579-1106-34     | L6ARDD70UW  | 2503A-RDD70UW |

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

| DASY Version                 | DASY5                     | V5.2        |  |
|------------------------------|---------------------------|-------------|--|
| Extrapolation                | Advanced Extrapolation    |             |  |
| Phantom                      | Modular Flat Phantom V4.9 |             |  |
| Distance Dipole Center - TSL | 10 mm                     | with Spacer |  |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm         |             |  |
| Frequency                    | 2450 MHz ± 1 MHz          |             |  |

### **Head TSL parameters**

The following parameters and calculations were applied.

|                                  | Temperature     | Permittivity | Conductivity     |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters      | 22.0 °C         | 39.2         | 1.80 mho/m       |
| Measured Head TSL parameters     | (22.0 ± 0.2) °C | 39.1 ± 6 %   | 1.78 mho/m ± 6 % |
| Head TSL temperature during test | (21.3 ± 0.2) °C |              |                  |

#### SAR result with Head TSL

| SAR averaged over 1 cm3 (1 g) of Head TSL | Condition          |                           |
|---|--------------------|---------------------------|
| SAR measured                              | 250 mW input power | 13.3 mW / g               |
| SAR normalized                            | normalized to 1W   | 53.2 mW / g               |
| SAR for nominal Head TSL parameters       | normalized to 1W   | 53.4 mW /g ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                          |  |
|---|--------------------|--------------------------|--|
| SAR measured  | 250 mW input power | 6.23 mW / g              |  |
| SAR normalized  | normalized to 1W   | 24.9 mW / g              |  |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 24.9 mW/g ± 16.5 % (k=2) |  |

| Testing<br>Services™ | Appendix D for the BlackB<br>SAR Report | erry® Smartphone Mod | lel RDD71UW | Page 34(36)   |
|----------------------|---|----------------------|-------------|---------------|
| Author Data          | Dates of Test                           | Test Report No       | FCC ID:     | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011                  | RTS-2579-1106-34     | L6ARDD70UW  | 2503A-RDD70UW |

#### Appendix

#### Antenna Parameters with Head TSL

| Impedance, transformed to feed point | 51.9 Ω + 0.9 jΩ |
|--------------------------------------|-----------------|
| Return Loss                          | - 33.9 dB       |

#### General Antenna Parameters and Design

| Electrical Delay (one direction) | 1.161 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

| Manufactured by | SPEAG             |  |  |
|-----------------|-------------------|--|--|
| Manufactured on | December 01, 2003 |  |  |

Certificate No: D2450V2-747 Nov09 Page 4 of 6

| Testing<br>Services™ | Appendix D for the BlackB<br>SAR Report | Berry® Smartphone Mod | lel RDD71UW | Page 35(36)   |
|----------------------|---|-----------------------|-------------|---------------|
| Author Data          | Dates of Test                           | Test Report No        | FCC ID:     | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011                  | RTS-2579-1106-34      | L6ARDD70UW  | 2503A-RDD70UW |

#### **DASY5 Validation Report for Head TSL**

Date/Time: 11.11.2009 15:04:10

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:747

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U11 BB

Medium parameters used: f = 2450 MHz;  $\sigma = 1.79 \text{ mho/m}$ ;  $\varepsilon_r = 39.2$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 26.06.2009

Sensor-Surface: 3mm (Mechanical Surface Detection)
 Electronics: DAE4 Sn601; Calibrated: 07.03.2009

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

#### Head/d=10mm, Pin=250 mW, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.3 V/m; Power Drift = 0.067 dB

Peak SAR (extrapolated) = 27 W/kg

SAR(1 g) = 13.3 mW/g; SAR(10 g) = 6.23 mW/g

Maximum value of SAR (measured) = 17.1 mW/g

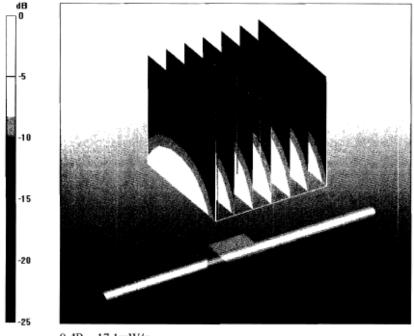

0 dB = 17.1 mW/g

Certificate No: D2450V2-747\_Nov09

Page 5 of 6

| Testing<br>Services™ | Appendix D for the BlackB<br>SAR Report | Berry® Smartphone Mod | lel RDD71UW | Page 36(36)   |
|----------------------|---|-----------------------|-------------|---------------|
| Author Data          | Dates of Test                           | Test Report No        | FCC ID:     | IC ID         |
| Andrew Becker        | Apr 13 – June 16, 2011                  | RTS-2579-1106-34      | L6ARDD70UW  | 2503A-RDD70UW |

### Impedance Measurement Plot for Head TSL

