Testing Services™	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report Page 1(52)			
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Hang Wang Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW			
			L6ARDP70UW	2503A-RDP70UW

APPENDIX D: PROBE & DIPOLE CALIBRATION DATA

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report Page 2(52)			Page 2(52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW L6ARDP70UW				2503A-RDH70CW 2503A-RDP70UW

Calibration Laboratory of Schmid & Partner Engineering AG





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client RTS (RIM Testing Services)

Certificate No: ET3-1643_Mar10

Accreditation No.: SCS 108

CALIBRATION CERTIFICATE ET3DV6 - SN:1643 Object QA CAL-01.v6, QA CAL-23.v3 and QA CAL-25.v2 Calibration procedure(s) Calibration procedure for dosimetric E-field probes Calibration date: March 9, 2010 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID# Cal Date (Certificate No.) Scheduled Calibration Power meter E4419B GB41293874 1-Apr-09 (No. 217-01030) Apr-10 Power sensor E4412A MY41495277 1-Apr-09 (No. 217-01030) Apr-10 Power sensor E4412A MY41498087 1-Apr-09 (No. 217-01030) Apr-10 Reference 3 dB Attenuator SN: S5054 (3c) 31-Mar-09 (No. 217-01026) Mar-10 Reference 20 dB Attenuator SN: S5086 (20b) 31-Mar-09 (No. 217-01028) Mar-10 Reference 30 dB Attenuator SN: S5129 (30b) 31-Mar-09 (No. 217-01027) Mar-10 Reference Probe ES3DV2 SN: 3013 30-Dec-09 (No. ES3-3013_Dec09) Dec-10 DAE4 SN: 660 29-Sep-09 (No. DAE4-660_Sep09) Sep-10 Secondary Standards ID# Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 18-Oct-01 (in house check Oct-09) In house check: Oct10 Name **Eunction** Calibrated by: Laboratory Technician Approved by: Technical Manager Issued: March 10, 2010 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ET3-1643_Mar10

Page 1 of 11

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report Page 3(52)			Page 3(52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW L6ARDP70UW				2503A-RDH70CW 2503A-RDP70UW

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty_cycle) of the RF signal A, B, C modulation dependent linearization parameters

Polarization φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z; Bx,y,z; Cx,y,z, VRx,y,z: A, B, C are numerical linearization parameters assessed based on the data of
 power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
 maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1643_Mar10 Page 2 of 11

Testing Services	Appendix D for the Black RDH71CW/RDP71UW S	Page 4 (52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW			
			L6ARDP70UW	2503A-RDP70UW

Probe ET3DV6

SN:1643

Manufactured: November 7, 2001 Last calibrated: March 10, 2009 Recalibrated: March 9, 2010

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: ET3-1643_Mar10

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report Page 5(52)			
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW L6ARDP70UW				2503A-RDH70CW 2503A-RDP70UW

DASY - Parameters of Probe: ET3DV6 SN:1643

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m) ²) ^A	1.75	2.01	1.79	± 10.1%
DCP (mV) ^B	93.2	91.0	90.9	

Modulation Calibration Parameters

UID	Communication System Name	PAR		A dB	B dBuV	С	VR mV	Unc ^E (k=2)
10000	cw	0.00	×	0.00	0.00	1.00	300.0	± 1.5%
			Y	0.00	0.00	1.00	300.0	
			Z	0.00	0.00	1.00	300.0	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: ET3-1643_Mar10

A The uncertainties of NormX,Y,Z do not affect the E-field uncertainty inside TSL (see Pages 5 and 6).

⁸ Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the maximum deviation from linear response applying recatangular distribution and is expressed for the square of the field value.

Testing Services	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report Page 6(52)			
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	2503A-RDH70CW		
			L6ARDP70UW	2503A-RDP70UW

DASY - Parameters of Probe: ET3DV6 SN:1643

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz]	Validity [MHz] ^C	Permittivity	Conductivity	ConvF X Co	nvFY Co	nvF Z	Alpha	Depth Unc (k=2)	_
900	±50/±100	$41.5 \pm 5\%$	$0.97 \pm 5\%$	6.01	6.01	6.01	0.42	2.35 ± 11.0%	
1810	± 50 / ± 100	$40.0 \pm 5\%$	$1.40 \pm 5\%$	4.99	4.99	4.99	0.62	2.35 ± 11.0%	
1950	±50/±100	40.0 ± 5%	1.40 ± 5%	4.74	4.74	4.74	0.79	2.10 ± 11.0%	

The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Testing Services™	Appendix D for the Black! RDH71CW/RDP71UW SA	Page 7(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW			2503A-RDH70CW
		2503A-RDP70UW		

DASY - Parameters of Probe: ET3DV6 SN:1643

Calibration Parameter Determined in Body Tissue Simulating Media


f [MHz]	Validity [MHz] ^C	Permittivity	Conductivity	ConvF X Con	nvFY Cor	nvF Z	Alpha	Depth Unc (k=2)	_
900	± 50 / ± 100	55.0 ± 5%	1.05 ± 5%	5.93	5.93	5.93	0.33	2.77 ± 11.0%	
1810	±50/±100	53.3 ± 5%	1.52 ± 5%	4.58	4.58	4.58	0.75	2.63 ± 11.0%	
1950	±50/±100	53.3 ± 5%	1.52 ± 5%	4.54	4.54	4.54	0.99	2.20 ± 11.0%	

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report Page 8(52)				
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID	
Hang Wang	ang Wang Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW				
			L6ARDP70UW	2503A-RDP70UW	

Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

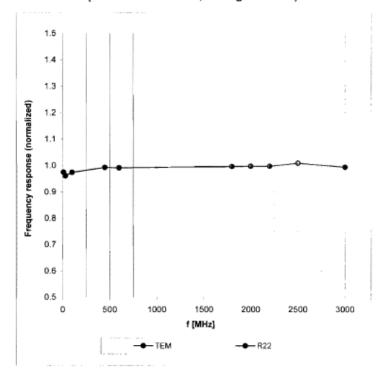


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Testing Services™	Appendix D for the Black! RDH71CW/RDP71UW SA	Page 9(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

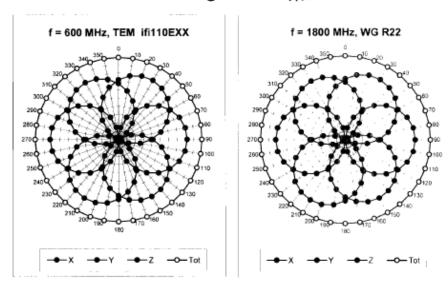

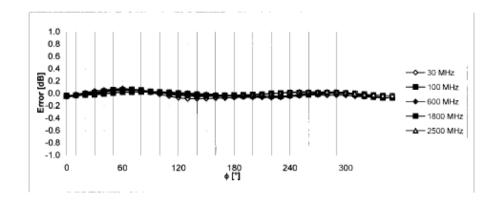


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Testing Services™	Appendix D for the BlackB RDH71CW/RDP71UW SA	Page 10(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Dynamic Range f(SAR_{head})

(Waveguide R22, f = 1800 MHz)

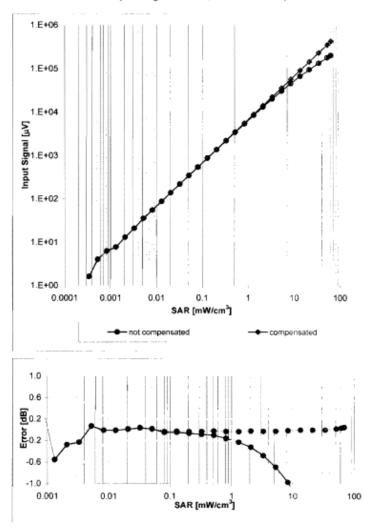



Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Testing Services	Appendix D for the Black RDH71CW/RDP71UW S	Page 11(52)			
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID	1
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW	
			L6ARDP70UW	2503A-RDP70UW	

March 9, 2010 ET3DV6 SN:1643


Conversion Factor Assessment





Deviation from Isotropy in HSL

Error (φ, θ), f = 900 MHz

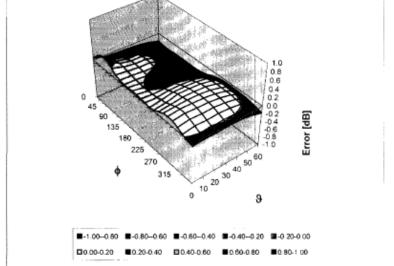

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Testing Services™	Appendix D for the Black RDH71CW/RDP71UW SA	Page 12(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	enabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	6.8 mm
Probe Tip to Sensor X Calibration Point	2.7 mm
Probe Tip to Sensor Y Calibration Point	2.7 mm
Probe Tip to Sensor Z Calibration Point	2.7 mm
Recommended Measurement Distance from Surface	4 mm

Testing Services™	Appendix D for the BlackB RDH71CW/RDP71UW SA	Page 13(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW 2		2503A-RDH70CW	
			L6ARDP70UW	2503A-RDP70UW

Calibration Laboratory of Schmid & Partner Engineering AG Zeoghausstrasse 43, 8064 Zurich, Switzerland

Certificate No: ET3-1844 Nov10





S Schwelzenscher Kollbrierdienst
C Service suisse d'étalonnage
Servizio svizzoro di taratura
S Swies Colibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signaturies to the EA

Multileferal Agreement for the recognition of calibration certificates

RTS (RIM Testing Services) Certificate No: ET3-1644 Nov10 CALIBRATION CERTIFICATE Objet: ET3DV6 - SN:1644 QA CAL-01.v6, QA CAL-23.v3 and QA CAL-25.v2. Calibration procedure(s) Calibration procedure for dosimetric E-field probes Calibration date November 16, 2010 This calibration conflictle documents the traceability to national alandards, which realize the physical units of measurements (SI) The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate All celibrations have been conducted in the closed taboratory facility: environment temperature (22 ± 3)°C and number < 79%, Calibration Equipment used (M&TE ciritical for calibration) Primary Standards ID# Cal Date (Certificate No.) Scheduled Calibration Power meter E4419B GB41293874 1-Apr-10 (No. 217-01136) Apr-11 Power sensor E4412A MY4 1495277 1-Agr-10 (No. 217-01136) A84-11 Prover sensor F4412A MY41498087 1-Apr-10 (No. 217-01136) Apr-11 Reference 3 dB Attenuator SN: \$5054 (3¢) 30-Mar-10 (No. 217-01159) Mar-11 Reference 20 dB Attenuator SN: \$5086 (20b) 30-Mar-10 (No. 217-01161) Mar-11 Reference 30 dB Attenuator SN: 35129 (30b) 30-Mar-10 (No. 217-01160) Reference Probe ES3DV2 SN: 3013 30-Dec-09 (No. ES3-3013 Dec00) Dec-10 DAE4 SN: 860 20-Apr-10 (No. DAE4-560_Apr10) Apr-11 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 864BC US3642U01700 4-Aug-99 (in house check Oct-09) In house ahear Dal-11. Network Analyzer HP 8763E U\$37390585 18-Oct-01 (in house check Oct-10). In house check: Oct-11 **Function** Calibrated by: Leborator Technisian Approved by: Issued: November 17, 2010 This callbration ceruficate shall not be reproduced except in full without written approval of the laboratory

This report shall <u>NOT</u> be reproduced except in full without the written consent of RIM Testing Services Copyright 2005-2011, RIM Testing Services, a division of Research In Motion Limited

Page 1 of 11

Testing Services™	Appendix D for the BlackB RDH71CW/RDP71UW SA	Page 14(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW 2		2503A-RDH70CW	
			L6ARDP70UW	2503A-RDP70UW

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrosso 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibriardienst

C Service sulses d'étalonnage Servizio svizzere di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest fector (1/duty_cycle) of the RF signal A, B, C modulation dependent linearization parameters

Polarization φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 3 = 0 is normal to probe axis.

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1. "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell: f > 1800 MHz: R22 waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x, y.z = NORMx, y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConyF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax, y, z; Bx, y, z; Cx, y, z, VRx, y, z; A, B, C are numerical linearization parameters assessed based on the data of
 power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
 maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f ≥ 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset. The sensor offset corresponds to the offset of virtual measurement center from the probe tip
 (on probe axis). No tolerance required.

Certificate No: ET3-1644 Nov10

Testing Services™	Appendix D for the BlackB RDH71CW/RDP71UW SA	Page 15(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Probe ET3DV6

SN:1644

Manufactured: November 7, 2001
Last calibrated: November 11, 2009
Recalibrated: November 16, 2010

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: €T3-1644_Nov10

Testing Services™	Appendix D for the BlackB RDH71CW/RDP71UW SA	Page 16(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

DASY/EASY - Parameters of Probe: ET3DV6 SN:1644

Basic Calibration Parameters

	Sensor X	Sensor Y	SensorZ	Une (k=2)
Norm (μV/(V/m) ^z) ^A	1.83	1.95	2.01	± 10.1%
DCP (mV) ⁵	97.9	97.9	96.6	

Modulation Calibration Parameters

סוט	Communication System Name	PAR		A dB	B dBuV	С	VR mV	Unc ^e (k=2)
10000	¢₩	0.00	x	0.00	0.00	1.00	143.5	± 3.4 %
			Y	0.00	0.00	1.00	146.8	
			_ , z	0.00	0.00	1.00	148.4	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

 $^{^{\}circ}$ The uncontainties of NormX Y Z do not effect the E held uncertainty noise TSL (see Pages 8 and 6)

⁸ Numerical integrization parameter uncertainty not required.

Lincertainty is determined using the maximum deviation from linear response applying recatangular distribution and is expressed for the square of the field value.

Testing Services	Appendix D for the Black RDH71CW/RDP71UW S	Page 17 (52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

DASY/EASY - Parameters of Probe: ET3DV6 SN:1644

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz]	Validity [MHz] ⁶	Permittivity	Conductivity	ConvEX Co	nvFY Co	nvF Z	Alpha	Depth Unc (k=2)
76D	$\pm 50/\pm 100$	41.9 ± 5%	$0.89 \pm 5\%$	6.54	6.54	6.54	0.31	3.05 ± 11.0%
900	$\pm 507 \pm 100$	41.5 ± 5%	$0.97 \pm 5\%$	6.00	6.00	6.00	0.27	3.46 ± 11.0%
1810	±50/±100	$40.0 \pm 5\%$	1 40 ± 5%	5.09	5.09	5.09	0.40	2.50 ± 11.0%
2450	±50/±100	39.2 ± 5%	$1.80 \pm 5\%$	4.42	4.42	4.42	0.99	1.27 ± 11.0%

The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the CortoF uncertainty at calibration frequency and the uncertainty for the improved frequency band.

Testing Services	Appendix D for the Black RDH71CW/RDP71UW S	Page 18 (52)			
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID	İ
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW	
			L6ARDP70UW	2503A-RDP70UW	

DASY/EASY - Parameters of Probe: ET3DV6 SN:1644

Calibration Parameter Determined in Body Tissue Simulating Media


f (MHz)	Validity [MHz] ^c	Permittivity	Conductivity	ConvF X Cor	nvFY Co	nvF Z	Alpha	Depth Unc (k=2)
750	± 50 / ± 100	55 5 ± 5%	$0.96 \pm 5\%$	6.14	8.14	6.14	0.31	3.06 ± 11.0%
900	± 50 (± 100	55 0 ± 5%	$1.05\pm5\%$	5.93	5.93	5 93	0.36	2.71 ± 11.0%
1810	± 50 f ± 100	53 3 ± 5%	$1.52 \pm 5\%$	4.59	4.59	4 59	0 32	2.60 ± 11.0%
2450	± 50 / ± 100	52.7 ± 5%	$1.95\pm5\%$	4.05	4.05	4 05	0.99	1.23 ± 11.0%

The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the ASS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Testing Services™	Appendix D for the BlackB RDH71CW/RDP71UW SA	Page 19(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

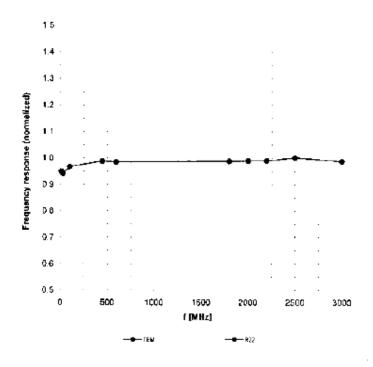


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Testing Services	Appendix D for the Black RDH71CW/RDP71UW S	Page 20 (52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

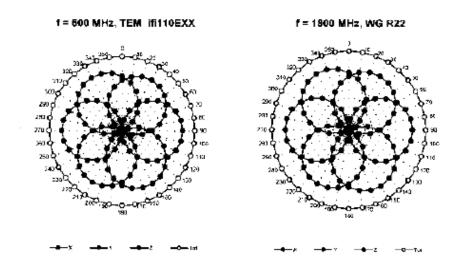


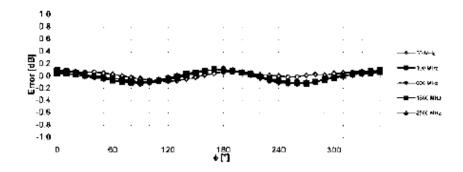

Uncertainty of Axial isotropy Assessment: ± 0.5% (k=2)

Testing Services™	Appendix D for the BlackB RDH71CW/RDP71UW SA	Page 21(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW


Dynamic Range f(SAR_{head})

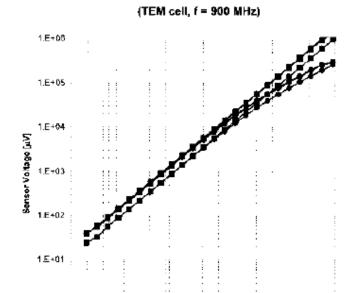

0 1

10

100

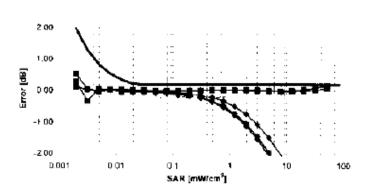


Uncertainty of Linearity Assessment: ± 0.6% (k-2)


1.E+00 0.001

0.01

Testing Services™	Appendix D for the BlackB RDH71CW/RDP71UW SA	Page 22(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW


Conversion Factor Assessment





Deviation from Isotropy in HSL

Error (4, 9), f = 900 MHz



Uncortainty of Spherical Isotropy Assessment: ± 2.6% (k=2)


Certificate No ET3-1644 Nov10

Page 10 of 11

Testing Services	* *	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report				
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID		
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW		
			L6ARDP70UW	2503A-RDP70UW		

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (*)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	enabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	6.8 mm
Probe Tip to Sensor X Calibration Point	2.7 mm
Probe Tip to Sensor Y Calibration Point	2.7 mm
Probe Tip to Sensor Z Calibration Point	2.7 mm
Recommended Measurement Distance from Surface	3.7 mm



Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerlscher Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client RTS (RIM Testing Services)

Accreditation No.: SCS 108

Certificate No: ES3-3225_Jan11

CALIBRATION CERTIFICATE ES3DV3 - SN:3225 Object QA CAL-01.v7, QA CAL-23.v4 and QA CAL-25.v3 Calibration procedure(s) Calibration procedure for dosimetric E-field probes January 13, 2011 Calibration date: This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards Cal Date (Certificate No.) Scheduled Calibration Power meter E4419B GB41293874 1-Apr-10 (No. 217-01136) Apr-11 MY41495277 Power sensor E4412A 1-Apr-10 (No. 217-01136) Apr-11 Power sensor E4412A MY41498087 1-Apr-10 (No. 217-01136) Apr-11 Reference 3 dB Attenuator SN: S5054 (3c) 30-Mar-10 (No. 217-01159) Mar-11 Reference 20 dB Attenuator SN: S5086 (20b) 30-Mar-10 (No. 217-01161) Mar-11 SN: S5129 (30b) Reference 30 dB Attenuator 30-Mar-10 (No. 217-01160) Mar-11 Reference Probe ES3DV2 SN: 3013 29-Dec-10 (No. ES3-3013_Dec10) Dec-11 DAE4 SN: 660 20-Apr-10 (No. DAE4-660_Apr10) Apr-11 Secondary Standards ID# Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 18-Oct-01 (in house check Oct-10) In house check: Oct-11 Function Calibrated by: Laboratory Technician Approved by: Issued: January 15, 2011 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ES3-3225_Jan11

Page 1 of 11

Testing Services				Page 25 (52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A L6ARDH70CW		2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty_cycle) of the RF signal A, B, C modulation dependent linearization parameters

Polarization φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- EC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z; Bx,y,z; Cx,y,z, VRx,y,z; A, B, C are numerical linearization parameters assessed based on the data of
 power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
 maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ES3-3225 Jan11 Page 2 of 11

Testing Services		Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report				
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID	1	
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW		
			L6ARDP70UW	2503A-RDP70UW		

Probe ES3DV3

SN:3225

Manufactured: September 1, 2009
Last calibrated: December 11, 2009
Recalibrated: January 13, 2011

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Testing Services™	Appendix D for the Black RDH71CW/RDP71UW S	Page 27 (52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

DASY/EASY - Parameters of Probe: ES3DV3 SN:3225

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) ²) ^A	1.26	1.21	1.31	± 10.1%
DCP (mV) ⁸	102.1	100.8	99.1	

Modulation Calibration Parameters

UID	Communication System Name	PAR		A dB	B dBuV	С	VR mV	Unc ^E (k=2)
10000	cw	0.00	×	0.00	0.00	1.00	149.8	± 2.6 %
			Υ	0.00	0.00	1.00	148.1	
			Z	0.00	0.00	1.00	110.7	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

 $^{^{\}rm A}$ The uncertainties of NormX,Y,Z do not affect the E^2 -field uncertainty inside TSL (see Pages 5 and 6).

⁸ Numerical linearization parameter, uncertainty not required.

⁶ Uncertainty is determined using the maximum deviation from linear response applying recatangular distribution and is expressed for the square of the field value.

Testing Services™	Appendix D for the Black! RDH71CW/RDP71UW SA	Page 28(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

ES3DV3 SN:3225

January 13, 2011

DASY/EASY - Parameters of Probe: ES3DV3 SN:3225

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz]	Validity [MHz] ^C	Permittivity	Conductivity	ConvF X Co	nvFY Cor	ıvF Z	Alpha	Depth Unc (k=2)
750	±50/±100	$41.9 \pm 5\%$	$0.89 \pm 5\%$	6.47	6.47	6.47	0.89	1.08 ± 11.0%
900	±50/±100	$41.5 \pm 5\%$	$0.97 \pm 5\%$	6.11	6.11	6.11	0.81	1.10 ± 11.0%
1810	±50/±100	40.0 ± 5%	$1.40 \pm 5\%$	5.26	5.26	5.26	0.37	1.68 ± 11.0%
1950	±50/±100	$40.0\pm5\%$	$1.40 \pm 5\%$	4.98	4.98	4.98	0.48	1.51 ± 11.0%
2450	±50/±100	39.2 ± 5%	1.80 ± 5%	4.60	4.60	4.60	0.52	1.54 ± 11.0%
2600	±50/±100	$39.0\pm5\%$	1.96 ± 5%	4.52	4.52	4.52	0.53	1.58 ± 11.0%

^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Testing Services™	Appendix D for the Black RDH71CW/RDP71UW S	Page 29 (52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

ES3DV3 SN:3225

January 13, 2011

DASY/EASY - Parameters of Probe: ES3DV3 SN:3225

Calibration Parameter Determined in Body Tissue Simulating Media


f [MHz]	Validity [MHz] ^C	Permittivity	Conductivity	ConvF X Co	nvFY Co	nvF Z	Alpha	Depth Unc (k=2)
750	±50/±100	$55.5 \pm 5\%$	$0.96 \pm 5\%$	6.30	6.30	6.30	0.76	1.17 ± 11.0%
900	±50/±100	$55.0\pm5\%$	1.05 ± 5%	6.12	6.12	6.12	0.72	1.20 ± 11.0%
1810	±50/±100	53.3 ± 5%	1.52 ± 5%	4.88	4.88	4.88	0.26	2.70 ± 11.0%
1950	±50/±100	$53.3 \pm 5\%$	1.52 ± 5%	4.89	4.89	4.89	0.33	2.28 ± 11.0%
2450	± 50 / ± 100	52.7 ± 5%	$1.95 \pm 5\%$	4.43	4.43	4.43	0.99	1.04 ± 11.0%
2600	±50/±100	52.5 ± 5%	2.16 ± 5%	4.29	4.29	4.29	0.99	1.05 ± 11.0%

The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Testing Services	Appendix D for the Black RDH71CW/RDP71UW S	Page 30(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

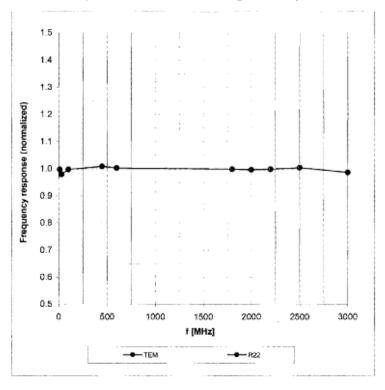


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Testing Services™	Appendix D for the Black RDH71CW/RDP71UW S	Page 31(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW L6ARDP70UW	2503A-RDH70CW 2503A-RDP70UW

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

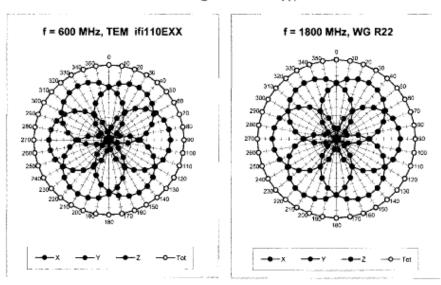

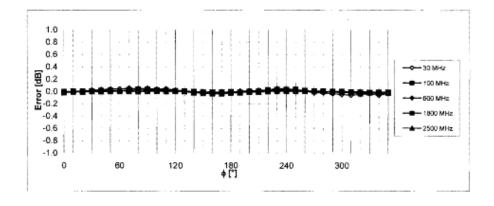



Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Testing Services™	Appendix D for the Black RDH71CW/RDP71UW S.	Page 32(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Dynamic Range f(SAR_{head})

(TEM cell, f = 900 MHz)

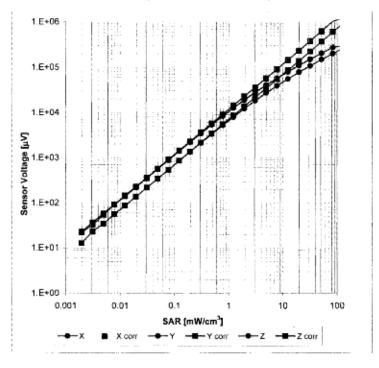


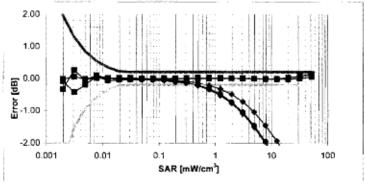


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

				L6ARDP70UW	2503A-RDP70UW
Hang Wang		Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
Author Data		Dates of Test	Test Report No	FCC ID:	IC ID
ABAT 1	Services™	RDH71CW/RDP71UW SA			
2677	lesting	Appendix D for the Black	33(52)		


Conversion Factor Assessment





Deviation from Isotropy in HSL

Error (ϕ , ϑ), f = 900 MHz

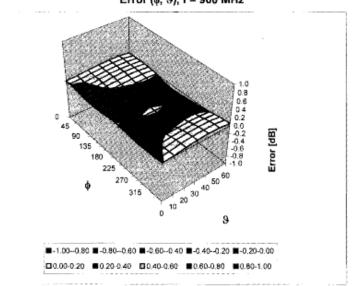

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ES3-3225_Jan11

Page 10 of 11


Testing Services™	Appendix D for the Black! RDH71CW/RDP71UW SA	Page 34(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

ES3DV3 SN:3225

January 13, 2011

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm



Calibration Laboratory of Schmid & Partner Engineering AG



Schweizerischer Kalibrierdienst Service suisse d'étalonnage С Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

RTS (RIM Testing Services) Certificate No: D835V2-446_Jan11

CALIBRATION CERTIFICATE D835V2 - SN: 446 Object QA CAL-05.v8 Calibration procedure(s) Calibration procedure for dipole validation kits Calibration date: January 21, 2011 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards Cal Date (Certificate No.) Scheduled Calibration Power meter FPM-442A GB37480704 06-Oct-10 (No. 217-01266) Oct-11 Power sensor HP 8481A US37292783 06-Oct-10 (No. 217-01266) Oct-11 Reference 20 dB Attenuator SN: 5086 (20a) 30-Mar-10 (No. 217-01158) Mar-11 Type-N mismatch combination SN: 5047.2 / 06327 30-Mar-10 (No. 217-01162) Mar-11 Reference Probe ES3DV3 SN: 3205 30-Apr-10 (No. ES3-3205_Apr10) Apr-11 DAE4 SN: 601 10-Jun-10 (No. DAE4-601_Jun10) Jun-11 Secondary Standards ID# Check Date (in house) Scheduled Check MY41092317 Power sensor HP 8481A 18-Oct-02 (in house check Oct-09) In house check: Oct-11 RF generator R&S SMT-06 100005 4-Aug-99 (in house check Oct-09) In house check: Oct-11 Network Analyzer HP 8753E US37390585 S4206 18-Oct-01 (in house check Oct-10) In house check: Oct-11 Function Calibrated by: Approved by: Issued: January 21, 2011 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D835V2-446_Jan11

Page 1 of 6

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report			Page 36(52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW L6ARDP70UW	2503A-RDH70CW 2503A-RDP70UW

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage

C Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D835V2-446_Jan11	Page 2 of 6	

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report			Page 37(52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.3 ± 6 %	0.89 mho/m ± 6 %
Head TSL temperature during test	(21.8 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.39 mW / g
SAR normalized	normalized to 1W	9.56 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	9.63 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.56 mW / g
SAR normalized	normalized to 1W	6.24 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	6.27 mW /g ± 16.5 % (k=2)

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report			Page 38(52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW L6ARDP70UW	2503A-RDH70CW 2503A-RDP70UW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.6 Ω - 7.7 jΩ
Return Loss	- 22.2 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.386 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG		
Manufactured on	October 24, 2001		

Testing Services	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report			Page 39 (52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

DASY5 Validation Report for Head TSL

Date/Time: 21.01.2011 10:18:05

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:446

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL900

Medium parameters used: f = 835 MHz; $\sigma = 0.89$ mho/m; $\varepsilon_r = 41.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

Probe: ES3DV3 - SN3205; ConvF(6.03, 6.03, 6.03); Calibrated: 30.04.2010

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 10.06.2010

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

Measurement SW: DASY52, V52.6.1 Build (408)

Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)


Pin=250 mW /d=15mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement

grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.426 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 3.600 W/kg

SAR(1 g) = 2.39 mW/g; SAR(10 g) = 1.56 mW/gMaximum value of SAR (measured) = 2.790 mW/g

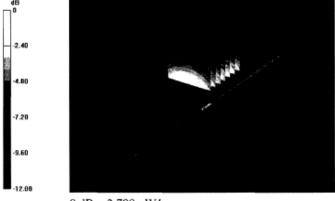


0 dB = 2.790 mW/g

Certificate No: D835V2-446_Jan11

Testing Services	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report			Page 40(52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW			2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Impedance Measurement Plot for Head TSL

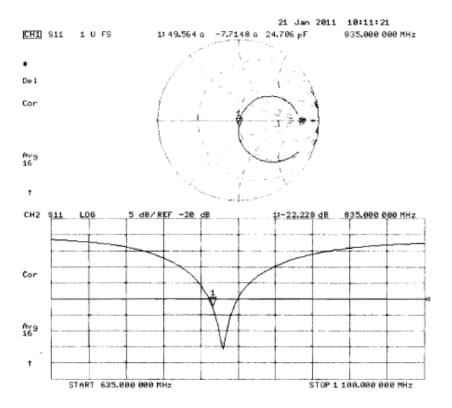

Testing Services	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report			Page 41 (52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW			2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Calibration Laboratory of Schmid & Partner Engineering AG





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

RTS (RIM Testing Services) Client

Certificate No: D1900V2-545_Jan11

Accreditation No.: SCS 108

CALIBRATION CERTIFICATE

D1900V2 - SN: 545 Object

QA CAL-05.v8 Calibration procedure(s)

Calibration procedure for dipole validation kits

January 13, 2011 Calibration date:

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37292783	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01158)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe ES3DV3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11
	Name	Function	Signature
Calibrated by:	Direct Rev	Laboratory Technician	N Viv
		court with an idea of the water owners are a particular of the same of the same	W 4000
Approved by:	Katja Pokovic	Technical Manager	L. Kal
	Analytical Property of	en en antigen de la company de	The state of the s

Issued: January 14, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Testing Services™				Page 42(52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW			2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Calibration Laboratory of

Schmid & Partner Engineering AG





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossarv:

TSL

tissue simulating liquid

ConvF N/A

sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET). "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofreguency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point, No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D1900V2-545_Jan11

Page 2 of 6

Testing Services™	Appendix D for the BlackBerry® Smartphone Model RDH71CW/RDP71UW SAR Report			Page 43 (52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW			2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.5 ± 6 %	1.43 mho/m ± 6 %
Head TSL temperature during test	(21.2 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.2 mW / g
SAR normalized	normalized to 1W	40.8 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	40.0 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.26 mW / g
SAR normalized	normalized to 1W	21.0 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	20.8 mW /g ± 16.5 % (k=2)

Testing Services™	Appendix D for the BlackE RDH71CW/RDP71UW SA	Page 44(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW			2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.8 Ω + 1.8 jΩ
Return Loss	- 34.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.199 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG		
Manufactured on	November 15, 2001		

Testing Services				Page 45 (52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	2503A-RDH70CW		
			L6ARDP70UW	2503A-RDP70UW

DASY5 Validation Report for Head TSL

Date/Time: 13.01.2011 14:52:49

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:545

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: f = 1900 MHz; $\sigma = 1.43 \text{ mho/m}$; $\varepsilon_r = 38.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

Probe: ES3DV3 - SN3205; ConvF(5.09, 5.09, 5.09); Calibrated: 30.04.2010

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 10.06.2010

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

Measurement SW: DASY52, V52.6.1 Build (408)

Postprocessing SW: SEMCAD X, V14.4.2 Build (2595)

Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) /Cube 0: Measurement


grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.053 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 18.648 W/kg

SAR(1 g) = 10.2 mW/g; SAR(10 g) = 5.26 mW/g


Maximum value of SAR (measured) = 12.743 mW/g

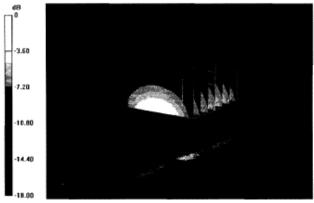

0 dB = 12.740 mW/g

Testing Services Services	Appendix D for the Black RDH71CW/RDP71UW S.		del	Page 46(52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Impedance Measurement Plot for Head TSL

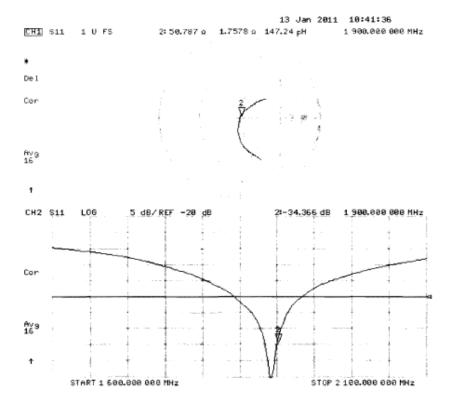

Appendix D for the BlackBerry® Smartphone Model 47(52) RDH71CW/RDP71UW SAR Report Dates of Test Test Report No FCC ID: IC ID Author Data **Hang Wang** Jan 14 – June 09, 2011 RTS-2605-1102-05A L6ARDH70CW 2503A-RDH70CW L6ARDP70UW 2503A-RDP70UW

Calibration Laboratory of Schmid & Partner

Engineering AG





Schweizerischer Kalibrierdienst Service suisse d'étalonnage С Servizio svizzero di taratura s Swiss Calibration Service

Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 108

RTS (RIM Testing Services) Client

Certificate No: D2450V2-747_Nov09

	ung outvious)	Secretaria (2010) (2010	
CALIBRATION	CERTIFICATE		
Object	D2450V2 - SN: 7	47, 114 (114 (114)	
Calibration procedure(s)	QA CAL-05.v7 Calibration proce	dure for dipole validation kits	
Calibration date:	November 11, 20	(69	
The measurements and the unc	certainties with confidence p	onal standards, which realize the physical un robability are given on the following pages an ry facility: environment temperature (22 ± 3)°(d are part of the certificate.
All calibrations have been cond	ucled in the closed laborator	y lacinty, environment temperature (22 ± 5) t	and numbers < 70%.
Calibration Equipment used (Ma	&TE critical for calibration)		
Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-09 (No. 217-01086)	Oct-10
Power sensor HP 8481A	US37292783	06-Oct-09 (No. 217-01086)	Oct-10
Reference 20 dB Attenuator	SN: 5086 (20g)	31-Mar-09 (No. 217-01025)	Mar-10
Type-N mismatch combination	SN: 5047.2 / 06327	31-Mar-09 (No. 217-01029)	Mar-10
The second secon			Mai-10
Reference Probe ES3DV3	SN: 3205	26-Jun-09 (No. ES3-3205_Jun09)	Jun-10
Reference Probe ES3DV3	SN: 3205 SN: 601	26-Jun-09 (No. ES3-3205_Jun09) 07-Mar-09 (No. DAE4-601_Mar09)	
Reference Probe ES3DV3 DAE4	SN: 601	07-Mar-09 (No. DAE4-601_Mar09)	Jun-10 Mar-10
Reference Probe ES3DV3 DAE4 Secondary Standards	SN: 601	07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house)	Jun-10 Mar-10 Scheduled Check
Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A	SN: 601 ID # MY41092317	07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-09)	Jun-10 Mar-10 Scheduled Check In house check; Oct-11
Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	SN: 601	07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house)	Jun-10 Mar-10 Scheduled Check
**	SN: 601 ID # MY41092317 100005 US37390585 S4206	07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-09) 4-Aug-99 (in house check Oct-09) 18-Oct-01 (in house check Oct-09)	Jun-10 Mar-10 Scheduled Check In house check: Oct-11 In house check: Oct-11 In house check: Oct-10
Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	SN: 601 ID # MY41092317 100005	07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-09) 4-Aug-99 (in house check Oct-09)	Jun-10 Mar-10 Scheduled Check In house check: Oct-11 In house check: Oct-11
Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	SN: 601 ID # MY41092317 100005 US37390685 S4206 Name	07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-09) 4-Aug-99 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) Function	Jun-10 Mar-10 Scheduled Check In house check: Oct-11 In house check: Oct-11 In house check: Oct-10

Certificate No: D2450V2-747_Nov09 Page 1 of 6

Testing Services	Appendix D for the Black RDH71CW/RDP71UW S		del	Page 48 (52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst

C Service suisse d'étalonnage

Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Testing Services	Appendix D for the Black RDH71CW/RDP71UW S.		del	Page 49 (52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

-	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.1 ± 6 %	1.78 mho/m ± 6 %
Head TSL temperature during test	(21.3 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm3 (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.3 mW / g
SAR normalized	normalized to 1W	53.2 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	53.4 mW /g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.23 mW / g
SAR normalized	normalized to 1W	24.9 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.9 mW /g ± 16.5 % (k=2)

Testing Services™	Appendix D for the BlackB RDH71CW/RDP71UW SA	•	lel	Page 50(52)
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.9 Ω + 0.9 jΩ
Return Loss	- 33.9 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.161 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	December 01, 2003

Testing Services™	Appendix D for the BlackB RDH71CW/RDP71UW SA	Page 51(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

DASY5 Validation Report for Head TSL

Date/Time: 11.11.2009 15:04:10

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:747

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U11 BB

Medium parameters used: f = 2450 MHz; $\sigma = 1.79 \text{ mho/m}$; $\varepsilon_r = 39.2$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 26.06.2009

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 07.03.2009

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

Head/d=10mm, Pin=250 mW, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.3 V/m; Power Drift = 0.067 dB

Peak SAR (extrapolated) = 27 W/kg

SAR(1 g) = 13.3 mW/g; SAR(10 g) = 6.23 mW/g

Maximum value of SAR (measured) = 17.1 mW/g

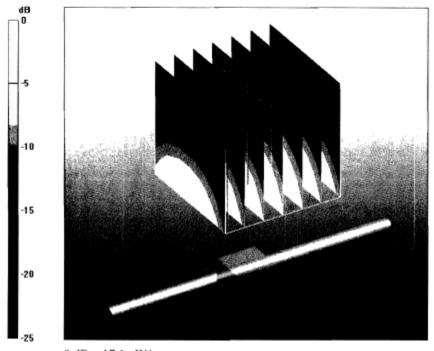

0 dB = 17.1 mW/g

Testing Services™	Appendix D for the Black RDH71CW/RDP71UW S.	Page 52(52)		
Author Data	Dates of Test	Test Report No	FCC ID:	IC ID
Hang Wang	Jan 14 – June 09, 2011	RTS-2605-1102-05A	L6ARDH70CW	2503A-RDH70CW
			L6ARDP70UW	2503A-RDP70UW

Impedance Measurement Plot for Head TSL

