
Testing Services™	Annex B to Hearing Aid Co Report for the BlackBerry®			Page 1(13)
Author Data	Dates of Test	Report No	FCC ID	
Andrew Becker	Mar. 22-23, June 19-22, 2011	RTS-2604-1107-11	L6ARDS40C	W

Annex B: Probe and dipole descriptions and calibration certificates

B.2 Dipole calibration certificate

	Ces™ Report	for the BlackBerry® Sm	artphone mode	I RDS41CW 2(13)
r Data drew Becker	Dates of Test Mar. 22-	-23, June 19-22, 2011 RT	^{т No} S-2604-1107-11	FCC ID L6ARDS40CW
Calibration Laborato Schmid & Partner Engineering AG eughausstrasse 43, 8004 Zurk	ch, Switzerland	Source diation	Service suisse d'étalonn Servizio svizzero di tarat	hage tura
he Swiss Accreditation Servic fultilateral Agreement for the r	-			
CALIBRATION			o: CD835V3-1011_No	0009
Object	CD835V3 - SN:			
Calibration procedure(s)	QA CAL-20.v4 Calibration procession	edure for dipoles in air		
	COMPRESSION AND ADDRESS AND ADDR ADDRESS AND ADDRESS AN ADDRESS AND ADDRESS	Environmental and the second sec	CERTIFICATION CONTRACTOR AND	16
Calibration date:	November 17, 2	009 ^{(**} y ^{.9} y ^{.9} y ^{.9}) (**)	1.000	R
This calibration certificate docun All calibrations have been condu Calibration Equipment used (M8	nents the traceability to na ucted in the closed laboration)	tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)	C and humidity < 70%.	1
This calibration certificate docum	nents the traceability to na acted in the closed laborate	tional standards, which realize the physical u		×1
This calibration certificate docun All calibrations have been condu Calibration Equipment used (M& Primary Standards	nents the traceability to na acted in the closed laborate TE critical for calibration)	tional standards, which realize the physical un ory facility: environment temperature (22 ± 3) Cal Date (Certificate No.)	C and humidity < 70%. Scheduled Calibratio	<u>n</u>
This calibration certificate docun All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6	ID # GB37480704 US37292783 SN: 2336	tional standards, which realize the physical up ory facility: environment temperature (22 ± 3) ⁴ Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09	<u>n</u>
This calibration certificate docun All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	ID # GB37480704 US37292783 SN: 2336 SN: 6065	tional standards, which realize the physical us ory facility: environment temperature (22 ± 3) ⁴ Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09	xn
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781	Cal Date (Certificate No.) Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08) 22-Dec-08 (No. DAE4-781_Feb09)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10	2n
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER30V6 Probe H30V6 DAE4 Secondary Standards	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID #	tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. A3-6065Dec08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check	
This calibration certificate docun All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER30V6 Probe H30V6 DAE4 Secondary Standards Power meter Agilent 44198	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB42420191	tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Gal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct-	-10
This calibration certificate docun All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilant 44198 Power sensor HP 8482H	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450	tional standards, which realize the physical us ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct-	-10 -10
This calibration certificate docun All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER30V6 Probe H30V6 DAE4 Secondary Standards Power meter Agilent 44198	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB42420191	tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Gal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct-	-10 -10 -10
This calibration certificate docun All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilant 44198 Power sensor HP 8482H Power sensor HP 8482A	ID # GB37480704 UD # GB37480704 US37292783 SN: 2336 SN: 6055 SN: 781 ID # ID # I	tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* 06-Oct-09 (No. 217-01066) 06-Oct-09 (No. 217-01066) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. A5-6065Dec08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct- In house check: Oct-	-10 -10 -10 -10
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe H3DV6 DAE4 Secondary Standards Power sensor HP 8482H Power sensor HP 8482H Regenerator E4433B	nents the traceability to na acted in the closed laboration TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37296597 US37390585 MY 41000675 Name	tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. A5-6065Dec08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 18-Oct-09 (in house check Oct-09) 03-Nov-04 (in house check Oct-09) 03-Nov-04 (in house check Oct-09)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct-	-10 -10 -10 -10
This calibration certificate docun All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter EPM-442A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	nents the traceability to na acted in the closed laboration) ID # GB37480704 US37292783 SN: 2336 SN: 6055 SN: 781 ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37295597 US37290585 MY 41000675	tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Gel Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 18-Oct-09 (in house check Oct-09) 03-Nov-04 (in house check Oct-09)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct-	-10 -10 -10 -10
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe H3DV6 DAE4 Secondary Standards Power sensor HP 8482H Power sensor HP 8482H Regenerator E4433B	nents the traceability to na acted in the closed laboration TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37296597 US37390585 MY 41000675 Name	tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 18-Oct-09 (in house check Oct-09) 03-Nov-04 (in house check Oct-09) 03-Nov-04 (in house check Oct-09)	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct-	-10 -10 -10 -10
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER30V6 DAE4 Secondary Standards Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E RF generator E4433B	ID # GB37480704 US # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB42420191 SN: 318A09450 SN: US37296597 US37290585 MY 41000675 Name Nike Meil Fin Bombolt	Cal Date (Certificate No.) Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 03-Nov-04 (in house check Oct-09) 03-Nov-04 (in house check Oct-09) Eunction	C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct-	-10 -10 -10 -10 -11

This report shall <u>NOT</u> be reproduced except in full without the written consent of RIM Testing Services Copyright 2005-2011, RIM Testing Services, A division of Research In Motion Limited



SNISS

ØR6

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kallbrierdienst C Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

References

 ANSI-C63.19-2006 American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

[2] ANSI-C63.19-2007

American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with the standards [1, 2], the measurement planes (probe sensor center) are selected to be at a distance of 10 mm above the top edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections. It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY5 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe sensor offset.
- Feed Point Impedance and Return Loss: These parameters are measured using a HP 8753E Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- E- field distribution: E field is measured in the x-y-plane with an isotropic ER3D-field probe with 100 mW forward power to the antenna feed point. In accordance with [1, 2], the scan area is 20mm wide, its length exceeds the dipole arm length (180 or 90mm). The sensor center is 10 mm (in z) above the top of the dipole arms. Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any non-parallelity to the measurement plane as well as the sensor displacement. The E-field value stated as calibration value represents the maximum of the interpolated 3D-E-field, 10mm above the dipole surface.
- H-field distribution: H-field is measured with an isotropic H-field probe with 100mW forward power to the
 antenna feed point, in the x-y-plane. The scan area and sensor distance is equivalent to the E-field
 scan. The maximum of the field is available at the center (subgrid 5) above the feed point. The H-field
 value stated as calibration value represents the maximum of the interpolated H-field, 10mm above the
 dipole surface at the feed point.

Certificate No: CD835V3-1011_Nov09

Page 2 of 6

This report shall <u>NOT</u> be reproduced except in full without the written consent of RIM Testing Services Copyright 2005-2011, RIM Testing Services, A division of Research In Motion Limited

Testing Services [™]	Annex B to Hearing Aid Con Report for the BlackBerry®			Page 4(13)
Author Data	Dates of Test	Report No	FCC ID	

1 Measurement Conditions

DASY system configuration,	as far as not gi	iven on page 1.
----------------------------	------------------	-----------------

DASY Version	DASY5	V5.2 B157
DASY PP Version	SEMCAD X	V14.0 B57
Phantom	HAC Test Arch	SD HAC P01 BA, #1070
Distance Dipole Top - Probe Center	10 mm	
Scan resolution	dx, dy = 5 mm	area = 20 x 180 mm
Frequency	835 MHz ± 1 MHz	
Forward power at dipole connector	20.0 dBm = 100mW	
Input power drift	< 0.05 dB	

2 Maximum Field values

	H-field 10 mm above dipole surface	condition	interpolated maximum
	Maximum measured	100 mW forward power	0.464 A/m
ţ	Incertainty for H-field measurement: 8.2% (k=2)		

E-field 10 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end-	100 mW forward power	168.6 V/m
Maximum measured above low end	100 mW forward power	157.4 V/m
Averaged maximum above arm	100 mW forward power	163.0 V/m

Uncertainty for E-field measurement: 12.8% (k=2)

3 Appendix

3.1 Antenna Parameters

Frequency	Return Loss	Impedance
800 MHz	15.7 dB	(44.8 – j14.9) Ohm
835 MHz	31.8 dB	(48.5 + j2.0) Ohm
900 MHz	17.7 dB	(54.3 – j12.9) Ohm
950 MHz	20.5 dB	(44.7 + j7.2) Ohm
960 MHz	16.3 dB	(51.0 + j15.7) Ohm

3.2 Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.

The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.

Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.


Certificate No: CD835V3-1011_Nov09

Page 3 of 6

Testing Services™	Annex B to Hearing Aid Co Report for the BlackBerry®			Page 5(13)
Author Data	Dates of Test	Report No	FCC ID	
Andrew Becker	Mar. 22-23, June 19-22, 2011	RTS-2604-1107-11	L6ARDS40C	W


3.3 Measurement Sheets

3.3.1 Return Loss and Smith Chart

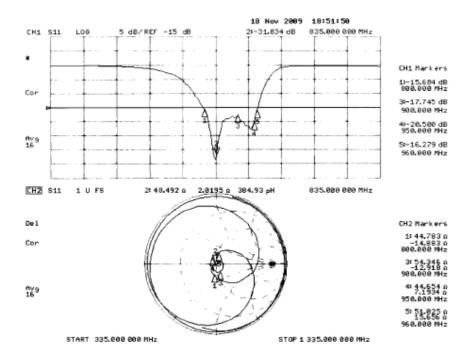

Certificate No: CD835V3-1011_Nov09

Page 4 of 6



3.3.2 DASY4 H-field Result

Date/Time: 17.11.2009 15:02:26

Test Laboratory: SPEAG Lab2


 $\label{eq:hackbox} \begin{array}{l} \mbox{HAC RF_CD835_1011_091117_H_MM} \\ \mbox{DUT: HAC-Dipole 835 MHz; Type: D835V3; Serial: 1011} \\ \mbox{Communication System: CW; Frequency: 835 MHz} \\ \mbox{Medium parameters used: $\sigma = 0$ mho/m, $e_r = 1$; $\rho = 1$ kg/m^3$ \\ \mbox{Phantom section: RF Section} \\ \mbox{Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)} \\ \mbox{DASY5 Configuration:} \\ \mbox{Probe: H3DV6 - SN6065; ; Calibrated: 22.12.2008} \\ \end{array}$

- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 20.02.2009
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

Dipole H-Field measurement @ 835MHz/H Scan - measurement distance from the probe sensor center to CD835 Dipole = 10mm/Hearing Aid Compatibility Test (41x361x1):

Measurement grid: dx=5mm, dy=5mm Maximum value of peak Total field = 0.464 A/m Probe Modulation Factor = 1 Device Reference Point: 0, 0, -6.3 mm Reference Value = 0.494 A/m; Power Drift = -0.00467 dB Hearing Aid Near-Field Category: M4 (AWF 0 dB)


Grid 1	Grid 2	Grid 3
0.384	0.405	0.386
M4	M4	M4
Grid 4	Grid 5	Grid 6
).441	0.464	0.439
M4	M4	M4
Grid 7	Grid 8	Grid 9
0 .390	0.409	0.382
M4	M4	M4



0 dB = 0.464A/m

Certificate No: CD835V3-1011_Nov09

Page 5 of 6



3.3.3 DASY4 E-field Result

Date/Time: 17.11.2009 11:56:37

Test Laboratory: SPEAG Lab2

Sensor-Surface: (Fix Surface)

Electronics: DAE4 Sn781; Calibrated: 20.02.2009


Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070

Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

Dipole E-Field measurement @ 835MHz/E Scan - measurement distance from the probe sensor center to CD835 Dipole = 10mm/Hearing Aid Compatibility Test (41x361x1):

Measurement grid: dx=5mm, dy=5mm Maximum value of peak Total field = 168.6 V/m Probe Modulation Factor = 1 Device Reference Point: 0, 0, -6.3 mm Reference Value = 109.2 V/m; Power Drift = -0.023 dB Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field	in V/m	
Grid 1	Grid 2	Grid 3
152.1	157.4	154.5
M4	M4	M4
Grid 4	Grid 5	Grid 6
84.1	86.8	84.5
M4	M4	M4
Grid 7	Grid 8	Grid 9
165.5	168.6	158.2
M4	M4	M4




0 dB = 168.6 V/m

Certificate No: CD835V3-1011_Nov09

Page 6 of 6

Jarra Testi	10 Annox	B to Hearing Aid Compa	tibility DE Emic	cione Toet	
		• •	•		
Service Service	Ces™ Report	for the BlackBerry® Sma	artphone mode	RD541CW	8(13)
r Data	Dates of Test	22 Lange 10 22 2011 PT		FCC ID	aw
drew Becker	Mar. 22-	-23, June 19-22, 2011 RT	S-2604-1107-11	L6ARDS40	CW
Calibration Laborato	ry of	SNISS S	Schweizerischer Kalibrie	erdienst	
Schmid & Partner			Service suisse d'étalonn		
Engineering AG Leughausstrasse 43, 8004 Zurid	-h Switzerland	The stand	Servizio svizzero di tara		
cognaassaase 40, 0004 zant	an, owneen and	And and a state of the state of	Swiss Galibration Servic		
Accredited by the Swiss Accred	ditation Service (SAS)	Accreditation	No.: SCS 108		
The Swiss Accreditation Servic	-				
Multilateral Agreement for the r			: CD1880V3-1008	10000	
Client RTS (RIM Test	ou care i carefor i dave i i fosso	an 200 an 199	0: CO 1000V3-1000_1		
CALIBRATION (CERTIFICAT	E contract of the			
		Ninneisse with signific second of	enhiller) Jakob objiret octob		
Object	CD1880V3 - SN	: 1008	Carefornia Carefornia		
Calibration procedure(s)	QA CAL-20.v4			影 ね	
	Calibratian prop			1847	
	Calibration proc	edure for dipoles in air			
Calibration date:		edure for dipoles in air			
Calibration date:					
Calibration date:					
Calibration date:					
	November 18, 2			200 20 20 20	
This calibration certificate docum	November 18, 2	009	nits of measurements (SI).	2007 	
This calibration certificate docum	November 18, 2 nents the traceability to na cted in the closed laborate	009 tional standards, which realize the physical u	nits of measurements (SI).	27 	
This calibration certificate docur All calibrations have been condu Celibration Equipment used (M&	November 16, 2 nents the traceability to na cted in the closed laboration TE critical for calibration)	009 tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)*	hits of measurements (SI). C and humidity < 70%.		
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M& Primary Standards	November 18, 2 nents the traceability to na cted in the closed laboration TE critical for calibration)	009 tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio	n	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A	November 18, 2 nerts the traceability to na icted in the closed laboration TE critical for calibration)	009 tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086)	ults of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10	<u>n</u>	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	November 16, 2 November 16, 2 Novemb	009 tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086)	nits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10	<u>n</u>	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6	November 18, 2 November 18, 2 nents the traceability to na inter critical for calibration) ID # GB37480704 US37292783 SN: 2336	009 tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. ER3-2336_Dec08)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09	n	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	November 16, 2 November 16, 2 Novemb	009 tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086)	nits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10	<u>n</u>	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Prote ER3DV6 Probe H3DV6	November 18, 2 nents the traceability to na icted in the closed laboration TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065	009 tional standards, which realize the physical us ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09	n	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Prote ER3DV6 Probe H3DV6	November 18, 2 nents the traceability to na icted in the closed laboration TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065	009 tional standards, which realize the physical us ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09	n	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards	November 18, 2 nents the traceability to ra- icted in the closed laboral TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID #	009 tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. DAE4-781_Feb09) Check Date (in house)	nits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check		
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4	November 18, 2 November 18, 2 nents the traceability to na inter control laboration TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 2005 SN: 781 ID # ID # SN: GB42420191	009 tional standards, which realize the physical up ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6085Oec08) 22-Dec-08 (No. H3-6085Oec08) 22-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct-	10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Prote ER3DV6 Prote H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H	November 18, 2 November 18, 2 nents the traceability to na cted in the closed laboration TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450	009 tional standards, which realize the physical us ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct-	10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482A	November 18, 2 November 18, 2 ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # ID N SN: GB42420191 SN: 3318A09450 SN: US37295597	009 tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dac-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct- In house check: Oct-	10 10 10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	November 18, 2 November 18, 2 nerts the traceability to na icted in the closed laboratory TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # ID # ID # ID # ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37295597 US37390585	009 tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. ER3-2336, Dec08) 22-Dec-08 (No. ER3-2336, Dec08) 22-Dec-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 18-Oct-09 (in house check Oct-09) 18-Oct-01 (in house check Oct-09)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct-	10 10 10 10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482A	November 18, 2 November 18, 2 ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # ID N SN: GB42420191 SN: 3318A09450 SN: US37295597	009 tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dac-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct- In house check: Oct-	10 10 10 10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	November 18, 2 November 18, 2 nerts the traceability to na icted in the closed laboratory TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # ID # ID # ID # ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37295597 US37390585	009 tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. ER3-2336, Dec08) 22-Dec-08 (No. ER3-2336, Dec08) 22-Dec-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 18-Oct-09 (in house check Oct-09) 18-Oct-01 (in house check Oct-09)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct-	10 10 10 10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E RF generator E4433B	November 18, 2 herits the traceability to na icted in the closed laboration TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # ID # ID # SN: GB42420191 SN: 3318A09450 SN: US3729597 US37390585 MY 41000675 Name	009 tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-09 (No. DAE4-781_Feb09) 09-Oct-09 (No. DAE4-781_Feb09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 18-Oct-01 (In house check Oct-09) 18-Oct-01 (In house check Oct-09) 03-Nov-04 (In house check Oct-09) 03-Nov-04 (In house check Oct-09)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct-	10 10 10 10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	November 18, 2 herits the traceability to na icted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: 6065 SN: 781 ID # SN: 3318A09450 SN: US37295597 US37290685 MY 41000675	009 tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. DAE4-781_Feb09) 20-Feb-09 (No. DAE4-781_Feb09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 03-Nov-04 (in house check Oct-09)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct-	10 10 10 10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power sensor HP 8482A Power sensor HP 8482A Network Analyzer HP 8753E RF generator E4433B Calibrated by:	November 18, 2 herits the traceability to na icted in the closed laboration TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # ID # ID # SN: GB42420191 SN: 3318A09450 SN: US3729597 US37390585 MY 41000675 Name	009 tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-09 (No. DAE4-781_Feb09) 09-Oct-09 (No. DAE4-781_Feb09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 18-Oct-01 (In house check Oct-09) 18-Oct-01 (In house check Oct-09) 03-Nov-04 (In house check Oct-09) 03-Nov-04 (In house check Oct-09)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct-	10 10 10 10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E RF generator E4433B	November 18, 2 herits the traceability to na icted in the closed laboration TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # ID # ID # SN: GB42420191 SN: 3318A09450 SN: US3729597 US37390585 MY 41000675 Name	009 tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-09 (No. DAE4-781_Feb09) 09-Oct-09 (No. DAE4-781_Feb09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 18-Oct-01 (In house check Oct-09) 18-Oct-01 (In house check Oct-09) 03-Nov-04 (In house check Oct-09) 03-Nov-04 (In house check Oct-09)	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct-	10 10 10 10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power sensor HP 8482A Power sensor HP 8482A Network Analyzer HP 8753E RF generator E4433B Calibrated by:	November 18, 2 nents the traceability to ra- icted in the closed laboration TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37295597 US37295655 MY 41000675 Name Claudio Leubler	009 tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08) 22-Dec-08 (No. H3-6065Dec08) 22-Dec-09 (No. DAE4-781_Feb09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 09-Oct-01 (In house check Oct-09) 03-Nov-04 (In house check Oct-09) 03-Nov-04 (In house check Oct-09) Eunction Laboratory Technicien	hits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct- In house check: Oct-	10 10 10 10	
This calibration certificate docum All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Aglient 4419B Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E RF generator E4433B Calibrated by: Approved by:	November 18, 2 nerts the traceability to na icted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: 6085 SN: 00812420191 SN: 3318A09450 SN: US37295597 US37390585 MY 41000675 Name Claudio Leubler Fin Bomholt	009 tional standards, which realize the physical un ory facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-09 (No. DAE4-781_Feb09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 09-Oct-01 (In house check Oct-09) 03-Nov-04 (In house check Oct-09) 03-Nov-04 (In house check Oct-09) Eunction Laboratory Technicien	nits of measurements (SI). C and humidity < 70%. Scheduled Calibratio Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: Oct- In house check: Oct-	10 10 10 10 11	

This report shall <u>NOT</u> be reproduced except in full without the written consent of RIM Testing Services Copyright 2005-2011, RIM Testing Services, A division of Research In Motion Limited



WISS

BRD

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



s Service suisse d'étalonnage С Servizio svizzero di taratura s

Schweizerischer Kalibrierdienst

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

References

- ANSI-C63.19-2006 [1]
 - American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

[2] ANSI-C63.19-2007

American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms, x-axis is normal to the other axes. In coincidence with the standards [1, 2], the measurement planes (probe sensor center) are selected to be at a distance of 10 mm above the top edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections. It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY5 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a HP 8753E Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- E- field distribution: E field is measured in the x-y-plane with an isotropic ER3D-field probe with 100 mW forward power to the antenna feed point. In accordance with [1, 2], the scan area is 20mm wide, its length exceeds the dipole arm length (180 or 90mm). The sensor center is 10 mm (in z) above the top of the dipole arms. Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any non-parallelity to the measurement plane as well as the sensor displacement. The E-field value stated as calibration value represents the maximum of the interpolated 3D-E-field, 10mm above the dipole surface.
- H-field distribution: H-field is measured with an isotropic H-field probe with 100mW forward power to the antenna feed point, in the x-y-plane. The scan area and sensor distance is equivalent to the E-field scan. The maximum of the field is available at the center (subgrid 5) above the feed point. The H-field value stated as calibration value represents the maximum of the interpolated H-field, 10mm above the dipole surface at the feed point.

Certificate No: CD1880V3-1008_Nov09

Page 2 of 6

This report shall NOT be reproduced except in full without the written consent of RIM Testing Services Copyright 2005-2011, RIM Testing Services, A division of Research In Motion Limited

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDS41CW		Page 10(13)	
Author Data	Dates of Test	Report No	FCC ID	
Andrew Becker	Mar. 22-23, June 19-22, 2011	RTS-2604-1107-11	L6ARDS40C	W

1. Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.2 B157
DASY PP Version	SEMCAD X	V14.0 B57
Phantom	HAC Test Arch	SD HAC P01 BA, #1070
Distance Dipole Top - Probe Center	10 mm	
Scan resolution	dx, dy = 5 mm	area = 20 x 90 mm
Frequency	1880 MHz ± 1 MHz	
Forward power at dipole connector	20.0 dBm = 100mW	
Input power drift	< 0.05 dB	

2. Maximum Field values

H-field 10 mm above dipole surface	condition	Interpolated maximum	
Maximum measured	100 mW forward power	0.471 A/m	
Uncertainty for H-field measurement: 8.2% (k=2)			

Uncertainty for H-field measurement: 8.2% (k=2)

E-field 10 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end	100 mW forward power	136.2 V/m
Maximum measured above low end	100 mW forward power	132.1 V/m
Averaged maximum above arm	100 mW forward power	134.2 V/m

Uncertainty for E-field measurement: 12.8% (k=2)

3. Appendix

3.1 Antenna Parameters

Frequency	Return Loss	Impedance
1710 MHz	22.8 dB	(52.2 + j7.1) Ohm
1880 MHz	20.0 dB	(50.5 + j10.1) Ohm
1900 MHz	20.9 dB	(53.2 + j8.8) Ohm
1950 MHz	29.5 dB	(52.3 + j2.6) Ohm
2000 MHz	18.7 dB	(43.2 + j8.4) Ohm

3.2 Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.

The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.

Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.


Certificate No: CD1880V3-1008_Nov09

Page 3 of 6

Testing Services™	Annex B to Hearing Aid Co Report for the BlackBerry®			Page 11(13)
Author Data	Dates of Test	Report No	FCC ID	
Andrew Becker	Mar. 22-23, June 19-22, 2011	RTS-2604-1107-11	L6ARDS40C	W

3.3 Measurement Sheets

3.3.1 Return Loss and Smith Chart

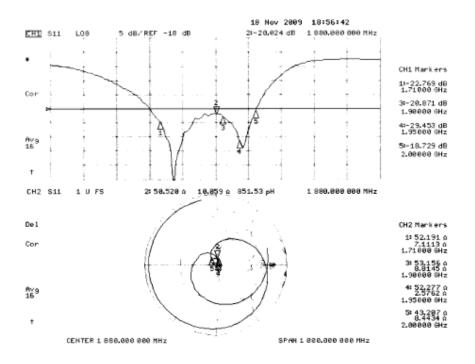

Certificate No: CD1880V3-1008_Nov09

Page 4 of 6

Testing Services™	Annex B to Hearing Aid Co Report for the BlackBerry®			Page 12(13)
Author Data	Dates of Test	Report No	FCC ID	
Andrew Becker	Mar. 22-23. June 19-22. 2011	RTS-2604-1107-11	L6ARDS40C	W

3.3.2 DASY4 H-Field Result

Date/Time: 18.11.2009 12:32:23

Test Laboratory: SPEAG Lab2

Sensor-Surface: (Fix Surface)


Electronics: DAE4 Sn781; Calibrated: 20.02.2009

- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

Dipole H-Field measurement @ 1880MHz/H Scan - measurement distance from the probe sensor center to CD1880 Dipole = 10mm/Hearing Aid Compatibility Test (41x181x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.471 A/m Probe Modulation Factor = 1 Device Reference Point: 0, 0, -6.3 mm Reference Value = 0.499 A/m; Power Drift = 0.00498 dB Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak H-field	Peak H-field in A/m			
Grid I	Grid 2	Grid 3		
0.408	0.423	0.398		
M2	M2	M2		
Grid 4	Grid 5	Grid 6		
0.456	0.471	0.439		
M2	M2	M2		
Grid 7	Grid 8	Grid 9		
0.420	0.435	0.400		
M2	M2	M2		



0 dB = 0.471 A/m

Certificate No: CD1880V3-1008_Nov09

Page 5 of 6

Testing Services™	Annex B to Hearing Aid Co Report for the BlackBerry®			Page 13(13)
Author Data	Dates of Test	Report No	FCC ID	
Andrew Becker	Mar. 22-23, June 19-22, 2011	RTS-2604-1107-11	L6ARDS40C	X 7

3.3.3 DASY4 E-Field Result

Date/Time: 18.11.2009 17:16:43

Test Laboratory: SPEAG Lab2


Electronics: DAE4 Sn781; Calibrated: 20.02.2009

- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

Dipole E-Field measurement @ 1880MHz/E Scan - measurement distance from the probe sensor center to CD1880 Dipole = 10mm/Hearing Aid Compatibility Test (41x181x1):

Measurement grid: dx=5mm, dy=5mm Maximum value of peak Total field = 136.2 V/m Probe Modulation Factor = 1 Device Reference Point: 0, 0, -6.3 mm Reference Value = 152.3 V/m; Power Drift = -0.00386 dB Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak E-field	Peak E-field in V/m			
Grid 1	Grid 2	Grid 3		
124.7	132.1	131.1		
M2	M2	M2		
Grid 4	Grid 5	Grid 6		
86.6	90.1	87.7		
M3	M3	M3		
Grid 7	Grid 8	Grid 9		
130.7	136.2	132.2		
M2	M2	M2		



0 dB = 136.2V/m

Certificate No: CD1880V3-1008_Nov09

Page 6 of 6