Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDZ21CW			Page 1(13)
Author Data	Dates of Test	Report No	FCC ID	
Hang Wang	July 28, Aug 4, 2011	RTS-2604-1108-06	L6ARDZ20C	2W

## Annex B: Probe and dipole descriptions and calibration certificates

**B.2** Dipole calibration certificate

Servin						
Servin		B to Hearing Aid	Compat	ibility RF Emi	ssions Test	
	Ces™ Report	for the BlackBe	rrv® Sma	rtphone mode	el RDZ21CW	2(13)
	663					2(13)
r Data	Dates of Test		Report No	4 4 4 0 0 0 6	FCC ID	
ng Wang	<b>July 28</b> ,	Aug 4, 2011	RTS-260	4-1108-06	L6ARDZ2	OCW
		autou				
Calibration Laborator	ry or	S SN	ISS S	Schweizerischer Kalib		
Schmid & Partner		IC MRA	🕽 z 🗋 C	Service suisse d'étalor	-	
Engineering AG (eughausstrasse 43, 8004 Zuric	h Switzerland		∜ s	Servizio svizzero di ta Swiss Calibration Serv		
cuyilaussuasse 43, 0004 zuile	an, awnaterionita	All	141	Swiss Galibration Serv	nce	
executived by the Purior Assess	ditation Convice (CAC)		Accorditation	No.: SCS 108		
Accredited by the Swiss Accred The Swiss Accreditation Servic		es to the EA	Accreditation	No.: 303 100		
Multilateral Agreement for the r	*					
	an too - radiately to a complete	and a contract without a	Law Martin V.			
Client RTS (RIM Test			Certificate No.	CD835V3-1011_I	Nov09	
CALIBRATION (	CERTIFICAT	E 👌 🖉 🏸			ゴラシ	
		and a second second second	uninindest, scalin	NUM ADMINISTRATION	10.495	
Object	CD835V3 - SN:	1011	12 (2) (2) (2) (2) (2) (2) (2) (2) (2) (2	Statements and Provide	199	
	and a submitted and a submitted in the			antistus anna anniaitean - con anna an	x	
Calibration procedure(s)	QA CAL-20.v4	in the deadly of	Section 1	Star and a star	感	
	Calibration proc	edure for dipoles in air		المرادي المحافظ والمستحصي المستحصي		
					昭禄	
Calibration date:	November 17, 2	009	None and the second second	NUMBER OF STREET, STREE	100 March	
Calibration date:	NOVEITIDEI 17, 2	009	Strategics, Cristina		BERGE	
This calibration certificate docum	nents the traceability to na	tional standards, which realize	the physical uni	is of measurements (SI).		
This calibration certificate docum All calibrations have been condu						
All calibrations have been condu	cted in the closed laborat					
	cted in the closed laborat					
All calibrations have been condu	cted in the closed laborat				tion	
All calibrations have been condu Calibration Equipment used (M&	cted in the closed laborat	ory facility: environment tempe	rature (22 ± 3)°C	and humidity < 70%.	ion	
All calibrations have been condu Calibration Equipment used (M& Primary Standards	TE critical for calibration)	ory facility: environment temper Gal Date (Certificate No.)	rature (22 ± 3)°C	and humidity < 70%. Scheduled Calibra	ion	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A	ID # GB37480704	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086)	rature (22 ± 3)°C	and humidity < 70%. Scheduled Calibra Oct-10	tion	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	ID # GB37480704 US37292783	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086)	rature (22 ± 3)°C	Scheduled Calibra Oct-10 Oct-10	tion	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6	ID # GB37490704 US37292783 SN: 2336	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01066) 06-Oct-09 (No. 217-01066) 22-Dec-08 (No. ER3-2336)	rature (22 ± 3)°C 	Scheduled Calibra Oct-10 Oct-10 Dec-09	tion	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01066) 06-Oct-09 (No. 217-01066) 22-Dec-08 (No. ER3-2336) 22-Dec-08 (No. ER3-2336) 22-Dec-08 (No. DAE4-781)	rature (22 ± 3)°C 	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10	tion	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID #	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336) 22-Dec-08 (No. H3-605 20-Feb-09 (No. DAE4-781) Check Date (in house)	nature (22 ± 3)°C Dec08) Dec08) Feb09)	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check		
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 44198	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB42420191	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dac-08 (No. ER3-2336) 22-Dac-08 (No. H3-6065 20-Fab-09 (No. DAE4-781) Check Date (in house) 09-Oct-09 (in house check	nature (22 ± 3)°C Dec08) Dec08) Feb09) Oct-09)	Scheduled Calibra Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: O	ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. H3-6065,- 20-Feb-09 (No. DAE4-781, Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check	(22 ± 3)°C (22 ± 3)°C (22 ± 3)°C (22 ± 03) (22 ± 03) (22 ± 03) (22 ± 03) (22 ± 03) (22 ± 03) (22 ± 03)°C	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O	ct-10 ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilant 44198 Power sensor HP 8482H Power sensor HP 8482A	ID # GB37490704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37295597	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. H3-6065,- 20-Feb-09 (No. DAE4-781, Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check	(22 ± 3)°C (0,000) (0,	Scheduled Calibra Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O	ct-10 ct-10 ct-10 ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER30V6 Probe H30V6 DAE4 Secondary Standards Power meter Agilent 44198 Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37296597 US37390585	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. H3-6065 20-Feb-09 (No. DAE4-781, Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-01 (in house check	ct-09) Cct-09) Cct-09) Cct-09) Cct-09)	Scheduled Calibra Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O	et-10 ct-10 ct-10 ct-10 ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilant 44198 Power sensor HP 8482H Power sensor HP 8482A	ID # GB37490704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37295597	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. H3-6065,- 20-Feb-09 (No. DAE4-781, Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check	ct-09) Cct-09) Cct-09) Cct-09) Cct-09)	Scheduled Calibra Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O	et-10 ct-10 ct-10 ct-10 ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER30V6 Probe H30V6 DAE4 Secondary Standards Power meter Agilent 44198 Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37296597 US37390585	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. H3-6065 20-Feb-09 (No. DAE4-781, Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-01 (in house check	ct-09) Cct-09) Cct-09) Cct-09) Cct-09)	Scheduled Calibra Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O	et-10 ct-10 ct-10 ct-10 ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER30V6 Probe H30V6 DAE4 Secondary Standards Power meter Agilent 44198 Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781 ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37296597 US37390585	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. H3-6065 20-Feb-09 (No. DAE4-781, Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-01 (in house check	ct-09) Cct-09) Cct-09) Cct-09) Cct-09)	Scheduled Calibra Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O	et-10 ct-10 ct-10 ct-10 ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilant 44198 Power sensor HP 8482A Network Analyzer HP 8482A Network Analyzer HP 8753E RF generator E4433B	ID # GB37480704 US37282783 SN: 2336 SN: 2336 SN: 6665 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37290585 MY 41000675	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. H3-6065 20-Feb-09 (No. DAE4-781) Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-01 (in house check 03-Nov-04 (in house check 03-Nov-04 (in house check	rature (22 ± 3)°C Dec08) Dec08) Feb09) Oct-09) Oct-09) Oct-09) Oct-09) Oct-09)	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O	et-10 ct-10 ct-10 ct-10 ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER30V6 Probe H30V6 DAE4 Secondary Standards Power meter Agilent 44198 Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	ID # GB37490704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37295597 US37290585 MY 41000675 Name	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. H3-6065,- 20-Feb-09 (No. DAE4-781, Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-09 (in house check 18-Oct-01 (in house check 03-Nov-04 (in house check	rature (22 ± 3)°C Dec08) Dec08) Feb09) Oct-09) Oct-09) Oct-09) Oct-09) Oct-09)	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O	et-10 ct-10 ct-10 ct-10 ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Ref generator E4433B	ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 2336 SN: 781 ID # SN: GB42420191 SN: 318A09450 SN: US37296597 US37390585 MY 41000675 Name Mike Meil	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01066) 06-Oct-09 (No. 217-01066) 22-Dec-08 (No. ER3-2336) 22-Dec-08 (No. H3-6065 20-Feb-09 (No. DAE4-781) Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-01 (in house check 03-Nov-04 (in house check Sinvor-04 (in house check Eunction	rature (22 ± 3)°C Dec08) Dec08) Dec08) Feb09) Oct-09) Oct-09) Oct-09) Oct-09) Oct-09) Atriciao	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O	et-10 ct-10 ct-10 ct-10 ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilant 44198 Power sensor HP 8482A Network Analyzer HP 8482A Network Analyzer HP 8753E RF generator E4433B	ID # GB37490704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37295597 US37290585 MY 41000675 Name	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 08-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336, 22-Dec-08 (No. H3-6065 20-Feb-09 (No. DAE4-781) Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-01 (in house check 03-Nov-04 (in house check 03-Nov-04 (in house check	rature (22 ± 3)°C Dec08) Dec08) Dec08) Feb09) Oct-09) Oct-09) Oct-09) Oct-09) Oct-09) Atriciao	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O	et-10 ct-10 ct-10 ct-10 ct-10	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Ref generator E4433B	in the closed laboral           ID #           GB37480704           US37292783           SN: 2336           SN: 2336           SN: 781           ID #           SN: GB42420191           SN: 3318A09450           SN: US37290585           MY 41000675           Name           Mike Meili           Fin Bomholt	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01066) 06-Oct-09 (No. 217-01066) 22-Dec-08 (No. ER3-2336) 22-Dec-08 (No. H3-6065 20-Feb-09 (No. DAE4-781) Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-01 (in house check 03-Nov-04 (in house check Sinvor-04 (in house check Eunction	rature (22 ± 3)°C Dec08) Dec08) Dec08) Feb09) Oct-09) Oct-09) Oct-09) Oct-09) Oct-09) Atriciao	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O Signature	ct-10 ct-10 ct-10 ct-10 ct-11	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Ref generator E4433B	in the closed laboral           ID #           GB37480704           US37292783           SN: 2336           SN: 2336           SN: 781           ID #           SN: GB42420191           SN: 3318A09450           SN: US37290585           MY 41000675           Name           Mike Meili           Fin Bomholt	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01066) 06-Oct-09 (No. 217-01066) 22-Dec-08 (No. ER3-2336) 22-Dec-08 (No. H3-6065 20-Feb-09 (No. DAE4-781) Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-01 (in house check 03-Nov-04 (in house check Sinvor-04 (in house check Eunction	rature (22 ± 3)°C Dec08) Dec08) Dec08) Feb09) Oct-09) Oct-09) Oct-09) Oct-09) Oct-09) Atriciao	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O	ct-10 ct-10 ct-10 ct-10 ct-11	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E RF generator E4433B Calibrated by: Approved by:	ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37296597 US37390585 MY 41000675 Name Mike Meil	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01066) 06-Oct-09 (No. 217-01066) 22-Dac-08 (No. ER3-2336) 22-Dac-08 (No. H3-6065 20-Fab-09 (No. DAE4-781) Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-01 (in house check 03-Nov-04 (in house check 03-Nov-04 (in house check Eurotion Laboratory Tec	rature (22 ± 3)°C ) Dec08) Dec08) Feb09) Oct-09) Oct-09) Oct-09) Oct-09) Oct-09) Stricten	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O Signature	ct-10 ct-10 ct-10 ct-10 ct-11	
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Ref generator E4433B	ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37296597 US37390585 MY 41000675 Name Mike Meil	Cal Date (Certificate No.) 06-Oct-09 (No. 217-01066) 06-Oct-09 (No. 217-01066) 22-Dac-08 (No. ER3-2336) 22-Dac-08 (No. H3-6065 20-Fab-09 (No. DAE4-781) Check Date (in house) 09-Oct-09 (in house check 09-Oct-09 (in house check 09-Oct-09 (in house check 18-Oct-01 (in house check 03-Nov-04 (in house check 03-Nov-04 (in house check Eurotion Laboratory Tec	rature (22 ± 3)°C ) Dec08) Dec08) Feb09) Oct-09) Oct-09) Oct-09) Oct-09) Oct-09) Stricten	Scheduled Calibra Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: O In house check: O In house check: O In house check: O Signature	ct-10 ct-10 ct-10 ct-10 ct-11	



NISe

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst s Service suisse d'étalonnage С Servizio svizzero di taratura s

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### References

[1]

ANSI-C63.19-2006 American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.


#### [2] ANSI-C63.19-2007 American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

#### Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with the standards [1, 2], the measurement planes (probe sensor center) are selected to be at a distance of 10 mm above the top edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections. It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY5 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a HP 8753E Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- E- field distribution: E field is measured in the x-y-plane with an isotropic ER3D-field probe with 100 mW forward power to the antenna feed point. In accordance with [1, 2], the scan area is 20mm wide, its length exceeds the dipole arm length (180 or 90mm). The sensor center is 10 mm (in z) above the top of the dipole arms. Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any non-parallelity to the measurement plane as well as the sensor displacement. The E-field value stated as calibration value represents the maximum of the interpolated 3D-E-field, 10mm above the dipole surface.
- H-field distribution: H-field is measured with an isotropic H-field probe with 100mW forward power to the antenna feed point, in the x-y-plane. The scan area and sensor distance is equivalent to the E-field scan. The maximum of the field is available at the center (subgrid 5) above the feed point. The H-field value stated as calibration value represents the maximum of the interpolated H-field, 10mm above the dipole surface at the feed point.

Certificate No: CD835V3-1011\_Nov09

Page 2 of 6



## 1 Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.2 B157
DASY PP Version	SEMCAD X	V14.0 B57
Phantom	HAC Test Arch	SD HAC P01 BA, #1070
Distance Dipole Top - Probe Center	10 mm	
Scan resolution	dx, dy = 5 mm	area = 20 x 180 mm
Frequency	835 MHz ± 1 MHz	
Forward power at dipole connector	20.0 dBm = 100mW	
Input power drift	< 0.05 dB	

#### 2 Maximum Field values

H-field 10 mm above dipole surface	condition	interpolated maximum
Maximum measured	100 mW forward power	0.464 A/m
Uncertainty for H-field measurement: 8.2% (k=2)		

I	Uncertainty	for	H-field	measurement:	8.2%	(k=2)	

E-field 10 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end-	100 mW forward power	168.6 V/m
Maximum measured above low end	100 mW forward power	157.4 V/m
Averaged maximum above arm	100 mW forward power	163.0 V/m

Uncertainty for E-field measurement: 12.8% (k=2)

#### 3 Appendix

#### 3.1 Antenna Parameters

Frequency	Return Loss	Impedance
800 MHz	15.7 dB	(44.8 – j14.9) Ohm
835 MHz	31.8 dB	(48.5 + j2.0) Ohm
900 MHz	17.7 dB	(54.3 – j12.9) Ohm
950 MHz	20.5 dB	(44.7 + j7.2) Ohm
960 MHz	16.3 dB	( 51.0 + j15.7 ) Ohm

#### 3.2 Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.

The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.

Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.


Certificate No: CD835V3-1011\_Nov09

Page 3 of 6

Testing Services™	Annex B to Hearing Aid Report for the BlackBer			Page <b>5(13)</b>
Author Data	Dates of Test	Report No	FCC ID	W
Hang Wang	July 28, Aug 4, 2011	RTS-2604-1108-06	L6ARDZ20C	


## 3.3 Measurement Sheets

#### 3.3.1 Return Loss and Smith Chart

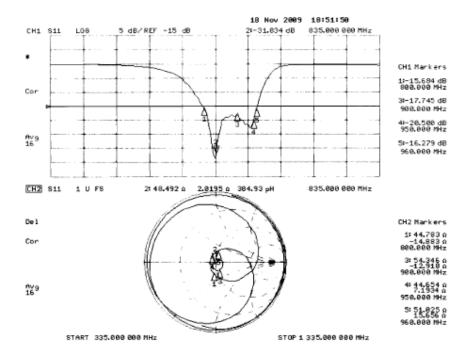

Certificate No: CD835V3-1011\_Nov09

Page 4 of 6



Author Data Hang Wang

------

## 3.3.2 DASY4 H-field Result

Date/Time: 17.11.2009 15:02:26

Test Laboratory: SPEAG Lab2

HAC RF\_CD835\_1011\_091117\_H\_MM DUT: HAC-Dipole 835 MHz; Type: D835V3; Serial: 1011 Communication System: CW; Frequency: 835 MHz Medium parameters used:  $\sigma = 0$  mho/m,  $\epsilon_r = 1$ ;  $\rho = 1$  kg/m<sup>3</sup> Phantom section: RF Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:

- Probe: H3DV6 SN6065; ; Calibrated: 22.12.2008
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 20.02.2009
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

# Dipole H-Field measurement @ 835MHz/H Scan - measurement distance from the probe sensor center to CD835 Dipole = 10mm/Hearing Aid Compatibility Test (41x361x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 0.464 A/m


Probe Modulation Factor = 1

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 0.494 A/m; Power Drift = -0.00467 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Grid 1	Grid 2	Grid 3
0.384	0.405	0.386
M4	M4	M4
Grid 4	Grid 5	Grid 6
0.441	0.464	0.439
M4	M4	M4
Grid 7	Grid 8	Grid 9
0.390	0.409	0.382
M4	M4	M4



0 dB = 0.464A/m

Certificate No: CD835V3-1011\_Nov09

Page 5 of 6



Author Data

Hang Wang

#### 3.3.3 DASY4 E-field Result

Date/Time: 17.11.2009 11:56:37

Test Laboratory: SPEAG Lab2

HAC RF\_CD835\_1011\_091117\_E\_MM DUT: HAC-Dipole 835 MHz; Type: D835V3; Serial: 1011 Communication System: CW; Frequency: 835 MHz Medium parameters used:  $\sigma = 0$  mho/m,  $\epsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: RF Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:

Probe: ER3DV6 - SN2336; ConvF(1, 1, 1); Calibrated: 22.12.2008

- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 20.02.2009
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

Dipole E-Field measurement @ 835MHz/E Scan - measurement distance from the probe sensor center to CD835 Dipole = 10mm/Hearing Aid Compatibility Test (41x361x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 168.6 V/m


Probe Modulation Factor = 1

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 109.2 V/m; Power Drift = -0.023 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field	Peak E-field in V/m					
Grid I	Grid 2	Grid 3				
152.1	157.4	154.5				
M4	M4	M4				
Grid 4	Grid 5	Grid 6				
84.1	86.8	84.5				
M4	M4	M4				
Grid 7	Grid 8	Grid 9				
165.5	168.6	158.2				
M4	M4	M4				




0 dB = 168.6V/m

Certificate No: CD835V3-1011\_Nov09

Page 6 of 6

Data Ig Wang	Dates of Test July 28,	Aug 4, 2011 RTS-	.2604-1108-06	FCC ID L6ARDZ20	CW
Calibration Laborato Schmid & Partner Engineering AG eughausstrasse 43, 8004 Zuri	-	Hac MRA (P. D. Z)	S Schweizerischer Kalibri C Service suisse d'étalon Servizio svizzero di tara S Swiss Calibration Servi	nage atura	
-		And		ce	
Accredited by the Swiss Accre The Swiss Accreditation Servio Multilateral Agreement for the	e is one of the signatori	es to the EA	ation No.: SCS 108		
client RTS (RIM Tes			te No: CD1880V3-1008	Nov09	
CALIBRATION	en.o Yordin Jan. Brish				
JALIBHAMON	JENTIFICAT			K.C. and Constant	
Object	CD1880V3 - SN	: 1008	enternet senter senter		
Calibration procedure(s)	QA CAL-20.v4 Calibration proce	edure for dipoles in air		秒 编	
Calibration date:	November 18, 2	009		197. 197.	
This calibration certificate docur All calibrations have been conde	nents the traceability to na acted in the closed laborate	009 tional standards, which realize the physic by facility: environment temperature (22	al units of measurements (SI).	197 64.	
This calibration certificate docur All calibrations have been conder Calibration Equipment used (Ma	nents the traceability to na acted in the closed laborate	tional standards, which realize the physic	al units of measurements (SI). # 3)*C and humidity < 70%.	20	
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M8 Primery Standards Power meter EPM-442A	nents the traceability to na acted in the closed laborate NTE critical for calibration)	tional standards, which realize the physic ory facility: environment temperature (22	al units of measurements (SI).	<u>201</u>	
This calibration certificate docur All calibrations have been conde Calibration Equipment used (M8 Primery Standards Power meter EPM-442A Power sensor HP 8481A	nents the traceability to na acted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783	tional standards, which realize the physic ory facility: environment temperature (22 Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086)	al units of measurements (SI). ± 3)°C and humidity < 70%. Scheduled Calibration Oct-10 Oct-10	<u>on</u>	
This calibration certificate docur All calibrations have been conde Calibration Equipment used (M& Primery Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6	ID # GB37480704 US37292783 SN: 2336	tional standards, which realize the physic sry facility: environment temperature (22 Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08)	al units of measurements (SI). # 3)°C and humidity < 70%. Scheduled Calibration Oct-10 Oct-10 Dec-09	<u>90</u>	
This calibration certificate docur All calibrations have been conde Calibration Equipment used (M& Primery Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6	nents the traceability to na acted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783	tional standards, which realize the physic ory facility: environment temperature (22 Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086)	al units of measurements (SI). ± 3)°C and humidity < 70%. Scheduled Calibration Oct-10 Oct-10	2 <b>n</b>	
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M8 Primery Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4	ID # ID # ID # ID ST222783 SN: 2336 SN: 6065	tional standards, which realize the physic ary facility: environment temperature (22 Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. H3-6065Dec08) 22-Dec-08 (No. H3-6065Dec08)	al units of measurements (SI). # 3)*C and humidity < 70%. Scheduled Calibration Oct-10 Oct-10 Dec-09 Dec-09	on	
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M8 Primery Standards Power meter EPM-442A	ID # GB37480704 US37292783 SN: 2336 SN: 781	tional standards, which realize the physic rry facility: environment temperature (22 Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08) 20-Feb-09 (No. DAE4-781_Feb09)	al units of measurements (SI). # 3)*C and humidity < 70%. Scheduled Calibration Oct-10 Oct-10 Dec-09 Dec-09 Feb-10		
This calibration certificate docur All calibrations have been conde Calibration Equipment used (Ma Primery Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H	ID # ID # ID # ID # ID 555 SN: 2336 SN: 2665 SN: 781	tional standards, which realize the physic any facility: environment temperature (22 Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. H3-6065Dac08) 22-Dec-08 (No. H3-6065Dac08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09)	al units of measurements (SI). # 3)*C and humidity < 70%. Scheduled Calibratic Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct In house check: Oct	⊨10 ⊨10	
This calibration certificate docur All calibrations have been conde Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe ER3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482A	ID # GB37480704 UD # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37295597	tional standards, which realize the physic ory facility: environment temperature (22) Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09)	al units of measurements (SI). # 3)*C and humidity < 70%. Scheduled Calibratic Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: Oct In house check: Oct In house check: Oct	-10 -10 -10	
This calibration certificate docur All calibrations have been condu Calibration Equipment used (Ma Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	ID # ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # ID # ID # ID # ID # ID # ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37295597 US37390585	tional standards, which realize the physic ory facility: environment temperature (22) Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 20-Feb-09 (No. DAE4-781_Feb09) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 18-Oct-01 (in house check Oct-09)	al units of measurements (SI). # 3)*C and humidity < 70%. Scheduled Calibratic Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct In house check: Oct In house check: Oct In house check: Oct In house check: Oct	+10 +10 +10 +10	
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	ID # GB37480704 UD # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37295597	tional standards, which realize the physic ory facility: environment temperature (22) Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. H3-6065Dec08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09)	al units of measurements (SI). # 3)*C and humidity < 70%. Scheduled Calibratic Oct-10 Oct-10 Dec-09 Feb-10 Scheduled Check In house check: Oct In house check: Oct In house check: Oct	+10 +10 +10 +10	
This calibration certificate docur All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	ID # ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # ID # ID # ID # ID # ID # ID # ID # ID # SN: GB42420191 SN: 3318A09450 SN: US37295597 US37390585	tional standards, which realize the physic ory facility: environment temperature (22) Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. ER3-2336_Dec08) 22-Dec-08 (No. ER3-2336_Dec08) 20-Feb-09 (No. DAE4-781_Feb09) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 18-Oct-01 (in house check Oct-09)	al units of measurements (SI). # 3)*C and humidity < 70%. Scheduled Calibratic Oct-10 Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct In house check: Oct In house check: Oct In house check: Oct In house check: Oct	+10 +10 +10 +10	
This calibration certificate docur All calibrations have been conde Calibration Equipment used (Ma Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe ER3DV6 DAE4 Secondary Standards Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E RF generator E4433B	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US3729597 US37390585 MY 41000675	tional standards, which realize the physic any facility: environment temperature (22 Cal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. 217-01086) 22-Dec-08 (No. H3-6065Dac08) 22-Dec-08 (No. H3-6065Dac08) 20-Feb-09 (No. DAE4-781_Feb09) Check Date (in house) 09-Oct-09 (in house check Oct-09) 09-Oct-09 (in house check Oct-09) 18-Oct-09 (in house check Oct-09) 18-Oct-01 (in house check Oct-09) 03-Nov-04 (in house check Oct-09)	al units of measurements (SI). # 3)*C and humidity < 70%. Scheduled Calibratic Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct In house check: Oct In house check: Oct In house check: Oct In house check: Oct	+10 +10 +10 +10	
This calibration certificate docur All calibrations have been condu- Calibration Equipment used (M& Primery Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards	ID # ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37295597 US37290685 MY 41000675 Name	tional standards, which realize the physic ory facility: environment temperature (22) Gal Date (Certificate No.) 06-Oct-09 (No. 217-01086) 22-Dec-08 (No. 217-01086) 22-Dec-08 (No. 217-01086) 22-Dec-08 (No. H3-6065Dec08) 20-Feb-09 (No. DAE4-781_Feb09) 09-Oct-09 (No. DAE4-781_Feb09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 09-Oct-09 (In house check Oct-09) 18-Oct-01 (In house check Oct-09) 03-Nov-04 (In house check Oct-09) 03-Nov-04 (In house check Oct-09)	al units of measurements (SI). # 3)*C and humidity < 70%. Scheduled Calibratic Oct-10 Dec-09 Dec-09 Feb-10 Scheduled Check In house check: Oct In house check: Oct In house check: Oct In house check: Oct In house check: Oct	+10 +10 +10 +10	



Hang Wang

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



ORP

- Schweizerischer Kalibrierdienst s Service suisse d'étalonnage С Servizio svizzero di taratura
- s Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### References


- ANSI-C63.19-2006 [1] American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.
- [2] ANSI-C63.19-2007 American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

#### Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with the standards [1, 2], the measurement planes (probe sensor center) are selected to be at a distance of 10 mm above the top edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections. It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY5 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a HP 8753E Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- E- field distribution: E field is measured in the x-y-plane with an isotropic ER3D-field probe with 100 mW forward power to the antenna feed point. In accordance with [1, 2], the scan area is 20mm wide, its length exceeds the dipole arm length (180 or 90mm). The sensor center is 10 mm (in z) above the top of the dipole arms. Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any non-parallelity to the measurement plane as well as the sensor displacement. The E-field value stated as calibration value represents the maximum of the interpolated 3D-E-field, 10mm above the dipole surface.
- H-field distribution: H-field is measured with an isotropic H-field probe with 100mW forward power to the antenna feed point, in the x-y-plane. The scan area and sensor distance is equivalent to the E-field scan. The maximum of the field is available at the center (subgrid 5) above the feed point. The H-field value stated as calibration value represents the maximum of the interpolated H-field, 10mm above the dipole surface at the feed point.

Certificate No: CD1880V3-1008\_Nov09

Page 2 of 6



#### 1. Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.2 B157
DASY PP Version	SEMCAD X	V14.0 B57
Phantom	HAC Test Arch	SD HAC P01 BA, #1070
Distance Dipole Top - Probe Center	10 mm	
Scan resolution	dx, dy = 5 mm	area = 20 x 90 mm
Frequency	1880 MHz ± 1 MHz	
Forward power at dipole connector	20.0 dBm = 100mW	
Input power drift	< 0.05 dB	

#### 2. Maximum Field values

H-field 10 mm above dipole surface	condition	Interpolated maximum
Maximum measured	100 mW forward power	0.471 A/m
Uncertainty for H-field measurement: 8.2% (k=2)		

E-field 10 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end	100 mW forward power	136.2 V/m
Maximum measured above low end	100 mW forward power	132.1 V/m
Averaged maximum above arm	100 mW forward power	134.2 V/m

Uncertainty for E-field measurement: 12.8% (k=2)

#### 3. Appendix

#### 3.1 Antenna Parameters

Frequency	Return Loss	Impedance
1710 MHz	22.8 dB	(52.2 + j7.1) Ohm
1880 MHz	20.0 dB	(50.5 + j10.1) Ohm
1900 MHz	20.9 dB	(53.2 + j8.8 ) Ohm
1950 MHz	29.5 dB	(52.3 + j2.6) Ohm
2000 MHz	18.7 dB	(43.2 + j8.4) Ohm

#### 3.2 Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.

The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.

Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.


Certificate No: CD1880V3-1008\_Nov09

Page 3 of 6

Testing Services™	Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RDZ21CW		Page 11(13)	
Author Data	Dates of Test	Report No	FCC ID	
Hang Wang	July 28, Aug 4, 2011	RTS-2604-1108-06	L6ARDZ20C	W


## 3.3 Measurement Sheets

#### 3.3.1 Return Loss and Smith Chart

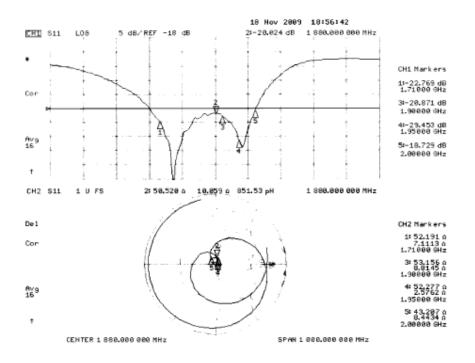

Certificate No: CD1880V3-1008\_Nov09

Page 4 of 6



Author Data Hang Wang

#### 3.3.2 DASY4 H-Field Result

Date/Time: 18.11.2009 12:32:23

Test Laboratory: SPEAG Lab2

#### HAC\_RF\_CD1880\_1008\_091118\_H\_CL DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: 1008 Communication System: CW; Frequency: 1880 MHz Medium parameters used: $\sigma = 0$ mho/m, $\varepsilon_r = 1$ ; $\rho = 1$ kg/m<sup>3</sup> Phantom section: RF Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: Probe: H3DV6 - SN6065; ; Calibrated: 22.12.2008 Sensor-Surface: (Fix Surface) ٠


- Electronics: DAE4 Sn781; Calibrated: 20.02.2009 ٠ Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

## Dipole H-Field measurement @ 1880MHz/H Scan - measurement distance from the probe sensor center to CD1880 Dipole = 10mm/Hearing Aid Compatibility Test (41x181x1):

Measurement grid: dx=5mm, dy=5mm Maximum value of peak Total field = 0.471 A/m Probe Modulation Factor = 1 Device Reference Point: 0, 0, -6.3 mm Reference Value = 0.499 A/m; Power Drift = 0.00498 dB Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak H-field in A/m


Grid I	Grid 2	Grid 3
0.408	0.423	0.398
M2	M2	M2
Grid 4	Grid 5	Grid 6
0.456	0.471	0.439
M2	M2	M2
Grid 7	Grid 8	Grid 9
0.420	0.435	0.400
M2	M2	M2



0 dB = 0.471A/m

Certificate No: CD1880V3-1008\_Nov09

Page 5 of 6



Author Data
Hang Wang

### 3.3.3 DASY4 E-Field Result

Date/Time: 18.11.2009 17:16:43

Test Laboratory: SPEAG Lab2

 $\begin{array}{l} \label{eq:hardward} \mbox{HAC_RF_CD1880_1008_091118_E_CL} \\ \mbox{DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: 1008} \\ \mbox{Communication System: CW; Frequency: 1880 MHz} \\ \mbox{Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_{c} = 1$; $\rho = 1000$ kg/m^3$ \\ \mbox{Phantom section: RF Section} \\ \mbox{Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)} \\ \mbox{DASY5 Configuration:} \\ \mbox{Probe: ER3DV6 - SN2336; ConvF(1, 1, 1); Calibrated: 22.12.2008} \\ \mbox{Sensor-Surface: (Fix Surface)} \\ \mbox{Electronics: DAE4 Sn781; Calibrated: 20.02.2009} \\ \end{array}$ 


- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- Measurement SW: DASY5, V5.2 Build 157; SEMCAD X Version 14.0 Build 57

## Dipole E-Field measurement @ 1880MHz/E Scan - measurement distance from the probe sensor center to CD1880 Dipole = 10mm/Hearing Aid Compatibility Test (41x181x1):

Measurement grid: dx=5mm, dy=5mm Maximum value of peak Total field = 136.2 V/m Probe Modulation Factor = 1 Device Reference Point: 0, 0, -6.3 mm Reference Value = 152.3 V/m; Power Drift = -0.00386 dB Hearing Aid Near-Field Category: M2 (AWF 0 dB)

Peak E-field in V/m

Grid I	Grid 2	Grid 3
124.7	132.1	131.1
M2	M2	M2
Grid 4	Grid 5	Grid 6
86.6	90.1	87.7
M3	M3	M3
Grid 7	Grid 8	Grid 9
130.7	136.2	132.2
M2	M2	M2



0 dB = 136.2V/m

Certificate No: CD1880V3-1008\_Nov09

Page 6 of 6