Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFD31CW		Page 1(7)	
Author Data	Dates of Test	Report No	FCC ID	
Andrew Becker	Feb. 29 & March 1-22, 2012	RTS-5994-1203-81	L6ARFD30C	W


# Annex B: Probe and dipole descriptions and calibration certificates

**B.2** Dipole calibration certificate

a	Dates of Test	Report No	FCC ID
w Becker	Feb. 29 & Marc	-	
Calibration Laborato	ry of	GNISS S	Schweizerischer Kalibrierdienst
Schmid & Partner			Service suisse d'étalonnage
Engineering AG		S S S	Servizio svizzero di taratura
Zeughausstrasse 43, 8004 Zuri	ch, Switzerland	Manager S	Swiss Calibration Service
Accredited by the Swiss Accredit			No.: SCS 108
The Swiss Accreditation Servi Multilateral Agreement for the	-		
Client RTS (RIM Tes	ting Services)	Contilicate No	CD835V3-1011_Nov11
CALIBRATION	CERTIFICAT		
Object	CD835V3 - SN:	1011 6 6 8 8 8 8 8	チュディティー・ト
Calibration procedure(s)	QA CAL-20.v5	E M S I B B B B B B B B	
caloration procedure(s)		edure for dipoles in air	
		8 18 1. 2. 8 A. M. M. M. M. M.	
	- 医颈连霉素	医丁丁甘草菊菊 医手	「新聞」「新聞」です。
	ments the traceability to na	tional standards, which realize the physical un	its of measurements (SI).
This calibration certificate docu The measurements and the und All calibrations have been cond	ments the traceability to na ertainties with confidence ucted in the closed laborat		its of measurements (SI). d are part of the certificate.
This calibration certificate docu The measurements and the und All calibrations have been cond Calibration Equipment used (Me	ments the traceability to na certainties with confidence ucted in the closed laborat &TE critical for calibration)	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)%	its of measurements (SI). d are part of the certificate. C and humidity < 70%.
This calibration certificate docur The measurements and the und All calibrations have been cond Calibration Equipment used (Ma Primary Standards	ments the traceability to na certainties with confidence ucted in the closed laborat &TE critical for calibration)	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)% Cal Date (Certificate No.)	its of measurements (SI). d are part of the certificate. C and humidity < 70%. Scheduled Calibration
This calibration certificate docur The measurements and the unit All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter EPM-442A	ments the traceability to na certainties with confidence ucted in the closed laborat &TE critical for calibration) ID # GB37480704	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)°0 <u>Cal Date (Certificate No.)</u> 05-Oct-11 (No. 217-01451)	its of measurements (SI). d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-12
This calibration certificate docur The measurements and the und All calibrations have been cond Calibration Equipment used (Ma Primary Standards	ments the traceability to na certainties with confidence ucted in the closed laborat &TE critical for calibration)	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)% Cal Date (Certificate No.)	its of measurements (SI). d are part of the certificate. C and humidity < 70%. Scheduled Calibration
This calibration certificate docu The measurements and the une All calibrations have been cond Calibration Equipment used (MA Primary Standards Power meter EPM-442A Power sensor HP 6481A	ments the traceability to na certainties with confidence ucted in the closed laborat &TE critical for calibration) ID # GB37480704 US37292783	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 ( No. 217-01451)	its of measurements (SI). d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12
This calibration certificate docur The measurements and the unit All calibrations have been cond Calibration Equipment used (Ma Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6	ments the traceability to na certainties with confidence ucted in the closed laborat &TE critical for calibration) ID # GB37480704 US37292783 SN: 2336	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)°0 <u>Cal Date (Certificate No.)</u> 05-Oct-11 (No. 217-01451) 05-Oct-11 ( No. 217-01451) 29-Dec-10 (No. ER3-2336_Dec10)	its of measurements (SI). d are part of the certificate. C and humidity < 70%. <u>Scheduled Calibration</u> Oct-12 Oct-12 Dec-11
This calibration certificate docu The measurements and the unit All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4	ments the traceability to na certainties with confidence ucted in the closed laborat &TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. H3-6065_Dec10) 20-Apr-11 (No. DAE4-781_Apr11)	its of measurements (SI). d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Dec-11 Dec-11 Apr-12
This calibration certificate docu The measurements and the unit All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards	ID #	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)*0 Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. H3-6065_Dec10) 20-Apr-11 (No. DAE4-781_Apr11) Check Date (in house)	its of measurements (SI). d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Dec-11 Dec-11 Apr-12 Scheduled Check
This calibration certificate docu The measurements and the unit All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4	ments the traceability to na certainties with confidence ucted in the closed laborat &TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. H3-6065_Dec10) 20-Apr-11 (No. DAE4-781_Apr11) Check Date (in house) 09-Oct-09 (in house check Oct-11)	its of measurements (SI). d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Dec-11 Dec-11 Apr-12
This calibration certificate docu The measurements and the unit All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 44198	ments the traceability to na certainties with confidence ucted in the closed laborat &TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 2336 SN: 2336 SN: 781 ID # SN: GB42420191	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)*0 Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. H3-6065_Dec10) 20-Apr-11 (No. DAE4-781_Apr11) Check Date (in house)	its of measurements (SI). d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Oct-12 Dec-11 Dec-11 Apr-12 Scheduled Check In house check: Oct-12
This calibration certificate docu The measurements and the uno All calibrations have been cond Calibration Equipment used (MA Primary Standards Power meter EPM-442A Power sensor HP B481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 44198 Power sensor HP B482H	ments the traceability to na certainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 2336 SN: 781 ID # SN: GB42420191 SN: 3318A09450	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)*0 Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. H3-6065_Dec10) 20-Apr-11 (No. DAE4-781_Apr11) Check Date (in house) 09-Oct-09 (in house check Oct-11) 09-Oct-09 (in house check Oct-11)	its of measurements (SI). d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Dec-11 Dec-11 Dec-11 Apr-12 Scheduled Check In house check: Oct-12 In house check: Oct-12
This calibration certificate docu The measurements and the und All calibrations have been cond Calibration Equipment used (Me Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe H3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 44198 Power sensor HP 8482A	ments the traceability to na certainties with confidence ucted in the closed laborat &TE critical for calibration) ID # GB37480704 US37292783 SN: 2336 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US37295597	tional standards, which realize the physical un probability are given on the following pages an ory facility: environment temperature (22 ± 3)% Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. H3-6065_Dec10) 20-Apr-11 (No. DAE4-781_Apr11) Check Date (in house) 09-Oct-09 (in house check Oct-11) 09-Oct-09 (in house check Oct-11)	its of measurements (SI). Id are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Dec-11 Dec-11 Apr-12 Scheduled Check In house check: Oct-12 In house check: Oct-12 In house check: Oct-12
This calibration certificate docur The measurements and the unit All calibrations have been cond Calibration Equipment used (Ma Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 44198 Power sensor HP 8482A Power sensor HP 8482A Network Analyzer HP 8753E RF generator E4433B	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US3729597 US37390585 MY 41000675 Name	tional standards, which realize the physical un probability are given on the following pages and ony facility: environment temperature (22 ± 3)*0 Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. H3-6065_Dec10) 20-Apr-11 (No. DAE4-781_Apr11) Check Date (in house) 09-Oct-09 (in house check Oct-11) 09-Oct-09 (in house check Oct-11) 18-Oct-01 (in house check Oct-11) 18-Oct-01 (in house check Oct-11) 03-Nov-04 (in house check Oct-11) Function	its of measurements (SI). Id are part of the certificate. C and humidity < 70%. <u>Scheduled Calibration</u> Oct-12 Oct-12 Dec-11 Dec-11 Apr-12 <u>Scheduled Check</u> In house check: Oct-12 In house check: Oct-12
This calibration certificate docu The measurements and the uno All calibrations have been cond Calibration Equipment used (Me Primary Standards Power meter EPM-442A Power sensor HP 8481A Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 44198 Power sensor HP 8482H Power sensor HP 8482A Network Analyzer HP 8753E	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US3729597 US37390585 MY 41000675	tional standards, which realize the physical un probability are given on the following pages and ony facility: environment temperature (22 ± 3)*0 Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. ER3-2336_Dec10) 20-Apr-11 (No. DAE4-781_Apr11) Check Date (in house) 09-Oct-09 (in house check Oct-11) 09-Oct-09 (in house check Oct-11) 18-Oct-01 (in house check Oct-11) 03-Nov-04 (in house check Oct-11)	its of measurements (SI). Id are part of the certificate. C and humidity < 70%. <u>Scheduled Calibration</u> Oct-12 Oct-12 Dec-11 Dec-11 Apr-12 <u>Scheduled Check</u> In house check: Oct-12 In house check: Oct-12
This calibration certificate docu The measurements and the unit All calibrations have been cond Calibration Equipment used (Ma Primary Standards Power meter EPM-442A Power sensor HP B481A Probe ER3DV6 Probe H3DV6 DAE4 Secondary Standards Power meter Agilent 44198 Power sensor HP 8482A Power sensor HP 8482A Network Analyzer HP 8753E RF generator E4433B	ID # GB37480704 US37292783 SN: 2336 SN: 6065 SN: 781 ID # SN: GB42420191 SN: 3318A09450 SN: US3729597 US37390585 MY 41000675 Name	tional standards, which realize the physical un probability are given on the following pages and ony facility: environment temperature (22 ± 3)*0 Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. ER3-2336_Dec10) 29-Dec-10 (No. H3-6065_Dec10) 20-Apr-11 (No. DAE4-781_Apr11) Check Date (in house) 09-Oct-09 (in house check Oct-11) 09-Oct-09 (in house check Oct-11) 18-Oct-01 (in house check Oct-11) 18-Oct-01 (in house check Oct-11) 03-Nov-04 (in house check Oct-11) Function	its of measurements (SI). Id are part of the certificate. C and humidity < 70%. <u>Scheduled Calibration</u> Oct-12 Oct-12 Dec-11 Dec-11 Apr-12 <u>Scheduled Check</u> In house check: Oct-12 In house check: Oct-12

Certificate No: CD835V3-1011\_Nov11

Page 1 of 6

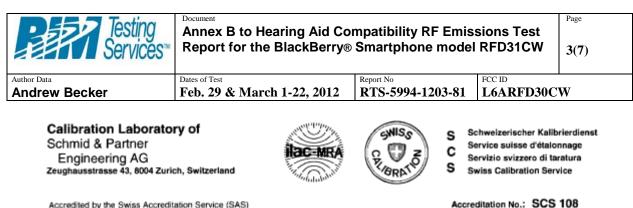

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

#### References

[1] ANSI-C63.19-2007

American National Standard for Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

### Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with the standards [1], the measurement planes (probe sensor center) are selected to be at a distance of 10 mm above the top edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All
  figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector
  is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a
  directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections. It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASYS Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a HP 8753E Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- E-field distribution: E field is measured in the x-y-plane with an isotropic ER3D-field probe with 100 mW forwarc
  power to the antenna feed point. In accordance with [1], the scan area is 20mm wide, its length exceeds the
  dipole arm length (180 or 90mm). The sensor center is 10 mm (in z) above the top of the dipole arms. Two 3D
  maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one line, the
  average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any non-parallelity
  to the measurement plane as well as the sensor displacement. The E-field value stated as calibration value
  represents the maximum of the interpolated 3D-E-field, 10mm above the dipole surface.
- H-field distribution: H-field is measured with an isotropic H-field probe with 100mW forward power to the
  antenna feed point, in the x-y-plane. The scan area and sensor distance is equivalent to the E-field scan. The
  maximum of the field is available at the center (subgrid 5) above the feed point. The H-field value stated as
  calibration value represents the maximum of the interpolated H-field, 10mm above the dipole surface at the
  feed point.

Certificate No: CD835V3-1011\_Nov11

Testing Services™	Annex B to Hearing Aid Con Report for the BlackBerry®			Page 4(7)
Author Data	Dates of Test	Report No	FCC ID	
Andrew Becker	Feb. 29 & March 1-22, 2012	RTS-5994-1203-81	L6ARFD30C	W

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	HAC Test Arch	
Distance Dipole Top - Probe Center	10 mm	
Scan resolution	dx, dy = 5 mm	
Frequency	835 MHz ± 1 MHz	
input power drift	< 0.05 dB	

# Maximum Field values

H-field 10 mm above dipole surface	condition	interpolated maximum
Maximum measured	100 mW input power	0.462 A / m ± 8.2 % (k=2)
E-field 10 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end	100 mW input power	161.2 V / m
Maximum measured above low end	100 mW input power	158.2 V / m
Averaged maximum above arm	100 mW input power	159.7 V / m ± 12.8 % (k=2)

# Appendix

## Antenna Parameters with Head TSL

Frequency	Return Loss	Impedance
800 MHz	14.5 dB	41.1 Ω - 15.0 jΩ
835 MHz	24.4 dB	48.1 Ω + 5.6 jΩ
900 MHz	16.0 dB	56.8 Ω - 15.6 jΩ
950 MHz	17.8 dB	40.7 Ω + 7.2 jΩ
960 MHz	14.6 dB	46.7 Ω + 17.9 jΩ

#### Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.

The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.


Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Certificate No: CD835V3-1011\_Nov11

Testing Services™	Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFD31CW		Page 5(7)	
Author Data	Dates of Test	Report No	FCC ID	
Andrew Becker	Feb. 29 & March 1-22, 2012	RTS-5994-1203-81	L6ARFD30C	W

# Impedance Measurement Plot

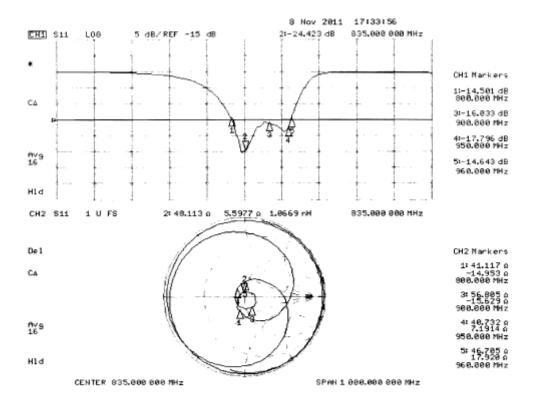

Certificate No: CD835V3-1011\_Nov11

Page 4 of 6



# DASY4 H-field Result

Date/Time: 08.11.2011 10:14:07

Test Laboratory: SPEAG Lab2

## DUT: HAC-Dipole 835 MHz; Type: CD835V3; Serial: CD835V3 - SN: 1011

Communication System: CW; Frequency: 835 MHz Medium parameters used:  $\sigma = 0$  mho/m,  $\epsilon_r = 1$ ;  $\rho = 1$  kg/m<sup>3</sup> Phantom section: RF Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)


DASY Configuration:

- Probe: H3DV6 SN6065; ; Calibrated: 29.12.2010
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 20.04.2011
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

### Dipole H-Field measurement @ 835MHz/H-Scan - 835MHz d=10mm/Hearing Aid Compatibility Test (41x361x1):

Measurement grid: dx=5mm, dy=5mm Maximum value of peak Total field = 0.462 A/m Probe Modulation Factor = 1.000 Device Reference Point: 0, 0, -6.3 mm Reference Value = 0.491 A/m; Power Drift = -0.0027 dB Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak H-field in A/m				
Grid 1	Grid 2	Grid 3		
0.372	0.396	0.381		
M4	M4	M4		
Grid 4	Grid 5	Grid 6		
0.426	0.462	0.449		
M4	M4	M4		
Grid 7	Grid 8	Grid 9		
0.375	0.410	0.399		
M4	M4	M4		



Certificate No: CD835V3-1011\_Nov11

Page 5 of 6



## DASY4 E-field Result

Date/Time: 08.11.2011 15:05:22

Test Laboratory: SPEAG Lab2

#### DUT: HAC-Dipole 835 MHz; Type: CD835V3; Serial: CD835V3 - SN: 1011

Communication System: CW; Frequency: 835 MHz Medium parameters used:  $\sigma = 0$  mho/m,  $\varepsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: RF Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)


DASY Configuration:

- Probe: ER3DV6 SN2336; ConvF(1, 1, 1); Calibrated: 29.12.2010
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 20.04.2011
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

## Dipole E-Field measurement @ 835MHz/E-Scan - 835MHz d=10mm/Hearing Aid Compatibility Test (41x361x1):

Measurement grid: dx=5mm, dy=5mm Maximum value of peak Total field = 161.2 V/m Probe Modulation Factor = 1.000 Device Reference Point: 0, 0, -6.3 mm Reference Value = 119.5 V/m; Power Drift = -7.4e-005 dB Hearing Aid Near-Field Category: M4 (AWF 0 dB)

Peak E-field in V/m			
Grid 1	Grid 2	Grid 3	
154.9	161.2	156.1	
M4	M4	M4	
Grid 4	Grid 5	Grid 6	
80.699	88.078	87.550	
M4	M4	M4	
Grid 7	Grid 8	Grid 9	
142.8	158.2	157.7	
M4	M4	M4	



Certificate No: CD835V3-1011\_Nov11

Page 6 of 6