

Annex B: Probe and dipole description and calibration certificates

B.1 Probe, measurement chain description, specification and calibration certificate

Document Annex B to Hearing Aid Compatibility RF Emissions T Report for the BlackBerry® Smartphone model RFY11			I	Page 2(14)	
Author Data Daoud Attayi	Dates of Test June 13		Report No RTS-6046-1308-24	FCC ID	RFY110LW

DASY Dosimetric Assessment System by Schmid & Partner Engineering AG

DASY Schmid & Partner Engineering AG News Sales Contact		A CONTRACT OF A
Applications	ER3DV6 ISOTRO MEASUREMENTS	PIC E-FIELD PROBE FOR GENERAL NEAR-FIELD
Support & Downloads		
Products	🛆 <u>Download Produ</u>	<u>ct Flyer</u> (PDF, 192kB)
DASV4 Packages		
EASY4 Probes ET3DV6 - Isotropic Dos-Probe ES3DV3 - Isotropic Dos-Probe	Construction	One dipole parallel, two dipoles normal to probe axis Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., glycolether)
EX3DV4 - Isotropic Dos-Probe ET1DV3 - D-Probe	Calibration	In air from 100 MHz to 3.0 GHz (absolute accuracy ±6.0%, k=2)
EUV3 - Universal Vector E-Probe	Frequency	100 MHz to > 6 GHz; Linearity: \pm 0.2 dB (100 MHz to 3 GHz)
H3DV6 - Isotropic H-Probe HUV4 - Universal Vector H-Probe T1V3 - Temp-Probe DP1 - Dummy-Probe	Directivity	± 0.2 dB in air (rotation around probe axis) ± 0.4 dB in air (rotation normal to probe axis)
• Data Acquisition System	Dynamic Range	2 V/m to > 1000 V/m; Linearity: \pm 0.2 dB
Software Phantoms Robots	Dimensions	Overall length: 330 mm (Tip: 16 mm) Tip diameter: 8 mm (Body: 12 mm) Distance from probe tip to dipole centers: 2.5 mm
 Validation Kits & Calibration Dipoles Hearing Aid Compatibility (HAC) Ext Tissue Simulating Liquids 	Application	General near-field measurements up to 6 GHz Field component measurements Fast automatic scanning in phantoms
SPEAG Home		


http://www.dasy4.com/er3.htm

Testing Services**		Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFY111LW		Page 3(14)	
Author Data Dates of Test			Report No	FCC ID	
Daoud Attayi June 13-July 04, 2013		RTS-6046-1308-24	L6A	RFY110LW	

All measurements were performed to the nearest element point as per the C63.19 standard. Offset distances were entered in the DASY5 software so that the measurement was to the nearest element.

Figures 1, provided by the manufacturer, illustrate detail of the probe tip and its dimensions.

ER3DV6 E-Field probe: The distances from the probe tip to the closest points on the dipole sensors are 1.45mm for X and Y and 1.25mm for Z. From the probe tip to the center of the sensors is 2.5mm.

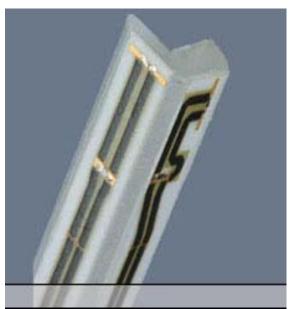

E-Field Probe (ER3DV6)

Testing Services**		Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFY111LW			Page 4(14)
Author Data Dates of Test Daoud Attayi June 13		-July 04, 2013	Report No RTS-6046-1308-24	FCC ID	RFY110LW

The following information is from the system manufacturer user manual describing the process chain:

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$
(20.1)

with	V_i	= compensated signal of channel i	(i = x, y, z)
	U_i	= input signal of channel i	(i = x, y, z)
	cf	= crest factor of exciting field	(DASY parameter)
	dcp_i	= diode compression point	(DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

	$\mathrm{E-field probes}$:	$E_i = \sqrt{\frac{V_i}{Norm_i \cdot c}}$	ConvF
	${ m H}-{ m field probes}$:	$H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}}{2}$	$\frac{f + a_{i2}f^2}{f}$
with	= compensated signal of c = sensor sensitivity of cha $\mu V/(V/m)^2$ for E-field = sensitivity enhancement = sensor sensitivity factor = carrier frequency [GHz] = electric field strength of = magnetic field strength	nnel i l Probes t in solution s for H-field probes f channel i in V/m	$\begin{array}{l} (i=x,y,z) \\ (i=x,y,z) \end{array}$

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$
(20.2)

The measurement / integration time per point is > 500 ms, as per the system manufacturer:

The time response of the field probes has been assessed by exposing the probe to a well-controlled field producing signals larger than HAC E- and H-fields of class M4. The signal response time is evaluated as the time required by the system to reach 90% of the expected final value after an on/off switch of the power source with an integration time of 500 ms and a probe response time of <5 ms. In the current implementation, DASY4 waits longer than 100 ms after having reached the grid point before starting a measurement, i.e., the response time uncertainty is negligible.

If the device under test does not emit a CW signal, the integration time applied to measure the electric field at a specific point may introduce additional uncertainties due to the discretization. The tolerances for the different systems had the worst-case of 2.6%.

THE REPORT OF THE REPORT OF	vices		• ·	bility RF Emissions Tea tphone model RFY111		5(14)
	Dates of Test			Report No	FCC ID	
d Attayi	June 13-	July 04, 20	13	RTS-6046-1308-24	L6A	RFY110LV
			, .			
Calibration La Schmid & Partr Engineering A Zeughausstrasse 43,	ner AG		HAC MEA	Service suisse d'étalonnage		
Accredited by the Swis The Swiss Accreditat Multilateral Agreemer	tion Service is c	one of the signatorie	s to the EA	n No.: SCS 108		
	IM Testing			o: ER3-2286_jan13		
CALIBRAT	ION CE	RTIFICATI	1			
Object	Ê	R3DV6 - SN:22	86			
Calibration procedure	C	A CAL-02.v6, C alibration proce valuations in air	dure for E-field probes optimize	for close near field		
Calibration date:	J	anuary 11, 2013	J			
1						
The measurements ar	nd the uncertaint	ties with confidence p	anal standards, which realize the physical unrobability are given on the following pages a y facility: environment temperature (22 ± 3) ⁴	nd are part of the certificate.		
The measurements an All calibrations have b	nd the uncertaint	ties with confidence p	robability are given on the following pages a	nd are part of the certificate. C and humidity < 70%.		
The measurements an All cellibrations have b Calibration Equipment Primary Standards	nd the uncertaint been conducted i it used (M&TE cr	ties with confidence p in the closed laborator ritical for calibration)	robability are given on the following pages a y facility: environment temperature (22 ± 3) ⁴ Cal Date (Certificate No.)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration		
The measurements an All calibrations have b Calibration Equipment Primary Standards Power meter E44198	nd the uncertaint been conducted i it used (M&TE or ID 3 GE	ties with confidence p in the closed laborator (tical for calibration) 341293874	robability are given on the following pages a y facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 29-Mar-12 (No. 217-01508)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-13		
The measurements an All celibrations have b Calibration Equipment Primary Standards Power meter E44198 Power sensor E4412	nd the uncertaint been conducted i at used (M&TE or ID 3 GE 2A M1	ties with confidence p in the closed laborator (tical for calibration) 341293874 (41498087	cobability are given on the following pages a y facility: environment temperature (22 ± 3) ⁴ Cal Date (Certificate No.) 29-Mar-12 (No. 217-01508) 29-Mar-12 (No. 217-01508)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration		
The measurements an All calibrations have b Calibration Equipment Primary Standards Power meter E44198	nd the uncertaint been conducted i at used (M&TE or ID 3 GE 24 MT nuator SN	ties with confidence p in the closed laborator (tical for calibration) 341293874	robability are given on the following pages a y facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 29-Mar-12 (No. 217-01508)	A are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-13 Apr-13		
The measurements ar All calibrations have b Calibration Equipment Primary Standards Power meter E44198 Power sensor E4412 Reference 3 dB Atter Reference 3 dB Atter Reference 30 dB Atte	nd the uncertaint seen conducted in trused (M&TE or ID 3 GE 9 M Muator SN enuator SN enuator SN	ties with confidence p in the closed laborator itical for calibration) 341293874 (41498087 4: 55054 (3c) 4: 55086 (20b) 4: 55129 (30b)	Cal Date (Certificate No.) 29-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01508)	A pr-13 Apr-13 Apr-13 Apr-13 Apr-13 Apr-13 Apr-13		
The measurements ar All celibrations have b Calibration Equipment Primary Standards Power meter E44198 Power sensor E4419 Reference 3 dB Atter Reference 20 dB Atte Reference 30 dB Atter Reference Probe ER	nd the uncertaint been conducted it it used (M&TE or ID 3 GE 20 M 20 M 20 M 20 SN enuator SN enuator SN enuator SN enuator SN enuator SN	ties with confidence p in the closed laborator itical for calibration) 341293874 (41498087 4: \$5054 (3c) 4: \$5054 (3c) 4: \$5129 (30b) 4: \$5129 (30b)	cal Date (Certificate No.) 29-Mar-12 (No. 217-01508) 29-Mar-12 (No. 217-01508) 29-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01529) 27-Mar-12 (No. 217-01529) 27-Mar-12 (No. 217-01522) 27-Mar-12 (No. 217-01522)	Apr-13 Oct-13		
The measurements ar All calibrations have b Calibration Equipment Primary Standards Power meter E44198 Power sensor E4412 Reference 3 dB Atter Reference 3 dB Atter Reference 30 dB Atte	nd the uncertaint been conducted it it used (M&TE or ID 3 GE 20 M 20 M 20 M 20 SN enuator SN enuator SN enuator SN enuator SN enuator SN	ties with confidence p in the closed laborator itical for calibration) 341293874 (41498087 4: 55054 (3c) 4: 55086 (20b) 4: 55129 (30b)	Cal Date (Certificate No.) 29-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01508)	A pr-13 Apr-13 Apr-13 Apr-13 Apr-13 Apr-13 Apr-13		
The measurements ar All celibrations have b Calibration Equipment Primary Standards Power meter E44198 Power sensor E4419 Reference 3 dB Atter Reference 20 dB Atte Reference 30 dB Atter Reference Probe ER	nd the uncertaint been conducted if at used (M&TE or ib) 3 GE ba MN houstor SN enuator SN enuator SN s0V6 SN SN	ties with confidence p in the closed laborator (tical for calibration) 341293874 (41498087 4: \$5054 (3c) 4: \$5054 (3c) 4: \$5086 (20b) 4: \$5129 (30b) 4: \$328 4: 789	cal Date (Certificate No.) 29-Mar-12 (No. 217-01508) 29-Mar-12 (No. 217-01508) 29-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01529) 27-Mar-12 (No. 217-01529) 27-Mar-12 (No. 217-01522) 27-Mar-12 (No. 217-01522)	Apr-13 Oct-13		
The measurements ar All collibrations have b Calibration Equipment Primary Standards Power meter E4419B Power sensor E4412 Reference 30 dB Atter Reference 30 dB Atte Reference 30 dB Atte Reference Probe ER DAE4	nd the uncertaint been conducted i at used (M&TE or iD 3 GE 3 GE 3 GE 4A MN nuator SN enuator SN enuator SN enuator SN s3DV6 SN s ID	ties with confidence p in the closed laborator (tical for calibration) 341293874 (41498087 4: \$5054 (3c) 4: \$5054 (3c) 4: \$5086 (20b) 4: \$5129 (30b) 4: \$328 4: 789	coability are given on the following pages a y facility: environment temperature (22 ± 3) ⁴ Cal Date (Certificate No.) 29-Mar-12 (No. 217-01508) 29-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01531) 27-Mar-12 (No. 217-01529) 27-Mar-12 (No. 217-01532) 12-Oci-12 (No. ER3-2326_Oci12) 18-Sep-12 (No. DAE4-789_Sep12)	A are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-13 Apr-13 Apr-13 Apr-13 Apr-13 Oct-13 Sep-13 Sep-13		
The measurements ar All collibrations have b Calibration Equipment Primary Standards Power meter E44198 Power sensor E4412 Reference 3 dB Atter Reference 30 dB Atter Reference 20 dB Atter Reference Probe ER DAE4 Secondary Standards	nd the uncertaint been conducted i at used (M&TE or ID 3 GE 2A MT nuator SN enuator SN enuator SN enuator SN enuator SN enuator SN enuator SN enuator SN enuator SN s ID 48C US	ties with confidence p in the closed laborator itical for calibration) 341293874 (41498087 4: 55054 (3c) 4: 55086 (20b) 4: 55129 (30b) 4: 2328 4: 789	coability are given on the following pages a y facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 29-Mar-12 (No. 217-01508) 29-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01529) 27-Mar-12 (No. 217-01529) 27-Mar-12 (No. 217-01532) 12-Oci-12 (No. ER3-2382_Oct12) 18-Sep-12 (No. DAE4-789_Sep12) Check Date (in house)	A are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-13 Apr-13 Apr-13 Apr-13 Apr-13 Oct-13 Sep-13 Scheduled Check		
The measurements ar All collibrations have b Calibration Equipment Primary Standards Power meter E44198 Power sensor E4412 Reference 30 dB Atte Reference 30 dB Atte Reference 70 dB Atte Reference Probe ER DAE4 Secondary Standards RF generator HP 864	nd the uncertaint been conducted if it used (M&TE or ID) 3 GE 3 GE 3 GE 4A MN nuator SN enuator SN enuator SN sautor SN sb s ID 48C US 2 8763E US	ties with confidence p in the closed laborator itical for calibration) 341293874 (41498087 4: \$5054 (3c) 4: \$5086 (20b) 4: \$5129 (30b) 4: \$5129 (30b) 4: \$789 \$3842U01700	coability are given on the following pages a y facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 29-Mar-12 (No. 217-01508) 29-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01531) 27-Mar-12 (No. 217-01532) 12-Oct-12 (No. ER3-2326_Oct12) 18-Sep-12 (No. DAE4-789_Sep12) Check Date (in house) 4-Aug-99 (in house check Apr-11)	A are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-13 Apr-13 Apr-13 Apr-13 Apr-13 Oct-13 Sep-13 Scheduled Check In house check: Apr-13		
The measurements ar All collibrations have b Calibration Equipment Primary Standards Power meter E44199 Power sensor E4412 Reference 30 dB Atter Reference 30 dB Atter Reference 20 dB Atte Reference Probe ER DAE4 Secondary Standardt RF generator HP 864 Network Analyzer HP	nd the uncertaint been conducted i at used (M&TE or iD 3 GE bA MN nuator SN enuator SN enuator SN enuator SN s ID 3 SN s ID 48C US 2 8763E US	ties with confidence p in the closed laborator (tical for calibration) 341293874 (41498087 4: 55054 (3c) 4: 55054 (3c) 4: 55056 (20b) 4: 5329 (30b) 4: 5328 4: 789 33842U01700 337390585 Name	coability are given on the following pages a y facility: environment temperature (22 ± 3)* Cal Date (Certificate No.) 29-Mar-12 (No. 217-01508) 29-Mar-12 (No. 217-01508) 29-Mar-12 (No. 217-01508) 27-Mar-12 (No. 217-01531) 27-Mar-12 (No. 217-01532) 12-Oci-12 (No. ER3-2328_Oci12) 18-Sep-12 (No. DAE4-789_Sep12) Check Date (in house) 4-Aug-99 (in house check Apr-11) 18-Oci-01 (in house) Function	A are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-13 Apr-13 Apr-13 Apr-13 Apr-13 Oct-13 Sep-13 Scheduled Check In house check: Oct-13 In house check: Oct-13		

Certificate No: ER3-2286_Jan13

Page 1 of 10



Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFY111LW

S

С

S

Page

Author Data Daoud Attayi Dates of Test June 13-July 04, 2013

Document

Report No RTS-6046-1308-24 FCC ID

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

Giussary.	
NORMx,y,z	sensitivity in free space
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization ϕ	φ rotation around probe axis
Polarization 8	8 rotation around an axis that is in the plane normal to probe axis (at measurement center),
	i.e., 9 = 0 is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

 a) IEEE Std 1309-2005, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", December 2005

b) CTIA Test Plan for Hearing Aid Compatibility, April 2010.

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 for XY sensors and 9 = 90 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart).
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: ER3-2286_Jan13

Page 2 of 10

Author Data		Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFY111LW		Page 7(14)
Author Data Dates of Test Daoud Attayi June 13-July 04, 2013		Report No RTS-6046-1308-24	FCC ID	RFY110LW

January 11, 2013

Probe ER3DV6

SN:2286

Manufactured: Calibrated: September 18, 2002 January 11, 2013

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: ER3-2286_ Jan13

Page 3 of 10



Author Data	Dates of Test	Report No	FCC ID
Daoud Attayi	June 13-July 04, 2013	RTS-6046-1308-24	L6ARFY110LW

January 11, 2013

DASY/EASY - Parameters of Probe: ER3DV6 - SN:2286

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) ²)	2.20	1.47	1.51	± 10.1 %
DCP (mV) ^B	98.4	100.5	99.6	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dBõV	с	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	194.1	±2.5 %
		Y	0.0	0.0	1.0		197.9	
		Z	0.0	0.0	1.0		176.0	


The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^B Numerical linearization parameter: uncertainty not required.
^E Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFY111LW				Page 9(14)	
Author Data	Dates of Test		Report No	FCC ID	
Daoud Attayi	June 13	June 13-July 04, 2013 RTS-6046-1308-24 L6A			RFY110LW

January 11, 2013

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

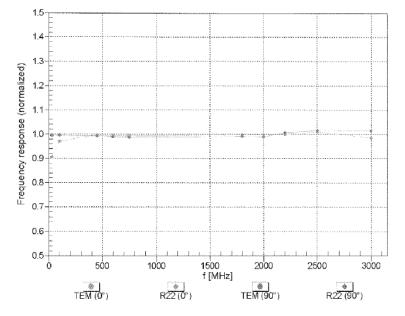




Certificate No: ER3-2286_Jan13

Page 5 of 10


lesting A		Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFY111LW		I	Page 10(14)
Author Data Daoud Attayi	Dates of Test June 13-July 04, 2013		Report No RTS-6046-1308-24	FCC ID	RFY110LW

January 11, 2013

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

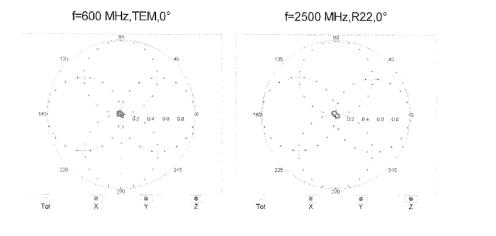

Receiving Pattern (ϕ), $\vartheta = 90^{\circ}$

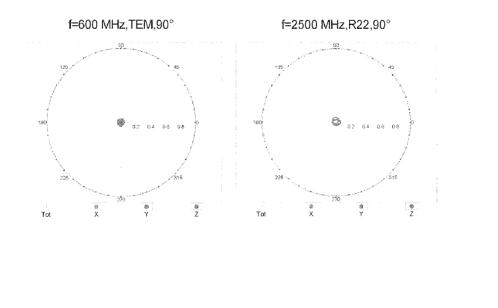


Certificate No: ER3-2286_Jan13


Page 6 of 10

lesting		Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFY111LW		Page 11(14)	
Author Data Daoud Attayi	/i June 13-July 04, 2013		Report No RTS-6046-1308-24	FCC ID	RFY110LW


January 11, 2013

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

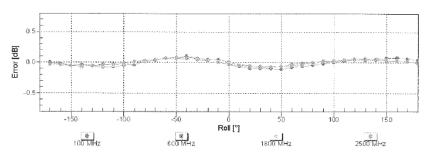



Receiving Pattern (ϕ), $\vartheta = 90^{\circ}$

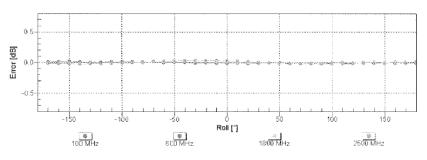


Uncertainty of Axial Isotropy Assessment: \pm 0.5% (k=2)

Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFY111LW				Page 12(14)	
Author Data Daoud Attayi	Dates of Test June 13-July 04, 2013		Report No RTS-6046-1308-24	FCC ID	RFY110LW

January 11, 2013

Dynamic Range f(E-field) (TEM cell , f = 900 MHz)

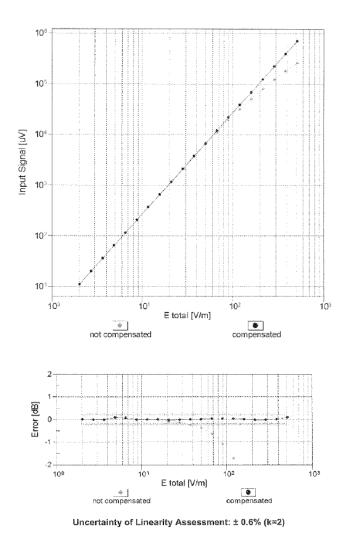


Certificate No: ER3-2286_Jan13


Page 8 of 10

This report shall <u>NOT</u> be reproduced except in full without the written consent of RTS Copyright 2005-2013, RTS, a division of BlackBerry Limited

Document Annex B to Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RFY111LW			Page 13(14)		
Author Data Daoud Attayi	Dates of Test June 13-July 04, 2013		Report No RTS-6046-1308-24	FCC ID	RFY110LW

January 11, 2013





Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ER3-2286_Jan13

Page 9 of 10



Author DataDates of TestReport NoFCC IDDaoud AttayiJune 13-July 04, 2013RTS-6046-1308-24L6ARFY110LW

ER3DV6-- SN:2286

January 11, 2013

DASY/EASY - Parameters of Probe: ER3DV6 - SN:2286

Other Probe Parameters

Sensor Arrangement	Rectangular
Connector Angle (°)	-10.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	8 mm
Probe Tip to Sensor X Calibration Point	2.5 mm
Probe Tip to Sensor Y Calibration Point	2.5 mm
Probe Tip to Sensor Z Calibration Point	2.5 mm

Certificate No: ER3-2286_Jan13

Page 10 of 10