BlackBerry RTS		Hearing Aid Compatibility the BlackBerry® Smartph	Page 1(14)	
Author Data Dates of Test		Report No	Auf	hor Data
Daoud Attayi	Sep. 19-20, 2	013 RTS-6	6050-1309-28 Da	aoud Attayi

# Annex B: Probe and dipole description and calibration certificates

B.1 Probe, measurement chain description, specification and calibration certificate

Document

Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

Report No

Page

2(14)

Author Data

Daoud Attayi

Dates of Test

Sep. 19-20, 2013


RTS-6050-1309-28

Author Data

Daoud Attayi

DASY Dosimetric Assessment System by Schmid & Partner Engineering AG



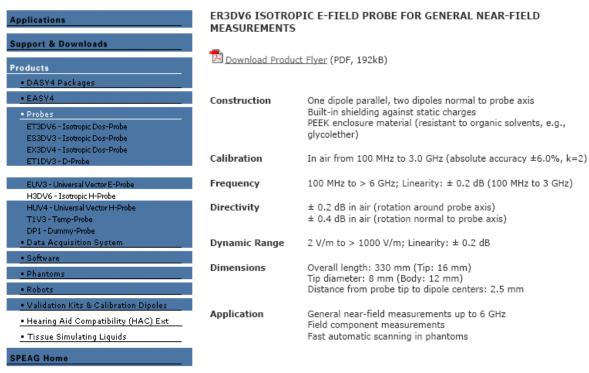


http://www.dasy4.com/er3.htm

BlackBerry RTS		Hearing Aid Compa the BlackBerry® Sm	Page 3(14)		
Author Data			Report No	Author	
Daoud Attayi	Sep. 19-20, 2	2013	RTS-6050-1309-28 Dag		ud Attayi

All measurements were performed to the nearest element point as per the C63.19 standard. Offset distances were entered in the DASY5 software so that the measurement was to the nearest element.

Figures 1, provided by the manufacturer, illustrate detail of the probe tip and its dimensions.

**ER3DV6** E-Field probe: The distances from the probe tip to the closest points on the dipole sensors are 1.45mm for X and Y and 1.25mm for Z. From the probe tip to the center of the sensors is 2.5mm.

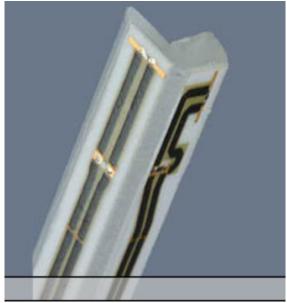

E-Field Probe (ER3DV6)

Document

# Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

Report No

Page

4(14)

Author Data

Daoud Attayi

Dates of Test **Sep. 19-20, 2013** 

RTS-6050-1309-28

Author Data

Daoud Attayi

The following information is from the system manufacturer user manual describing the process chain:

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$
(20.1)

From the compensated input signals the primary field data for each channel can be evaluated:

E – field probes :  $E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$ 

 ${
m H-field probes}$  :  $H_i = \sqrt{V_i} \cdot rac{a_{i0} + a_{i1}f + a_{i2}f^2}{f}$ 

with  $V_i$  = compensated signal of channel i (i = x, y, z)  $Norm_i$  = sensor sensitivity of channel i (i = x, y, z)

 $\mu V/(V/m)^2$  for E-field Probes

ConvF = sensitivity enhancement in solution

 $a_{ij}$  = sensor sensitivity factors for H-field probes

f = carrier frequency [GHz]

 $E_i$  = electric field strength of channel i in V/m  $H_i$  = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$
(20.2)

The measurement / integration time per point is > 500 ms, as per the system manufacturer:

The time response of the field probes has been assessed by exposing the probe to a well-controlled field producing signals larger than HAC E- and H-fields of class M4. The signal response time is evaluated as the time required by the system to reach 90% of the expected final value after an on/off switch of the power source with an integration time of 500 ms and a probe response time of <5 ms. In the current implementation, DASY4 waits longer than 100 ms after having reached the grid point before starting a measurement, i.e., the response time uncertainty is negligible.

If the device under test does not emit a CW signal, the integration time applied to measure the electric field at a specific point may introduce additional uncertainties due to the discretization. The tolerances for the different systems had the worst-case of 2.6%.

#### Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

Page

5(14)

Author Data **Daoud Attavi**  Dates of Test

Sep. 19-20, 2013

Report No RTS-6050-1309-28 Author Data **Daoud Attayi** 

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdlenst Service suisse d'étalonnage С Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

RTS (RIM Testing Services)

Accreditation No.: SCS 108

Certificate No: ER3-2286\_Jan13

#### CALIBRATION CERTIFICATE

Object ER3DV6 - SN:2286

Calibration procedure(s)

QA CAL-02,v6, QA CAL-25,v4

Calibration procedure for E-field probes optimized for close near field

Calibration date: January 11, 2013

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%

Calibration Equipment used (M&TE critical for calibration)

			0.1.1.10.25
Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Catibration
Power meter E44198	GB41293874	29-Mar-12 (No. 217-01508)	Apr-13
Power sensor E4412A	MY41498087	29-Mar-12 (No. 217-01508)	Apr-13
Reference 3 dB Attenuator	SN: S5054 (3c)	27-Mar-12 (No. 217-01531)	Apr-13
Reference 20 dB Attenuator	SN: S5086 (20b)	27-Mar-12 (No. 217-01529)	Apr-13
Reference 30 dB Attenuator	SN: S5129 (30b)	27-Mar-12 (No. 217-01532)	Apr-13
Reference Probe ER3DV6	SN: 2328	12-Oct-12 (No. ER3-2328_Oct12)	Oct-13
DAE4	SN: 789	18-Sep-12 (No. DAE4-789_Sep12)	Sep-13
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-11)	in house check: Apr-13
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-12)	In house check: Oct-13

Name Function Signature Calibrated by: Jeton Kastrati Laboratory Technician Technical Manager Katja Pokovic Approved by: Issued: January 11, 2013 This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Page 1 of 10 Certificate No: ER3-2286\_Jan13

#### Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

Page

6(14)

Author Data Daoud Attavi Dates of Test

Sep. 19-20, 2013

Report No RTS-6050-1309-28

С

Author Data Daoud Attavi

Calibration Laboratory of

Certificate No: ER3-2286\_Jan13

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

NORMx, y, zsensitivity in free space DCP diode compression point

crest factor (1/duty\_cycle) of the RF signal CF A, B, C, D modulation dependent linearization parameters

Polarization () o rotation around probe axis

Polarization 8 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., 9 = 0 is normal to probe axis

information used in DASY system to align probe sensor X to the robot coordinate system Connector Angle

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1309-2005, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", December 2005
- b) CTIA Test Plan for Hearing Aid Compatibility, April 2010.

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 for XY sensors and 9 = 90 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart).
- DCPx,v,z; DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Page 2 of 10

Document

Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

7(14)

Author Data

Daoud Attavi

Dates of Test

Sep. 19-20, 2013

Report No **RTS-6050-1309-28** 

Author Data

Daoud Attayi

Page

ER3DV6 - SN:2286

January 11, 2013

# Probe ER3DV6

SN:2286

Manufactured: Calibrated:

September 18, 2002 January 11, 2013

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: ER3-2286\_Jan13

Page 3 of 10

Document

# Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

Page

8(14)

Author Data

Daoud Attayi

Dates of Test **Sep. 19-20, 2013** 

Report No RTS-6050-1309-28 Author Data

Daoud Attayi

ER3DV6- SN:2286

January 11, 2013

### DASY/EASY - Parameters of Probe: ER3DV6 - SN:2286

**Basic Calibration Parameters** 

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m) <sup>2</sup> )	2.20	1.47	1.51	± 10.1 %
DCP (mV) <sup>B</sup>	98.4	100.5	99.6	

Modulation Calibration Parameters

UID	Communication System Name		Α	В	€	D	VR	Unc
			dΒ	dB√μV		dB	mV	(k=2)
0	CW	X	0.0	0.0	1.0	0.00	194.1	±2.5 %
		Υ	0.0	0.0	1.0		197.9	
		Z	0.0	0.0	1.0		176.0	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

B Numerical linearization parameter: uncertainty not required.

E. Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Document

Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

9(14)

Page

Author Data

Daoud Attayi

Dates of Test

Sep. 19-20, 2013

Report No **RTS-6050-1309-28** 

Author Data


Daoud Attayi

ER3DV6- SN:2286

January 11, 2013

### Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

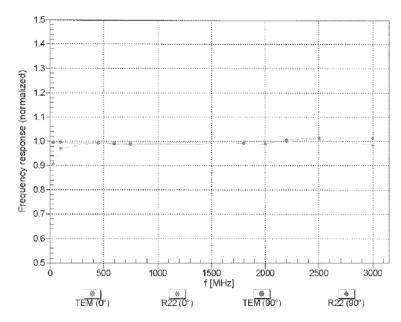

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: ER3-2286\_Jan13

Page 5 of 10

Document

Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

.

10(14)

Author Data

Daoud Attayi

Dates of Test **Sep. 19-20, 2013** 

Report No RTS-6050-1309-28 Author Data

Daoud Attayi

ER3DV6-- SN:2286

January 11, 2013


### Receiving Pattern ( $\phi$ ), $9 = 0^{\circ}$


f=600 MHz,TEM,0°

180 62 64 08 00 9

f=2500 MHz,R22,0°

### Receiving Pattern ( $\phi$ ), $\theta$ = 90°





Certificate No: ER3-2286\_Jan13

Page 6 of 10

Document

Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

11(14)

Page

Author Data

Daoud Attayi

Dates of Test

Sep. 19-20, 2013

Report No RTS-6050-1309-28


Author Data

Daoud Attayi

ER3DV6-- SN:2286


January 11, 2013

### Receiving Pattern ( $\phi$ ), $9 = 0^{\circ}$

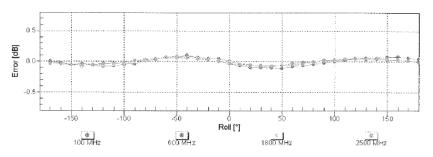

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

### Receiving Pattern ( $\phi$ ), $\vartheta = 90^{\circ}$

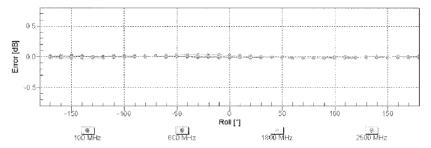

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ER3-2286\_Jan13

Page 7 of 10

Document

Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

Page

12(14)

Author Data

Daoud Attayi

Dates of Test **Sep. 19-20, 2013** 

Report No RTS-6050-1309-28 Author Data


Daoud Attayi


ER3DV6- SN:2286

January 11, 2013

### Dynamic Range f(E-field)

(TEM cell , f = 900 MHz)

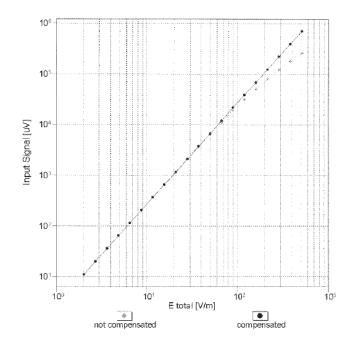



Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: ER3-2286\_Jan13

Page 8 of 10

Document

Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

Page

the BlackBerry® Smartphone model RGF111LW 13(14)

Data Dates of Test Report No Author Data

Author Data

Daoud Attayi

Dates of Test **Sep. 19-20, 2013** 

RTS-6050-1309-28

Author Data


Daoud Attayi

ER3DV6- SN:2286

January 11, 2013

### Deviation from Isotropy in Air

Error (6, 8), f = 900 MHz

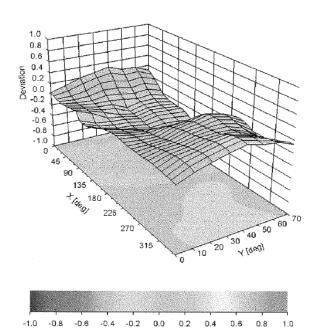

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ER3-2286\_Jan13

Page 9 of 10

Document

# Hearing Aid Compatibility RF Emissions Test Report for the BlackBerry® Smartphone model RGF111LW

Page

14(14)

Author Data

Daoud Attayi

Dates of Test **Sep. 19-20, 2013** 

Report No **RTS-6050-1309-28** 

Author Data

Daoud Attayi

ER3DV6-- SN:2286

January 11, 2013

#### DASY/EASY - Parameters of Probe: ER3DV6 - SN:2286

#### Other Probe Parameters

Sensor Arrangement	Rectangular
Connector Angle (°)	-10.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	8 mm
Probe Tip to Sensor X Calibration Point	2.5 mm
Probe Tip to Sensor Y Calibration Point	2.5 mm
Probe Tip to Sensor Z Calibration Point	2.5 mm

Certificate No: ER3-2286\_Jan13

Page 10 of 10