

UC200101312b EN / PN220335-002

8840 Programmer – Label Placement



The following documentation includes a letter from the FCC accepting that the compliance statement for a product similar to this product (FCC ID: LF57435) was not on the label, but in the User's Manual.

If this is not acceptable by the TCB for the unit we are currently submitting application for (FCC ID: LF58840), please request a ruling from the FCC.

CONTROLLED **NEUROLOGICAL DIVISION** DOCUMENT/RECORD When Life Depends on Medical Technology PROJECT NO: REV. NO. RECORD DESCRIPTION MODEL OR BUCKET NO. RECORD NO. 690013 N1019 FCC Approval Letter for Labeling 7434 Exemption (00010 DHF 🖂 PMR 🔲 PHR 🗌 TYPE OF RECORD: Federal Communications Commission SUBMITTED BY: J. Grevious **AUTHOR:** ASSOCIATING RECORD: Models Affected: 7435, 7436, 3031A, 3032A. **DOCUMENT/RECORD HISTORY:** FCC approval letter with attached letter of request submitted to FCC to support design of universal labels for Patient Programmers. **AUTHORIZATION SIGNATURES SIGNATURE** DATE NAME **FUNCTION TITLE** John Grevious Design

NOTIFICATION OF COMPLETION

NAME	NAME
Eric Bonde	
Wynee Igel	

JUL. 1.1999 3:26PM CONG



FEDERAL COMMUNICATIONS COMMISSION

Laboratory Division, Equipment Authorization Branch 7435 Oakland Mills Road, Columbia, MD 21046 Telephone: (301) 362-3027, Facsimile: (301) 344-2050 July 1, 1999

TO: John Grevious

ORGANIZATION: Medtronic, Inc.

PHONE NUMBER: 612-514-5210

FAX NUMBER: 612-514-5612

FROM: Richard Fabina

NO. OF PAGES: 1

TITLE: Acting Chief, Equipment Authorization Branch

Please direct inquiries, if any, to the sender at the telephone number above.

Dear Mr. Grevious:

The following is in response to your faxes of May 28 and June 30, 1999, regarding proposed labeling changes to a device identified by FCC ID: LF57435. In the referenced communication, you ask if it is permissible to move the compliance statement required by Section 15.19(a)(3) of the FCC Rules from the label of the device to the user's manual. I apologize for the delay in answering this simple question. Apparently, the May 28th incoming correspondence was lost in our volume of paperwork.

Yes, it is acceptable to place the compliance statement in the user's manual of a device in accordance with Section 15.19(a)(5) of the Rules when the device is so small, or it is not practical, to place the compliance statement on it. We concur that this device meets this criteria to permit the compliance statement to be located in the user's manual.

I trust that this has answered your questions. However, if you have any additional questions about this matter, please contact me at the address or telephone numbers above.



Medtronic Neurological 800 53rd Avenue NE P.O. Box 1250 Minneapolis, MN 55440-9087 Internet: www.medtronic.com Telephone: (612) 514-5000 Toll Free: 1-800-328-0810

FAX: (612) 514-5078

Richard Fabina Federal Communications Commission Washington, D.C. 20554

May 28, 1999

Dear Mr. Fabina:

The purpose of this letter is to determine if we may be exempted from placing the FCC part 15 statement ("This device complies with...") on the labels of our hand held patient programmers. These programmers are best categorized as inefficient radiators that use short-range inductive coupling (i.e. within a few inches) at 175 kHz to communicate to implanted medical devices.

Presently we print both the FCC ID# and the FCC part 15 statement on both the device label and in the manual. We wish to make a universal label for worldwide use. The label designers require more print space on the label to accomplish this task. I understand such exemptions can be applied to other devices such as hearing aids where obvious space/size restrictions become an issue. In our case we have maximized the label size and use it for both user instruction and industry standards information. Please refer to the attached edited drawings (A, B, C1, C2, D) for an overview of this product and to better understand this request.

To meet the FCC labeling requirements and achieve our universal labeling needs we are requesting allowance to apply the FCC information per attachment D for our patient programmer products. Thank you for your time to review this request.


Sincerely,

John Grevious Principal Engineer Medtronic, Inc.


Phone: (612) 514-5210 Fax: (612) 514-5612

e-mail john.grevious@medtronic.com



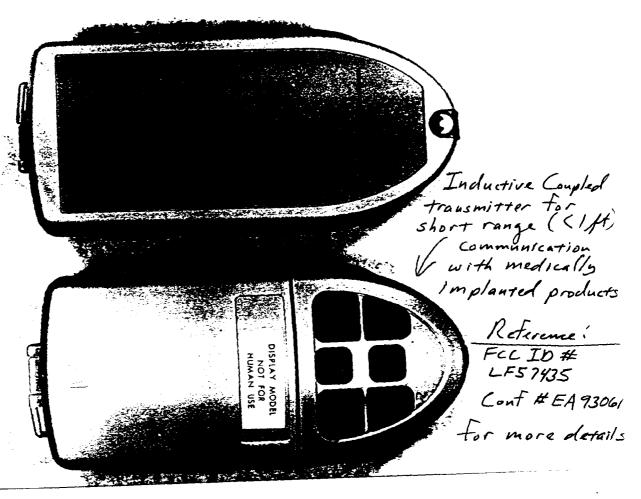


Note: These photos depict a sample of the device (Patient Programmer) For which our labeling question applies.

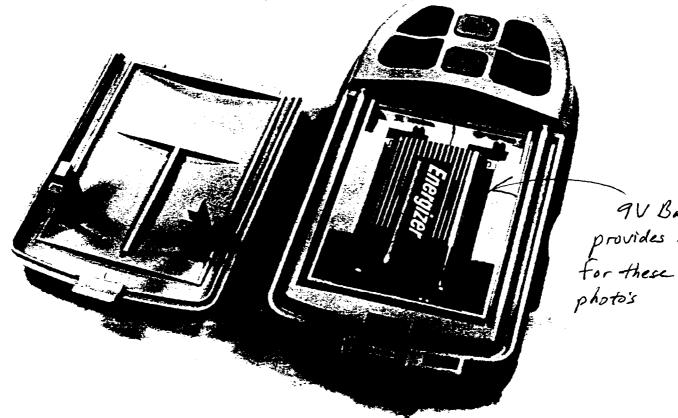

9V Battery provides scale




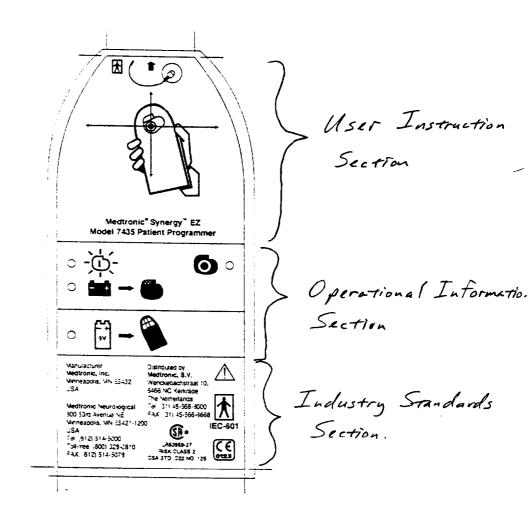

- Label for use outside U.S.


UC9700819cEN/194733-004



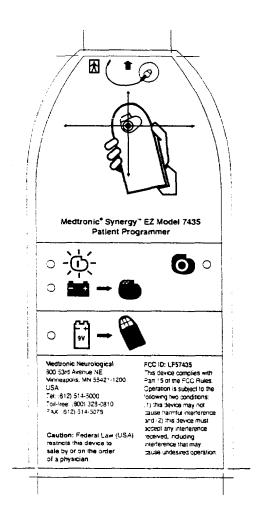

Example of Lable used for products within the US. UC9900344EN/220183_001



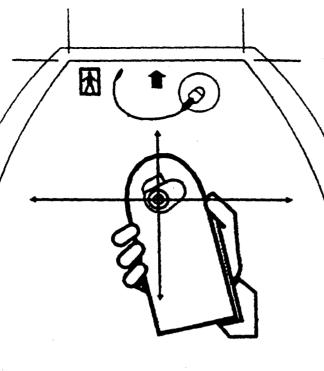

Medtronic* Synergy* EZ Model 7435 Patient Programmer













Medtronic Neurological 800 53rd Avenue NE Minneapolis, MN 55421-1200 **USA** Tel: (612) 514-5000

Toll-free: (800) 328-0810 FAX: (612) 514-5078


Caution: Federal Law (USA) restricts this device to sale by or on the order of a physician.

FCC ID: LF57435_

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference and (2) this device must accept any interference received, including interference that may cause undesired operation.

- Our product Tlabel designers need more label space to acheive a universal label design. - This statement is also provided in the device manual.

D) A prototype DRAFT of a "universal label"

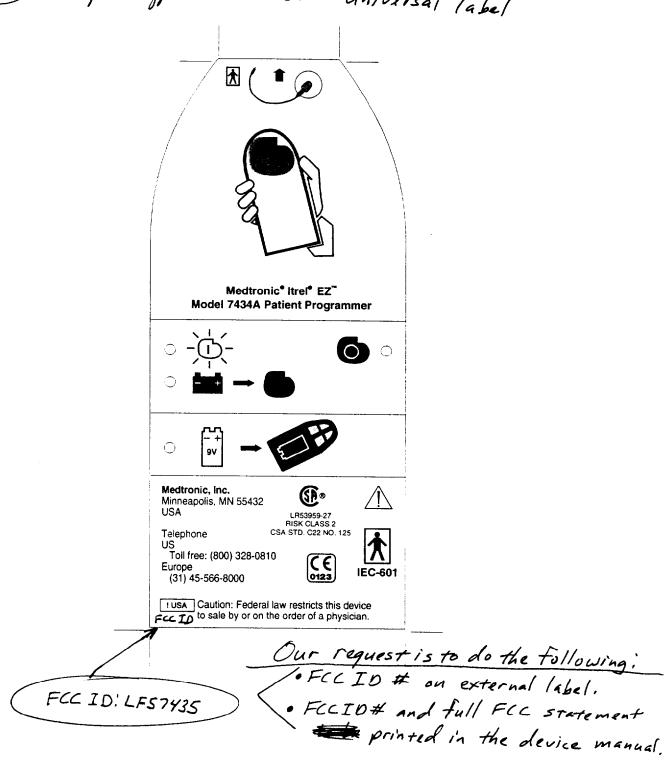

Draft UC9900371 EE/220181-001