



**Medtronic**

RestoreAdvanced® SureScan® MRI  
Rechargeable neurostimulator

97713

Implant manual

! USA Rx only

**CE0123**  
2013



## Explanation of symbols on product or package labeling

Refer to the appropriate product for symbols that apply.



Open here



Do not use if package is damaged



Do not reuse



Do not resterilize



Sterilized using ethylene oxide



Consult instructions for use



Date of manufacture



Manufacturer



Use by



Temperature limitation



Serial number

**CE0123**

Conformité Européenne (European Conformity). This symbol means that the device fully complies with AIMD Directive 90/385/EEC (NB 0123).



Authorized Representative in the European Community



For USA audiences only

Medtronic®, GroupAdjust®, MyStim®, RestoreAdvanced®, SoftStart/Stop®, and SureScan® are trademarks of Medtronic, Inc., registered in the U.S. and other countries.

# Table of contents

## **Description 7**

Neurostimulation systems with SureScan MRI Technology 7

## **Package contents 7**

## **Patient identification card 7**

## **Device specifications 7**

## **Declaration of conformity 10**

## **Implanted components and MRI scans 11**

Implant criteria for full-body MRI scan eligibility 11

When changing components 11

When explanting components 12

## **Instructions for use 12**

Charging the neurostimulator battery 12

Verifying neurostimulator operation 12

Connecting the extension or lead to the neurostimulator 13

Implanting the neurostimulator 15

**Refer to the indications sheet for indications and related information.**

**Refer to the appropriate information for prescribers booklet for contraindications, warnings, precautions, adverse events summary, individualization of treatment, patient selection, use in specific populations, resterilization, and component disposal.**

**Refer to the MRI Guidelines for Medtronic Neurostimulation Systems for Chronic Pain instructions for use manual for the MRI conditions and MRI-specific warnings and precautions for conducting an MRI scan.**

**Refer to the System Eligibility, Battery Longevity, Specifications reference manual for neurostimulator selection, battery longevity calculations and specific neurostimulator specifications.**

**! USA Refer to the clinical summary booklet for information on the clinical study results of the neurostimulation system and individualization of treatment.**

Checking system integrity 17  
Completing the implant procedure 17

## Description

The Medtronic RestoreAdvanced SureScan MRI Model 97713 Neurostimulator is part of a neurostimulation system for pain therapy.

### Neurostimulation systems with SureScan MRI Technology

When a Medtronic neurostimulation system with SureScan MRI Technology is implanted as directed (see "Implant criteria for full-body MRI scan eligibility" on page 11), a patient's full body may be eligible for MRI scans under specific conditions, ie, any part of the patient's anatomy can be scanned when specific conditions are met.

For the MRI conditions and MRI-specific warnings and precautions for conducting an MRI scan, refer to the *MRI guidelines for Medtronic neurostimulation systems for chronic pain instructions for use manual*.

### Package contents

- Neurostimulator
- Torque wrench
- Product literature
- Warranty card
- Registration form
- Patient identification card

### Patient identification card

A patient identification card is packaged with this device. Advise the patient to carry the most up-to-date identification card at all times and to bring the card to all MRI appointments.

**[USA]** The patient identification card packaged with the device is temporary; a permanent card will be mailed to the patient when Medtronic receives the registration form.

The implant registration form registers the device warranties and creates a record of the device in Medtronic's implant data system.

### Device specifications

The neurostimulator is a multi-programmable, rechargeable device that delivers stimulation through 1 or more leads. The stimulation settings are stored in programs. A program is a specific combination of pulse width, rate, and amplitude settings acting on a specific electrode combination (up to 16 electrodes per program). Up to four programs can be combined into a MyStim group. When using more than one program, the pulses are delivered sequentially—first a pulse from one program, then a pulse from the next program.

Pulse width, amplitude, and electrode polarity for each program within the group can have different values. Rate, rate limits, ramping, and cycling for each program within the group have the same values.

**Table 1. Operating values for the RestoreAdvanced SureScan MRI Model 97713 neurostimulator<sup>a</sup>**

<b>Programmable parameter</b>	<b>Operating range and resolution</b>
Number of defined MyStim groups	1 to 26 <sup>b</sup>
Number of programs per MyStim group	1 to 4 <sup>b</sup>
Electrode configuration	2 to 16 electrodes as anode (+), cathode (-), or Off
Amplitude	0 to 10.5 V with 0.05 V or 0.1 V resolution <sup>c</sup>
Amplitude – upper patient limit	Tracking limit: programmed value +0 to +4 V (0.5 V resolution) Custom limit: programmed value up to 10.5 V (same resolution as amplitude)
Amplitude – lower patient limit	Custom limit: 0 V to the programmed value (same resolution as amplitude)
Pulse width	60 to 450 $\mu$ s (10 $\mu$ s resolution)
Pulse width – upper patient limit	Tracking limit: programmed value +0 to +150 $\mu$ s (30 $\mu$ s resolution) Custom limit: programmed value up to 450 $\mu$ s (10 $\mu$ s resolution)
Pulse width – lower patient limit	Custom limit: 60 $\mu$ s to the programmed value (10 $\mu$ s resolution)
Rate	2 to 130 Hz (1 Hz resolution to 10 Hz; 5 Hz resolution from 10 Hz to 130 Hz)
Rate – upper patient limit	Tracking limit: programmed value +0 to +50 Hz (10 Hz resolution) <sup>d</sup>
Rate – lower patient limit	Custom limit: 2 Hz to the programmed value (1 Hz resolution to 10 Hz; 5 Hz resolution from 10 Hz to 130 Hz) <sup>d</sup>
SoftStart/Stop	Off, On: 1, 2, 4, or 8 sec ramp duration
Cycling	Off, On: 0.1 sec to 30 min (resolution: 0.1 sec from 0.1 sec to 1 sec; 1 sec from 1 sec to 1 min; 1 min from 1 min to 30 min)



**Table 1. Operating values for the RestoreAdvanced SureScan MRI Model 97713 neurostimulator<sup>a</sup> (continued)**

<b>Programmable parameter</b>	<b>Operating range and resolution</b>
Scheduled therapy	Off, On: 1 to 8 events per 24 h period
GroupAdjust	Off, On

<sup>a</sup> All values are approximate.

<sup>b</sup> No more than 32 programs may be defined within the 26 MyStim groups.

<sup>c</sup> Only 0.1 V resolution possible from 10.0 V to 10.5 V amplitude.

<sup>d</sup> Rate limited to 85 Hz when 3 programs/group are active and to 65 Hz when 4 programs/group are active.

**Table 2. Physical characteristics of the RestoreAdvanced SureScan MRI Model 97713 neurostimulator<sup>a</sup>**

<b>Description</b>	<b>Value</b>
Connector type	Octapolar, in-line 2.8 mm (0.110 in) spacing
Height	65.0 mm (2.6 in)
Length	49.0 mm (1.9 in)
Thickness	
case	15.0 mm (0.6 in)
connector	15.0 mm (0.6 in)
Weight	72.0 g (2.5 oz)
Volume	39.0 cm <sup>3</sup> (2.38 in <sup>3</sup> )
Battery life	9 years
Power source <sup>b</sup>	Lithium ion rechargeable battery
Temperature limitation	-18 °C to +52 °C (0 °F to +126 °F)
Serial number model designator <sup>c</sup>	NMC
Radiopaque identification (ID) code <sup>d</sup>	NMA

<sup>a</sup> All measurements are approximate.

<sup>b</sup> The neurostimulator is not shipped with a full battery charge. Refer to the charging system user manual for neurostimulator charging instructions.

<sup>c</sup> The serial number is the model designator followed by a number. The clinician programmer displays the entire serial number beginning with the model designator.

<sup>d</sup> The radiopaque ID code is located in the connector block; NMA indicates that the neurostimulator has SureScan MRI Technology. This radiopaque ID code is for confirming, if needed, that a SureScan MRI

**Table 2. Physical characteristics of the RestoreAdvanced SureScan MRI Model 97713 neurostimulator<sup>a</sup>**

Description	Value
neurostimulator is implanted and is not to be used for concluding that the entire neurostimulation system is full-body MRI scan eligible.	

**Table 3. Material of components in the RestoreAdvanced SureScan MRI Model 97713 package**

Components	Material	Material contacts human tissue
Neurostimulator		
Case	Titanium	Yes
Connector block	Polyurethane, silicone rubber, silicone medical adhesive	Yes
Recharge coil	Polysulfone	Yes
Grommets, seals	Silicone rubber	Yes
Setscrews	Titanium alloy	Yes
Adhesive	Silicone medical adhesive	Yes
Torque wrench		
Handle	Polyetherimide	Yes
Shaft	Stainless steel	Yes

## Declaration of conformity

Medtronic declares that this product is in conformity with the essential requirements of Directive 90/385/EEC on Active Implantable Medical Devices.

For additional information, contact the appropriate Medtronic representative listed on the inside back cover of this manual.

# Implanted components and MRI scans

## Implant criteria for full-body MRI scan eligibility



**Caution:** To allow a patient full-body MRI scan eligibility under specific conditions, implant a Medtronic neurostimulation system with SureScan MRI Technology as follows:

- Use only SureScan MRI neurostimulation system components (eg, leads and neurostimulators).

**Note:** Extension model numbers in the 3708 series (eg, 37081, 37082, 37083) are not full-body MRI scan eligible.

- Implant the neurostimulator in the buttocks, abdomen, or flank (ie, the lateral and posterior region between the ribs and pelvis).
- Place the lead tip(s) in the spinal epidural space.
- Explant any previously abandoned pain leads or extensions that may be in the patient (ie, leads or extensions, or portions of, that are not connected to a neurostimulator).

**Note:** Confirm MRI compatibility of any other implanted medical devices. Other implanted medical devices may limit or restrict MRI scans.

- Enter all component model number and implant location information using the clinician programmer.

If the above implant criteria are not met, the patient will not have a neurostimulation system with full-body MRI scan eligibility. MRI scan eligibility will be restricted.

For the MRI conditions and MRI-specific warnings and precautions for conducting an MRI scan, refer to the *MRI guidelines for Medtronic neurostimulation systems for chronic pain instructions for use* manual. MR scans performed under different conditions can result in patient injury or damage to the implantable device.

## When changing components




**Warning:** Before explanting and replacing an existing neurostimulator, print a report from the existing neurostimulator that shows implanted and any abandoned component information. When adding, changing, or removing neurostimulators, leads, extensions, and accessories, always program up-to-date component model numbers, implant locations, and any abandoned component information to re-establish MRI-scan eligibility.

If this information is not updated or is entered incorrectly, MRI scan-type eligibility data will be inaccurate, and the patient is at risk for one of the following:


- The patient is allowed to have an MRI scan inappropriate for the implanted components, which could cause tissue heating, resulting in tissue damage or serious patient injury.
- The patient is unnecessarily restricted from having an MRI scan.



## When explanting components

-  **Caution:** If permanently explanting a neurostimulator, be sure to also explant all leads, extensions, and accessories. Abandoned components may prevent the patient from being allowed MRI scans in the future due to concerns of lead electrode heating that can result in tissue damage.

## Instructions for use

Implanting physicians should be experienced in epidural-access procedures and should be thoroughly familiar with all product labeling.

-  **Warning:** DO NOT use the recharger on an unhealed wound. The recharging system is not sterile, and contact with the wound can cause an infection.

-  **Caution:** Advise patients to charge the neurostimulator when a **Low battery** () screen is displayed on the patient programmer or recharger; this prevents the battery from overdischarging. If the neurostimulator battery is allowed to overdischarge, the patient cannot charge the neurostimulator; however, the clinician may be able to restore the battery function using the Physician Recharge Mode on the recharger (refer to the troubleshooting section of the software manual).

Allowing the neurostimulator battery to overdischarge will permanently affect the neurostimulator in one of the following ways:

- Battery function is restored; however, charging sessions may be more frequent because battery capacity has been reduced.
- Battery function is not restored and the neurostimulator must be surgically replaced. Battery function is not restored when:
  - the neurostimulator battery is permanently damaged.
  - the neurostimulator battery has been overdischarged and restored twice before. The third time the battery is overdischarged, the neurostimulator will reach end of service. Surgery is required to replace the neurostimulator.

### **Cautions:**

- When using sharp instruments near the neurostimulator, be extremely careful to avoid nicking or damaging the case, the insulation, or the connector block. Damaging the neurostimulator may require surgical replacement.
- Do not use saline or other ionic fluids at connections, which could result in a short circuit.


## Charging the neurostimulator battery

Charge the neurostimulator battery before opening the package. For charging instructions, refer to the charging system user manual.

## Verifying neurostimulator operation


Before opening the sterile neurostimulator package, verify that the neurostimulator is operable by using the clinician programmer to interrogate the neurostimulator and read the

neurostimulator battery charge level. (Refer to the software manual for instructions on how to read the battery charge level.)

 **Caution:** Do not implant a neurostimulator if it was dropped onto a hard surface from a height of 30 cm (12 in) or more, because the neurostimulator may be damaged and fail to operate properly.

**Note:** The neurostimulator pocket may be flushed with an antibiotic solution; do not submerge the neurostimulator in fluid.


## Connecting the extension or lead to the neurostimulator


 **Caution:** Before connecting components, wipe off any body fluids and dry all connections. Fluids in the connection may result in stimulation at the connection site, intermittent stimulation, or loss of stimulation.

1. Wipe the extension or lead connector pins with sterile gauze. If necessary, use sterile (United States Pharmacopeia [USP]) water or a nonionic antibiotic solution.
2. Make sure the connector block receptacles are dry and clean.
3. Insert the appropriate extension or lead connector pins into the appropriate neurostimulator socket until they are seated fully within the connector block (Figure 1).

### Notes:

- During insertion, some resistance is typical.
- To retract the setscrews, insert the torque wrench into the self-sealing grommet and rotate the setscrews counterclockwise; however, do not remove the setscrews from the connector block.

 **Caution:** Do not insert the extension or lead connector into the connector block if the setscrews are not sufficiently retracted. Unretracted setscrews may damage the extension or lead and prevent the extension or lead from fully seating into the connector block.

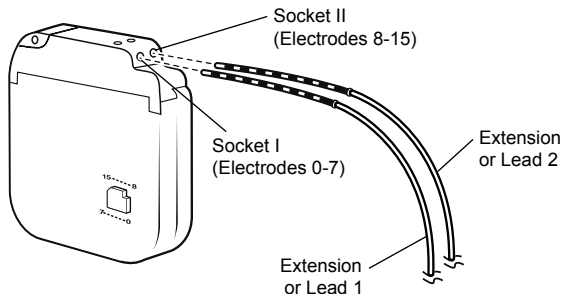


**Figure 1.** Insert the extension or lead connector pins fully into the neurostimulator.

**Note:** Insert a connector plug (from an accessory kit) into any unused neurostimulator socket.

4. For each extension, lead, or plug, fully insert the torque wrench into each self-sealing grommet of the connector block and tighten each setscrew (Figure 2).




 **Cautions:**

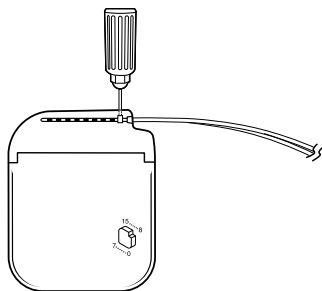- Be sure the torque wrench is fully inserted into the self-sealing grommet. If the torque wrench is not fully inserted, the setscrew may be damaged, resulting in intermittent or loss of stimulation.
- Before tightening setscrews, ensure that the extension or lead connector pins are inserted into the connector block to prevent damaging the lead or extension.
- Verify that each leaf of the self-sealing grommet is closed after the torque wrench is withdrawn. If fluid leaks through a grommet seal that is not fully closed, the patient may experience shocking, burning, or irritation at the neurostimulator implant location, or intermittent stimulation, or loss of stimulation.




**Figure 2.** Tightening the setscrews in the self-sealing grommet.


## Implanting the neurostimulator

-  **Warning:** Do not enclose a neurostimulator with SureScan MRI Technology in a cover, such as those used to mitigate a titanium allergy. A neurostimulator cover may cause significant heating of the lead electrodes during an MRI scan, placing the patient at risk for tissue heating, resulting in tissue damage or serious patient injury.
-  **Warning:** Do not tie ligatures directly around the lead body. Ligatures around the lead body can damage the lead body or conductor wires, resulting in a loss of therapy. During an MRI scan, the patient could be at risk of tissue heating, resulting in tissue damage or serious patient injury.
-  **Caution:** To prevent device inversion, do not make the neurostimulator pocket any larger than necessary to fit the neurostimulator and excess lead or extension. Device inversion may result in component damage, lead dislodgement, skin erosion, or stimulation at the implant site, requiring repeat surgery to restore therapy.

**Note:** For full-body MRI scan eligibility, confirm that the subcutaneous pocket for the neurostimulator has been created in the buttocks, abdomen, or flank. (See the caution in "Implant criteria for full-body MRI scan eligibility" on page 11.)

1. With the Medtronic logo facing outward, away from muscle tissue, rotate the neurostimulator counterclockwise to coil the excess lead or extension (Figure 3).

-  **Caution:** Do not twist or kink the lead or extension bodies when rotating the neurostimulator and coiling the excess lead or extension. Twisting or kinking of the components creates a torsional load that may increase the risk of unwanted movement or damage to the neurostimulation system components.

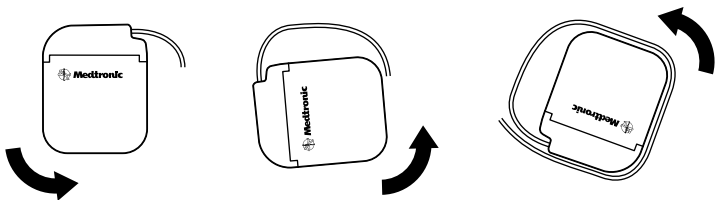


**Figure 3.** Rotate counterclockwise to coil excess lead or extension length.

2. Insert the neurostimulator and excess lead or extension coils into the subcutaneous pocket with the Medtronic logo facing outward, away from muscle tissue. Ensure that the leads or extensions are not twisted or bent sharply.



**Cautions:**

- Ensure that the neurostimulator is placed no deeper than 1 cm (0.4 in) below the skin and is parallel to the skin. If the neurostimulator is too deep or is not parallel to the skin, recharge may be inefficient or unsuccessful.
- Position the neurostimulator with the white surface facing outward. If implanted with the white surface facing inward, the neurostimulator cannot be charged.
- Do not coil excess extensions or leads in front of the neurostimulator. Wrap excess extensions or leads around the perimeter (Figure 4) or behind the neurostimulator to help minimize potential damage during neurostimulator replacement surgery, help minimize potential kinking of the extension or lead, and minimize interference with telemetry and recharge operation.

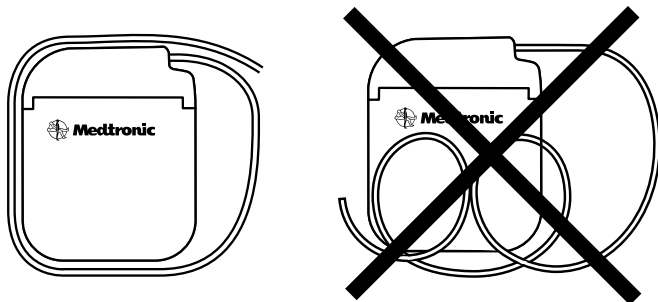

**Figure 4.** Wrap excess extensions or leads around the perimeter (or behind) the neurostimulator.



3. Use the suture holes in the connector block to secure the neurostimulator to the muscle fascia with nonabsorbable silk.

**Notes:**

- Secure the neurostimulator in the pocket to minimize movement or migration of the neurostimulator.
- Suturing the neurostimulator also may prevent movement of the neurostimulator from torque and other forces during an MRI scan.

## Checking system integrity

1. To ensure that you have properly connected each extension or lead to the neurostimulator, use the clinician programmer to confirm the integrity of the connected system.



**Caution:** To use the nonsterile clinician programmer in a sterile field, place a sterile barrier between the patient and the programming head to prevent infection. Do not sterilize any part of the clinician programmer. Sterilization may damage the programmer.

**Note:** The neurostimulator should be in the pocket during system interrogation for integrity to ensure proper readings.

If the system integrity test results are not acceptable, refer to "Connecting the extension or lead to the neurostimulator" on page 13.

2. Program the basic stimulation parameters and check the battery status; if applicable, check the electrode impedances to rule out a short or open circuit.
3. Complete the stimulation assessment form.

## Completing the implant procedure

1. Close and dress all incisions.
2. Ensure that a patient control device and a completed patient identification card are given to the patient.
3. Complete the device tracking and patient registration paperwork and return the documents to Medtronic.

**Contacts:****Asia:**

Medtronic International Ltd.  
Tel. 02919-1300  
Fax 02891-6830

Medtronic Asia Ltd.

Tel. (02)-548-1148  
Fax (02)-518-4786

**Australia:**

Medtronic Australasia Pty. Ltd.  
97 Waterloo Road  
North Ryde, NSW 2113  
Australia  
Tel. +61-2-9857-9000  
Fax +61-2-9878-5100  
Toll-free 1-800-668-670

**Austria:**

Medtronic Österreich GmbH  
Tel. 01-240440  
Fax 01-24044-100

**Belgium:**

Medtronic Belgium S.A.  
Tel. 02-456-0900  
Fax 02-460-2667

**Canada:**

Medtronic of Canada Ltd.  
Tel. (1-905)-460-3800  
Fax (1905)-826-6620

**Czech Republic:**

Medtronic Czechia s.r.o.  
Tel. 2-965-795-80  
Fax 2-965-795-89

**Denmark:**

Medtronic Danmark A/S  
Tel. 45-32-48-18-00  
Fax 45-32-48-18-01

**Finland:**

Medtronic Finland Oy/LTD  
Tel. (09)-755-2500  
Fax (09)-755-25018

**France:**

Medtronic France S.A.S.  
Tel. 01-5538-1700  
Fax 01-5538-1800

**Germany:**

Medtronic GmbH  
Tel. (02159)-81490  
Fax (02159)-8149100

**Greece:**

Medtronic Hellas S.A.  
Tel. 210-67-79-099  
Fax 210-67-79-399

**Hungary:**

Medtronic Hungária Kft.  
Tel. 1-889-06-00  
Fax 1-889-06-99

**Ireland:**

Medtronic Ireland Ltd.  
Tel. (01)-890-6522  
Fax (01)-890-7220

**Italy:**

Medtronic Italia SpA  
Tel. 02-241371  
Fax 02-241381  
Tel. 06-328141  
Fax 06-3215812

**Japan:**

Medtronic Japan  
Tel. 03-6776-0017  
Fax 03-6774-4645

**Latin America:**

Medtronic, Inc.  
Tel. (1305)-500-9328  
Fax (1786)-709-4244

**Norway:**

Medtronic Norge AS  
Tel. 67-10-32-00  
Fax 67-10-32-10

**Poland:**

Medtronic Poland Sp. z.o.o.  
Tel. (022)-465-69-00  
Fax (022)-465-69-17

**Portugal:**

Medtronic Portugal, Lda.  
Tel. 21-724-5100  
Fax 21-724-5199

**Russia:**

Medtronic Russia  
Tel. (8495) 580-7377  
Fax (8495) 580-7378

**Slovakia:**

Medtronic Slovakia, o.z.  
Tel. 0268 206 911  
Fax 0268 206 999

**Spain:**

Medtronic Ibérica, S.A.  
Tel. 91-625-0400  
Fax 91-650-7410

**Sweden:**

Medtronic AB  
Tel. 08-568-585-00  
Fax 08-568-585-01

**Switzerland:**

Medtronic (Schweiz) AG

Tel. 031-868-0100

Fax 031-868-0199

**The Netherlands:**

Medtronic B.V.

Tel. (045)-566-8000

Fax (045)-566-8668

**Turkey:**

Medtronic Turkey

Tel. +90 216 636 1000

Fax +90 216 636 1008

**U.K.:**

Medtronic U.K. Ltd.

Tel. 01923-212213

Fax 01923-241004

**USA:**

Medtronic, Inc.

Tel. (1-763)-505-5000

Fax (1-763)-505-1000

Toll-free: (1-800)-328-0810



# Medtronic

## Manufacturer

Medtronic, Inc.  
710 Medtronic Parkway,  
Minneapolis, MN 55432-5604,  
USA  
www.medtronic.com  
Tel. +1-763-505-5000  
Fax +1-763-505-1000

## Authorized Representative in the European Community



Medtronic B.V.  
Earl Bakkenstraat 10,  
6422 PJ Heerlen,  
The Netherlands  
Tel. +31-45-566-8000  
Fax +31-45-566-8668

## Europe/Africa/Middle East Headquarters

Medtronic International Trading Sàrl  
Route du Molliau 31,  
Case Postale 84  
CH - 1131 Tolothenaz,  
Switzerland  
www.medtronic.eu  
Tel. +41-21-802-7000  
Fax +41-21-802-7900

## Asia-Pacific

Medtronic International Ltd.  
Suite 1106-11, 11/F, Tower 1, The Gateway,  
25 Canton Road, Tsimshatsui,  
Kowloon,  
Hong Kong  
Tel. +852-2919-1300  
Fax +852-2891-6830

Contacts for specific countries are listed inside this cover.



\* M 9 4 0 0 9 9 A 0 0 7 \*

© Medtronic, Inc. 2016  
All Rights Reserved

M940099A007 Rev A