

---

**APPENDIX D: RELEVANT PAGES FROM DIPOLE VALIDATION KIT REPORT(S)**

See the following pages.



Accredited by the Swiss Federal Office of Metrology and Accreditation  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Nokia Salo TCC**

Certificate No: **D835V2-480\_May07**

## CALIBRATION CERTIFICATE

Object **D835V2 - SN: 480**

Calibration procedure(s) **QA CAL-05.v6**  
**Calibration procedure for dipole validation kits**

Calibration date: **May 21, 2007**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #             | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration  |
|-----------------------------|------------------|-------------------------------------------|------------------------|
| Power meter EPM-442A        | GB37480704       | 03-Oct-06 (METAS, No. 217-00608)          | Oct-07                 |
| Power sensor HP 8481A       | US37292783       | 03-Oct-06 (METAS, No. 217-00608)          | Oct-07                 |
| Reference 20 dB Attenuator  | SN: 5086 (20g)   | 10-Aug-06 (METAS, No 217-00591)           | Aug-07                 |
| Reference 10 dB Attenuator  | SN: 5047.2 (10r) | 10-Aug-06 (METAS, No 217-00591)           | Aug-07                 |
| Reference Probe ET3DV6 (HF) | SN 1507          | 19-Oct-06 (SPEAG, No. ET3-1507_Oct06)     | Oct-07                 |
| DAE4                        | SN 601           | 30-Jan-07 (SPEAG, No. DAE4-601_Jan07)     | Jan-08                 |
| Secondary Standards         | ID #             | Check Date (in house)                     | Scheduled Check        |
| Power sensor HP 8481A       | MY41092317       | 18-Oct-02 (SPEAG, in house check Oct-05)  | In house check: Oct-07 |
| RF generator Agilent E4421B | MY41000675       | 11-May-05 (SPEAG, in house check Nov-05)  | In house check: Nov-07 |
| Network Analyzer HP 8753E   | US37390585 S4206 | 18-Oct-01 (SPEAG, in house check Oct-06)  | In house check: Oct-07 |

|                |             |                       |           |
|----------------|-------------|-----------------------|-----------|
|                | Name        | Function              | Signature |
| Calibrated by: | Marcel Fehr | Laboratory Technician |           |

|              |               |                   |
|--------------|---------------|-------------------|
| Approved by: | Katja Pokovic | Technical Manager |
|--------------|---------------|-------------------|

Issued: May 30, 2007

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## DASY4 Validation Report for Head TSL

Date/Time: 21.05.2007 15:29:18

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:480**

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL 900 MHz;

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.9 \text{ mho/m}$ ;  $\epsilon_r = 41.6$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

### DASY4 Configuration:

- Probe: ET3DV6 - SN1507 (HF); ConvF(6.09, 6.09, 6.09); Calibrated: 19.10.2006
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; ;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Pin = 250 mW; d = 15 mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 54.7 V/m; Power Drift = 0.003 dB

Peak SAR (extrapolated) = 3.29 W/kg

**SAR(1 g) = 2.29 mW/g; SAR(10 g) = 1.5 mW/g**

Maximum value of SAR (measured) = 2.47 mW/g

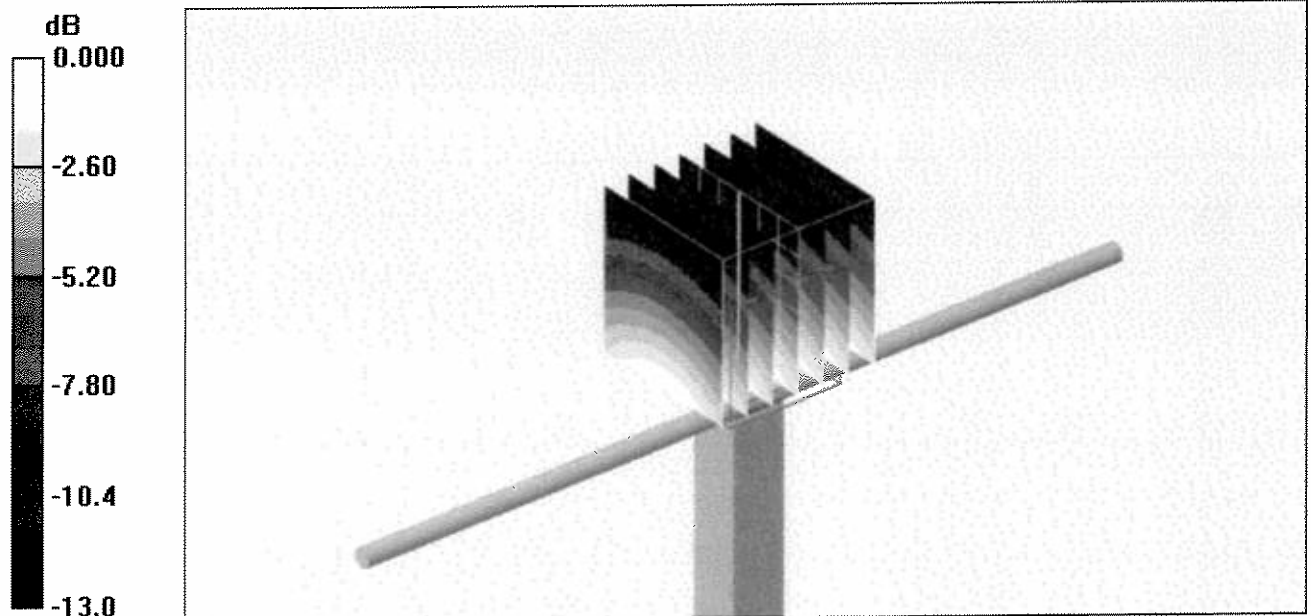

0 dB = 2.47mW/g

## DASY4 Validation Report for Body TSL

Date/Time: 21.05.2007 12:35:17

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:480**

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: MSL900;

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.98 \text{ mho/m}$ ;  $\epsilon_r = 53$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

### DASY4 Configuration:

- Probe: ET3DV6 - SN1507 (HF); ConvF(5.75, 5.75, 5.75); Calibrated: 19.10.2006
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; ;
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

### **Pin = 250mW, d = 15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 54.8 V/m; Power Drift = 0.013 dB

Peak SAR (extrapolated) = 3.45 W/kg

**SAR(1 g) = 2.48 mW/g; SAR(10 g) = 1.65 mW/g**

Maximum value of SAR (measured) = 2.69 mW/g

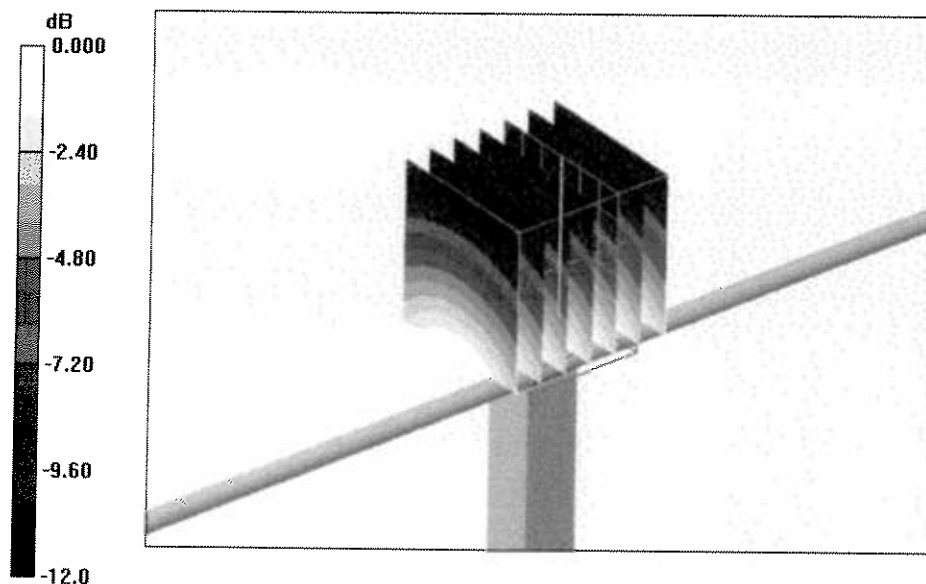

0 dB = 2.69mW/g



Accredited by the Swiss Federal Office of Metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Nokia Salo TCC**

Certificate No: **D1900V2-5d013\_Jul06**

## CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d013**

Calibration procedure(s) **QA CAL-05.v6**  
**Calibration procedure for dipole validation kits**

Calibration date: **July 07, 2006**

Condition of the calibrated item **In Tolerance**


This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.


All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID #             | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|----------------------------|------------------|-------------------------------------------|-----------------------|
| Power meter EPM-442A       | GB37480704       | 04-Oct-05 (METAS, No. 251-00516)          | Oct-06                |
| Power sensor HP 8481A      | US37292783       | 04-Oct-05 (METAS, No. 251-00516)          | Oct-06                |
| Reference 20 dB Attenuator | SN: 5086 (20g)   | 11-Aug-05 (METAS, No 251-00498)           | Aug-06                |
| Reference 10 dB Attenuator | SN: 5047.2 (10r) | 11-Aug-05 (METAS, No 251-00498)           | Aug-06                |
| Reference Probe ET3DV6     | SN: 1507         | 28-Oct-05 (SPEAG, No. ET3-1507_Oct05)     | Oct-06                |
| DAE4                       | SN: 601          | 15-Dec-05 (SPEAG, No. DAE4-601_Dec05)     | Dec-06                |

| Secondary Standards         | ID #             | Check Date (in house)                    | Scheduled Check        |
|-----------------------------|------------------|------------------------------------------|------------------------|
| Power sensor HP 8481A       | MY41092317       | 18-Oct-02 (SPEAG, in house check Oct-05) | In house check: Oct-07 |
| RF generator Agilent E4421B | MY41000675       | 11-May-05 (SPEAG, in house check Nov-05) | In house check: Nov-07 |
| Network Analyzer HP 8753E   | US37390585 S4206 | 18-Oct-01 (SPEAG, in house check Nov-05) | In house check: Nov-06 |

Calibrated by: **Claudio Leubler** **Laboratory Technician** 

Approved by: **Katja Pokovic** **Technical Manager** 

Issued: July 10, 2006

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d013**

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB;

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.44$  mho/m;  $\epsilon_r = 39.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507 (HF); ConvF(4.74, 4.74, 4.74); Calibrated: 28.10.2005
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 15.12.2005
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 171


**Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 93.5 V/m; Power Drift = 0.005 dB

Peak SAR (extrapolated) = 16.7 W/kg

**SAR(1 g) = 9.69 mW/g; SAR(10 g) = 5.11 mW/g**

Maximum value of SAR (measured) = 11.0 mW/g

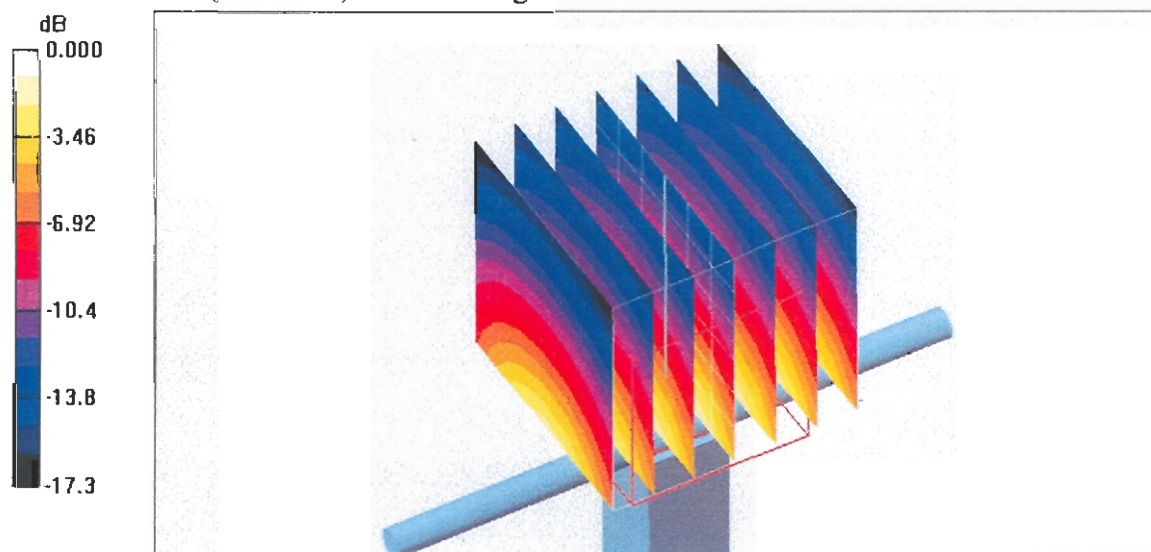

0 dB = 11.0mW/g



Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d013**

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: MSL U10;

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.57$  mho/m;  $\epsilon_r = 52.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

#### DASY4 Configuration:

- Probe: ET3DV6 - SN1507 (HF); ConvF(4.3, 4.3, 4.3); Calibrated: 28.10.2005
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 15.12.2005
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 171


**Pin = 250 mW; d = 10 mm big batch/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 87.1 V/m; Power Drift = 0.079 dB

Peak SAR (extrapolated) = 17.4 W/kg

**SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.36 mW/g**

Maximum value of SAR (measured) = 11.3 mW/g

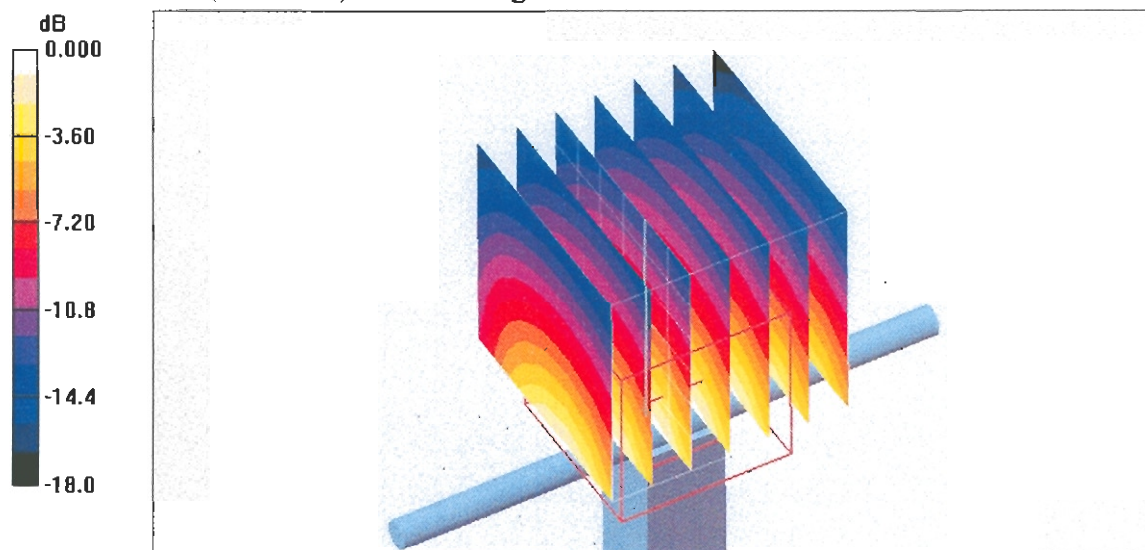

0 dB = 11.3mW/g