

System Check_B2450

DUT: Dipole 2450 MHz D2450V2; SN: 1221;


Communication System: UID 0, CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.973$ S/m; $\epsilon_r = 53.183$; $\rho = 1000$ kg/m³
Ambient Temperature : 21.9 °C; Liquid Temperature : 21.3 °C

DASY Configuration:

- Probe: EX3DV4 - SN7369; ConvF(7.19, 7.19, 7.19); Calibrated: 8/18/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 31.0$
- Electronics: DAE4 Sn1486; Calibrated: 8/27/2015
- Phantom: Oval Flat Phantom ELI 5.0; Type: QD OVA 002 A ; Serial: TP-1240
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Area Scan (9x9x1): Measurement grid: $dx=12$ mm, $dy=12$ mm
Maximum value of SAR (measured) = 18.3 W/kg

Zoom Scan (7x7x7)/Cube 0: Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm
Reference Value = 96.98 V/m; Power Drift = 0.02 dB
Peak SAR (extrapolated) = 25.4 W/kg
SAR(1 g) = 12.2 W/kg; SAR(10 g) = 5.63 W/kg
Maximum value of SAR (measured) = 18.7 W/kg

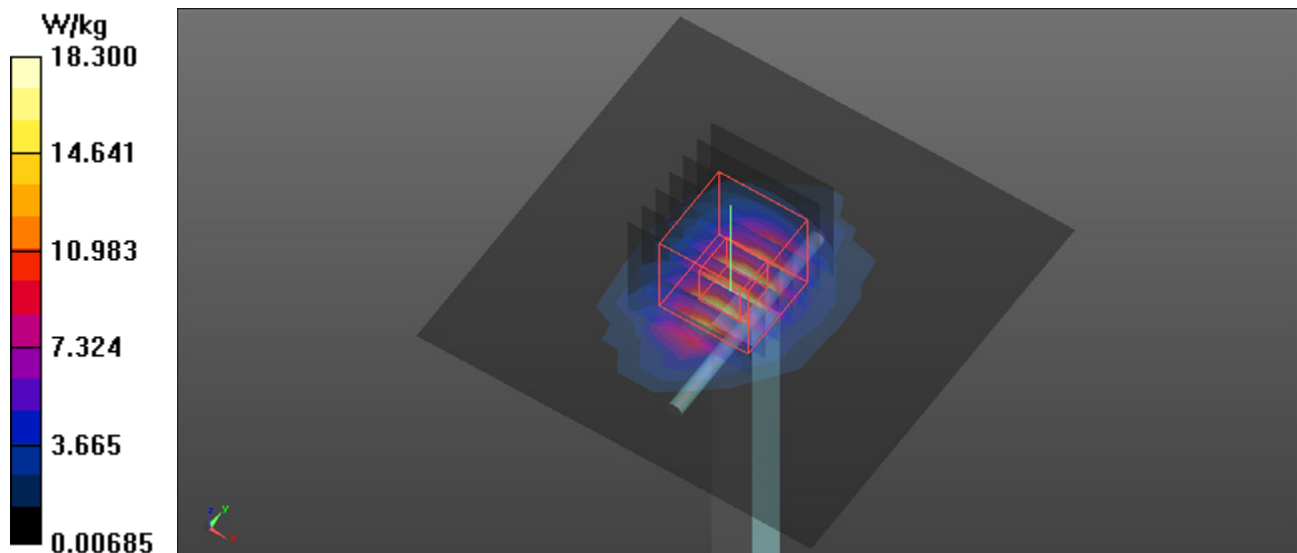

System Check_B5200

DUT: Dipole D5GHzV2; SN: 1221;


Communication System: UID 0, CW (0); Frequency: 5200 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5200$ MHz; $\sigma = 5.347$ S/m; $\epsilon_r = 47.581$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.2 °C; Liquid Temperature : 21.5 °C

DASY Configuration:

- Probe: EX3DV4 - SN7369; ConvF(4.57, 4.57, 4.57); Calibrated: 8/18/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 21.0$
- Electronics: DAE4 Sn1486; Calibrated: 8/27/2015
- Phantom: Oval Flat Phantom ELI 5.0; Type: QD OVA 002 A ; Serial: TP-1240
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Area Scan (10x10x1): Measurement grid: $dx=10$ mm, $dy=10$ mm
Maximum value of SAR (measured) = 10.8 W/kg

Zoom Scan (7x7x12)/Cube 0: Measurement grid: $dx=4$ mm, $dy=4$ mm, $dz=2$ mm
Reference Value = 56.39 V/m; Power Drift = 0.01 dB
Peak SAR (extrapolated) = 27.0 W/kg
SAR(1 g) = 7.18 W/kg; SAR(10 g) = 2.04 W/kg
Maximum value of SAR (measured) = 14.9 W/kg

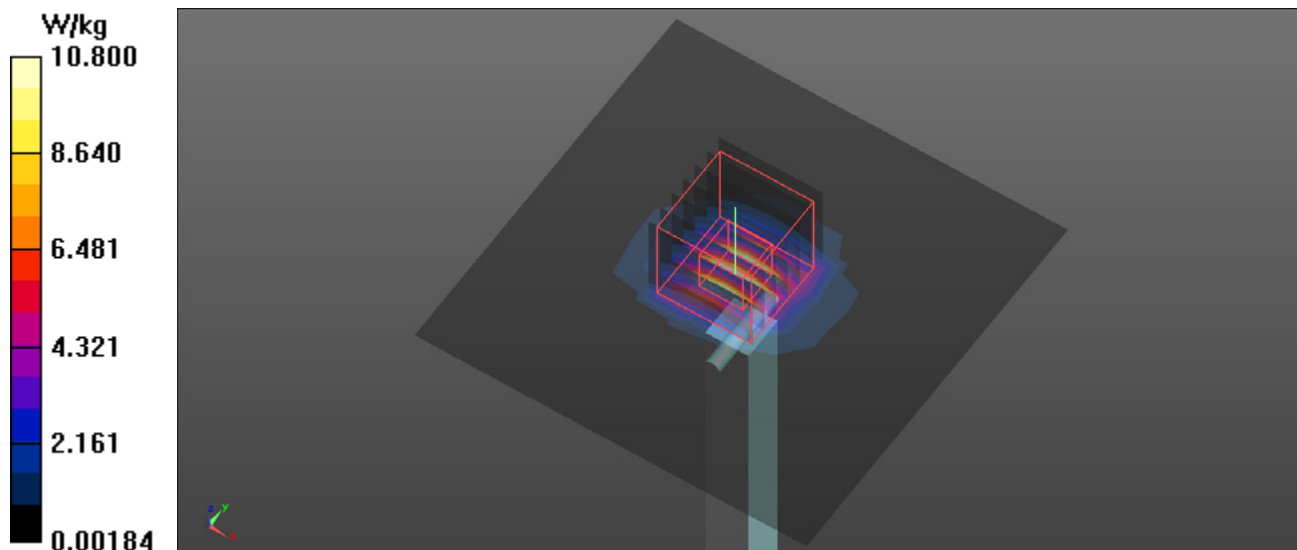

System Check_B5300

DUT: Dipole D5GHzV2; SN: 1221;


Communication System: UID 0, CW (0); Frequency: 5300 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5300$ MHz; $\sigma = 5.481$ S/m; $\epsilon_r = 47.409$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.2 °C; Liquid Temperature : 21.5 °C

DASY Configuration:

- Probe: EX3DV4 - SN7369; ConvF(4.38, 4.38, 4.38); Calibrated: 8/18/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 21.0$
- Electronics: DAE4 Sn1486; Calibrated: 8/27/2015
- Phantom: Oval Flat Phantom ELI 5.0; Type: QD OVA 002 A ; Serial: TP-1240
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Area Scan (10x10x1): Measurement grid: $dx=10$ mm, $dy=10$ mm
Maximum value of SAR (measured) = 8.34 W/kg

Zoom Scan (7x7x12)/Cube 0: Measurement grid: $dx=4$ mm, $dy=4$ mm, $dz=2$ mm
Reference Value = 57.07 V/m; Power Drift = 0.05 dB
Peak SAR (extrapolated) = 31.4 W/kg
SAR(1 g) = 7.29 W/kg; SAR(10 g) = 2.02 W/kg
Maximum value of SAR (measured) = 15.6 W/kg

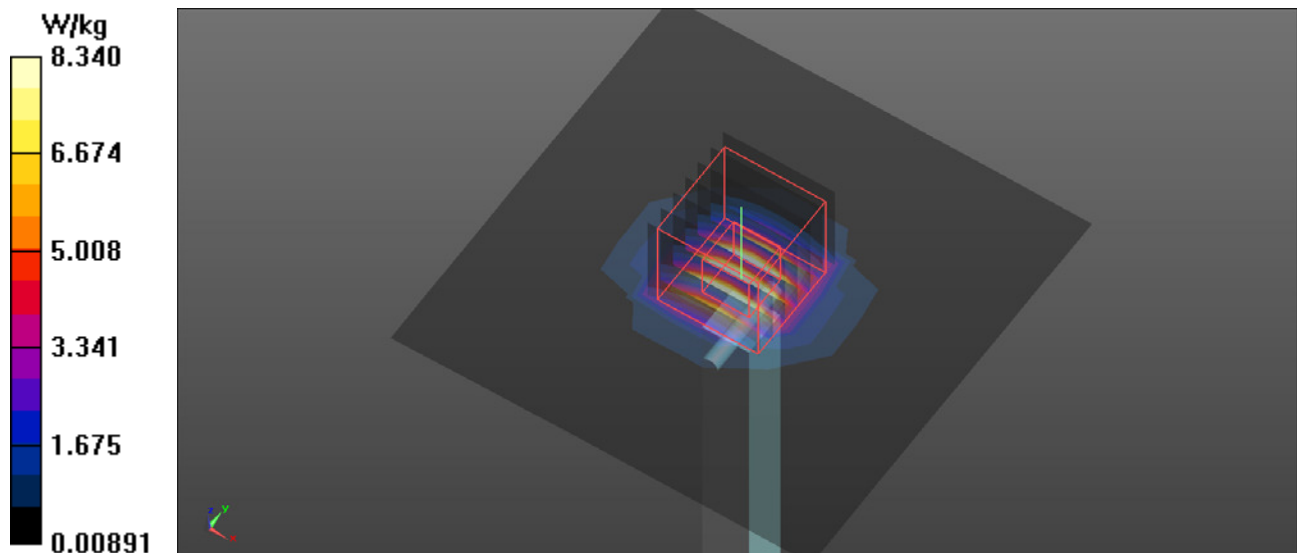

System Check_B5600

DUT: Dipole D5GHzV2; SN: 1221;

Communication System: UID 0, CW (0); Frequency: 5600 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5600$ MHz; $\sigma = 5.912$ S/m; $\epsilon_r = 46.863$; $\rho = 1000$ kg/m³
Ambient Temperature : 22.2 °C; Liquid Temperature : 21.5 °C

DASY Configuration:

- Probe: EX3DV4 - SN7369; ConvF(3.81, 3.81, 3.81); Calibrated: 8/18/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection), $z = 1.0, 21.0$
- Electronics: DAE4 Sn1486; Calibrated: 8/27/2015
- Phantom: Oval Flat Phantom ELI 5.0; Type: QD OVA 002 A ; Serial: TP-1240
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Area Scan (10x10x1): Measurement grid: $dx=10$ mm, $dy=10$ mm
Maximum value of SAR (measured) = 8.79 W/kg

Zoom Scan (7x7x12)/Cube 0: Measurement grid: $dx=4$ mm, $dy=4$ mm, $dz=2$ mm
Reference Value = 56.10 V/m; Power Drift = 0.09 dB
Peak SAR (extrapolated) = 34.2 W/kg
SAR(1 g) = 7.54 W/kg; SAR(10 g) = 2.08 W/kg
Maximum value of SAR (measured) = 16.3 W/kg

