


D450V3-SN:1113; 450Head

Calibrated impedance: $55.7\Omega - 5.3j\Omega$; Measurement impedance: $59.3\Omega - 6.9j\Omega$ (within 5Ω)



Calibrated return loss: -22.6dB; Measurement return loss: -22.8 dB (within 20%)

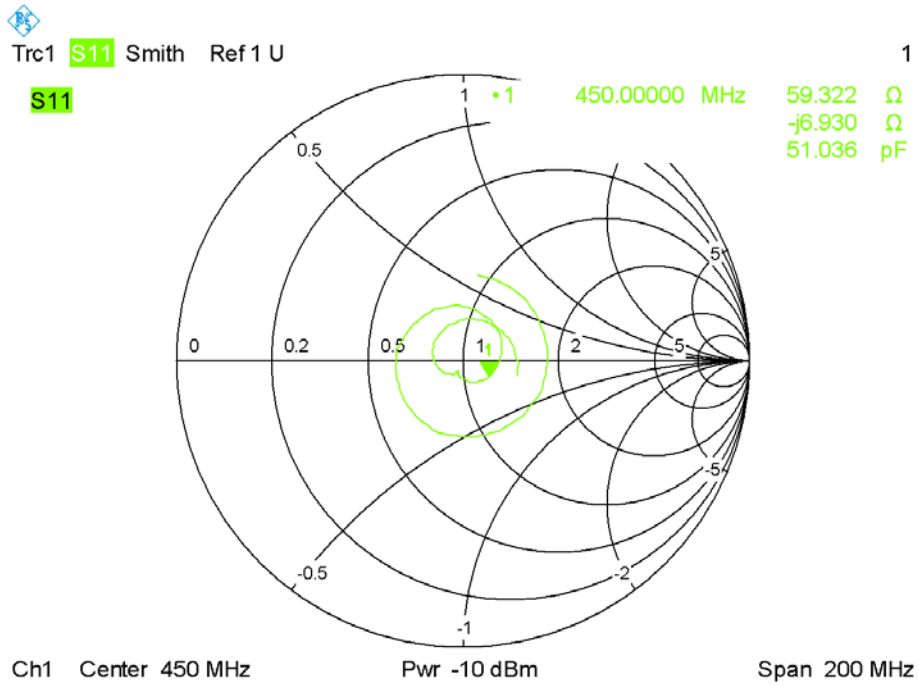