

### **SAR Test Report**

Product Name	: 802.11a/b/g Wireless SDIO Card
Model No.	: SDW3100

Applicant	: AboCom System, Inc	
Address	: 77, Yu-Yih Rd., Chu-Nan Chen, Miao-Lih	
	Hsuan, Taiwan	

Date of Receipt	: 2009/01/15
Issued Date	: 2009/01/19
Report No.	: 091220R-HPUSP09V01
Version	: V1.0

The test results relate only to the samples tested.

The test report shall not be reproduced except in full without the written approval of Quie Tek Corporation.

### **Test Report Certification**

Issued Date: 2009/01/19 Report No.:091220R-HPUSP09V01

# QuieTek

Product Name Applicant Address Manufacturer	: A : 7	02.11a/b/g Wireless SDIO Card boCom System, Inc 7, Yu-Yih Rd., Chu-Nan Chen, Miao-Lih Hsuan, Taiwan boCom System, Inc
Model No.	: 8	SDW3100
Trade Name	: A	boCom
FCC ID.	: N	/IQ4SDW3100
Applicable Standard	: F	CC Oet65 Supplement C June 2001
		EEE Std. 1528-2003 47CFR § 2.1093
Test Result	: N	/lax. SAR Measurement (1g)
		.2GHz Band (5200MHz~5320MHz): 0.273 W/kg .8GHz Band (5745MHz~5825MHz): 0.333 W/kg
Application Type: CertificationThe test results relate only to the samples tested.The test report shall not be reproduced except in full without the written approval of Quie Tek Corporation.		
Documented By	:	Nicole Huang
		(Engineering Adm. Assistant / Nicole Huang)
Tested By	:	Jung Chang
		(Engineer / Jung Chang)
Approved By	:	Hombo
		(Manager / Vincent Lin)



### TABLE OF CONTENTS

Desc	cription	Page
1.	General Information	5
	1.1 EUT Description	5
	1.2 Test Environment	6
2.	SAR Measurement System	7
	2.1 ALSAS-10U System Description	7
	2.1.1 Applications	7
	2.1.2 Area Scans	7
	2.1.3 Zoom Scan (Cube Scan Averaging)	8
	2.1.4 ALSAS-10U Interpolation and Extrapolation Uncertainty	8
	2.2 Isotropic E-Field Probe	8
	2.2.1 Isotropic E-Field Probe Specification	10
	2.3 Boundary Detection Unit and Probe Mounting Device	10
	2.4 Daq-Paq (Analog to Digital Electronics)	11
	2.5 Axis Articulated Robot	11
	2.6 ALSAS Universal Workstation	
	2.7 Universal Device Positioner	
	2.8 Phantom Types	
	2.8.1 APREL SAM Phantoms	13
	2.8.2 APREL Laboratories Universal Phantom	13
3.	Tissue Simulating Liquid	14
	3.1 The composition of the tissue simulating liquid	14
	3.2 Tissue Calibration Result	14
	3.3 Tissue Dielectric Parameters for Head and Body Phantoms	16
4.	SAR Measurement Procedure	17
	4.1 SAR System Validation	17
	4.1.1 Validation Dipoles	17
	4.1.2 Validation Result	17
	4.2 SAR Measurement Procedure	
5.	SAR Exposure Limits	19
6.	Test Equipment List	20
7.	Measurement Uncertainty	
8.	Test Results	
	8.1 SAR Test Results Summary	22

Appendix	24
Appendix A. SAR System Validation Data	
Appendix B. SAR measurement Data	
Appendix C. Test Setup Photographs & EUT Photographs	
Appendix D. Probe Calibration Data	
Appendix E. Dipole Calibration Data	

### 1. General Information

#### 1.1 EUT Description

Product Name	802.11a/b/g Wireless SDIO Card
Trade Name	AboCom
Model No.	SDW3100
FCC ID	MQ4SDW3100
TX Frequency	5180MHz~5320MHz
	5745MHz~5825MHz
Number of Channel	5.2GHz Band: 64
	5.8GHz Band (802.11n): 165
Type of Modulation	DSSS/OFDM
Antenna Type	Printing Antenna
Device Category	Portable
RF Exposure Environment	Uncontrolled
Transfer Rate	802.11a: 54Mbps

#### **1.2 Test Environment**

Ambient conditions in the laboratory:

Items	Required	Actual
Temperature (°C)	18-25	22.5±2
Humidity (%RH)	30-70	53

Site Description:

Accredited by TAF Accredited Number: 0914 Effective through: December 12, 2011



- Site Name: Quietek Corporation
- Site Address: No. 5, Ruei-Shu Valley, Ruei-Ping Tsuen, Lin-Kou Shiang, Taipei, Taiwan, R.O.C. TEL : 886-2-8601-3788 / FAX : 886-2-8601-3789 E-Mail : <u>service@quietek.com</u>

### 2. SAR Measurement System

### 2.1 ALSAS-10U System Description

ALSAS-10-U is fully compliant with the technical and scientific requirements of IEEE 1528, IEC 62209, CENELEC, ARIB, ACA, and the Federal Communications Commission. The system comprises of a six axes articulated robot which utilizes a dedicated controller.

ALSAS-10U uses the latest methodologies and FDTD modeling to provide a platform which is repeatable with minimum uncertainty.

### 2.1.1 Applications

Predefined measurement procedures compliant with the guidelines of CENELEC, IEEE, IEC, FCC, etc are utilized during the assessment for the device. Automatic detection for all SAR



maxima are embedded within the core architecture for the system, ensuring that peak locations used for centering the zoom scan are within a 1mm resolution and a 0.05mm repeatable position. System operation range currently available up-to 6 GHz in simulated tissue.

#### 2.1.2 Area Scans

Area scans are defined prior to the measurement process being executed with a user defined variable spacing between each measurement point (integral) allowing low uncertainty measurements to be conducted. Scans defined for FCC applications utilize a 10mm<sup>2</sup> step integral, with 1mm interpolation used to locate the peak SAR area used for zoom scan assessments.

Where the system identifies multiple SAR peaks (which are within 25% of peak value) the system will provide the user with the option of assessing each peak location individually for zoom scan averaging.

#### 2.1.3 Zoom Scan (Cube Scan Averaging)

The averaging zoom scan volume utilized in the ALSAS-10U software is in the shape of a cube and the side dimension of a 1 g or 10 g mass is dependent on the density of the liquid representing the simulated tissue. A density of 1000 kg/m<sup>3</sup> is used to represent the head and body tissue density and not the phantom liquid density, in order to be consistent with the definition of the liquid dielectric properties, i.e. the side length of the 1 g cube is 10mm, with the side length of the 10 g cube 21,5mm.

When the cube intersects with the surface of the phantom, it is oriented so that 3 vertices touch the surface of the shell or the center of a face is tangent to the surface. The face of the cube closest to the surface is modified in order to conform to the tangent surface.

The zoom scan integer steps can be user defined so as to reduce uncertainty, but normal practice for typical test applications (including FCC) utilize a physical step of 5x5x8 (8mmx8mmx5mm) providing a volume of 32mm in the X & Y axis, and 35mm in the Z axis.

#### 2.1.4 ALSAS-10U Interpolation and Extrapolation Uncertainty

The overall uncertainty for the methodology and algorithms the used during the SAR calculation was evaluated using the data from IEEE 1528 based on the example f3 algorithm:

$$f_3(x, y, z) = A \frac{a^2}{\frac{a^2}{4} + {x'}^2 + {y'}^2} \cdot \left(e^{-\frac{2z}{a}} + \frac{a^2}{2(a+2z)^2}\right)$$


#### 2.2 Isotropic E-Field Probe

The isotropic E-Field probe has been fully calibrated and assessed for isotropicity, and boundary effect within a controlled environment. Depending on the frequency for which the probe is calibrated the method utilized for calibration will change. A number of methods is used for calibrating probes, and these are outlined in the table below:

Calibration Frequency	Air Calibration	Tissue Calibration
5200MHz	Waveguide	Temperature
5800MHz	Waveguide	Temperature



The E-Field probe utilizes a triangular sensor arrangement as detailed in the diagram below:

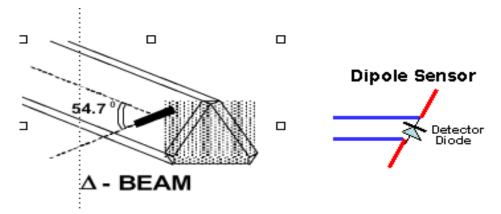

SAR is assessed with a calibrated probe which moves at a default height of 5mm from the center of the diode, which is mounted to the sensor, to the phantom surface (in the Z Axis). The 5mm offset height has been selected so as to minimize any resultant boundary effect due to the probe being in close proximity to the phantom surface.

The following algorithm is an example of the function used by the system for linearization of the output from the probe when measuring complex modulation schemes.

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$



#### 2.2.1 Isotropic E-Field Probe Specification

Calibration in Air	Frequency Dependent	
	Below 2GHz Calibration in air performed in a TEM Cell	
	Above 2GHz Calibration in air performed in waveguide	
Sensitivity	0.70 $\mu$ V/(V/m) <sup>2</sup> to 0.85 $\mu$ V/(V/m) <sup>2</sup>	
Dynamic Range	0.0005 W/kg to 100W/kg	
Isotropic Response	Better than 0.2dB	
Diode Compression point	Calibration for Specific Frequency	
(DCP)		
Probe Tip Radius	< 5mm	
Sensor Offset	1.56 (+/- 0.02mm)	
Probe Length	290mm	
Video Bandwidth	@ 500 Hz: 1dB	
	@1.02 KHz: 3dB	
Boundary Effect	Less than 2% for distance greater than 2.4mm	
Spatial Resolution	Diameter less than 5mm Compliant with Standards	

#### 2.3 Boundary Detection Unit and Probe Mounting Device

ALSAS-10U incorporates a boundary detection unit with a sensitivity of 0.05mm for detecting all types of surfaces. The robust design allows for detection during probe tilt (probe normalize) exercises, and utilizes a second stage emergency stop. The signal electronics are fed directly into the robot controller for high accuracy surface detection in lateral and axial detection modes (X, Y, & Z).

The probe is mounted directly onto the Boundary Detection unit for accurate tooling and displacement calculations controlled by the robot kinematics. The probe is connect to an isolated probe interconnect where the output stage of the probe is fed directly into the amplifier stage of the Daq-Paq.



#### 2.4 Daq-Paq (Analog to Digital Electronics)

ALSAS-10U incorporates a fully calibrated Daq-Paq (analog to digital conversion system) which has a 4 channel input stage, sent via a 2 stage auto-set amplifier module. The input signal is amplified accordingly so as to offer a dynamic range from  $5\mu$ V to 800mV. Integration of the fields measured is carried out at board level utilizing a Co-Processor which then sends the measured fields down into the main computational module in digitized form via an RS232 communications port. Probe linearity and duty cycle compensation is carried out within the main Daq-Paq module.

ADC	12 Bit	
Amplifier Range	20mV to 200mV and 150mV to 800mV	
Field Integration	Local Co-Processor utilizing proprietary integration	
	algorithms	
Number of Input Channels	4 in total 3 dedicated and 1 spare	
Communication	Packet data via RS232	

#### 2.5 Axis Articulated Robot



ALSAS-10U utilizes a six axis articulated robot, which is controlled using a Pentium based real-time movement controller. The movement kinematics engine utilizes proprietary (Thermo CRS) interpolation and extrapolation algorithms, which allow full freedom of movement for each of the six joints within the working envelope. Utilization of joint 6 allows for full probe rotation with a tolerance better than 0.05mm around the central axis.

Robot/Controller Manufacturer	Thermo CRS
Number of Axis	Six independently controlled axis
Positioning Repeatability	0.05mm
Controller Type	Single phase Pentium based C500C
Robot Reach	710mm
Communication	RS232 and LAN compatible

#### 2.6 ALSAS Universal Workstation

ALSAS Universal workstation allows for repeatability and fast adaptability. It allows users to do calibration, testing and measurements using different types of phantoms with one set up, which significantly speeds up the measurement process.

#### 2.7 Universal Device Positioner

The universal device positioner allow complete freedom of movement of the EUT. Developed to hold a EUT in a free-space scenario any additional loading attributable to the material used in the construction of the positioner has been eliminated. Repeatability has been enhanced through the linear scales which form the design used to indicate positioning for any given test scenario in all major axes. A 15° tilt indicator is included for the of aid cheek to tilt movements for head SAR analysis. Overall uncertainty for measurements have been reduced due to the design of the Universal device positioner, which allows positioning of a device in as near to a free-space scenario as possible, and by providing the means for complete repeatability.




#### 2.8 Phantom Types

The ALSAS-10U allows the integration of multiple phantom types. SAM Phantoms fully compliant with IEEE 1528, Universal Phantom, and Universal Flat.



#### 2.8.1 APREL SAM Phantoms

The SAM phantoms developed using the IEEE SAM CAD file. They are fully compliant with the requirements for both IEEE 1528 and FCC Supplement C. Both the left and right SAM phantoms are interchangeable, transparent and include the IEEE 1528 grid with visible NF and MB lines.

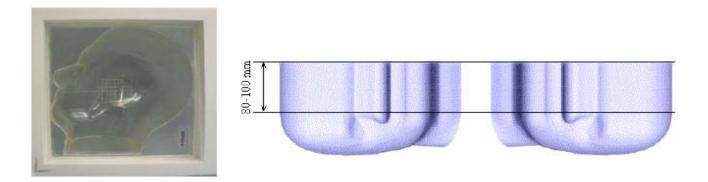

#### 2.8.2 APREL Laboratories Universal Phantom

The Universal Phantom is used on the ALSAS-10U as a system validation phantom. The Universal Phantom has been fully validated both experimentally from 800MHz to 6GHz and numerically using XFDTD numerical software. The shell thickness is 2mm overall, with a 4mm spacer located at the NF/MB intersection providing an overall thickness of 6mm in line with the requirements of IEEE-1528.



The design allows for fast and accurate measurements, of

handsets, by allowing the conservative SAR to be evaluated at on frequency for both left and right head experiments in one measurement.

#### 3. Tissue Simulating Liquid

#### 3.1 The composition of the tissue simulating liquid

INGREDIENT	2450MHz	2450MHz	5200MHz	5200MHz	5800MHz	5800MHz
(% Weight)	Head	Body	Head	Body	Head	Body
Water			67.63	76	68.29	75.68
Salt			0.00	0.00	0.00	0.43
Sugar			0.00	0.00	0.00	0.00
HEC			0.00	0.00	0.00	0.00
Preventol			0.00	0.00	0.00	0.00
DGBE			3.38	4.44	2.44	4.42
Triton X-100			28.99	19.56	29.27	19.47

#### 3.2 Tissue Calibration Result

The dielectric parameters of the liquids were verified prior to the SAR evaluation using APREL Dielectric Probe Kit and Anritsu MS4623B Vector Network Analyzer.

Head Tissue Simulant Measurement						
Frequency	Description	Dielectric Pa	Tissue Temp.			
[MHz]	Description	ε <sub>r</sub>	σ [s/m]	[°C]		
	Reference result	39.94	5.24	N/A		
5200MHz	± 5% window	37.943 to 41.937	4.987 to 5.502			
	16-Jan-09	40.33	5.35	21.7		

Body Tissue Simulant Measurement					
Frequency		Dielectric F	Parameters	Tissue	
[MHz]	Description	٤r	σ [s/m]	Temp. [°C]	
	Reference result	48.9	5.35	N/A	
5200MHz	± 5% window	46.455 to 51.345	5.0825 to 5.6175	IN/A	
	16-Jan-09	48.43	5.42	21.7	
5180 MHz	Low channel	48.47	5.35	21.7	
5260 MHz	Mid channel	48.37	5.41	21.7	
5320 MHz	High channel	48.25	5.49	21.7	

Head Tissue Simulant Measurement					
Frequency	Description	Dielectric F	Tissue Temp.		
[MHz]	Description	ε <sub>r</sub>	σ [s/m]	[°C]	
	Reference result	35.15	6.4	N/A	
5800MHz	± 5% window	33.393 to 36.908	6.08 to 6.72	IN/A	
	16-Jan-09	35.55	6.54	21.7	

Body Tissue Simulant Measurement						
Frequency		Dielectric F	Dielectric Parameters			
[MHz]	Description	ε <sub>r</sub>	σ [s/m]	Temp. [°C]		
	Reference result	48.2	6	N/A		
5800MHz	± 5% window	45.79 to 50.61	5.7 to 6.3	IN/A		
	16-Jan-09	49.22	6.14	21.7		
5500 MHz	Low channel	49.32	6.11	21.7		
5640 MHz	Mid channel	49.29	6.12	21.7		
5825 MHz	High channel	49.16	6.15	21.7		
	•					

#### 3.3 Tissue Dielectric Parameters for Head and Body Phantoms

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in P1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. Other head and body tissue parameters that have not been specified in P1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equations described in Reference [12] and extrapolated according to the head parameters specified in P1528.


Target Frequency	He	ad	Во	dy
(MHz)	ε <sub>r</sub>	σ (S/m)	٤r	σ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800 – 2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00

( $\varepsilon_r$  = relative permittivity,  $\sigma$  = conductivity and  $\rho$  = 1000 kg/m<sup>3</sup>)



#### 4. SAR Measurement Procedure

- 4.1 SAR System Validation
- 4.1.1 Validation Dipoles



The dipoles used is based on the IEEE-1528 standard, and is complied with mechanical and electrical specifications in line with the requirements of both IEEE and FCC Supplement C. the table below provides details for the mechanical and electrical specifications for the dipoles.

Frequency	L (mm)	h (mm)	d (mm)
5200MHz	23.1	14.2	3.6
5800MHz	21.2	13.1	3.6

#### 4.1.2 Validation Result

System Performance Check at 5200MHz					
Validation Kit: ASL	-D-5200-S-2				
Frequency [MHz]	Description	SAR [w/kg] 1g	Tissue Temp. [°C]		
5200 MHz	Reference result ± 10% window	58.8 55.86 to 61.74	N/A		
16-Jan-09 61.072 21.7					
Note: All SAR values are normalized to 1W forward power.					

System Performance Check at 5800MHz Validation Kit: ASL-D-5800-S-2					
Frequency [MHz]	Description	SAR [w/kg] 1g	Tissue Temp. [°C]		
5800 MHz	Reference result ± 10% window	57.9 55.005 to 60.795	N/A		
16-Jan-09 60.332 21.7					
Note: All SAR values are normalized to 1W forward power.					

#### 4.2 SAR Measurement Procedure

The ALSAS-10U calculates SAR using the following equation,

$$SAR = \frac{\sigma |\mathbf{E}|^2}{\rho}$$

 $\sigma$ : represents the simulated tissue conductivity

 $\boldsymbol{\rho}:$  represents the tissue density

The EUT is set to transmit at the required power in line with product specification, at each frequency relating to the LOW, MID, and HIGH channel settings.

Pre-scans are made on the device to establish the location for the transmitting antenna, using a large area scan in either air or tissue simulation fluid.

The EUT is placed against the Universal Phantom where the maximum area scan dimensions are larger than the physical size of the resonating antenna. When the scan size is not large enough to cover the peak SAR distribution, it is modified by either extending the area scan size in both the X and Y directions, or the device is shifted within the predefined area.

The area scan is then run to establish the peak SAR location (interpolated resolution set at 1mm<sup>2</sup>) which is then used to orient the center of the zoom scan. The zoom scan is then executed and the 1g and 10g averages are derived from the zoom scan volume (interpolated resolution set at 1mm<sup>3</sup>).

#### 5. SAR Exposure Limits

SAR assessments have been made in line with the requirements of IEEE-1528, FCC Supplement C, and comply with ANSI/IEEE C95.1-1992 "Uncontrolled Environments" limits. These limits apply to a location which is deemed as "Uncontrolled Environment" which can be described as a situation where the general public may be exposed to an RF source with no prior knowledge or control over their exposure.

Type Exposure	Uncontrolled Environment Limit
Spatial Peak SAR (1g cube tissue for brain or body)	1.60 W/kg
Spatial Average SAR (whole body)	0.08 W/kg
Spatial Peak SAR (10g for hands, feet, ankles and wrist)	4.00 W/kg

#### Limits for General Population/Uncontrolled Exposure (W/kg)

### 6. Test Equipment List

Instrument	Manufacturer	Model No.	Serial No.	Last Calibration	Next Calibration
Data Acquisition Package	Aprel	ALS-DAQ-PAQ-2	QTK-337	Nov. 2006	only once
Aprel Laboratories Probe	Aprel	ALS-E020	265	May. 2008	May. 2009
Aprel Reference Dipole 5200Mhz	Aprel	ALS-D-5200-S-2	QTK-320	May. 2008	May. 2010
Aprel Reference Dipole 5800Mhz	Aprel	ALS-D-5800-S-2	QTK-321	May. 2008	May. 2010
Boundary Detection Sensor System	Aprel	ALS-PMDPS-2	QTK-336	N/A	N/A
Dielectric Probe Kit	Aprel	ALS-PR-DIEL	QTK-296	N/A	N/A
Universal Work Station	Aprel	ALS-UWS	QTK-326	N/A	N/A
Device Holder 2.0	Aprel	ALS-H-E-SET-2	QTK-294	N/A	N/A
Left Ear SAM Phantom	Aprel	ALS-P-SAM-L	QTK-292	N/A	N/A
Right Ear SAM Phantom	Aprel	ALS-P-SAM-R	QTK-288	N/A	N/A
Universal Phantom	Aprel	ALS-P-UP-1	QTK-246	N/A	N/A
Aprel Dipole Spacer	Aprel	ALS-DS-U	QTK-295	N/A	N/A
SAR Software	Aprel	ALSAS-10	Ver. 2.3.6	N/A	N/A
CRS C500C Controller	Thermo	ALS-C500	RCF0404433	N/A	N/A
CRF F3 Robot	Thermo	ALS-F3	RAF0412222	N/A	N/A
Power Amplifier	Mini-Circuit	ZHL-42	D051404-20	N/A	N/A
Directional Coupler	Agilent	778D-012	50550	N/A	N/A
Universal Radio	Rohde &	CMU 200	104846	Mar. 2008	Mar. 2009
Communication Tester	Schwarz				
Vector Network	Anritsu	MS4623B	992801	Aug. 2008	Aug. 2009
Signal Generator	Anritsu	MG3692A	042319	Jun. 2008	Jun. 2009
Power Meter	Anritsu	ML2487A	6K00001447	Apr. 2008	Apr. 2009
Wide Bandwidth Sensor	Anritsu	MA2491	030677	Apr. 2008	Apr. 2009



### 7. Measurement Uncertainty

### Exposure Assessment Measurement Uncertainty

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	c,` (1-g)	ci (10-g)	Standard Uncertainty (1-g) %	Standard Uncertainty (10-g) %
Measurement System							
Measurement system							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	√3	(1- cp) <sup>1/2</sup>	(1- cp) <sup>1/2</sup>	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	√3	√cp	√cp	4.4	4.4
Boundary Effect	1.0	rectangular	√3	1	1	0.6	0.6
Linearity	4.7	rectangular	√3	1	1	2.7	2.7
Detection Limit	1.0	rectangular	√3	1	1	0.6	D.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	√3	1	1	0.5	0.5
Integration Time	1.7	rectangular	√3	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	√3	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	√3	1	1	0.2	0.2
B							
Restriction			-	-			
Probe Positioning with respect to Phantom Shell	2.9	rectangular	√3	1	1	1.7	1.7
Extrapolation and	3.7	rectangular	√3	1	1	2.1	2.1
Integration	2.7	reconguiar	v -	-	1	~	~
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	4.7	rectangular	ЛЗ	1	1	2.7	2.7
Phantom and Setup							
Phantom Uncertainty(shape & thickness tolerance)	3.4	rectangular	√3	1	1	2.0	2.0
Liquid Conductivity(target)	5.0	rectangular	√3	0.7	0.5	2.0	1.4
Liquid Conductivity(meas.)	0.1	normal	1	0.7	0.5	0.1	0.0
Liquid Permittivity(target)	2.0	rectangular	νa	0.6	0.5	0.7	0.6
Liquid Permittivity(meas.)	2.6	normal	1	0.6	0.5	1.6	1.3
Combined Uncertainty		RSS				9.6	9.5
Combined Uncertainty (coverage factor=2)		Normal(k=2)				19.3	18.9

#### 8. Test Results

#### 8.1 SAR Test Results Summary

SAR MEASUREMENT						
Ambient Tem	perature (°C)	: 22.5 ±2	Relative Humidity (%): 53			
Liquid Temperature (°C) : 21.7 ±2				Depth of Liquid (cm):>15		
Product: 802.11a/b/g Wireless SDIO Card						
Test Mode: 802.11a(5200MHz)						
Test PositionAntennaBodyPosition	Antenna	Frequency		Conducted Power	SAR 1g	Limit
	Position	Channel	MHz	(dBm)	(W/kg)	(W/kg)
Bottom	Fixed	36	5180	16.96	0.174	1.6
Bottom	Fixed	52	5260	17.95	0.192	1.6
Bottom	Fixed	64	5320	17.82	0.273	1.6
Note: EUT was tested with IBM Notebook, M/N:X60.						

SAR MEASUREMENT						
Ambient Tem	perature (°C)	: 22.5 ±2	Relative Humidity (%): 53			
Liquid Temperature (°C) : 21.7 ±2				Depth of Liquid (cm):>15		
Product: 802.11a/b/g Wireless SDIO Card						
Test Mode: 802.11a(5800MHz)						
Test Position Antenna Body Position	Antenna	Frequency		Conducted Power (dBm)	<b>SAR</b> 1g (W/kg)	Limit (W/kg)
	Channel	MHz				
Bottom	Fixed	149	5745	18.16	0.323	1.6
Bottom	Fixed	157	5785	17.91	0.333	1.6
Bottom	Fixed	165	5825	18.41	0.324	1.6
Note: EUT was tested with IBM Notebook, M/N:X60.						

- Appendix
- Appendix A. SAR System Validation Data
- Appendix B. SAR measurement Data
- Appendix C. Test Setup Photographs & EUT Photographs
- Appendix D. Probe Calibration Data
- Appendix E. Dipole Calibration Data


#### Appendix A. SAR System Validation Data

ALSAS-10U VER 2.3.6 APREL Laboratories SAR Test Report

Report Date : 16-Jan-2009 Measurement Date : 16-Jan-2009 Product Data Device Name : Dipole-5200 Type : Dipole Frequency : 5200.00 MHz Max. Transmit Pwr : 1 W Drift Time : 0 min(s) Length : 23 mm Length 
 Width
 : 3.6 mm


 Depth
 : 89.8 mm
 Power Drift-Start : 30.768 W/kg Power Drift-Finish: 30.245 W/kg Power Drift (%) : -1.699 Phantom Data : Uni-Phantom Type Size (mm) : 280 x 280 x 200 : Center Location Tissue Data Type : HEAD Serial No. : 326-H Frequency : 5200.00 MHz Last Calib. Date : 16-Jan-2009 Last Callb. Date : 10-0an 2000Temperature: 21.70 °CAmbient Temp.: 22.50 °CHumidity: 53.00 RH%Epsilon: 40.33 F/mSigma: 5.35 S/mDensity: 1000.00 kg/cu. m Probe Data Name : Probe 265 : E020 Model Type : E-Field Triangle Serial No. : 265 Last Calib. Date : 09-May-2008 Frequency : 5200.00 MHz Duty Cycle Factor: 1 Conversion Factor: 3.5 Probe Sensitivity: 1.20 1.20 1.20  $\mu V/(V/m)^{2}$ Compression Point: 95.00 mV Offset : 1.56 mm

Measurement Dat	a
Crest Factor	: 1
Temperature	: 21.70 °C
Ambient Temp.	: 22.50 °C
Area Scan	: 5x6x1 : Measurement x=12mm, y=12mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Frequency	: 5200 MHz

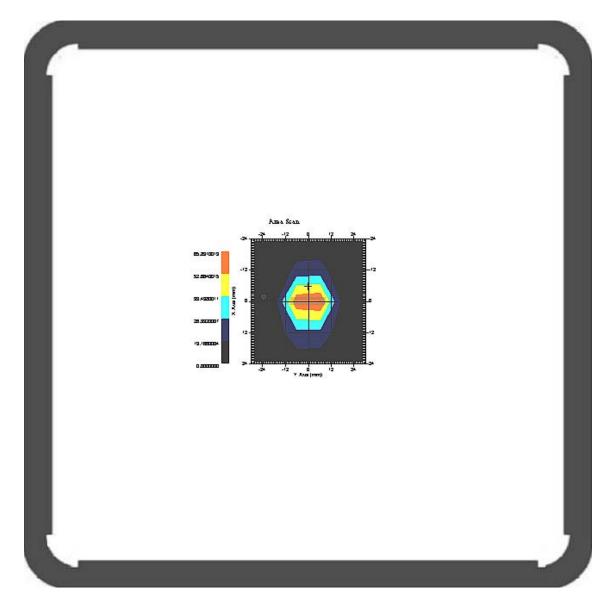


1 gram SAR value : 61.072 W/kg 10 gram SAR value : 20.625 W/kg Area Scan Peak SAR : 65.832 W/kg Zoom Scan Peak SAR : 190.11 W/kg

### This is previous page plot (zoom in)

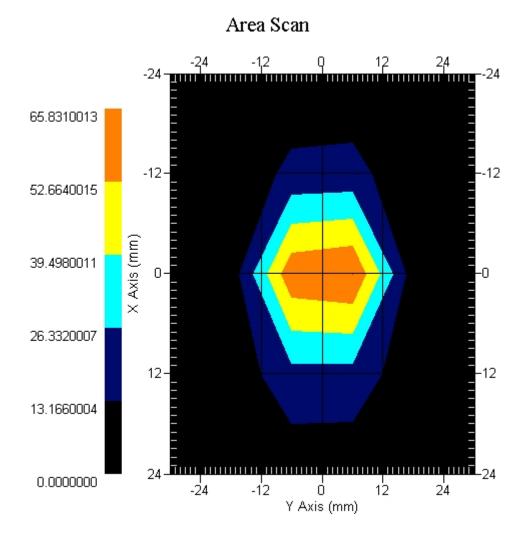



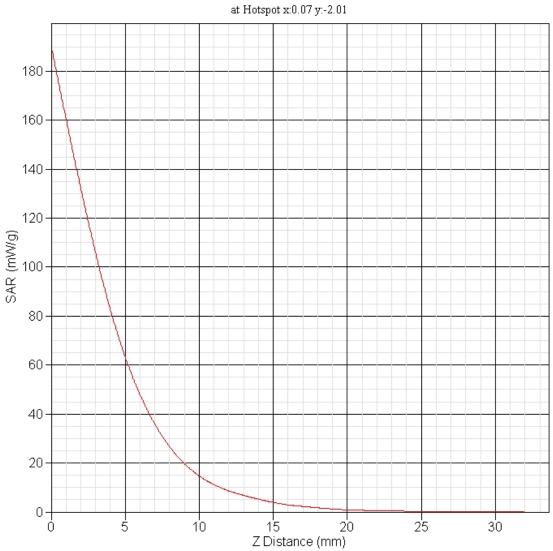

SAR-Z Axis




#### ALSAS-10U VER 2.3.6 APREL Laboratories

#### SAR Test Report

Report Date : 16-Jan-2009 Measurement Date : 16-Jan-2009 Product Data Device Name : Dipole-5200 Type : Dipole Frequency : 5800.00 MHz Туре : Dipole Max. Transmit Pwr : 1 W Drift Time : 0 min(s) Lenqth : 21.4 mm 
 Width
 : 3.6 mm


 Depth
 : 89.8 mm
 : 89.8 mm Power Drift-Start : 30.754 W/kg Power Drift-Finish: 31.367 W/kg Power Drift (%) : 1.993 Phantom Data Туре : Uni-Phantom : 280 x 280 x 200 : Center Size (mm) Location Tissue Data Type : HEAD Serial No. : 327-H Frequency : 5800.00 MHz Last Calib. Date : 16-Jan-2009 Last Callb. Date : 16-0all-2009Temperature: 20.80 °CAmbient Temp.: 21.30 °CHumidity: 55.00 RH%Epsilon: 35.55 F/mSigma: 6.54 S/mDensity: 1000.00 kg/cu. m Probe Data Name : Probe 265 : Probe : E020 Model Type : E-Field Triangle Serial No. : 265 Last Calib. Date : 09-May-2008 Frequency : 5800.00 MHz Duty Cycle Factor: 1 Conversion Factor: 3.4 Probe Sensitivity: 1.20 1.20 1.20  $\mu V / (V/m)^{2}$ Compression Point: 95.00 mV Offset : 1.56 mm

Measurement Dat	a
Crest Factor	: 1
Tissue Temp.	: 20.80 °C
Ambient Temp.	: 21.30 °C
Area Scan	: 5x6x1 : Measurement x=12mm, y=12mm, z=4mm
Zoom Scan	: 7x7x7 : Measurement x=5mm, y=5mm, z=5mm
Frequency	: 5800 MHz

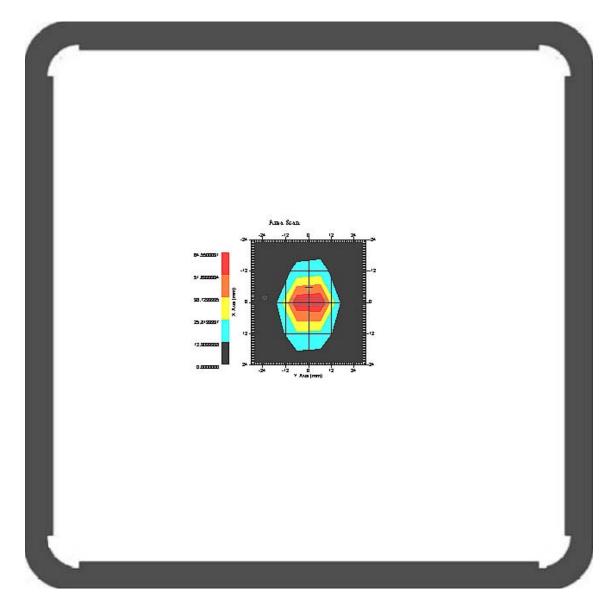


1 gram SAR value : 60.332 W/kg 10 gram SAR value : 21.142 W/kg Area Scan Peak SAR : 64.552 W/kg Zoom Scan Peak SAR : 203.161 W/kg

### This is previous page plot (zoom in)

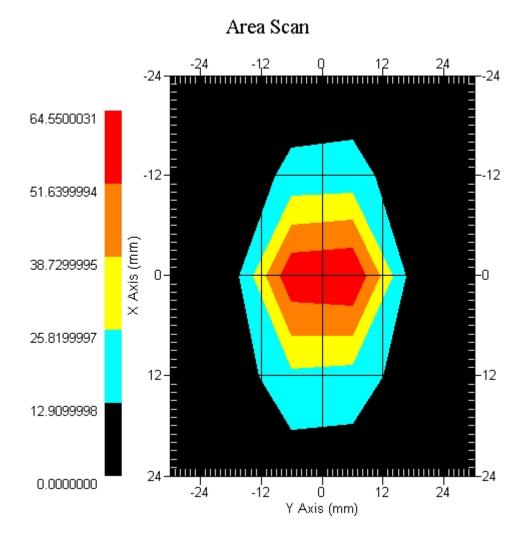



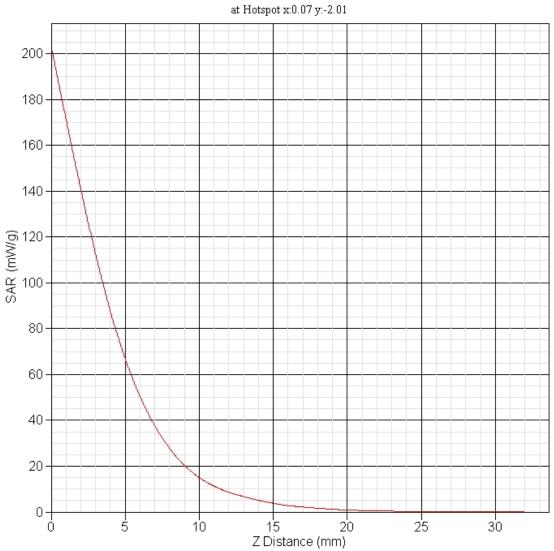

SAR-Z Axis




#### Appendix B. SAR measurement Data

ALSAS-10U VER 2.3.6 APREL Laboratories


SAR Test Report –802.11a(5200MHz)


Report Date : 16-Jan-2009 Measurement Date : 16-Jan-2009 Product Data Device Name : 802.11a/b/q Wireless SDIO Card : Other : SDW3100 Туре Model Model: SDW3100Frequency: 5200.00 MHzDrift Time: 0 min(s)Length: 39.8 mmWidth: 24 mmDepth: 2.2 mmAntenna Type: Internal Phantom Data : Uni-Phantom : 280 x 280 x 200 : Center Type Size (mm) Location Tissue Data Type : BODY Serial No. : 326-B Frequency : 5200.00 MHz Last Calib. Date : 16-Jan-2009 Last Callb. Date : 16-Jan-2009 Temperature : 21.70 °C Ambient Temp. : 22.50 °C Humidity : 53.00 RH% Epsilon : 48.43 F/m Sigma : 5.42 S/m Density : 1000.00 kg/cu. m Probe Data Name : Probe 265 Model : E020 Type : E-Field Triangle Serial No. : 265 Last Calib. Date : 09-May-2008 Frequency : 5200.00 MHz Duty Cycle Factor: 1 Conversion Factor: 4.3 Probe Sensitivity: 1.20 1.20 1.20  $\mu V/(V/m)^{2}$ Compression Point: 95.00 mV Offset : 1.56 mm

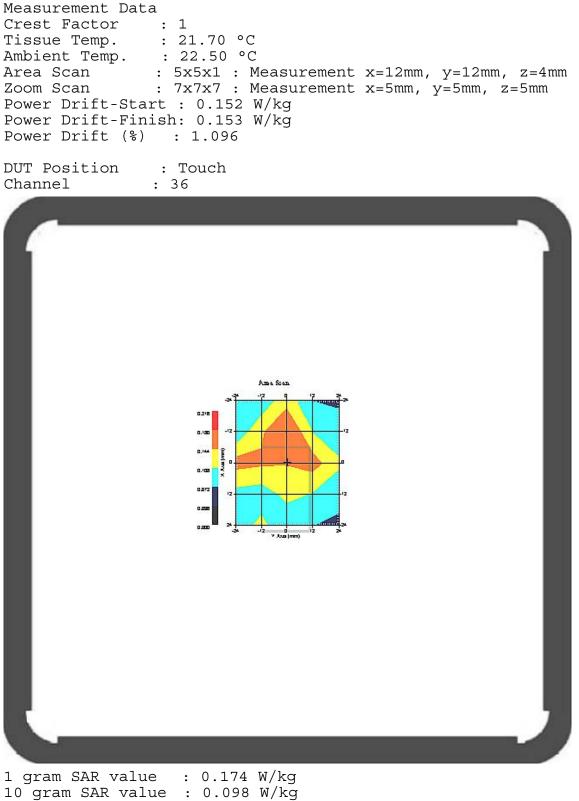

1 gram SAR value : 0.174 W/kg 10 gram SAR value : 0.098 W/kg Area Scan Peak SAR : 0.182 W/kg Zoom Scan Peak SAR : 0.400 W/kg


### This is previous page plot (zoom in)

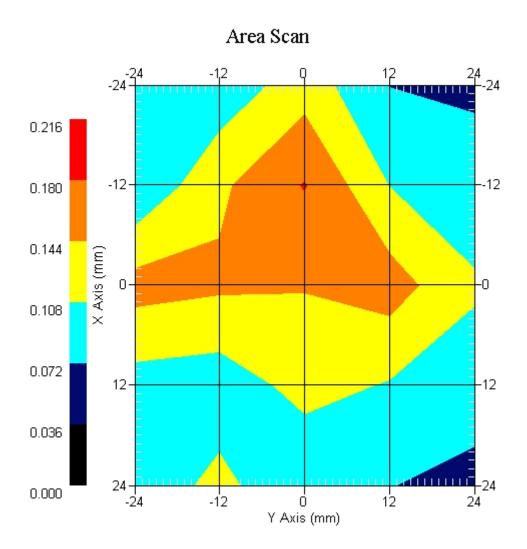


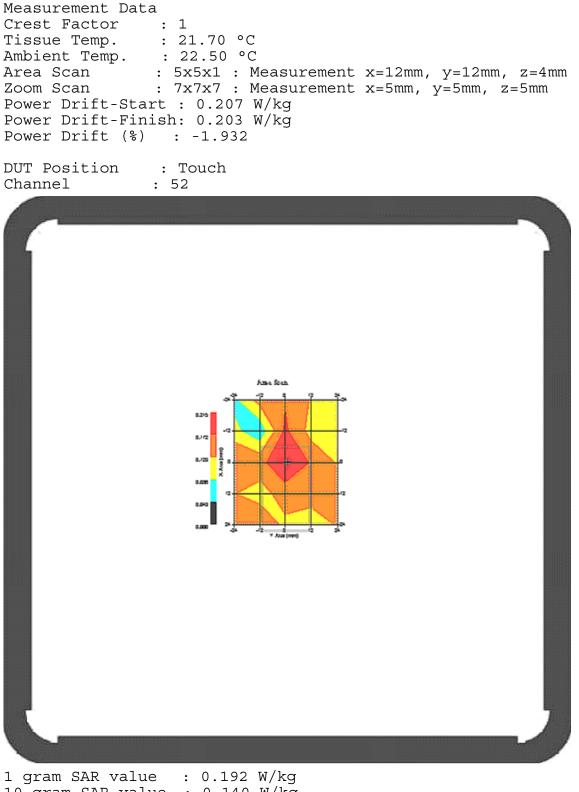

1 gram SAR value : 0.192 W/kg 10 gram SAR value : 0.140 W/kg Area Scan Peak SAR : 0.214 W/kg Zoom Scan Peak SAR : 0.100 W/kg


## This is previous page plot (zoom in)

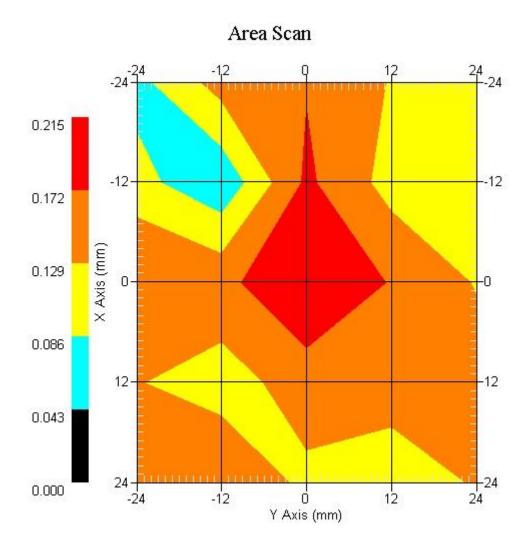

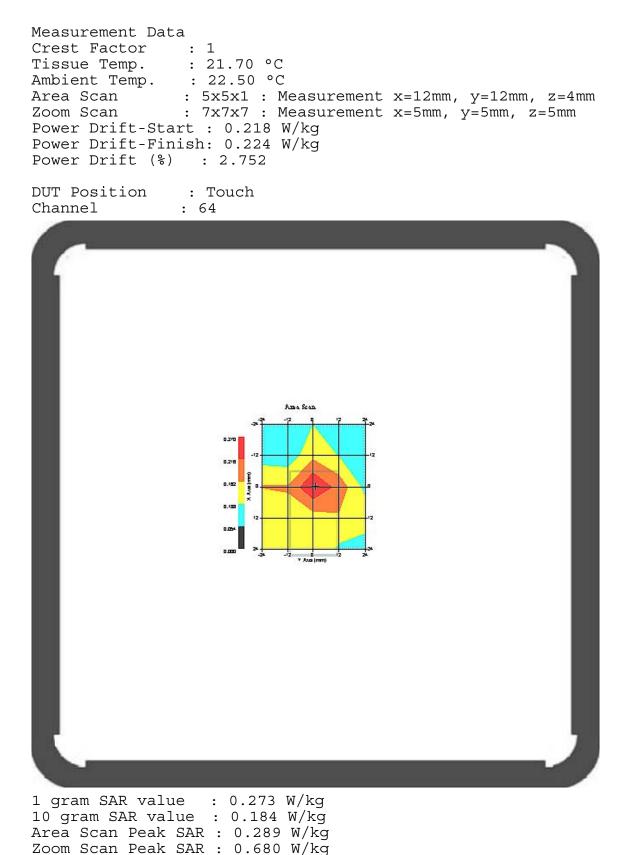


Page: 6 of 16

This is previous page plot (zoom in)

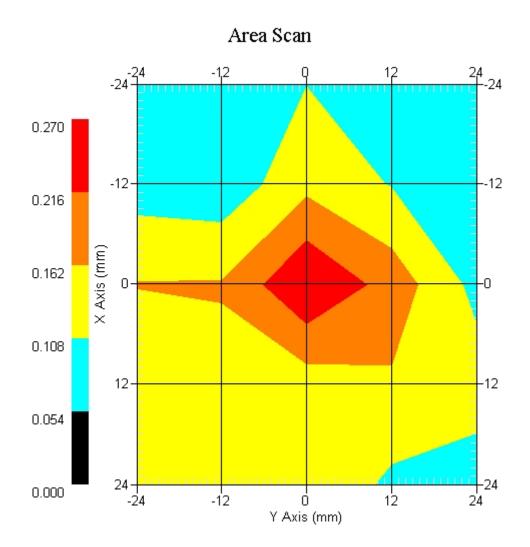


## 802.11a(5200MHz) EUT Bottom Z-Axis plot Channel: 64

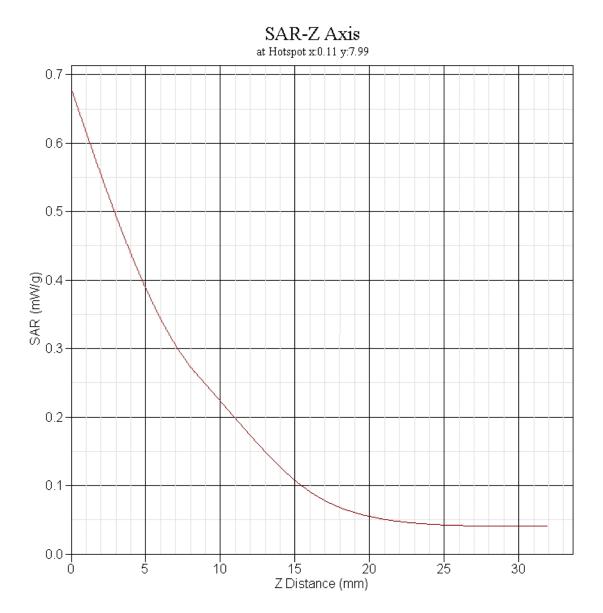


#### SAR measurement Data


ALSAS-10U VER 2.3.6 APREL Laboratories SAR Test Report -802.11a(5800MHz) Report Date : 16-Jan-2009 Measurement Date : 16-Jan-2009 Product Data Device Name : 802.11a/b/g Wireless SDIO Card : Other Туре Model : SDW3100 : 5800.00 MHz : 0 min(s) : 39.8 mm Frequency Drift Time Length Width: 24 mmDepth: 2.2 mmAntenna Type: Internal Phantom Data : Uni-Phantom mm) : 280 x 280 x 200 on : Center Type Size (mm) Location Tissue Data Type : BODY Serial No. : 327-B Frequency : 5800.00 MHz Last Calib. Date : 16-Jan-2009 Temperature : 21.70 °C Ambient Temp. : 22.50 °C Humidity : 53.00 RH% Epsilon : 49.22 F/m Sigma : 6.14 S/m Density : 1000.00 kg/cu. m Probe Data Name : Probe 265 Model : E020 · E-Field T Model Type Type : E-Field Triangle Serial No. : 265 Last Calib. Date : 09-May-2008 Frequency : 5800.00 MHz Duty Cycle Factor: 1 Conversion Factor: 3.9 Probe Sensitivity: 1.20 1.20 1.20  $\mu V/(V/m)^{2}$ Compression Point: 95.00 mV Offset : 1.56 mm

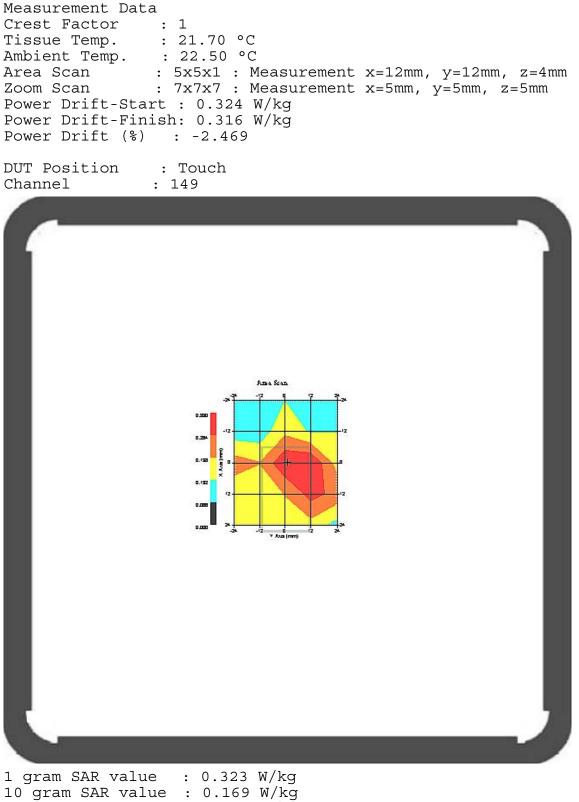

10 gram SAR value : 0.1525 W/kg Area Scan Peak SAR : 0.330 W/kg Zoom Scan Peak SAR : 0.825 W/kg


This is previous page plot (zoom in)

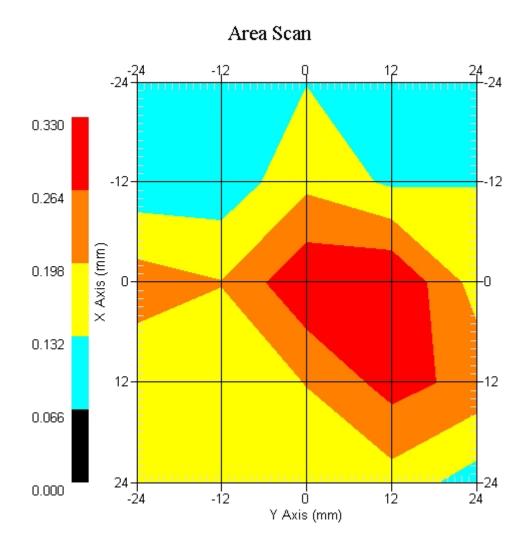


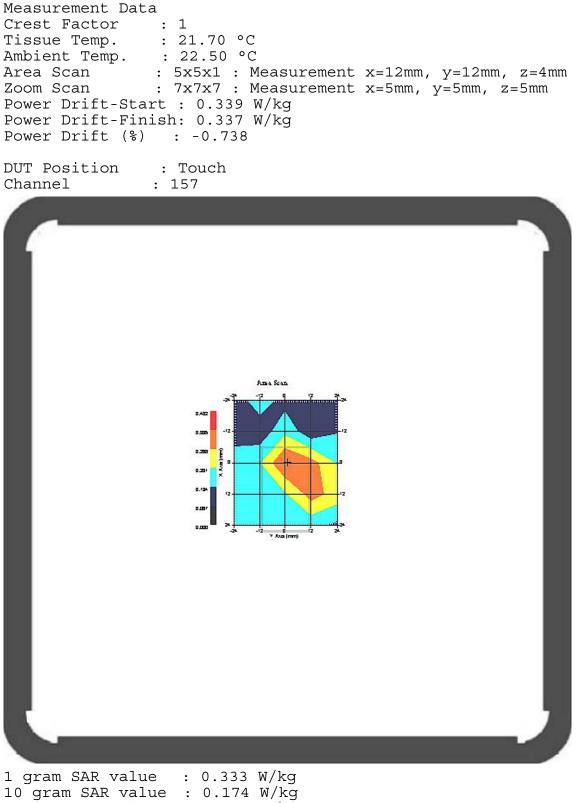

10 gram SAR value : 0.174 W/kg Area Scan Peak SAR : 0.336 W/kg Zoom Scan Peak SAR : 0.830 W/kg


## This is previous page plot (zoom in)

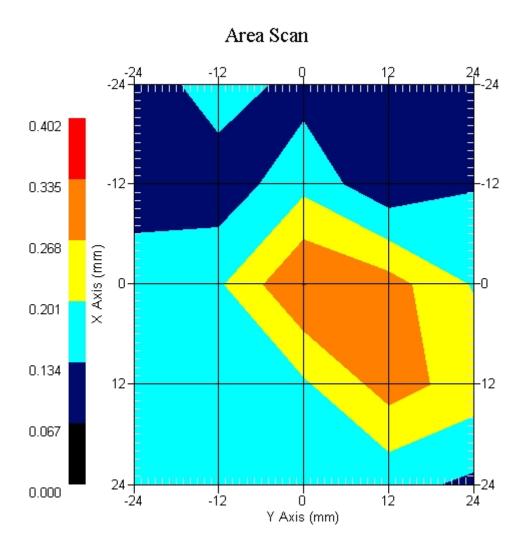

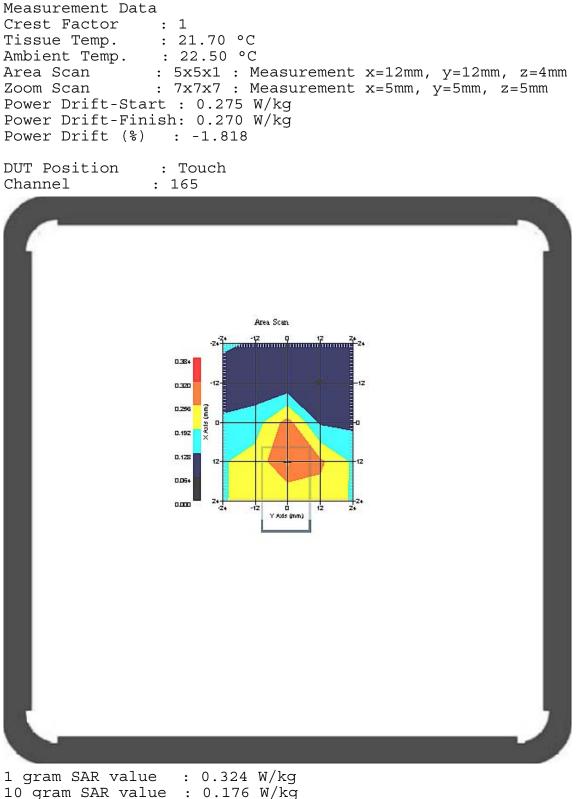


1 gram SAR value : 0.324 W/kg 10 gram SAR value : 0.176 W/kg Area Scan Peak SAR : 0.322 W/kg Zoom Scan Peak SAR : 0.790 W/kg

## This is previous page plot (zoom in)

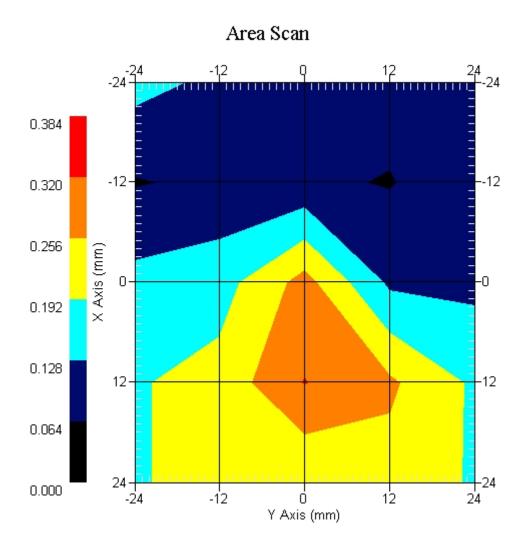



#### 802.11a(5800MHz) EUT Bottom Z-Axis plot Channel: 157

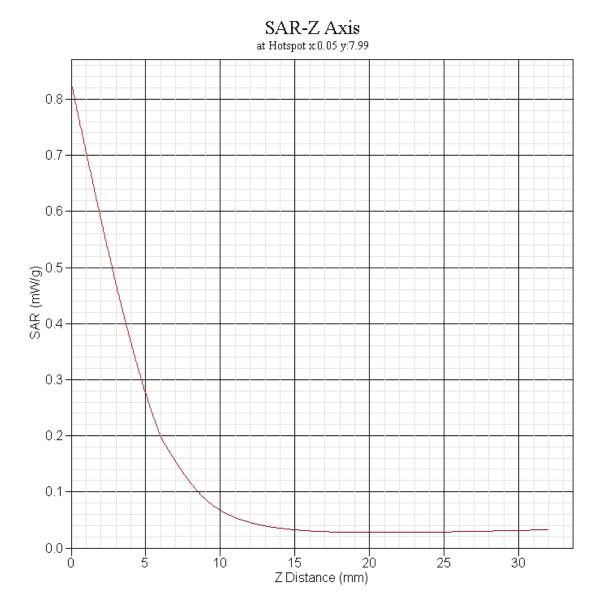




### Appendix C. Test Setup Photographs & EUT Photographs Test Setup Photographs



EUT Bottom-Zoom out

**EUT Bottom-Zoom In** 

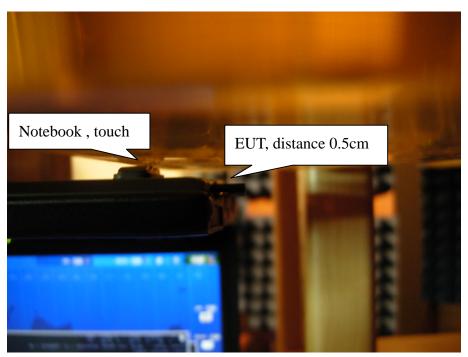

Note: The positions used in the measurements were according to IEEE 1528-2003.



## EUT Photographs









## Appendix D. Probe Calibration Data

Miniature Isotropic RF Probe M/N: ALS-E-020 S/N: 265

5200 MHz Head Calibration 5200 MHz Body Calibration

#### NCL CALIBRATION LABORATORIES

Calibration File No.: CP-883

**Client: QUIETEK** 

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5200 MHz

Manufacturer: APREL Laboratories Model No.: ALS-E-020 Serial No.: 265

**HEAD** Calibration

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2 Project No: QTKB-ALS-E20-CAL-5335

> Calibrated: 9<sup>th</sup> May 2008 Released on: 9<sup>th</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary Released By: <u>
NCLCALIBRATION LABORATORIES</u> 51 SPECTRUM WAY Division of APREL Lab.

TEL: (613) 820-4988

FAX: (613) 820-4161

NEPEAN, ONTARIO

CANADA K2R 1E6

#### Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 265.

#### References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head Due to Wireless Communications Devices: Experimental Techniques"

SSI-TP-011 Tissue Calibration Procedure

IEC 62209 "Human exposure to radio frequency fields from hand-held and Headmounted wireless communication devices – Human models, instrumentation, and procedures –Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for hand-held devices used in close proximity of the ear (frequency range of 300 MHz to 3 GHz)"

IEEE 1309 Draft Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9kHz to 40GHz

### Conditions

Probe 265 is a re-calibration.

Ambient Temperature of the Laboratory: $22 \ ^{\circ}C \ +/- \ 0.5^{\circ}C$ Temperature of the Tissue: $21 \ ^{\circ}C \ +/- \ 0.5^{\circ}C$ 

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within/this report has been reviewed for accuracy.

Stuart Nicol

Jesse Hones

## **Calibration Results Summary**

Probe Type:	E-Field Probe E-020
Serial Number:	265
Frequency:	5200 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

## Sensitivity in Air

Channel X: Channel Y:	1.2 μV/(V/m) <sup>2</sup> 1.2 μV/(V/m) <sup>2</sup>
Channel Z:	$1.2 \mu V/(V/m)^2$
Diode Compression Point:	95 mV

Frequency	:	5200 MHz	
Epsilon:	35.9 (+/-10%)	Sigma:	4.7 S/m (+/-5%)
ConvF			
Channel X:	3.5		
Channel Y:	3.5		
Channel Z:	3.5		

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


#### **Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.


### **Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

## **Receiving Pattern 5200 MHz (Air)**

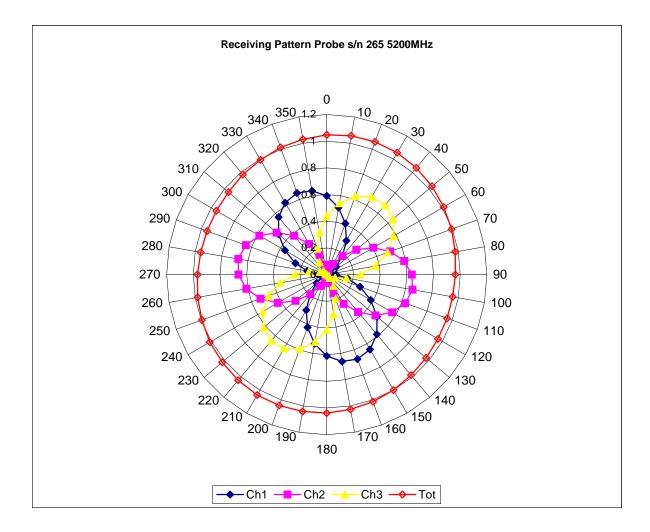

## Isotropy Error 5200 MHz (Air)

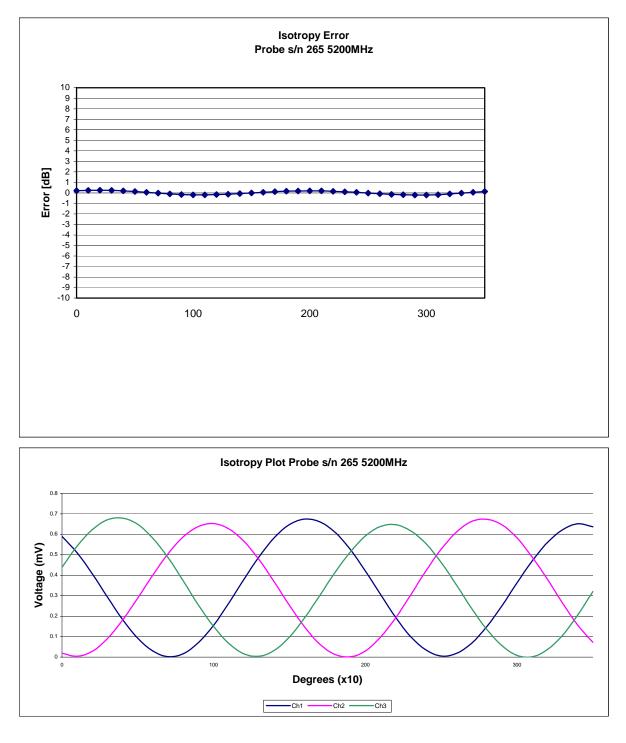


#### **Isotropicity in Tissue:**

0.10 dB


#### **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Dynamic Range**

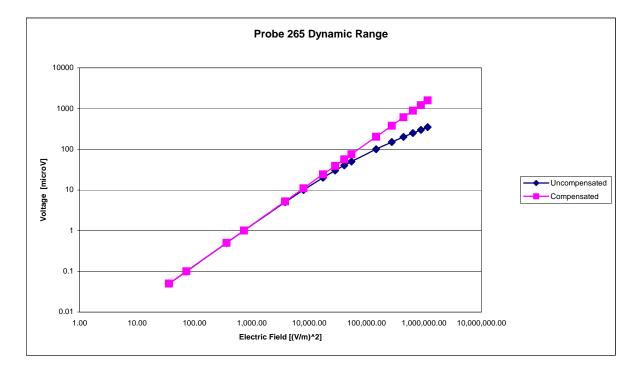

## Video Bandwidth

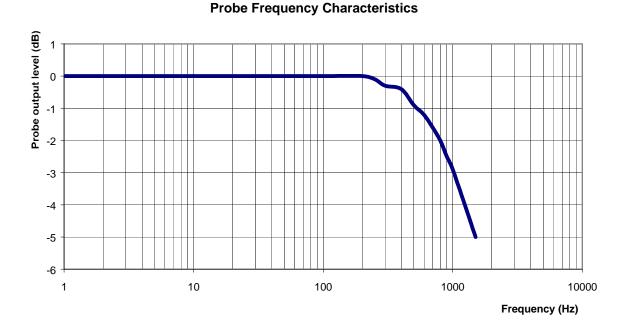

Video Bandwidth at 500 Hz1 dBVideo Bandwidth at 1000 Hz3 dB

### **Conversion Factor Uncertainty Assessment**

Frequency:		5200MHz	
Epsilon:	35.9 (+/-10%)	Sigma:	4.7 S/m (+/-5%)
ConvF			
Channel X:	3.5	7%(K=2)	
Channel Y:	3.5	7%(K=2)	
Channel Z:	3.5	7%(K=2)	

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

#### **Boundary Effect:**

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

### **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

### NCL CALIBRATION LABORATORIES

Calibration File No.: CP-884

Client: QUIETEK

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5200 MHz

Manufacturer: APREL Laboratories Model No.: ALS-E-020 Serial No.: 265

**BODY Calibration** 

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2 Project No: QTKB-ALS-E20-CAL-5335

> Calibrated: 9<sup>th</sup> May 2008 Released on: 9<sup>th</sup> May 2008

This Calibration Certific	ate is Incomplete Unless Accom	panied with the Calibration Results Summary	
Released By:	Smalla	Ŵ	
<b>NCL</b> CALIBRATION LABORATORIES			
	51 SPECTRUM WAY	Division of APREL Lab.	

51 SPECTRUM WAY NEPEAN, ONTARIO CANADA K2R 1E6 Division of APREL Lab. TEL: (613) 820-4988 FAX: (613) 820-4161

#### Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 265.

#### References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head Due to Wireless Communications Devices: Experimental Techniques"

SSI-TP-011 Tissue Calibration Procedure

IEC 62209 "Human exposure to radio frequency fields from hand-held and Headmounted wireless communication devices – Human models, instrumentation, and procedures –Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for hand-held devices used in close proximity of the ear (frequency range of 300 MHz to 3 GHz)"

IEEE 1309 Draft Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9kHz to 40GHz

### Conditions

Probe 265 is a re-calibration.

Ambient Temperature of the Laboratory:	22 °C +/- 0.5°C
Temperature of the Tissue:	21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within/this report has been reviewed for accuracy.

Stuart Nicol

Jesse Hones

## **Calibration Results Summary**

Probe Type:	E-Field Probe E-020
Serial Number:	265
Frequency:	5200 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

## Sensitivity in Air

Channel X: Channel Y:	1.2 μV/(V/m) <sup>2</sup> 1.2 μV/(V/m) <sup>2</sup>
Channel Z:	$1.2 \mu V/(V/m)^2$
Diode Compression Point:	95 mV

Frequency	:	5200 MHz	
Epsilon:	48.9 (+/-10%)	Sigma:	5.35 S/m (+/-5%)
ConvF			
Channel X:	4.3		
Channel Y:	4.3		
Channel Z:	4.3		

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


#### **Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.


### **Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

## **Receiving Pattern 5200 MHz (Air)**

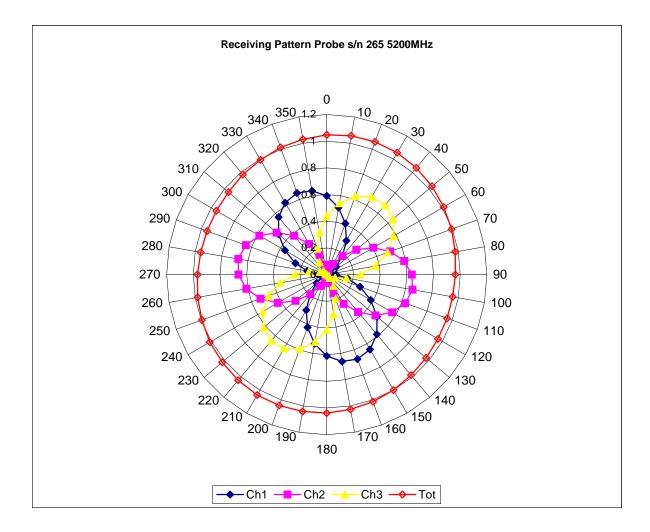

## Isotropy Error 5200 MHz (Air)

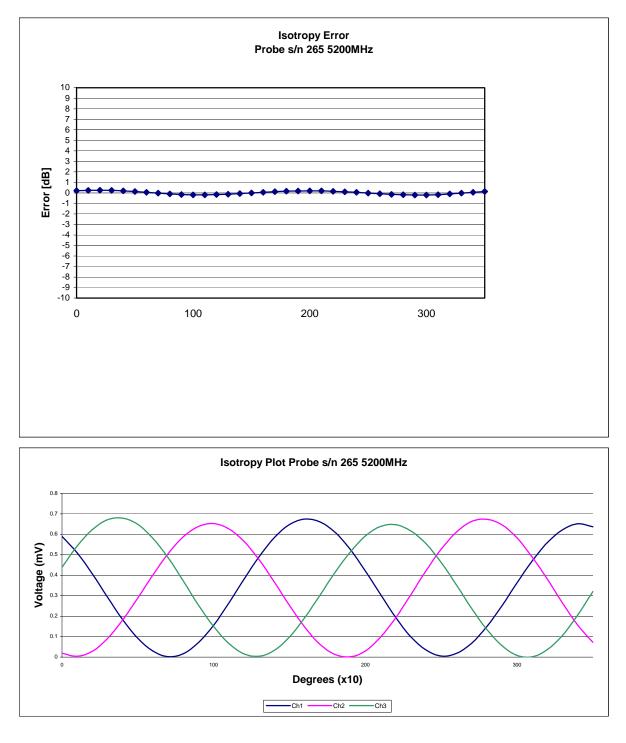


#### **Isotropicity in Tissue:**

0.10 dB


#### **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Dynamic Range**

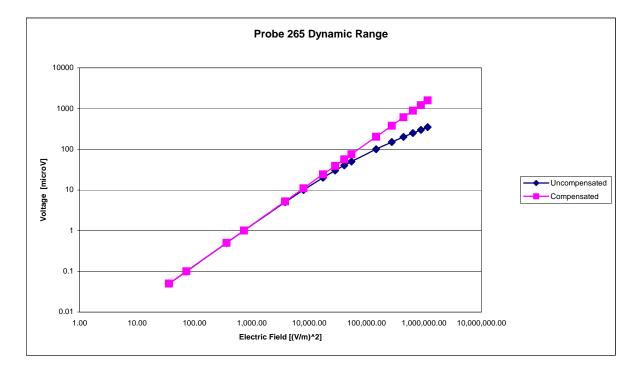

## Video Bandwidth

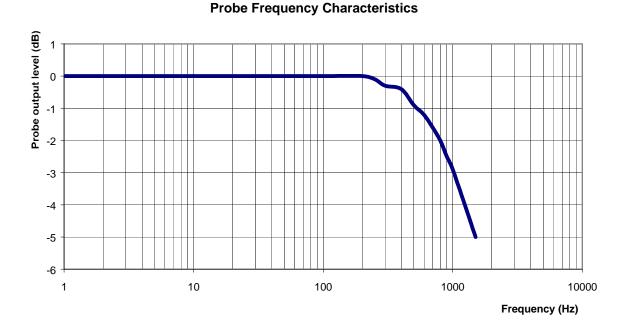

Video Bandwidth at 500 Hz1 dBVideo Bandwidth at 1000 Hz3 dB

### **Conversion Factor Uncertainty Assessment**

Frequency:		5200MHz	
Epsilon:	48.9 (+/-10%)	Sigma:	5.35 S/m (+/-5%)
ConvF			
Channel X:	4.3	7%(K=2)	
Channel Y:	4.3	7%(K=2)	
Channel Z:	4.3	7%(K=2)	

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

#### **Boundary Effect:**

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

### **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.



## Appendix D. Probe Calibration Data

Miniature Isotropic RF Probe M/N: ALS-E-020 S/N: 265

5800 MHz Head Calibration 5800 MHz Body Calibration

#### NCL CALIBRATION LABORATORIES

Calibration File No.: CP-885

Client: QUIETEK

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5800 MHz

Manufacturer: APREL Laboratories Model No.: ALS-E-020 Serial No.: 265

**HEAD** Calibration

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2 Project No: QTKB-ALS-E20-CAL-5335

> Calibrated: 9<sup>th</sup> May 2008 Released on: 9<sup>th</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary Released By: <u>
NCL CALIBRATION LABORATORIES</u> 51 SPECTRUM WAY NEPEAN, ONTARIO Division of APREL Lab. TEL: (613) 820-4988

FAX: (613) 820-4161

CANADA K2R 1E6

#### Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 265.

#### References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head Due to Wireless Communications Devices: Experimental Techniques"

SSI-TP-011 Tissue Calibration Procedure

IEC 62209 "Human exposure to radio frequency fields from hand-held and Headmounted wireless communication devices – Human models, instrumentation, and procedures –Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for hand-held devices used in close proximity of the ear (frequency range of 300 MHz to 3 GHz)"

IEEE 1309 Draft Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9kHz to 40GHz

### Conditions

Probe 265 is a re-calibration.

Ambient Temperature of the Laboratory: $22 \ ^{\circ}C \ +/- \ 0.5^{\circ}C$ Temperature of the Tissue: $21 \ ^{\circ}C \ +/- \ 0.5^{\circ}C$ 

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within/this report has been reviewed for accuracy.

Stuart Nicol

Jesse Hones

## Calibration Results Summary

Probe Type:	E-Field Probe E-020
Serial Number:	265
Frequency:	5800 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

## Sensitivity in Air

Channel X: Channel Y:	1.2 μV/(V/m) <sup>2</sup> 1.2 μV/(V/m) <sup>2</sup>
Channel Z:	$1.2 \mu V/(V/m)^2$
Diode Compression Point:	95 mV

Frequency	:	5800 MHz	
Epsilon:	35.3 (+/-10%)	Sigma:	5.27 S/m (+/-5%)
ConvF			
Channel X:	3.4		
Channel Y:	3.4		
Channel Z:	3.4		

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


#### **Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.


### **Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

## **Receiving Pattern 5800 MHz (Air)**

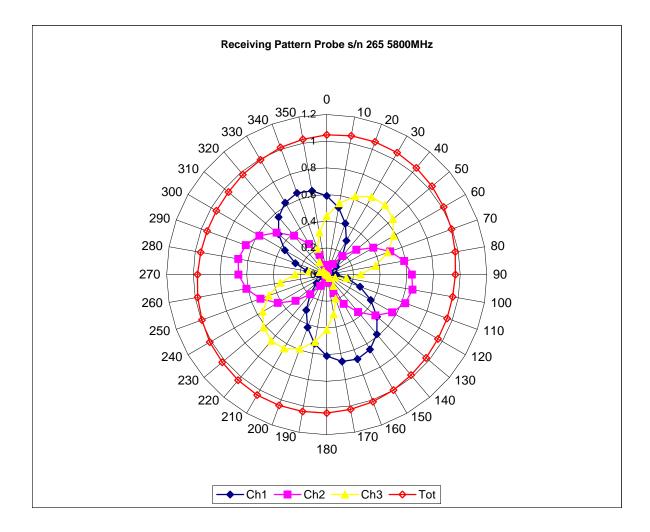

## Isotropy Error 5800 MHz (Air)

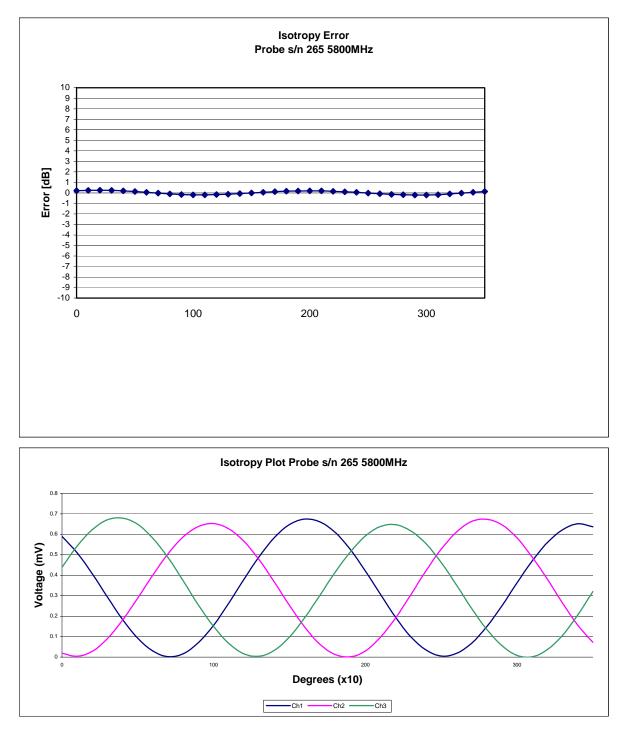


#### **Isotropicity in Tissue:**

0.10 dB


#### **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Dynamic Range**

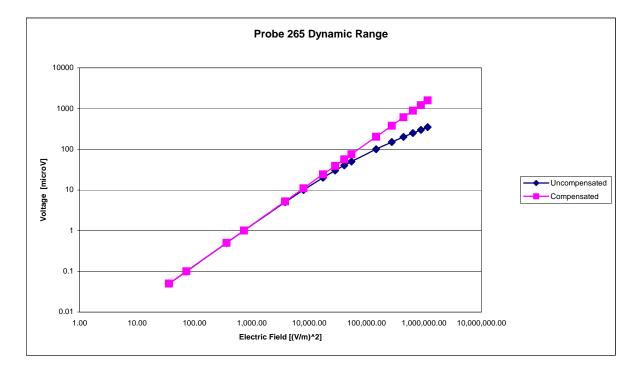

## Video Bandwidth

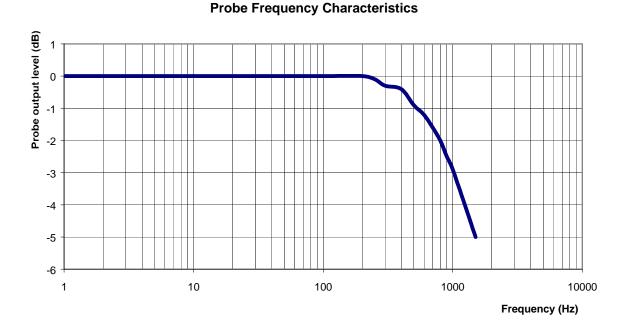

Video Bandwidth at 500 Hz1 dBVideo Bandwidth at 1000 Hz3 dB

## **Conversion Factor Uncertainty Assessment**

Frequency:		5800MHz
Epsilon:	35.3 (+/-10%)	Sigma: 5.27 S/m (+/-5%)
ConvF		
Channel X:	3.4	7%(K=2)
Channel Y:	3.4	7%(K=2)
Channel Z:	3.4	7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

#### **Boundary Effect:**

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.

#### NCL CALIBRATION LABORATORIES

Calibration File No.: CP-886

**Client: QUIETEK** 

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5800 MHz

Manufacturer: APREL Laboratories Model No.: ALS-E-020 Serial No.: 265

**BODY Calibration** 

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2 Project No: QTKB-ALS-E20-CAL-5335

> Calibrated: 9<sup>th</sup> May 2008 Released on: 9<sup>th</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary
Released By:
NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY NEPEAN, ONTARIO CANADA K2R 1E6 Division of APREL Lab. TEL: (613) 820-4988 FAX: (613) 820-4161

#### Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 265.

#### References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head Due to Wireless Communications Devices: Experimental Techniques"

SSI-TP-011 Tissue Calibration Procedure

IEC 62209 "Human exposure to radio frequency fields from hand-held and Headmounted wireless communication devices – Human models, instrumentation, and procedures –Part 1 & 2: Procedure to determine the Specific Absorption Rate (SAR) for hand-held devices used in close proximity of the ear (frequency range of 300 MHz to 3 GHz)"

IEEE 1309 Draft Standard for Calibration of Electromagnetic Field Sensors and Probes, Excluding Antennas, from 9kHz to 40GHz

#### Conditions

Probe 265 is a re-calibration.

Ambient Temperature of the Laboratory: $22 \degree C + - 0.5\degree C$ Temperature of the Tissue: $21 \degree C + - 0.5\degree C$ 

We the undersigned attest that to the best of our knowledge the calibration of this probe has been accurately conducted and that all information contained within/this report has been reviewed for accuracy.

Stuart Nicol

Jesse Hones

## **Calibration Results Summary**

Probe Type:	E-Field Probe E-020
Serial Number:	265
Frequency:	5800 MHz
Sensor Offset:	1.56 mm
Sensor Length:	2.5 mm
Tip Enclosure:	Ertalyte*
Tip Diameter:	<5 mm
Tip Length:	60 mm
Total Length:	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

## Sensitivity in Air

Channel X: Channel Y:	1.2 μV/(V/m) <sup>2</sup> 1.2 μV/(V/m) <sup>2</sup>
Channel Z:	$1.2 \mu V/(V/m)^2$
Diode Compression Point:	95 mV

Frequency	:	5800 MHz	
Epsilon:	48.2 (+/-10%)	Sigma:	6.0 S/m (+/-5%)
ConvF			
Channel X:	3.9		
Channel Y:	3.9		
Channel Z:	3.9		

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.


#### **Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.44mm.


### **Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.

## Receiving Pattern 5800 MHz (Air)

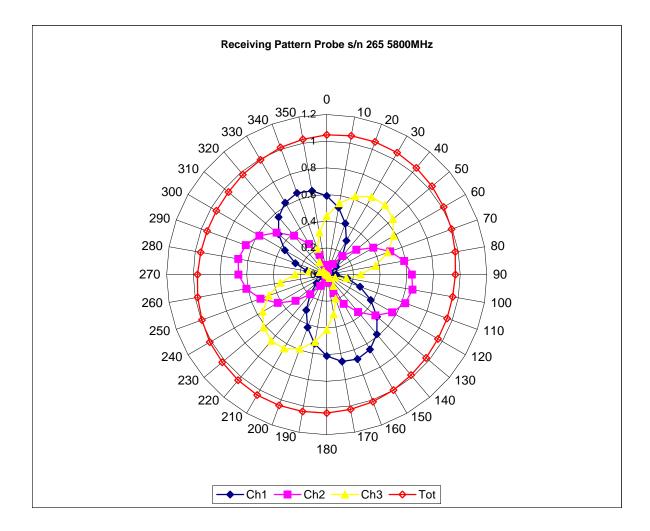

## Isotropy Error 5800 MHz (Air)

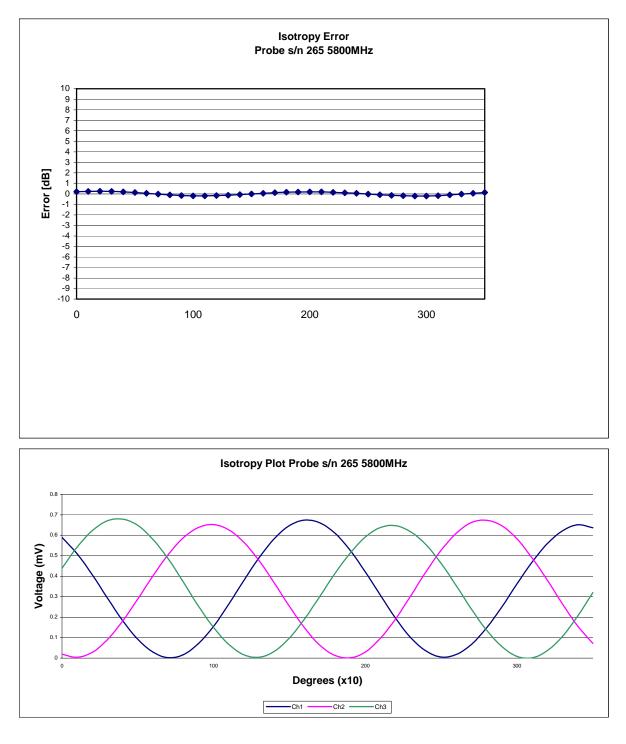


#### **Isotropicity in Tissue:**

0.10 dB


#### **NCL Calibration Laboratories**

Division of APREL Laboratories.

## **Dynamic Range**

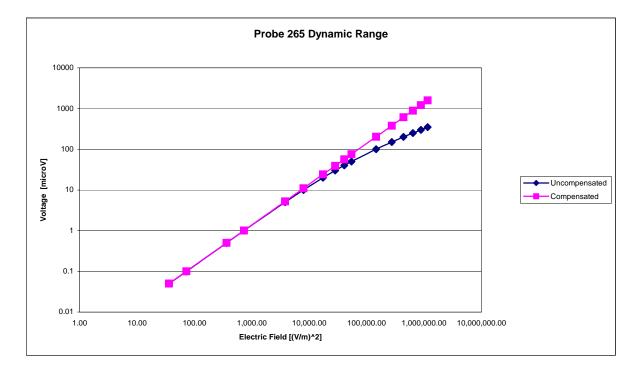

## Video Bandwidth

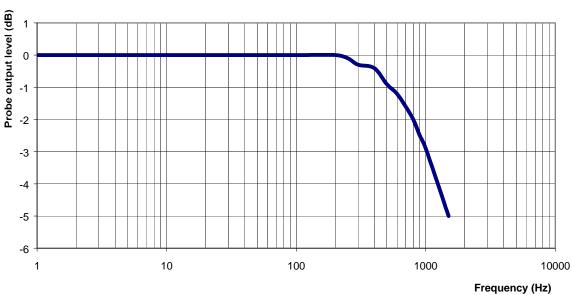

Probe Frequency Characteristics

Video Bandwidth at 500 Hz	1 dB
Video Bandwidth at 1000 Hz	3 dB

## **Conversion Factor Uncertainty Assessment**

Frequency:		5800MHz
Epsilon:	48.2 (+/-10%)	Sigma: 6.0 S/m (+/-5%)
ConvF		
Channel X:	3.9	7%(K=2)
Channel Y:	3.9	7%(K=2)
Channel Z:	3.9	7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

#### **Boundary Effect:**

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.



## Appendix E. Dipole Calibration

Validation Dipole 5200 MHz M/N: ALS-D-5200-S-2 S/N: QTK-320

#### **NCL CALIBRATION LABORATORIES**

Calibration File No: DC-892

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the NCL CALIBRATION LABORATORIES by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

**Quietek Validation Dipole** 

Manufacturer: APREL Laboratories Part number: ALS-D-5200-S-2 Frequency: 5.2 GHz Serial No: QTK-320

Customer: Quietek

Project Number: QTKB-Dipole-CAL-5336

Calibrated: 9<sup>th</sup> May 2008 Released on: 9<sup>th</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summar	v
This Calibration Certificate is incomplete offess Accompanied with the Calibration Results outfinnar	y
$\langle \mathbf{x}   \mathbf{x} \rangle$	
Released By:	
NCL CALIBRATION LABORATORIES	

51 SPECTRUM WAY Division of APREL Lab. NEPEAN, ONTARIO CANADA K2R 1E6

TEL: (613) 820-4988 FAX: (613) 820-4161

## **Calibration Results Summary**

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

#### **Mechanical Dimensions**

Length:	23.6 mm
Height:	14.0 mm

#### **Electrical Specification**

SWR:	1.57 U
Return Loss:	-13.15 dB
Impedance:	78.2 Ω

#### **System Validation Results**

5200 GHz 58.8 Course Scan Data X Axis (mm) -10 0 10 20 30 20 10 20 10 20 10 10 20 10 20 10 10 20 10 0 10 20 10 0 10 20 10 0 10 20 10 0 10 20 10 0 10 20 10 0 10 20 10 0 10 20 10 0 10 20 10 0 10 20 10 0 10 20 10 0 10 20 10 0 10 20 -10 0 10 20 -10 0 10 20 -10 -10 0 0 -20 -30 -10 0 10 20 -30 -10 -20 -30 -10 0 10 20 X Axis (mm)	Frequency	1 Gram	
X Axis (mm) $-10 \ 0 \ 10 \ 20$ $30^{-10} \ 0 \ 10 \ 20$ $10^{-10} \ 0 \ 10 \ 20$ $10^{-10} \ 0 \ 10 \ 20$ $10^{-10} \ 0 \ -10$ $-20^{-10} \ -10 \ -20$ $-30^{-10} \ 0 \ 10 \ 20$	5200 GHz	58.8	]
$(u_{w})$ $(v_{w})$ $(v_{$	- 1( 30 -	Course Scan Data X Axis (mm	20
	(mm) sixA - 10		- 10 (mm) 0 ivy - 10 × - 10 × - 20

### Conditions

Dipole 320 is a recalibration.

Ambient Temperature of the Laboratory:	22 °C +/- 0.5°C
Temperature of the Tissue:	21 °C +/- 0.5°C

#### References

SSI-TP-018-ALSAS Dipole Calibration Procedure

SSI-TP-016 Tissue Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

IEC 62209 "Human exposure to radio frequency fields from hand-held and bodymounted wireless communication devices – Human models, instrumentation, and procedures –Part 1 & Part 2: Procedure to determine the specific absorption rate (SAR) for mobile wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

Stuart Nicol

C. Teodorian

# **NCL Calibration Laboratories** Division of APREL Laboratories.

## **Dipole Calibration Results**

#### **Mechanical Verification**

APREL	APREL	Measured	Measured
Length	Height	Length	Height
23.6 mm	14.0 mm	23.1 mm	14.2 mm


#### **Tissue Validation**

Head Tissue 5200 MHz	Measured
Dielectric constant, ε <sub>r</sub>	39.94
Conductivity, σ [S/m]	5.24

#### **Electrical Calibration**

Test	Result
S11 R/L	-13.15 dB
SWR	1.57 U
Impedance	78.2 Ω

The Following Graphs are the results as displayed on the Vector Network Analyzer.

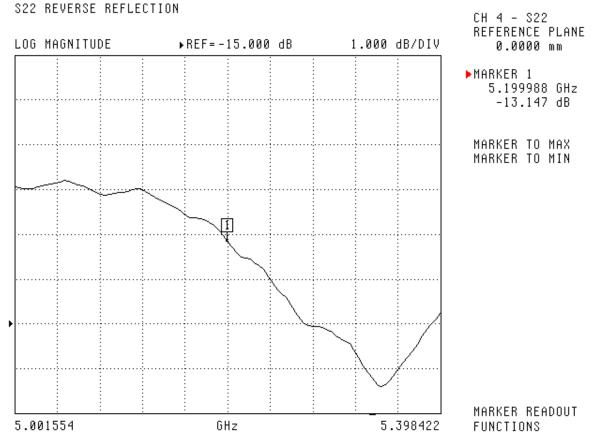

#### S11 Parameter Return Loss

#### **NCL Calibration Laboratories**


Division of APREL Laboratories.

S22 REVERSE REFLECTION




SWR

## **Smith Chart Dipole Impedance**

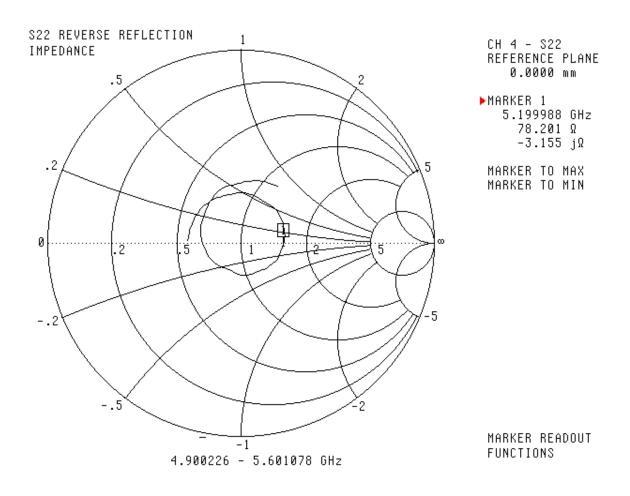

#### System Validation Results Using a Complex Dipole Model (FDTD calculations)

Frequency	1 Gram
5.2 GHz	58.8

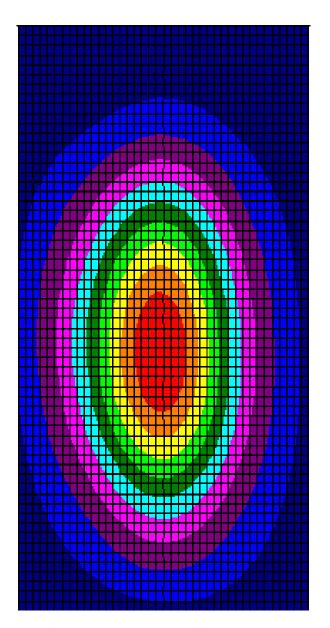

**Test Equipment** 

#### **NCL Calibration Laboratories**

Division of APREL Laboratories.

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration List May 2008.



## Appendix E. Dipole Calibration

Validation Dipole 5800 MHz M/N: ALS-D-5800-S-2 S/N: QTK-321

### NCL CALIBRATION LABORATORIES

Calibration File No: DC-893

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Quietek Validation Dipole

Manufacturer: APREL Laboratories Part number: ALS-D-5800-S-2 Frequency: 5.8 GHz Serial No: QTK-321

Customer: Quietek

Project Number: QTKB-Dipole-CAL-5336

Calibrated: 9<sup>th</sup> May 2008 Released on: 9<sup>th</sup> May 2008

This Calibration Certific Released By:	ate is Incomplete Unless	Accompanied with the Calibration Results Summary
-	51 SPECTRUM WAY NEPEAN, ONTARIO CANADA K2R 1E6	TION LABORATORIES Division of APREL Lab. TEL: (613) 820-4988 FAX: (613) 820-4161

## **Calibration Results Summary**

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

#### **Mechanical Dimensions**

Length:	21.6 mm
Height:	12.6 mm

#### **Electrical Specification**

SWR:	1.74 U
Return Loss:	-11.5 dB
Impedance:	68.3 Ω

#### **System Validation Results**

Frequency	1 Gram	
5800 GHz	57.9	
	Course Scan Data ( Axis (mm ) 0 10	) 20 
X	( Axis (mm	ר)

### Conditions

Dipole 321 is a recalibration.

Ambient Temperature of the Laboratory:	22 °C +/- 0.5°C
Temperature of the Tissue:	21 °C +/- 0.5°C

#### References

SSI-TP-018-ALSAS Dipole Calibration Procedure

SSI-TP-016 Tissue Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

IEC 62209 "Human exposure to radio frequency fields from hand-held and bodymounted wireless communication devices – Human models, instrumentation, and procedures –Part 1 & Part 2: Procedure to determine the specific absorption rate (SAR) for mobile wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

Stuart Nicol

C. Teodorian

# **NCL Calibration Laboratories** Division of APREL Laboratories.

## **Dipole Calibration Results**

#### **Mechanical Verification**

APREL	APREL	Measured	Measured
Length	Height	Length	Height
21.6 mm	12.6 mm	21.2 mm	13.1 mm

#### **Tissue Validation**


Head Tissue 5800 MHz	Measured
Dielectric constant, ε <sub>r</sub>	35.15
Conductivity, σ [S/m]	6.4

#### **Electrical Calibration**

Test	Result
S11 R/L	-11.5 dB
SWR	1.74 U
Impedance	68.3 Ω

The Following Graphs are the results as displayed on the Vector Network Analyzer.

#### S11 Parameter Return Loss

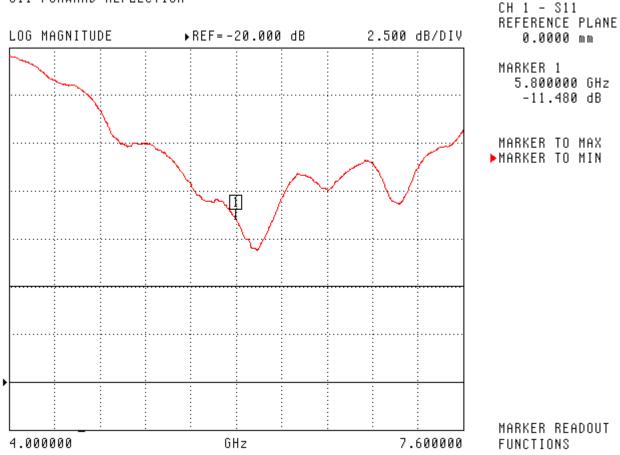

#### S11 FORWARD REFLECTION

#### **NCL Calibration Laboratories**


Division of APREL Laboratories.

#### SWR

## CH 1 - S11 REFERENCE PLANE SWR ▶REF=500.000 mU 1.000 U/DIV 0.0000 mm MARKER 1 5.800000 GHz 1.737 U MARKER TO MAX ▶MARKER TO MIN Í MARKER READOUT 4.000000 GHz 7.600000 FUNCTIONS


#### S11 FORWARD REFLECTION

### **Smith Chart Dipole Impedance**

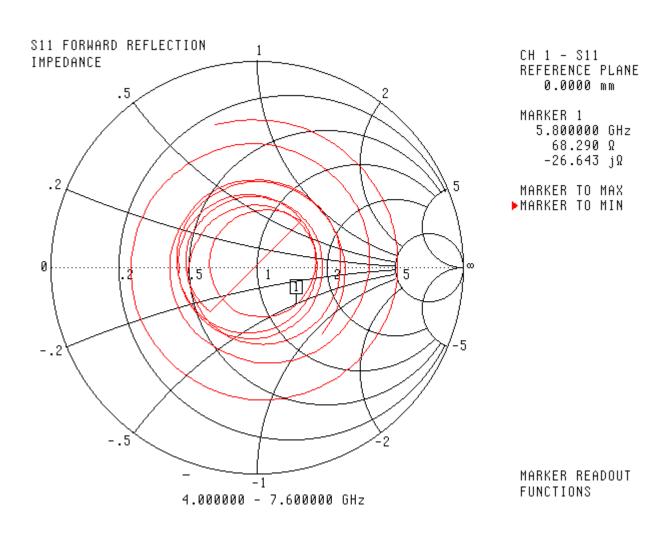

#### System Validation Results Using a Complex Dipole Model (FDTD calculations)

Frequency	1 Gram
5.8 GHz	57.9

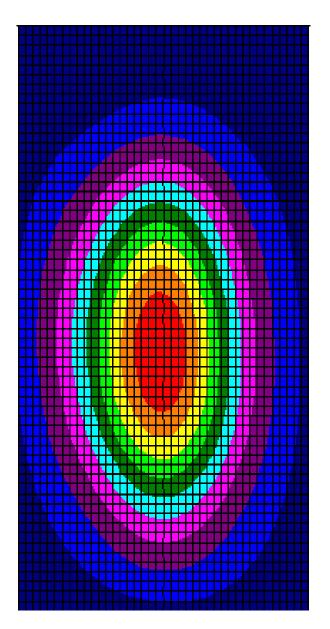

## **Test Equipment**

#### **NCL Calibration Laboratories**

Division of APREL Laboratories.

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration List May 2008.