





# Specific Absorption Rate (SAR) Test Report

for

# AboCom Systems, Inc

on the

# 802.11 b/g/n Mini Wireless LAN USB 2.0 Adapter

Report Number: FA860629-03

Trade Name : AboCom Model Name : WU5214

FCC ID : MQ4WU5214
Date of Testing : Nov. 06, 2008
Date of Report : Nov. 19, 2008
Date of Review : Nov. 19, 2008

- The test results refer exclusively to the tested model/sample only.
- Without written approval of SPORTON INTERNATIONAL INC., the test report shall not be reproduced except in full.
- Report Version: Rev. 02



# **Table of Contents**

		nent of Compliance	
2.	Admir	nistration Data	4
	2.1	Testing Laboratory	
	2.2	Detail of Applicant	
	2.3	Detail of Manufacturer	
	2.4	Application Details	
3.	Gener	al Information	
	3.1	Description of Device Under Test (DUT)	5
	3.2	Product Photos	
	3.3	Applied Standards	
	3.4	Device Category and SAR Limits	5
	3.5	Test Conditions	
		3.5.1 Ambient Condition	
		3.5.2 Test Configuration	
4.	Specif	ic Absorption Rate (SAR)	
	4.1	Introduction	
	4.2	SAR Definition	
5.		leasurement Setup	
	5.1	DASY4 E-Field Probe System	
		5.1.1 ET3DV6 E-Field Probe Specification	
		5.1.2 ET3DV6 E-Field Probe Calibration	
	5.2	DATA Acquisition Electronics (DAE)	
	5.3	Robot	
	5.4	Measurement Server	
	5.5	SAM Twin Phantom	
	5.6	Device Holder for SAM Twin Phantom	
	5.7	Data Storage and Evaluation	
		5.7.1 Data Storage	
		5.7.2 Data Evaluation	13
	5.8	Test Equipment List	
6.		Simulating Liquids	
7.	Uncer	tainty Assessment	18
8.		leasurement Evaluation	
	8.1	Purpose of System Performance Check	
	8.2	System Setup	
	8.3	Validation Results	
9.		iption for DUT Testing Position	
		irement Procedures	
	10.1	Spatial Peak SAR Evaluation	
	10.2	Scan Procedures	
	10.3	SAR Averaged Methods	
11.		est Results	26
	11.1	Conducted Power	
	11.2	SAR Test Record	
12.		ence	
۸nr	andiv	A System Berformance Check Date	

Appendix A - System Performance Check Data

Appendix B - SAR Measurement Data Appendix C - Calibration Data

Appendix D - Product Photos

Appendix E - Test Setup Photos



# 1. Statement of Compliance

The Specific Absorption Rate (SAR) maximum result found during testing for the AboCom Systems, Inc 802.11 b/g/n Mini Wireless LAN USB 2.0 Adapter AboCom WU5214 is 1.1 W/Kg on the 802.11b/g/n body SAR with expanded uncertainty 21.9%. It is in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1999 and had been tested in accordance with the measurement methods and procedures specified in OET Bulletin 65 Supplement C (Edition 01-01).

Approved by

Roy Wu Manager

# 2. Administration Data

## 2.1 Testing Laboratory

**Company Name:** Sporton International Inc.

Address: No.52, Hwa-Ya 1<sup>st</sup> RD., Hwa Ya Technology Park, Kwei-Shan Hsiang,

Test Report No : FA860629-03

TaoYuan Hsien, Taiwan, R.O.C.

**Test Site:** SAR01-HY

**Telephone Number:** 886-3-327-3456 **Fax Number:** 886-3-328-4978

## 2.2 Detail of Applicant

**Company Name:** AboCom Systems, Inc

**Address:** No.77, Yu-Yih Rd., Chu-Nan, Miao-Lih County 35059, Taiwan R.O.C.

# 2.3 <u>Detail of Manufacturer</u>

**Company Name:** AboCom Systems, Inc

**Address:** No.77, Yu-Yih Rd., Chu-Nan, Miao-Lih County 35059, Taiwan R.O.C.

## 2.4 Application Details

Date of reception of application:Sep. 24, 2008Start of test:Nov. 06, 2008End of test:Nov. 06, 2008



# 3. General Information

# 3.1 <u>Description of Device Under Test (DUT)</u>

Product Feature & Specification				
<b>DUT Type:</b> 802.11 b/g/n Mini Wireless LAN USB 2.0 Adapter				
Trade Name :	AboCom			
Model Name :	WU5214			
FCC ID:	MQ4WU5214			
Frequency Range:	2400 MHz ~ 2483.5 MHz			
Maximum Output Power to Antenna :	802.11b : 17.52 dBm 802.11g : 18.80 dBm 802.11n (BW 20MHz) : 18.75 dBm 802.11n (BW 40MHz) : 16.58 dBm			
Antenna Type :	Dipole Antenna			
Type of Modulation :	802.11b : DSSS 802.11g/n : OFDM			
DUT Stage :	Production Unit			

### 3.2 Product Photos

Refer to Appendix D.

### 3.3 Applied Standards

The Specific Absorption Rate (SAR) testing specification, method and procedure for this 802.11 b/g/n Mini Wireless LAN USB 2.0 Adapter is in accordance with the following standards:

47 CFR Part 2 (2.1093)

IEEE C95.1-1999

IEEE C95.3-2002

OET Bulletin 65 Supplement C (Edition 01-01)

KDB 248227 r1.2 SAR Measurement Procedures for 802.11abg Transmitters

KDB 447498 D01 v03r02 Mobile and Portable Device RF Exposure Procedures

### 3.4 Device Category and SAR Limits

This device belongs to portable device category because its radiating structure is allowed to be used within 20 centimeters of the body of the user. Limit for General Population/Uncontrolled exposure should be applied for this device, it is 1.6 W/kg as averaged over any 1 gram of tissue.



### 3.5 Test Conditions

# 3.5.1 Ambient Condition

Ambient Temperature	20-24
Humidity	<60 %

### 3.5.2 Test Configuration

For WLAN link mode, engineering testing software installed on the EUT can provide continuous transmitting RF signal. This RF signal utilized in SAR measurement has almost 100% duty cycle and its crest factor is 1. Measurements were performed on the lowest, middle, and highest channel for each testing position. However, measurements were performed only on the middle channel if the SAR is below 3 dB of limit for body SAR testing.

The data rates for WLAN SAR testing were set in 1Mbps for 802.11b, 6Mbps for 802.11g and 13Mbps for 802.11n due to the highest RF output power.



# 4. Specific Absorption Rate (SAR)

### 4.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The FCC recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

### 4.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density.

). The equation description is as below:

$$\mathbf{SAR} = \frac{d}{dt} \left( \frac{dW}{dm} \right) = \frac{d}{dt} \left( \frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$\mathbf{SAR} = C \frac{\delta T}{\delta t}$$

, where C is the specific head capacity,  $\delta T$  is the temperature rise and  $\delta t$  the exposure duration,

or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\sigma |E|^2}{\rho}$$

, where  $\,$  is the conductivity of the tissue,  $\,$  is the mass density of the tissue and E is the rms electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.



# 5. SAR Measurement Setup

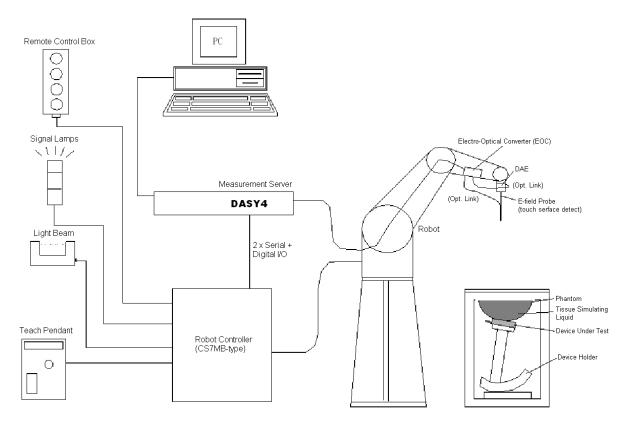


Fig. 5.1 DASY4 System

The DASY4 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- A dosimetric probe equipped with an optical surface detector system
- The electro-optical converter (ECO) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the accuracy of the probe positioning
- ➤ A computer operating Windows XP
- DASY4 software
- Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- > The SAM twin phantom
- > A device holder
- > Tissue simulating liquid
- > Dipole for evaluating the proper functioning of the system

Some of the components are described in details in the following sub-sections.




### 5.1 DASY4 E-Field Probe System

The SAR measurement is conducted with the dosimetric probe ET3DV6 (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency. This probe has a built in optical surface detection system to prevent from collision with phantom.

# 5.1.1 ET3DV6 E-Field Probe Specification

<ET3DV6>

\E13DV0>		-
Construction	Symmetrical design with triangular core	
	Built-in optical fiber for surface detection	
	system	
	Built-in shielding against static charges	-
	PEEK enclosure material (resistant to organic	
	solvents)	
Frequency	10 MHz to 3 GHz	
Directivity	$\pm$ 0.2 dB in brain tissue (rotation around probe	Place /
	axis)	No.
	$\pm$ 0.4 dB in brain tissue (rotation perpendicular	
	to probe axis)	
Dynamic Range	5 μ W/g to 100mW/g; Linearity: ±0.2dB	2
<b>Surface Detection</b>	$\pm$ 0.2 mm repeatability in air and clear liquids on	
	reflecting surface	
Dimensions	Overall length: 330mm	Fig. 5.2 I
	Tip length: 16mm	Fig. 5.2 I
	Body diameter: 12mm	
l	Tip diameter: 6.8mm	
	Distance from probe tip to dipole centers:	
	2.7mm	
Application	General dosimetry up to 3GHz	
	Compliance tests for mobile phones and	
	Wireless LAN	
	Fast automatic scanning in arbitrary phantoms	



**Probe Setup on Robot** 

### 5.1.2 ET3DV6 E-Field Probe Calibration

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than  $\pm$  10%. The spherical isotropy shall be evaluated and within  $\pm$  0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data are as below:

# > ET3DV6 sn1787

/ E13D v O SH17O7						
Sensitivity	X axis : 1.63 μV		Y axis : 1.67 μV		Z axis : 2.18 μV	
Diode compression point	X axis : 90 mV		Y axis : 93 mV		Z axis: 92 mV	
Conversion factor	Frequency (MHz)	X a	xis	Y axis	Z axis	
(Head / Body)	2350~2550	4.49 /	3.79	4.49 / 3.79	4.49 / 3.79	
Boundary effect (Head / Body)	Frequency (MHz)	Alp	ha	Depth		
(Head / Body)	2350~2550	0.77 /	0.90	1.57 / 1.51		

NOTE: The probe parameters have been calibrated by the SPEAG.



# 5.2 <u>DATA Acquisition Electronics (DAE)</u>

The data acquisition electronics (DAE4) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.

### 5.3 Robot

The DASY4 system uses the high precision robots RX90BL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY4 system, the CS7MB robot controller version from Stäubli is used. The RX robot series have many features that are important for our application:

- ➤ High precision (repeatability 0.02 mm)
- ➤ High reliability (industrial design)
- > Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- ► 6-axis controller

### 5.4 Measurement Server

The DASY4 measurement server is based on a PC/104 CPU board with 166 MHz CPU 32 MB chipset and 64 MB RAM.

Communication with the DAE4 electronic box

the 16-bit AD-converter system for optical detection and digital I/O interface.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.



### 5.5 SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- ➤ Left head
- > Right head
- Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

The phantom can be used with the following tissue simulating liquids:

- \*Water-sugar based liquid
- \*Glycol based liquids

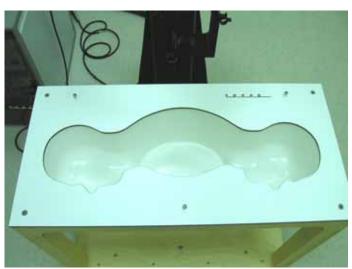


Fig. 5.3 Top View of Twin Phantom



Fig. 5.4 Bottom View of Twin Phantom



### 5.6 Device Holder for SAM Twin Phantom

The SAR in the Phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source in 5 mm distance, a positioning uncertainty of  $\pm 0.5$ mm would produce a SAR uncertainty of  $\pm 20\%$ . An accurate device position is therefore crucial for accurate and repeatable measurement. The position in which the devices must be measured, are defined by the standards.

The DASY4 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation center for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The DASY4 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity  $_{\rm r}$  =3 and loss tangent  $\delta$  = 0.02. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



Fig. 5.5 Device Holder



### 5.7 <u>Data Storage and Evaluation</u>

### 5.7.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The post-processing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [A/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a non-louse media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

### 5.7.2 Data Evaluation

The DASY4 post-processing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

**Probe parameters**: - Sensitivity Norm<sub>i</sub>,  $a_{i0}$ ,  $a_{i1}$ ,  $a_{i2}$ 

Conversion factor ConvF<sub>i</sub>
 Diode compression point dcp<sub>i</sub>
 Frequency f

**Device parameters**: - Frequency f
- Crest factor cf

**Media parameters:** - Conductivity

- Density

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY4 components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power.



The formula for each channel can be given as:

$$Vi = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with

 $V_i$  = compensated signal of channel i (i = x, y, z)

 $U_i$  = input signal of channel i (i = x, y, z)

cf = crest factor of exciting field (DASY parameter)

 $dcp_i = diode\ compression\ point\ (DASY\ parameter)$ 

From the compensated input signals, the primary field data for each channel can be evaluated:

E-field probes :  $E_i = \sqrt{\frac{V_i}{Norm_i ConvF}}$ 

H-field probes:  $H_i = \sqrt{V_i} \frac{a_{i0+} a_{i1} f + a_{i2} f^2}{f}$ 

with

 $V_i$  = compensated signal of channel i (i = x, y, z)

 $Norm_i$  = sensor sensitivity of channel i (i = x, y, z)

 $\mu V/(V/m)$ 2 for E-field Probes

ConvF = sensitivity enhancement in solution

 $a_{ii}$  = sensor sensitivity factors for H-field probes

f = carrier frequency [GHz]

 $E_i$  = electric field strength of channel *i* in V/m

 $H_i$  = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with

SAR = local specific absorption rate in mW/g

Etot = total field strength in V/m

= conductivity in [mho/m] or [Siemens/m]

= equivalent tissue density in g/cm<sup>3</sup>

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770} \qquad \text{or} \quad P_{pwe} = H_{tot}^2 \cdot 37.7$$

with

 $P_{pwe}$  = equivalent power density of a plane wave in mW/cm<sup>2</sup>

 $E_{tot}$  = total electric field strength in V/m

 $H_{tot}$  = total magnetic field strength in A/m

<sup>\*</sup> Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.



5.8 Test Equipment List

Manufacturer	Nome of Equipment	Tyme/Model	Serial Number	Calib	Calibration	
Manufacturer	Name of Equipment	Type/Model	Seriai Number	Last Cal.	<b>Due Date</b>	
SPEAG	Dosimetric E-Filed Probe	ET3DV6	1787	Aug. 26, 2008	Aug. 25, 2009	
SPEAG	2450MHz System Validation Kit	D2450V2	736	Jul. 12, 2007	Jul. 11, 2009	
SPEAG	Data Acquisition Electronics	DAE4	679	May 21, 2008	May 20, 2009	
SPEAG	Device Holder	N/A	N/A	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1303	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1446	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1383	NCR	NCR	
SPEAG	ELI4 Phantom	QD 0VA 001 BA	1029	NCR	NCR	
Agilent	PNA Series Network Analyzer	E8358A	US40260131	Apr. 02, 2008	Apr. 01, 2009	
Agilent	Dielectric Probe Kit	85070D	US01440205	NCR	NCR	
Agilent	Dual Directional Coupler	778D	50422	NCR	NCR	
AR	Power Amplifier	5S1G4M2	0328767	NCR	NCR	
R&S	Power Meter	NRVD	101394	Oct. 20, 2008	Oct. 19, 2009	
R&S	Power Sensor	NRV-Z1	100130	Oct. 20, 2008	Oct. 19, 2009	

**Table 5.1 Test Equipment List** 



# 6. Tissue Simulating Liquids

For the measurement of the field distribution inside the SAM phantom with DASY4, the phantom must be filled with around 25 liters of homogeneous body tissue simulating liquid. The liquid height from the bottom of the phantom body is 15.2 centimeters, which is shown in Fig. 6.1.

The following ingredients for tissue simulating liquid are used:

- **Water**: deionized water (pure  $H_20$ ), resistivity ≥16MΩ- as basis for the liquid
- Sugar: refined sugar in crystals, as available in food shops to reduce relative permittyvity
- ➤ Salt: pure NaCl to increase conductivity
- ➤ Cellulose: Hydroxyethyl-cellulose, medium viscosity (75-125 mPa.s, 2% in water, 20°C), CAS#54290-to increase viscosity and to keep sugar in solution.
- ➤ **Preservative**: Preventol D-7 Bayer AG, D-51368 Leverkusen, CAS#55965-84-9- to prevent the spread of bacteria and molds.
- ➤ **DGMBE**: Deithlenglycol-monobuthyl ether (DGMBE), Fluka Chemie GmbH, CAS#112-34-5 to reduce relative permittivity.

Table 6.1 gives the recipes for one liter of tissue simulating liquid for frequency band 2450 MHz.

Ingredient	MSL-2450
Water	698.3 ml
DGMBE	301.7 ml
Total amount	1 liter (1.0 kg)
Dielectric Parameters at 22°	f = 2450MHz
	$r = 52.7 \pm 5\%, = 1.95 \pm 5\% \text{ S/m}$

Table 6.1 Recipes of tissue Simulating Liquid

The dielectric parameters of the liquids were verified prior to the SAR evaluation using an Agilent 85070D Dielectric Probe Kit and an Agilent Network Analyzer.



Table 6.2 shows the measuring results for muscle simulating liquid.

Band	Temperature ( )	Frequency (MHz)	Permittivity (ε <sub>r</sub> )	Conductivity (σ)	Measurement date
		2412	1.95	51.3	
802.11b/g/n	21.4	2437	1.97	51.2	Nov. 06, 2008
		2462	2.00	51.1	

Table 6.2 Measuring Results for Muscle Simulating Liquid

The measuring data are consistent with  $_{r} = 52.7 \pm 5\%$  and  $= 1.95 \pm 5\%$ .

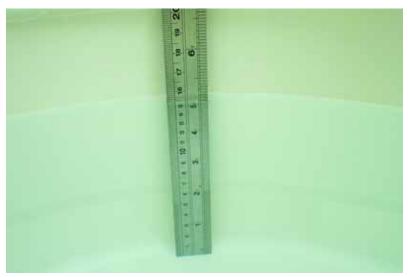


Fig 6.1 Liquid Height from the Bottom of the Phantom Body is 15.2 Centimeters



# 7. Uncertainty Assessment

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table 7.1

Uncertainty Distributions	Normal	Rectangular	Triangular	U-shape
Multiplying factor <sup>(a)</sup>	1/k (b)	1/ 3	1/ 6	1/ 2

<sup>(</sup>a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity

(b) is the coverage factor

Table 7.1 Standard Uncertainty for Assumed Distribution

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY4 uncertainty Budget is showed in Table 7.2.



Error Description	Uncertainty Value ± %	Probability Distribution	Divisor	Ci (1g)	Standard Unc. (1g)	vi or Veff
Measurement Equipment				_		
Probe Calibration	±5.9 %	Normal	1	1	±5.9 %	$\infty$
Axial Isotropy	±4.7 %	Rectangular	$\sqrt{3}$	0.7	±1.9 %	$\infty$
Hemispherical Isotropy	±9.6 %	Rectangular	$\sqrt{3}$	0.7	±3.9 %	$\infty$
Boundary Effects	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	$\infty$
Linearity	±4.7 %	Rectangular	$\sqrt{3}$	1	±2.7 %	$\infty$
System Detection Limits	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	$\infty$
Readout Electronics	±0.3 %	Normal	1	1	±0.3 %	$\infty$
Response Time	±0.8 %	Rectangular	$\sqrt{3}$	1	±0.5 %	$\infty$
Integration Time	±2.6 %	Rectangular	$\sqrt{3}$	1	±1.5 %	$\infty$
RF Ambient Noise	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	$\infty$
RF Ambient Reflections	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	$\infty$
Probe Positioner	±0.4 %	Rectangular	$\sqrt{3}$	1	±0.2 %	$\infty$
Probe Positioning	±2.9 %	Rectangular	$\sqrt{3}$	1	±1.7 %	$\infty$
Max. SAR Eval.	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	$\infty$
Test Sample Related						
Device Positioning	±2.9 %	Normal	1	1	±2.9	145
Device Holder	±3.6 %	Normal	1	1	±3.6	5
Power Drift	±5.0 %	Rectangular	$\sqrt{3}$	1	±2.9	$\infty$
Phantom and Setup						_
Phantom Uncertainty	±4.0 %	Rectangular	$\sqrt{3}$	1	±2.3	$\infty$
Liquid Conductivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.64	±1.8	$\infty$
Liquid Conductivity (meas.)	±2.5 %	Normal	1	0.64	±1.6	$\infty$
Liquid Permittivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.6	±1.7	$\infty$
Liquid Permittivity (meas.)	±2.5 %	Normal	1	0.6	±1.5	$\infty$
Combined Standard Uncertainty					±10.9	387
Coverage Factor for 95 %		K=2				
Expanded uncertainty (Coverage factor = 2)					±21.9	

**Table 7.2 Uncertainty Budget of DASY4** 



## 8. SAR Measurement Evaluation

Each DASY4 system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY4 software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

### 8.1 Purpose of System Performance Check

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

### 8.2 System Setup

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave which comes from a signal generator at frequency 2450 MHz. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

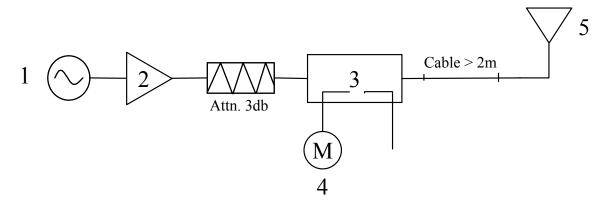


Fig. 8.1 System Setup for System Evaluation



- 1. Signal Generator
- 2. Amplifier
- 3. Directional Coupler
- 4. Power Meter
- 5. 2450 MHz Dipole

The output power on dipole port must be calibrated to 100 mW (20 dBm) before dipole is connected.



Fig 8.2 Dipole Setup



# 8.3 Validation Results

Comparing to the original SAR value provided by SPEAG, the validation data should within its specification of 10 %. Table 8.1 shows the target SAR and measured SAR after normalized to 1W input power.

Frequency	SAR	Target (W/kg)	Measurement data (W/kg)	Variation	Measurement date
2450 MHz	SAR (1g)	52.5	55.1	5.0 %	Nov. 06, 2009
	SAR (10g)	24.4	25.4	4.1 %	Nov. 06, 2008


Table 8.1 Target and Measured SAR after Normalized

The table above indicates the system performance check can meet the variation criterion.



# 9. <u>Description for DUT Testing Position</u>

This DUT was tested in four different USB configurations. They are "direct laptop plug-in for configuration 1" and "USB cable plug-in for configuration 2 to 4" shown as below. Both direct laptop plug-in and cable plug-in test configurations are tested with 5 mm separation between the particular dongle orientation and the flat phantom.

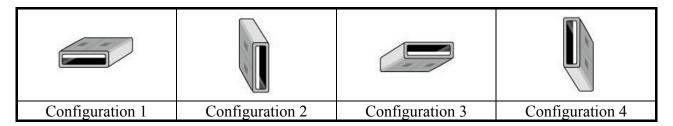

Remark: Please refer to Appendix E for the test setup photos.



# 10.Measurement Procedures

The measurement procedures are as follows:

- Using engineering software to transmit RF power continuously (continuous Tx)
- Placing the DUT in the positions described in the last section
- Setting scan area, grid size and other setting on the DASY4 software
- Taking data for the middle channel
- Repeat the previous steps for the low and high channels.

According to the OET Bulletin 65 Supplement C standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- Power reference measurement
- Area scan
- Zoom scan
- Power reference measurement

### 10.1 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the OET Bulletin 65 Supplement C standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY4 software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.

The entire evaluation of the spatial peak values is performed within the post-processing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- extraction of the measured data (grid and values) from the Zoom Scan
- calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- generation of a high-resolution mesh within the measured volume
- interpolation of all measured values form the measurement grid to the high-resolution grid
- extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- calculation of the averaged SAR within masses of 1g and 10g



### 10.2 Scan Procedures

First Area Scan is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an Area Scan is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, Zoom Scan is required. The Zoom Scan measures 5x5x7 points with step size 8, 8 and 5 mm. The Zoom Scan is performed around the highest E-field value to determine the averaged SAR-distribution over 1 g.

### 10.3 SAR Averaged Methods

In DASY4, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.



# 11. SAR Test Results

# 11.1 Conducted Power

Band Channel Date B	802.11b (dBm)	802.11g (dBm)	802.11n (BW 20M) (dBm)	-
Data Rate	1 Mbps	6 Mbps	13 Mbps	-
1	17.07	16.94	17.34	-
6	17.52	18.80	18.75	=
11	16.41	15.04	17.19	-

Band Channel Date B	802.11n (BW 40M) (dBm)	-	-	-
Data Rate	13 Mbps	-	-	-
3	16.05	-	-	-
6	16.58	-	-	-
9	15.81	-	-	=

# 11.2 SAR Test Record

USB Configuration	Antenna Status	Mode	Chan.	Frequency (MHz)	Modulation Type	Measured 1g SAR (W/kg)	Limit (W/kg)	Result
1	Straight	802.11b	6	2437	DSSS	0.839	1.6	Pass
1	Perpendicular	802.11b	6	2437	DSSS	0.046	1.6	Pass
2	Straight	802.11b	6	2437	DSSS	0.354	1.6	Pass
3	Straight	802.11b	6	2437	DSSS	0.739	1.6	Pass
4	Straight	802.11b	6	2437	DSSS	0.322	1.6	Pass
1	Straight	802.11b	1	2412	DSSS	1.1	1.6	Pass
1	Straight	802.11b	11	2462	DSSS	0.780	1.6	Pass
1	Straight	802.11g	6	2437	OFDM	0.654	1.6	Pass
1	Straight	802.11n (20M)	6	2437	OFDM	0.771	1.6	Pass
1	Straight	802.11n (40M)	6	2437	OFDM	0.793	1.6	Pass

Test Engineer: Jason Wang and Robert Liu



# 12.Reference

- [1] FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2] IEEE Std. P1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", April 21, 2003.
- [3] Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 97-01), "Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to RF Emissions", June 2001
- [4] IEEE Std. C95.3-2002, "IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields-RF and Microwave", 2002
- [5] IEEE Std. C95.1-1999, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", 1999
- [6] Robert J. Renka, "Multivariate Interpolation Of Large Sets Of Scattered Data", University of North Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988, pp. 139-148
- [7] DASY4 System Handbook
- [8] KDB 248227 r1.2 SAR Measurement Procedures for 802.11abg Transmitters
- [9] KDB 447498 D01 v03r02 Mobile and Portable Device RF Exposure Procedures



# Appendix A - System Performance Check Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab Date: 2008/11/6

### System Check\_Body\_2450MHz\_081106

### **DUT: Dipole 2450 MHz**

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL 2450 Medium parameters used: f = 2450 MHz;  $\sigma = 1.99 \text{ mho/m}$ ;  $\varepsilon_r = 51.1$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Ambient Temperature: 22.0 °C; Liquid Temperature: 22.0 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(3.79, 3.79, 3.79); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn679; Calibrated: 2008/5/21
- Phantom: ELI 4.0 Front; Type: QDOVA001BB; Serial: 1026
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

# Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm


Maximum value of SAR (interpolated) = 6.30 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 56.9 V/m; Power Drift = 0.022 dB

Peak SAR (extrapolated) = 12.8 W/kg

SAR(1 g) = 5.51 mW/g; SAR(10 g) = 2.54 mW/g Maximum value of SAR (measured) = 6.12 mW/g

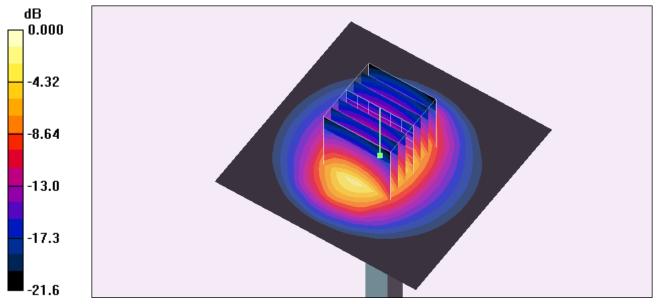

0 dB = 6.12 mW/g



# Appendix B - SAR Measurement Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab Date: 2008/11/6

### Body\_802.11b Ch1\_USB Configuration 1\_Ant set Straight

DUT: 860829-03

Communication System: 802.11b; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: MSL 2450 Medium parameters used: f = 2412 MHz;  $\sigma = 1.95$  mho/m;  $\epsilon_r = 51.3$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.7 °C; Liquid Temperature: 21.4 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(3.79, 3.79, 3.79); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn679; Calibrated: 2008/5/21
- Phantom: ELI 4.0 Front; Type: QDOVA001BB; Serial: 1026
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

# Ch1/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 1.38 mW/g

### Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.85 V/m; Power Drift = 0.006 dB

Peak SAR (extrapolated) = 2.71 W/kg

### SAR(1 g) = 1.1 mW/g; SAR(10 g) = 0.494 mW/g Maximum value of SAR (measured) = 1.22 mW/g

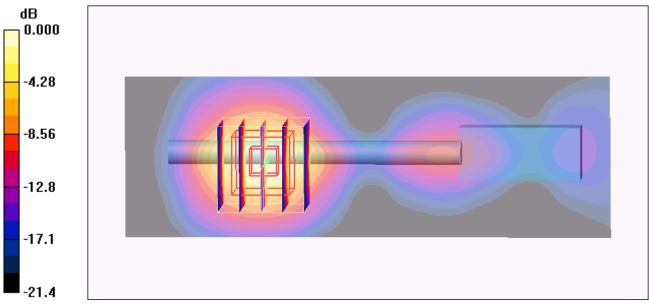

0 dB = 1.22 mW/g



### Body\_802.11b Ch6\_USB Configuration 1\_Ant set Perpendicular

### **DUT: 860829-03**

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL 2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.97$  mho/m;  $\varepsilon_r = 51.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.7 °C; Liquid Temperature: 21.4 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(3.79, 3.79, 3.79); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn679; Calibrated: 2008/5/21
- Phantom: ELI 4.0 Front; Type: QDOVA001BB; Serial: 1026
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch6/Area Scan (41x71x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.053 mW/g


Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.42 V/m; Power Drift = -0.199 dB

Peak SAR (extrapolated) = 0.093 W/kg

SAR(1 g) = 0.046 mW/g; SAR(10 g) = 0.024 mW/g

Maximum value of SAR (measured) = 0.052 mW/g

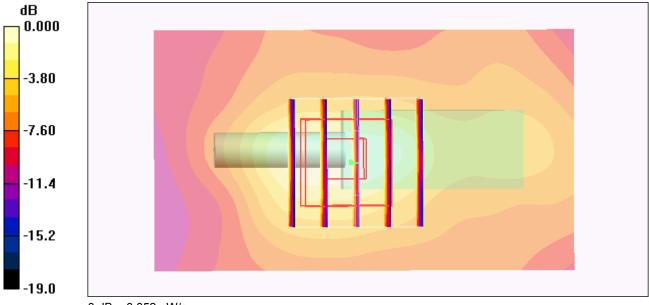

0 dB = 0.052 mW/g



### Body 802.11b Ch6 USB Configuration 2 Ant set Straight

### **DUT: 860629-03**

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL 2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.97$  mho/m;  $\varepsilon_r = 51.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.7 °C; Liquid Temperature: 21.4 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(3.79, 3.79, 3.79); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn679; Calibrated: 2008/5/21
- Phantom: ELI 4.0 Front; Type: QDOVA001BB; Serial: 1026
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

# Ch6/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.411 mW/g


### Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 2.84 V/m; Power Drift = 0.175 dB

Peak SAR (extrapolated) = 0.762 W/kg

## SAR(1 g) = 0.354 mW/g; SAR(10 g) = 0.179 mW/g

Maximum value of SAR (measured) = 0.382 mW/g

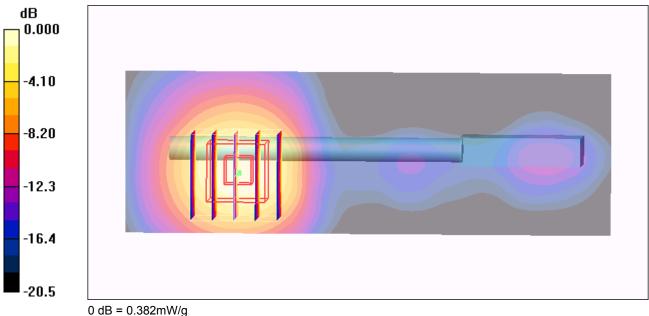



### Body\_802.11b Ch6\_USB Configuration 3\_Ant set Straight

### **DUT: 860629-03**

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL 2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.97$  mho/m;  $\varepsilon_r = 51.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.7 °C; Liquid Temperature: 21.4 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(3.79, 3.79, 3.79); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn679; Calibrated: 2008/5/21
- Phantom: ELI 4.0 Front; Type: QDOVA001BB; Serial: 1026
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch6/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.944 mW/g


Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 2.14 V/m; Power Drift = 0.124 dB

Peak SAR (extrapolated) = 1.76 W/kg

SAR(1 g) = 0.739 mW/g; SAR(10 g) = 0.342 mW/g

Maximum value of SAR (measured) = 0.810 mW/g

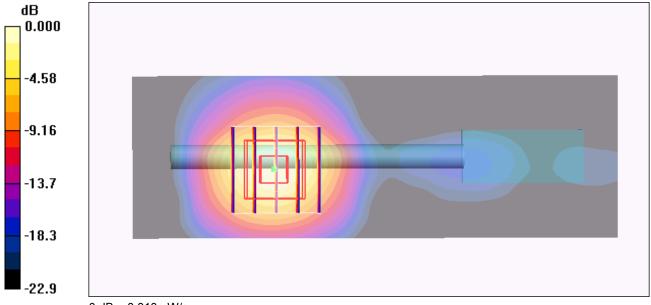

0 dB = 0.810 mW/g



### Body\_802.11b Ch6\_USB Configuration 4\_Ant set Straight

### **DUT: 860629-03**

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL 2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.97$  mho/m;  $\varepsilon_r = 51.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.7 °C; Liquid Temperature: 21.4 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(3.79, 3.79, 3.79); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn679; Calibrated: 2008/5/21
- Phantom: ELI 4.0 Front; Type: QDOVA001BB; Serial: 1026
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

Ch6/Area Scan (41x121x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.361 mW/g


Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.05 V/m; Power Drift = 0.138 dB

Peak SAR (extrapolated) = 0.720 W/kg

SAR(1 g) = 0.322 mW/g; SAR(10 g) = 0.161 mW/g

Maximum value of SAR (measured) = 0.349 mW/g

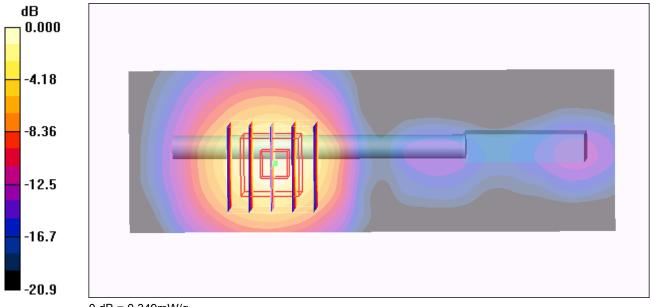

0 dB = 0.349 mW/g



### Body\_802.11b Ch1\_USB Configuration 1\_Ant set Straight\_2D

**DUT: 860829-03** 

Communication System: 802.11b; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma$  = 1.95 mho/m;  $\epsilon_r$  = 51.3;  $\rho$  = 1000 kg/m<sup>3</sup>

Ambient Temperature: 22.7 °C; Liquid Temperature: 21.4 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(3.79, 3.79, 3.79); Calibrated: 2008/8/26
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn679; Calibrated: 2008/5/21
- Phantom: ELI 4.0 Front; Type: QDOVA001BB; Serial: 1026
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184


**Ch1/Area Scan (41x121x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.38 mW/g

Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.85 V/m; Power Drift = 0.006 dB

Peak SAR (extrapolated) = 2.71 W/kg

SAR(1 g) = 1.1 mW/g; SAR(10 g) = 0.494 mW/g Maximum value of SAR (measured) = 1.22 mW/g

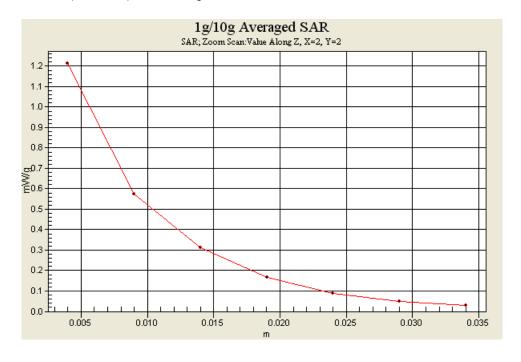

# Appendix C - Calibration Data

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Galibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton (Auden)

Accreditation No.: SCS 108

Certificate No: D2450V2-736\_Jul07

bject	D2450V2 - SN: 7	36	THE SECTION SECTION
calibration procedure(s)	QA CAL-05.v6 Calibration proce	dure for dipole validation kits	
Calibration date:	July 12, 2007		
Condition of the calibrated item	In Tolerance		o que a de la constante de la
alibration Equipment used (M&	TE critical for calibration)	y facility: environment temperature (22 ± 3)°C and	
albration Equipment used (M&	TE critical for calibration)	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
alibration Equipment used (M& nimary Standards ower mater EPM-442A	TE critical for calibration)  ID #  GB37480704	Cal Date (Calibrated by, Cartificate No.) C3-Oct-06 (METAS, No. 217-00608)	Scheduled Calibration Oct-07
alibration Equipment used (M& imary Standards ower mater EPM-442A ower sensor HP 8431A	TE critical for calibration)  ID #  GB37480704  US37292783	Cal Date (Calibrated by, Cartificate No.) C3-Oct-06 (METAS, No. 217-00608) C3-Oct-06 (METAS, No. 217-00608)	Scheduled Calibration Oct-07 Oct-07
alibration Equipment used (M& timary Standards ower mater EPM-442A ower sensor HP 8431A eference 20 dB Attenuator	TE critical for calibration)  ID #  GB37480704  US37292783  SN: 5066 (20g)	Cal Date (Calibrated by, Cartificate No.)  G3-Oct-06 (METAS, No. 217-00608)  G3-Oct-06 (METAS, No. 217-00608)  10-Aug-06 (METAS, No. 217-00691)	Scheduled Calibration Oct-07 Oct-07 Aug-07
minary Standards ower meter EPM-442A ower sensor HP 8431A deference 20 d5 Attenuator deference 10 d8 Attenuator	TE critical for calibration)  ID #  GB37480704  US37292783  SN: 5066 (20g)  SN: 5047.2 (10r)	Cal Date (Calibrated by, Cartificate No.) G3-Oct-06 (METAS, No. 217-00608) G3-Oct-06 (METAS, No. 217-00608) 10-Aug-06 (METAS, No. 217-00691) 10-Aug-06 (METAS, No. 217-00591)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07
calibration Equipment used (M& minary Standards. Power mater EPM-442A Power sensor HP 8481A telerence 20 dB Attenuator telerence 10 dB Attenuator telerence Probe ES3DV3	TE critical for calibration)  ID #  GB37480704  US37292783  SN: 5066 (20g)	Csl Date (Calibrated by, Certificate No.) C3-Oct-06 (METAS, No. 217-00608) C3-Oct-06 (METAS, No. 217-00608) 10-Aug-08 (METAS, No. 217-00591) 10-Aug-08 (METAS, No. 217-00591) 19-Oct-06 (SPEAG, No. ES3-3025_Oct06)	Scheduled Calibration Oct-07 Oct-07 Aug-07
minary Standards.  minary Standards.  minary Standards.  mover mater EPM-442A  over sensor HP 8481A  deference 20 dB Attenuator deference 10 dB Attenuator deference Probe ES3DV3  AE4	TE critical for calibration)  ID #  GB37480704  US37292783  SN: 5066 (20g)  SN: 5047.2 (10r)  SN 3025  SN 601	Cal Date (Calibrated by, Certificate No.) 63-Oct-06 (METAS, No. 217-00608) 63-Oct-06 (METAS, No. 217-0008) 10-Aug-08 (METAS, No. 217-00591) 10-Aug-08 (METAS, No. 217-00591) 19-Oct-08 (SPEAG, No. ES3-3025_Oct06) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07 Jan-08
Calibration Equipment used (M& minary Standards brower meter EPW-442A brower sensor HP 8431A telerence 20 dB Attenuator telerence 10 dB Attenuator telerence Probe ES3DV3 JAE4	TE critical for calibration)  ID #  GB37480704  US37292783  SN: 5066 (20g)  SN: 5047.2 (10r)  SN 3025  SN 601	Cal Date (Calibrated by, Certificate No.)  G3-Oct-06 (METAS, No. 217-00608)  G3-Oct-06 (METAS, No. 217-00608)  10-Aug-08 (METAS, No. 217-00591)  10-Aug-08 (METAS, No. 217-00591)  10-Oct-08 (SPEAG, No. ES3-3025_Oct06)  S0-Jan-07 (SPEAG, No. DAE4-601_Jan07)  Check Date (in house)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07 Jan-08 Scheduled Chack
Calibration Equipment used (M& mimary Standards hower mater EPM-442A hower sensor HP 8481A telerence 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV3 JAE4 Secondary Standards hower sensor HP 8481A	TE critical for calibration)  ID #  GB37480704  US37292783  SN: 5066 (20g)  SN: 5047.2 (10r)  SN 3025  SN 601  ID #  MY41092317	Cal Date (Calibrated by, Certificate No.)  G3-Oct-06 (METAS, No. 217-00608)  G3-Oct-06 (METAS, No. 217-00608)  10-Aug-08 (METAS, No. 217-00591)  10-Aug-08 (METAS, No. 217-00591)  19-Oct-08 (SPEAG, No. E53-3025_Oct06)  30-Jan-07 (SPEAG, No. DAE4-601_Jan07)  Check Date (in house)  18-Oct-02 (SPEAG, in house check Oct-05)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07 Jan-08 Scheduled Chack In house check: Oct-07
minary Standards  ower sensor HP 8431A telerence 20 d5 Attenuator telerence Probe ES3DV3 AE4 econdary Standards ower sensor HP 8481A	TE critical for calibration)  ID #  G637480704  US37292783  SN: 5066 (200)  SN: 5047.2 (10r)  SN 3025  SN 601  ID #  MY41092317  MY41090675	Cal Date (Calibrated by, Certificate No.)  G3-Oct-06 (METAS, No. 217-00608)  G3-Oct-06 (METAS, No. 217-00608)  10-Aug-06 (METAS, No. 217-00691)  10-Aug-06 (METAS, No. 217-00691)  10-Oct-06 (SPEAG, No. ES3-3025_Oct06)  30-Jan-07 (SPEAG, No. DAE4-601_Jan07)  Check Date (in house)  18-Oct-02 (SPEAG, in house check Oct-05)  11-May-05 (SPEAG, in house check Nov-05)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07 Jan-08 Scheduled Chack In house check: Nov-07 In house check: Nov-07
minary Standards  rower mater EPW-442A  rower sensor HP 8431A  telerence 20 dB Attenuator  telerence 10 dB Attenuator  telerence Probe ES3DV3  AE4  secondary Standards	TE critical for calibration)  ID #  GB37480704  US37292783  SN: 5066 (20g)  SN: 5047.2 (10r)  SN 3025  SN 601  ID #  MY41092317	Cal Date (Calibrated by, Certificate No.)  G3-Oct-06 (METAS, No. 217-00608)  G3-Oct-06 (METAS, No. 217-00608)  10-Aug-08 (METAS, No. 217-00591)  10-Aug-08 (METAS, No. 217-00591)  19-Oct-08 (SPEAG, No. E53-3025_Oct06)  30-Jan-07 (SPEAG, No. DAE4-601_Jan07)  Check Date (in house)  18-Oct-02 (SPEAG, in house check Oct-05)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07 Jan-08 Scheduled Chack In house check: Oct-07
minary Standards  ower sensor HP 8431A telerence 20 d5 Attenuator telerence Probe ES3DV3 AE4 econdary Standards ower sensor HP 8481A	TE critical for calibration)  ID #  GB37480704  U337292783  SN: 5067 (20g)  SN: 5047.2 (10r)  SN 3025  SN 601  ID #  MY41092317  MY41090575  US37390585 S4206	Cal Date (Calibrated by, Certificate No.) C3-Oct-06 (METAS, No. 2:7-00608) C3-Oct-06 (METAS, No. 2:7-00608) 10-Aug-06 (METAS, No. 2:7-00591) 10-Aug-06 (METAS, No. 2:7-00591) 19-Oct-06 (SPEAG, No. ES3-3025_Oct06) S0-Jan-07 (SPEAG, No. DAE4-001_Jan07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Nov-05) 11-May-05 (SPEAG, in house check Nov-05)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Oct-07 Jan-08 Scheduled Chack In house check: Oct-07 In house check: Oct-07
alibration Equipment used (M& nimary Standards ower mater EPM-442A ower sensor HP 8431A efference 20 dB Attenuator eference 10 dB Attenuator eference Probe ES3DV3 AE4 econdary Standards ower sensor HP 8481A F generator Agilent E4421B etwork Analyzer HP 8753E	TE critical for calibration)  ID #  GB37480704  US37292783  SN: 5066 (20g)  SN: 5047.2 (10r)  SN 3025  SN 601  ID #  MY41092317  MY41090675  US37390585 S4206	Cal Date (Calibrated by, Certificate No.)  63-Oct-06 (METAS, No. 217-00608)  63-Oct-06 (METAS, No. 217-00608)  10-Aug-08 (METAS, No. 217-00591)  10-Aug-08 (METAS, No. 217-00591)  19-Oct-08 (SPEAG, No. ES3-3025_Oct06)  30-Jan-07 (SPEAG, No. DAE4-601_Jan07)  Check Date (in house)  18-Oct-02 (SPEAG, in house check Oct-05)  11-May-05 (SPEAG, in house check Nov-05)  18-Oct-01 (SPEAG, in house check Oct-06)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Aug-07 Oct-07 Jan-08 Scheduled Chack In house check: Nov-07 In house check: Nov-07
calibration Equipment used (M& many Standards ) Tower sensor HP 8431A  telerence 20 dB Attenuator  telerence Probe ES3DV3  JAE4  Jacondary Standards  Tower sensor HP 8481A  Jacondary Standards  Tower sensor HP 8481A  Jacondary Standards  Tower sensor HP 8481A  Jacondary Aglent E4421B	TE critical for calibration)  ID #  GB37480704  U337292783  SN: 5067 (20g)  SN: 5047.2 (10r)  SN 3025  SN 601  ID #  MY41092317  MY41090575  US37390585 S4206	Cal Date (Calibrated by, Certificate No.) C3-Oct-06 (METAS, No. 2:7-00608) C3-Oct-06 (METAS, No. 2:7-00608) 10-Aug-06 (METAS, No. 2:7-00591) 10-Aug-06 (METAS, No. 2:7-00591) 19-Oct-06 (SPEAG, No. ES3-3025_Oct06) S0-Jan-07 (SPEAG, No. DAE4-001_Jan07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Nov-05) 11-May-05 (SPEAG, in house check Nov-05)	Scheduled Calibration Oct-07 Oct-07 Aug-07 Oct-07 Jan-08 Scheduled Chack In house check: Oct-07 In house check: Oct-07

Certificate No: D2450V2-736\_Jul07

Page 1 of 9



## Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst C Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D2450V2-736\_Jul07

Page 2 of 9



#### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mha/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.6 ± 6 %	1.81 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C	******	

#### SAR result with Head TSL

SAR averaged over 1 cm3 (1 g) of Head TSL	condition	
SAR measured	250 mW input power	13.3 mW / g
SAR normalized	normalized to 1W	53.2 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	52.7 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.17 mW/g
SAR normalized	normalized to 1W	24.7 mW / g
SAR for nominal Hoad TSL parameters 1	-normalized to 1W	24.5 mW / g ± 16.5 % (k=2)

Certificate No: D2450V2-736\_Jul07

Page 3 of 9

<sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"



Body TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.5 ± 8 %	1.94 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		

### SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.0 mW / g
SAR normalized	normalized to 1W	52,0 mW / g
SAR for nominal Body TSL parameters 2	normalized to 1W	52.5 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	6.05 mW / g
SAR normalized	normalized to 1W	24.2 mW / g
SAR for nominal Body TSL parameters *	normalized to 1W	24.4 mW / g ± 16.5 % (k=2)

Certificate No: D2450V2-736\_Jul07

Page 4 of 9

<sup>&</sup>lt;sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"



#### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.1 Ω + 3.0 jΩ	
Return Loss	- 27.6 dB	

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	$48.7 \Omega + 4.6 j\Omega$	
Return Loss	- 26.3 dB	

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.158 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	August 26, 2003

Certificate No: D2450V2-736 Jul07

Page 5 of 9



#### DASY4 Validation Report for Head TSL

Date/Time: 12.07.2007 11:00:03

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB;

Medium parameters used: f = 2450 MHz,  $\sigma = 1.81$  mho/m;  $\epsilon_r = 38.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

#### DASY4 Configuration:

- Probe: ES3DV2 SN3025 (HF); ConvF(4.5, 4.5, 4.5); Calibrated: 19.10.2006
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronies: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

#### Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 93.0 V/m; Power Drift = -0.004 dB

Peak SAR (extrapolated) = 28.1 W/kg

SAR(1 g) = 13.3 mW/g; SAR(10 g) = 6.17 mW/g

Maximum value of SAR (measured) = 15.0 mW/g

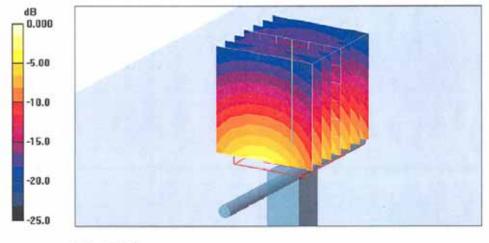


0 dB = 15.0 mW/g

Certificate No. D2450V2-736\_Jul07

Page 6 of 9



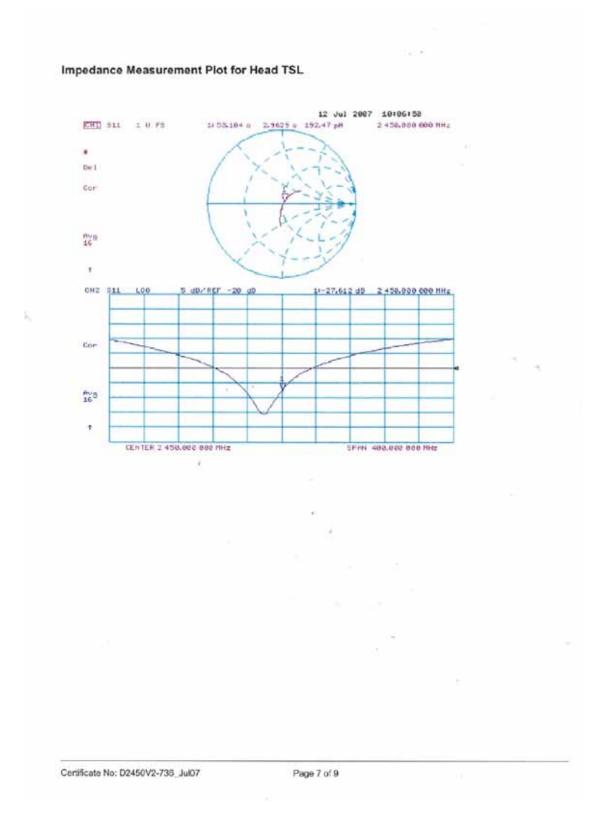



#### DASY4 Validation Report for Body TSL

Date/Time: 12.07.2007 12:28:49

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U10 BB;

Medium parameters used: f = 2450 MHz;  $\sigma = 1.94 \text{ mho/m}$ ;  $\varepsilon_r = 53.5$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

#### DASY4 Configuration:

- Probe: ES3DV2 SN3025 (HF); ConvF(4.16, 4.16, 4.16); Calibrated: 19.10.2006
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172.


#### Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx-5mm, dy-5mm, dz-5mm Reference Value = 88.6 V/m; Power Drift = 0.005 dB

Peak SAR (extrapolated) = 27.0 W/kg

SAR(1 g) = 13 mW/g; SAR(10 g) = 6.05 mW/g

Maximum value of SAR (measured) = 14.8 mW/g

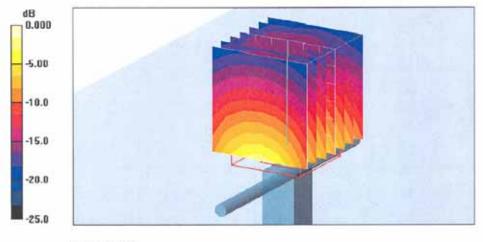


0 dB = 14.8mW/g

Certificate No: D2450V2-736\_Jul07

Page 8 of 9



## Impedance Measurement Plot for Body TSL

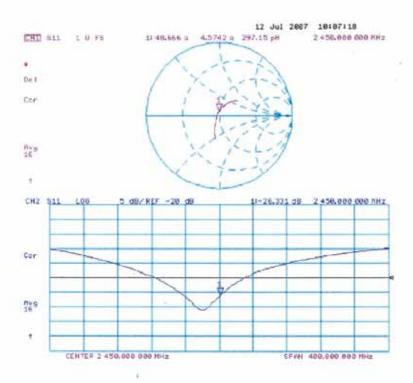

Certificate No: D2450V2-736\_Jul07

Page 9 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Auden

Accreditation No.: SCS 108

S

C

Certificate No: DAE4-679\_May08

#### Client CALIBRATION CERTIFICATE DAE4 - SD 000 D04 BA - SN: 679 Object QA CAL-06.v12 Calibration procedure(s) Calibration procedure for the data acquisition electronics (DAE) Calibration date: May 21, 2008 Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Scheduled Calibration Cal Date (Certificate No.) Primary Standards ID# 04-Oct-07 (No: 6467) 044-08 Fluke Process Calibrator Type 702 SN: 6295803 Oct-08 03-Oct-07 (No: 6465) SN: 0810278 Keithley Multimeter Type 2001 Scheduled Check Check Date (in house) Secondary Standards ID# In house check: Jun-08 SE UMS 006 AB 1004 25-Jun-07 (in house check) Calibrator Box V1,1 Function Name Dominique Steffen Technician Calibrated by: R&D Director Approved by: Fin Bombolt issued: May 21, 2008 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: DAE4-679\_May08

Page 1 of 5



Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerlscher Kallbrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE data acquisition electronics

Connector angle information used in DASY system to align probe sensor X to the robot

coordinate system.

#### Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an
    input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-679\_May08

Page 2 of 5



#### DC Voltage Measurement

A/D - Converter Resolution nominal

6.1µV , full range = -100...+300 mV 61nV , full range = -1......+3mV High Range: 1LSB = Low Range: 1LSB =

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	404.509 ± 0.1% (k=2)	404.928 ± 0.1% (k=2)	405.207 ± 0.1% (k=2)
Low Range	3.98477 ± 0.7% (k=2)	3.94731 ± 0.7% (k=2)	3.98878 ± 0.7% (k=2)

#### **Connector Angle**

Connector Angle to be used in DASY system	316°±1°
---	---------

Certificate No: DAE4-679\_May08

Page 3 of 5



#### Appendix

1. DC Voltage Linearity

High Range	Input (μV)	Reading (µV)	Error (%)
Channel X + Input	200000	199999.5	0.00
Channel X + Input	20000	20003.57	0.02
Channel X - Input	20000	-19999.29	0.00
Channel Y + Input	200000	199999.4	0.00
Channel Y + Input	20000	20003.45	0.02
Channel Y - Input	20000	-20004.32	0.02
Channel Z + Input	200000	199999.8	0.00
Channel Z + Input	20000	20002.50	0.01
Channel Z - Input	20000	-20004.27	0.02

Low Range	Input (μV)	Reading (µV)	Error (%)
Channel X + Input	2000	2000	0.00
Channel X + Input	200	200.27	0.13
Channel X - Input	200	-199.47	-0.27
Channel Y + Input	2000	1999.9	0.00
Channel Y + Input	200	199.26	-0.37
Channel Y - Input	200	-199.82	-0.09
Channel Z + Input	2000	2000	0.00
Channel Z + Input	200	199.19	-0.41
Channel Z - Input	200	-200.77	0.39

#### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	4.20	4.06
	- 200	-2.14	-1.85
Channel Y	200	6.39	6.01
	- 200	-6.03	-5.79
Channel Z	200	-4.80	-5.16
	- 200	4.08	4.80

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (µV)	Channel Z (μV)
Channel X	200		1.42	0.07
Channel Y	200	1.22	-	3.06
Channel Z	200	-1.13	1.08	

Certificate No: DAE4-679\_May08

Page 4 of 5



#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec: Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16182	17365
Channel Y	15398	16603
Channel Z	16047	16211

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	1.05	-1.09	2.60	0.50
Channel Y	-0.43	-2.28	1.41	0.66
Channel Z	-0.33	-2.83	1.40	0.56

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	198.9
Channel Y	0.2000	197.7
Channel Z	0.1999	196.5

8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	0.40	+7.9
Supply (- Vcc)	19	+7.6

9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.0	+6	+14
Supply (- Vcc)	-0.01	-8	-9



## Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C

Servizio svizzero di taratura S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Sporton (Auden)

Accreditation No.: SCS 108

Certificate No: ET3-1787\_Aug08 CALIBRATION CERTIFICATE ET3DV6 - SN:1787 Object QA CAL-01.v6 and QA CAL-23.v3 Calibration procedure(s) Calibration procedure for dosimetric E-field probes August 26, 2008 In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (Si) The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70% Calibration Equipment used (M&TE critical for calibration) Primary Standards Cal Date (Certificate No.) Scheduled Calibration Power meter E44198 GB41293874 1-Apr-08 (No. 217-00788) Apr-09 Power sensor E4412A MY41495277 1-Apr-08 (No. 217-00768) Power sensor E4412A MY41498087 1-Apr-08 (No. 217-00788) Apr-09 SN: S5054 (3c) 1-Jul-08 (No. 217-00865) Jul-09 Reference 3 dB Attenuator Apr-09 Reference 20 dB Attenuator SN: \$5086 (20b) 31-Mar-08 (No. 217-00787) Jul-09 Reference 30 dB Attenuator SN: \$5129 (30b) 1-Jul-08 (No. 217-00866) Reference Probe ES3DV2 SN: 3013 2-Jan-08 (No. ES3-3013\_Jan08) Jan-09 DAE4 SN: 660 3-Sep-07 (No. DAE4-660\_Sep07) Sep-08 Secondary Standards Check Date (in house) RF generator HP 8648C U\$3642U01700 4-Aug-99 (in house check Oct-07) In house check: Oct-09 Network Analyzer HP 8753E US37390585 18-Oct-01 (in house check Oct-07) in house check: Oct-08 Function Calibrated by: Katja Pokovic Technical Manager Approved by: Niels Kuster Quality Manag Issued: August 26, 2008

Certificate No: ET3-1787\_Aug08

Page 1 of 9

This calibration certificate shall not be reproduced except in full without written approval of the laboratory



#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

Service suisse d'étalonnage

C Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL NORMx,y,z

ConvF

tissue simulating liquid sensitivity in free space sensitivity in TSL / NORMx,y,z

DCP

diode compression point φ rotation around probe axis

Polarization o Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at

measurement center), i.e., 9 = 0 is normal to probe axis

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques\*, December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E2-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1787 Aug08

Page 2 of 9

August 26, 2008

# Probe ET3DV6

SN:1787

Manufactured:

Last calibrated: Recalibrated: May 28, 2003

August 28, 2007 August 26, 2008

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: ET3-1787\_Aug08

Page 3 of 9



August 26, 2008

### DASY - Parameters of Probe: ET3DV6 SN:1787

Sensitivity in Free Space<sup>A</sup>

Diode Compression<sup>B</sup>

NormX	1.63 ± 10.1%	$\mu V/(V/m)^2$	DCP X	90 mV
NormY	1.67 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	93 mV
NormZ	2.18 ± 10.1%	$\mu V/(V/m)^2$	DCP Z	92 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

#### **Boundary Effect**

TSL

900 MHz Typical SAR gradient: 5 % per mm

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR <sub>be</sub> [%]	Without Correction Algorithm	11.3	7.5
SAR <sub>50</sub> [%]	With Correction Algorithm	0.8	0.5

TSL

1750 MHz

Typical SAR gradient: 10 % per mm

Sensor Cente	r to Phantom Surface Distance	3.7 mm	4.7 mm
SAR <sub>60</sub> [%]	Without Correction Algorithm	10.1	6.5
SAR <sub>00</sub> [%]	With Correction Algorithm	8.0	0.6

#### Sensor Offset

Probe Tip to Sensor Center

2.7 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: ET3-1787\_Aug08

Page 4 of 9


<sup>&</sup>lt;sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 8).

Numerical linearization parameter: uncertainty not required.

August 26, 2008

# Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

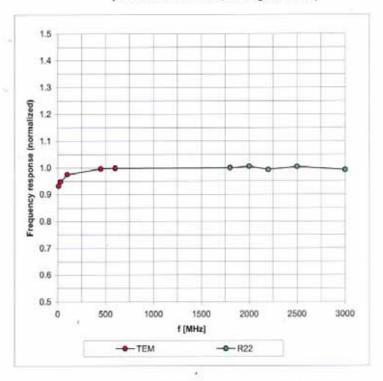


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Certificate No: ET3-1787\_Aug08


Page 5 of 9

#### August 26, 2008

# Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$





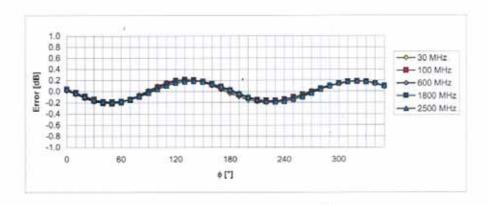

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Certificate No: ET3-1787\_Aug08


Page 6 of 9

August 26, 2008

# Dynamic Range f(SAR<sub>head</sub>)

(Waveguide R22, f = 1800 MHz)

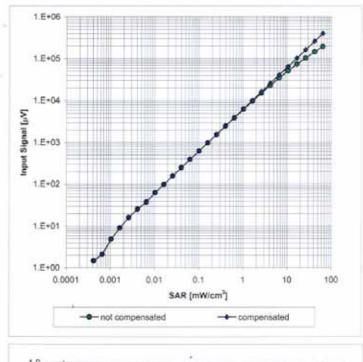

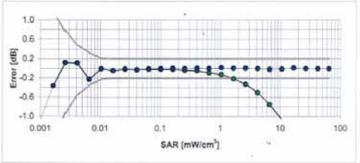


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Certificate No: ET3-1787\_Aug08

Page 7 of 9

August 26, 2008

#### Conversion Factor Assessment





f [MHz]	Validity [MHz] <sup>©</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	±50/±100	Head	41.5 ± 5%	0.97 ± 5%	0.30	2.80	6.06 ± 11.0% (k=2)
1750	±50/±100	Head	40.1 ± 5%	1.37 ± 5%	0.53	2.11	5.36 ± 11.0% (k=2)
1950	±50/±100	Head	40.0 ± 5%	1.40 ± 5%	0.59	1.96	5.01 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1,80 ± 5%	0.77	1.57	4.49 ± 11.0% (k=2)
				19			
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.31	2.98	5.91 ± 11.0% (k=2)
1750	±50/±100	Body	53.4 ± 5%	$1.49 \pm 5\%$	0.60	2.20	4.73 ± 11.0% (k=2)
1950	±50/±100	Body	53.3 ± 5%	$1.52 \pm 5\%$	0.68	1.95	4.49 ± 11.0% (k=2)
2450	±50/±100	Body	52.7 ± 5%	1.95 ± 5%	0.90	1.51	3.79 ±11.0% (k=2)

Certificate No: ET3-1787\_Aug08


Page 8 of 9

<sup>&</sup>lt;sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

August 26, 2008

## Deviation from Isotropy in HSL

Error (6, 8), f = 900 MHz

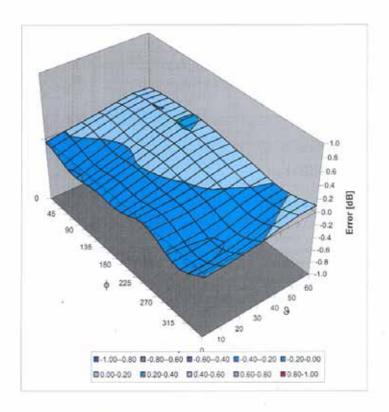


Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ET3-1787\_Aug08

Page 9 of 9




# Appendix D - Product Photos

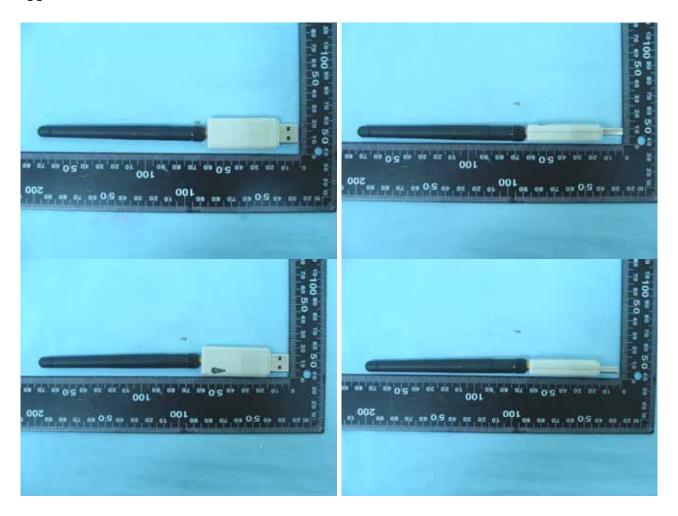




# Appendix E - Test Setup Photos

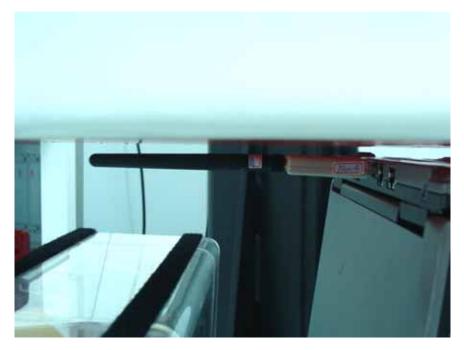


USB Configuration 1 and Antenna set Straight




USB Configuration 1 and Antenna set Perpendicular

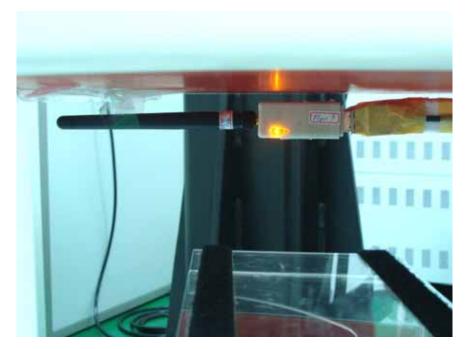

USB Configuration 2 and Antenna set Straight

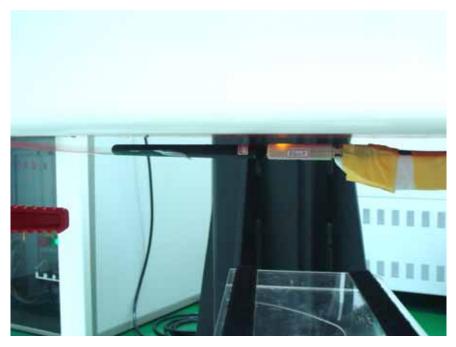

USB Configuration 3 and Antenna set Straight

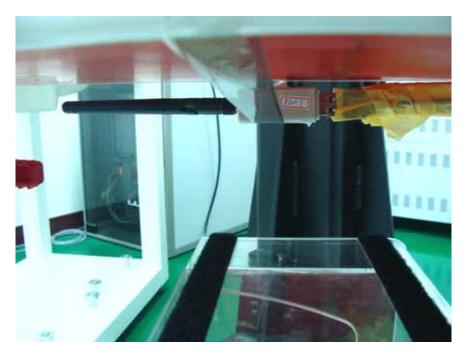

USB Configuration 4 and Antenna set Straight