



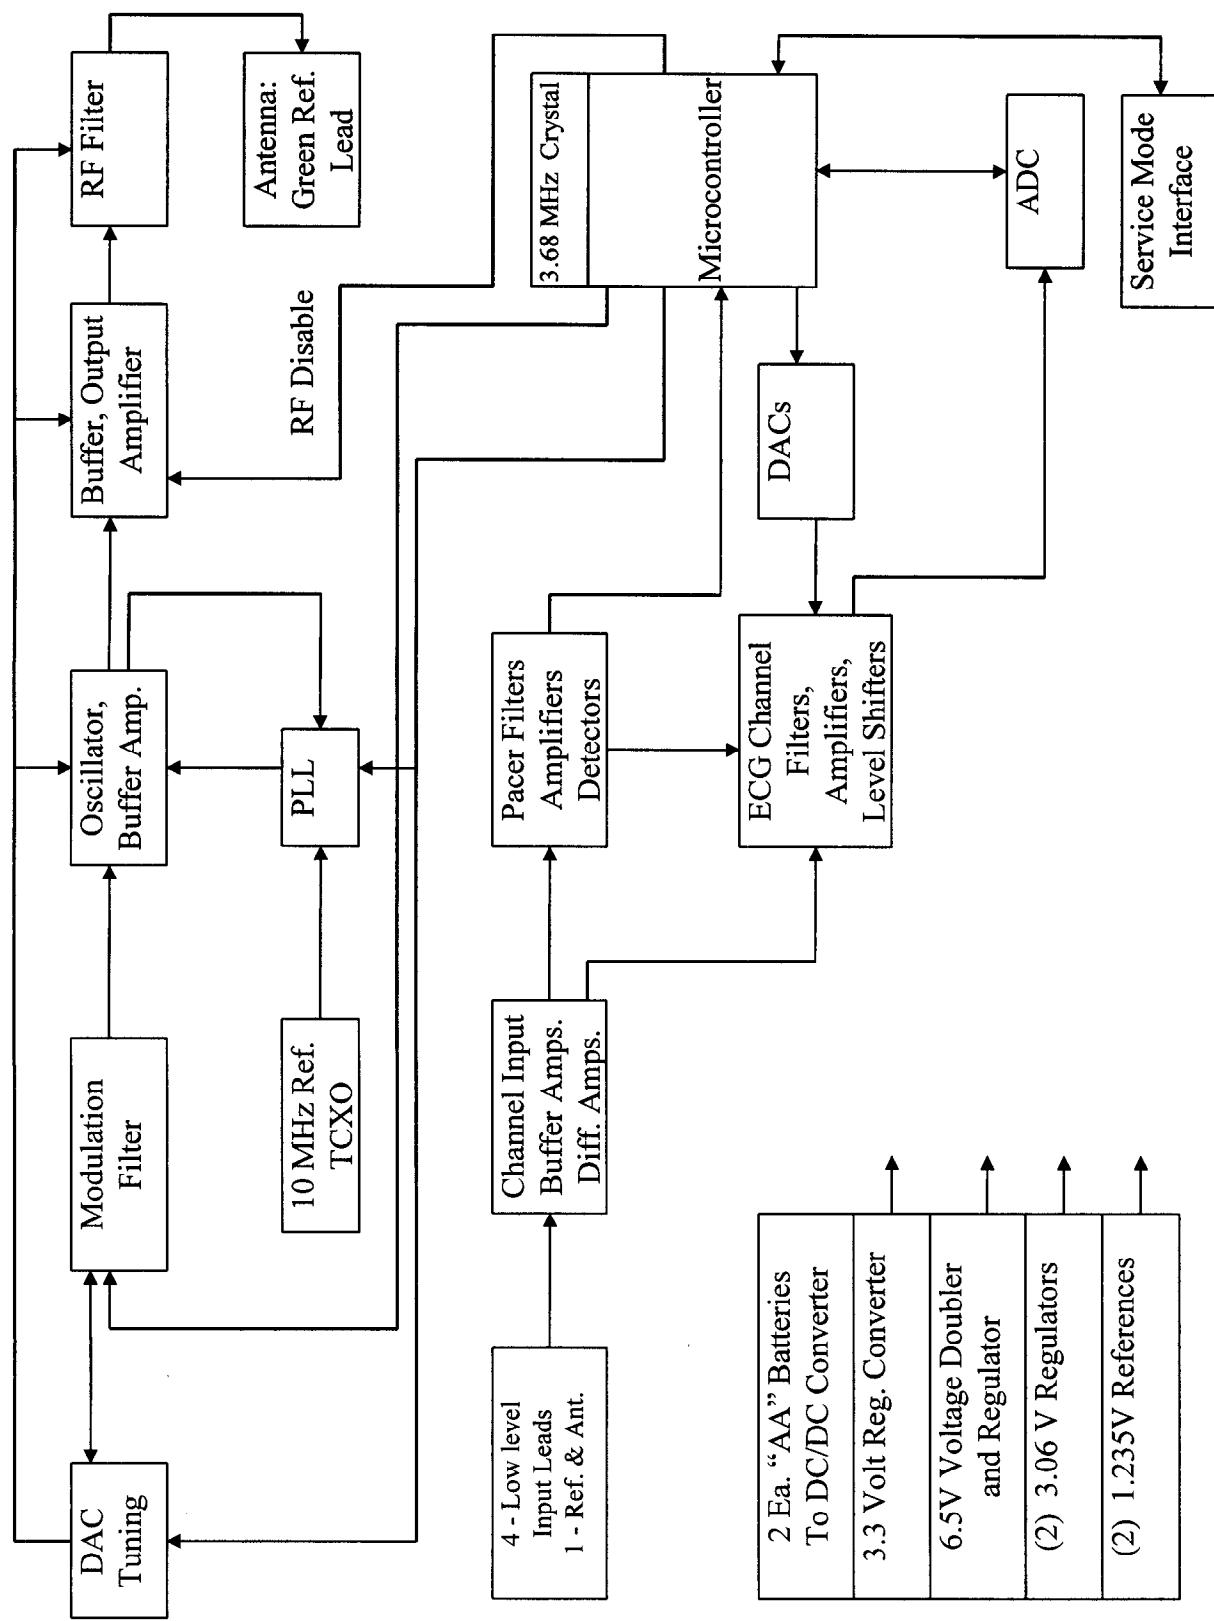

Transmitter Block Diagram

FCC ID: MRA-109153

1 2 3 4 5 6 7 8

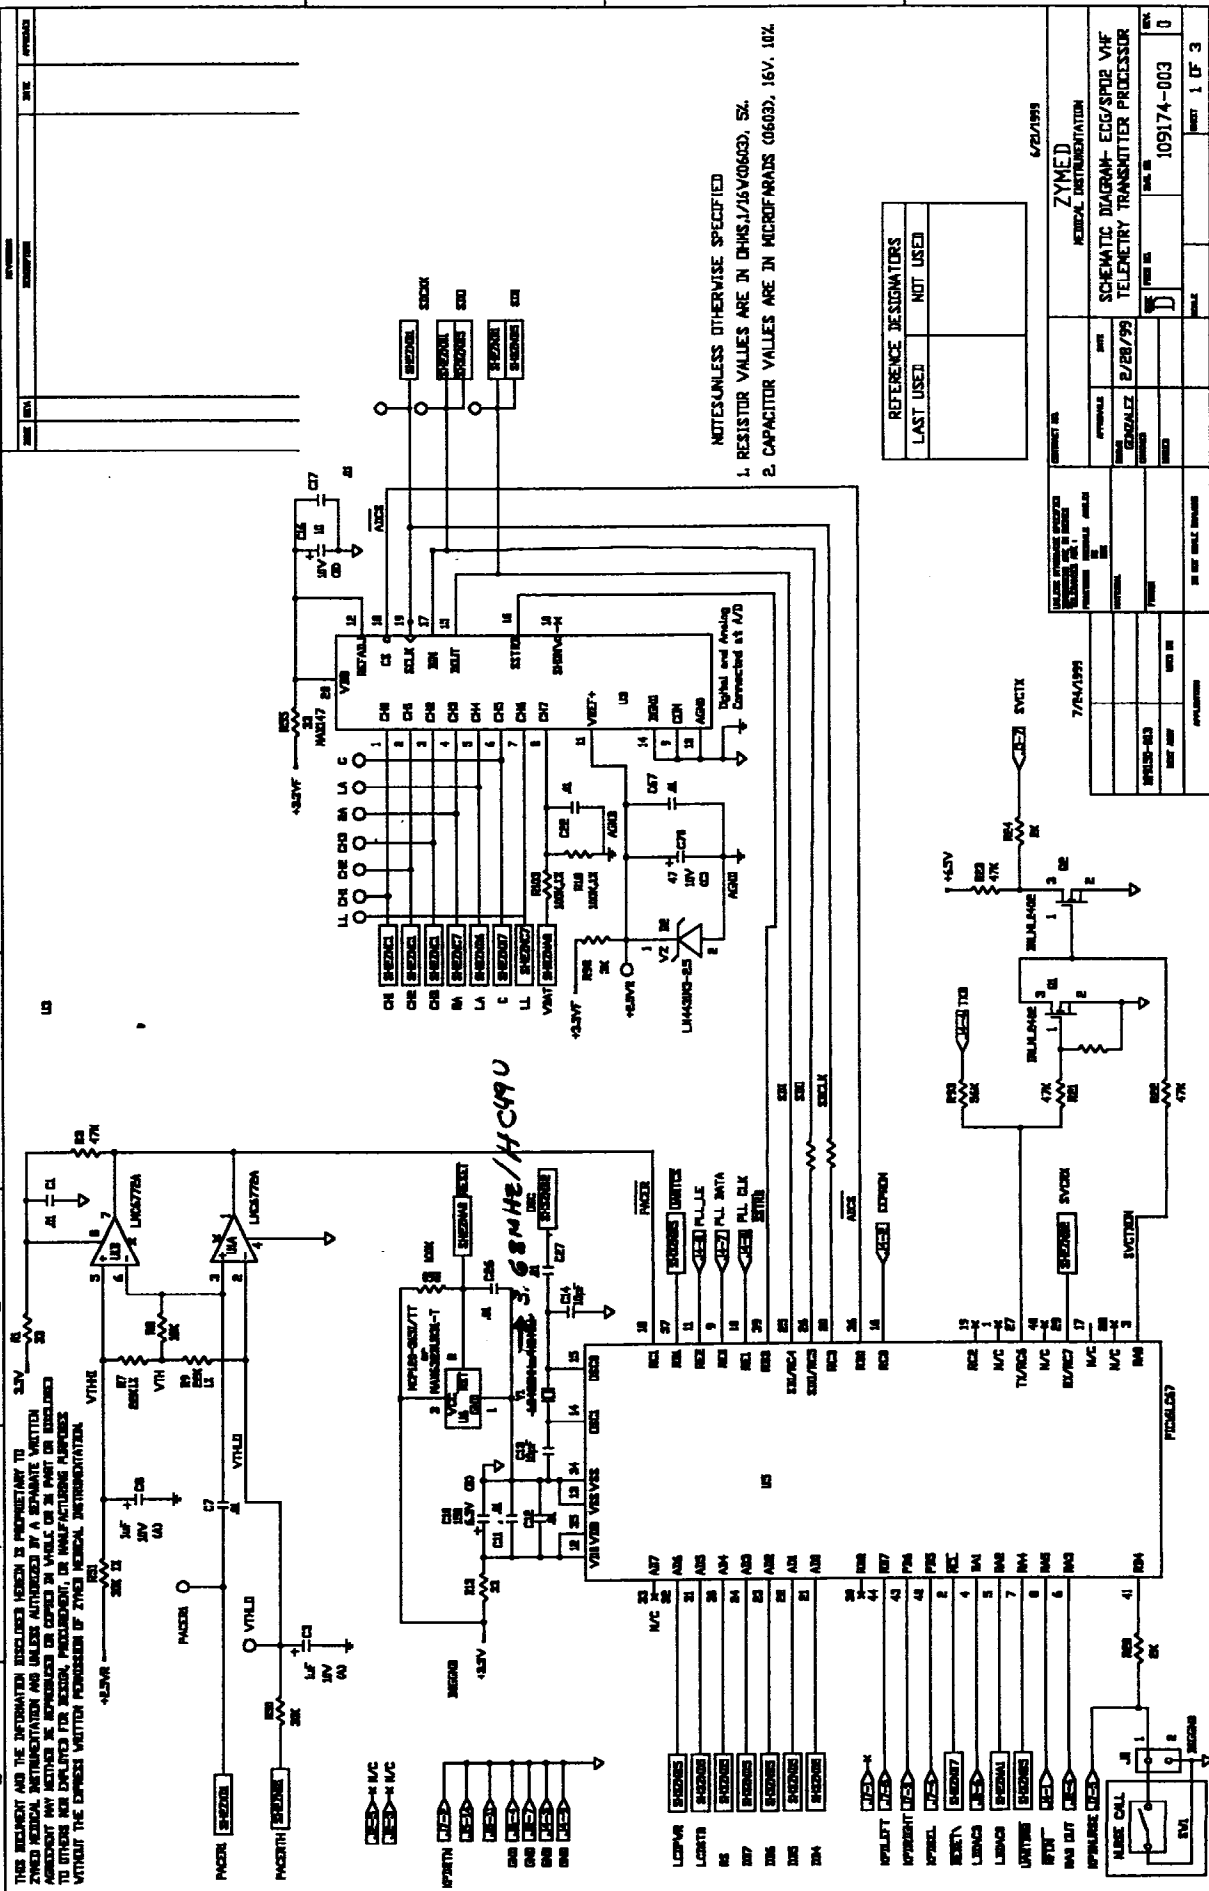


NOTES UNLESS OTHERWISE SPECIFIED
 1. RESISTOR VALUES ARE IN OHMS, 1/16W, 0603, 5%.
 2. CAPACITOR VALUES ARE IN MICROFARADS 0603, 16V, 10%.

REFERENCE DESIGNATORS	
LAST USED	NOT USED

ZYMED MEDICAL INSTRUMENTATION	
DATE	8/20/1999
DESIGNED BY	SCHEMATIC DIAGRAM - ECG/SPUR VHF TELEMETRY TRANSMITTER PROCESSOR
DATE	8/20/1999
REV	0
REV	109174-003
REV	0

1 2 3 4 5 6 7 8



8 7 6 5 4 3 2 1

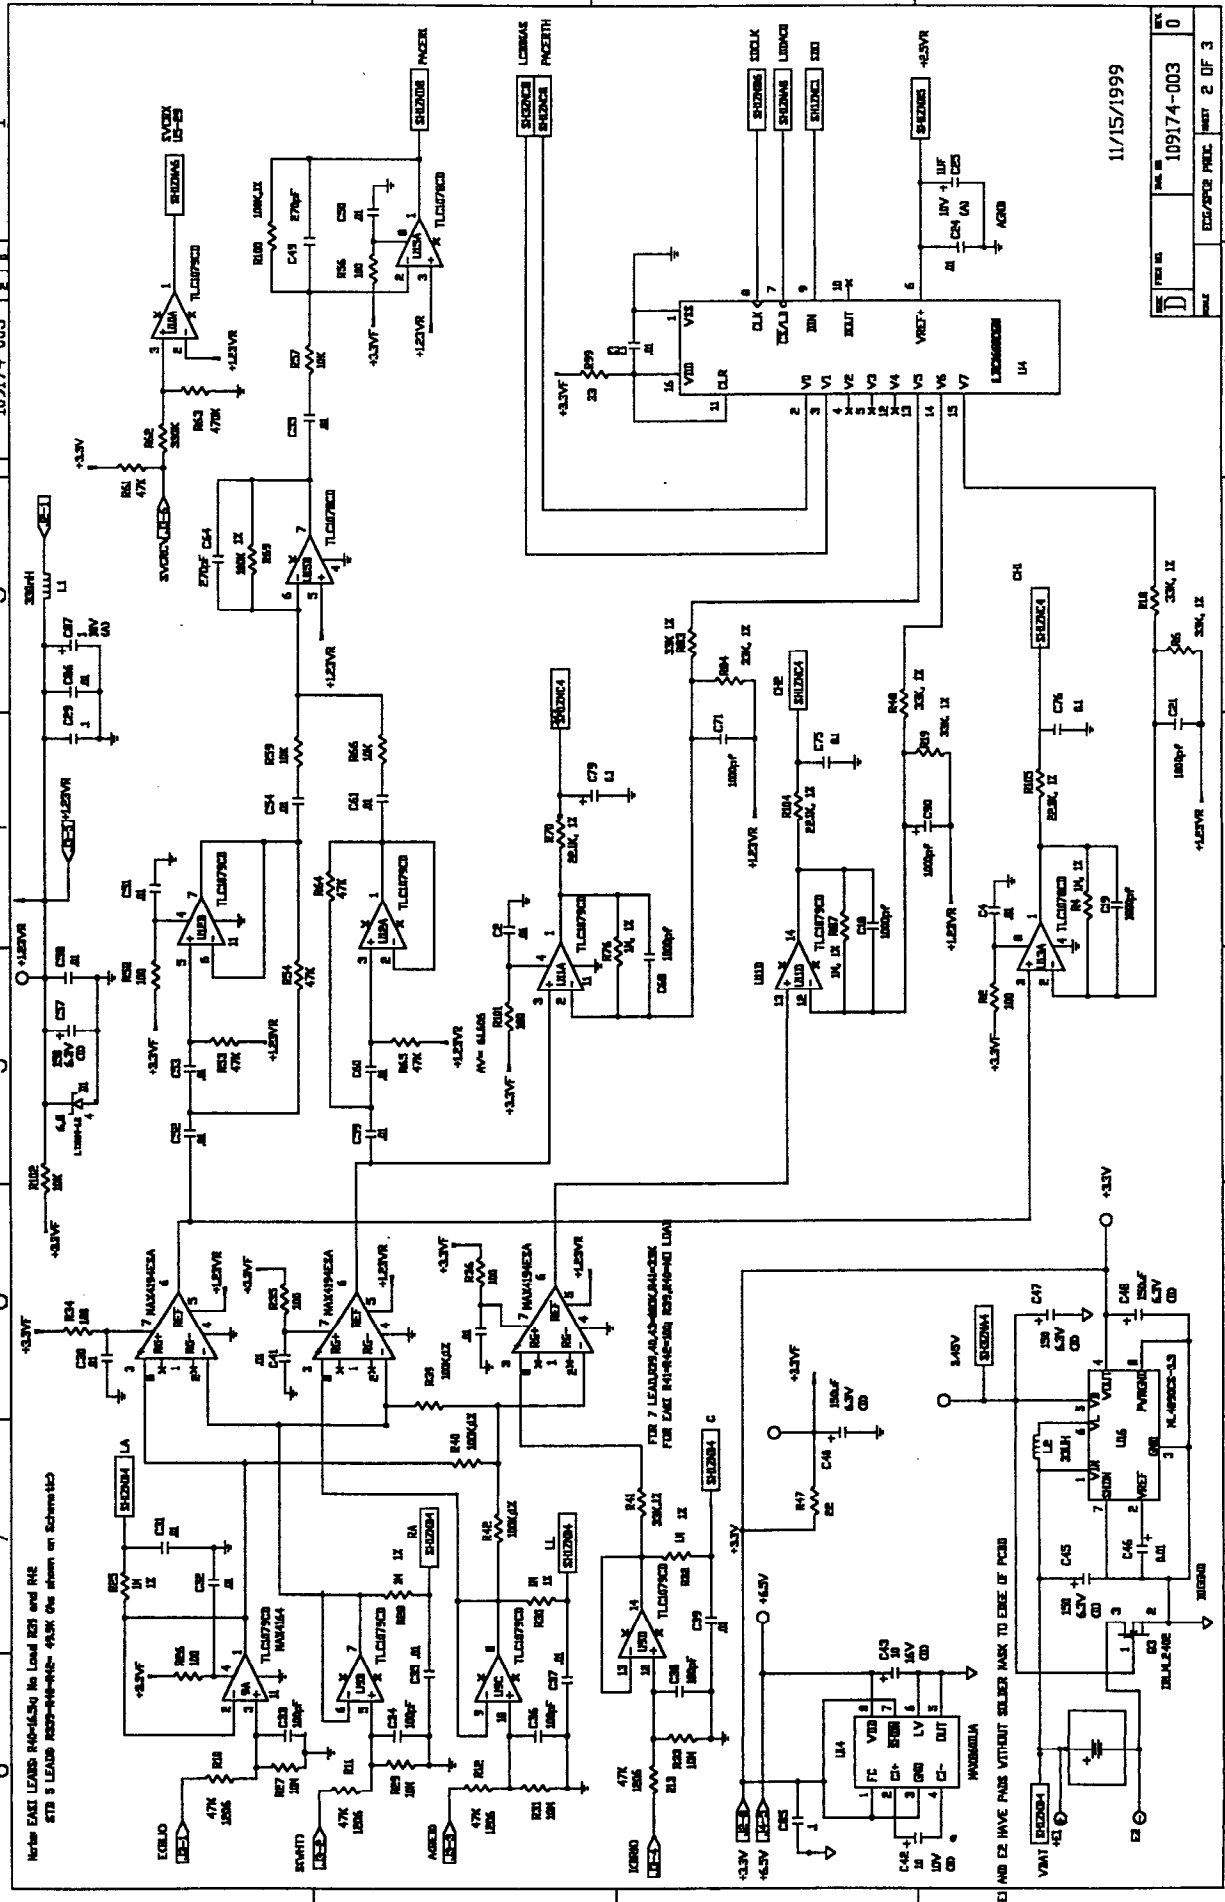

11/15/1999

REV	0
DATE	11/15/1999
DESIGNER	109174-003
CHKD BY	
DATE	
REV	0
DATE	
DESIGNER	
CHKD BY	
DATE	

THIS DOCUMENT AND THE INFORMATION ENCLOSED HEREIN IS PROPRIETARY TO
ZYMED MEDICAL INSTRUMENTATION AND UNLESS AUTHORIZED BY A SEPARATE WRITTEN
AGREEMENT MAY NEITHER BE REPRODUCED OR COPIED IN WHOLE OR IN PART OR ENCLOSED
TO OTHERS NOR EMPLOYED FOR DESIGN, PROCUREMENT, OR MANUFACTURING PURPOSES
WITHOUT THE EXPRESS WRITTEN PERMISSION OF ZYMED MEDICAL INSTRUMENTATION.

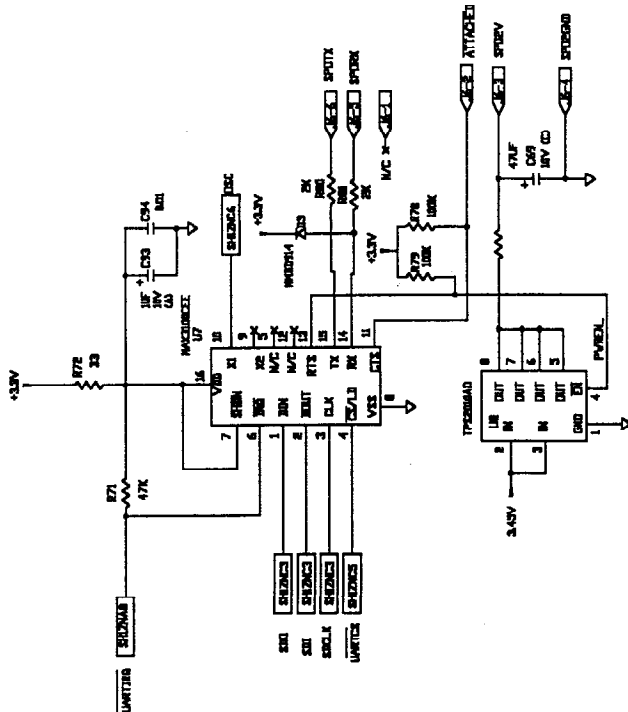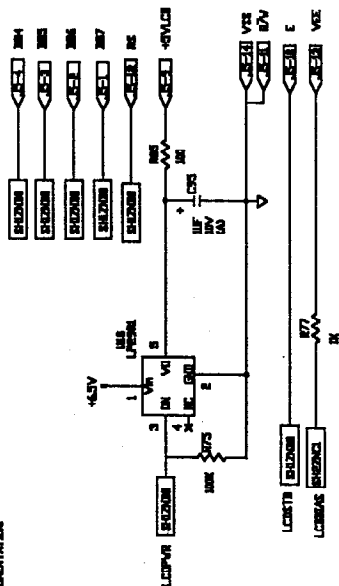

7/21/1999

REV	0
DATE	10/17/94
BY	109174-003
HEET	3 OF 3