



Specific Absorption Rate (SAR) Test Report for ASUSTeK computer INC.

on the

3G Smart Phone (GSM900/DCS1800/PCS1900/WCDMA2100/Bluetooth)

Report No.	: FA680808-1-2-03
Trade Name	: Vodafone
Model Name	: VDA IV
FCC ID	: MSQ-1210
Date of Testing	: Aug. 08-09, 2006
Date of Report	: Sep. 15, 2006
Date of Review	: Sep. 15, 2006

- The test results refer exclusively to the presented test model/sample only.
- Without written approval of SPORTON International Inc., the test report shall not be reproduced except in full.
- Report Version: Rev. 04.

SPORTON International Inc.

6F, No.106, Sec. 1, Hsin Tai Wu Rd., Hsi Chih, Taipei Hsien, Taiwan, R.O.C.



Table of Contents

1. Statement of Compliance	1
2. Administration Data	2
2.1 Testing Laboratory	2
2.2 Detail of Applicant	2
2.3 Detail of Manufacturer	2
2.4 Application Detail	2
3. General Information	3
3.1 Description of Device Under Test (DUT)	3
3.2 Product Photo	4
3.3 Applied Standards:	5
3.4 Device Category and SAR Limits	6
3.5 Test Conditions:	6
3.5.1 Ambient Condition	6
3.5.2 Test Configuration	6
4. Specific Absorption Rate (SAR)	7
4.1 Introduction	
4.2 SAR Definition	7
5. SAR Measurement Setup	8
5.1 DASY4 E-Field Probe System	
5.1.1 ET3DV6 E-Field Probe Specification	10
5 1 2 FT3DV6 F-Field Probe Calibration	
5.2 DATA Acquisition Electronics (DAE)	11
5.3 Robot	12
5.4 Measurement Server	12
5.5 SAM Twin Phantom	
5.6 Device Holder for SAM Twin Phantom	14
5.7 Data Storage and Evaluation	15
5.7.1 Data Storage	15
5.7.2 Data Evaluation	15
5.8 Test Equipment List	18
6. Tissue Simulating Liquids	19
7. Uncertainty Assessment	21
8. SAR Measurement Evaluation	
8.1 Purpose of System Performance check	23
8.2 System Setup	23
8.3 Validation Results	25
9. Description for DUT Testing Position	26
10. Measurement Procedures	31
11. SAR Test Results	33
11.1 Right Cheek	
11.2 Right Tilted	33
11.3 Left Cheek	33
11.4 Left Tilted	33
11.5 Keypad Up with 1.5 cm Gap	34
11.6 Keypad Down with 1.5 cm Gap	34
12. References	

Appendix A - System Performance Check Data Appendix B - SAR Measurement Data Appendix C - Calibration Data

1. Statement of Compliance

The Specific Absorption Rate (SAR) maximum results found during testing for the ASUSTeK computer INC. 3G Smart Phone (GSM900/DCS1800/PCS1900/WCDMA2100/Bluetooth) Vodafone VDA IV are 0.722 W/kg for PCS head SAR and 0.766 W/kg for PCS body SAR with expanded uncertainty 20.6%. The co-location of GSM/GPRS and Bluetooth were also checked. They are in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1999 and had been tested in accordance with the measurement methods and procedures specified in OET Bulletin 65 Supplement C (Edition 01-01).

Approved by

00-

Dr. Daniel Lee EMC/SAR Director

©2006 SPORTON International Inc. SAR Testing Lab This report shall not be reproduced except in full, without the written approval of Sporton. Page 1 of 35 Rev. 04 SECRETOR LAR. FCC SAR Test Report

Test Report No 🔅 FA680808-1-2-03

2. Administration Data

2.1 Testing Laboratory

Company Name :	Sporton International Inc.
Department :	Antenna Design/SAR
Address :	No.52, Hwa-Ya 1 st RD., Hwa Ya Technology Park, Kwei-Shan Hsiang, TaoYuan
	Hsien, Taiwan, R.O.C.
Telephone Number :	886-3-327-3456
Fax Number :	886-3-327-0973

2.2 Detail of Applicant

Company Name :	ASUSTeK computer INC.	
Address :	No. 150, Li-Te Rd., Peitou, Taiwan, R.O.C.	
Telephone Number :	02-2799-8800 ext.6840	
Fax Number :	02-2656-6399	
Contact Person :	Rex.yang@benq.com	

2.3 Detail of Manufacturer

Company Name :	ASUSTeK computer INC.
Address :	No. 5 Shing Yeh St., Kwei Shan Hsiang, Tao Yuan Hsien, Taiwan, R.O.C.

2.4 Application Detail

Date of reception of application:	Aug. 08, 2006
Start of test :	Aug. 08, 2006
End of test :	Aug. 09, 2006



3. General Information

3.1 Description of Device Under Test (DUT)

DUT Type :	3G Smart Phone (GSM900/DCS1800/PCS1900/WCDMA2100/Bluetooth)	
Trade Name :	Vodafone	
Model Name :	VDA IV	
FCC ID :	MSQ-1210	
Tx Frequency :	PCS : 1850-1910 MHz BT : 2400-2483.5 MHz	
Rx Frequency : PCS : 1930-1990 MHz BT : 2400-2483.5 MHz		
Antenna Type :	PCS : PIFA Antenna BT : Chip Antenna	
Maximum Output Power :	PCS : 29.63 dBm BT : 1.67 dBm	
HW Version :	R1.4.1	
SW Version :	v2.2.0d	
Power Rating (DC/AC, Voltage)	DC 3.7V / 1100mA	
Type of Modulation :	PCS : GMSK BT : GFSK	
DUT Stage :	Identical Prototype	
Application Type :	Certification	



3.2 Product Photo





3.3 Applied Standards:

The Specific Absorption Rate (SAR) testing specification, method and procedure for this 3G Smart Phone (GSM900/DCS1800/PCS1900/WCDMA2100/Bluetooth) is in accordance with the following standards:

47 CFR Part 2 (2.1093), IEEE C95.1-1999, IEEE C95.3-2002, IEEE P1528-2003, and OET Bulletin 65 Supplement C (Edition 01-01)



3.4 Device Category and SAR Limits

This device belongs to portable device category because its radiating structure is allowed to be used within 20 centimeters of the body of the user.

Limit for General Population/Uncontrolled exposure should be applied for this device, it is 1.6 W/kg as averaged over any 1 gram of tissue.

3.5 Test Conditions:

3.5.1 Ambient Condition

Item	Head	Body	
Ambient Temperature (°C)	20-24		
Tissue simulating liquid temperature (°C)	21.0 20.8		
Humidity (%)	<60 %		

3.5.2 Test Configuration

The device was controlled by using a base station emulator R&S CMU200. Communication between the device and the emulator was established by air link. The distance between the DUT and the antenna of the emulator is larger than 50 cm and the output power radiated from the emulator antenna is at least 30 dB smaller than the output power of DUT.

Measurements were performed on the lowest, middle, and highest channel for each testing position for head SAR testing. Measurements were performed only on the middle channel if the SAR is below 3 dB of limit for body SAR testing.

The DUT was set from the emulator to radiate maximum output power during all testings.

For head SAR testing, EUT is in GSM link mode, and its crest factor is 8.3. For body SAR testing, EUT is in GPRS link mode, and its crest factor is 4 because EUT is GPRS class 10 device.



4. Specific Absorption Rate (SAR)

4.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

4.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density.

). The equation description is as below:

$$\mathbf{SAR} = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

SAR =
$$C \frac{\delta T}{\delta t}$$

, where C is the specific head capacity, δT is the temperature rise and δt the exposure duration,

or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\sigma |E|^2}{\rho}$$

, where is the conductivity of the tissue, is the mass density of the tissue and E is the rms electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.

©2006 SPORTON International Inc. SAR Testing Lab

Page 7 of 35 Rev. 04

This report shall not be reproduced except in full, without the written approval of Sporton.



5. SAR Measurement Setup

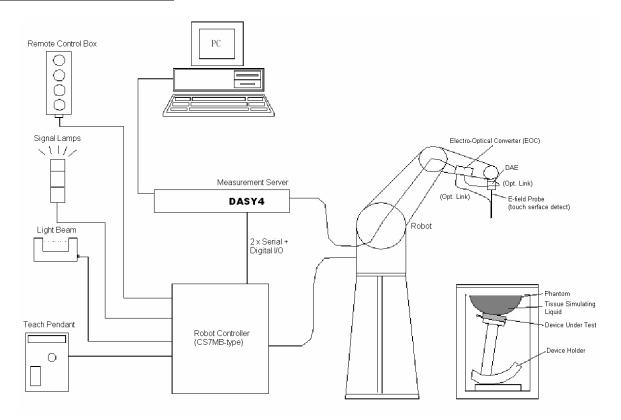


Fig. 5.1 DASY4 system



The DASY4 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- A dosimetric probe equipped with an optical surface detector system
- > The electro-optical converter (ECO) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the accuracy of the probe positioning
- A computer operating Windows XP
- DASY4 software
- Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- The SAM twin phantom
- A device holder
- Tissue simulating liquid
- > Dipole for evaluating the proper functioning of the system

Some of the components are described in details in the following sub-sections.

5.1 DASY4 E-Field Probe System


The SAR measurement is conducted with the dosimetric probe ET3DV6 (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency. This probe has a built in optical surface detection system to prevent from collision with phantom.



5.1.1 ET3DV6 E-Field Probe Specification

Construction	Symmetrical design with triangular core Built-in optical fiber for surface detection system Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents)
Calibration	Simulating tissue at frequencies of 900MHz, 1.8GHz and 2.45GHz for brain and muscle (accuracy $\pm 8\%$)
Frequency	10 MHz to $>$ 3 GHz
Directivity	\pm 0.2 dB in brain tissue (rotation around probe axis) \pm 0.4 dB in brain tissue (rotation perpendicular to probe axis)
Dynamic Range	$5 \mu W/g \text{ to } > 100 \text{mW/g; Linearity: } \pm 0.2 \text{dB}$
Surface Detection	\pm 0.2 mm repeatability in air and clear liquids on reflecting surface
Dimensions	Overall length: 330mm Tip length: 16mm Body diameter: 12mm
Application	Tip diameter: 6.8mm Distance from probe tip to dipole centers: 2.7mm General dosimetry up to 3GHz Compliance tests for mobile phones and Wireless LAN Fast automatic scanning in arbitrary phantoms





5.1.2 ET3DV6 E-Field Probe Calibration

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy shall be evaluated and within \pm 0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data are as below:

Page 10 of 35 Rev. 04



Sensitivity	X axis : 1.57 μV		Y axis : 1.71 μV		Z axis : 2.09 μV	
Diode compression point	X axis : 94 mV		Y axis : 94 mV		Z axis : 94 mV	
	Frequency (MHz) X axis		Y axis	Z axis		
Conversion factor (Head / Body)	800~1000	6.38 /	6.18	6.38 / 6.18	6.38 / 6.18	
	1710~1910	5.26 /	4.66	5.26 / 4.66	5.26 / 4.66	
	Frequency (MHz)	Alp	oha	Depth		
Boundary effect (Head / Body)	800~1000	0.50 /	0.44	1.85 / 2.10		
	1710~1910	0.59/	0.62	2.46 / 2.44		

NOTE:

> The probe parameters have been calibrated by the SPEAG.

5.2 DATA Acquisition Electronics (DAE)

The data acquisition electronics (DAE) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.



5.3 Robot

The DASY4 system uses the high precision robots RX90BL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASYS system, the CS7MB robot controller version from Stäubli is used. The RX robot series have many features that are important for our application:

- ➢ High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- ➢ 6-axis controller

5.4 Measurement Server

The DASY4 measurement server is based on a PC/104 CPU board with 166 MHz CPU 32 MB chipset and 64 MB RAM.

Communication with the DAE4 electronic box the 16-bit AD-converter system for optical detection and digital I/O interface.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.

5.5 SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- ➢ Left head
- Right head
- ➢ Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections.

A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters.



On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

The phantom can be used with the following tissue simulating liquids:

- *Water-sugar based liquid
- *Glycol based liquids

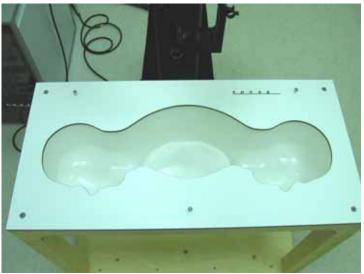


Fig. 5.3 Top view of twin phantom



Fig. 5.4 Bottom view of twin phantom



5.6 Device Holder for SAM Twin Phantom

The SAR in the Phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source in 5 mm distance, a positioning uncertainty of ± 0.5 mm would produce a SAR uncertainty of $\pm 20\%$. An accurate device position is therefore crucial for accurate and repeatable measurement. The position in which the devices must be measured, are defined by the standards.

The DASY device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (EPR). Thus the device needs no repositioning when changing the angles.

The DASY device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity r=3 and loss tangent $\delta = 0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



Fig. 5.5 Device Holder



5.7 Data Storage and Evaluation

5.7.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The postprocessing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [A/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a loseless media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

5.7.2 Data Evaluation

The DASY4 postprocessing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software :

Probe parameters :	- Sensitivity	Norm _{<i>i</i>} , a_{i^0} , a_{i^1} , a_{i^2}
	- Conversion factor	ConvF _i
	- Diode compression point	dcp <i>i</i>
Device parameters :	- Frequency	f
	- Crest factor	cf
Media parameters :	- Conductivity	
	- Density	

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel



can be given as :

$$Vi = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with

 V_i = compensated signal of channel i (i = x, y, z) U_i = input signal of channel i (i = x, y, z) cf = crest factor of exciting field (DASY parameter) dcp_i = diode compression point (DASY parameter)

From the compensated input signals, the primary field data for each channel can be evaluated :

E-field probes :
$$E_i = \sqrt{\frac{V_i}{Norm_iConvF}}$$

H-field probes : $H_i = \sqrt{V_i \frac{a_{i0+}a_{i1}f + a_{i2}f^2}{f}}$

with V_i = compensated signal of channel i (i = x, y, z) $Norm_i$ = sensor sensitivity of channel i (i = x, y, z) $\mu V/(V/m)2$ for E-field Probes ConvF = sensitivity enhancement in solution a_{ij} = sensor sensitivity factors for H-field probes f = carrier frequency [GHz] E_i = electric field strength of channel i in V/m H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude) :

$$E_{tot} = \sqrt{E_X^2 + E_Y^2 + E_Z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with

SAR = local specific absorption rate in mW/g
Etot = total field strength in V/m
= conductivity in [mho/m] or [Siemens/m]
= equivalent tissue density in g/cm³



* Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or $P_{pwe} = H_{tot}^2 \cdot 37.7$

with P_{pwe} = equivalent power density of a plane wave in mW/cm² E_{tot} = total electric field strength in V/m H_{tot} = total magnetic field strength in A/m



5.8 Test Equipment List

		Type/Model Serial Number		Calibration		
Manufacture	Name of Equipment	Type/Model	Serial Number	Last Cal.	Due Date	
SPEAG	Dosimetric E-Filed Probe	ET3DV6	1787	May 31, 2006	May 31, 2007	
SPEAG	835MHz System Validation Kit	D835V2	499	Mar. 15, 2006	Mar. 15, 2008	
SPEAG	900MHz System Validation Kit	D900V2	190	Jul. 19, 2005	Jul. 19, 2007	
SPEAG	1800MHz System Validation Kit	D1800V2	2d076	Jul. 20, 2005	Jul. 20, 2007	
SPEAG	1900MHz System Validation Kit	D1900V2	5d041	Mar. 21, 2006	Mar. 21, 2008	
SPEAG	2450MHz System Validation Kit	D2450V2	736	Jul. 12, 2005	Jul. 12, 2007	
SPEAG	Data Acquisition Electronics	DAE3	577	Nov. 11, 2005	Nov. 11, 2006	
SPEAG	Device Holder	N/A	N/A	NCR	NCR	
SPEAG	Phantom	QD 000 P40 C	TP-1150	NCR	NCR	
SPEAG	Robot	Staubli RX90BL	F03/5W15A1/A/01	NCR	NCR	
SPEAG	Software	DASY4 V4.6 Build 23	N/A	NCR	NCR	
SPEAG	Software	SEMCAD V1.8 Build 161	N/A	NCR	NCR	
SPEAG	Measurement Server	SE UMS 001 BA	1021	NCR	NCR	
Agilent	S-Parameter Network Analyzer (PNA)	E8358A	US40260131	Sep. 16, 2005	Sep. 16, 2006	
Agilent	Dielectric Probe Kit	85070D	US01440205	NCR	NCR	
Agilent	Dual Directional Coupler	778D	50422	NCR	NCR	
Agilent	Power Amplifier	8449B	3008A01917	NCR	NCR	
R&S	Radio Communication Tester	CMU200	105934	Aug. 24, 2004	Aug. 24, 2006	
Agilent	Power Meter	E4416A	GB41292344	Jan. 23, 2006	Jan. 23, 2008	
Agilent	Power Sensor	E9327A	US40441548	Feb. 6, 2006	Feb. 6, 2007	
Agilent	Signal Generator	E8247C	MY43320596	Mar. 1, 2006	Mar. 1, 2008	

Table 5.1 Test Equipment List



6. Tissue Simulating Liquids

For the measurement of the field distribution inside the SAM phantom with DASY4, the phantom must be filled with around 25 liters of homogeneous tissue simulating liquid. The liquid height from the ear reference point (ERP) of the phantom to the liquid top surface is (head SAR)or from the flat phantom to the liquid top surface (body SAR) is 15.2cm.

The following ingredients for tissue simulating liquid are used:

- **Water**: deionized water (pure H_20), resistivity 16M as basis for the liquid
- **Sugar**: refined sugar in crystals, as available in food shops to reduce relative permittivity
- Salt: pure NaCl to increase conductivity
- Cellulose: Hydroxyethyl-cellulose, medium viscosity (75-125 mPa.s, 2% in water, 20°C), CAS#54290-to increase viscosity and to keep sugar in solution.
- Preservative: Preventol D-7 Bayer AG, D-51368 Leverkusen, CAS#55965-84-9- to prevent the spread of bacteria and molds.
- DGMBE: Deithlenglycol-monobuthyl ether (DGMBE), Fluka Chemie GmbH, CAS#112-34-5 to reduce relative permittivity.

Table 6.1 gives the recipes for one liter of head and body tissue simulating liquid for frequency band 1900 MHz.

Ingredient	HSL-1900	MSL-1900
Water	552.42 g	716.56 g
Cellulose	0 g	0 g
Salt	3.06 g	4.0 g
Preventol D-7	0 g	0 g
Sugar	0 g	0 g
DGMBE	444.52 g	300.67 g
Total amount	1 liter (1.0 kg)	1 liter (1.0 kg)
Dielectric Parameters at 22°	f= 1900 MHz	f= 1900 MHz
	$_{\rm r}$ = 40.0±5%, = 1.4±5% S/m	$_{\rm r}$ = 53.3±5 %, = 1.52±5% S/m
	Π-1-1- (1	

Table 6.1

The dielectric parameters of the liquids were verified prior to the SAR evaluation using an Agilent 85070D Dielectric Probe Kit and an Agilent E8358A Network Analyzer.

	Bands	Frequency(MHz)	Permittivity (r)	Conductivity ()	Measurement Date
	PCS band	1850.2	41.6	1.43	
Head	(1850 ~ 1910	1880.0	41.5	1.45	Aug. 08, 2006
	MHz)	1909.8	41.1	1.46	
	PCS band	1850.2	52.0	1.49	
Body	(1850 ~ 1910	1880.0	51.9	1.52	Aug. 08, 2006
	MHz)	1909.8	51.9	1.55	
			Table 6.2		

Table 6.2 shows the measuring results for head and muscle simulating liquid.

The measuring data are consistent with $r = 40.0 \pm 5\%$ and $= 1.4 \pm 5\%$ for head PCS band and $r = 53.3 \pm 5\%$ and $= 1.52 \pm 5\%$ for body PCS band.



7. Uncertainty Assessment

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table 6.1

Uncertainty Distributions	Normal	Rectangular	Triangular	U-shape
Multiplying factor ^(a)	$_{1/k}$ (b)	1/ 3	1/ 6	1/ 2

(a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity
 (b) is the coverage factor

Table 7.1

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY4 uncertainty Budget is showed in Table 7.2.



Error Description	Uncertainty Value ± %	Probability Distribution	Divisor	Ci Ig	Standard Unc. (1-g)	Vi or Veff
Measurement System				II		
Probe Calibration	± 4.8	Normal	1	1	±4.8	
Axial Isotropy	± 4.7	Rectangular	$\sqrt{3}$	$(1-Cp)^{1/2}$	±1.9	
Hemispherical Isotropy	± 9.6	Rectangular	$\sqrt{3}$	$(Cp)^{1/2}$	±3.9	
Boundary Effect	± 1.0	Rectangular	$\sqrt{3}$	1	±0.6	
Linearity	± 4.7	Rectangular	$\sqrt{3}$	1	±2.7	
System Detection Limit	± 1.0	Rectangular	$\sqrt{3}$	1	±0.6	
Readout Electronics	± 1.0	Rectangular	1	1	±1.0	
Response Time	± 0.8	Normal	$\sqrt{3}$	1	± 0.5	
Integration time	±2.6	Rectangular	$\sqrt{3}$	1	±1.5	
RF Ambient Conditions	± 3.0	Rectangular	$\sqrt{3}$	1	±1.7	
Probe Positioner Mech. Tolerance	± 0.4	Rectangular	$\sqrt{3}$	1	±0.2	
Probe Positioning with respect to Phantom Shell	± 2.9	Rectangular	$\sqrt{3}$	1	±1.7	
Extrapolation and Interpolation Algorithms for Max. SAR Evaluation	± 1.0	Rectangular	$\sqrt{3}$	1	±0.6	
Test sample Related						
Test sample Positioning	±2.9	Normal	1	1	±2.9	145
Device Holder Uncertainty	±3.6	Normal	1	1	±3.6	5
Output Power Variation-SAR drift measurement	±2.5	Rectangular	$\sqrt{3}$	1	±1.4	
Phantom and Tissue						
parameters						
Phantom uncertainty(Including shar and thickness tolerances)	±4.0	Rectangular	$\sqrt{3}$	1	±2.3	
Liquid Conductivity Target tolerance	±5.0	Rectangular	$\sqrt{3}$	0.64	±1.8	
Liquid Conductivity measurement uncertainty	±2.5	Normal	1	0.64	±1.6	
Liquid Permittivity Target tolerance	±5.0	Rectangular	$\sqrt{3}$	0.6	±1.7	
Liquid Permittivity measurement uncertainty	±2.0	Normal	1	0.6	±1.2	
Combined standard uncertainty					±10.3	330
Coverage Factor for 95 %		K=2				
Expanded uncertainty (Coverage factor = 2)					±20.6	

Table 7.2 Uncertainty Budget of DASY

©2006 SPORTON International Inc. SAR Testing Lab This report shall not be reproduced except in full, without the written approval of Sporton.



8. SAR Measurement Evaluation

Each DASY system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

8.1 Purpose of System Performance check

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

8.2 System Setup

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave which comes from a signal generator at frequency 1900 MHz. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

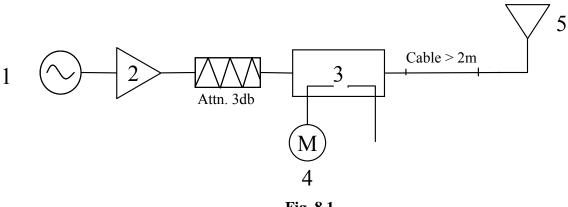


Fig. 8.1



- 1. Signal Generator
- Amplifier
 Directional Coupler
- 4. Power Meter
- 5. 1900 MHz Dipole

The output power on dipole port must be calibrated to 20dBm (100mW) before dipole is connected.



Fig 8.2 Dipole Setup

Page 24 of 35 Rev. 04



8.3 Validation Results

Comparing to the original SAR value provided by Speag, the validation data should be within its specification of 10 %. Table 8.1 shows the target SAR and measured SAR after normalized to 1W input power.

		Target (W/kg)	Measurement data (W/kg)	Variation	Measurement Date
PCS band (1900MHz) for head	SAR (1g)	38.4	39.5	2.9 %	Aug. 08, 2006
	SAR (10g)	20.5	21.2	3.4 %	Aug. 08, 2006
PCS band (1900MHz) for body	SAR (1g)	41.1	40.5	-1.5 %	Aug. 08, 2006
	SAR (10g)	21.8	21.5	-1.4 %	Aug. 08, 2006

Table 8.1

The table above indicates the system performance check can meet the variation criterion.



9. Description for DUT Testing Position

This DUT was tested in 6 different positions. They are left cheek, left tilted, right cheek, right tilted, body worn with keypad up and body worn with keypad down as illustrated below:

- 1) "Cheek Position"
 - i) To position the device with the vertical center line of the body of the device and the horizontal line crossing the center piece in a plane parallel to the sagittal plane of the phantom. While maintaining the device in this plane, align the vertical center line with the reference plane containing the three ear and mouth reference point (M, RE and LE) and align the center of the ear piece with the line RE-LE.
 - ii) To move the device towards the phantom with the ear piece aligned with the line LE-RE until the phone touched the ear. While maintaining the device in the reference plane and maintaining the phone contact with the ear, move the bottom of the phone until any point on the front side is in contact with the cheek of the phantom or until contact with the ear is lost (see Fig. 9.1).

2) "Tilted Position"

- i) To position the device in the "cheek" position described above.
- ii) While maintaining the device the reference plane described above and pivoting against the ear, move it outward away from the mouth by an angle of 15 degrees or until contact with the ear is lost (see Fig. 9.2).

3) "Body Worn"

- i) To position the device parallel to the phantom surface with either keypad up or down.
- ii) To adjust the phone parallel to the flat phantom.
- iii) To adjust the distance between the phone top/bottom surface and the flat phantom to 1.5 cm.



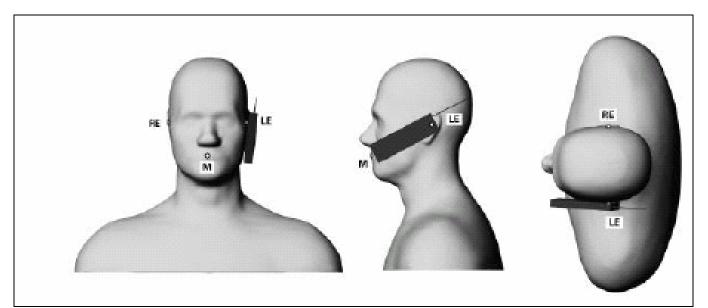


Fig. 9.1 Phone Position 1, "Cheek" or "Touch" Position. The reference points for the right ear (RE), left ear (LE) and mouth (M), which define the plane for phone positioning, are indicated.

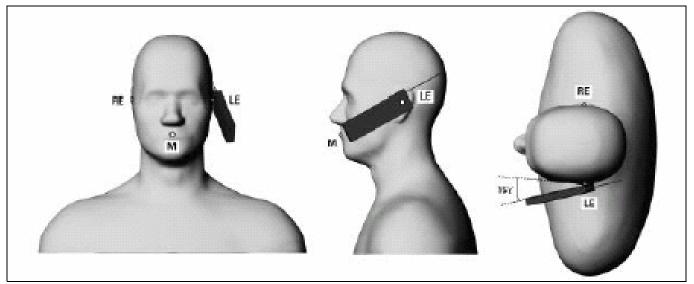


Fig. 9.2 Phone Position 2, "Tilted Position". The reference point for the right ear (RE), left ear (LE) and mouth (M), which define the plane for phone positioning, are indicated.



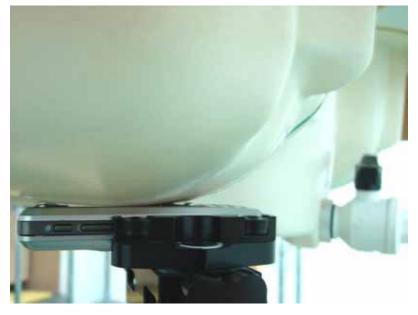


Fig. 9.3 Right Cheek

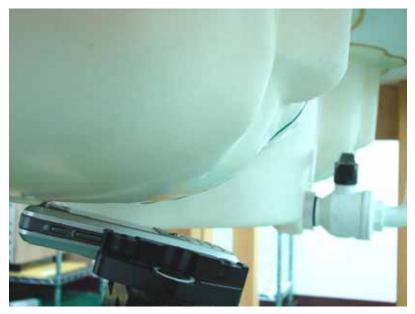


Fig. 9.4 Right Tilted



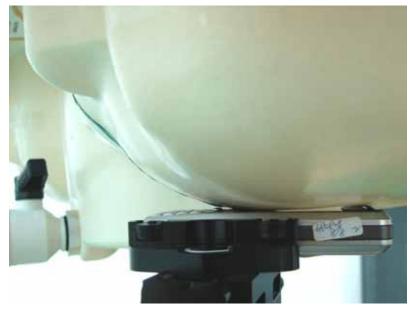


Fig. 9.5 Left Cheek



Fig. 9.6 Left Tilted



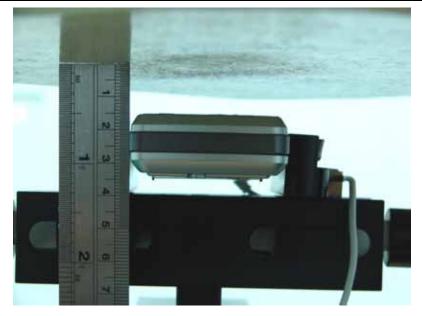


Fig. 9.7 Keypad Up with 1.5cm Gap

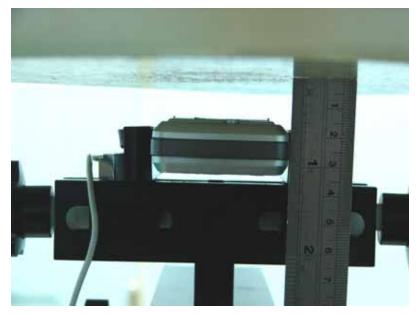


Fig. 9.8 Keypad Down with 1.5cm Gap

10. Measurement Procedures

The measurement procedures are as follows:

- Linking DUT with base station emulator CMU200 in middle channel for PCS band
- Setting PCL=0 for PCS on CMU200 to allow DUT to radiate maximum output power
- Measuring output power through RF cable and power meter
- Placing the DUT in the positions described in the last section
- Setting scan area, grid size and other setting on the DASY4 software
- > Taking data for the lowest, middle, and highest channel on each testing position

According to the IEEE P1528 draft standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- Power reference measurement
- Area scan
- Zoom scan
- Power reference measurement

10.1 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1528-2003 standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY4 software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

Base on the Draft: SCC-34, SC-2, WG-2-Computational Dosimetry, IEEE P1528/D1.2 (Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques), a new algorithm has been implemented. The spatial-peak SAR can be computed over any required mass.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.

The entire evaluation of the spatial peak values is performed within the postprocessing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:



- extraction of the measured data (grid and values) from the Zoom Scan
- calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- generation of a high-resolution mesh within the measured volume
- interpolation of all measured values form the measurement grid to the high-resolution grid
- extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- calculation of the averaged SAR within masses of 1g and 10g

10.2 Scan Procedures

First **Area Scan** is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an **Area Scan** is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, **Zoom Scan** is required. The **Zoom Scan** measures 5x5x7 points with step size 8, 8 and 5 mm. The **Zoom Scan** is performed around the highest E-field value to determine the averaged SAR-distribution over 1 g.

10.3 SAR Averaged Methods

In DASY4, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.



11. SAR Test Results

11.1 Right Cheek

Mode	Chan.	Freq. (MHz)		Conducted Power (dBm)		Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
	512 (Low)	1850.2	GMSK	29.56	-	-	-	-
PCS	661(Mid)	1880.0	GMSK	29.51	-0.008	0.343	1.6	Pass
	810 (High)	1909.8	GMSK	29.63	-	-	-	-

11.2 Right Tilted

Mode	Chan.	Freq. (MHz)		Conducted Power (dBm)		Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
	512 (Low)	1850.2	GMSK	29.56	-	-	-	-
PCS	661(Mid)	1880.0	GMSK	29.51	-0.052	0.533	1.6	Pass
	810 (High)	1909.8	GMSK	29.63	-	-	-	-

11.3 Left Cheek

Mode	Chan.	Freq. (MHz)		Conducted Power (dBm)		Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
	512 (Low)	1850.2	GMSK	29.56	-	-	-	-
PCS	661(Mid)	1880.0	GMSK	29.51	0.019	0.466	1.6	Pass
	810 (High)	1909.8	GMSK	29.63	-	-	-	-

11.4 Left Tilted

Mode	Chan.	Freq. (MHz)		Conducted Power (dBm)		Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
	512 (Low)	1850.2	GMSK	29.56	-0.017	0.551	1.6	Pass
PCS	661(Mid)	1880.0	GMSK	29.51	-0.011	0.64	1.6	Pass
	810 (High)	1909.8	GMSK	29.63	-0.029	0.722	1.6	Pass
PCS with BT On	810 (High)	1909.8	GMSK	29.63	-0.048	0.714	1.6	Pass

©2006 SPORTON International Inc. SAR Testing Lab

This report shall not be reproduced except in full, without the written approval of Sporton.



11.5 Keypad Up with 1.5 cm Gap

Mode	Chan.	Freq. (MHz)		Conducted Power (dBm)		Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
	512 (Low)	1850.2	GMSK	29.56	-	-	-	-
PCS	661(Mid)	1880.0	GMSK	29.51	-0.135	0.278	1.6	Pass
	810 (High)	1909.8	GMSK	29.63	-	-	-	-

11.6 Keypad Down with 1.5 cm Gap

Mode	Chan.	Freq. (MHz)	Modulation type	Conducted Power (dBm)		Measured 1g SAR (W/kg)	Limits (W/Kg)	Results
	512 (Low)	1850.2	GMSK	29.56	-0.109	0.724	1.6	Pass
PCS	661(Mid)	1880.0	GMSK	29.51	-0.106	0.752	1.6	Pass
	810 (High)	1909.8	GMSK	29.63	-0.069	0.72	1.6	Pass
PCS with BT On	661(Mid)	1880.0	GMSK	29.51	-0.007	0.766	1.6	Pass

Test Engineer : John Tsai



12. References

- [1] FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2] IEEE Std. P1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", April 21, 2003
- [3] Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 97-01), "Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to RF Emissions", June 2001
- [4] IEEE Std. C95.3-2002, "IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields-RF and Microwave", 2002
- [5] IEEE Std. C95.1-1999, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", 1999
- [6] Robert J. Renka, "Multivariate Interpolation Of Large Sets Of Scattered Data", University of Noth Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988, pp. 139-148
- [7] DAYS4 System Handbook



Appendix A - System Performance Check Data

Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/8/2006 8:11:24 PM

System Check_Head_1900MHz_20060808

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041

Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: HSL_1900 Medium parameters used: f = 1900 MHz; σ = 1.46 mho/m; ϵ_r = 41.2; ρ = 1000 kg/m³ Ambient Temperature : 22.6 °C; Liquid Temperature : 21.0 °C


DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(5.26, 5.26, 5.26); Calibrated: 5/31/2006

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 4.55 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 59.0 V/m; Power Drift = 0.018 dB Peak SAR (extrapolated) = 6.57 W/kg SAR(1 g) = 3.95 mW/g; SAR(10 g) = 2.12 mW/g Maximum value of SAR (measured) = 4.49 mW/g

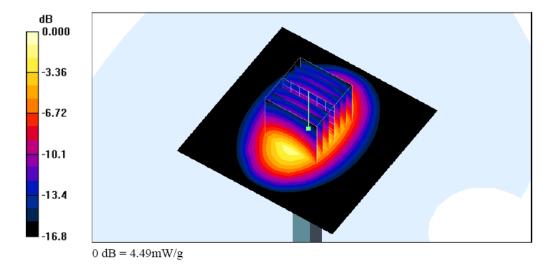



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/8/2006 11:21:54 PM

System Check_Body_1900MHz_20060808

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1 Medium: MSL_1900 Medium parameters used: f = 1900 MHz; $\sigma = 1.54 \text{ mho/m}$; $\varepsilon_r = 51.9$; $\rho = 1000 \text{ kg/m}^3$ Ambient Temperature : 22.4 °C; Liquid Temperature : 21.0 °C

DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(4.66, 4.66, 4.66); Calibrated: 5/31/2006

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)Sensor-Surface: 4mm (Mechanical Surface Detection)


- Electronics: DAE3 Sn577; Calibrated: 11/11/2005

- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383

- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 4.75 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 52.2 V/m; Power Drift = -0.010 dB Peak SAR (extrapolated) = 6.92 W/kg SAR(1 g) = 4.05 mW/g; SAR(10 g) = 2.15 mW/g Maximum value of SAR (measured) = 4.61 mW/g

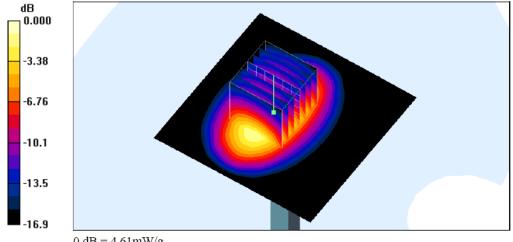

 $0 \, dB = 4.61 \, mW/g$



Appendix B - SAR Measurement Data

Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/8/2006 11:55:47 PM

Right Cheek_PCS Ch661_20060808

DUT: 680808; Type: Mobile Phone

Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:8.3 Medium: HSL_1900 Medium parameters used: f = 1880 MHz; $\sigma = 1.45$ mho/m; $\epsilon_r = 41.5$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.7 °C; Liquid Temperature : 21.0 °C


DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(5.26, 5.26, 5.26); Calibrated: 5/31/2006

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch661/Area Scan (41x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.395 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 15.3 V/m; Power Drift = -0.008 dB Peak SAR (extrapolated) = 0.543 W/kg SAR(1 g) = 0.343 mW/g; SAR(10 g) = 0.210 mW/g Maximum value of SAR (measured) = 0.372 mW/g

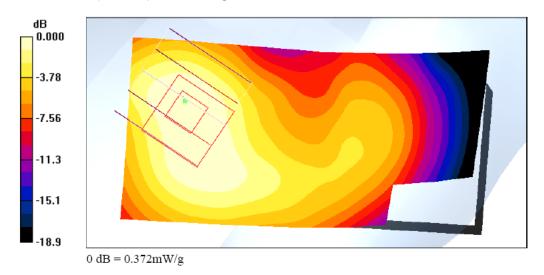



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/9/2006 12:15:16 AM

Right Tilted_PCS Ch661_20060808

DUT: 680808; Type: Mobile Phone


Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:8.3 Medium: HSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.45 mho/m; ϵ_r = 41.5; ρ = 1000 kg/m³ Ambient Temperature : 22.7 °C; Liquid Temperature : 21.0 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.26, 5.26, 5.26); Calibrated: 5/31/2006
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch661/Area Scan (41x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.618 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 19.9 V/m; Power Drift = -0.052 dB Peak SAR (extrapolated) = 0.884 W/kg SAR(1 g) = 0.533 mW/g; SAR(10 g) = 0.296 mW/g Maximum value of SAR (measured) = 0.584 mW/g

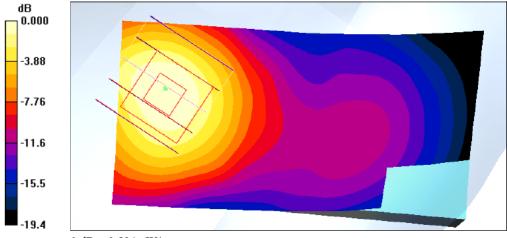

 $0 \, dB = 0.584 mW/g$



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/9/2006 12:30:17 AM

Left Cheek_PCS Ch661_20060808

DUT: 680808; Type: Mobile Phone


Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:8.3 Medium: HSL_1900 Medium parameters used: f = 1880 MHz; $\sigma = 1.45$ mho/m; $\epsilon_r = 41.5$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.4 °C; Liquid Temperature : 21.0 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.26, 5.26, 5.26); Calibrated: 5/31/2006
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch661/Area Scan (41x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.515 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 15.4 V/m; Power Drift = 0.019 dB Peak SAR (extrapolated) = 0.813 W/kg SAR(1 g) = 0.466 mW/g; SAR(10 g) = 0.249 mW/g Maximum value of SAR (measured) = 0.495 mW/g

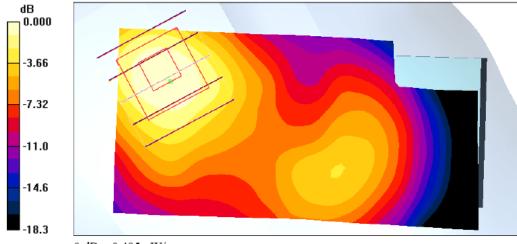

0 dB = 0.495 mW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/9/2006 1:17:27 AM

Left Tilted_PCS Ch810_20060808

DUT: 680808; Type: Mobile Phone

Communication System: PCS; Frequency: 1909.8 MHz;Duty Cycle: 1:8.3 Medium: HSL_1900 Medium parameters used: f = 1910 MHz; σ = 1.46 mho/m; ϵ_r = 41.1; ρ = 1000 kg/m³ Ambient Temperature : 22.6 °C; Liquid Temperature : 21.0 °C

DASY4 Configuration:


- Probe: ET3DV6 - SN1787; ConvF(5.26, 5.26, 5.26); Calibrated: 5/31/2006

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch810/Area Scan (41x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.819 mW/g

Ch810/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 20.5 V/m; Power Drift = -0.029 dB Peak SAR (extrapolated) = 1.30 W/kg SAR(1 g) = 0.722 mW/g; SAR(10 g) = 0.377 mW/g Maximum value of SAR (measured) = 0.808 mW/g

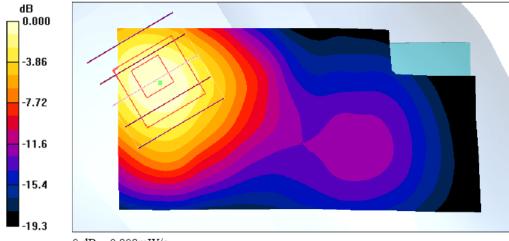

0 dB = 0.808 mW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/9/2006 1:30:08 AM

Left Tilted_PCS Ch810_20060808_Bluetooth On

DUT: 680808; Type: Mobile Phone


Communication System: PCS; Frequency: 1909.8 MHz;Duty Cycle: 1:8.3 Medium: HSL_1900 Medium parameters used: f = 1910 MHz; σ = 1.46 mho/m; ϵ_r = 41.1; ρ = 1000 kg/m³ Ambient Temperature : 22.4 °C; Liquid Temperature : 21.0 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.26, 5.26, 5.26); Calibrated: 5/31/2006
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch810/Area Scan (41x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.823 mW/g

 $\label{eq:charge} \begin{array}{l} \textbf{Ch810/Zoom Scan (5x5x7)/Cube 0:} \ \text{Measurement grid: dx=8mm, dy=8mm, dz=5mm} \\ \text{Reference Value = 20.4 V/m; Power Drift = -0.048 dB} \\ \text{Peak SAR (extrapolated) = 1.27 W/kg} \\ \textbf{SAR(1 g) = 0.714 mW/g; SAR(10 g) = 0.373 mW/g} \\ \text{Maximum value of SAR (measured) = 0.808 mW/g} \end{array}$

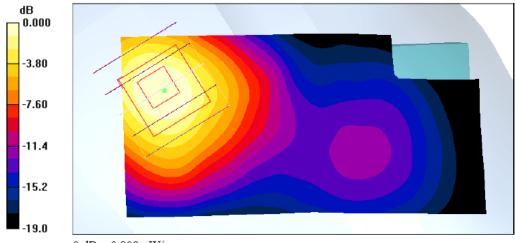

0 dB = 0.808 mW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/9/2006 2:01:02 AM

Body_PCS Ch661_Keypad Up with 1.5cm Gap_20060809

DUT: 680808; Type: Mobile Phone

Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:4

Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.52 mho/m; ε_r = 51.9; ρ = 1000 kg/m³ Ambient Temperature : 22.5 °C; Liquid Temperature : 20.8 °C


DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(4.66, 4.66, 4.66); Calibrated: 5/31/2006

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch661/Area Scan (41x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.311 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 14.5 V/m; Power Drift = -0.135 dB Peak SAR (extrapolated) = 0.419 W/kg SAR(1 g) = 0.278 mW/g; SAR(10 g) = 0.175 mW/g Maximum value of SAR (measured) = 0.300 mW/g

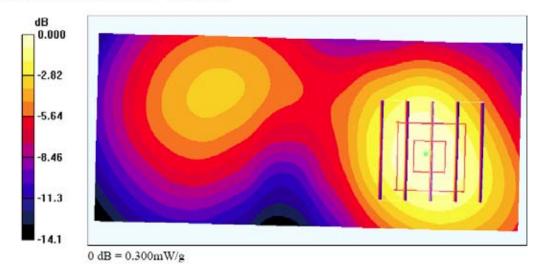



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/9/2006 2:21:09 AM

Body_PCS Ch661_Keypad Down with 1.5cm Gap_20060809

DUT: 680808; Type: Mobile Phone

Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:4 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.52 mho/m; ε_r = 51.9; ρ = 1000 kg/m³ Ambient Temperature : 22.3 °C; Liquid Temperature : 20.8 °C


DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(4.66, 4.66, 4.66); Calibrated: 5/31/2006

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch661/Area Scan (41x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.835 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 23.3 V/m; Power Drift = -0.106 dB Peak SAR (extrapolated) = 1.21 W/kg SAR(1 g) = 0.752 mW/g; SAR(10 g) = 0.447 mW/g Maximum value of SAR (measured) = 0.815 mW/g

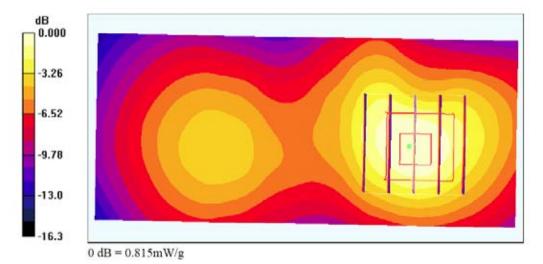



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/9/2006 3:07:28 AM

Body_PCS Ch661_Keypad Down with 1.5cm Gap_20060809_Bluetooth On

DUT: 680808; Type: Mobile Phone

Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:4


Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.52 mho/m; ε_r = 51.9; ρ = 1000 kg/m³ Ambient Temperature : 22.4 °C; Liquid Temperature : 20.8 °C

DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.66, 4.66, 4.66); Calibrated: 5/31/2006
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch661/Area Scan (41x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.840 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 23.1 V/m; Power Drift = -0.007 dB Peak SAR (extrapolated) = 1.24 W/kg SAR(1 g) = 0.766 mW/g; SAR(10 g) = 0.458 mW/g Maximum value of SAR (measured) = 0.826 mW/g

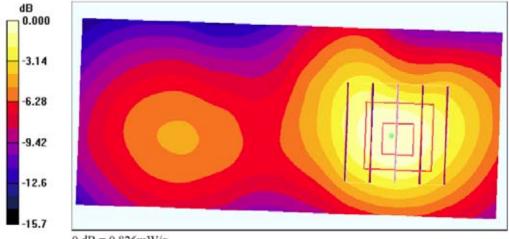

0 dB = 0.826 mW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/9/2006 1:17:27 AM

Left Tilted_PCS Ch810_20060808_2D

DUT: 680808; Type: Mobile Phone

Communication System: PCS; Frequency: 1909.8 MHz;Duty Cycle: 1:8.3 Medium: HSL_1900 Medium parameters used: f = 1910 MHz; $\sigma = 1.46$ mho/m; $\epsilon_r = 41.1$; $\rho = 1000$ kg/m³ Ambient Temperature : 22.6 °C; Liquid Temperature : 21.0 °C

DASY4 Configuration:


- Probe: ET3DV6 - SN1787; ConvF(5.26, 5.26, 5.26); Calibrated: 5/31/2006

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch810/Area Scan (41x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.819 mW/g

Ch810/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 20.5 V/m; Power Drift = -0.029 dB Peak SAR (extrapolated) = 1.30 W/kg SAR(1 g) = 0.722 mW/g; SAR(10 g) = 0.377 mW/g

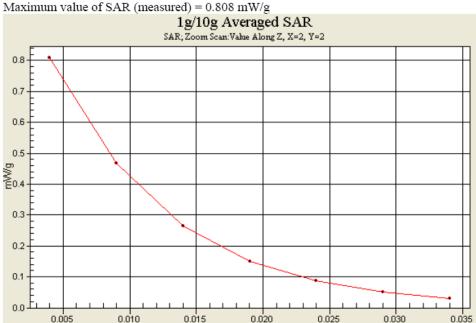

m



Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 8/9/2006 3:07:28 AM

Body_PCS Ch661_Keypad Down with 1.5cm Gap_20060809_Bluetooth On_2D

DUT: 680808; Type: Mobile Phone

Communication System: PCS; Frequency: 1880 MHz;Duty Cycle: 1:4

Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.52 mho/m; ε_r = 51.9; ρ = 1000 kg/m³ Ambient Temperature : 22.4 °C; Liquid Temperature : 20.8 °C

DASY4 Configuration:

- Probe: ET3DV6 - SN1787; ConvF(4.66, 4.66, 4.66); Calibrated: 5/31/2006

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch661/Area Scan (41x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.840 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 23.1 V/m; Power Drift = -0.007 dB Peak SAR (extrapolated) = 1.24 W/kg SAR(1 g) = 0.766 mW/g; SAR(10 g) = 0.458 mW/g Maximum value of SAR (measured) = 0.826 mW/g





Appendix C – Calibration Data

chmid & Partner Engineering AG ughausstrasse 43, 8004 Zuric	ry of		chweizerischer Kalibrierdienst ervice suisse d'étalonnage arvizio svizzero di taratura wiss Calibration Service
ccredited by the Swiss Federal (he Swiss Accreditation Servic) ultilateral Agreement for the r	e is one of the signatorie	es to the EA	a SCS 108
lient Sporton (Aude			1900V2-5d041_Mar06
CALIBRATION C	CERTIFICATE		
Dbject	D1900V2 - SN: 5	d041	
Calibration procedure(s)	QA CAL-05.v6 Calibration proce	dure for dipole validation kits	
Calibration date:	March 21, 2006		
Condition of the calibrated item	In Tolerance		
The measurements and the unce	ertainties with confidence p	ional standards, which realize the physical units o robability are given on the following pages and arr ry facility: environment temperature (22 ± 3)°C and	e part of the certificate.
ihe measurements and the unce II calibrations have been conduct Calibration Equipment used (M&)	artainties with confidence p Inter the closed laborator TE critical for calibration)	robability are given on the following pages and an ry facility: environment temperature (22 \pm 3)°C and	e part of the certificate. d humidity < 70%.
he measurements and the unce Il calibrations have been conduc calibration Equipment used (M& rimary Standards	ertainties with confidence pro- incted in the closed laborator TE critical for calibration)	robability are given on the following pages and are ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.)	e part of the cartificate. d humidity < 70%. Scheduled Calibration
he measurements and the unce alibrations have been conduct alibration Equipment used (M& rimary Standards ower meter EPM-442A	artainties with confidence p Inter the closed laborator TE critical for calibration)	robability are given on the following pages and are ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-06
he measurements and the unce II calibrations have been conduct alibration Equipment used (M& rimary Standards ower meter EPM-442A ower sensor HP 8481A	ertainties with confidence pro- incted in the closed laborator TE critical for calibration) ID # GB37480704	robability are given on the following pages and are ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.)	e part of the cartificate. d humidity < 70%. Scheduled Calibration
The measurements and the unce all calibrations have been conduct calibration Equipment used (M&) rimary Standards tower meter EPM-442A tower sensor HP 8481A teference 20 dB Attenuator	ertainties with confidence pro- icted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783	robability are given on the following pages and are ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516)	e part of the cartificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06
he measurements and the unce alibration Equipment used (M& rimary Standards lower meter EPM-442A lower sensor HP 8481A teference 20 dB Attenuator teference 10 dB Attenuator teference Probe ET3DV6	ertainties with confidence pro- icted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g)	robability are given on the following pages and are ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498)	e part of the cartificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06
he measurements and the unce alibration Equipment used (M& rimary Standards ower meter EPM-442A ower sensor HP 8481A leference 20 dB Attenuator leference 10 dB Attenuator leference Probe ET3DV6	ertainties with confidence print incred in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r)	robability are given on the following pages and are ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06
the measurements and the unce alibration Equipment used (M& calibration Equipment used (M& ca	ertainties with confidence provide the confidence provided in the closed laborator (TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507	robability are given on the following pages and are ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No. 251-00498) 11-Aug-05 (METAS, No. 251-00498) 28-Oct-05 (SPEAG, No. 273-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06
The measurements and the unce NI calibration Equipment used (M& Primary Standards Prover meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4 Becondary Standards	artainties with confidence pro- icted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 507 SN: 601	robability are given on the following pages and are ry facility: environment temperature (22 ± 3)°C and O4-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No. 251-00498) 11-Aug-05 (METAS, No. 251-00498) 11-Aug-05 (METAS, No. 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DE3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Prower meter EPM-442A Prower sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 PAE4 Recondary Standards Prower sensor HP 8481A	artainties with confidence pro- icted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 507 SN: 601 ID #	robability are given on the following pages and are ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No. 251-00498) 11-Aug-05 (METAS, No. 251-00498) 28-Oct-05 (SPEAG, No. 273-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06
he measurements and the unce all calibrations have been conduct calibration Equipment used (M& rimary Standards fower meter EPM-442A lower sensor HP 8481A teference 20 dB Attenuator teference 10 dB Attenuator teference Probe ET3DV6 tAE4 lecondary Standards fower sensor HP 8481A te generator Agilent E4421B	ertainties with confidence pr incted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 507 SN: 601 ID # MY41092317	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and O4-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No. 251-00498) 11-Aug-05 (METAS, No. 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05)	e part of the cartificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Oct-07
he measurements and the unce all calibrations have been conduct calibration Equipment used (M& rimary Standards fower meter EPM-442A lower sensor HP 8481A teference 20 dB Attenuator teference 10 dB Attenuator teference Probe ET3DV6 tAE4 lecondary Standards fower sensor HP 8481A te generator Agilent E4421B	artainties with confidence print inteed in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 601 ID # MY41092317 MY41000675	robability are given on the following pages and are ry facility: environment temperature (22 ± 3)°C and 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05)	e part of the cartificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Oct-06 Dec-06 Scheduled Check In house check: Nov-07
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Prover meter EPM-442A Prover sensor HP 8481A Reference 20 dB Attenuator Reference Probe ET3DV6 PAE4 Prover sensor HP 8481A Regenerator Agilent E4421B	ertainties with confidence pro- incted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 5067 SN: 601 ID # MY41092317 MY41002675 US37390585 S4206	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-0048) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	e part of the cartificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Nov-07 In house check: Nov-06
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Prower meter EPM-442A Prower sensor HP 8481A Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ET3DV6 JAE4 Prower sensor HP 8481A Regenerator Agilent E4421B Retwork Analyzer HP 8753E	ertainties with confidence pr incted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 601 ID # MY41092317 MY4100675 US37390585 S4206 Name	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00496) 11-Aug-05 (METAS, No 251-00496) 11-Aug-05 (METAS, No 251-00496) 11-Aug-05 (METAS, No 251-00496) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	e part of the cartificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Nov-07 In house check: Nov-06 Signature
The measurements and the unce VII calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8461A Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Drobe ET3DV6 DAE4 Becondary Standards Power sensor HP 8461A RF generator Agilent E4421B Vetwork Analyzer HP 8753E	ertainties with confidence pro- incted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 5067 SN: 601 ID # MY41092317 MY41002675 US37390585 S4206	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-0048) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	e part of the cartificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Nov-07 In house check: Nov-06 Signature MMMMMM
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ET3DV6 DAE4 Becondary Standards Power sensor HP 8481A Reference Analyzer HP 8753E Calibrated by:	ertainties with confidence pr incted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 601 ID # MY41092317 MY4100675 US37390585 S4206 Name	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00496) 11-Aug-05 (METAS, No 251-00496) 11-Aug-05 (METAS, No 251-00496) 11-Aug-05 (METAS, No 251-00496) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	e part of the cartificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Nov-07 In house check: Nov-06 Signature
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 6481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference 10 dB Attenuator Reference 10 dB Attenuator Bater DAE4 Secondary Standards Power sensor HP 6481A RF generator Agilent E4421B Network Analyzer HP 8753E - Calibrated by: Approved by:	ertainties with confidence pro- cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 5047.2 (10r) SN: 601 ID # MY41092317 MY41000675 US37390585 S4206 Name Judith Müller Katja Pokovic	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No. 251-00498) 13-Aug-05 (METAS, No. 251-00498) 28-Oct-05 (SPEAG, No. 251-00498) 28-Oct-05 (SPEAG, No. 251-00498) 18-Oct-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) Function Laboratory Technician Technical Manager	e part of the cartificate. d humidity < 70%. Scheduled Calibration Oct-06 Oct-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Nov-07 In house check: Nov-06 Signature MMMMMM
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 10 dB Attenuator Reference 10 dB Attenuator Reference 10 dB Attenuator Reference 10 dB Attenuator Reference To B Attenuator Reference T	ertainties with confidence pro- cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 5047.2 (10r) SN: 601 ID # MY41092317 MY41000675 US37390585 S4206 Name Judith Müller Katja Pokovic	robability are given on the following pages and an ry facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00498) 11-Aug-05 (METAS, No. 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Nov-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) Function Laboratory Technician	e part of the certificate: d humidity < 70%. Scheduled Calibration Oct:06 Oct:06 Aug-06 Oct:08 Dec-06 Scheduled Check In house check: Nov-07 In house check: Nov-07 Signature MMMMMM MMMMMM

©2006 SPORTON International Inc. SAR Testing Lab This report shall not be reproduced except in full, without the written approval of Sporton.



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

S

С

S

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- · SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D1900V2-5d041_Mar06

Page 2 of 9



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Area Scan resolution	dx, dy = 15 mm	12
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.4 ± 6 %	1.42 mho/m ± 6 %
Head TSL temperature during test	(21.5 ± 0.2) °C		

SAR result with Head TSL

condition	
250 mW input power	9.75 mW / g
normalized to 1W	39.0 mW / g
normalized to 1W	38.4 mW / g ± 17.0 % (k=2)
Condition	
	225-2253 139-255 C
250 mW input power	5.17 mW / g
250 mW input power normalized to 1W	5.17 mW / g 20.7 mW / g
	250 mW input power normalized to 1W normalized to 1W Condition

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D1900V2-5d041_Mar06

4

Page 3 of 9

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.7 ± 6 %	1.54 mho/m ± 6 %
Body TSL temperature during test	(21.6 ± 0.2) °C		

a (*)

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.2 mW / g
SAR normalized	normalized to 1W	40.8 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	41.1 mW / g ± 17.0 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
	condition 250 mW input power	5.40 mW / g
SAR averaged over 10 cm ³ (10 g) of Body TSL SAR measured SAR normalized		5.40 mW / g 21.6 mW / g

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D1900V2-5d041_Mar06

Page 4 of 9

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.5 Ω + 5.1 jΩ
Return Loss	- 24.8 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.9 Ω + 6.3 JΩ	
Return Loss	- 23.4 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.200 ns	÷.
----------------------------------	----------	----

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the force must be applied to the dipole arms, because they might bend or the soldered connections near the

feedpoint may be damaged.

Additional EUT Data


Manufactured by	SPEAG
Manufactured on	July 4, 2003

Certificate No: D1900V2-5d041_Mar06

Page 5 of 9


©2006 SPORTON International Inc. SAR Testing Lab



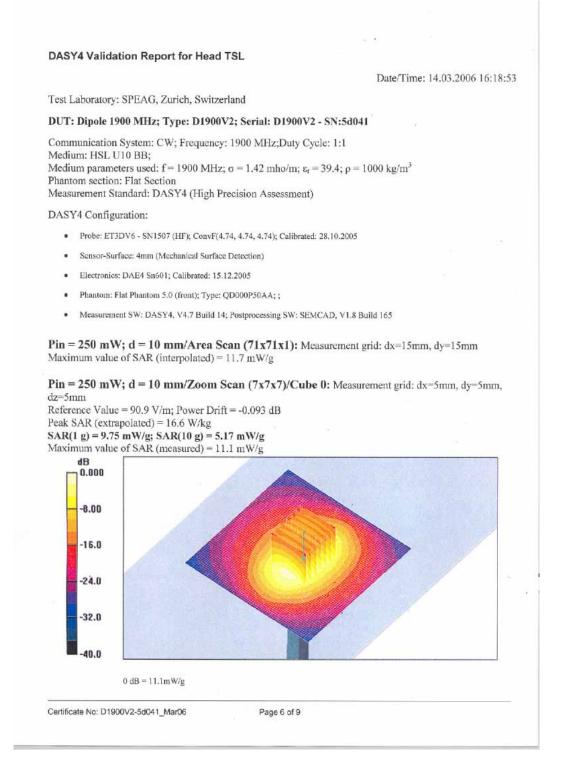

©2006 SPORTON International Inc. SAR Testing Lab



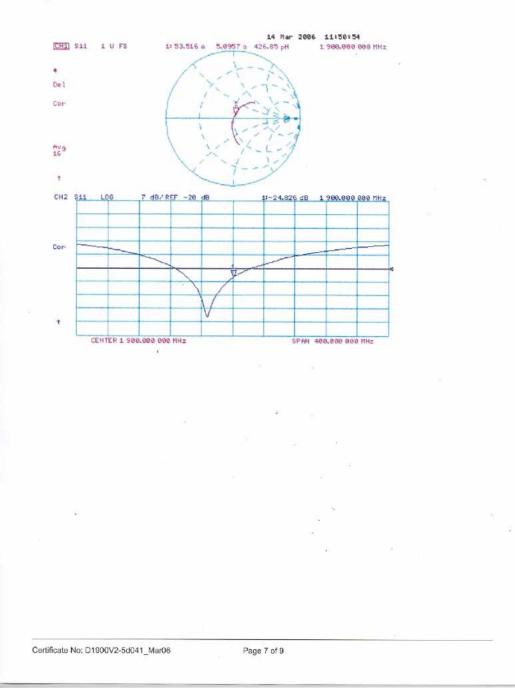

Impedance Measurement Plot for Head TSL

©2006 SPORTON International Inc. SAR Testing Lab This report shall not be reproduced except in full, without the written approval of Sporton.



DASY4 Validation Report for Body TSL

Date/Time: 21.03.2006 13:59:55

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041

Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: MSL U10; Medium parameters used: f = 1900 MHz; σ = 1.54 mho/m; ϵ_r = 54.7; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)


DASY4 Configuration:

- Probe: ET3DV6 SN1507 (HF); ConvF(4.3, 4.3, 4.3); Calibrated: 28.10.2005
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 15.12.2005
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Pin = 250 mW; d = 10 mm/Area Scan (71x71x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 11.8 mW/g

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Reference Value = 89.3 V/m; Power Drift = 0.045 dB Peak SAR (extrapolated) = 17.4 W/kg SAR(1 g) = 10.2 mW/g; SAR(10 g) = 5.4 mW/g Maximum value of SAR (measured) = 11.6 mW/g

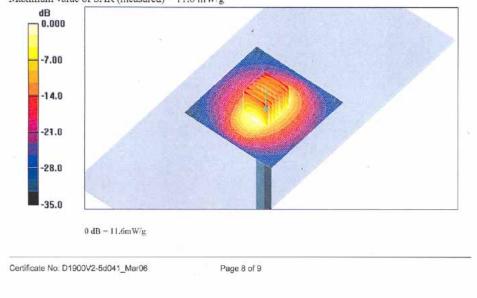

©2006 SPORTON International Inc. SAR Testing Lab





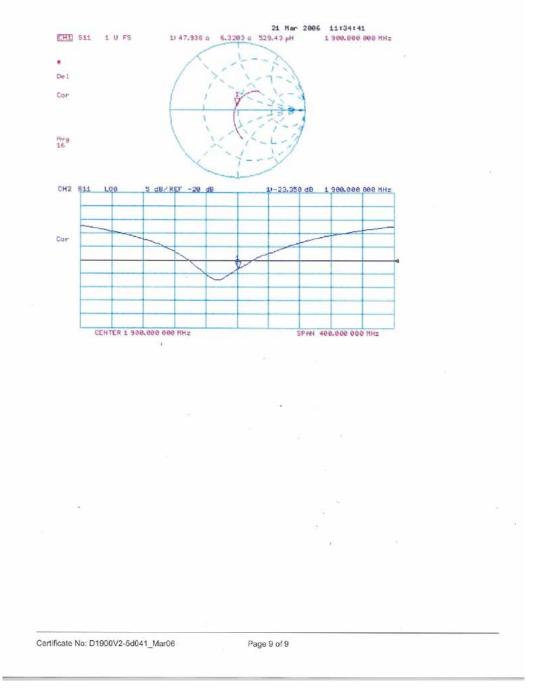

©2006 SPORTON International Inc. SAR Testing Lab



Engineering AG Reughausstrasse 43, 8004 Zuric	ry of	Nac MEA (C) Z C	chweizarischer Kalibrierdienst ervice aulase d'étalonnage ervizie svizzero di taratura wiss Calibration Service
Accredited by the Swiss Federal (The Swiss Accreditation Servic Autiliateral Agreement for the n	e is one of the signator	ies to the EA	.: SCS 108
Sporton (Aude			T3-1787_May06
CALIBRATION C	ET3DV6 - SN: 1		
Galibration procedure(s)	QA CAL-01.v5 Calibration proc	edure for dosimetric E-field probes	
Calibration data:	May 31, 2006		
Condition of the calibrated item	In Tolerance		
The measurements and the unce	intainties with confidence	ational standards, which realize the physical units o probability are given on the following pages and an lory facility: environment temperature (22 ± 3)°C an	a part of the certificate.
The measurements and the unce All calibrations have been conduc	intainties with confidence	probability are given on the following pages and an lory facility: environment temperature (22 ± 3)°C an	a part of the certificate.
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M8)	intainties with confidence	probability are given on the following pages and an lory facility: environment temperature (22 ± 3)°C an	a part of the certificate. d humidity < 70%.
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M81 Primary Standards	intainties with confidence cted in the closed laborat TEleritical for calibration)	probability are given on the following pages and an lory facility: environment temperature (22 ± 3)°C an	a part of the certificate.
The measurements and the unce All culibrations have been conduc Calibration Equipment used (M81 Primary Standards Power meter E4415B Power sensor E4412A	Interface with confidence cted in the closed laborat TE-critical for calibration) ID # GB41293674 MY41495277	probability are given on the following pages and an lony facility: environment temperature (22 ± 3)°C an Call Date (Calibrated by, Certificate No.)	a part of the certificate. d humidity < 70%. Scheduled Galibration Apr-07 Apr-07
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M8) Primary Standards Prover sensor E44198 Prover sensor E4419A Prover sensor E4419A	Interface with confidence cted in the closed laborat TE-ionitical for calibration) iD # GB41293874 MY41498067	probability are given on the following pages and an lory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 5-Apr-06 (METAS, No. 251-00557) 5-Apr-06 (METAS, No. 251-00557)	s part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M8) Primary Standards Prover sensor E4412A Prover sensor E4412A Reference 3 dB Attenuator	Interface with confidence cted in the closed laboral TE-critical for calibration) ID # GB41293674 MY41495277 MY41495067 SN: S5054 (3c)	probability are given on the following pages and an locy facility: environment temperature (22 ± 3)°C an Call Date (Calibrated by, Dertificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557)	a part of the certificate. d humidity < 70%. Scheduled Galibration Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Apr-07
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4419A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator	Interface with confidence cted in the closed laboral TE-onlicel for calibration) ID # GB41293674 MY41495277 MY41495067 SNE S5054 (3c) SNE S5056 (20b)	probability are given on the following pages and an locy facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Dertificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 11-Aug-06 (METAS, No. 251-00599) 4-Apr-06 (METAS, No. 251-00598)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Apr-06 Apr-07
The measurements and the unoc All calibrations have been conduc Calibration Equipment used (M&I Primary Sounderds Power meter E44198 Power sensor E4419A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator	Interface with confidence cted in the closed laborat TEFor lical for calibration) ID # GB41293674 MY41495277 MY41495277 MY41495277 SN: S5085 (3c) SN: S5085 (2cb) SN: S5129 (3cb)	probability are given on the following pages and an tory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Dertificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 51-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00558)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Apr-07
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M8) Primary Standards Power sensor E44198 Power sensor E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 9 nobe E530V2	Interface with confidence cted in the closed laboral TE-onlicel for calibration) ID # GB41293674 MY41495277 MY41495067 SNE S5054 (3c) SNE S5056 (20b)	probability are given on the following pages and an locy facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Dertificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 11-Aug-06 (METAS, No. 251-00599) 4-Apr-06 (METAS, No. 251-00598)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Apr-06 Apr-07
The measurements and the unoc All calibrations have been conduc Calibration Equipment used (M& Primary Standards Prover sensor E4412A Prover sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 90 dB Attenuator	Italities with confidence cted in the closed laboral TE-critical for calibration) ID # GB41293874 MY41498067 SN: S5054 (3c) SN: S5029 (30b) SN: S5129 (30b) SN: 3013	probability are given on the following pages and an locy facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00500) 2-Jan-06 (SPEAG, No. ES3-3013; Jano6)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-05 Apr-07 Aug-05 Jan-07
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M&I Calibration Equipment used (M&I Primary Standards Power sensor E44198 Power sensor E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 9 robe E530V2 DAE4 Secondary Standards	Interface with confidence cted in the closed laboral TE-critical for calibration) ID # GB41293674 MY41495067 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 654	probability are given on the following pages and an locy facility: environment temperature (22 ± 3)°C an Call Date (Calibrated by, Dertificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 2-Jan-06 (SPEAG, No. ES3-3013: Jan06) 2-Feb-06 (SPEAG, No. DAE4-654_Feb06)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Apr-07 Aug-05 Apr-07 Aug-06 Jan-07 Feb-07
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M81 Primary Standards Power sensor E44198 Power sensor E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator	Interface with confidence cted in the closed laborat TEFor lical for calibration) ID # GB41253674 MY41495277 MY41495067 SN: 55054 (3c) SN: 55086 (20b) SN: 55129 (30b) SN: 3013 SN: 654 ID #	probability are given on the following pages and an losy facility: environment temperature (22 ± 3)°C an Call Date (Calibrated by, Dertificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00508) 11-Aug-05 (METAS, No. 251-00508) 11-Aug-05 (METAS, No. 251-00508) 11-Aug-05 (METAS, No. 251-00508) 2-Jan-06 (SPEAG, No. BS3-3013_Jan06) 2-Feb-06 (SPEAG, No. DAE4-654_Feb06) Check Date (in house)	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-05 Apr-07 Aug-06 Jan-07 Feb-07 Scheduled Chock
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M&) Primary Standards Prover sensor E44198 Prover sensor E4419A Reference 3 dB Attenuator Reference 30 dB Attenuator	Intellifies with confidence cted in the closed laboral TE-critical for calibration) ID # GB41293674 MY41495067 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3542U01700 US357390585 Name	probability are given on the following pages and an losy facility: environment temperature (22 ± 3)°C an Call Date (Calibrated by, Dertificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 2-Feb-06 (SPEAG, No. DAE4-654_Feb06) Check Date (in house) 4-Aug-99 (SFEAG, in house check Nov-05) 15-Oct-01 (SPEAG, in house check Nov-05) 15-Oct-01 (SPEAG, in house check Nov-05) Function	a part of the certificate. d humidity < 70%. Scheduled Calibration Apr-07 Apr-07 Aug-05 Apr-07 Aug-05 Jan-07 Feb-07 Scheduled Check In house check: Nov-07
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M&) Primary Standards Prover sensor E44198 Prover sensor E4419A Reference 3 dB Attenuator Reference 30 dB Attenuator	Intellifies with confidence cted in the closed laboral TE-critical for calibration) ID # GB41293674 MY41495277 MY41495067 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 5514 ID # US3542U01700 US37390585	probability are given on the following pages and an locy facility: environment temperature (22 ± 3)°C an Call Date (Calibrated by, Certificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 4-Apr-06 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 2-Jan 06 (SPEAG, No. 253-0013, Jan06) 2-Feb 06 (SPEAG, No. DAE4-654_Feb06) Check Date (in house) 4-Aug-99 (SFEAG, in house check Nov-05) 16-Oct-01 (SPEAG, in house check Nov-05)	a part of the certificate. d humidity < 70%. Scheduled Galibration Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Scheduled Check In house check: Nov-07 In house check: Nov-08
The measurements and the unce All calibrations have been conduct Calibrations Equipment used (M81 Primary Standards Power sensor E4412A Power sensor E4412A Reference 30 dB Attenuator Reference 30 dB Attenuator	Intellifies with confidence cted in the closed above TE-or licel for calibration) ID # GB41293874 MY41498277 MY41498067 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 5514 ID # US35422001700 US35422001700 US37390585 Name Katja Pinkovio	probability are given on the following pages and an locy facility: environment temperature (22 ± 3)°C an Call Date (Calibrated by, Certificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-06 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 12-Bob (METAS, No. 251-00568) 13-Doc (METAS, No. 251-00568) 2-Feb-06 (SPEAG, No. DAE4-654_Feb06) Check Date (in house) 4-Aug-96 (GFEAG, in house check Nov-05) 15-Oct-01 (SPEAG, in house check Nov-05) Function Technical Manager	a part of the certificate. d humidity < 70%. Scheduled Galibration Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Scheduled Check In house check: Nov-07 In house check: Nov-08
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M&) Primary Standards Prover sensor E44198 Prover sensor E4419A Reference 3 dB Attenuator Reference 30 dB Attenuator	Intellifies with confidence cted in the closed laboral TE-critical for calibration) ID # GB41293674 MY41495067 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3542U01700 US357390585 Name	probability are given on the following pages and an losy facility: environment temperature (22 ± 3)°C an Call Date (Calibrated by, Dertificate No.) S-Apr-06 (METAS, No. 251-00557) S-Apr-06 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00557) 11-Aug-05 (METAS, No. 251-00558) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 11-Aug-05 (METAS, No. 251-00568) 2-Feb-06 (SPEAG, No. DAE4-654_Feb06) Check Date (in house) 4-Aug-99 (SFEAG, in house check Nov-05) 15-Oct-01 (SPEAG, in house check Nov-05) 15-Oct-01 (SPEAG, in house check Nov-05) Function	a part of the certificate. d humidity < 70%. Scheduled Galibration Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Apr-07 Scheduled Check In house check: Nov-07 In house check: Nov-08

Certificate No: ET3-1787_Mey06

Page 1 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstresse 43, 8004 Zurich, Switzerland



s

Ċ

S

Schweizerischer Kalibrierdienst

Service suisse d'étalonnage

Servizio svizzero di taratura

S Swiss Calibration Service

Accreding by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

 TSL
 tissue simulating liquid

 NORMx,y,z
 sensitivity in free space

 ConF
 sensitivity in TSL / NORMx,y,z

 DCP
 diode compression point

 Polarization φ
 φ rotation around probe axis

 Polarization 9
 ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., ϑ = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below *ConvF*).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This
 linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of
 the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of
 power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to *NORMx,y,z* * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1787_May06

Page 2 of 9



ET3DV6 SN:1787

May 31, 2006

Probe ET3DV6

SN:1787

Manufactured: Last calibrated: Recalibrated: May 28, 2003 August 29, 2003 May 31, 2006

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: ET3-1787_May06

Page 3 of 9

©2006 SPORTON International Inc. SAR Testing Lab This report shall not be reproduced except in full, without the written approval of Sporton.



ET3DV6 SN:1787

May 31, 2006

DASY - Parameters of Probe: ET3DV6 SN:1787

Sens	sitivity in Fi	ree Spac	e ^A		Diode	Compress	ion ^B
	NormX	1.5	7 ± 10.1%	μV/(V/m) ²	DCP X	94 mV	
	NormY	1.7	1 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	94 mV	
	NormZ	2.0	9 ± 10.1%	$\mu V/(V/m)^2$	DCP Z	94 mV	
Sens	sitivity in Ti	issue Sin	nulating Li	quid (Convers	ion Factor	s)	
Please	a see Page 8.						
Bour	ndary Effec	ot					
TSL		900 MHz	Typical S/	AR gradient: 5 % p	er mm		
	Sensor Cen	ter to Phants	om Surface D	istance	3.7 mm	4.7 mm	
	SARte [%]	Withou	t Correction A	Ugorithm	7.2	3.8	
	SAR ₈₄ [%]	With C	orrection Algo	nithm	0.0	0.2	
TSL		1810 MHz	Typical S/	AR gradient: 10 %	per mm		
	Sensor Cen	ter to Phanta	om Surface D	istance	3.7 mm	4.7 mm	
	SAR ₆₀ [%]	Withou	t Correction A	Ugorithm	6.3	3.6	
	SAR _{bo} [%]	With C	orrection Algo	withm	0.1	0.3	2
Sens	sor Offset			<i></i>			
	Probe Tip to	Sensor Cer	nter		2.7 mm		

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^ The uncertainties of NormX,V,Z do not affect the E^2 -field uncertainty inside TSL (see Page 6).

⁸ Numerical linearization parameter: uncertainty not required.

Certificate No: ET3-1787_May06


Page 4 of 9



ET3DV6 SN:1787

Test Report No 👘 FA680808-1-2-03

May 31, 2006

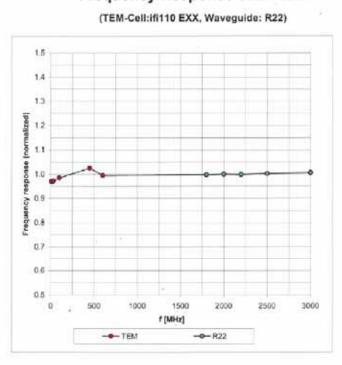

Frequency Response of E-Field

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: ET3-1787_May06


Page 5 of 9

©2006 SPORTON International Inc. SAR Testing Lab



ET3DV6 SN:1787

May 31, 2006

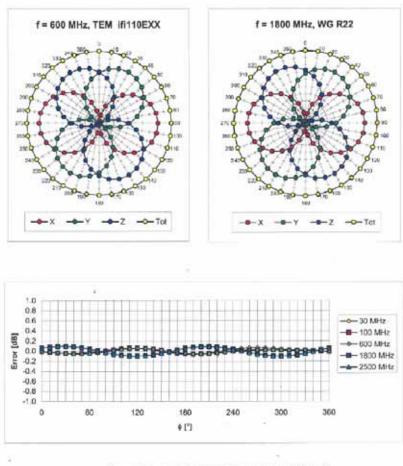


Receiving Pattern (6), 9 = 0°

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ET3-1787_May06

Page 6 of 9



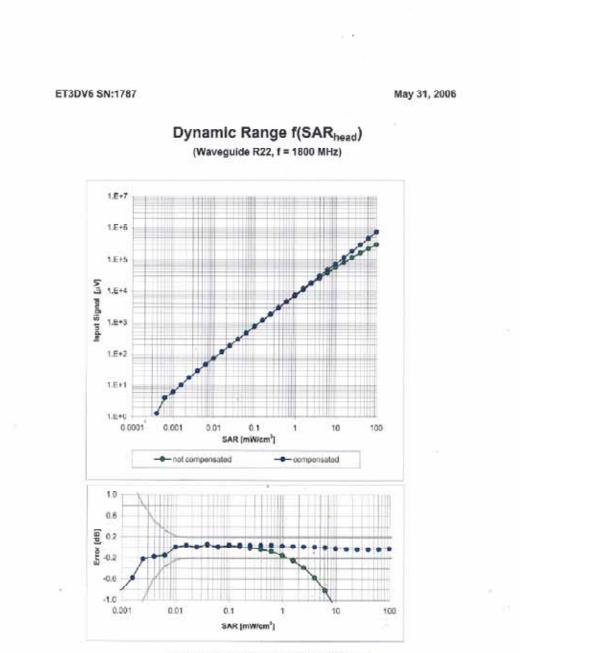


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: ET3-1787_May06

Page 7 of 9

©2006 SPORTON International Inc. SAR Testing Lab



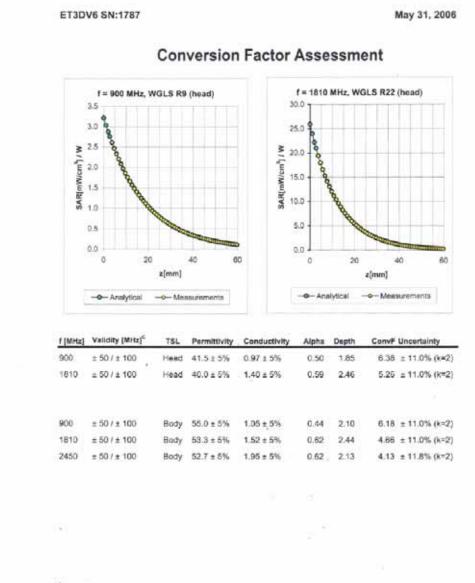


⁶ The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: ET3-1787_May06

Page 6 of 9

©2006 SPORTON International Inc. SAR Testing Lab This report shall not be reproduced except in full, without the written approval of Sporton.



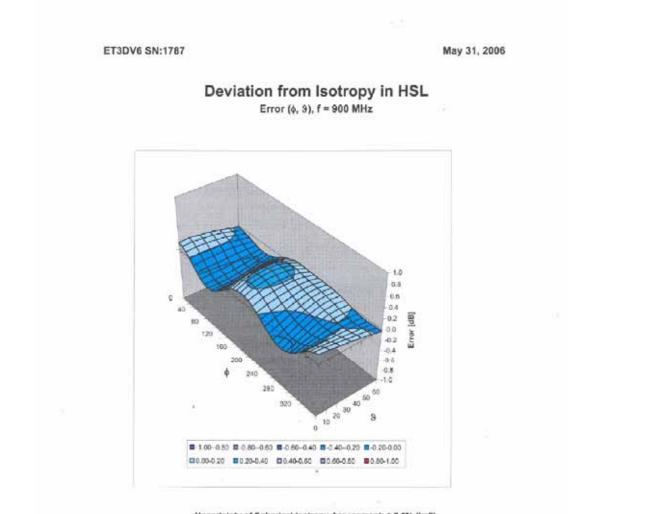

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ET3-1787_May06

Page 9 of 9

©2006 SPORTON International Inc. SAR Testing Lab



The Swiss Accreditation Service i Multilateral Agreement for the rec Client Sporton (Auden	ognition of calibration of	ertificates	
-			
			DAE3-577 Nov05
CALIBRATION C	ERTIFICATE		
Object	DAE3 - SD 000 D	03 AA - SN: 577	
	in the second		
Calibration procedure(s)	QA CAL-06.v12		
ner se aus en de la primeira de la constant de la sette (b)	Calibration proces	lure for the data acquisition electr	onics (DAE)
Calibration date:	November 11, 200	05	
Condition of the calibrated item	In Tolerance		
	ed in the closed laboratory	obability are given on the following pages and $_{\rm f}$ facility: environment temperature (22 \pm 3)°C a	
All calibrations have been conducte Calibration Equipment used (M&TE	ed in the closed laboratory		are part of the certificate. and humidity < 70%.
Calibration Equipment used (M&TE Primary Standards	ed in the closed laboratory critical for calibration)	rfacility; environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.)	are part of the certificate. and humidity < 70%. Scheduled Calibration
Calibration Equipment used (M&TE	ed in the closed laboratory critical for calibration)	facility: environment temperature $(22 \pm 3)^{\circ}C$ a	are part of the certificate. and humidity < 70%.
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702	ed in the closed laboratory critical for calibration) ID # SN: 6295803	rfacility; environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.) 7-Oct-05 (Sintrel, No.E-050073)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-06
Calibration Equipment used (M&TE Primary Standards	ed in the closed laboratory critical for calibration) ID # SN: 6295803	rfacility; environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.)	are part of the certificate, and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Secondary Standards	ed in the closed laboratory critical for calibration) ID # SN: 6295803	rfacility; environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.) 7-Oct-05 (Sintrel, No.E-050073) Check Date (in house)	are part of the certificate, and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Secondary Standards	ed in the closed laboratory critical for calibration) ID # SN: 6295803	rfacility; environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.) 7-Oct-05 (Sintrel, No.E-050073) Check Date (in house)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Secondary Standards	ed in the closed laboratory critical for calibration) ID # SN: 6295803	rfacility; environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.) 7-Oct-05 (Sintrel, No.E-050073) Check Date (in house)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Secondary Standards	ed in the closed laboratory critical for calibration) ID # SN: 6295803	rfacility; environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.) 7-Oct-05 (Sintrel, No.E-050073) Check Date (in house)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Secondary Standards	ed in the closed laboratory critical for calibration) ID # SN: 6295803	rfacility; environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.) 7-Oct-05 (Sintrel, No.E-050073) Check Date (in house)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Secondary Standards	ed in the closed laboratory critical for calibration) ID # SN: 6295803	rfacility; environment temperature (22 ± 3)°C a Cal Date (Calibrated by, Certificate No.) 7-Oct-05 (Sintrel, No.E-050073) Check Date (in house)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Secondary Standards	ed in the closed laboratory critical for calibration) ID # SN: 6295803 ID # SE UMS 006 AB 1002	r facility: environment temperature (22 ± 3)°C a <u>Cal Date (Calibrated by, Certificate No.)</u> 7-Oct-05 (Sintrel, No.E-050073) <u>Check Date (in house)</u> 29-Jun-05 (SPEAG, in house check)	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check In house check Jun-06 Signature
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Secondary Standards Calibrator Box V1.1	ed in the closed laboratory critical for calibration) ID # SN: 6295803 ID # SE UMS 006 AB 1002 Name	rfacility: environment temperature (22 ± 3)°C a <u>Cal Date (Calibrated by, Certificate No.)</u> 7-Oct-05 (Sintrel, No.E-050073) <u>Check Date (in house)</u> 29-Jun-05 (SPEAG, in house check) Function Technician	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check In house check Jun-06 Signature
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Secondary Standards Calibrator Box V1.1	ed in the closed laboratory critical for calibration) ID # SN: 6295803 ID # SE UMS 006 AB 1002 Name	rfacility: environment temperature (22 ± 3)°C a <u>Cal Date (Calibrated by, Certificate No.)</u> 7-Oct-05 (Sintrel, No.E-050073) <u>Check Date (in house)</u> 29-Jun-05 (SPEAG, in house check) Function Technician	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check In house check Jun-06 Signature
Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Secondary Standards Calibrator Box V1.1	ed in the closed laboratory critical for calibration) ID # SN: 6295803 ID # SE UMS 006 AB 1002 Name Daniel Steinacher	rfacility: environment temperature (22 ± 3)°C a <u>Cal Date (Calibrated by, Certificate No.)</u> 7-Oct-05 (Sintrel, No.E-050073) <u>Check Date (in house)</u> 29-Jun-05 (SPEAG, in house check) Function Technician	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-06 Scheduled Check In house check Jun-06



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



WISS

BRP

 S
 Schweizerischer Kallbrierdienst

 C
 Service suisse d'étalonnage

 S
 Servizio svizzero di taratura

 S
 Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE Connector angle

r angle information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters contain technical information as a result from the performance test and require no uncertainty.
- DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
- Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
- Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
- AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
- Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
- Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
- Input resistance: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
- Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
- Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE3-577_Nov05

Page 2 of 5



DC Voltage Measurement

1LSB =	6.1µV,	full range =	-100+300 mV
1LSB =	61nV,	full range =	-1+3mV
		/ 옷이 집 집 같아요	

Calibration Factors	X	Y	Z
High Range	404.445 ± 0.1% (k=2)	403.896 ± 0.1% (k=2)	404.369 ± 0.1% (k=2)
Low Range	3.94241 ± 0.7% (k=2)	3.89919 ± 0.7% (k=2)	3.95427 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	130 ° ± 1 °
---	-------------

Certificate No: DAE3-577_Nov05

Page 3 of 5



Appendix

1. DC Voltage Linearity

High Range	Input (µV)	Reading (µV)	Error (%)
Channel X + Input	200000	199999.3	0.00
Channel X + Input	20000	20006.75	0.03
Channel X - Input	20000	-19997.90	-0.01
Channel Y + Input	200000	200000.3	0.00
Channel Y + Input	20000	20004.58	0.02
Channel Y - Input	20000	-20000.75	0.00
Channel Z + Input	200000	199999.6	0.00
Channel Z + Input	20000	20001.43	0.01
Channel Z - Input	20000	-20003.93	0.02

Low Range		Input (µV)	Reading (µV)	Error (%)
Channel X	+ Input	2000	2000.1	0.00
Channel X	+ Input	200	200.42	0.21
Channel X	- Input	200	-200.30	0.15
Channel Y	+ Input	2000	2000.1	0.00
Channel Y	+ Input	200	199.35	-0.32
Channel Y	- Input	200	-200.96	0.48
Channel Z	+ Input	2000	1999.9	0.00
Channel Z	+ Input	200	199.37	-0.31
Channel Z	- Input	200	-200.62	0.31

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (µV)
Channel X	200	13.40	12.55
	- 200	-12.29	-13.06
Channel Y	200	-6.93	-7.43
	- 200	6.72	6.47
Channel Z	200	0.71	0.36
	- 200	-1.67	-1.93

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200		1.59	0.08
Channel Y	200	1.69	-	3.62
Channel Z	200	-0.73	-1.49	-

Certificate No: DAE3-577_Nov05

Page 4 of 5

©2006 SPORTON International Inc. SAR Testing Lab



4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15946	15679
Channel Y	15960	16151
Channel Z	16233	15968

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input $10 M \Omega$

	Average (µV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	0.08	-1.13	2.31	0.51
Channel Y	-0.35	-2.00	0.81	0.43
Channel Z	-0.38	-2.76	1.68	0.40

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	200.8
Channel Y	0.2000	201.4
Channel Z	0.2001	200.3

8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.0	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE3-577_Nov05

Page 5 of 5

©2006 SPORTON International Inc. SAR Testing Lab