

## System Cheek\_6500MHz

### DUT: D6.5GHzV2-SN:1026

Communication System: Custom Band; Frequency: 6500.0

Medium: HSL\_6500\_230328 Medium parameters used:  $f = 6500.0$  MHz;  $\sigma = 6.08$  S/m;  $\epsilon_r = 34.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3826; ConvF(4.95, 4.95, 4.95); Calibrated: 2022/8/8
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2022/5/30
- Phantom: Twin-SAM1(P1aP2a20); Type: QD 000 P40 CD; Serial: TP:1670
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--

**Area Scan (51.0 mm x 51.0 mm):** Measurement Grid: 8.5 mm x 8.5 mm


SAR (1g) = 21.7 W/kg; SAR (10g) = 4.63 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 27.8 W/kg; SAR (10g) = 4.91 W/kg;

psAPD (4.0cm<sup>2</sup>, sq) = 119 [W/m<sup>2</sup>];

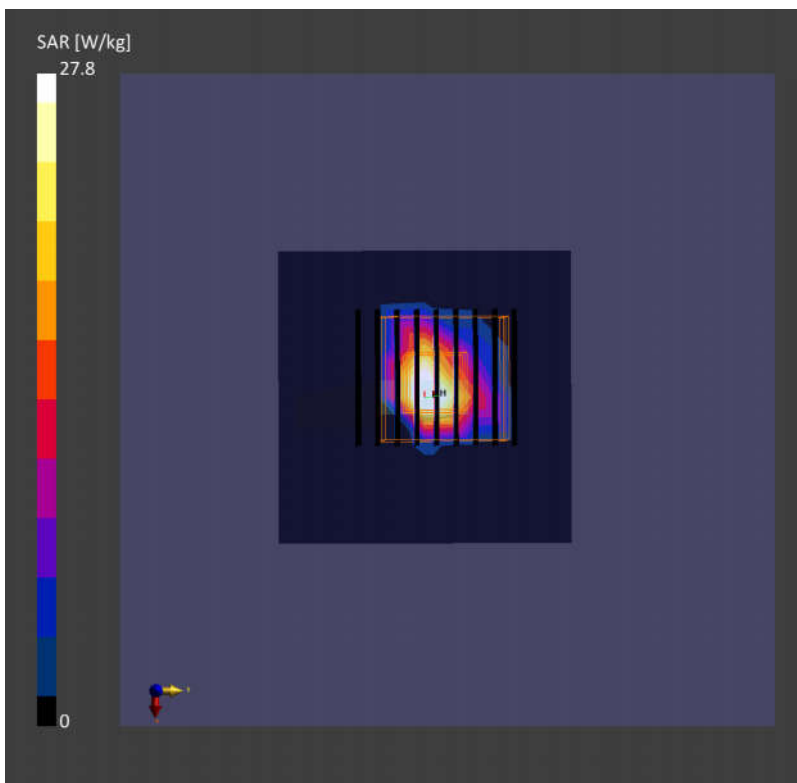

Date: 2023/3/30

## System Check\_6500MHz

### DUT: D6.5GHzV2-SN:1026

Communication System: Custom Band; Frequency: 6500.0

Medium: HSL\_6500\_230330 Medium parameters used:  $f = 6500.0$  MHz;  $\sigma = 6.12$

S/m;  $\epsilon_r = 34.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3826; ConvF(4.95, 4.95, 4.95); Calibrated: 2022/8/8
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2022/5/30
- Phantom: Twin-SAM1(P1aP2a20); Type: QD 000 P40 CD; Serial: TP:1670
- Measurement Software: cDASY6 V16.0.0.116
- UID: CW, 0--

**Area Scan (51.0 mm x 51.0 mm):** Measurement Grid: 8.5 mm x 8.5 mm


SAR (1g) = 21.8 W/kg; SAR (10g) = 4.66 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = 0.06 dB

SAR (1g) = 27.5 W/kg; SAR (10g) = 4.96 W/kg;

psAPD (4.0cm<sup>2</sup>, sq) = 118 [W/m<sup>2</sup>];

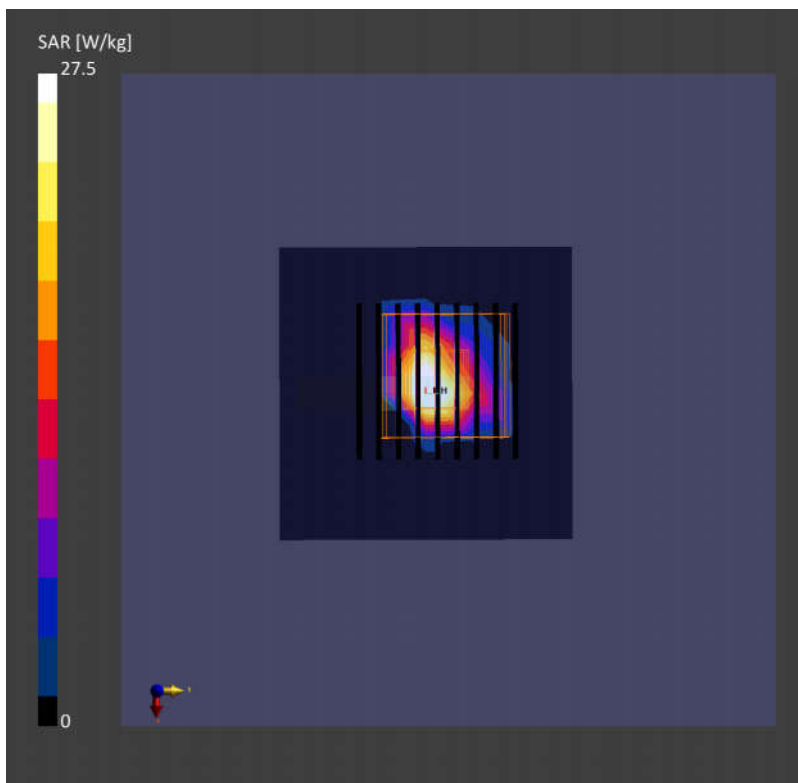

Measurement Report for Device, FRONT, Validation band, CW, Channel 10000 (10000.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
Device,	100.0 x 100.0 x 105.0		Source

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor
5G	FRONT, 10.00	Validation band	CW, 0--	10000.0, 10000	1.0

Hardware Setup

Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave	Air -	EUmmWV3 - SN9424_F1-55GHz, 2022-04-06	DAE4 Sn1210, 2022-04-12

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	120.0 x 120.0
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.0
MAIA	N/A

Measurement Results

Scan Type	5G Scan
Date	2023-02-27
Avg. Area [cm <sup>2</sup> ]	4.00
psPDn+ [W/m <sup>2</sup> ]	168
psPDtot+ [W/m <sup>2</sup> ]	169
psPDmod+ [W/m <sup>2</sup> ]	172
E <sub>max</sub> [V/m]	295
Power Drift [dB]	0.01

