

FC

Test Report

Product Name	Mobile Clinical Assistant C5
Model No.	CFT-001
FCC ID.	MSQCFT01
Transmitter Module.	ASUS / BT-183

Applicant	ASUSTeK COMPUTER INC.
Address	4FL., No. 150, Li-Te Rd., Peitou, Taipei, Taiwan, R.O.C.

Date of Receipt	Apr. 17, 2007
Issued Date	May 17, 2007
Report No.	074L109-RFUSP06V01

The Test Results relate only to the samples tested.

The test report shall not be reproduced except in full without the written approval of Quietek Corporation.

This report must not be used to claim product endorsement by NVLAP any agency of the U.S. Government

Test Report Certification

Issued Date: May 17, 2007

Report No.: 074L109-RFUSP06V01



Product Name	Mobile Clinical Assistant C5
Applicant	ASUSTeK COMPUTER INC.
Address	4FL., No. 150, Li-Te Rd., Peitou, Taipei, Taiwan, R.O.C.
Manufacturer	ASUSTeK COMPUTER INC.
Model No.	CFT-001
FCC ID.	MSQCFT01
Rated Voltage	AC 120V/60Hz
Working Voltage	AC 120V/60Hz
Trade Name	Motion Computing Incorporated
Applicable Standard	FCC CFR Title 47 Part 15 Subpart C: 2005 ANSI C63.4: 2003
Test Result	Complied



The Test Results relate only to the samples tested.
 The test report shall not be reproduced except in full without the written approval of Quietek Corporation.
 This report must not be used to claim product endorsement by NVLAP any agency of the U.S. Government

Documented By : Rita Huang
 (Engineering Adm. Specialist / Rita Huang)



Tested By : Tim Sung
 (Engineer / Tim Sung)

Approved By : Gene Chang
 (President / Gene Chang)



TABLE OF CONTENTS

Description	Page
1. GENERAL INFORMATION	5
1.1. EUT Description.....	5
1.2. Operational Description.....	7
1.3. Tested System Details.....	8
1.4. Configuration of Tested System	8
1.5. EUT Exercise Software	8
1.6. Test Facility	9
2. CONDUCTED EMISSION	10
2.1. Test Equipment.....	10
2.2. Test Setup	10
2.3. Limits.....	11
2.4. Test Procedure	11
2.5. Uncertainty	11
2.6. Test Result of Conducted Emission.....	12
3. PEAK POWER OUTPUT	14
3.1. Test Equipment.....	14
3.2. Test Setup	14
3.3. Limit	14
3.4. Uncertainty	14
3.5. Test Result of Peak Power Output.....	15
4. RADIATED EMISSION	18
4.1. Test Equipment.....	18
4.2. Test Setup	19
4.3. Limits.....	19
4.4. Test Procedure	20
4.5. Uncertainty	20
4.6. Test Result of Radiated Emission.....	21
5. BAND EDGE	25
5.1. Test Equipment.....	25
5.2. Test Setup	25
5.3. Limit	26
5.4. Test Procedure	26
5.5. Uncertainty	26
5.6. Test Result of Band Edge	27
6. CHANNEL NUMBER.....	31
6.1. Test Equipment.....	31

6.2.	Test Setup	31
6.3.	Limit	31
6.4.	Uncertainty	31
6.5.	Test Result of Channel Number.....	32
7.	CHANNEL SEPARATION.....	33
7.1.	Test Equipment	33
7.2.	Test Setup	33
7.3.	Limit	33
7.4.	Uncertainty	33
7.5.	Test Result of Channel Separation.....	34
8.	DWELL TIME.....	35
8.1.	Test Equipment	35
8.2.	Test Setup	35
8.3.	Limit	35
8.4.	Uncertainty	35
8.5.	Test Result of Dwell Time.....	36
9.	OCCUPIED BANDWIDTH	38
9.1.	Test Equipment	38
9.2.	Test Setup	38
9.3.	Limits.....	38
9.4.	Uncertainty	38
9.5.	Test Result of Occupied Bandwidth	39
10.	EMI REDUCTION METHOD DURING COMPLIANCE TESTING	42

Attachment 1: EUT Test Photographs
Attachment 2: EUT Detailed Photographs

1. GENERAL INFORMATION

1.1. EUT Description

Product Name	Mobile Clinical Assistant C5
Trade Name	Motion Computing Incorporated
FCC ID.	MSQCFT01
Model No.	CFT-001
Frequency Range	2402 - 2480MHz
Channel Number	79
Type of Modulation	FHSS
Antenna type	Soldered on PCB
Channel Control	Auto
Antenna Gain	Refer to the table "Antenna List"
Power Adapter	MFR: DELTA, M/N: ADP-50HH REV.B Cable Out: Non-Shielded, 1.8m with one ferrite core bonded. Power Cord: Shielded, 1.8m

Antenna List

No.	Manufacturer	Part No.	Peak Gain
1	MAG LAYERS	LTA-5824-2G4H2-A1	0.64dBi for 2.4 GHz

Frequency of Each Channel:

Channel	Frequency	Channel	Frequency	Channel	Frequency	Channel	Frequency
Channel 00:	2402 MHz	Channel 20:	2422 MHz	Channel 40:	2442 MHz	Channel 60:	2462 MHz
Channel 01:	2403 MHz	Channel 21:	2423 MHz	Channel 41:	2443 MHz	Channel 61:	2463 MHz
Channel 02:	2404 MHz	Channel 22:	2424 MHz	Channel 42:	2444 MHz	Channel 62:	2464 MHz
Channel 03:	2405 MHz	Channel 23:	2425 MHz	Channel 43:	2445 MHz	Channel 63:	2465 MHz
Channel 04:	2406 MHz	Channel 24:	2426 MHz	Channel 44:	2446 MHz	Channel 64:	2466 MHz
Channel 05:	2407 MHz	Channel 25:	2427 MHz	Channel 45:	2447 MHz	Channel 65:	2467 MHz
Channel 06:	2408 MHz	Channel 26:	2428 MHz	Channel 46:	2448 MHz	Channel 66:	2468 MHz
Channel 07:	2409 MHz	Channel 27:	2429 MHz	Channel 47:	2449 MHz	Channel 67:	2469 MHz
Channel 08:	2410 MHz	Channel 28:	2430 MHz	Channel 48:	2450 MHz	Channel 68:	2470 MHz
Channel 09:	2411 MHz	Channel 29:	2431 MHz	Channel 49:	2451 MHz	Channel 69:	2471 MHz
Channel 10:	2412 MHz	Channel 30:	2432 MHz	Channel 50:	2452 MHz	Channel 70:	2472 MHz
Channel 11:	2413 MHz	Channel 31:	2433 MHz	Channel 51:	2453 MHz	Channel 71:	2473 MHz
Channel 12:	2414 MHz	Channel 32:	2434 MHz	Channel 52:	2454 MHz	Channel 72:	2474 MHz
Channel 13:	2415 MHz	Channel 33:	2435 MHz	Channel 53:	2455 MHz	Channel 73:	2475 MHz
Channel 14:	2416 MHz	Channel 34:	2436 MHz	Channel 54:	2456 MHz	Channel 74:	2476 MHz
Channel 15:	2417 MHz	Channel 35:	2437 MHz	Channel 55:	2457 MHz	Channel 75:	2477 MHz
Channel 16:	2418 MHz	Channel 36:	2438 MHz	Channel 56:	2458 MHz	Channel 76:	2478 MHz
Channel 17:	2419 MHz	Channel 37:	2439 MHz	Channel 57:	2459 MHz	Channel 77:	2479 MHz
Channel 18:	2420 MHz	Channel 38:	2440 MHz	Channel 58:	2460 MHz	Channel 78:	2480 MHz
Channel 19:	2421 MHz	Channel 39:	2441 MHz	Channel 59:	2461 MHz		

The system receivers have input bandwidths that match the hopping channel bandwidths of their corresponding transmitters and shift frequencies in synchronization with the transmitted signals.

Frequency hopping spread spectrum systems are not required to employ all available hopping channels during each transmission. The transmitter is presented with a continuous data stream. In addition, a system employing short transmission bursts must comply with the definition of a frequency hopping system and must distribute its 79 channels and over the minimum number of hopping channels (75 channels).

The incorporation of intelligence within a frequency hopping spread spectrum system that permits the system to recognize other users within the spectrum band so that it individually and independently chooses and adapts its hopsets to avoid hopping on occupied channels is permitted. The coordination of frequency hopping systems in any other manner for the express purpose of avoiding the simultaneous occupancy of individual hopping frequencies by multiple transmitters is not permitted.

Note:

1. This device is a Mobile Clinical Assistant C5 with a built-in 2.4GHz Bluetooth transceiver.
2. These tests were conducted on a sample for the purpose of demonstrating compliance of bluetooth transmitter with Part 15 Subpart C Paragraph 15.247 for spread spectrum devices.
3. Regarding to the operation frequency, the lowest, middle and highest frequency are selected to perform the test.
4. Quietek verified among construction and function in typical operation.

1.2. Operational Description

The EUT is an Mobile Clinical Assistant C5 with a built-in 2.4GHz Bluetooth transceiver. The number of the channels is 79 in 2402-2480MHz. The device adapts the frequency hopping spread spectrum modulation. The antenna is connector-type and provides diversity function to improve the receiving function.

This device provides wireless technology that revolutionizes personal connectivity. It is the solution for the seamless integration of Bluetooth technology into personal computer enabling short-range wireless connections between desktop/laptop computers, Bluetooth-enabled peripherals, and portable handheld devices.

Test Mode	Mode 1: Transmitter
-----------	---------------------


1.3. Tested System Details

The types for all equipment, plus descriptions of all cables used in the tested system (including inserted cards) are:

	Product	Manufacturer	Model No.	Serial No.	Power Cord
(1)	Keyboard	BTC	5200U	N/A	N/A
(2)	USB Mouse	Logitech	M-BE58	HCA30103100	N/A

	Signal Cable Type	Signal cable Description
A.	Keyboard Cable	Shielded, 1.8m
B.	Mouse Cable	Shielded, 1.8m

1.4. Configuration of Tested System

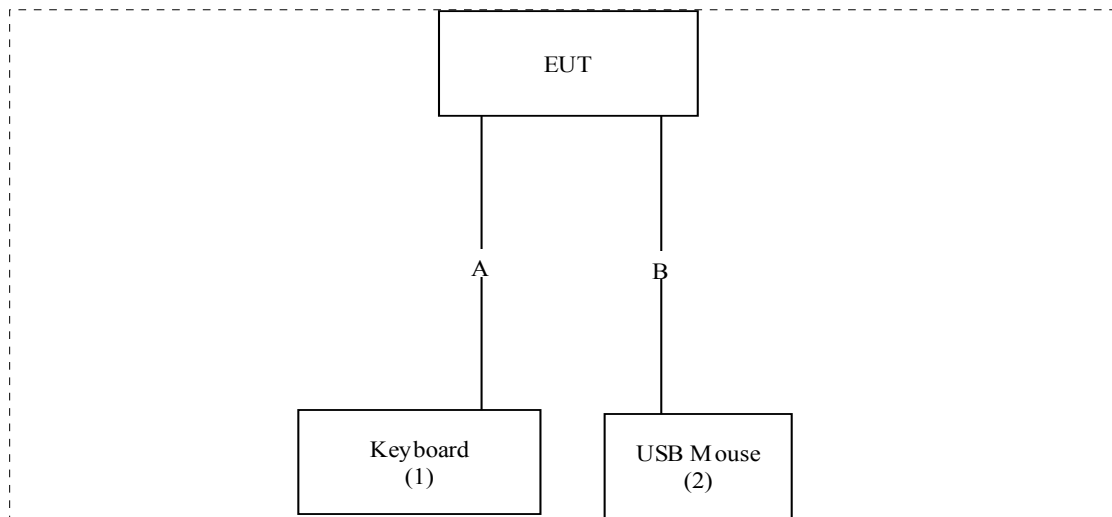

1.5. EUT Exercise Software

- 1 Setup the EUT and simulators as shown on 1.4.
- 2 Turn on the power of all equipment.
- 3 Messages will be transmitted and received through EUT.
- 4 Test is based on the mandatory continuous transmitter.
- 5 Repeat the above procedure (3) to (4).

1.6. Test Facility

Ambient conditions in the laboratory:

Items	Required (IEC 68-1)	Actual
Temperature (°C)	15-35	20-35
Humidity (%RH)	25-75	30-65
Barometric pressure (mbar)	860-1060	950-1000

Site Description: File on
 Federal Communications Commission
 FCC Engineering Laboratory
 7435 Oakland Mills Road
 Columbia, MD 21046
 Reference 31040/SIT1300F2



Accreditation on NVLAP
 NVLAP Lab Code: 200533-0



Site Name: Quietek Corporation
 Site Address: No. 5-22, Ruei-Shu Valley, Ruei-Ping Tsuen,
 Lin-Kou Shiang, Taipei,
 Taiwan, R.O.C.
 TEL: 886-2-8601-3788 / FAX : 886-2-8601-3789
 E-Mail : service@quietek.com



2. Conducted Emission


2.1. Test Equipment

The following test equipment are used during the conducted emission test:

Item	Instrument	Manufacturer	Type No./Serial No	Last Cal.	Remark
1	Test Receiver	R & S	ESCS 30/825442/17	May, 2007	
2	L.I.S.N.	R & S	ESH3-Z5/825016/6	May, 2007	EUT
3	L.I.S.N.	Kyoritsu	KNW-407/8-1420-3	May, 2007	Peripherals
4	Pulse Limiter	R & S	ESH3-Z2	May, 2007	
5	No.1 Shielded Room			N/A	

Note: All instruments are calibrated every one year.

2.2. Test Setup

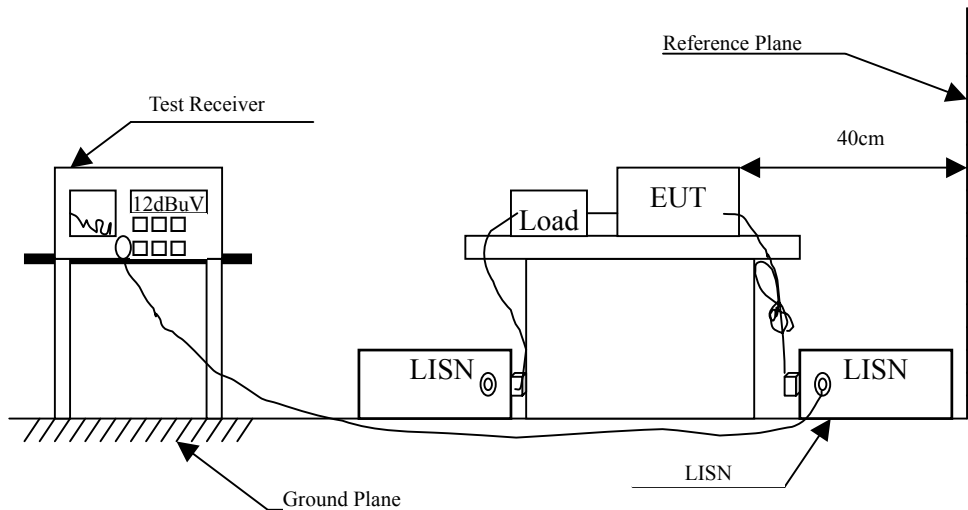

2.3. Limits

FCC Part 15 Subpart C Paragraph 15.207 (dBuV) Limit		
Frequency MHz	Limits	
	QP	AV
0.15 - 0.50	66-56	56-46
0.50-5.0	56	46
5.0 - 30	60	50

Remarks: In the above table, the tighter limit applies at the band edges.

2.4. Test Procedure

The EUT and simulators are connected to the main power through a line impedance stabilization network (L.I.S.N.). This provides a 50 ohm /50uH coupling impedance for the measuring equipment. The peripheral devices are also connected to the main power through a LISN that provides a 50ohm /50uH coupling impedance with 50ohm termination. (Please refer to the block diagram of the test setup and photographs.)

Both sides of A.C. line are checked for maximum conducted interference. In order to find the maximum emission, the relative positions of equipment and all the interface cables must be changed according to ANSI C63.4: 2003 on conducted measurement.

Conducted emissions were investigated over the frequency range from 0.15MHz to 30MHz using a receiver bandwidth of 9kHz.

2.5. Uncertainty

± 2.26 dB

2.6. Test Result of Conducted Emission

Product : Mobile Clinical Assistant C5
 Test Item : Conducted Emission Test
 Power Line : Line 1
 Test Mode : Mode 1: Transmitter (2441MHz)

Frequency MHz	Correct Factor dB	Reading Level dBuV	Measurement Level dBuV	Margin dB	Limit dBuV
LINE 1					
Quasi-Peak					
0.205	0.202	55.290	55.492	-8.937	64.429
0.270	0.210	46.740	46.950	-15.621	62.571
0.340	0.214	40.050	40.264	-20.307	60.571
0.410	0.215	40.780	40.995	-17.576	58.571
0.480	0.216	33.010	33.226	-23.345	56.571
0.550	0.217	33.760	33.977	-22.023	56.000
Average					
0.205	0.202	35.330	35.532	-18.897	54.429
0.270	0.210	28.400	28.610	-23.961	52.571
0.340	0.214	24.550	24.764	-25.807	50.571
0.410	0.215	25.860	26.075	-22.496	48.571
0.480	0.216	21.690	21.906	-24.665	46.571
0.550	0.217	21.580	21.797	-24.203	46.000

Note:

1. All Reading Levels are Quasi-Peak and average value.
2. "█" means the worst emission level.
3. Measurement Level = Reading Level + Correct Factor

Product : Mobile Clinical Assistant C5
 Test Item : Conducted Emission Test
 Power Line : Line 2
 Test Mode : Mode 1: Transmitter (2441MHz)

Frequency MHz	Correct Factor dB	Reading Level dBuV	Measurement Level dBuV	Margin dB	Limit dBuV
LINE 2					
Quasi-Peak					
0.203	0.202	53.190	53.392	-11.094	64.486
0.273	0.203	48.690	48.893	-13.593	62.486
0.343	0.214	39.650	39.864	-20.622	60.486
0.412	0.215	39.200	39.415	-19.099	58.514
0.482	0.216	30.860	31.076	-25.438	56.514
0.542	0.217	32.360	32.577	-23.423	56.000
Average					
0.203	0.202	34.190	34.392	-20.094	54.486
0.273	0.203	30.480	30.683	-21.803	52.486
0.343	0.214	24.690	24.904	-25.582	50.486
0.412	0.215	24.720	24.935	-23.579	48.514
0.482	0.216	20.630	20.846	-25.668	46.514
0.542	0.217	19.590	19.807	-26.193	46.000

Note:

1. All Reading Levels are Quasi-Peak and average value.
2. "█" means the worst emission level.
3. Measurement Level = Reading Level + Correct Factor

3. Peak Power Output


3.1. Test Equipment

The following test equipments are used during the radiated emission tests:

	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
X	Test Receiver	R & S	ESI 26 / 838786 / 004	May, 2007
X	Spectrum Analyzer	Agilent	E4407B / US39440758	May, 2007

Note: 1. All equipments are calibrated every one year.
 2. The test instruments marked by “X” are used to measure the final test results.

3.2. Test Setup

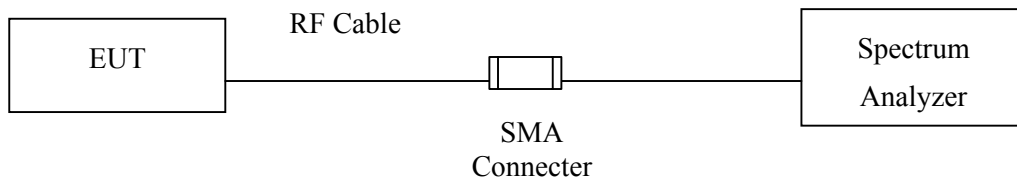

3.3. Limit

The maximum peak power shall be less 1Watt.

3.4. Uncertainty


± 1.27 dB

3.5. Test Result of Peak Power Output

Product : Mobile Clinical Assistant C5
 Test Item : Peak Power Output
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter


Channel No.	Frequency (MHz)	Measurement	Required Limit	Result
Channel 00	2402.00	3.11dBm	1 Watt= 30 dBm	Pass
Channel 39	2441.00	2.30dBm	1 Watt= 30 dBm	Pass
Channel 78	2480.00	1.29dBm	1 Watt= 30 dBm	Pass

Channel 00:

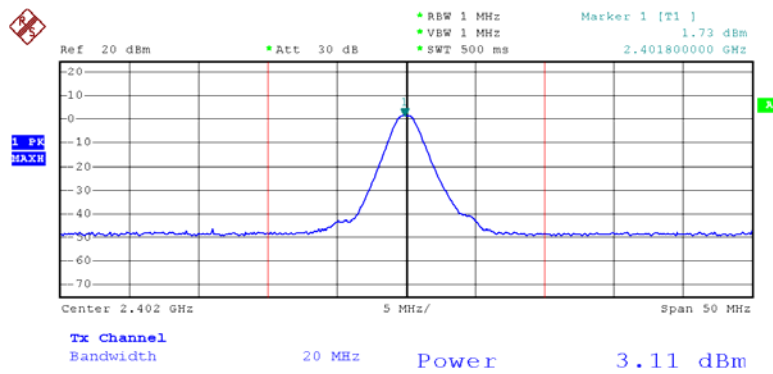


PN1
 Date: 5.MAY.2007 05:16:24

Channel 39:

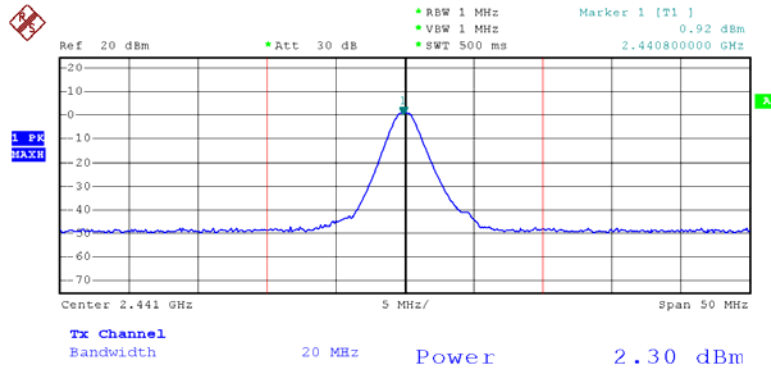

PN1
Date: 5.MAY.2007 05:17:00

Channel 78:

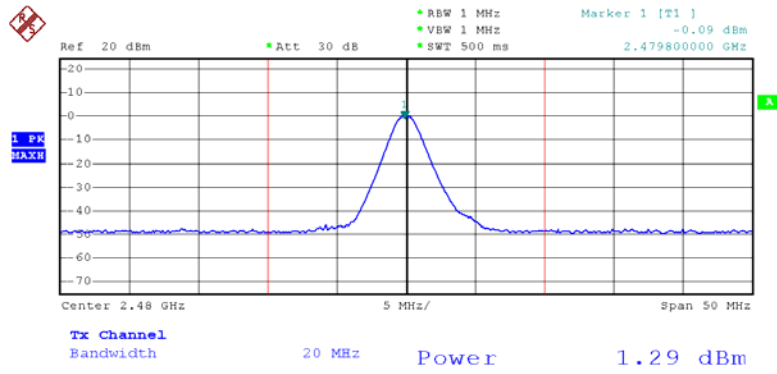

PN1

Date: 5.MAY.2007 05:17:33

4. Radiated Emission


4.1. Test Equipment

The following test equipments are used during the radiated emission test:

Test Site	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
<input type="checkbox"/> Site # 1	Test Receiver	R & S	ESVS 10 / 834468/003	May, 2007
	Spectrum Analyzer	Advantest	R3162/ 00803480	May, 2007
	Pre-Amplifier	Advantest	BB525C/ 3307A01812	May, 2007
	Bilog Antenna	SCHAFFNER	CBL6112B / 2697	Sep., 2006
<input type="checkbox"/> Site # 2	Test Receiver	R & S	ESCS 30 / 836858 / 022	May, 2007
	Spectrum Analyzer	Advantest	R3162 / 100803466	May, 2007
	Pre-Amplifier	Advantest	BB525C/3307A01814	May, 2007
	Bilog Antenna	SCHAFFNER	CBL6112B / 2705	May, 2007
	Horn Antenna	ETS	3115 / 0005-6160	Sep., 2006
	Pre-Amplifier	QTK	QTK-AMP-01/ 0001	May, 2007
<input checked="" type="checkbox"/> Site # 3	Test Receiver	R & S	ESI 26 / 838786 / 004	May, 2007
	Spectrum Analyzer	HP	E4407B / US39440758	May, 2007
	Bilog Antenna	SCHAFFNER	CBL6112B / 2697	May, 2007
	Horn Antenna	Schwarzbeck	BBHA9120D / 305, 306	July, 2006
	Horn Antenna	Schwarzbeck	BBHA9170 / 208, 209	July, 2006
	Pre-Amplifier	QTK	QTK-AMP-01 / 0001	July, 2006
	Pre-Amplifier	QTK	QTK-AMP-03 / 0003	May, 2007
	Pre-Amplifier	HP	8449B / 3008A01123	July, 2006

- Note:
1. All equipments are calibrated every one year.
 2. The test instruments marked by "X" are used to measure the final test results.

4.2. Test Setup

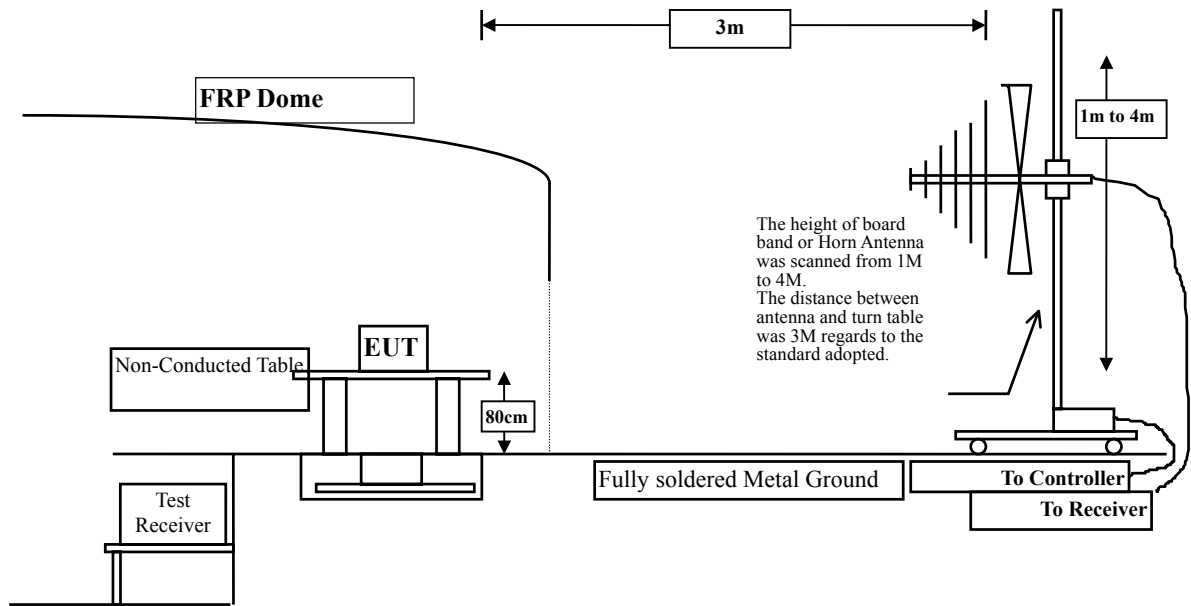

4.3. Limits

➤ General Radiated Emission Limits

Emissions radiated outside of the specified frequency bands, except for harmonics, shall be attenuated by at least 20dB below the level of the fundamental or to the general radiated emission limits in paragraph 15.209, whichever is the lesser attenuation.

FCC Part 15 Subpart C Paragraph 15.209 Limits		
Frequency MHz	uV/m @3m	dBuV/m@3m
30-88	100	40
88-216	150	43.5
216-960	200	46
Above 960	500	54

- Remarks:
1. RF Voltage (dBuV) = 20 log RF Voltage (uV)
 2. In the Above Table, the tighter limit applies at the band edges.
 3. Distance refers to the distance in meters between the measuring instrument antenna and the closed point of any part of the device or system.

4.4. Test Procedure

The EUT and its simulators are placed on a turn table which is 0.8 meter above ground. The turn table can rotate 360 degrees to determine the position of the maximum emission level.

The EUT was positioned such that the distance from antenna to the EUT was 3 meters.

The antenna can move up and down between 1 meter and 4 meters to find out the maximum emission level.

Both horizontal and vertical polarization of the antenna are set on measurement. In order to find the maximum emission, all of the interface cables must be manipulated according to ANSI C63.4: 2003 on radiated measurement.

The additional latch filter below 1GHz was used to measure the level of harmonics radiated emission during field strength of harmonics measurement.

The bandwidth below 1GHz setting on the field strength meter is 120 kHz, above 1GHz are 1 MHz.

The frequency range from 30MHz to 10th harmonics is checked.

4.5. Uncertainty

± 3.9 dB above 1GHz

± 3.8 dB below 1GHz

4.6. Test Result of Radiated Emission

Product : Mobile Clinical Assistant C5
 Test Item : Harmonic Radiated Emission
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2402MHz)

Frequency MHz	Correct Factor dB	Reading Level dBuV	Measurement Level dBuV/m	Margin dB	Limit dBuV/m
Horizontal					
Peak Detector:					
4803.625	3.661	52.403	56.064	-17.936	74.000
7206.000	9.357	36.016	45.372	-28.628	74.000
9608.250	11.841	41.119	52.961	-21.039	74.000
Average Detector:					
4803.625	3.661	36.360	40.022	-13.978	54.000
Vertical					
Peak Detector:					
4803.625	3.661	57.105	60.766	-13.234	74.000
7206.000	9.357	35.566	44.922	-29.078	74.000
9607.375	11.843	41.962	53.804	-20.196	74.000
Average Detector:					
4803.625	3.661	39.260	42.922	-11.078	54.000

Note:

1. All Readings below 1GHz are Quasi-Peak, above are performed with peak and/or average measurements as necessary.
2. Receiver setting (Peak Detector) : RBW:1MHz; VBW:1MHz; Span:100MHz ◦
3. Receiver setting (AVG Detector) : RBW:1MHz; VBW:30Hz; Span:20MHz ◦
4. Emission Level = Reading Level + Correct Factor.
5. The average measurement was not performed when the peak measured data under the limit of average detection. If the readings given are average, peak measurement should also be supplied.

Product : Mobile Clinical Assistant C5
 Test Item : Harmonic Radiated Emission
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2441MHz)

Frequency MHz	Correct Factor dB	Reading Level dBuV	Measurement Level dBuV/m	Margin dB	Limit dBuV/m
Horizontal					
Peak Detector:					
4882.000	3.921	54.339	58.260	-15.740	74.000
7323.000	9.657	36.063	45.720	-28.280	74.000
9764.000	11.798	40.942	52.740	-21.260	74.000
Average Detector:					
4882.000	3.921	36.637	40.558	-13.442	54.000
Vertical					
Peak Detector:					
4882.000	3.921	56.549	60.470	-13.530	74.000
7323.000	9.657	35.533	45.190	-28.810	74.000
9764.000	11.798	41.682	53.480	-20.520	74.000
Average Detector:					
4882.000	3.921	38.509	42.430	-11.570	54.000

Note:

1. All Readings below 1GHz are Quasi-Peak, above are performed with peak and/or average measurements as necessary.
2. Receiver setting (Peak Detector) : RBW:1MHz; VBW:1MHz; Span:100MHz ◦
3. Receiver setting (AVG Detector) : RBW:1MHz; VBW:30Hz; Span:20MHz ◦
4. Emission Level = Reading Level + Correct Factor.
5. The average measurement was not performed when the peak measured data under the limit of average detection. If the readings given are average, peak measurement should also be supplied.

Product : Mobile Clinical Assistant C5
 Test Item : Harmonic Radiated Emission
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2480MHz)

Frequency MHz	Correct Factor dB	Reading Level dBuV	Measurement Level dBuV/m	Margin dB	Limit dBuV/m
Horizontal					
Peak Detector:					
4960.000	4.197	54.134	58.330	-15.670	74.000
7440.000	9.951	35.999	45.950	-28.050	74.000
9920.000	11.856	40.814	52.670	-21.330	74.000
Average Detector:					
4960.000	4.197	36.384	40.580	-13.420	54.000
Vertical					
Peak Detector:					
4960.000	4.197	56.994	61.190	-12.810	74.000
7440.000	9.951	35.419	45.370	-28.630	74.000
9920.000	11.856	41.014	52.870	-21.130	74.000
Average Detector:					
4960.000	4.197	38.334	42.530	-11.470	54.000

Note:

1. All Readings below 1GHz are Quasi-Peak, above are performed with peak and/or average measurements as necessary.
2. Receiver setting (Peak Detector) : RBW:1MHz; VBW:1MHz; Span:100MHz ◦
3. Receiver setting (AVG Detector) : RBW:1MHz; VBW:30Hz; Span:20MHz ◦
4. Emission Level = Reading Level + Correct Factor.
5. The average measurement was not performed when the peak measured data under the limit of average detection. If the readings given are average, peak measurement should also be supplied.

Product : Mobile Clinical Assistant C5
 Test Item : General Radiated Emission
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2441MHz)

Frequency MHz	Correct Factor dB	Reading Level dBuV	Measurement Level dBuV/m	Margin dB	Limit dBuV/m
Horizontal					
97.900	11.961	25.900	37.861	-5.639	43.500
228.850	10.940	27.899	38.839	-7.161	46.000
240.975	12.077	29.780	41.857	-4.143	46.000
335.550	14.410	26.066	40.476	-5.524	46.000
432.550	17.666	21.801	39.467	-6.533	46.000
527.125	18.485	23.103	41.588	-4.412	46.000
Vertical					
97.900	10.460	28.726	39.186	-4.314	43.500
240.975	12.463	30.185	42.648	-3.352	46.000
260.375	14.610	25.671	40.281	-5.719	46.000
335.550	14.360	27.735	42.095	-3.905	46.000
432.550	19.299	16.096	35.395	-10.605	46.000
527.125	18.888	23.678	42.566	-3.434	46.000

Note:

1. All Readings below 1GHz are Quasi-Peak, above are performed with peak and/or average measurements as necessary.
2. "█" means the worst emission level.
3. Measurement Level = Reading Level + Correct Factor.
4. The radiated emissions below 1GHz of the lowest, middle, highest frequency are pretested. Only the worst case is shown on the report.

5. Band Edge

5.1. Test Equipment

The following test equipments are used during the band edge tests:


	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
X	Test Receiver	R & S	ESI 26 / 838786 / 004	May, 2007
X	Spectrum Analyzer	HP	E4407B / US39440758	May, 2007
X	Bilog Antenna	SCHAFFNER	CBL6112B / 2697	May, 2007
X	Horn Antenna	Schwarzbeck	BBHA9120D / 305, 306	July, 2006
X	Horn Antenna	Schwarzbeck	BBHA9170 / 208, 209	July, 2006
X	Pre-Amplifier	QTK	QTK-AMP-01 / 0001	July, 2006
X	Pre-Amplifier	QTK	QTK-AMP-03 / 0003	May, 2007
X	Pre-Amplifier	HP	8449B / 3008A01123	July, 2006

Test Site Site 3

- Note:
1. All equipments are calibrated every one year.
 2. The test instruments marked by “X” are used to measure the final test results.

5.2. Test Setup

RF Radiated Measurement:

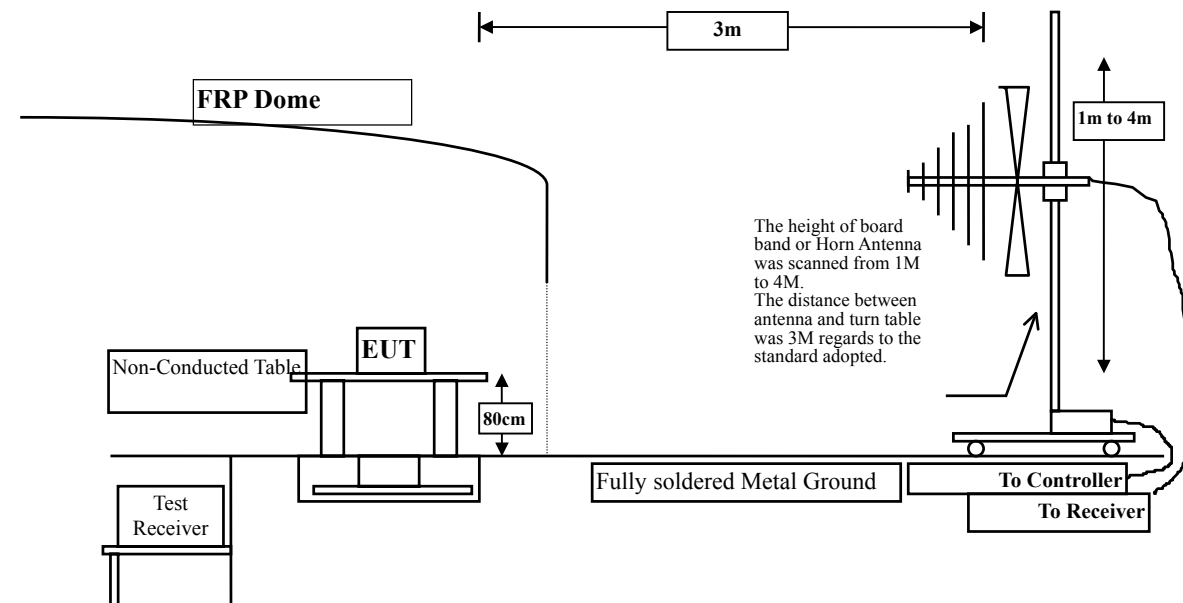

5.3. Limit

In any 100 kHz bandwidth outside the frequency band in which the spread spectrum intentional radiator is operating, the radio frequency power that is produced by the intentional radiator shall be at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of the desired power, based on either an RF conducted or a radiated measurement. Attenuation below the general limits specified in Section 15.209(a) is not required. In addition, radiated emissions which fall in the restricted bands, as defined in Section 15.205(a), must also comply with the radiated emission limits specified in Section 15.209(a) (see Section 15.205(c)).

5.4. Test Procedure

The EUT and its simulators are placed on a turn table which is 0.8 meter above ground. The turn table can rotate 360 degrees to determine the position of the maximum emission level. The EUT was positioned such that the distance from antenna to the EUT was 3 meters.

The antenna can move up and down between 1 meter and 4 meters to find out the maximum emission level.

Both horizontal and vertical polarization of the antenna are set on measurement. In order to find the maximum emission, all of the interface cables must be manipulated according to ANSI C63.4:2003 on radiated measurement.

The bandwidth below 1GHz setting on the field strength meter is 120 kHz, above 1GHz are 1 MHz.

5.5. Uncertainty

± 3.9 dB above 1GHz

± 3.8 dB below 1GHz

5.6. Test Result of Band Edge

Product : Mobile Clinical Assistant C5
 Test Item : Band Edge
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2402MHz)


RF Radiated Measurement:

Channel No.	Frequency (MHz)	Required Limit (dBc)	Result
00	<2400	>20	Pass

RF Radiated Measurement (Horizontal):

Channel	Frequency (MHz)	Correct Factor (dB)	Reading Level (dBuV)	Emission Level (dBuV/m)	Peak Limit (dBuV/m)	Average Limit (dBuV/m)	Result
00 (Peak)	2390.000	-2.378	46.696	44.319	74.00	54.00	Pass
00 (Average)	--	--	--	--	74.00	54.00	Pass

Figure Channel 00: (Horizontal)

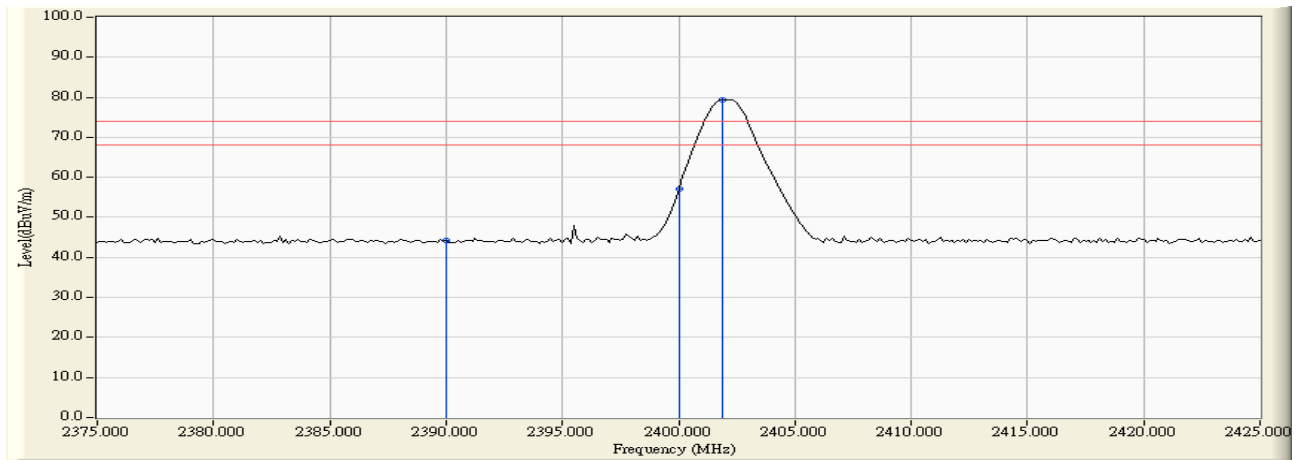

Note:

RBW=1MHz, VBW=1MHz, Sweep Time=500ms.

Product : Mobile Clinical Assistant C5
 Test Item : Band Edge
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2402MHz)


RF Radiated Measurement:

Channel No.	Frequency (MHz)	Required Limit (dBc)	Result
00	<2400	>20	Pass

RF Radiated Measurement (Vertical):

Channel	Frequency (MHz)	Correct Factor (dB)	Reading Level (dBuV)	Emission Level (dBuV/m)	Peak Limit (dBuV/m)	Average Limit (dBuV/m)	Result
00 (Peak)	2390.000	-2.378	46.300	43.923	74.00	54.00	Pass
00(Average)	--	--	--	--	74.00	54.00	Pass

Figure Channel 00: (Vertical)

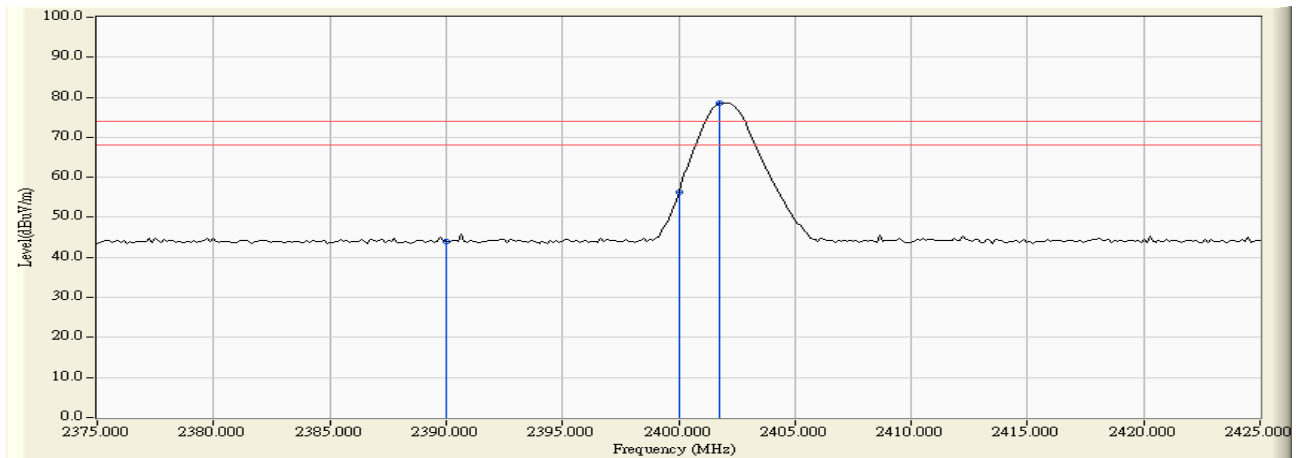

Note:

RBW=1MHz, VBW=1MHz, Sweep Time=500ms.

Product : Mobile Clinical Assistant C5
 Test Item : Band Edge
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2480MHz)


RF Radiated Measurement:

Channel No.	Frequency (MHz)	Required Limit (dBc)	Result
78	>2483.5	>20	Pass

RF Radiated Measurement (Horizontal):

Channel	Frequency (MHz)	Correct Factor (dB)	Reading Level (dBuV)	Emission Level (dBuV/m)	Peak Limit (dBuV/m)	Average Limit (dBuV/m)	Result
78(Peak)	2483.500	-1.937	46.451	44.514	74.00	54.00	Pass
78(Average)	--	--	--	--	74.00	54.00	Pass

Figure Channel 78: (Horizontal)

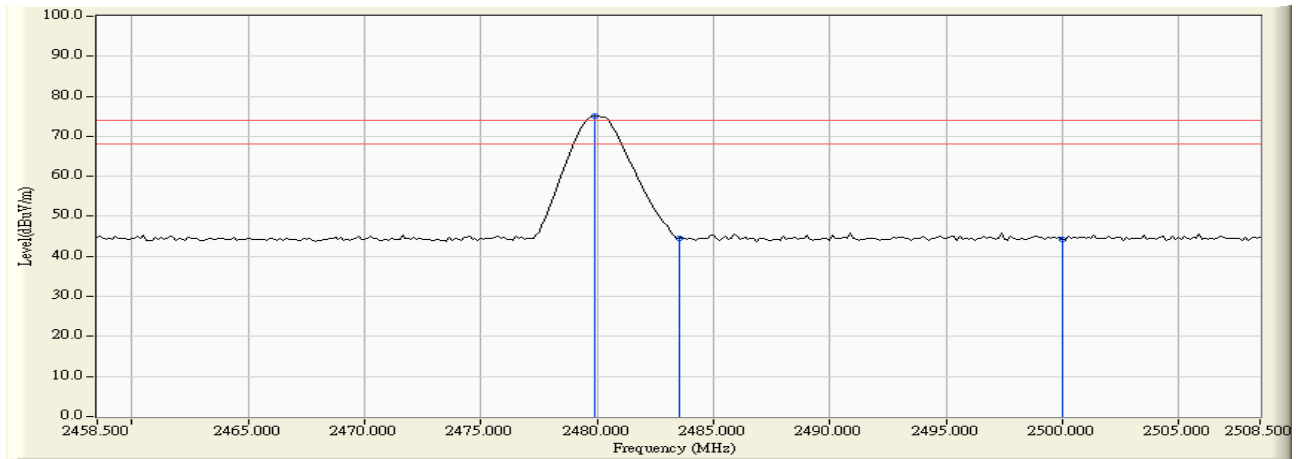

Note:

RBW=1MHz, VBW=1MHz, Sweep Time=500ms.

Product : Mobile Clinical Assistant C5
 Test Item : Band Edge
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2480MHz)


RF Radiated Measurement:

Channel No.	Frequency (MHz)	Required Limit (dBc)	Result
78	>2483.5	>20	Pass

RF Radiated Measurement (Vertical):

Channel	Frequency (MHz)	Correct Factor (dB)	Reading Level (dBuV)	Emission Level (dBuV/m)	Peak Limit (dBuV/m)	Average Limit (dBuV/m)	Result
78(Peak)	2498.125	-1.891	48.902	47.011	74.00	54.00	Pass
78(Average)	--	--	--	--	74.00	54.00	Pass

Figure Channel 78: (Vertical)

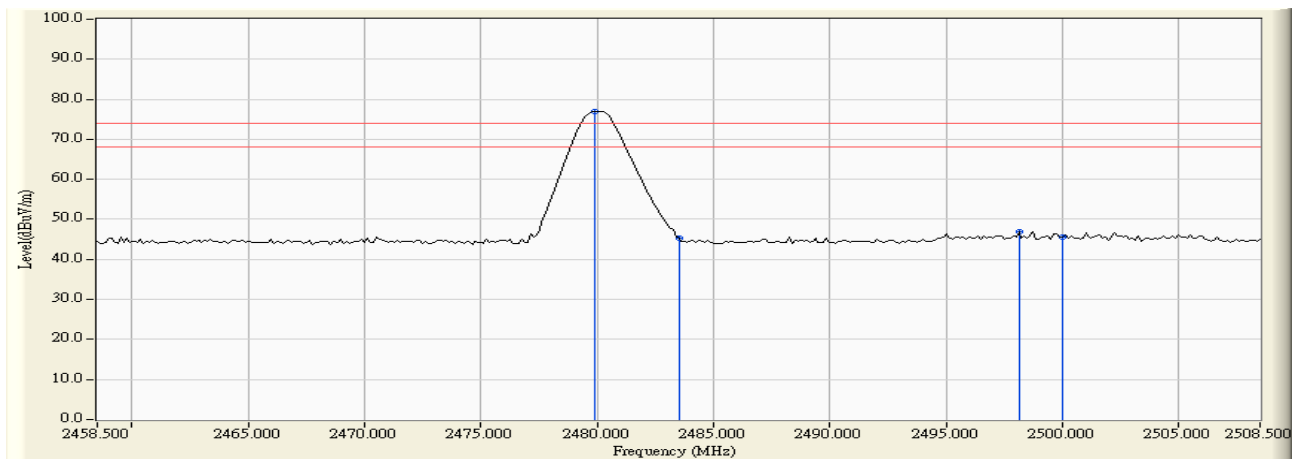

Note:

RBW=1MHz, VBW=1MHz, Sweep Time=500ms.

Note: The average measurement was not performed when the peak measured data under the limit of average detection. If the readings given are average, peak measurement should also be supplied.

6. Channel Number


6.1. Test Equipment

The following test equipments are used during the radiated emission tests:

	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
X	Test Receiver	R & S	ESI 26 / 838786 / 004	May, 2007
X	Spectrum Analyzer	Agilent	E4407B / US39440758	May, 2007

- Note:
1. All equipments are calibrated every one year.
 2. The test instruments marked by “X” are used to measure the final test results.

6.2. Test Setup

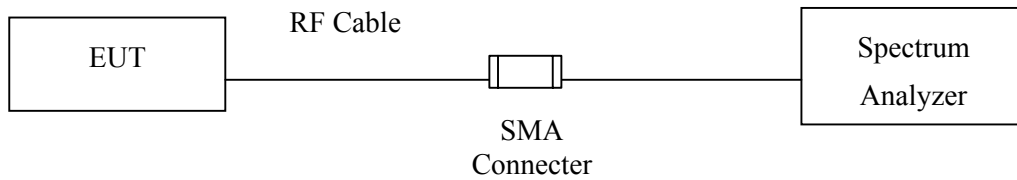

6.3. Limit

Frequency hopping systems operating in the 2400-2483.5 MHz bands shall use at least 75 hopping frequencies.

6.4. Uncertainty


N/A

6.5. Test Result of Channel Number

Product : Mobile Clinical Assistant C5
 Test Item : Channel Number
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter


Frequency Range (MHz)	Measurement (Hopping Channel)	Required Limit (Hopping Channel)	Result
2402 ~ 2480	79	>75	Pass

2402-2421MHz

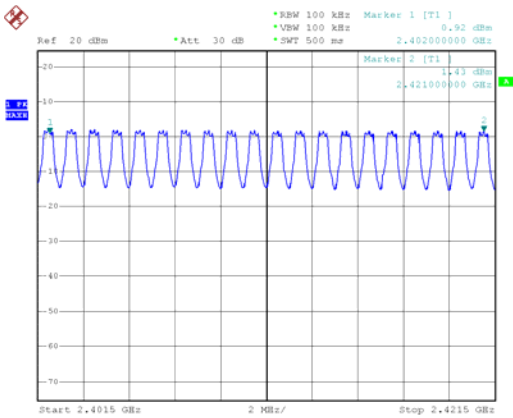


PN1
 Date: 5.MAY.2007 05:31:02

2422-2441MHz

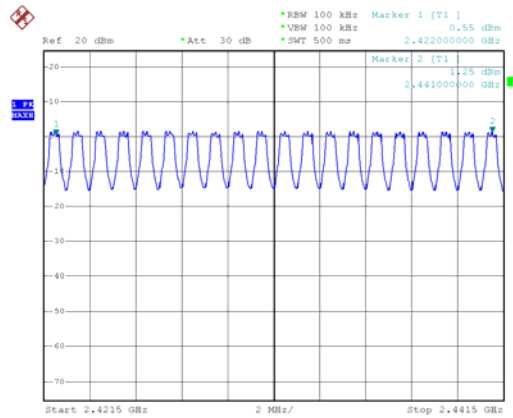


PN1
 Date: 5.MAY.2007 05:40:03

2442-2461MHz

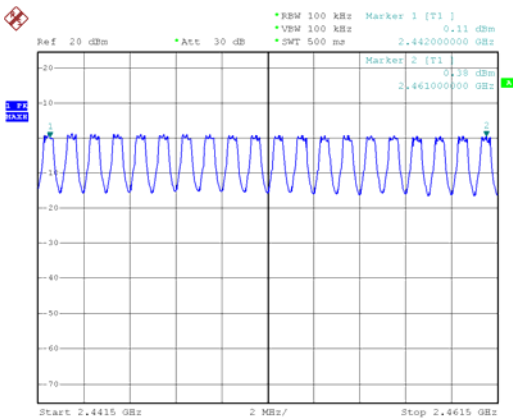

PN1
 Date: 5.MAY.2007 05:46:02

2462-2481MHz

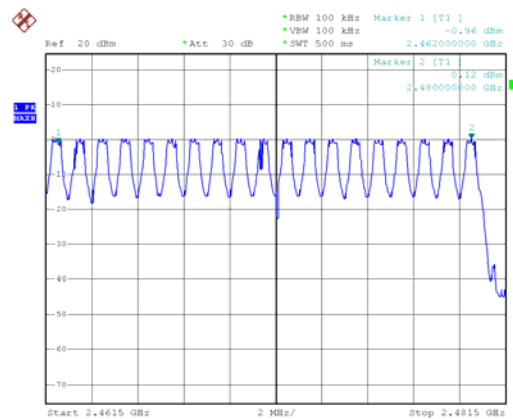

PN1
 Date: 5.MAY.2007 05:48:33

7. Channel Separation


7.1. Test Equipment

The following test equipments are used during the radiated emission tests:

	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
X	Test Receiver	R & S	ESI 26 / 838786 / 004	May, 2007
X	Spectrum Analyzer	Agilent	E4407B / US39440758	May, 2007

- Note: 1. All equipments are calibrated every one year.
 2. The test instruments mark by “X” are used to measure the final test results.

7.2. Test Setup

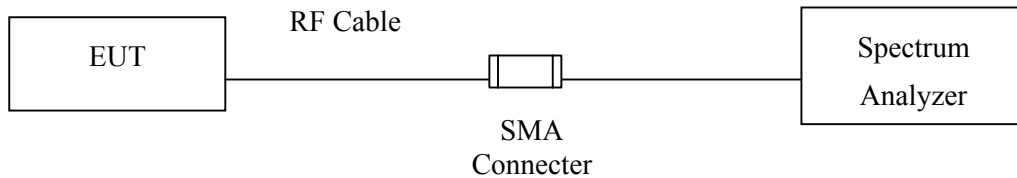

7.3. Limit

Frequency hopping systems shall have hopping channel carrier frequencies separated by a minimum of 25 kHz or the 20 dB bandwidth of the hopping channel, whichever is greater.

7.4. Uncertainty


± 150Hz

7.5. Test Result of Channel Separation

Product : Mobile Clinical Assistant C5
 Test Item : Channel Separation
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter


Frequency (MHz)	Measurement Level (MHz)	Required Limit	Result
2402	1.00	>25 kHz or 2/3 * 20 dB BW	Pass
2441	1.00	>25 kHz or 2/3 * 20 dB BW	Pass
2480	1.00	>25 kHz or 2/3 * 20 dB BW	Pass

Channel 00 2402MHz

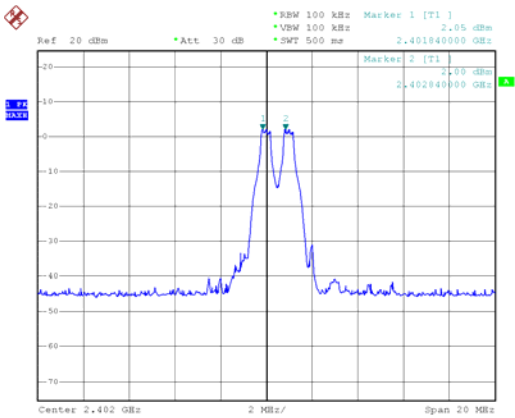


PN1
 Date: 5.MAY.2007 05:22:15

Channel 39 2441MHz

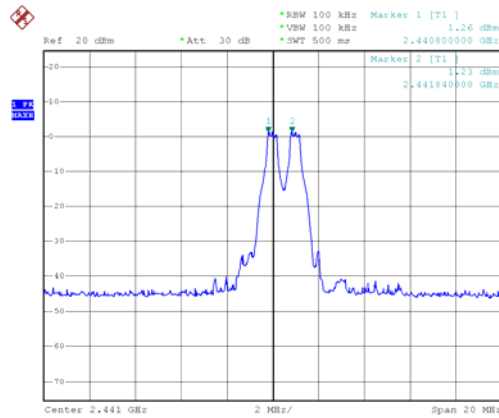

PN1
 Date: 5.MAY.2007 05:23:06

Channel 78 2480 MHz

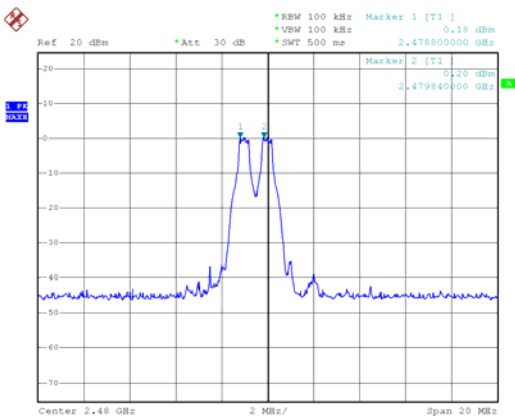

PN1
 Date: 5.MAY.2007 05:23:51

8. Dwell Time


8.1. Test Equipment

The following test equipments are used during the radiated emission tests:

	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
X	Test Receiver	R & S	ESI 26 / 838786 / 004	May, 2007
X	Spectrum Analyzer	Agilent	E4407B / US39440758	May, 2007

- Note: 1. All equipments are calibrated every one year.
 2. The test instruments marked by “X” are used to measure the final test results.

8.2. Test Setup

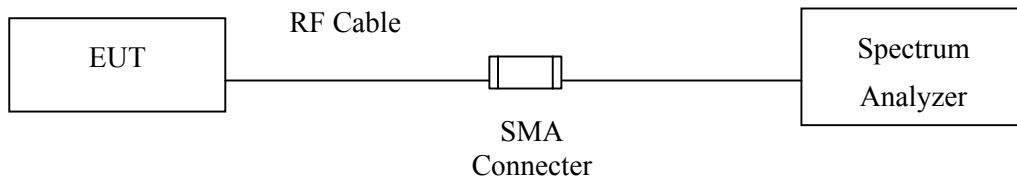

8.3. Limit

The dwell time shall be the average time of occupancy on any frequency shall not be greater than 0.4 seconds within a 30 second period.

8.4. Uncertainty

± 25msec


8.5. Test Result of Dwell Time

Product : Mobile Clinical Assistant C5
 Test Item : Dwell Time
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (Channel 00,39,78 –DH5)

Channel No.	Frequency (MHz)	Time Interval between hops (ms)	Transmission Time (us)	Dwell Time (ms)	Limit (ms)	Result
00	2402	296.818	2940	312.9998855	400	Pass
39	2441	298.618	2940	311.1131948	400	Pass
78	2480	298.618	2940	311.1131948	400	Pass


Note: Dwell Time = 79 * 400 / Time Interval Between Hops * Transmission Time / 1000

CH 2402MHz Time Interval between hops

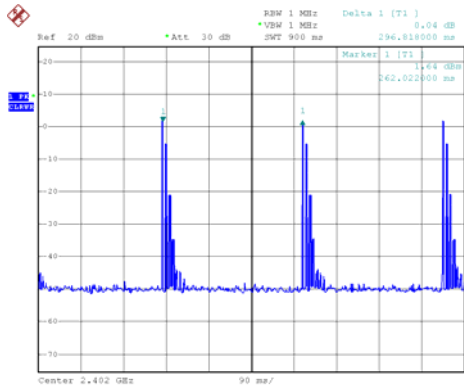


FN1
Date: 5.MAY.2007 07:03:23

Transmission Time

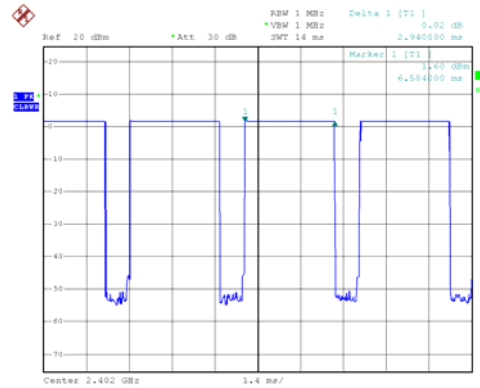


FN1
Date: 5.MAY.2007 07:05:16

CH 2441MHz Time Interval between hops

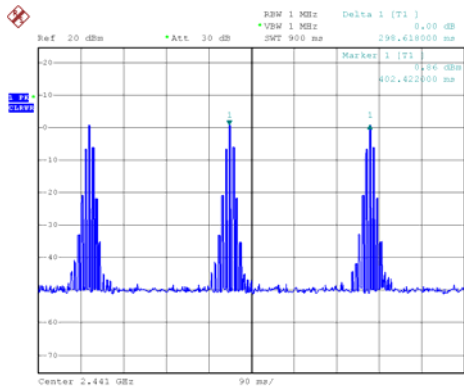


FN1
Date: 5.MAY.2007 07:04:05

Transmission Time

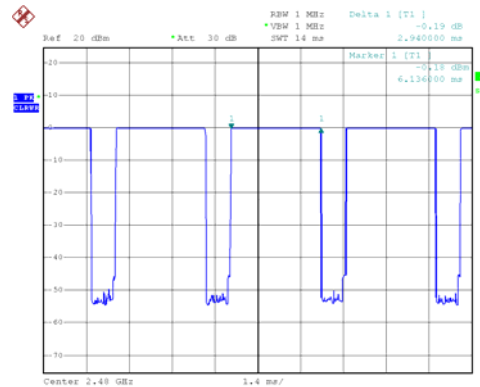


FN1
Date: 5.MAY.2007 07:06:43

CH 2480MHz Time Interval between hops

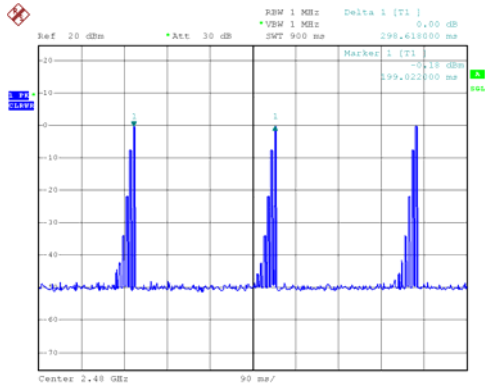

FN1
Date: 5.MAY.2007 07:04:34

Transmission Time

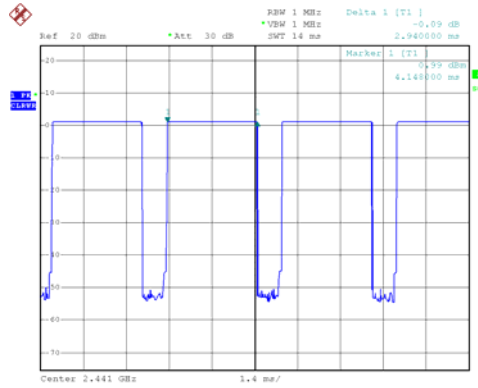

FN1
Date: 5.MAY.2007 09:24:37

Note:

The dwell times of the packet type of DH1, DH3, and DH3 are tested. Only the worst case is shown on the report.

9. Occupied Bandwidth


9.1. Test Equipment

The following test equipments are used during the radiated emission tests:

	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
X	Test Receiver	R & S	ESI 26 / 838786 / 004	May, 2007
X	Spectrum Analyzer	Agilent	E4407B / US39440758	May, 2007

- Note: 1. All equipments are calibrated every one year.
 2. The test instruments marked by “X” are used to measure the final test results.

9.2. Test Setup

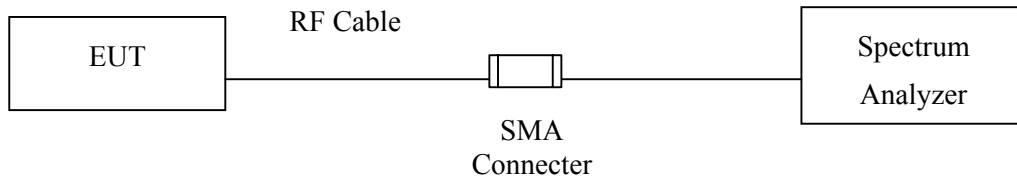

9.3. Limits

N/A

9.4. Uncertainty


± 150Hz

9.5. Test Result of Occupied Bandwidth

Product : Mobile Clinical Assistant C5
 Test Item : Occupied Bandwidth Data
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2402MHz)

Channel No.	Frequency (MHz)	Measurement Level (kHz)	Required Limit (kHz)	Result
00	2402	1160	--	NA

Figure Channel 00:

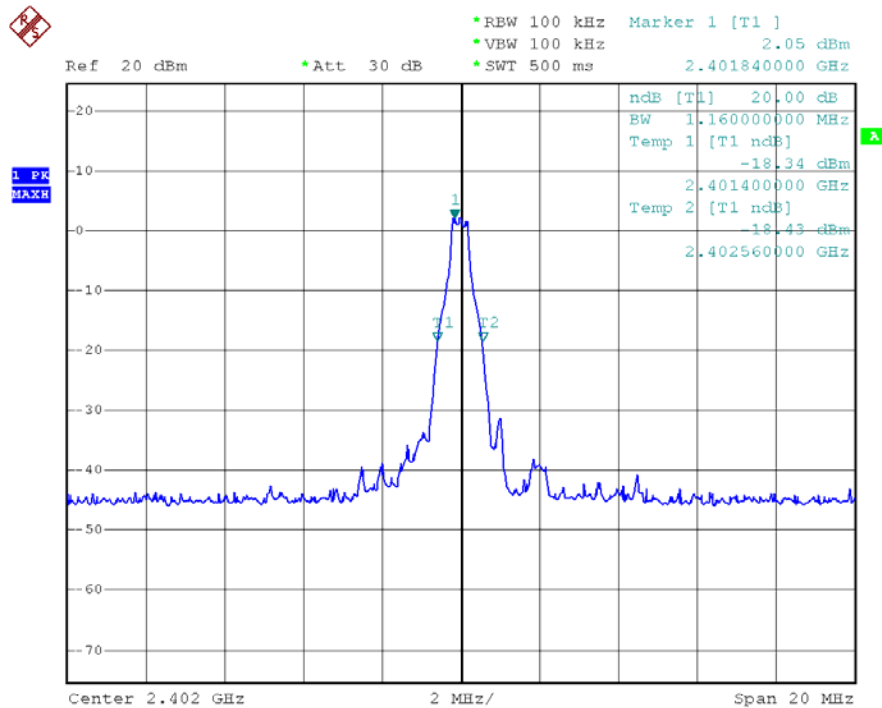


PN1
 Date: 5.MAY.2007 05:20:22

Product : Mobile Clinical Assistant C5
 Test Item : Occupied Bandwidth Data
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2441MHz)

Channel No.	Frequency (MHz)	Measurement Level (kHz)	Required Limit (kHz)	Result
39	2441	1160	--	NA

Figure Channel 39:

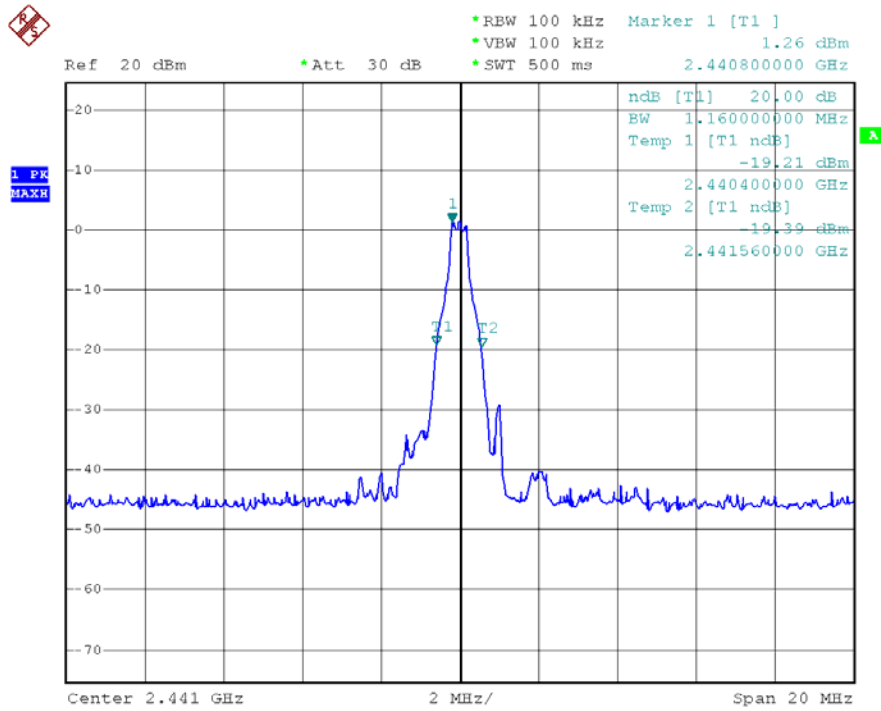


PN1

Date: 5.MAY.2007 05:20:55

Product : Mobile Clinical Assistant C5
 Test Item : Occupied Bandwidth Data
 Test Site : No.3 OATS
 Test Mode : Mode 1: Transmitter (2480MHz)

Channel No.	Frequency (MHz)	Measurement Level (kHz)	Required Limit (kHz)	Result
78	2480	1160	--	NA

Figure Channel 78:

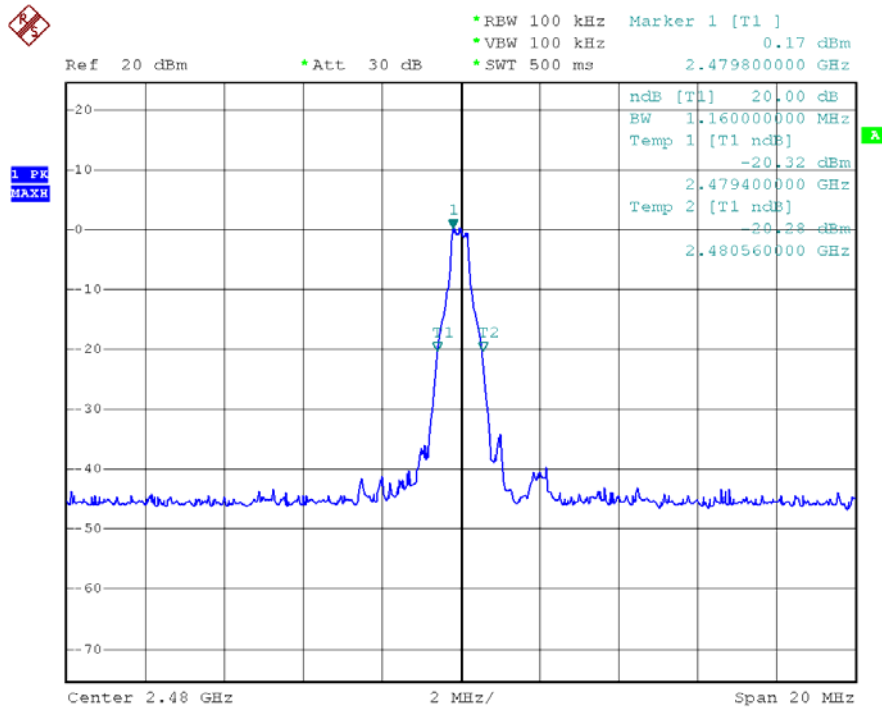

PN1

Date: 5.MAY.2007 05:21:16

10. EMI Reduction Method During Compliance Testing

No modification was made during testing.