

# **SAR Test Report**

Product Name : EeeKeyboard PC

Model No. : EK1542

Applicant: ASUSTeK COMPUTER INC.

Address : No. 150, Li-Te Rd., Peitou, Taipei, Taiwan, R.O.C.

Date of Receipt : 2009/08/10

Issued Date : 2009/08/18

Report No. : 098210R-HPUSP09V01

Report Version : V1.0

The test results relate only to the samples tested.

The test report shall not be reproduced except in full without the written approval of QuieTek Corporation.



# **Test Report Certification**

Issued Date: 2009/08/18

Report No.:098210R-HPUSP09V01

# QuieTek

Product Name : EeeKeyboard PC

Applicant : ASUSTeK COMPUTER INC.

Address : No. 150, Li-Te Rd., Peitou, Taipei, Taiwan, R.O.C.

Manufacturer : PROTEK (SHANGHAI) LIMITED

Model No. : EK1542
Trade Name : ASUS

FCC ID : MSQEK1542

Applicable Standard : FCC Oet65 Supplement C June 2001

IEEE Std. 1528-2003

47CFR § 2.1093

Test Result : Max. SAR Measurement (1g)

0.074 W/kg

Application Type : Certification

The test results relate only to the samples tested.

The test report shall not be reproduced except in full without the written approval of QuieTek Corporation.

Documented By : Needle Huang

(Engineering Adm. Assistant

/ Nicole Huang)

Tested By : Jung Chang

(Engineer / Jung Chang)

Approved By :

(Manager / Vincent Lin)



# TABLE OF CONTENTS

Desc	ription	Page
1.	General Information	5
	1.1 EUT Description	5
	1.2 Test Environment	6
2.	SAR Measurement System	7
	2.1 DASY5 System Description	7
	2.1.1 Applications	8
	2.1.2 Area Scans	8
	2.1.3 Zoom Scan (Cube Scan Averaging)	8
	2.1.4 Uncertainty of Inter-/Extrapolation and Averaging	8
	2.2 DASY5 E-Field Probe	9
	2.2.1 Isotropic E-Field Probe Specification	9
	2.3 Boundary Detection Unit and Probe Mounting Device	10
	2.4 DATA Acquisition Electronics (DAE) and Measurement Server	
	2.5 Robot	11
	2.6 Light Beam Unit	11
	2.7 Device Holder	12
	2.8 SAM Twin Phantom	12
3.	Tissue Simulating Liquid	13
	3.1 The composition of the tissue simulating liquid	
	3.2 Tissue Calibration Result	
	3.3 Tissue Dielectric Parameters for Head and Body Phantoms	14
4.	SAR Measurement Procedure	
	4.1 SAR System Validation	15
	4.1.1 Validation Dipoles	
	4.1.2 Validation Result	
	4.2 SAR Measurement Procedure	16
5.	SAR Exposure Limits	17
6.	Test Equipment List	
7.	Measurement Uncertainty	
8.	Test Results	
-	8.1 SAR Test Results Summary	
	Appendix	
	Appendix A. SAR System Validation Data	



Appendix B. SAR measurement Data

Appendix C. Test Setup Photographs & EUT Photographs

Appendix D. Probe Calibration Data

Appendix E. Dipole Calibration Data



# 1. General Information

# 1.1 EUT Description

Product Name	EeeKeyboard PC
Trade Name	ASUS
Model No.	EK1542
FCC ID	MSQEK1542
TX Frequency	2412MHz ~ 2462MHz
Number of Channel	11
Type of Modulation	DSSS/OFDM
Antenna Type	Printed on PCB
Antenna Kit	ACON: Main Antenna: APP6M-100000
Device Category	Portable
RF Exposure Environment	Uncontrolled
Max. Output Power	802.11b: 15.56 dBm
(Conducted)	802.11g: 20.49 dBm
	802.11n(20M): 19.58 dBm
	802.11n(40M): 19.51 dBm



#### 1.2 Test Environment

Ambient conditions in the laboratory:

Items	Required	Actual
Temperature (°C)	18-25	23.1
Humidity (%RH)	30-70	52

## Site Description:

Accredited by TAF Accredited Number: 0914

Effective through: December 12, 2011





Site Name: Quietek Corporation

Site Address: No. 5, Ruei-Shu Valley, Ruei-Ping Tsuen,

Lin-Kou Shiang, Taipei,

Taiwan, R.O.C.


TEL: 886-2-8601-3788 / FAX: 886-2-8601-3789

E-Mail: service@quietek.com



## 2. SAR Measurement System

## 2.1 DASY5 System Description

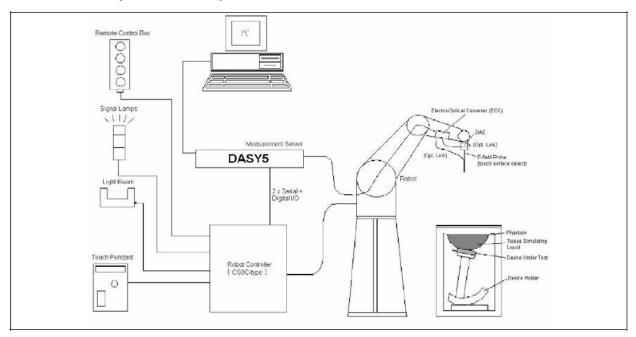

The DASY5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- > The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- A computer running WinXP and the DASY5 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.



#### 2.1.1 Applications

Predefined procedures and evaluations for automated compliance testing with all worldwide standards, e.g., IEEE 1528, OET 65, IEC 62209-1, IEC 62209-2, EN 50360, EN 50383 and others.

#### 2.1.2 Area Scans

Area scans are defined prior to the measurement process being executed with a user defined variable spacing between each measurement point (integral) allowing low uncertainty measurements to be conducted. Scans defined for FCC applications utilize a 10mm<sup>2</sup> step integral, with 1mm interpolation used to locate the peak SAR area used for zoom scan assessments.

When an Area Scan has measured all reachable points, it computes the field maxima found in the scanned area, within a range of the global maximum. The range (in dB) is specified in the standards for compliance testing. For example, a 2 dB range is required in IEEE 1528-2003, EN 50361 and IEC 62209 standards, whereby 3 dB is a requirement when compliance is assessed in accordance with the ARIB standard (Japan).

#### 2.1.3 Zoom Scan (Cube Scan Averaging)

Zoom Scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. A density of 1000 kg/m³ is used to represent the head and body tissue density and not the phantom liquid density, in order to be consistent with the definition of the liquid dielectric properties, i.e. the side length of the 1 g cube is 10mm, with the side length of the 10 g cube 21,5mm.

The zoom scan integer steps can be user defined so as to reduce uncertainty, but normal practice for typical test applications (including FCC) utilize a physical step of 5x5x7 (8mmx8mmx5mm) providing a volume of 32mm in the X & Y axis, and 30mm in the Z axis.

#### 2.1.4 Uncertainty of Inter-/Extrapolation and Averaging

In order to evaluate the uncertainty of the interpolation, extrapolation and averaged SAR calculation algorithms of the Postprocessor, DASY5 allows the generation of measurement grids which are artificially predefined by analytically based test functions. Therefore, the grids of area scans and zoom scans can be filled with uncertainty test data, according to the SAR benchmark functions of IEEE 1528. The three analytical functions shown in equations as below are used to describe the possible range of the expected SAR distributions for the tested handsets. The field gradients are covered by the spatially flat



distribution f1, the spatially steep distribution f3 and f2 accounts for H-field cancellation on the phantom/tissue surface.

$$f_1(x,y,z) = Ae^{-\frac{z}{2a}}\cos^2\left(\frac{\pi}{2}\frac{\sqrt{x'^2 + y'^2}}{5a}\right)$$

$$f_2(x,y,z) = Ae^{-\frac{z}{a}}\frac{a^2}{a^2 + x'^2}\left(3 - e^{-\frac{2z}{a}}\right)\cos^2\left(\frac{\pi}{2}\frac{y'}{3a}\right)$$

$$f_3(x,y,z) = A\frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2}\left(e^{-\frac{2z}{a}} + \frac{a^2}{2(a+2z)^2}\right)$$

#### 2.2 DASY5 E-Field Probe

The SAR measurement is conducted with the dosimetric probe manufactured by SPEAG. The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency.

SPEAG conducts the probe calibration in compliance with international and national standards (e.g. IEEE 1528, EN 62209-1, IEC 62209, etc.) under ISO 17025. The calibration data are in Appendix D.

#### 2.2.1 Isotropic E-Field Probe Specification

Model	Ex3DV4		
Construction	Symmetrical design with triangular core Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g.,		
	DGBE)	J , , , , , , ,	
Frequency	10 MHz to 6 GHz		
	Linearity: ± 0.2 dB (30 MHz to 6 GHz)		
Directivity	± 0.3 dB in HSL (rotation around probe axis)		
	± 0.5 dB in tissue material (rotation normal to	/	
	probe axis)		
Dynamic Range	10 μW/g to 100 mW/g		
	Linearity: ± 0.2 dB (noise: typically < 1 μW/g)		
Dimensions	Overall length: 330 mm (Tip: 20 mm)		
	Tip diameter: 2.5 mm (Body: 12 mm)		
	Typical distance from probe tip to dipole centers:		
	1 mm		
Application	High precision dosimetric measurements in any	•	
	(e.g., very strong gradient fields). Only pro		
	compliance testing for frequencies up to 6 GHz w	ith precision of better	
	30%.		



above 80dB.

#### 2.3 Boundary Detection Unit and Probe Mounting Device

The DASY probes use a precise connector and an additional holder for the probe, consisting of a plastic tube and a flexible silicon ring to center the probe. The connector at the DAE is flexibly mounted and held in the default position with magnets and springs. Two switching systems in the connector mount detect frontal and lateral probe collisions and trigger the necessary software response.



#### 2.4 DATA Acquisition Electronics (DAE) and Measurement Server

The data acquisition electronics (DAE) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit.

Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock. The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is



The DASY5 measurement server is based on a PC/104 CPU board with a 400MHz intel ULV Celeron, 128MB chipdisk and 128MB RAM. The necessary circuits for communication with the DAE electronics box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY5 I/O board, which is directly connected to the PC/104 bus of the CPU board.





#### 2.5 Robot

The DASY5 system uses the high precision robots TX90 XL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY5 system, the CS8C robot controller version from Stäubli is used.

The XL robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- 6-axis controller



#### 2.6 Light Beam Unit

The light beam switch allows automatic "tooling" of the probe. During the process, the actual position of the probe tip with respect to the robot arm is measured, as well as the probe length and the horizontal probe offset. The software then corrects all movements, such that the robot coordinates are valid for the probe tip.

The repeatability of this process is better than 0.1 mm. If a position has been taught with an aligned probe, the same position will be reached with another aligned probe within 0.1 mm, even if the other probe has different dimensions. During probe rotations, the probe tip will keep its actual position.





#### 2.7 Device Holder

The DASY5 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation center for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The DASY5 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity  $\epsilon r = 3$  and loss tangent  $\delta = 0.02$ . The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



#### 2.8 SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- Left head
- Right head
- Flat phantom



The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.



# 3. Tissue Simulating Liquid

## 3.1 The composition of the tissue simulating liquid

INGREDIENT	900MHz	1800MHz	2450MHz	2450MHz
(% Weight)	Head	Head	Head	Body
Water	-	-	46.7	73.2
Salt	-	-	0.00	0.04
Sugar			0.00	0.00
HEC			0.00	0.00
Preventol			0.00	0.00
DGBE			53.3	26.7

#### 3.2 Tissue Calibration Result

The dielectric parameters of the liquids were verified prior to the SAR evaluation using APREL Dielectric Probe Kit and Anritsu MS4623B Vector Network Analyzer.

Head Tissue Simulant Measurement					
Frequency	Description	Dielectric Pa	arameters	Tissue Temp.	
[MHz]	Description	ε <sub>r</sub>	σ [s/m]	[°C]	
	Reference result	40.1	1.78	N/A	
2450MHz	± 5% window	38.095 to 42.105	1.691 to 1.869	IN/A	
	14-Aug-09	39.36	1.83	22.5	

Body Tissue Simulant Measurement						
Frequency	Description	Dielectric P	Tissue Temp.			
[MHz]	Description	٤ <sub>٢</sub>	σ [s/m]	[°C]		
	Reference result	52.7	1.95	N/A		
2450MHz	± 5% window	50.065 to 55.335	1.8525 to 2.0475	19/74		
	14-Aug-09	52.83	1.97	22.5		
2412 MHz	Low channel	53.42	1.87	22.5		
2437 MHz	Mid channel	52.95	1.94	22.5		
2462 MHz	High channel	52.75	1.98	22.5		

Page: 13 of 21



#### 3.3 Tissue Dielectric Parameters for Head and Body Phantoms

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in P1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. Other head and body tissue parameters that have not been specified in P1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equations, as described by Dr. Camelia Gabriel and extrapolated according to the head parameters specified in P1528.

Target Frequency	He	ad	Во	dy
(MHz)	٤ <sub>r</sub>	σ (S/m)	٤ <sub>r</sub>	σ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800 – 2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00


( $\epsilon_r$  = relative permittivity,  $\sigma$  = conductivity and  $\rho$  = 1000 kg/m³)



#### 4. SAR Measurement Procedure

## 4.1 SAR System Validation

### 4.1.1 Validation Dipoles



The dipoles used is based on the IEEE-1528 standard, and is complied with mechanical and electrical specifications in line with the requirements of both IEEE and FCC Supplement C. the table below provides details for the mechanical and electrical specifications for the dipoles.

Frequency	L (mm)	h (mm)	d (mm)
2450MHz	53.5	30.4	3.6

#### 4.1.2 Validation Result

## **System Performance Check at 2450MHz**

Validation Kit: ASL-D-2450-S-2

Frequency [MHz]	Description	SAR [w/kg] 1g	SAR [w/kg] 10g	Tissue Temp. [°C]
2450 MHz	Reference result ± 10% window	48.07 43.263 to 52.877	25.65 23.085 to 28.215	N/A
	14-Aug-09	47.2	24.24	22.5

Note: All SAR values are normalized to 1W forward power.



#### 4.2 SAR Measurement Procedure

The ALSAS-10U calculates SAR using the following equation,

$$SAR = \frac{\sigma |E|^2}{\rho}$$

σ: represents the simulated tissue conductivity

ρ: represents the tissue density

The EUT is set to transmit at the required power in line with product specification, at each frequency relating to the LOW, MID, and HIGH channel settings.

Pre-scans are made on the device to establish the location for the transmitting antenna, using a large area scan in either air or tissue simulation fluid.

The EUT is placed against the Universal Phantom where the maximum area scan dimensions are larger than the physical size of the resonating antenna. When the scan size is not large enough to cover the peak SAR distribution, it is modified by either extending the area scan size in both the X and Y directions, or the device is shifted within the predefined area.

The area scan is then run to establish the peak SAR location (interpolated resolution set at 1mm<sup>2</sup>) which is then used to orient the center of the zoom scan. The zoom scan is then executed and the 1g and 10g averages are derived from the zoom scan volume (interpolated resolution set at 1mm<sup>3</sup>).



## 5. SAR Exposure Limits

SAR assessments have been made in line with the requirements of IEEE-1528, FCC Supplement C, and comply with ANSI/IEEE C95.1-1992 "Uncontrolled Environments" limits. These limits apply to a location, which is deemed as "Uncontrolled Environment" which can be described as a situation where the general public may be exposed to an RF source with no prior knowledge or control over their exposure.

### Limits for General Population/Uncontrolled Exposure (W/kg)

Type Exposure	Uncontrolled Environment Limit
Spatial Peak SAR (1g cube tissue for brain or body)	1.60 W/kg
Spatial Average SAR (whole body)	0.08 W/kg
Spatial Peak SAR (10g for hands, feet, ankles and wrist)	4.00 W/kg



# 6. Test Equipment List

Instrument	Manufactur	Model No.	Serial No.	Last	Next
	er			Calibration	Calibration
Stäubli Robot TX60L	Stäubli	TX60L	F09/5BL1A1/A06	May. 2009	only once
Controller	Speag	CS8c	N/A	May. 2009	only once
Aprel Reference Dipole 2450MHz	Aprel	ALS-D-2450-S-2	QTK-319	May. 2008	May. 2010
SAM Twin Phantom	Speag	QD000 P40 CA	Tp 1515	N/A	N/A
Device Holder	Speag	N/A	N/A	N/A	N/A
Data Acquisition Electronic	Speag	DAE4	1204	Apr. 2009	Apr. 2010
E-Field Probe	Speag	EX3DV4	3602	May. 2009	May. 2010
SAR Software	Speag	DASY5	V5.0 Build 125	N/A	N/A
Aprel Dipole Spaccer	Aprel	ALS-DS-U	QTK-295	N/A	N/A
Power Amplifier	Mini-Circuit	ZHL-42	D051404-20	N/A	N/A
Directional Coupler	Agilent	778D-012	50550	N/A	N/A
Universal Radio Communication	R&S	CMU 200	104846	May. 2009	May. 2010
Tester					
Vector Network	Anritsu	MS4623B	992801	Aug. 2009	Aug. 2010
Signal Generator	Anritsu	MG3692A	042319	Jun. 2009	Jun. 2010
Power Meter	Anritsu	ML2487A	6K00001447	Apr. 2009	Apr. 2010
Wide Bandwidth Sensor	Anritsu	MA2491	030677	Apr. 2009	Apr. 2010



# 7. Measurement Uncertainty

Uncertainty								
1882 - 535	Uncertainty	Prob.	Div.	$(c_i)$	$(c_i)$	Std. Unc.	Std. Unc.	$(v_i)$
Error Description	value	Dist.		1g	10g	(1g)	(10g)	$v_{eff}$
Measurement System	1							
Probe Calibration	$\pm 5.9 \%$	N	1	1	1	$\pm 5.9 \%$	$\pm 5.9 \%$	$\infty$
Axial Isotropy	$\pm 4.7 \%$	R.	$\sqrt{3}$	0.7	0.7	$\pm 1.9\%$	$\pm 1.9\%$	$\infty$
Hemispherical Isotropy	$\pm 9.6\%$	R	$\sqrt{3}$	0.7	0.7	$\pm 3.9\%$	$\pm 3.9\%$	$\infty$
Boundary Effects	$\pm 1.0\%$	R	$\sqrt{3}$	1	1	$\pm 0.6 \%$	$\pm 0.6 \%$	$\infty$
Linearity	$\pm 4.7 \%$	R	$\sqrt{3}$	1	1	$\pm 2.7 \%$	±2.7%	$\infty$
System Detection Limits	±1.0%	R	$\sqrt{3}$	1	1	$\pm 0.6 \%$	±0.6 %	$\infty$
Readout Electronics	±0.3 %	N	1	1	1	$\pm 0.3 \%$	±0.3%	$\infty$
Response Time	±0.8%	R	$\sqrt{3}$	1	1	$\pm 0.5 \%$	$\pm 0.5 \%$	$\infty$
Integration Time	$\pm 2.6 \%$	R	$\sqrt{3}$	1	1	$\pm 1.5\%$	$\pm 1.5 \%$	$\infty$
RF Ambient Noise	±3.0%	R.	$\sqrt{3}$	1	1	$\pm 1.7 \%$	$\pm 1.7\%$	$\infty$
RF Ambient Reflections	±3.0%	R	$\sqrt{3}$	1	1	$\pm 1.7 \%$	$\pm 1.7\%$	$\infty$
Probe Positioner	±0.4 %	R	$\sqrt{3}$	1	1	$\pm 0.2 \%$	$\pm 0.2\%$	$\infty$
Probe Positioning	$\pm 2.9 \%$	R	$\sqrt{3}$	1	1	$\pm 1.7 \%$	±1.7%	$\infty$
Max. SAR Eval.	±1.0%	R	$\sqrt{3}$	1	1	$\pm 0.6 \%$	±0.6%	$\infty$
Test Sample Related				- 10				
Device Positioning	$\pm 2.9 \%$	N	1	1	1	$\pm 2.9 \%$	$\pm 2.9 \%$	145
Device Holder	$\pm 3.6 \%$	N	1	1	1	$\pm 3.6\%$	$\pm 3.6 \%$	5
Power Drift	±5.0%	R	$\sqrt{3}$	1	1	$\pm 2.9 \%$	$\pm 2.9 \%$	$\infty$
Phantom and Setup			- 7					
Phantom Uncertainty	±4.0%	R	$\sqrt{3}$	1	1	$\pm 2.3\%$	$\pm 2.3\%$	$\infty$
Liquid Conductivity (target)	±5.0%	R	$\sqrt{3}$	0.64	0.43	±1.8 %	$\pm 1.2 \%$	$\infty$
Liquid Conductivity (meas.)	$\pm 2.5 \%$	N	1	0.64	0.43	±1.6 %	±1.1 %	$\infty$
Liquid Permittivity (target)	±5.0%	R	$\sqrt{3}$	0.6	0.49	±1.7 %	$\pm 1.4\%$	$\infty$
Liquid Permittivity (meas.)	$\pm 2.5 \%$	N	1	0.6	0.49	$\pm 1.5 \%$	±1.2%	$\infty$
Combined Std. Uncertainty						$\pm 10.9 \%$	±10.7 %	387
Expanded STD Uncertainty						$\pm 21.9 \%$	$\pm 21.4 \%$	



## 8. Test Results

# 8.1 SAR Test Results Summary

SAR MEAS	UREMENT						
Ambient Temperature (°C) : 23.1 ±2				Relative Humidity (%): 52			
Liquid Temperature (°C) : 22.5 ±2			Depth of Liquid (cm):>15				
Product: Eeel	Keyboard PC						
Test Mode: 80	02.11g						
Test Position Body	Antenna Position	Frequency		Conducted Power	SAR 1g	Limit	
		Channel	MHz	(dBm)	(W/kg)	(W/kg)	
Bottom	Fixed	6	2437	20.49	0.021	1.6	
Test Mode: 802.11b							
Bottom	Fixed	1	2412	15.56	0.060	1.6	
Bottom	Fixed	6	2437	15.49	0.070	1.6	
Bottom	Fixed	11	2462	15.54	0.074	1.6	
Test Mode: 802.11n(20M)							
Bottom	Fixed	6	2437	19.58	0.054	1.6	
Test Mode: 802.11n(40M)							
Bottom	Fixed	6	2437	19.51	0.00762	1.6	
				1			



## **Appendix**

**Appendix A. SAR System Validation Data** 

Appendix B. SAR measurement Data

**Appendix C. Test Setup Photographs & EUT Photographs** 

**Appendix D. Probe Calibration Data** 

**Appendix E. Dipole Calibration Data** 



#### Appendix A. SAR System Validation Data

Date/Time: 8/14/2009

Test Laboratory: QuieTek

SystemPerformanceCheck-2450

**DUT: Dipole 2450 MHz; Type: ALS-D-2450-S-2; Serial: QTK-319** 

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz;  $\sigma = 1.83$  mho/m;  $\epsilon_r = 39.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

**DASY4** Configuration:

- Probe: EX3DV4 SN3602; ConvF(7.1, 7.1, 7.1); Calibrated: 5/20/2009
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1207; Calibrated: 4/7/2009
- Phantom: SAM with CRP; Type: SAM
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

## d=10mm, Pin=250mW(24dBm), dist=4.0mm (EX-Probe)/Area Scan (7x7x1):


Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 18.6 mW/g

# d=10mm, Pin=250mW(24dBm), dist=4.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.5 V/m; Power Drift = -0.043 dB

Peak SAR (extrapolated) = 26.1 W/kg

SAR(1 g) = 11.8 mW/g; SAR(10 g) = 6.06 mW/g Maximum value of SAR (measured) = 18.8 mW/g

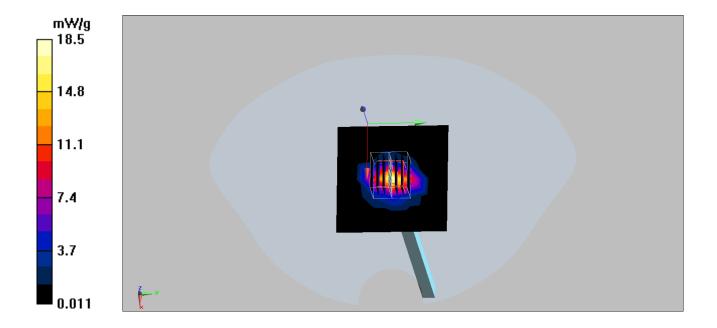



#### Appendix B. SAR measurement Data

Date/Time: 8/14/2009

Test Laboratory: QuieTek

802.11g\_6

DUT: EeeKeyboard PC; Type: EK1542

Communication System: 802.11b,g,n; Frequency: 2437 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2437 MHz;  $\sigma = 1.94$  mho/m;  $\varepsilon_r = 53$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

**DASY4** Configuration:

- Probe: EX3DV4 SN3602; ConvF(6.9, 6.9, 6.9); Calibrated: 5/20/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1207; Calibrated: 4/7/2009
- Phantom: SAM Left Table; Type: SAM;
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125


**Body/Area Scan (9x11x1):** Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 0.025 mW/g

**Body/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 1.5 V/m; Power Drift = 0.109 dB

Peak SAR (extrapolated) = 0.041 W/kg

SAR(1 g) = 0.021 mW/g; SAR(10 g) = 0.00946 mW/g Maximum value of SAR (measured) = 0.027 mW/g

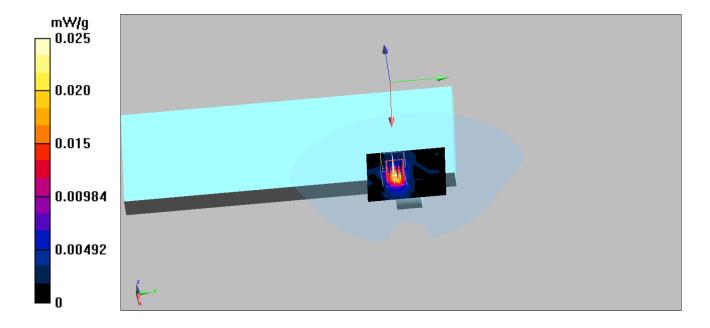



Test Laboratory: QuieTek

#### 802.11b 1

**DUT: EeeKeyboard PC: Type: EK1542** 

Communication System: 802.11b,g,n; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2412 MHz;  $\sigma = 1.87 \text{ mho/m}$ ;  $\epsilon_r = 53.4$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

**DASY4** Configuration:

- Probe: EX3DV4 SN3602; ConvF(6.9, 6.9, 6.9); Calibrated: 5/20/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1207; Calibrated: 4/7/2009 Phantom: SAM Left Table; Type: SAM;
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125


Body/Area Scan (9x11x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 0.067 mW/g

Body/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 2.87 V/m; Power Drift = 0.071 dB

Peak SAR (extrapolated) = 0.148 W/kg

SAR(1 g) = 0.066 mW/g; SAR(10 g) = 0.028 mW/gMaximum value of SAR (measured) = 0.077 mW/g

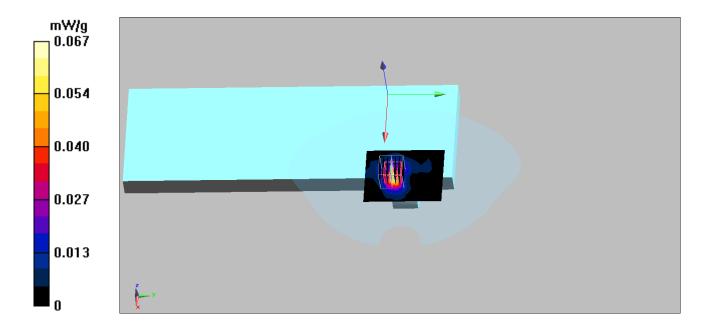



Test Laboratory: QuieTek

#### 802.11b 6

**DUT: EeeKeyboard PC: Type: EK1542** 

Communication System: 802.11b,g,n; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium parameters used: f = 2437 MHz;  $\sigma = 1.94 \text{ mho/m}$ ;  $\epsilon_r = 53$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

**DASY4** Configuration:

- Probe: EX3DV4 SN3602; ConvF(6.9, 6.9, 6.9); Calibrated: 5/20/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1207; Calibrated: 4/7/2009 Phantom: SAM Left Table; Type: SAM;
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125


Body/Area Scan (9x11x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 0.075 mW/g

Body/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 3.75 V/m; Power Drift = -0.074 dB

Peak SAR (extrapolated) = 0.157 W/kg

SAR(1 g) = 0.070 mW/g; SAR(10 g) = 0.030 mW/gMaximum value of SAR (measured) = 0.080 mW/g

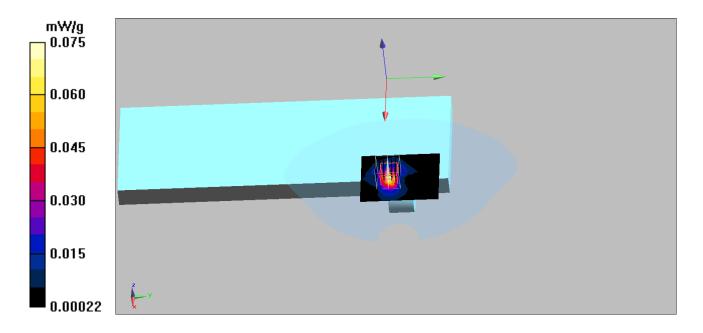



Test Laboratory: QuieTek

#### 802.11b 11

DUT: EeeKeyboard PC; Type: EK1542

Communication System: 802.11b,g,n; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz;  $\sigma = 1.98 \text{ mho/m}$ ;  $\epsilon_r = 52.8$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

**DASY4** Configuration:

- Probe: EX3DV4 SN3602; ConvF(6.9, 6.9, 6.9); Calibrated: 5/20/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1207; Calibrated: 4/7/2009
  Phantom: SAM Left Table; Type: SAM;
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125


Body/Area Scan (9x11x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 0.078 mW/g

Body/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 2.65 V/m; Power Drift = 0.119 dB

Peak SAR (extrapolated) = 0.159 W/kg

SAR(1 g) = 0.074 mW/g; SAR(10 g) = 0.032 mW/gMaximum value of SAR (measured) = 0.087 mW/g

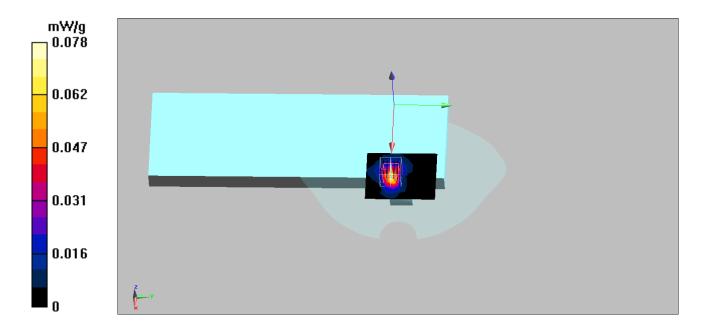



Test Laboratory: QuieTek

#### 802.11n 11 20M

DUT: EeeKeyboard PC; Type: EK1542

Communication System: 802.11b,g,n; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz;  $\sigma = 1.98 \text{ mho/m}$ ;  $\epsilon_r = 52.8$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

**DASY4** Configuration:

- Probe: EX3DV4 SN3602; ConvF(6.9, 6.9, 6.9); Calibrated: 5/20/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1207; Calibrated: 4/7/2009
  Phantom: SAM Left Table; Type: SAM;
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125


Body/Area Scan (9x11x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 0.059 mW/g

Body/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 2.23 V/m; Power Drift = 0.100 dB

Peak SAR (extrapolated) = 0.127 W/kg

SAR(1 g) = 0.054 mW/g; SAR(10 g) = 0.023 mW/gMaximum value of SAR (measured) = 0.064 mW/g

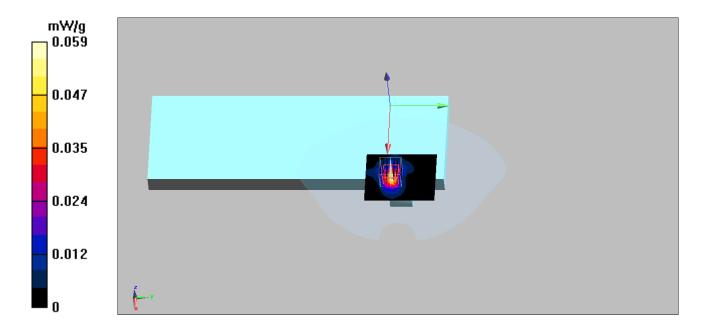



Test Laboratory: QuieTek

#### 802.11n 9 40M

**DUT: EeeKeyboard PC: Type: EK1542** 

Communication System: 802.11b,g,n; Frequency: 2452 MHz;Duty Cycle: 1:1

Medium parameters used: f = 2452 MHz;  $\sigma = 1.97 \text{ mho/m}$ ;  $\epsilon_r = 52.8$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

**DASY4** Configuration:

- Probe: EX3DV4 SN3602; ConvF(6.9, 6.9, 6.9); Calibrated: 5/20/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1207; Calibrated: 4/7/2009 Phantom: SAM Left Table; Type: SAM;
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125

Body/Area Scan (9x11x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (measured) = 0.0074 mW/g

Body/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm,


dz=5mm

Reference Value = 2.09 V/m; Power Drift = -0.1 dB

Peak SAR (extrapolated) = 0.00678 W/kg

SAR(1 g) = 0.00762 mW/g; SAR(10 g) = 0.00238 mW/g


Maximum value of SAR (measured) = 0.00302 mW/g

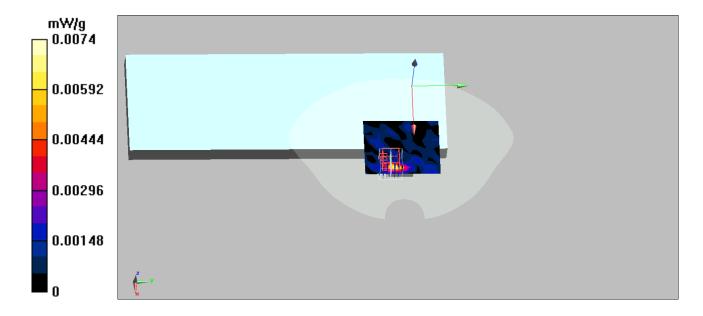



# 802.11b EUT Bottom Z-Axis plot

Channel: 11

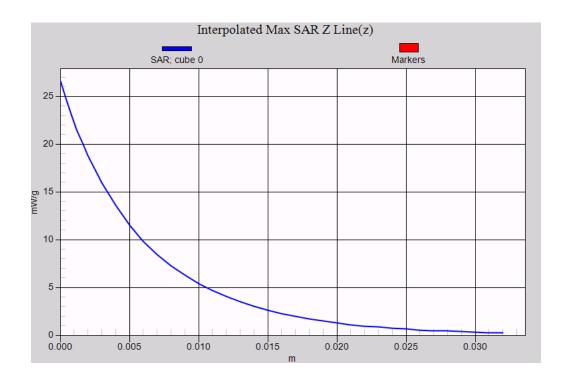



# Appendix C. Test Setup Photographs & EUT Photographs Test Setup Photographs

## **EUT Bottom**



Note: The positions used in the measurements were according to IEEE 1528-2003.




# **EUT Photographs**









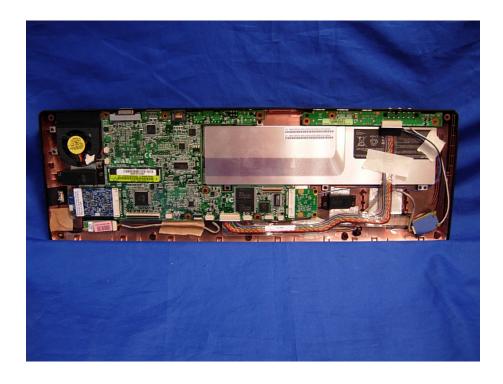













# **Appendix D. Probe Calibration Data**

**Miniature Isotropic RF Probe** 

S/N: 3602

### Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerlscher Kallbrierdienst Service sulsse d'étalonnage Servizio svizzero di taratura Swiss Callbration Service

Ancredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration contificates

Client

Quietek (Auden)

Accreditation No.: SCS 108

C

Certificate No: EX3-3602 May09

## **CALIBRATION CERTIFICATE**

Object EX3DV4 - SN:3602

Calibration procedure(s) QA CAL-01.v6, QA CAL-14.v3 and QA CAL-23.v3

Calibration procedure for dosimetric E-field probes

Calibration date: May 20, 2009

Condition of the calibrated item In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%...

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	# כוו	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	1-Apr-09 (No. 217-01030)	Apr-10
Power sensor E4412A	MY41495277	1-Apr-09 (No. 217-01030)	Apr-10
Power sensor E4412A	MY41498087	1-Apr-09 (No. 217-01030)	Apr-10
Reference 3 dB Attenuator	SN: S5054 (3c)	31-Mar-09 (No. 217-01026)	Mar-10
Reference 20 d8 Attenuator	SN: S5086 (20b)	31-Mar-09 (No. 217-01028)	Mar-10
Reference 30 dB Attenuator	SN: S5129 (30b)	31-Mar-09 (No. 217-01027)	Mar-10
Reference Probe ES3DV2	SN: 3013	2-Jan-09 (No. ES3-3013_Jan09)	Jan-10
DAE4	SN: 660	9-Sep-08 (No. DAE4-660_Sep08)	Sep-09
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Oct-07)	In house check: Oct-09
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-08)	In house check; Oct-09
	Name	Function	Signature
Calibrated by:	Katja Pokovic	Technical Manager	00 100

Approved by: Niels Kuster Quality Manage

Issued: May 20, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: EX3-3602\_May09

Page 1 of 9

## Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerlschor Kalibrierdienst S Sarvice suisse d'étalonnage C Servizio svizzero di taratura S **Swiss Calibration Service** 

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilatoral Agreement for the recognition of calibration certificates Accreditation No.: SCS 108

#### Glossary:

tissue simulating liquid TSL NORMx,y,z sensitivity in free space.

ConvE sensitivity in T\$L / NORMx,y,z DCP diode compression point φ rotation around probe axis Polarization φ

9 rotation around an axis that is in the plane normal to probe axis (at Polarization 3:

measurement center), i.e., 9 = 0 is normal to probe axis

#### Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,v.z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz; R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx.v.z does not effect the E<sup>2</sup>-field uncertainty inside TSL (see below *ConvF*).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx, v, z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm$  50 MHz to  $\pm$  100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: EX3-3602\_May09

# Probe EX3DV4

SN:3602

Manufactured: March 23, 2009 Calibrated: May 20, 2009

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: EX3-3602 May09 Page 3 of 9

## DASY - Parameters of Probe: EX3DV4 SN:3602

Sensitivity in Free Space <sup>A</sup>			Diode C	<b>ompressi</b> or	۱ <sup>B</sup>
NormX	<b>0.41</b> ± 10.1%	$\mu V / (V/m)^2$	DCP X	87 mV	
NormY	<b>0.40</b> ± 10.1%	$\mu V/(V/m)^2$	DCP Y	<b>89</b> mV	
NormZ	<b>0.52</b> ± 10.1%	$\mu V/(V/m)^2$	DCP Z	89 mV	

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

## Boundary Effect

I Q C TILLIE T PROPERTY OF THE PARTY OF THE	TSL	900 MHz	<ul> <li>Typical SAR gradient: 5 % per n</li> </ul>	nm
---	-----	---------	---	----

Sensor Center t	o Phantom Surface Distance	2.0 mm	3.0 mm
SAR <sub>be</sub> [%]	Without Correction Algorithm	10.2	6.1
SAR <sub>ue</sub> [%]	With Correction Algorithm	0.9	0.6

TSL 1810 MHz Typical SAR gradient: 10 % per mm

Sensor Center t	o Phantom Surface Distance	2.0 mm	3.0 mm
SAR <sub>be</sub> [%]	Without Correction Algorithm	6.7	2.9
SAR <sub>es</sub> [%]	With Correction Algorithm	0.5	0.3

### Sensor Offset

Probe Tip to Sensor Center

1.0 mm


The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>&</sup>lt;sup>6</sup> The uncertainties of NormX,Y,7 do not affect the E<sup>2</sup>-field uncertainty inside FSI, (see Page 8).

Numerical linearization parameter; uncertainty not required.


## Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

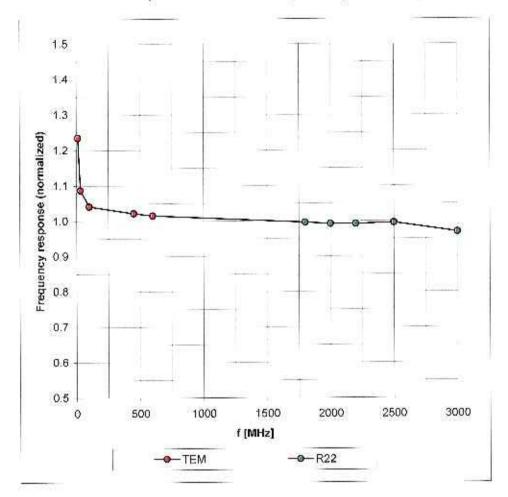

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

## Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

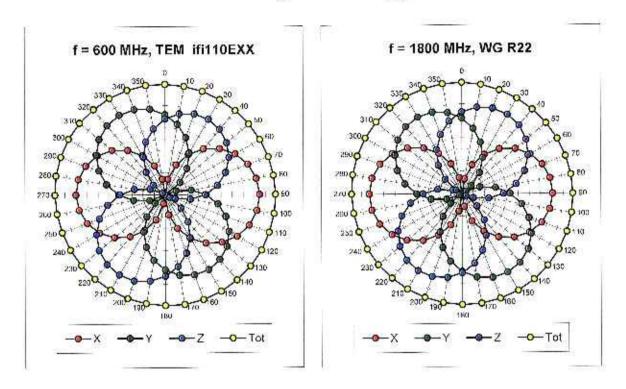


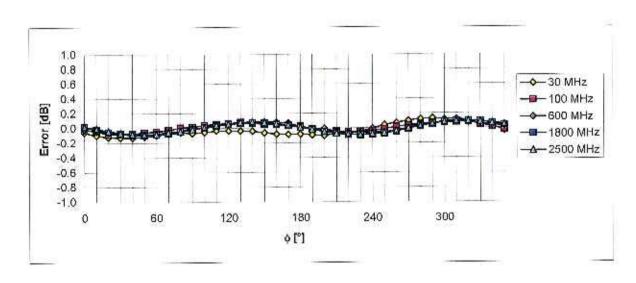

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

## Dynamic Range f(SAR<sub>head</sub>)

(Waveguide R22, f = 1800 MHz)

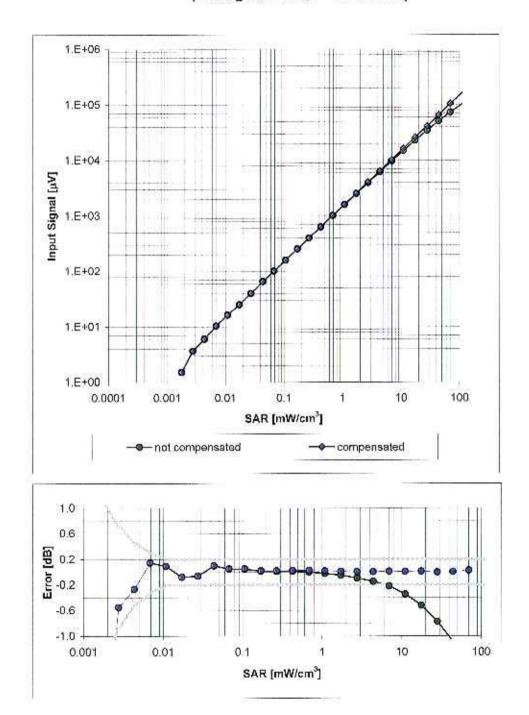

Uncertainty of Linearity Assessment: ± 0.6% (k=2)


## **Conversion Factor Assessment**

f [MHz]	Validity [MHz] <sup>c</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
835	± 50 / ± 100	Head	41.5 ± 5%	0.90 ± 5%	0.56	0.71	9.14 ± 11.0% (k=2)
900	± 50 / ± 100	Head	41.5 ± 5%	$0.97 \pm 5\%$	0.65	0.65	8.86 ± 11.0% (k=2)
1810	± 50 / ± 100	Head	$40.0 \pm 5\%$	$1.40 \pm 5\%$	0.84	0.55	7.81 ± 11.0% (k=2)
1950	$\pm 50 / \pm 100$	Head	$40.0 \pm 5\%$	$1.40\pm5\%$	0.84	0.56	7.55 ± 11.0% (k=2)
2450	$\pm$ 50 / $\pm$ 100	Head	39.2 ± 5%	$1.80 \pm 5\%$	0.46	0.70	7.10 $\pm$ 11.0% (k=2)
2600	± 50 / ± 100	Head	39.0 ± 5%	1.96 ± 5%	0.41	0.77	7.10 ± 11.0% (k=2)
3500	± 50 / ± 100	Head	$37.9 \pm 5\%$	2.91 ± 5%	0.42	1.00	6.26 ± 13.1% (k=2)
5200	± 50 / ± 100	Head	36.0 ± 5%	4. <del>6</del> 6 ± 5%	0.43	1.75	4.79 ± 13.1% (k=2)
<b>5</b> 300	± 50 / ± 100	Head	$35.9 \pm 5\%$	$4.76 \pm 5\%$	0.43	1.75	4.43 ± 13.1% (k=2)
5500	± 50 / ± 100	Head	35.8 ± 5%	$4.96\pm5\%$	0.50	1.75	4.44 ± 13.1% (k=2)
5600	± 50 / ± 100	Head	$35.5\pm5\%$	$5.07 \pm 5\%$	0.50	1.75	4.42 ± 13.1% (k=2)
5800	± 50 / ± 100	Head	$35.3\pm5\%$	5.27 ± 5%	0.52	1.75	4.21 ± 13.1% (k=2)
835	± 50 / ± 100	Body	55.2 ± 5%	$0.97 \pm 5\%$	0.72	0.65	9.32 ± 11.0% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.55	0.74	8.97 ± 11.0% (k=2)
1810	±50/±100	Body	53.3 ± 5%	1.52 ± 5%	0.70	0.85	7.97 ± 11.0% (k=2)
1950	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.48	0.78	7.68 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 <b>±</b> 5%	0.42	0.79	6.90 ± 11.0% (k=2)
2600	±50/±100	Body	$52.5 \pm 5\%$	2.16 ± 5%	0.28	1.23	6.81 ± 11.0% (k=2)
3500	± 50 / ± 100	Body	51.3 ± 5%	3.31 ± 5%	0.35	1.22	5.75 ± 13.1% (k=2)
5200	± 50 / ± 100	Body	$49.0 \pm 5\%$	$5.30\pm5\%$	0.50	1.80	4.43 ± 13.1% (k=2)
5300	± 50 / ± 100	Body	48.5 ± 5%	5.42 ± 5%	0.52	1.80	4.23 ± 13.1% (k=2)
5500	± 50 / ± 100	Body	$48.6 \pm 5\%$	5.65 ± 5%	0.55	1.80	4.08 ± 13.1% (k=2)
5600	± 50 / ± 100	Body	$48.5\pm5\%$	$5.77 \pm 5\%$	0.55	1.80	3.95 ± 13.1% (k=2)
5800	± 50 / ± 100	Body	48.2 ± 5%	$6.00 \pm 5\%$	0.61	1.80	4.00 ± 13.1% (k=2)

 $<sup>^{\</sup>rm C}$  The validity of  $\pm$  100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

## **Deviation from Isotropy in HSL**

Error (φ, θ), f = 900 MHz

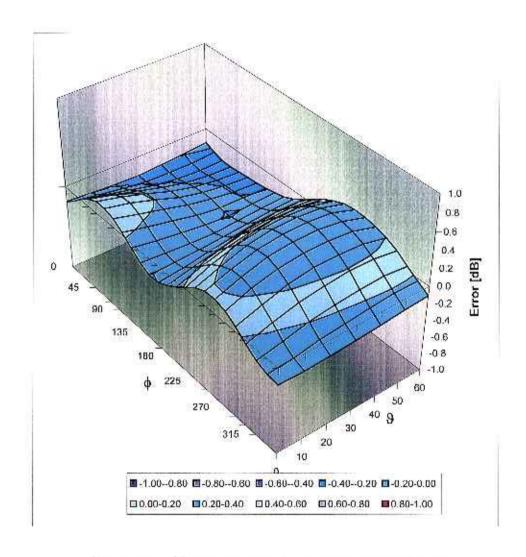

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

## **QuieTek**

## **Appendix E. Dipole Calibration**

Validation Dipole 2450 MHz

M/N: ALS-D-2450-S-2

S/N: QTK-319

### **NCL CALIBRATION LABORATORIES**

Calibration File No: DC-891

## CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Quietek Validation Dipole

Manufacturer: APREL Laboratories
Part number: ALS-D-2450-S-2
Frequency: 2.45 GHz
Serial No: QTK-319

Customer: Quietek

Project Number: QTKB-Dipole-CAL-5336

Calibrated: 9<sup>th</sup> May 2008 Released on: 9<sup>th</sup> May 2008

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By:

NCL CALIBRATION LABORATORIES

51 SPECTRUM WAY NEPEAN, ONTARIO CANADA K2R 1E6 Division of APREL Lab. TEL: (613) 820-4988 FAX: (613) 820-4161

## **Calibration Results Summary**

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

### **Mechanical Dimensions**


**Length:** 53.5 mm **Height:** 30.4 mm

## **Electrical Specification**

SWR: 1.19 U Return Loss: -20.8 dB Impedance:  $49.4 \Omega$ 

## **System Validation Results**

Frequency	1 Gram	10 Gram	Peak
2.45 GHz	48.07	25.65	95.6

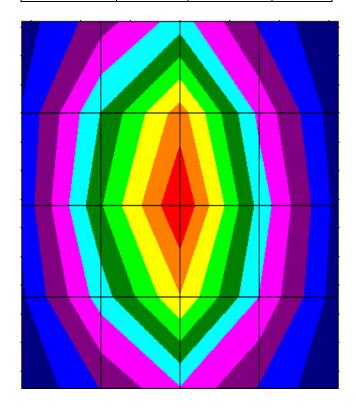

### **Conditions**

Dipole 319 is a recalibration.

Ambient Temperature of the Laboratory:  $22 \,^{\circ}\text{C} \, +/- \, 0.5 \,^{\circ}\text{C}$ Temperature of the Tissue:  $21 \,^{\circ}\text{C} \, +/- \, 0.5 \,^{\circ}\text{C}$ 

#### References

SSI-TP-018-ALSAS Dipole Calibration Procedure

SSI-TP-016 Tissue Calibration Procedure

IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

IEC 62209 "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures –Part 1 & Part 2: Procedure to determine the specific absorption rate (SAR) for mobile wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

**Stuart Nicol** 

C. Teodorian

## **Dipole Calibration Results**

### **Mechanical Verification**

IEEE Length	IEEE Height	Measured Length	Measured Height
51.5 mm	30.4 mm	53.5 mm	30.4 mm

### **Tissue Validation**


Head Tissue 2450 MHz	Measured
Dielectric constant, ε <sub>r</sub>	40.1
Conductivity, σ [S/m]	1.78

#### **Electrical Calibration**

Test	Result
S11 R/L	-20.8 dB
SWR	1.2 U
Impedance	49.4 Ω

The Following Graphs are the results as displayed on the Vector Network Analyzer.


#### **S11 Parameter Return Loss**

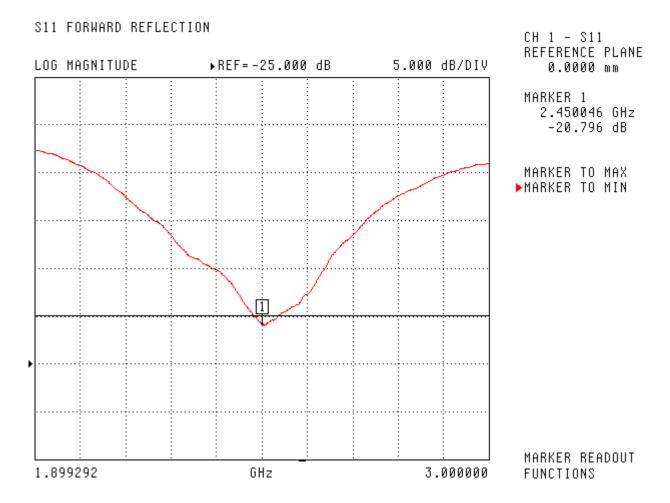

### **SWR**




## **Smith Chart Dipole Impedance**

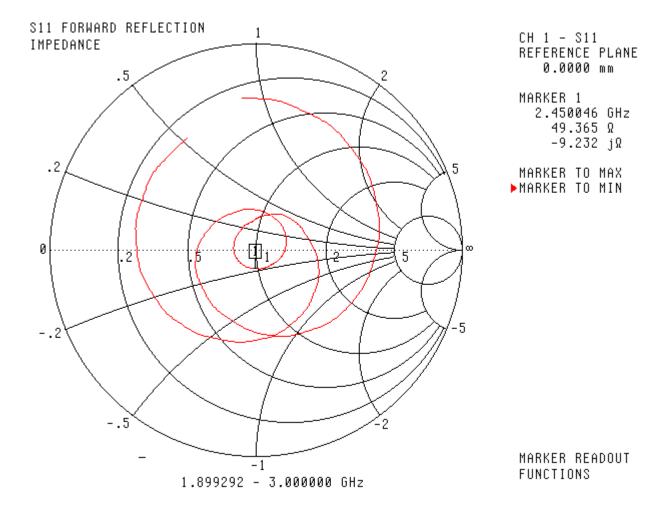

## **System Validation Results Using the Electrically Calibrated Dipole**

Frequency	1 Gram	10 Gram	Peak Above Feed Point
2.45 GHz	48.07	25.65	95.6

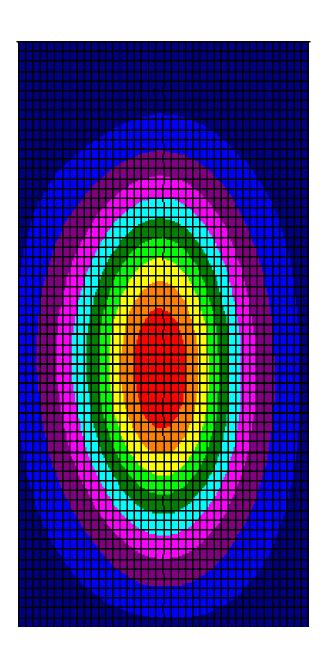

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2008.