

## System Check\_Head\_6500MHz\_210118

Communication System: Validation band; Frequency: 6500.0

Medium: HSL\_6G\_210118 Medium parameters used:  $f=6500.0$  MHz;  $\sigma=6.01$  S/m;  $\epsilon_r=34.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(4.85, 4.85, 4.85); Calibrated: 2020-02-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2020-02-18
- Phantom: Twin-SAM V4.0 (30deg probe tilt); Serial:1488; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926
- UID: CW, 0--
- MAIA: Area Scan: N/A; Zoom Scan: N/A


**Area Scan (51.0 mm x 51.0 mm):** Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 24.5 W/kg; SAR (10g) = 4.99 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 29.8 W/kg; SAR (10g) = 5.46 W/kg;

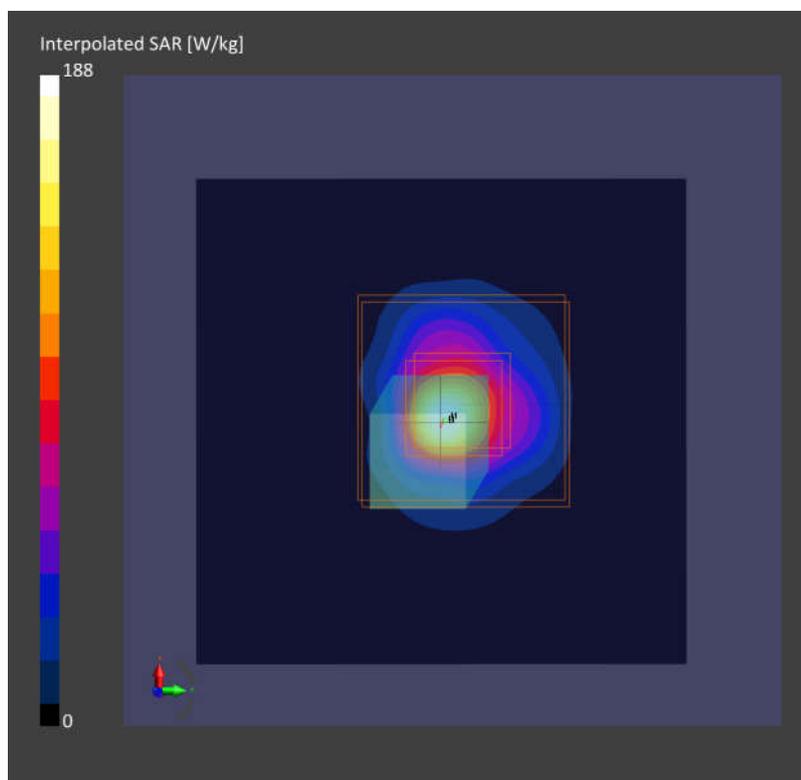

## System Check\_Head\_6500MHz\_210119

Communication System: Validation band; Frequency: 6500.0

Medium: HSL\_6G\_210119 Medium parameters used:  $f=6500.0$  MHz;  $\sigma=5.99$  S/m;  $\epsilon_r=34.2$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(4.85, 4.85, 4.85); Calibrated: 2020-02-04
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1399; Calibrated: 2020-02-18
- Phantom: Twin-SAM V4.0 (30deg probe tilt); Serial:1488; Section: Flat
- Measurement Software: cDASY6 V6.6.0.13926
- UID: CW, 0--
- MAIA: Area Scan: N/A; Zoom Scan: N/A

**Area Scan (51.0 mm x 85.0 mm):** Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 24.1 W/kg; SAR (10g) = 4.78 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 28.9 W/kg; SAR (10g) = 5.18 W/kg;

