Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/16

#### Body GSM850 Ch251 Keypad Down with 1.5cm Gap GPRS10 Bluetooth On

#### DUT: 781408

Communication System: GSM850; Frequency: 848.8 MHz; Duty Cycle: 1:4

Medium: MSL 850 Medium parameters used: f = 849 MHz;  $\sigma = 0.983$  mho/m;  $\varepsilon_r = 55$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.9 °C; Liquid Temperature: 21.5 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(6.1, 6.1, 6.1); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

# Ch251/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 1.10 mW/g

# Ch251/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 21.2 V/m; Power Drift = -0.022 dB

Peak SAR (extrapolated) = 1.31 W/kg

SAR(1 g) = 1.05 mW/g; SAR(10 g) = 0.775 mW/gMaximum value of SAR (measured) = 1.10 mW/g

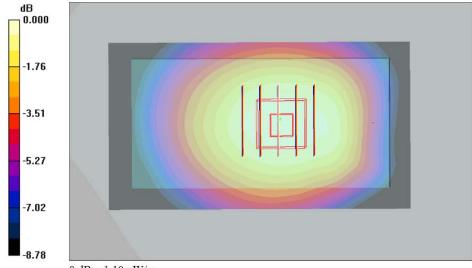

0 dB = 1.10 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/16

# Body\_GSM850 Ch189\_Keypad Down with 1.5cm Gap\_EDGE10

#### DUT: 781408

Communication System: GSM850; Frequency: 836.4 MHz; Duty Cycle: 1:4

Medium: MSL 850 Medium parameters used: f = 836.4 MHz;  $\sigma = 0.97 \text{ mho/m}$ ;  $\epsilon_{\nu} = 55.1$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Ambient Temperature: 23.0 °C; Liquid Temperature: 21.5 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(6.1, 6.1, 6.1); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

# Ch189/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.161 mW/g


Ch189/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 8.78 V/m; Power Drift = -0.072 dB

Peak SAR (extrapolated) = 0.194 W/kg

SAR(1 g) = 0.154 mW/g; SAR(10 g) = 0.114 mW/g

Maximum value of SAR (measured) = 0.163 mW/g

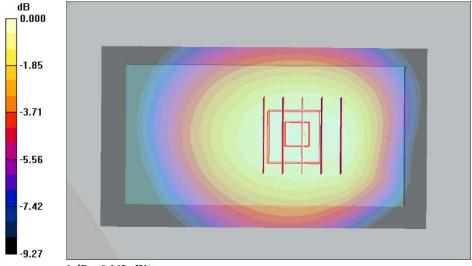

0 dB = 0.163 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/22

# Body\_PCS Ch661\_Keypad Up with 1.5cm Gap\_GPRS10

#### DUT: 781408

Communication System: PCS; Frequency: 1880 MHz; Duty Cycle: 1:4

Medium: MSL\_1900 Medium parameters used: f = 1880 MHz;  $\sigma = 1.48$  mho/m;  $\epsilon_r = 50.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0 °C; Liquid Temperature: 21.6 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.68, 4.68, 4.68); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

# Ch661/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.403 mW/g


#### Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 14.4 V/m; Power Drift = -0.070 dB

Peak SAR (extrapolated) = 0.549 W/kg

# SAR(1 g) = 0.362 mW/g; SAR(10 g) = 0.228 mW/g

Maximum value of SAR (measured) = 0.388 mW/g

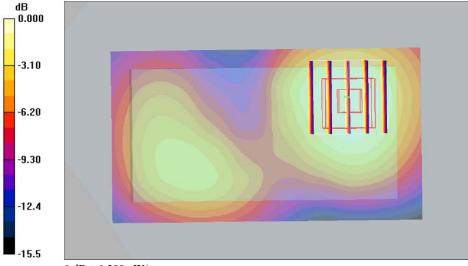

0 dB = 0.388 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/22

### Body\_PCS Ch661\_Keypad Down with 1.5cm Gap\_GPRS10

#### DUT: 781408

Communication System: PCS; Frequency: 1880 MHz; Duty Cycle: 1:4

Medium: MSL 1900 Medium parameters used: f = 1880 MHz;  $\sigma = 1.48$  mho/m;  $\epsilon_r = 50.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0 °C; Liquid Temperature: 21.6 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.68, 4.68, 4.68); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

# Ch661/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.594 mW/g


# Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 18.3 V/m; Power Drift = -0.094 dB

Peak SAR (extrapolated) = 0.837 W/kg

# SAR(1 g) = 0.540 mW/g; SAR(10 g) = 0.340 mW/g

Maximum value of SAR (measured) = 0.581 mW/g

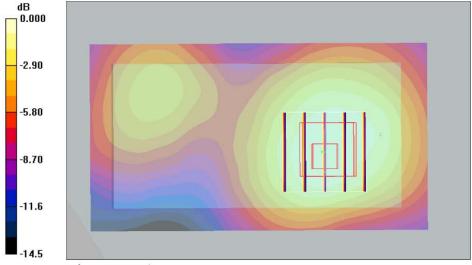

0 dB = 0.581 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/22

### Body\_PCS Ch661\_Keypad Down with 1.5cm Gap\_GPRS10\_Bluetooth On

#### DUT: 781408

Communication System: PCS; Frequency: 1880 MHz; Duty Cycle: 1:4

Medium: MSL 1900 Medium parameters used: f = 1880 MHz;  $\sigma = 1.48$  mho/m;  $\epsilon_r = 50.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.9 °C; Liquid Temperature: 21.6 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.68, 4.68, 4.68); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

# Ch661/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.573 mW/g


# Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 18.1 V/m; Power Drift = -0.013 dB

Peak SAR (extrapolated) = 0.811 W/kg

#### SAR(1 g) = 0.525 mW/g; SAR(10 g) = 0.332 mW/g

Maximum value of SAR (measured) = 0.565 mW/g

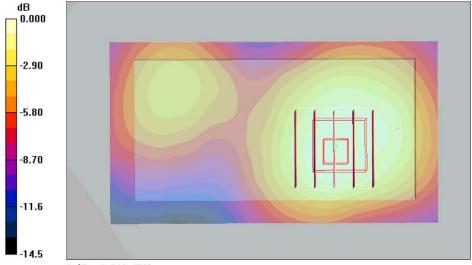

0 dB = 0.565 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/22

### Body\_PCS Ch661\_Keypad Down with 1.5cm Gap\_EDGE10

#### DUT: 781408

Communication System: PCS; Frequency: 1880 MHz; Duty Cycle: 1:4

Medium: MSL 1900 Medium parameters used: f = 1880 MHz;  $\sigma = 1.48$  mho/m;  $\epsilon_r = 50.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0 °C; Liquid Temperature: 21.6 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.68, 4.68, 4.68); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

# Ch661/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.235 mW/g


# Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 11.4 V/m; Power Drift = 0.090 dB

Peak SAR (extrapolated) = 0.329 W/kg

# SAR(1 g) = 0.211 mW/g; SAR(10 g) = 0.132 mW/g

Maximum value of SAR (measured) = 0.230 mW/g

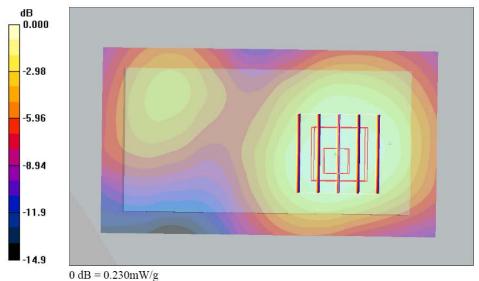

CC SAR Test Report Test Report No : FA781408-1-2-01

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/10/1

#### Body 802.11b Ch6 Keypad Up with 1.5cm Gap

#### DUT: 781408

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL 2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.92$  mho/m;  $\epsilon_r = 51.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0 °C; Liquid Temperature: 21.5 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.02, 4.02, 4.02); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

# Ch6/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.046 mW/g

#### Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.48 V/m; Power Drift = -0.126 dB

Peak SAR (extrapolated) = 0.074 W/kg

SAR(1 g) = 0.042 mW/g; SAR(10 g) = 0.024 mW/g

Maximum value of SAR (measured) = 0.045 mW/g


# Ch6/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.48 V/m; Power Drift = -0.126 dB

Peak SAR (extrapolated) = 0.067 W/kg

# SAR(1 g) = 0.035 mW/g; SAR(10 g) = 0.021 mW/g

Maximum value of SAR (measured) = 0.038 mW/g

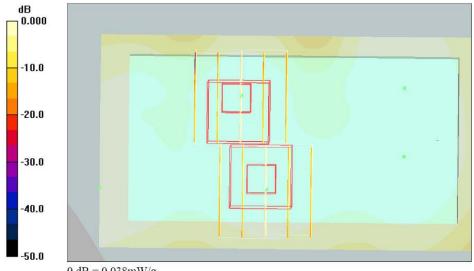

0 dB = 0.038 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/10/1

# Body\_802.11b Ch6\_Keypad Down with 1.5cm Gap

#### DUT: 781408

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.92$  mho/m;  $\epsilon_r = 51.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0 °C; Liquid Temperature: 21.5 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.02, 4.02, 4.02); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

# Ch6/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.156 mW/g


#### Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.92 V/m; Power Drift = 0.053 dB

Peak SAR (extrapolated) = 0.284 W/kg

#### SAR(1 g) = 0.141 mW/g; SAR(10 g) = 0.080 mW/g

Maximum value of SAR (measured) = 0.151 mW/g

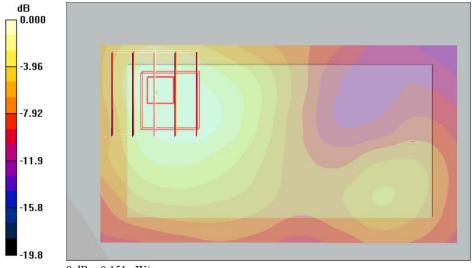

0 dB = 0.151 mW/g

CC SAR Test Report Test Report No : FA781408-1-2-01

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/10/1

### Body\_802.11b Ch6\_Keypad Down with 1.5cm Gap\_Bluetooth On

#### DUT: 781408

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL 2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.92$  mho/m;  $\epsilon_r = 51.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0 °C; Liquid Temperature: 21.5 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.02, 4.02, 4.02); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

#### Ch6/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.096 mW/g

#### Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.30 V/m; Power Drift = 0.098 dB

Peak SAR (extrapolated) = 0.171 W/kg

SAR(1 g) = 0.083 mW/g; SAR(10 g) = 0.044 mW/g

Maximum value of SAR (measured) = 0.090 mW/g


# Ch6/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.30 V/m; Power Drift = 0.098 dB

Peak SAR (extrapolated) = 0.150 W/kg

SAR(1 g) = 0.073 mW/g; SAR(10 g) = 0.040 mW/g

Maximum value of SAR (measured) = 0.080 mW/g

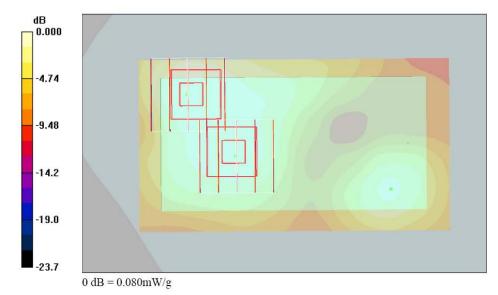

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/10/1

### Body\_802.11g Ch6\_Keypad Down with 1.5cm Gap

#### DUT: 781408

Communication System: 802.11g; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL 2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.92$  mho/m;  $\epsilon_r = 51.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.9 °C; Liquid Temperature: 21.5 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.02, 4.02, 4.02); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

# Ch6/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.053 mW/g


# Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 2.11 V/m; Power Drift = -0.170 dB

Peak SAR (extrapolated) = 0.096 W/kg

#### SAR(1 g) = 0.046 mW/g; SAR(10 g) = 0.024 mW/g

Maximum value of SAR (measured) = 0.050 mW/g

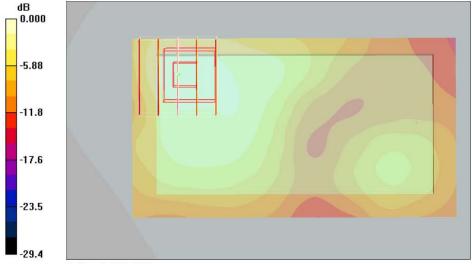

0 dB = 0.050 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/22

#### Right Cheek GSM850 Ch251 Bluetooth On 2D

DUT: 781408

Communication System: GSM850; Frequency: 848.8 MHz;Duty Cycle: 1:8.3

Medium: HSL 850 Medium parameters used: f = 849 MHz;  $\sigma = 0.915$  mho/m;  $\epsilon_r = 40.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.2 °C; Liquid Temperature: 21.8 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(6.58, 6.58, 6.58); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

# Ch251/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.389 mW/g


Ch251/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 18.7 V/m; Power Drift = -0.036 dB

Peak SAR (extrapolated) = 0.627 W/kg

SAR(1 g) = 0.355 mW/g; SAR(10 g) = 0.223 mW/g

Maximum value of SAR (measured) = 0.387 mW/g

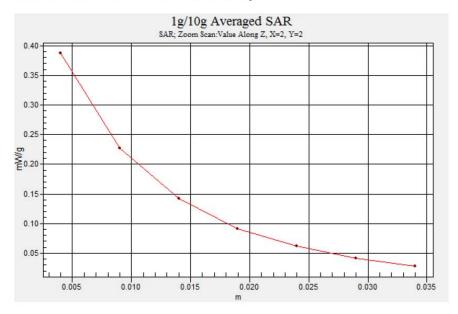

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/22

#### Right Tilted PCS Ch661 Bluetooth On 2D

DUT: 781408

Communication System: PCS; Frequency: 1880 MHz; Duty Cycle: 1:8.3

Medium: HSL 1900 Medium parameters used: f = 1880 MHz;  $\sigma = 1.39$  mho/m;  $\epsilon_e = 39.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0 °C; Liquid Temperature: 21.7 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(5.16, 5.16, 5.16); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch661/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.618 mW/g


Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 17.5 V/m; Power Drift = -0.010 dB

Peak SAR (extrapolated) = 1.02 W/kg

SAR(1 g) = 0.541 mW/g; SAR(10 g) = 0.287 mW/g

Maximum value of SAR (measured) = 0.624 mW/g

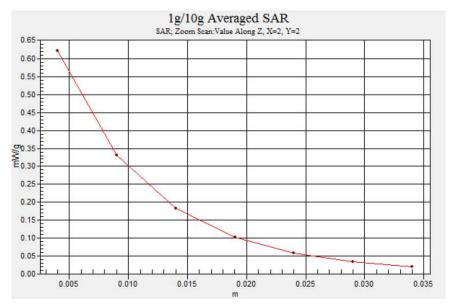

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/25

### Left Cheek\_802.11b Ch6\_2D

DUT: 781408

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: HSL 2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.83$  mho/m;  $\epsilon_e = 37.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.8 °C; Liquid Temperature: 21.4 °C

#### DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.5, 4.5, 4.5); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 176

# Ch6/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.419 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.23 V/m; Power Drift = 0.010 dB

Peak SAR (extrapolated) = 0.840 W/kg

SAR(1 g) = 0.414 mW/g; SAR(10 g) = 0.203 mW/gMaximum value of SAR (measured) = 0.479 mW/g


Ch6/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.23 V/m; Power Drift = 0.010 dB

Peak SAR (extrapolated) = 0.515 W/kg

SAR(1 g) = 0.292 mW/g; SAR(10 g) = 0.148 mW/g

Maximum value of SAR (measured) = 0.319 mW/g

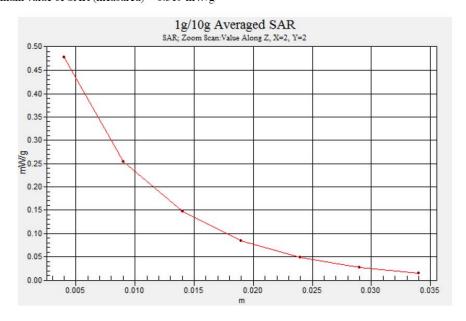

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/16

### Body\_GSM850 Ch251\_Keypad Down with 1.5cm Gap\_GPRS10\_2D

DUT: 781408

Communication System: GSM850; Frequency: 848.8 MHz;Duty Cycle: 1:4

Medium: MSL\_850 Medium parameters used: f = 849 MHz;  $\sigma = 0.983$  mho/m;  $\varepsilon_r = 55$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.9 °C; Liquid Temperature: 21.5 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(6.1, 6.1, 6.1); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

# Ch251/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 1.11 mW/g

Ch251/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 21.4 V/m; Power Drift = -0.042 dB

Peak SAR (extrapolated) = 1.32 W/kg

SAR(1 g) = 1.05 mW/g; SAR(10 g) = 0.776 mW/gMaximum value of SAR (measured) = 1.11 mW/g

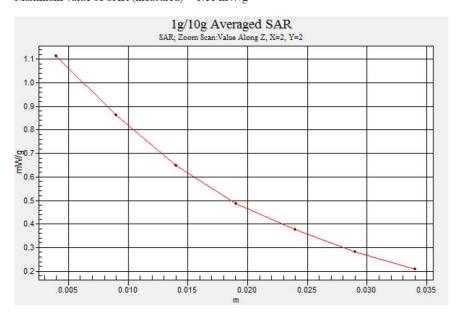

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/9/22

### Body\_PCS Ch661\_Keypad Down with 1.5cm Gap\_GPRS10\_2D

DUT: 781408

Communication System: PCS; Frequency: 1880 MHz; Duty Cycle: 1:4

Medium: MSL 1900 Medium parameters used: f = 1880 MHz;  $\sigma = 1.48$  mho/m;  $\epsilon_r = 50.8$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0 °C; Liquid Temperature: 21.6 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.68, 4.68, 4.68); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Ch661/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 0.594 mW/g

Ch661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 18.3 V/m; Power Drift = -0.094 dB

Peak SAR (extrapolated) = 0.837 W/kg

SAR(1 g) = 0.540 mW/g; SAR(10 g) = 0.340 mW/gMaximum value of SAR (measured) = 0.581 mW/g

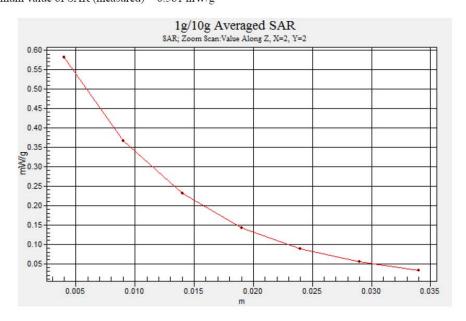

Test Laboratory: Sporton International Inc. SAR Testing Lab Date: 2007/10/1

# Body\_802.11b Ch6\_Keypad Down with 1.5cm Gap\_2D

DUT: 781408

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.92$  mho/m;  $\epsilon_r = 51.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0 °C; Liquid Temperature: 21.5 °C

# DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.02, 4.02, 4.02); Calibrated: 2007/8/28
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2006/11/21
- Phantom: SAM-B; Type: QD 000 P40 C; Serial: TP-1383
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Ch6/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 0.156 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.92 V/m; Power Drift = 0.053 dB

Peak SAR (extrapolated) = 0.284 W/kg

SAR(1 g) = 0.141 mW/g; SAR(10 g) = 0.080 mW/gMaximum value of SAR (measured) = 0.151 mW/g

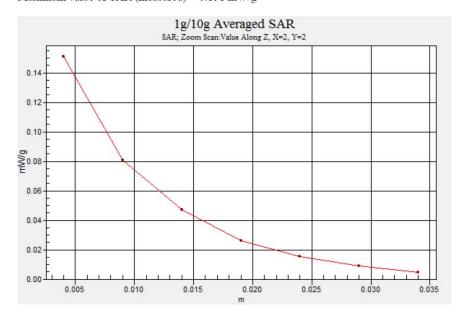

# Appendix C - Calibration Data

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





C

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Sporton (Auden)

Certificate No: D835V2-499\_Mar06

Accreditation No.: SCS 108

Object	D835V2 - SN: 49	9	
Calibration procedure(s)	QA CAL-05.v6		
	Calibration proce	dure for dipole validation kits	
Calibration date:	March 15, 2006		
	Carried to the Million Control		HEAVING TO SHOW THE S
Condition of the calibrated item	In Tolerance		
This calibration certificate docum	ents the traceability to nati	onal standards, which realize the physical units of	measurements (SI).
The measurements and the unce	rtainties with confidence p	robability are given on the following pages and are	e part of the certificate.
			H.
All calibrations have been condu	cted in the closed laborator	y facility: environment temperature (22 ± 3)°C and	numidity < 70%.
		y facility: environment temperature (22 ± 3)°C and	i humidity < 70%.
		y facility: environment temperature (22 ± 3)°C and	1 humidity < 70%.
Calibration Equipment used (M&		*	Scheduled Calibration
Calibration Equipment used (M& Primary Standards	TE critical for calibration)	y facility: environment temperature (22 ± 3)*C and  Cal Date (Calibrated by, Certificate No.)  04-Oct-05 (METAS, No. 251-00516)	
Calibration Equipment used (M& Primary Standards Power meter EPM-442A	TE critical for calibration)	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	TE critical for calibration)  ID #  GB37480704	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516)	Scheduled Calibration Oct-06
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	ID #  GB37480704  US37292783  SN: 5086 (20g)	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498)	Scheduled Calibration Oct-06 Oct-06
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator	ID #  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r)	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6	ID #  GB37480704  US37292783  SN: 5086 (20g)	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498)	Scheduled Calibration Oct-06 Oct-06 Aug-06
Calibration Equipment used (M8' Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4	ID #  GB37480704  US37292783  SN: 5086 (20g)  SN: 5047.2 (10r)  SN 1507  SN 601	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06
Calibration Equipment used (M8' Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4 Secondary Standards	ID #  GB37480704  US37292783  SN: 5086 (20g)  SN: 5047.2 (10r)  SN 1507  SN 601	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-S01_Dec05) Check Date (In house)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4 Secondary Standards Power sensor HP 8481A	ID #  GB37480704  US37292783  SN: 5086 (20g)  SN: 5047.2 (10r)  SN 1507  SN 601  ID #  MY41092317	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Oct-07
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4 Secondary Standards Power sensor HP 8481A RF generator Aglient E4421B	ID #  OB37480704  US37292783  SN: 5086 (20g)  SN: 5047.2 (10r)  SN 1507  SN 601  ID #  MY41092317  MY41000675	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-501_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4 Secondary Standards Power sensor HP 8481A RF generator Agilent E4421B	ID #  GB37480704  US37292783  SN: 5086 (20g)  SN: 5047.2 (10r)  SN 1507  SN 601  ID #  MY41092317	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Oct-07
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4 Secondary Standards Power sensor HP 8481A RF generator Agilent E4421B	ID #  OB37480704  US37292783  SN: 5086 (20g)  SN: 5047.2 (10r)  SN 1507  SN 601  ID #  MY41092317  MY41000675	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-501_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07
Calibration Equipment used (M8' Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4 Secondary Standards Power sensor HP 8481A RF generator Aglient E4421B Network Analyzer HP 8753E	ID #  GB37480704  US37292783  SN: 5046 (20g)  SN: 5047.2 (10r)  SN 1507  SN 601  ID #  MY41092317  MY41000675  US37390585 S4206	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05)  Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Nov-06
Calibration Equipment used (M8' Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ET3DV6 DAE4 Secondary Standards Power sensor HP 8481A RF generator Aglient E4421B Network Analyzer HP 8753E	ID #  GB37480704  US37292783  SN: 5086 (20g)  SN: 5047.2 (10r)  SN 1507  SN 601  ID #  MY41092317  MY41000675  US37390585 \$4206  Name	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Nov-06
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4	ID #  GB37480704  US37292783  SN: 5086 (20g)  SN: 5047.2 (10r)  SN 1507  SN 601  ID #  MY41092317  MY41000675  US37390585 \$4206  Name	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Nov-06
Calibration Equipment used (M8' Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ET3DV6 DAE4 Secondary Standards Power sensor HP 8481A RF generator Agilent E4421B Network Analyzer HP 8753E Calibrated by:	ID #  GB37480704  US37292783  SN: 5086 (20g)  SN: 5047.2 (10r)  SN 1507  SN 601  ID #  MY41092317  MY41000675  US37390585 S4206  Name  Judith Müller	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No. 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05) Function Laboratory Technician	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-08 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Nov-06

Certificate No: D835V2-499\_Mar06

Page 1 of 9





#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage

C Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

#### Additional Documentation:

d) DASY4 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D835V2-499\_Mar06

Page 2 of 9

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	15 mm	with Spacer
Area Scan resolution	dx, dy = 15 mm	
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

#### **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.94mho/m ± 6 %
Head TSL temperature during test	(22.2 ± 0.2) °C		_

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	condition	
SAR measured	250 mW input power	2.35 mW / g
SAR normalized	normalized to 1W	9.40 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	9.24 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.53 mW / g
SAR normalized	normalized to 1W	6.12 mW / g
SAR for nominal Head TSL parameters <sup>1</sup>	normalized to 1W	6.07 mW / g ± 16.5 % (k=2)

Certificate No: D835V2-499\_Mar06

Page 3 of 9

<sup>&</sup>lt;sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

# **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	56.8 ± 6 %	0.98 mho/m ± 6 %
Body TSL temperature during test	(21.4 ± 0.2) °C		

# SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	condition	
SAR measured	250 mW input power	2.45 mW / g
SAR normalized	normalized to 1W	9.80 mW/g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	9.91 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.62 mW / g
SAR normalized	normalized to 1W	6.48 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	6.55 mW / g ± 16.5 % (k=2)

Certificate No: D835V2-499\_Mar06

Page 4 of 9

<sup>&</sup>lt;sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

# Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.1 Ω - 2.9 jΩ	
Return Loss	- 29.1 dB	

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	$47.9 \Omega$ - $5.1 j\Omega$	
Return Loss	- 24.9 dB	

# General Antenna Parameters and Design

Electrical Delay (one direction)	1.391ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	July 10, 2003

Certificate No: D835V2-499\_Mar06

Page 5 of 9



#### **DASY4 Validation Report for Head TSL**

Date/Time: 15.03.2006 12:51:44

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:499

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB;

Medium parameters used: f = 835 MHz;  $\sigma = 0.942$  mho/m;  $\varepsilon_r = 42.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

#### DASY4 Configuration:

- Probe: ET3DV6 SN1507 (HF); ConvF(6.09, 6.09, 6.09); Calibrated: 28.10.2005
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- · Electronics: DAE4 Sn601; Calibrated: 15.12.2005
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA;;
- Measurement SW: DASY4, V4.7 Build 14; Postprocessing SW: SEMCAD, V1.8 Build 165

Pin = 250 mW; d = 10 mm/Area Scan (71x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 2.54 mW/g


Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 53.7 V/m; Power Drift = -0.008 dB

Peak SAR (extrapolated) = 3.53 W/kg

SAR(1 g) = 2.35 mW/g; SAR(10 g) = 1.53 mW/g

Maximum value of SAR (measured) = 2.55 mW/g

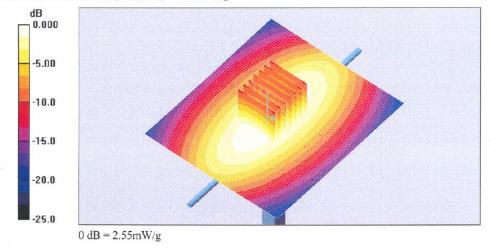


Certificate No: D835V2-499\_Mar06

Page 6 of 9



# Impedance Measurement Plot for Head TSL

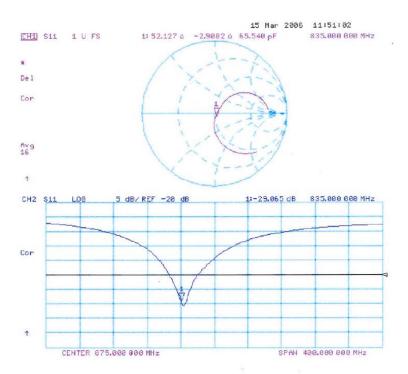

Certificate No: D835V2-499\_Mar06

Page 7 of 9

#### **DASY4 Validation Report for Body TSL**

Date/Time: 14.03.2006 12:37:15

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:499

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: MSL U10;

Medium parameters used: f = 835 MHz;  $\sigma = 0.972$  mho/m;  $\varepsilon_r = 56.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

#### DASY4 Configuration:

Probe: ET3DV6 - SN1507 (HF); ConvF(5.84, 5.84, 5.84); Calibrated: 28.10.2005

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 15.12.2005
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA;;
- Measurement SW: DASY4, V4.7 Build 14; Postprocessing SW: SEMCAD, V1.8 Build 165

Pin = 250 mW; d = 10 mm/Area Scan (71x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 2.63 mW/g


Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 53.3 V/m; Power Drift = 0.026 dB

Peak SAR (extrapolated) = 3.51 W/kg

SAR(1 g) = 2.45 mW/g; SAR(10 g) = 1.62 mW/g

Maximum value of SAR (measured) = 2.65 mW/g

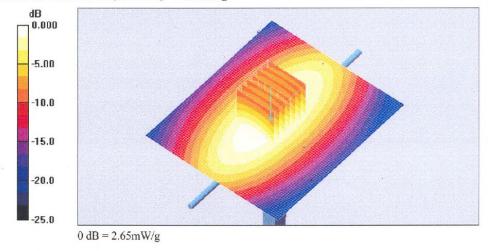


Certificate No: D835V2-499\_Mar06

Page 8 of 9



# Impedance Measurement Plot Body TSL

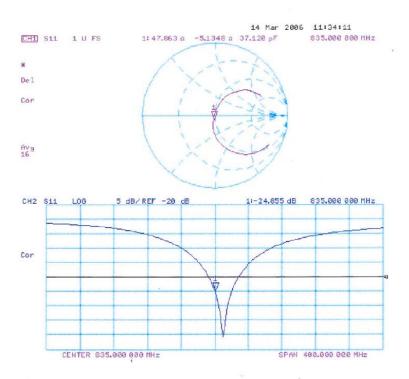

Certificate No: D835V2-499\_Mar06

Page 9 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

CALIBRATION	ERTIFICATE		
Object	D1900V2 - SN: 5	d041	
Calibration procedure(s)	QA CAL-05.v6 Calibration proce	dure for dipole validation kits	
Calibration date:	March 21, 2006		
Condition of the calibrated item	In Tolerance		
The measurements and the unce	rtainties with confidence p	onal standards, which realize the physical units of robability are given on the following pages and are $y$ facility: environment temperature (22 $\pm$ 3)°C and	e part of the certificate.
Calibration Equipment used (M&)	ΓE critical for calibration)		
	TE critical for calibration)	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6	Ÿ	Cal Date (Calibrated by, Certificate No.) 04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05)	Scheduled Calibration Oct-06 Oct-06 Aug-06 Aug-06 Oct-06 Dec-06
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4	ID# GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 601	04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05)	Oct-06 Oct-06 Aug-06 Aug-06 Oct-06 Dec-06
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4 Secondary Standards Power sensor HP 8481A RF generator Agilent E4421B	ID# GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507	04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05)	Oct-06 Oct-06 Aug-06 Aug-06 Oct-06
Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4 Secondary Standards Power sensor HP 8481A RF generator Agilent E4421B Network Analyzer HP 8753E	ID# GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 601 ID# MY41092317 MY41000675	04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No. 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05)  Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05)	Oct-06 Oct-06 Aug-06 Aug-06 Oct-06 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4 Recondary Standards Power sensor HP 8481A RF generator Agilent E4421B Network Analyzer HP 8753E	ID# GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 601 ID# MY41092317 MY41090675 US37390585 S4206	04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No. 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Nov-05) 11-May-05 (SPEAG, in house check Nov-05)	Oct-06 Oct-06 Aug-06 Aug-06 Oct-06 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Nov-06
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ET3DV6 DAE4  Secondary Standards Power sensor HP 8481A RF generator Agilent E4421B	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN: 1507 SN: 601 ID # MY41092317 MY41090675 US37390585 S4206	04-Oct-05 (METAS, No. 251-00516) 04-Oct-05 (METAS, No. 251-00516) 11-Aug-05 (METAS, No. 251-00498) 11-Aug-05 (METAS, No 251-00498) 28-Oct-05 (SPEAG, No. ET3-1507_Oct05) 15-Dec-05 (SPEAG, No. DAE4-601_Dec05) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-05) 11-May-05 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	Oct-06 Oct-06 Aug-06 Aug-06 Oct-06 Dec-06 Scheduled Check In house check: Oct-07 In house check: Nov-07 In house check: Nov-06

Certificate No: D1900V2-5d041\_Mar06

Page 1 of 9



Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z

not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

### **Additional Documentation:**

d) DASY4 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D1900V2-5d041	_Mar06
-------------------------------	--------

# **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Area Scan resolution	dx, dy = 15 mm	
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

#### **Head TSL parameters**

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.4 ± 6 %	1.42 mho/m ± 6 %
Head TSL temperature during test	(21.5 ± 0.2) °C		

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	condition	
SAR measured	250 mW input power	9.75 mW / g
SAR normalized	normalized to 1W	39.0 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	38.4 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.17 mW / g
SAR normalized	normalized to 1W	20.7 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	20.5 mW / g ± 16.5 % (k=2)

Certificate No: D1900V2-5d041\_Mar06 Page 3 of 9

<sup>&</sup>lt;sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

### **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.7 ± 6 %	1.54 mho/m ± 6 %
Body TSL temperature during test	(21.6 ± 0.2) °C		

# SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.2 mW / g
SAR normalized	normalized to 1W	40.8 mW / g
SAR for nominal Body TSL parameters 2	normalized to 1W	41.1 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm3 (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.40 mW / g
SAR normalized	normalized to 1W	21.6 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	21.8 mW / g ± 16.5 % (k=2)

Certificate No: D1900V2-5d041\_Mar06

<sup>&</sup>lt;sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.5 Ω + 5.1 jΩ	
Return Loss	- 24.8 dB	

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	$47.9 \Omega + 6.3 J\Omega$	
Return Loss	- 23.4 dB	

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.200 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

# Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	July 4, 2003	

Certificate No: D1900V2-5d041\_Mar06

Page 5 of 9