



D5: 5GHz SYSTEM VALIDATION DIPOLE SN: 1018

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland

Client **ADT (Auden)**

CALIBRATION CERTIFICATE



Object(s) **D5GHzV2 - SN:1018**
 Calibration procedure(s) **QA CAL-05.v2
Calibration procedure for dipole validation kits**
 Calibration date: **March 23, 2004**
 Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM E4419B	GB41293874	2-Apr-03 (METAS, No 252-0250)	Apr-04
Power sensor E4412A	MY41495277	2-Apr-03 (METAS, No 252-0250)	Apr-04
Power sensor HP 8481A	MY41092317	18-Oct-02 (Agilent, No. 20021018)	Oct-04
RF generator R&S SMT06	100058	23-May-01 (SPEAG, in house check May-03)	In house check: May-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-03)	In house check: Oct 05

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Laboratory Director	
Approved by:	Fin Bomholt	R&D Director	

Date issued: March 25, 2004

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

DASY

Dipole Validation Kit

Type: D5GHzV2

Serial: 1018

Manufactured: February 5, 2004

Calibrated: March 23, 2004

1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **head simulating solution** of the following electrical parameters:

Frequency:	5200 MHz	
Relative Dielectricity	36.3	± 5%
Conductivity	4.57 mho/m	± 5%
Frequency:	5800 MHz	
Relative Dielectricity	35.4	± 5%
Conductivity	5.20 mho/m	± 5%

The DASY4 System with a dosimetric E-field probe EX3DV3 - SN:3503 was used for the measurements. The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. Special 8x8x8 fine cube was chosen for cube integration (dx=dy=4.3mm, dz=3mm). Distance between probe sensors and phantom surface was set to 2.5 mm. The dipole input power (forward power) was 250 mW ± 3 %. The results are normalized to 1W input power.

2. SAR Measurement with DASY System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figures supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured at **5200 MHz (Head Tissue)** with the dosimetric probe EX3DV3 SN:3503 and applying the advanced extrapolation are:

averaged over 1 cm ³ (1 g) of tissue:	81.2 mW/g ± 20.3 % (k=2)¹
averaged over 10 cm ³ (10 g) of tissue:	22.9 mW/g ± 19.8 % (k=2)¹

The resulting averaged SAR-values measured at **5800 MHz (Head Tissue)** with the dosimetric probe EX3DV3 SN:3503 and applying the advanced extrapolation are:

averaged over 1 cm ³ (1 g) of tissue:	82.0 mW/g ± 20.3 % (k=2)²
averaged over 10 cm ³ (10 g) of tissue:	23.0 mW/g ± 19.8 % (k=2)²

¹ Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR_1g=76.5 mW/g, SAR_10g=21.6 mW/g and SAR_peak=310.3 mW/g.

² Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR_1g=78.0 mW/g, SAR_10g=21.9 mW/g and SAR_peak=340.9 mW/g.

3. Dipole Transformation Parameters

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint (please refer to the graphics attached to this document). The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	1.200 ns	(one direction)
Transmission factor:	0.974	(voltage transmission, one direction)

4. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **body simulating solution** of the following electrical parameters:

Frequency:	5200 MHz	
Relative Dielectricity	49.7	± 5%
Conductivity	5.18 mho/m	± 5%
Frequency:	5800 MHz	
Relative Dielectricity	48.5	± 5%
Conductivity	6.01 mho/m	± 5%

The DASY3 System with a dosimetric E-field probe EX3DV3 - SN:3503 was used for the measurements. The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 8x8x8 fine cube was chosen for cube integration ($dx=dy=4.3\text{mm}$, $dz=3\text{mm}$). Distance between probe sensors and phantom surface was set to 2.5 mm. The dipole input power (forward power) was 250 mW ± 3 %. The results are normalized to 1W input power.

5. SAR Measurement with DASY System

Standard SAR-measurements were performed according to the measurement conditions described in section 4. The results (see figures supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured at **5200 MHz (Body Tissue)** with the dosimetric probe EX3DV3 SN:3503 and applying the advanced extrapolation are:

averaged over 1 cm ³ (1 g) of tissue:	75.6 mW/g ± 20.3 % (k=2) ³
averaged over 10 cm ³ (10 g) of tissue:	21.3 mW/g ± 19.8 % (k=2) ³

The resulting averaged SAR-values measured at **5800 MHz (Body Tissue)** with the dosimetric probe EX3DV3 SN:3503 and applying the advanced extrapolation are:

averaged over 1 cm ³ (1 g) of tissue:	71.2 mW/g ± 20.3 % (k=2) ⁴
averaged over 10 cm ³ (10 g) of tissue:	20.0 mW/g ± 19.8 % (k=2) ⁴

6. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

7. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Small end caps have been added to the dipole arms in order to increase frequency bandwidth at the position as explained in Sections 1 and 4.

8. Power Test

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

³ Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR_1g=71.8 mW/g, SAR_10g=20.1 mW/g and SAR_peak=284.7 mW/g.

⁴ Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR_1g=74.1 mW/g, SAR_10g=20.5 mW/g and SAR_peak=324.7 mW/g.

Test Laboratory: SPEAG, Zurich, Switzerland
DUT: Dipole 5GHz; Serial: D5GHzV2 - SN:1018

Communication System: CW-5GHz;Duty Cycle: 1:1;Medium: HSL5800
 Medium parameters used: $f = 5200$ MHz; $\sigma = 4.57$ mho/m; $\epsilon_r = 36.3$; $\rho = 1000$ kg/m³
 Medium parameters used: $f = 5800$ MHz; $\sigma = 5.2$ mho/m; $\epsilon_r = 35.4$; $\rho = 1000$ kg/m³

DASY4 Configuration:

- Probe: EX3DV3 - SN3503; ConvF(5.7, 5.7, 5.7), ConvF(5, 5, 5);
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE4 600; Calibrated: 9/30/2003
- Phantom: SAM with CRP - TP:1312; Phantom section: Flat Section
- Measurement SW: DASY4, V4.2 Build 44;

d=10mm, Pin=250mW, f=5200 MHz/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 92.2 V/m; Power Drift = -0.0 dB

Maximum value of SAR (interpolated) = 36 mW/g

d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 92.2 V/m; Power Drift = -0.0 dB

Peak SAR (extrapolated) = 77.7 W/kg

SAR(1 g) = 20.3 mW/g; SAR(10 g) = 5.72 mW/g


d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 88.4 V/m; Power Drift = 0.003 dB

Peak SAR (extrapolated) = 85.6 W/kg

SAR(1 g) = 20.5 mW/g; SAR(10 g) = 5.74 mW/g

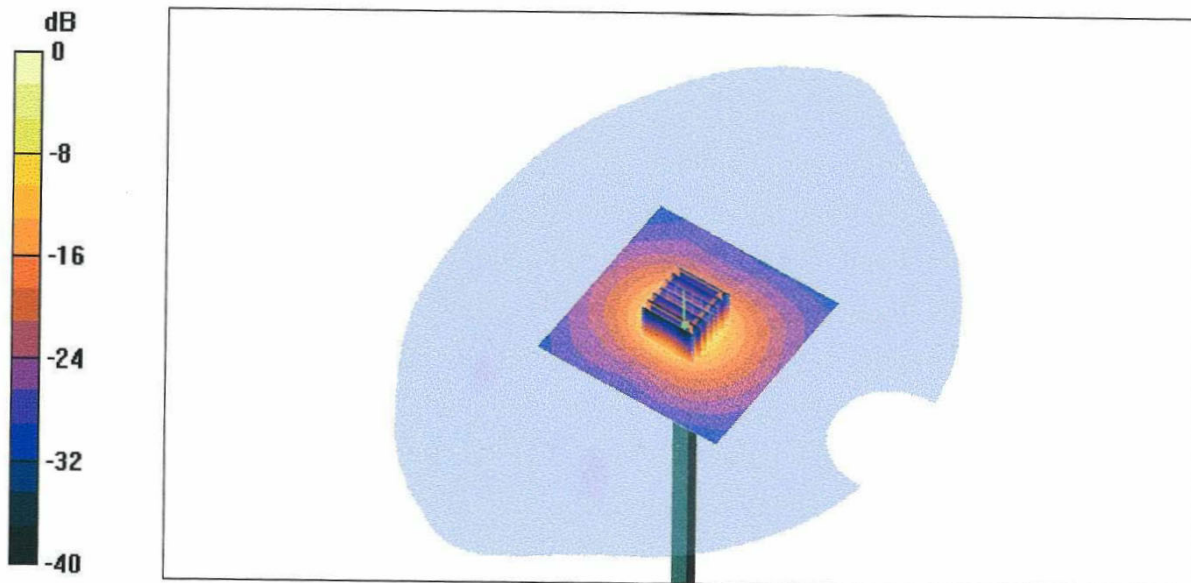


0 dB = 35.1mW/g

20 Feb 2004 11:16:18

CH1 S11 1 U FS 2: 46.307 Δ 8.9473 Δ 273.85 pH 5 200.000 000 MHz

De1
Smo
Cor

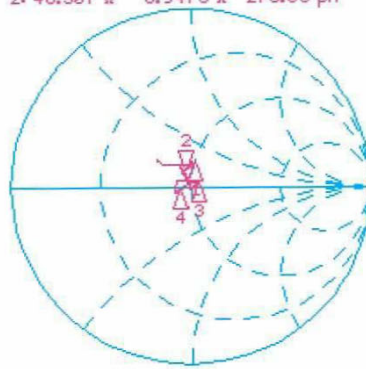

CH1 Markers

1: 49.512 Δ
13.678 Δ
5.10000 GHz

3: 53.717 Δ
2.3340 Δ
5.50000 GHz

4: 43.844 Δ
-1.5781 Δ
5.80000 GHz

Avg
16


↑

CH2 S11 LOG 5 dB/REF -20 dB 2: -19.962 dB 5 200.000 000 MHz

Smo
Cor

Avg
16

↑

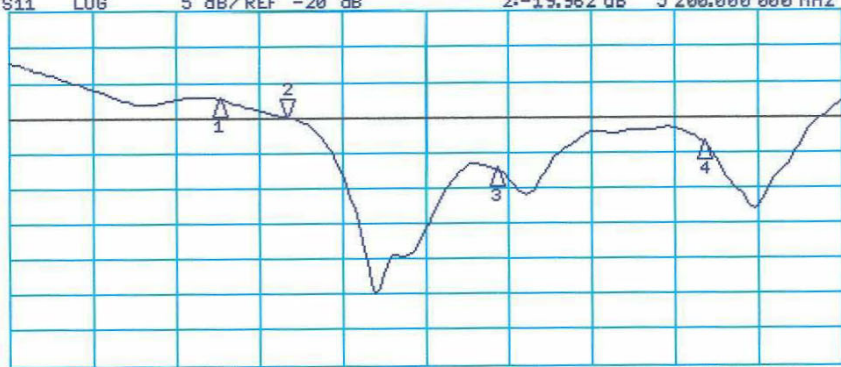

CH2 Markers

1: -17.284 dB
5.10000 GHz

3: -27.319 dB
5.50000 GHz

4: -23.503 dB
5.80000 GHz

START 4 800.000 000 MHz

STOP 6 000.000 000 MHz

Test Laboratory: SPEAG, Zurich, Switzerland
DUT: Dipole 5GHz; Serial: D5GHzV2 - SN:1018

Communication System: CW-5GHz;Duty Cycle: 1:1;Medium: MSL5800
 Medium parameters used: $f = 5200$ MHz; $\sigma = 5.18$ mho/m; $\epsilon_r = 49.7$; $\rho = 1000$ kg/m³
 Medium parameters used: $f = 5800$ MHz; $\sigma = 6.01$ mho/m; $\epsilon_r = 48.5$; $\rho = 1000$ kg/m³


DASY4 Configuration:

- Probe: EX3DV3 - SN3503; ConvF(5, 5, 5), ConvF(4.6, 4.6, 4.6);
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE4 600; Calibrated: 9/30/2003
- Phantom: SAM with CRP - TP:1312; Phantom section: Flat Section
- Measurement SW: DASY4, V4.2 Build 44;

d=10mm, Pin=250mW, f=5200 MHz/Area Scan (31x31x1): Measurement grid: dx=10mm, dy=10mm
 Reference Value = 78 V/m; Power Drift = 0.001 dB
 Maximum value of SAR (interpolated) = 35.6 mW/g

d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:
 Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm
 Reference Value = 69.3 V/m; Power Drift = -0.009 dB
 Peak SAR (extrapolated) = 71.2 W/kg
SAR(1 g) = 17.8 mW/g; SAR(10 g) = 5.01 mW/g


d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan (8x8x8), dist=2.5mm (7x7x8)/Cube 0:
 Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm
 Reference Value = 78 V/m; Power Drift = 0.001 dB
 Peak SAR (extrapolated) = 65 W/kg
SAR(1 g) = 18.9 mW/g; SAR(10 g) = 5.33 mW/g

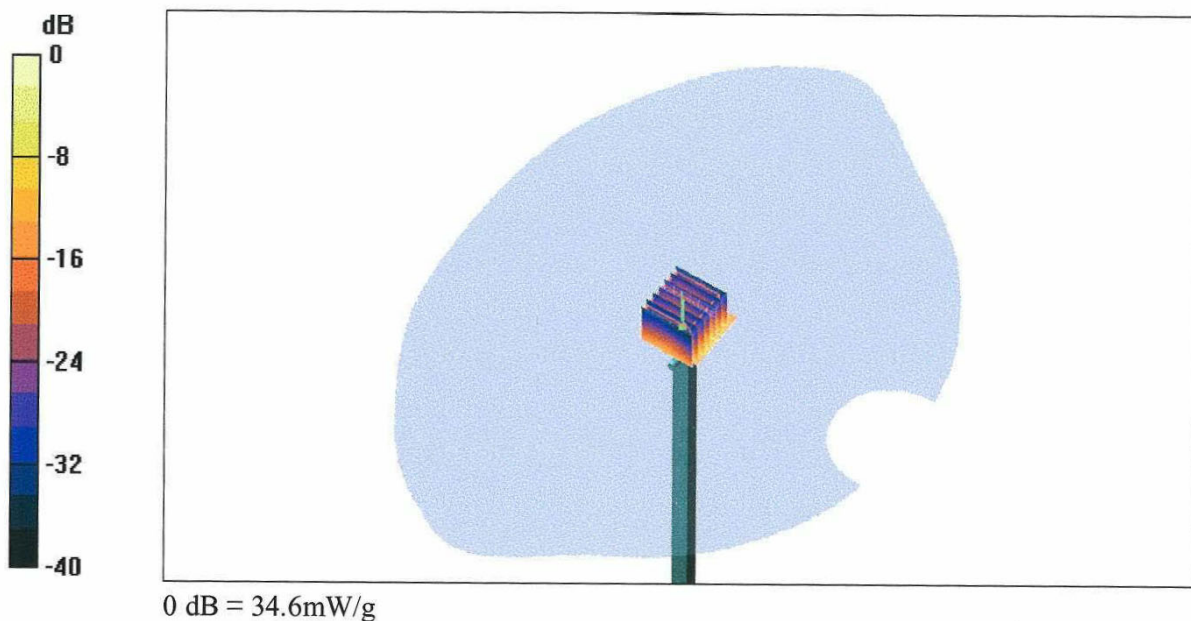

23 Mar 2004 10:00:31

CH1 S11 1 U FS 2: 51.336 Ω -7.8340 Ω 3.9069 pF 5 200.000 000 MHz


De1
Cor
Avg
16
↑

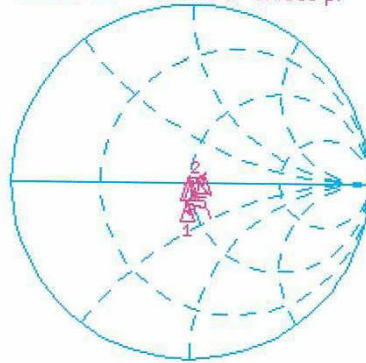

CH1 Markers
1: 46.119 Ω
-11.186 Ω
5.10000 GHz
3: 49.437 Ω
-50.781 m Ω
5.30000 GHz
4: 47.396 Ω
0.0664 Ω
5.50000 GHz
5: 56.244 Ω
4.2871 Ω
5.80000 GHz

CH2 S11 LOG 5 dB/REF -20 dB 2: -22.154 dB 5 200.000 000 MHz

Smo
Cor
↑

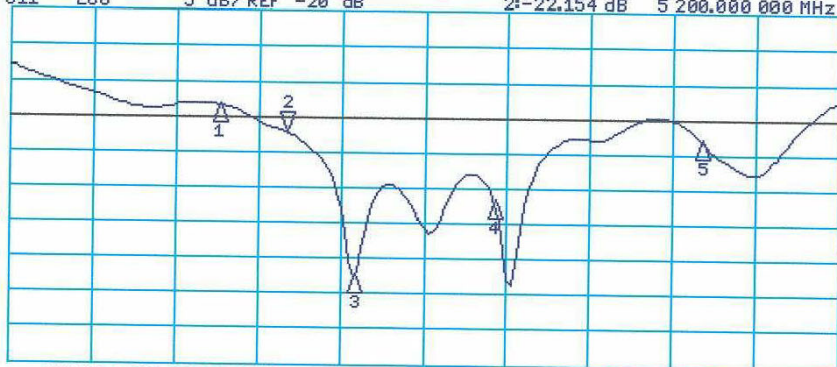

CH2 Markers
1: -18.290 dB
5.10000 GHz
3: -42.376 dB
5.30000 GHz
4: -31.714 dB
5.50000 GHz
5: -23.007 dB
5.80000 GHz

START 4 800.000 000 MHz

STOP 5 000.000 000 MHz