

## ANNEX G DIPOLE QUALIFICATION FOR THE EXTENDED 3-YEAR CALIBRATION INTERVAL

### G1 Dipole 835

The information and documentation below are provided to qualify the extended 3-year calibration interval of dipole.

#### G1.1 List of Equipment

No.	Name	Type	Serial Number
01	Network analyzer	E5071C	MY46103759
02	Power meter	NRVD	101253
03	Power sensor	NRV-Z5	100333
04	Signal Generator	E4438C	MY45095825
05	Amplifier	VTL5400	0404
06	E-field Probe	SPEAG ES3DV3	3151
07	DAE	SPEAG DAE4	786
08	Dipole Validation Kit	SPEAG D835 V2	443

#### G1.2 Results of Impedance, Return-loss and System validation

##### Dipole 835 - Head

		Year			Deviation		Limit
		2009	2010	2011	2010	2011	
Impedance	Real ( $\Omega$ )	52.1	53.7	52.8	1.6 $\Omega$	0.7 $\Omega$	Deviation < 5 $\Omega$
	Imaginary ( $\Omega$ )	-3.5	-3.7	-3.6	0.2 $\Omega$	0.1 $\Omega$	Deviation < 5 $\Omega$
Return-loss (dB)		-25.5	-25.63	-25.69	0.13dB	0.19dB	Deviate < 0.2dB
System validation	10g	1.57	1.55	1.56	-1.27%	-0.64%	Deviation < 10%
	1g	2.43	2.41	2.45	-0.82%	0.82%	Deviation < 10%

##### Dipole 835- Body


		Year			Deviation		Limit
		2009	2010	2011	2010	2011	
Impedance	Real ( $\Omega$ )	49.6	49.4	49.5	0.2 $\Omega$	0.1 $\Omega$	Deviation < 5 $\Omega$
	Imaginary ( $\Omega$ )	-5.3	-5.1	-5.0	0.2 $\Omega$	0.3 $\Omega$	Deviation < 5 $\Omega$
Return-loss (dB)		-25.8	-25.62	-25.68	0.18dB	0.12dB	Deviate < 0.2dB
System validation	10g	1.60	1.61	1.59	0.63%	-0.63%	Deviation < 10%
	1g	2.46	2.51	2.48	2.03%	0.81%	Deviation < 10%

According to the above tables, it is not necessary to recalibration the dipoles in 2010 and 2011.


Please see below for the detail information.

### G1.3 Detail Information


#### G1.3.1 Impedance Measurement Plot

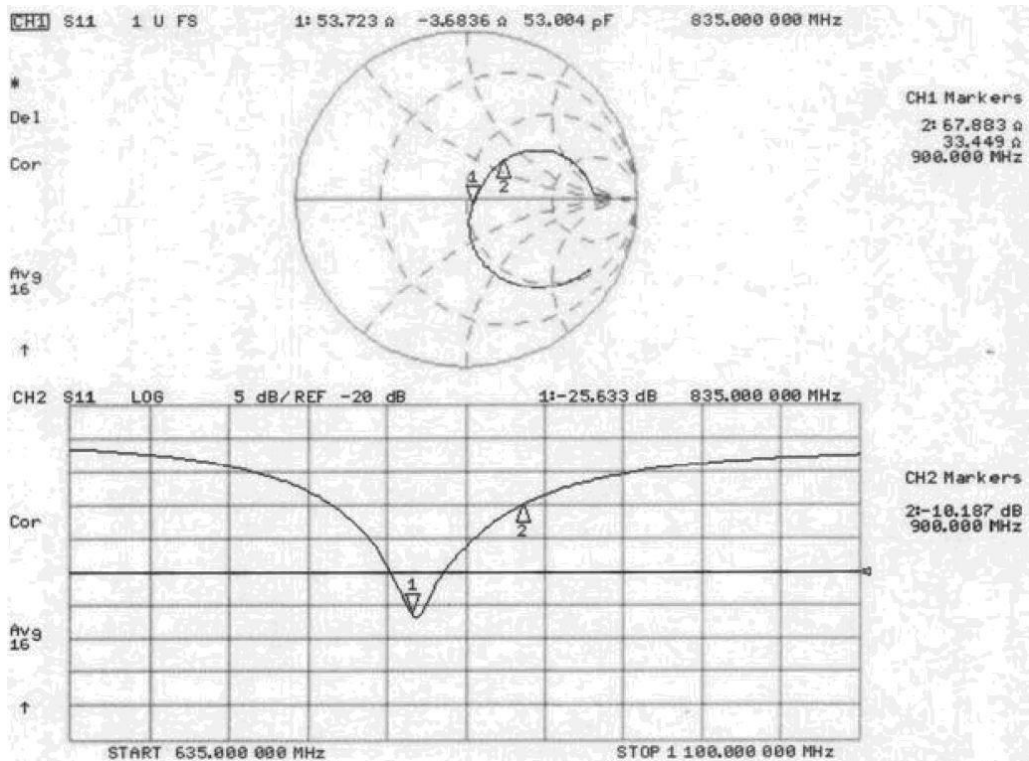


Picture G1: Impedance Measurement Plot \_Dipole 835 Head \_2010

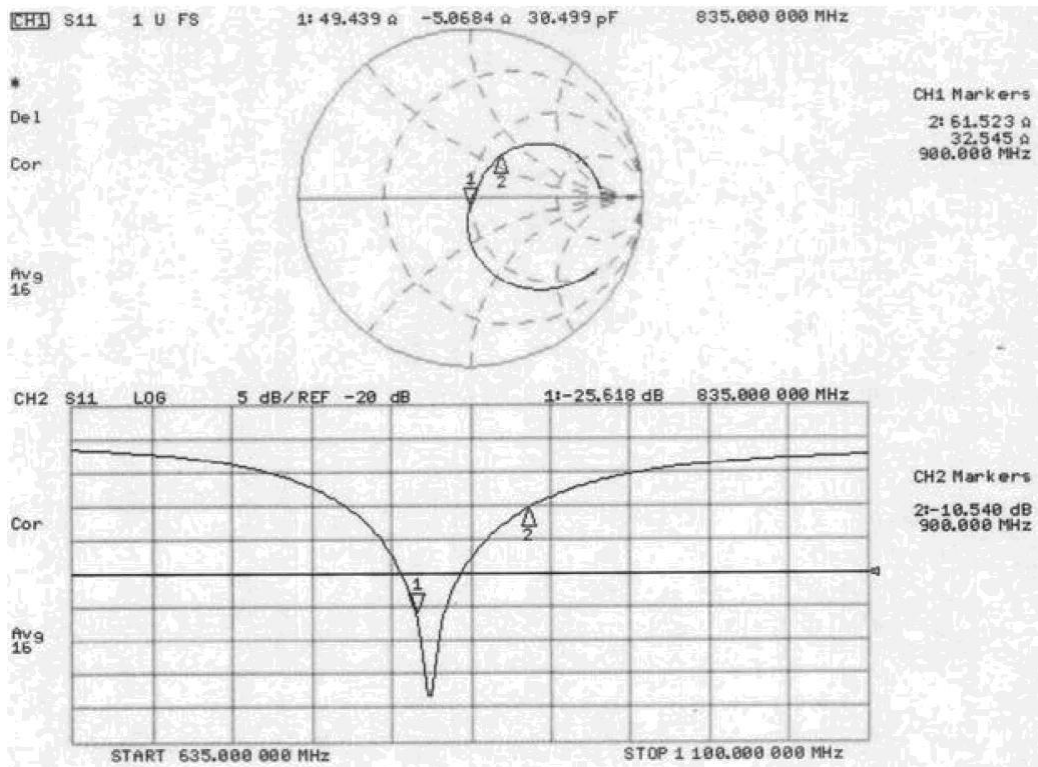

Picture G2: Impedance Measurement Plot \_Dipole 835 Body \_2010

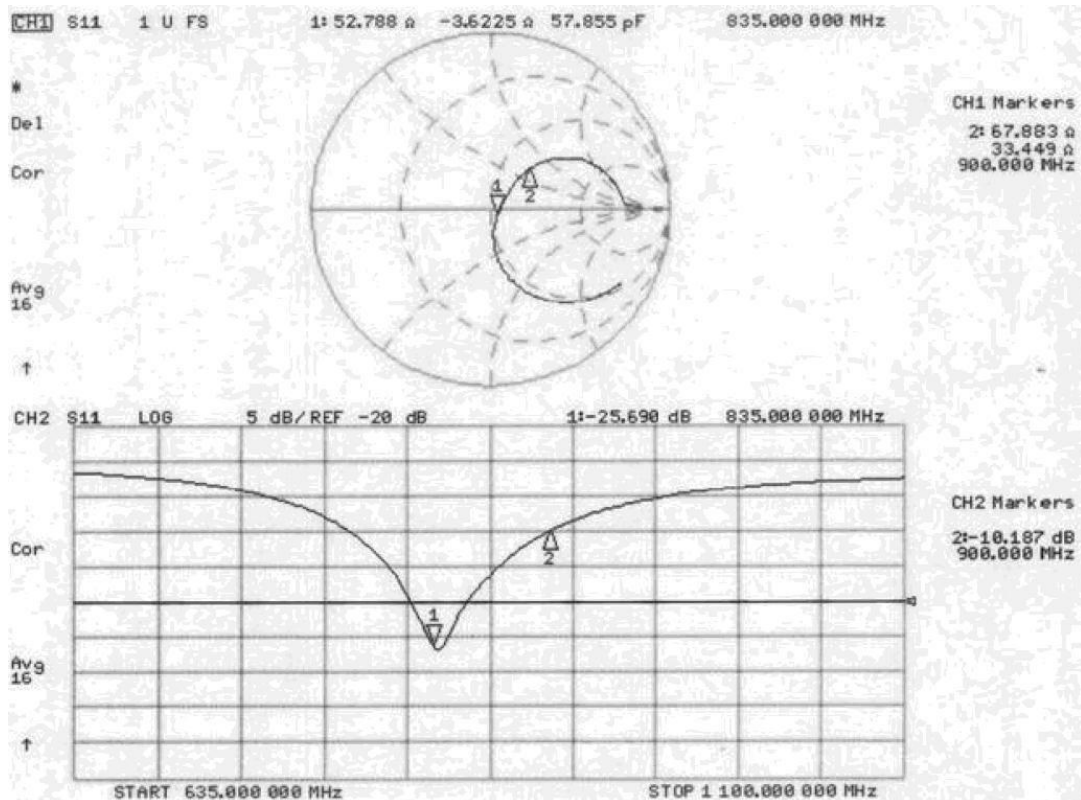

Picture G3: Impedance Measurement Plot \_Dipole 835 Head \_2011

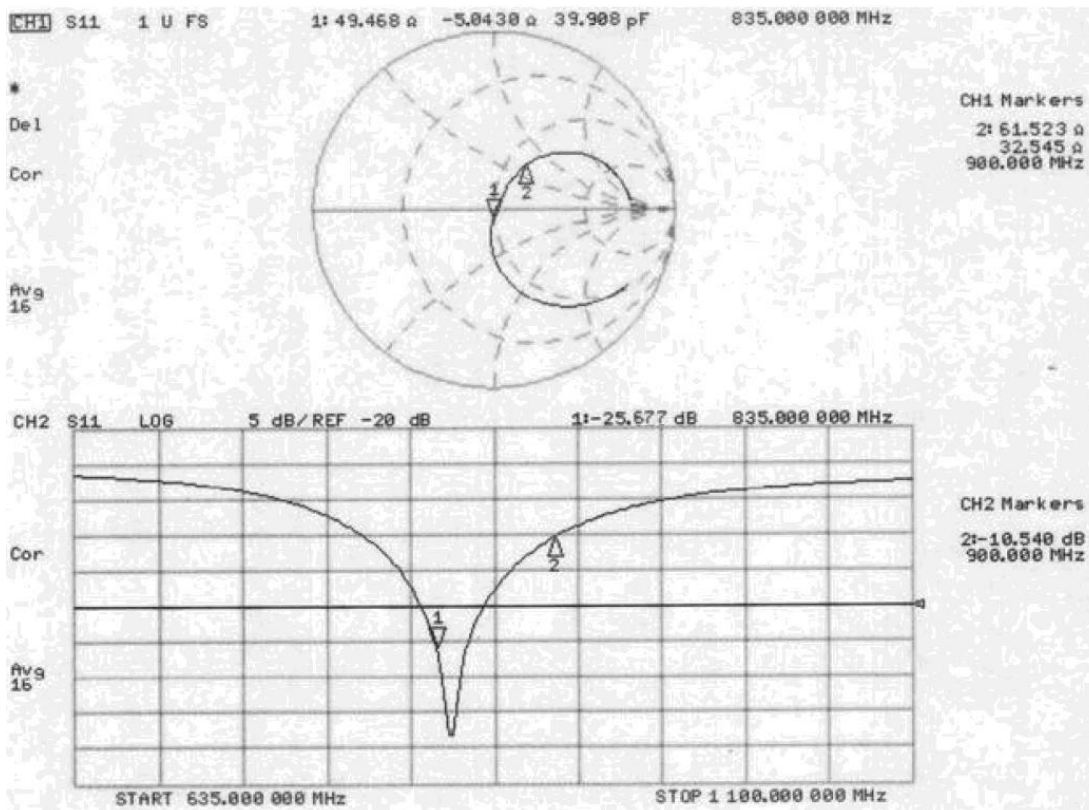

Picture G4: Impedance Measurement Plot \_Dipole 835 Body \_2011

### G1.3.2 System Validation Results

#### 835 MHz

Date/Time: 2010-10-23 9:17:25 AM

Electronics: DAE4 Sn786

Medium: 850 head

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.91 \text{ mho/m}$ ;  $\epsilon_r = 41.7$ ;  $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature:  $22.0^\circ\text{C}$       Liquid Temperature:  $22.0^\circ\text{C}$

Communication System: CW Frequency: 835 MHz Duty Cycle: 1:1

Probe: ES3DV3 - SN3151 ConvF (6.02, 6.02, 6.02)

**System Validation/Area Scan (101x101x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$

Maximum value of SAR (interpolated) =  $2.64 \text{ mW/g}$

**System Validation/Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,


$dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value =  $53.2 \text{ V/m}$ ; Power Drift =  $0.013 \text{ dB}$

Peak SAR (extrapolated) =  $3.57 \text{ W/kg}$

**SAR(1 g) =  $2.41 \text{ mW/g}$ ; SAR(10 g) =  $1.55 \text{ mW/g}$**

Maximum value of SAR (measured) =  $2.59 \text{ mW/g}$

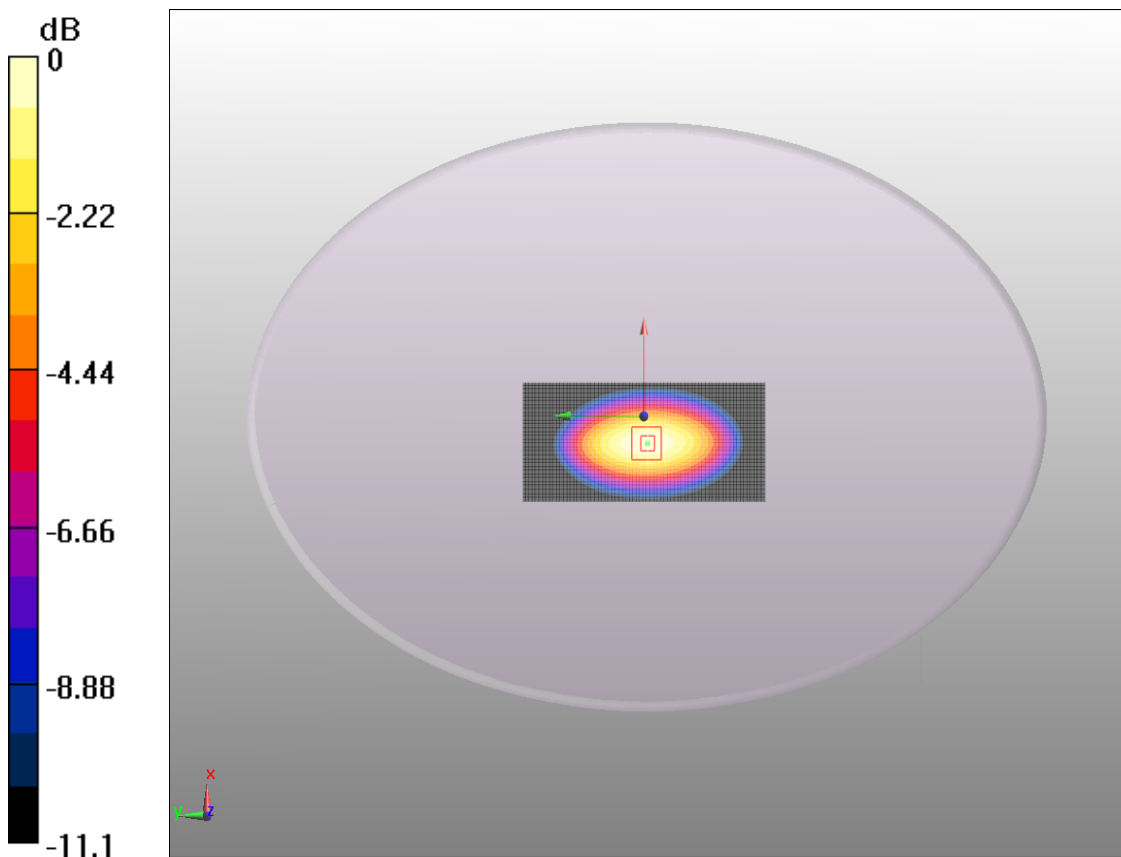

0 dB =  $2.59\text{mW/g}$

**Fig.G1 validation 835MHz 250mW**

### 835 MHz

Date/Time: 2010-10-24 11:17:25 AM

Electronics: DAE4 Sn786

Medium: 850 body

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.98 \text{ mho/m}$ ;  $\epsilon_r = 55.35$ ;  $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature:  $22.0^\circ\text{C}$       Liquid Temperature:  $22.0^\circ\text{C}$

Communication System: CW Frequency: 835 MHz Duty Cycle: 1:1

Probe: ES3DV3 - SN3151 ConvF (6.02, 6.02, 6.02)

**System Validation/Area Scan (101x101x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$

Maximum value of SAR (interpolated) =  $2.55 \text{ mW/g}$


**System Validation/Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  
 $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value =  $49.3\text{V/m}$ ; Power Drift =  $0.086 \text{ dB}$

Peak SAR (extrapolated) =  $3.46 \text{ W/kg}$

**SAR(1 g) =  $2.51 \text{ mW/g}$ ; SAR(10 g) =  $1.61 \text{ mW/g}$**

Maximum value of SAR (measured) =  $2.63 \text{ mW/g}$

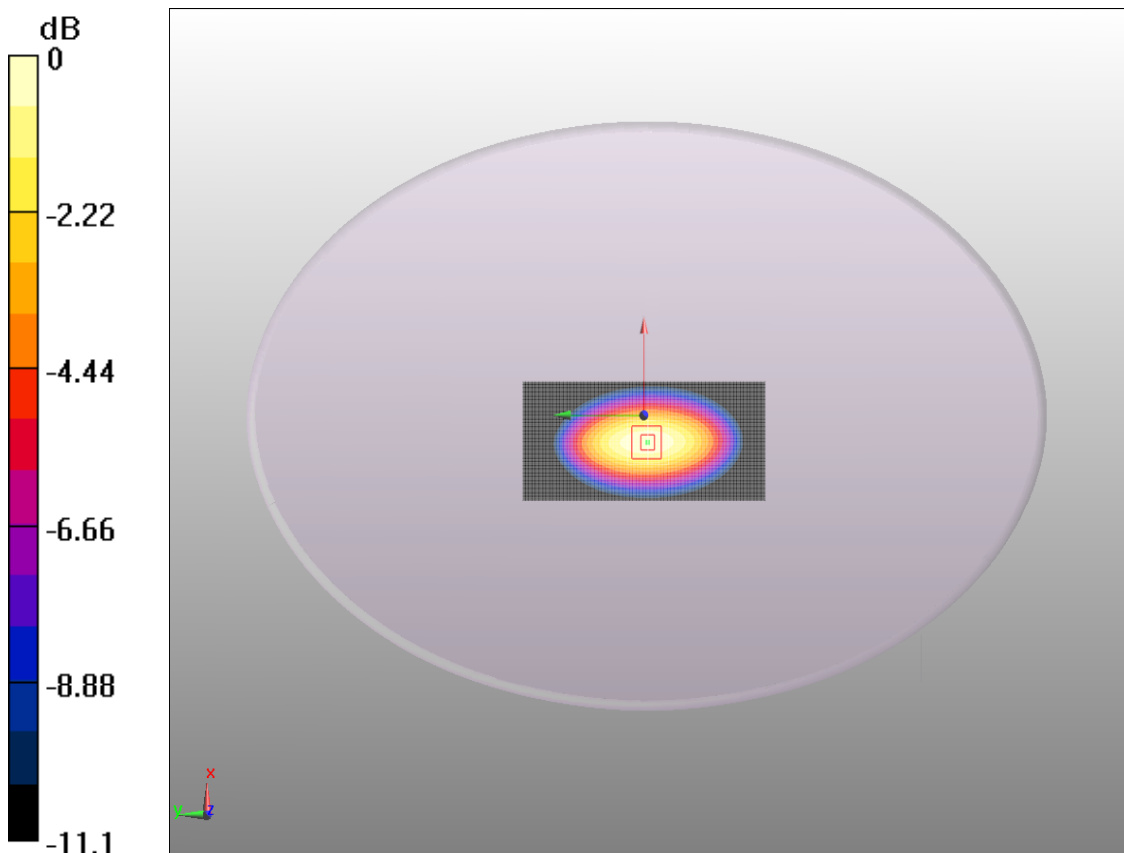

0 dB =  $2.63\text{mW/g}$

**Fig.G2 validation 835MHz 250mW**

### 835 MHz

Date/Time: 2011-10-22 08:37:24 AM

Electronics: DAE4 Sn786

Medium: 850 head

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.92 \text{ mho/m}$ ;  $\epsilon_r = 41.2$ ;  $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature:  $23.0^\circ\text{C}$       Liquid Temperature:  $23.0^\circ\text{C}$

Communication System: CW Frequency: 835 MHz Duty Cycle: 1:1

Probe: ES3DV3 - SN3151 ConvF (6.02, 6.02, 6.02)

**System Validation/Area Scan (101x101x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$   
Maximum value of SAR (interpolated) = 2.55 mW/g


**System Validation/Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  
 $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 51.2. V/m; Power Drift = 0.044 dB

Peak SAR (extrapolated) = 3.57 W/kg

**SAR(1 g) = 2.45 mW/g; SAR(10 g) = 1.56 mW/g**

Maximum value of SAR (measured) = 2.56 mW/g

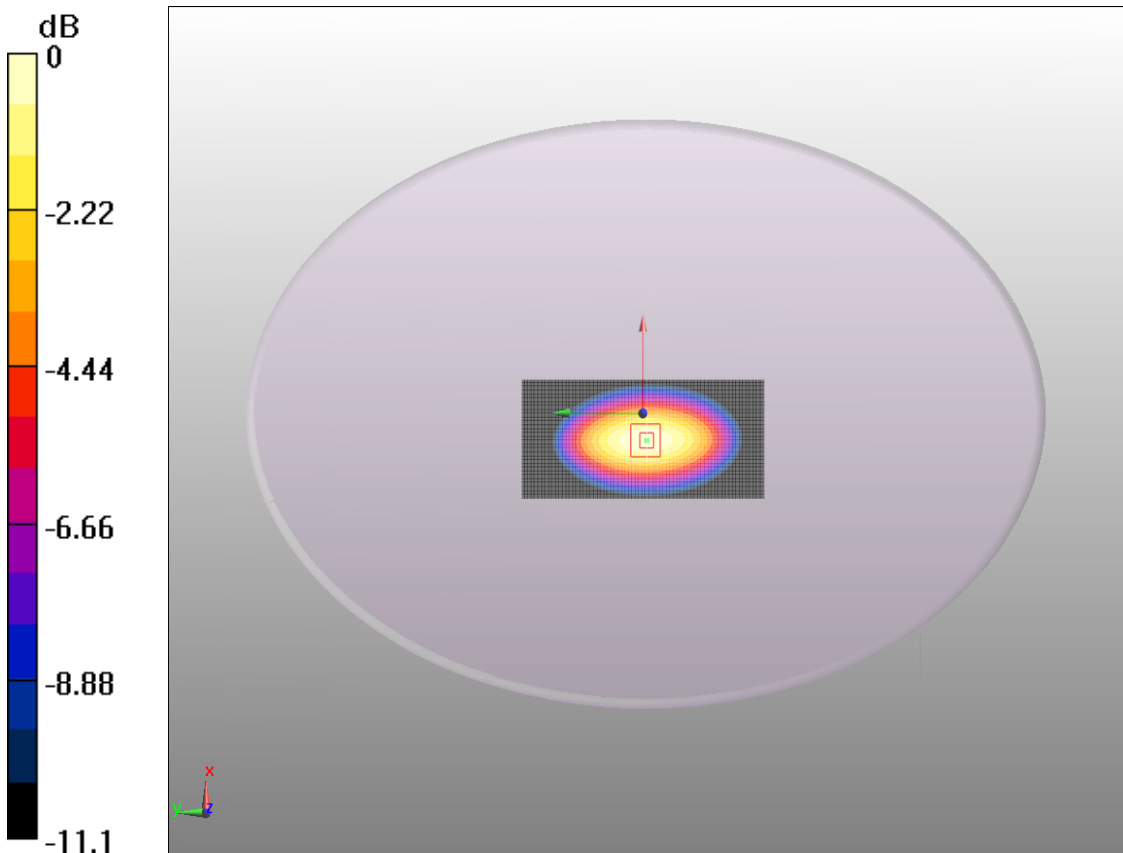

0 dB = 2.56mW/g

**Fig.G3 validation 835MHz 250mW**

### 835 MHz

Date/Time: 2011-10-23 10:57:25 AM

Electronics: DAE4 Sn786

Medium: 850 Body

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.98 \text{ mho/m}$ ;  $\epsilon_r = 53.29$ ;  $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature:  $23.0^\circ\text{C}$       Liquid Temperature:  $23.0^\circ\text{C}$

Communication System: CW Frequency: 835 MHz Duty Cycle: 1:1

Probe: ES3DV3 - SN3151 ConvF (6.02, 6.02, 6.02)

**System Validation/Area Scan (101x101x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$   
Maximum value of SAR (interpolated) =  $2.58 \text{ mW/g}$


**System Validation/Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  
 $dz=5\text{mm}$

Reference Value =  $48.0 \text{ V/m}$ ; Power Drift =  $0.053 \text{ dB}$

Peak SAR (extrapolated) =  $3.49 \text{ W/kg}$

**SAR(1 g) =  $2.48 \text{ mW/g}$ ; SAR(10 g) =  $1.59 \text{ mW/g}$**

Maximum value of SAR (measured) =  $2.66\text{mW/g}$

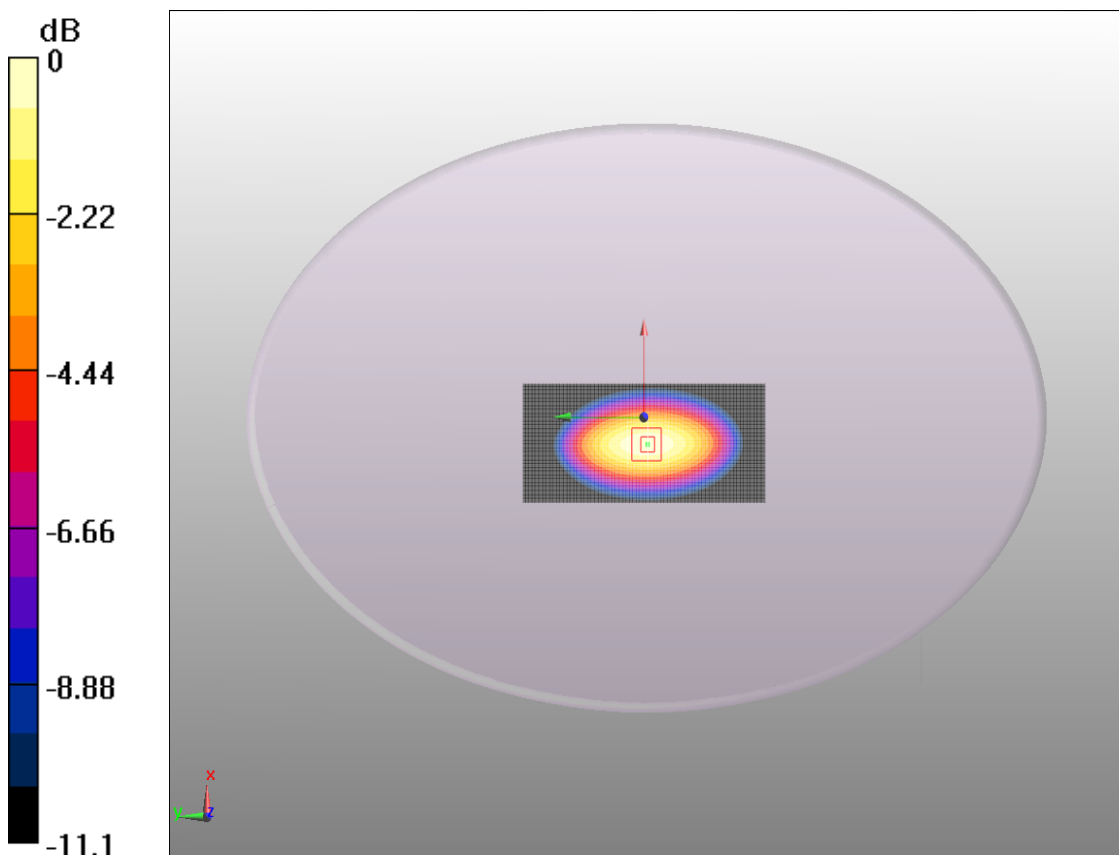

0 dB =  $2.66\text{mW/g}$

**Fig.G4 validation 835MHz 250mW**

## G2 Dipole1900

The information and documentation below are provided to qualify the extended 3-year calibration interval of dipole.

### G2.1 List of Equipment

No.	Name	Type	Serial Number
01	Network analyzer	E5071C	MY46103759
02	Power meter	NRVD	101253
03	Power sensor	NRV-Z5	100333
04	Signal Generator	E4438C	MY45095825
05	Amplifier	VTL5400	0404
06	E-field Probe	SPEAG ES3DV3	3151
07	DAE	SPEAG DAE4	786
08	Dipole Validation Kit	SPEAG D1900V2	541

### G2.2 Results of Impedance, Return-loss and System validation

#### Dipole1900 - Head

		Year			Deviation		Limit
		2009	2010	2011	2010	2011	
Impedance	Real ( $\Omega$ )	54.4	54.6	54.8	0.2 $\Omega$	0.4 $\Omega$	Deviation < 5 $\Omega$
	Imaginary ( $\Omega$ )	5.8	5.3	5.5	0.5 $\Omega$	0.3 $\Omega$	Deviation < 5 $\Omega$
Return-loss (dB)		-23.02	-23.10	-23.21	0.1dB	0.19dB	Deviate < 0.2dB
System validation	10g	5.12	5.14	5.16	0.39%	0.78%	Deviation < 10%
	1g	9.97	9.98	10.1	0.1%	1.3%	Deviation < 10%

#### Dipole 1900 - Body

		Year			Deviation		Limit
		2009	2010	2011	2010	2011	
Impedance	Real ( $\Omega$ )	47.6	47.5	47.4	0.1 $\Omega$	0.2 $\Omega$	Deviation < 5 $\Omega$
	Imaginary ( $\Omega$ )	7.0	7.2	7.2	0.2 $\Omega$	0.2 $\Omega$	Deviation < 5 $\Omega$
Return-loss (dB)		-22.4	-22.28	-22.50	0.12dB	0.10dB	Deviate < 0.2dB
System validation	10g	5.29	5.22	5.24	-1.32%	-0.95%	Deviation < 10%
	1g	10.4	10.6	10.8	1.92%	3.85%	Deviation < 10%


According to the above tables, it is not necessary to recalibration the dipoles in 2010 and 2011.

Please see below for the detail information.




## G2.3 Detail Information


### G2.3.1 Impedance Measurement Plot

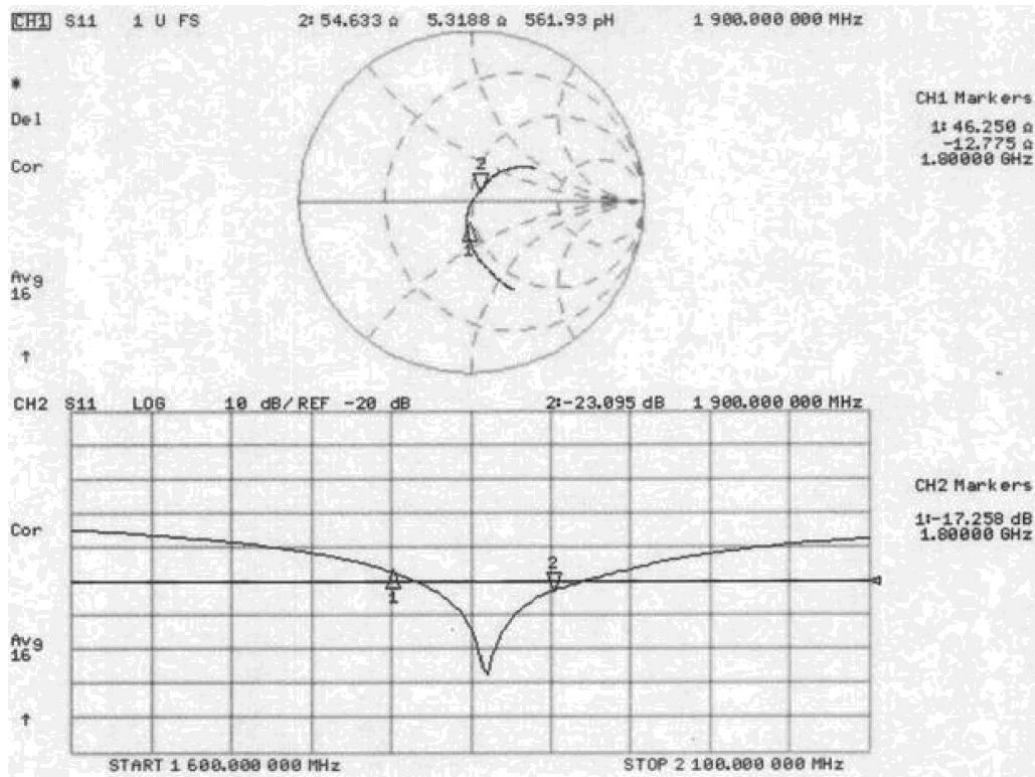


Picture G5: Impedance Measurement Plot \_Dipole 1900 Head\_2010

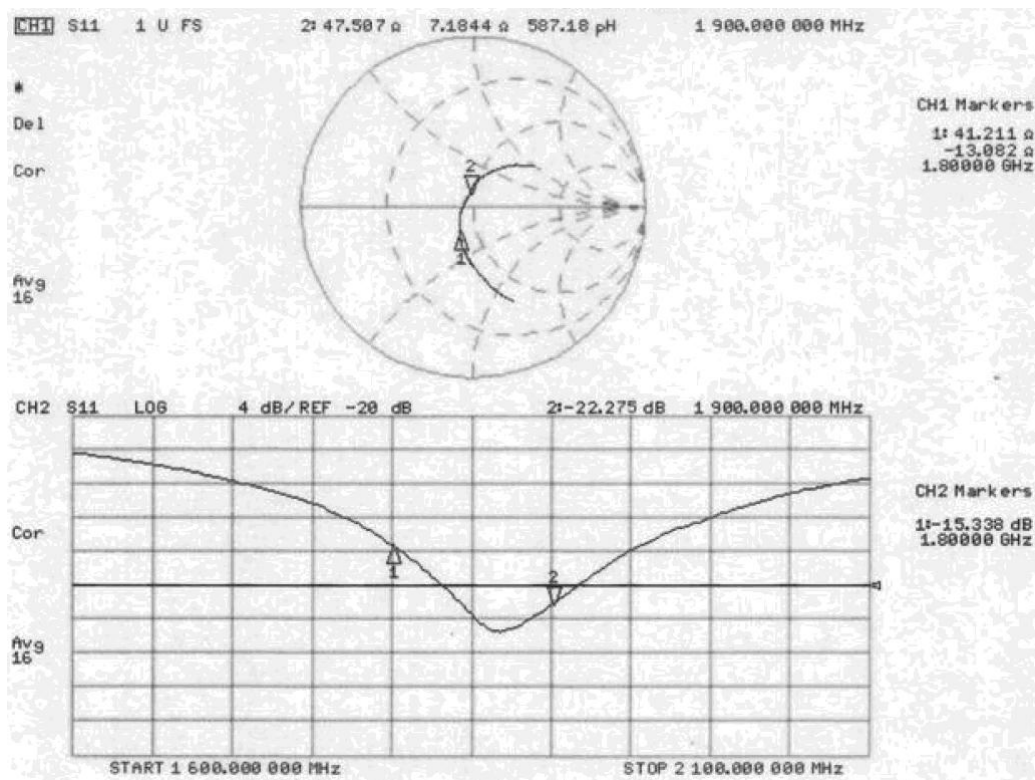

Picture G6: Impedance Measurement Plot \_Dipole 1900 body\_2010

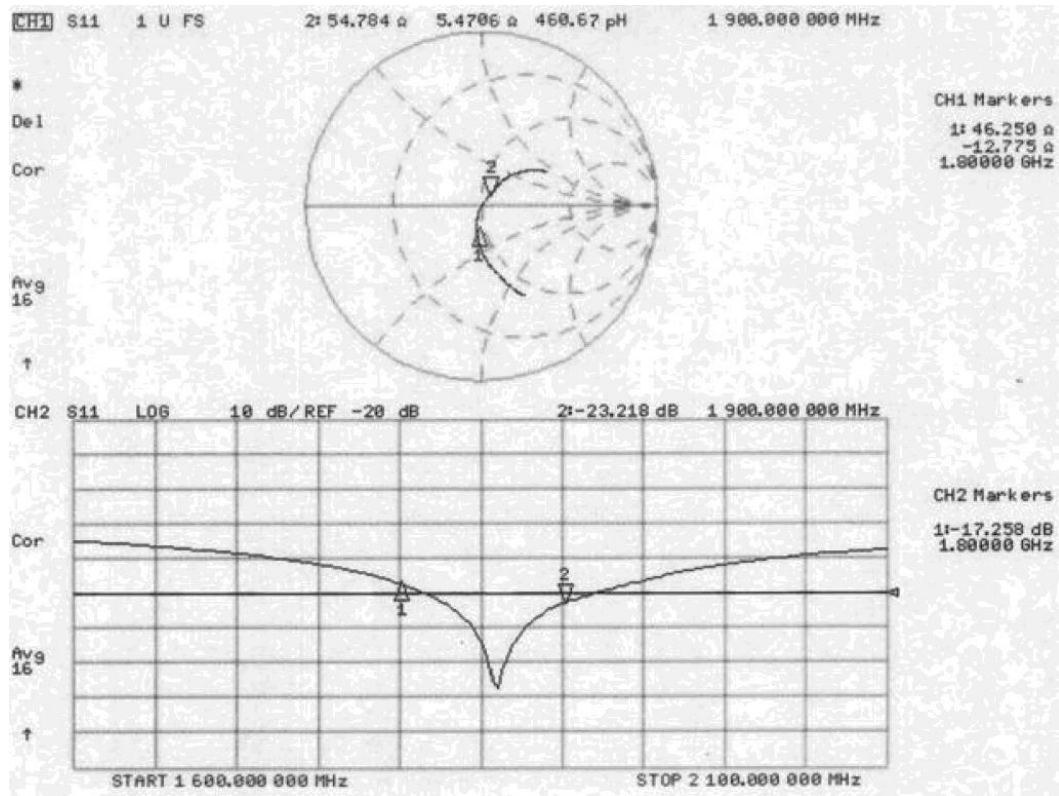

Picture G7: Impedance Measurement Plot \_Dipole 1900 Head\_2011

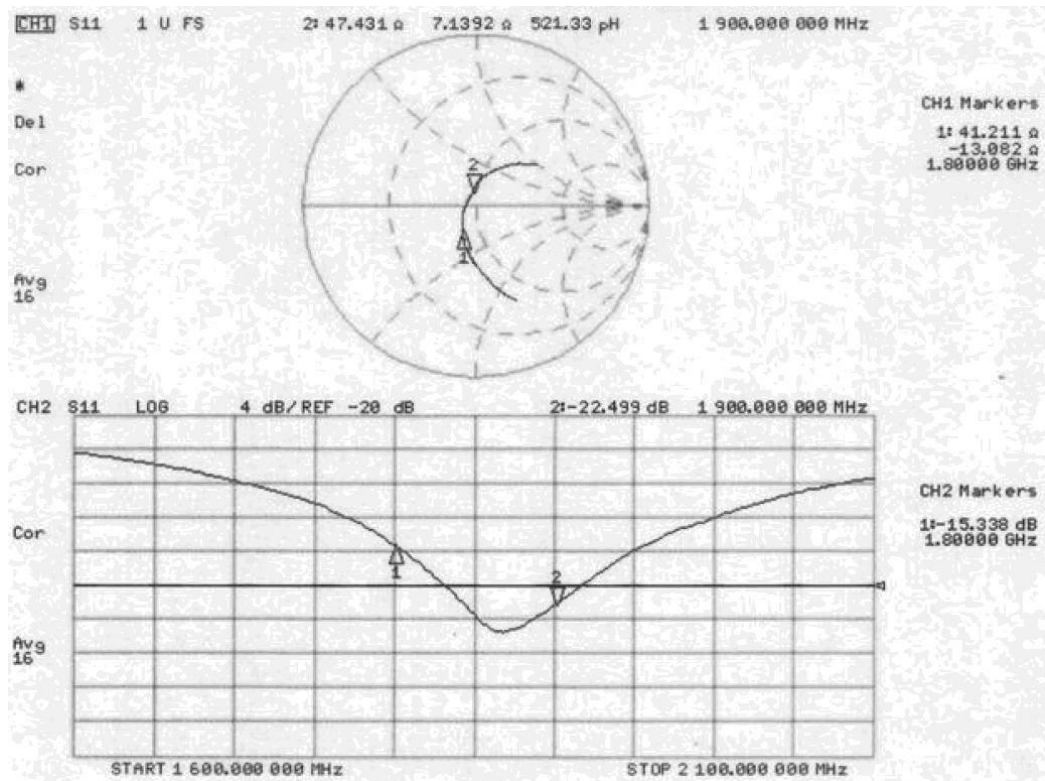

Picture G8: Impedance Measurement Plot \_Dipole 1900 body\_2011

### G2.3.2 System Validation Results

#### 1900MHz

Date/Time: 10/25/2010 8:36:15 AM

Electronics: DAE4 Sn786

Medium: head 1900 MHz

Medium parameters used:  $f = 1900 \text{ MHz}$ ;  $\sigma = 1.41 \text{ mho/m}$ ;  $\epsilon_r = 40.56$ ;  $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature:  $22.0^\circ\text{C}$       Liquid Temperature:  $22.0^\circ\text{C}$

Communication System: CW Frequency: 1900 MHz Duty Cycle: 1:1

Probe: ES3DV3 - SN3151 ConvF (4.87, 4.87, 4.87)

**System Validation/Area Scan (101x101x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$

Maximum value of SAR (interpolated) =  $11.2 \text{ mW/g}$


**System Validation/Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value =  $92.8 \text{ V/m}$ ; Power Drift =  $0.052 \text{ dB}$

Peak SAR (extrapolated) =  $16.9 \text{ W/kg}$

**SAR(1 g) =  $9.98 \text{ mW/g}$ ; SAR(10 g) =  $5.14 \text{ mW/g}$**

Maximum value of SAR (measured) =  $11.4 \text{ mW/g}$

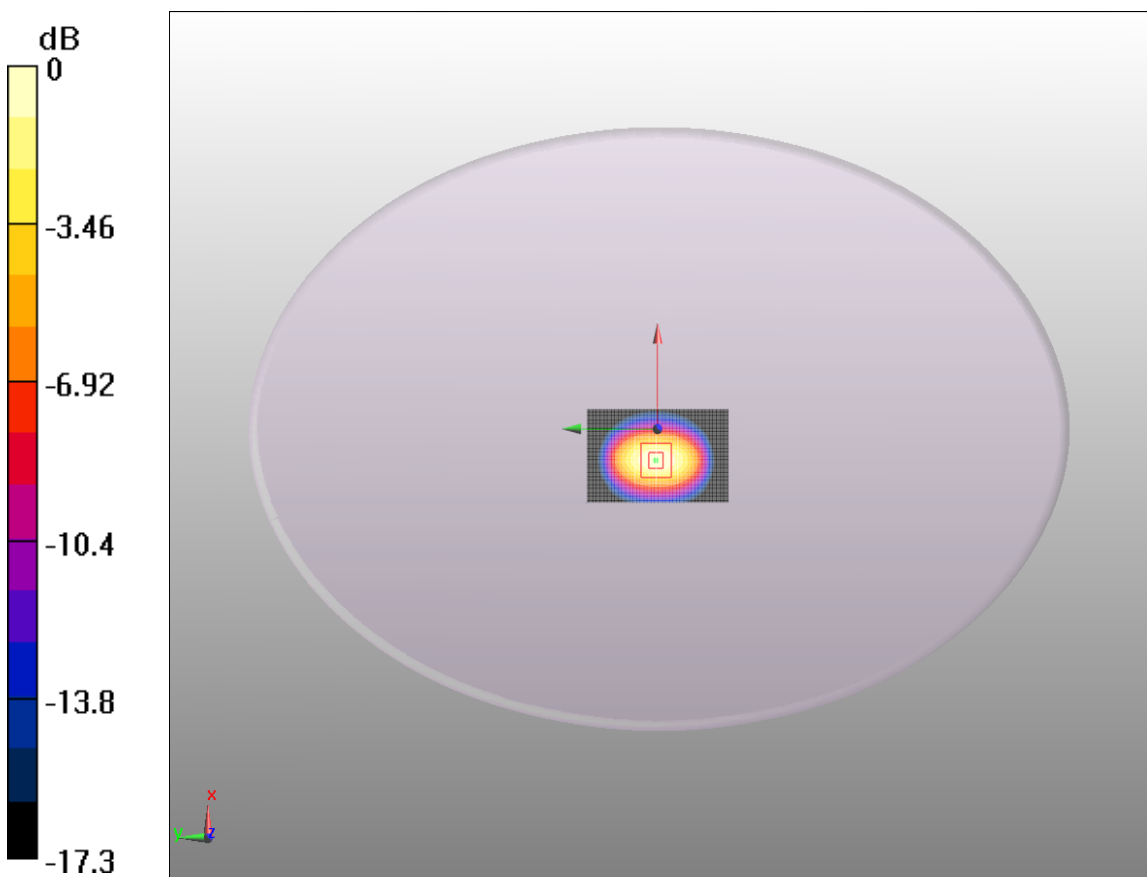

0 dB =  $11.4 \text{ mW/g}$

**Fig.G5 validation 1900MHz 250mW**

## 1900MHz

Date/Time: 10/25/2010 4:41:18 PM

Electronics: DAE4 Sn786

Medium: Body 1900 MHz

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.53$  mho/m;  $\epsilon_r = 52.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.0°C      Liquid Temperature: 22.0°C

Communication System: CW Frequency: 1900 MHz Duty Cycle: 1:1

Probe: ES3DV3 - SN3151 ConvF (4.87, 4.87, 4.87)

**System Validation/Area Scan (101x101x1):** Measurement grid: dx=10mm, dy=10mm  
Maximum value of SAR (interpolated) = 10.8 mW/g


**System Validation/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 90.2 V/m; Power Drift = 0.022 dB

Peak SAR (extrapolated) = 17.1 W/kg

**SAR(1 g) = 10.6 mW/g; SAR(10 g) = 5.22 mW/g**

Maximum value of SAR (measured) = 11.1 mW/g

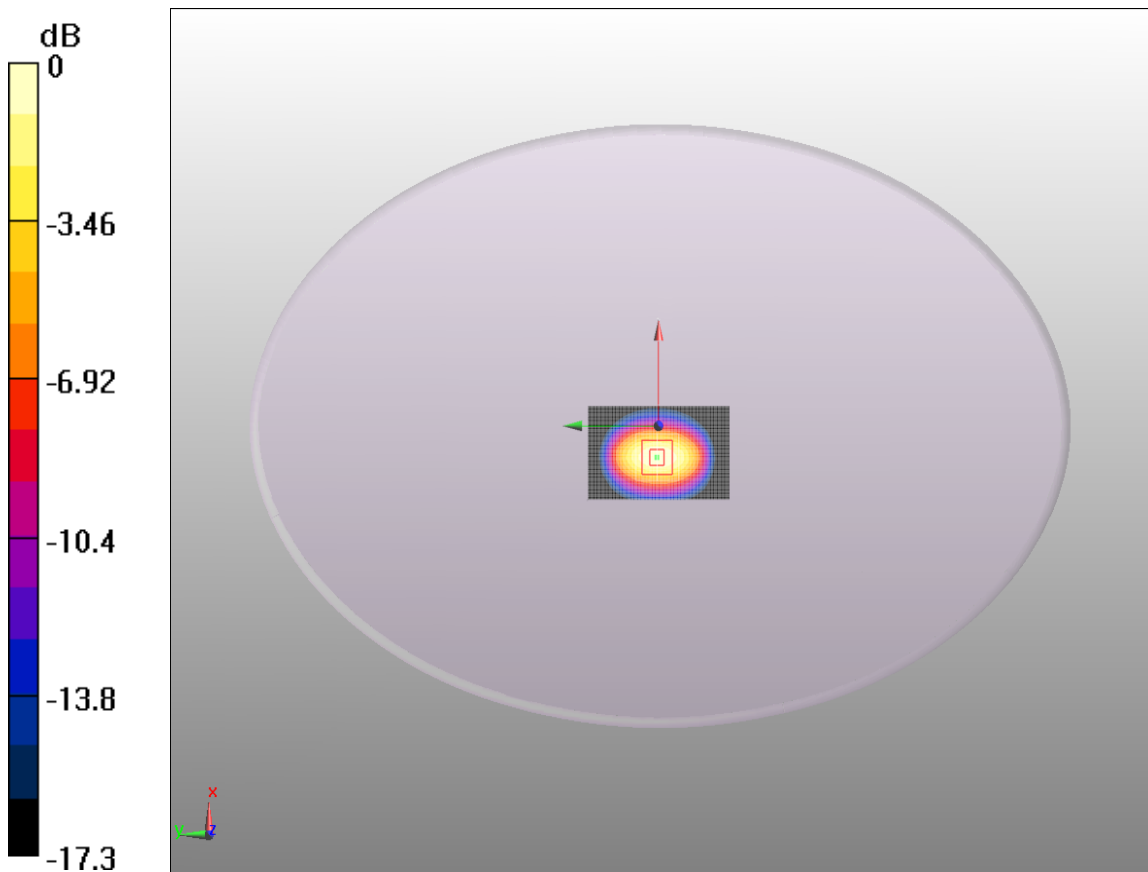

0 dB = 11.1mW/g

**Fig.G6 validation 1900MHz 250mW**

## 1900MHz

Date/Time: 10/24/2011 8:56:15 AM

Electronics: DAE4 Sn786

Medium: head 1900 MHz

Medium parameters used:  $f = 1900 \text{ MHz}$ ;  $\sigma = 1.44 \text{ mho/m}$ ;  $\epsilon_r = 40.65$ ;  $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature:  $23.0^\circ\text{C}$       Liquid Temperature:  $23.0^\circ\text{C}$

Communication System: CW Frequency: 1900 MHz Duty Cycle: 1:1

Probe: ES3DV3 - SN3151 ConvF (4.87, 4.87, 4.87)

**System Validation/Area Scan (101x101x1):** Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$   
Maximum value of SAR (interpolated) =  $10.6 \text{ mW/g}$


**System Validation/Zoom Scan (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  
 $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value =  $94.4 \text{ V/m}$ ; Power Drift =  $0.019 \text{ dB}$

Peak SAR (extrapolated) =  $16.9 \text{ W/kg}$

**SAR(1 g) =  $10.1 \text{ mW/g}$ ; SAR(10 g) =  $5.16 \text{ mW/g}$**

Maximum value of SAR (measured) =  $10.9 \text{ mW/g}$

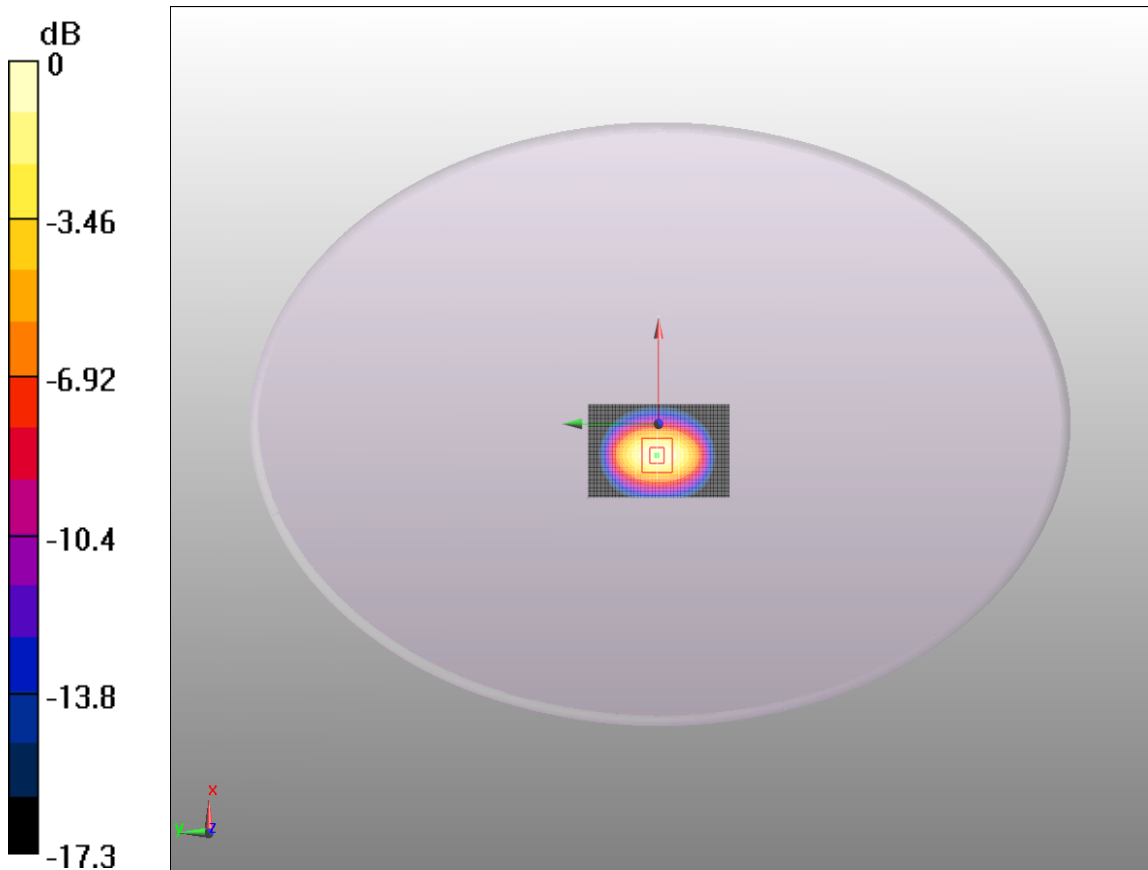

0 dB =  $10.9 \text{ mW/g}$

**Fig.G7 validation 1900MHz 250Mw**

## 1900MHz

Date/Time: 10/24/2011 4:51:12 PM

Electronics: DAE4 Sn786

Medium: Body 1900 MHz

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.54$  mho/m;  $\epsilon_r = 52.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0°C      Liquid Temperature: 23.0°C

Communication System: CW Frequency: 1900 MHz Duty Cycle: 1:1

Probe: ES3DV3 - SN3151 ConvF (4.87, 4.87, 4.87)

**System Validation/Area Scan (101x101x1):** Measurement grid: dx=10mm, dy=10mm  
Maximum value of SAR (interpolated) = 11.8 mW/g


**System Validation/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 89.5 V/m; Power Drift = 0.052 dB

Peak SAR (extrapolated) = 16.8 W/kg

**SAR(1 g) = 10.8 mW/g; SAR(10 g) = 5.24 mW/g**

Maximum value of SAR (measured) = 11.8 mW/g

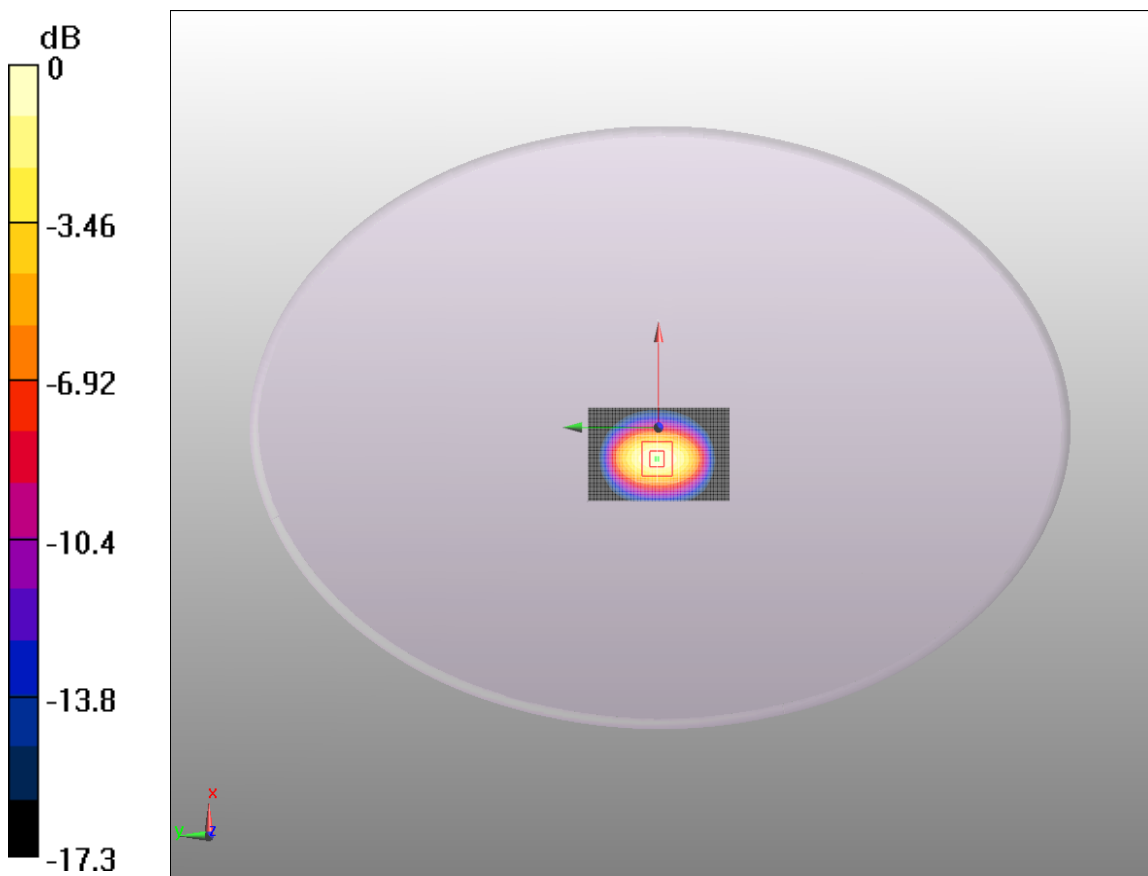


0 dB = 11.8 mW/g

**Fig.G8 validation 1900MHz 250mW**

## ANNEX H Analysis of Effective Frequency Interval of Probe

### ANNEX H.1 835 MHz\_12/22/2011

The test frequencies are properly matched as this is GSM850/WCDMA850. The probe calibration for permittivity and conductivity is within  $\pm 5\%$ , were the probe calibrated centre frequency at 900MHz has permittivity and conductivity of 55.0 and 1.05 respectively. At the probe extreme frequencies the following are true: at 800 MHz the permittivity and conductivity are 52.3 and 0.92 respectively. At 1000 MHz the permittivity and conductivity are 57.8 and 1.1 respectively. The probe was calibrated at these parameters in order to cover the frequency range 800 MHz to 1000 MHz.

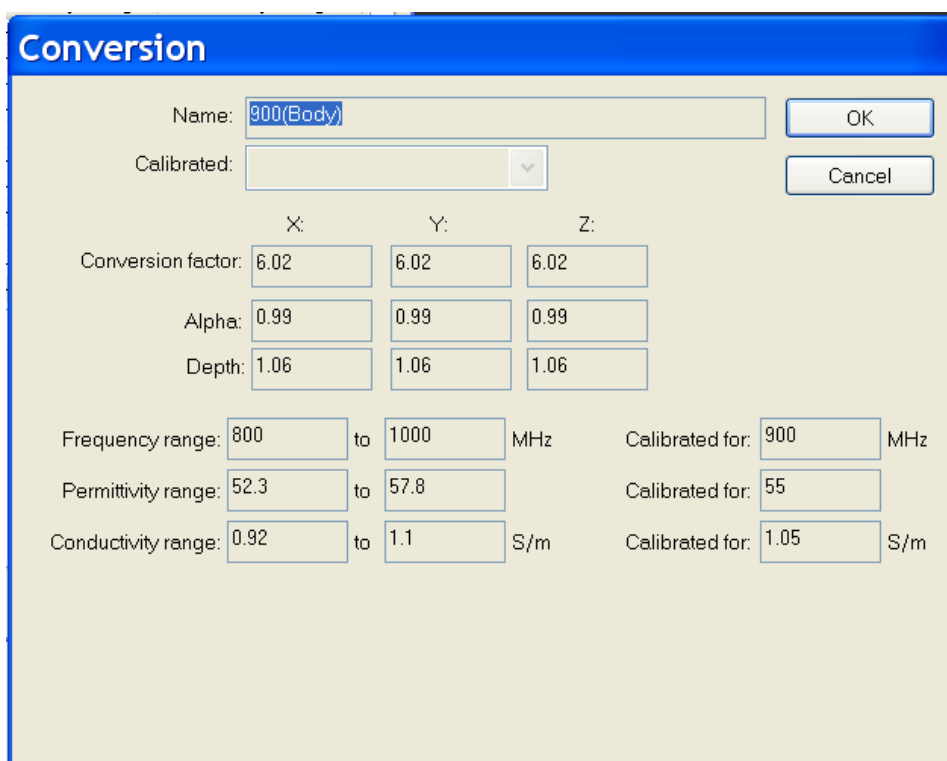

**Conversion**

Name:

Calibrated:

X: Y: Z:

Conversion factor:

Alpha:

Depth:

Frequency range:  to  MHz Calibrated for:  MHz

Permittivity range:  to  Calibrated for:

Conductivity range:  to  S/m Calibrated for:  S/m

The target permittivity and conductivity at 835 MHz is 55.2 and 0.97 respectively which is within the calibrated range of the probe parameter.

The following parameters are declared in the probe calibration certificate on page 8:

f[MHz]	Validity[MHz] <sup>C</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF	Uncertainty
450	$\pm 50 / \pm 100$	Head	43.5 $\pm 5\%$	0.87 $\pm 5\%$	0.82	1.44	7.42	$\pm 13.3\%$ (k=2)
900	$\pm 50 / \pm 100$	Head	41.5 $\pm 5\%$	0.97 $\pm 5\%$	0.80	1.29	6.23	$\pm 11.0\%$ (k=2)
1810	$\pm 50 / \pm 100$	Head	40.0 $\pm 5\%$	1.40 $\pm 5\%$	0.61	1.57	5.08	$\pm 11.0\%$ (k=2)
1900	$\pm 50 / \pm 100$	Head	40.0 $\pm 5\%$	1.40 $\pm 5\%$	0.63	1.44	4.98	$\pm 11.0\%$ (k=2)
2100	$\pm 50 / \pm 100$	Head	39.8 $\pm 5\%$	1.49 $\pm 5\%$	0.66	1.34	4.58	$\pm 11.0\%$ (k=2)
900	$\pm 50 / \pm 100$	Body	55.0 $\pm 5\%$	1.05 $\pm 5\%$	0.99	1.06	6.02	$\pm 11.0\%$ (k=2)
1810	$\pm 50 / \pm 100$	Body	53.3 $\pm 5\%$	1.52 $\pm 5\%$	0.75	1.34	4.87	$\pm 11.0\%$ (k=2)
1900	$\pm 50 / \pm 100$	Body	53.3 $\pm 5\%$	1.52 $\pm 5\%$	0.62	1.47	4.73	$\pm 11.0\%$ (k=2)
2100	$\pm 50 / \pm 100$	Body	53.5 $\pm 5\%$	1.57 $\pm 5\%$	0.68	1.34	4.35	$\pm 11.0\%$ (k=2)
2450	$\pm 50 / \pm 100$	Body	52.7 $\pm 5\%$	1.95 $\pm 5\%$	0.60	1.40	3.72	$\pm 11.0\%$ (k=2)


The system manufacturer has carried out addition steps as detailed on page 4 of KDB 450824.

This is detailed in the calibration certificates. The measured SAR values in the report are all below 10% of the SAR limit.


The measured fluid dielectric parameters for 835 MHz, performed during test values were all within  $\pm 5\%$  of the 835 MHz target value.

At 900 MHz, the probe was calibrated and validation performed, the tissue dielectric parameter measured for routine measurements at 900 MHz was less than the target parameter for 835 MHz  $\epsilon_r$  and higher than the target parameter for 835 MHz  $\sigma$ .

/	Measured Fluid Parameter Date : 12/22/2011		Nominal Fluid Parameter used by System manufacturer in calibrate certificate	
	$\epsilon_r$	$\sigma$	$\epsilon_r$	$\sigma$
Frequency (MHz)				
820	53.47	0.962	53.96	0.95
825	53.43	0.966	54.37	0.96
830	53.38	0.972	54.79	0.96
835	53.22	0.99	55.2	0.97
840	53.32	0.978	55.18	0.98
845	53.26	0.985	55.17	0.98
850	53.23	0.99	55.15	0.99
900	52.74	1.05	55.00	1.05

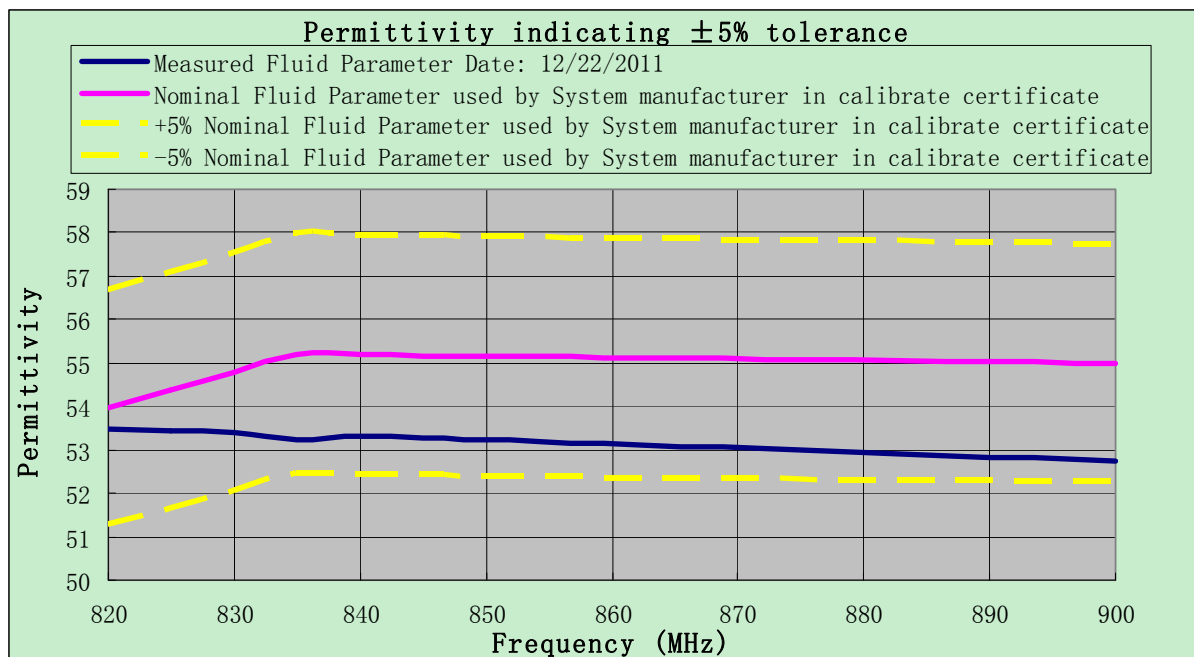



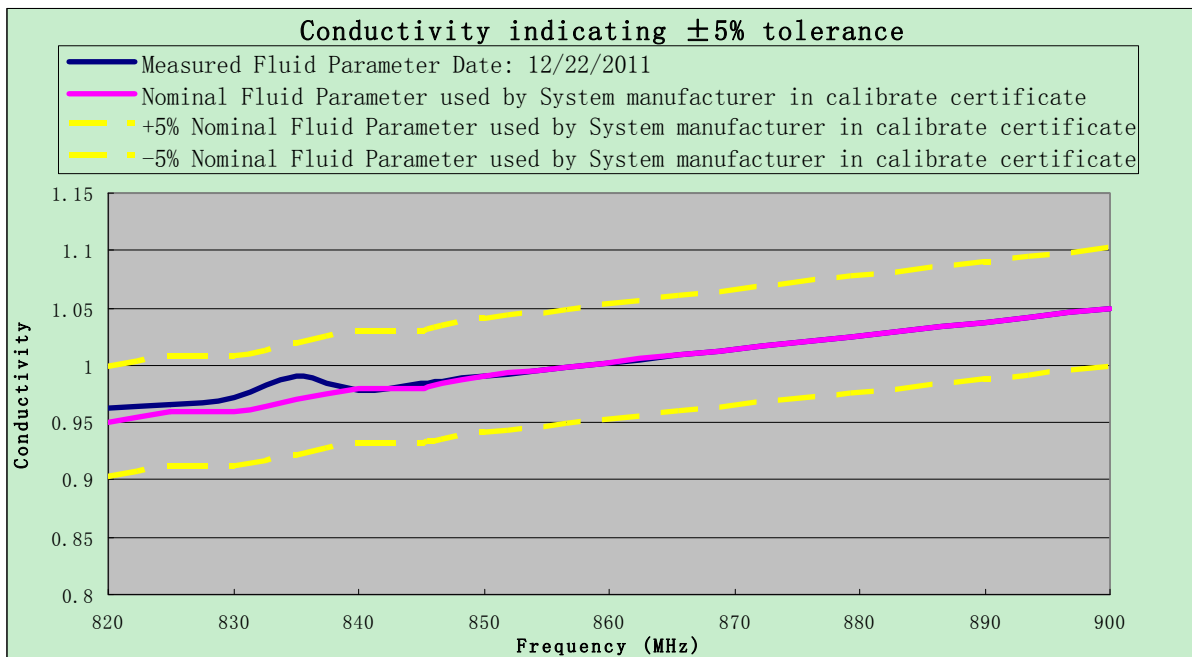

The probe conversion factor and its frequency response, with respect to the tissue dielectric media used during the probe calibration and routine measurements was examined to determine if the effective frequency interval is adequate for the intended measurements to satisfy protocol requirements. The frequency range at which the probe was calibrated for 900 MHz covered 800 MHz to 1000 MHz and the dielectric parameters required for 824 to 840 MHz were all within the calibrated range of the probe dielectric parameters.