



Appendix C – SAR Test Setup Photos

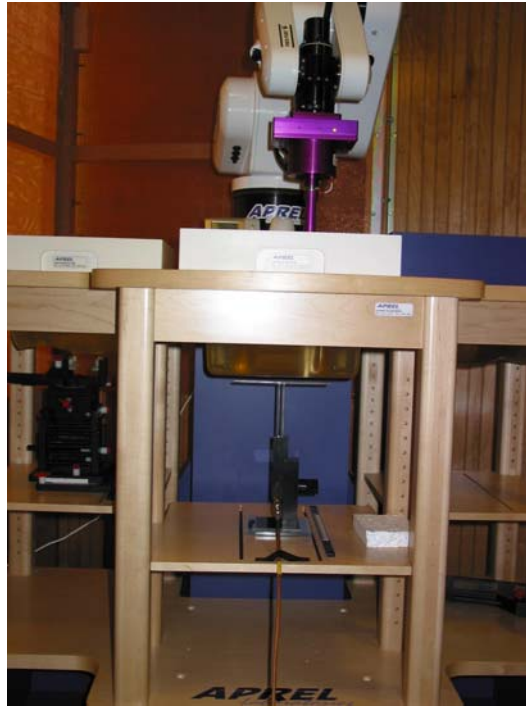

System Body Configuration

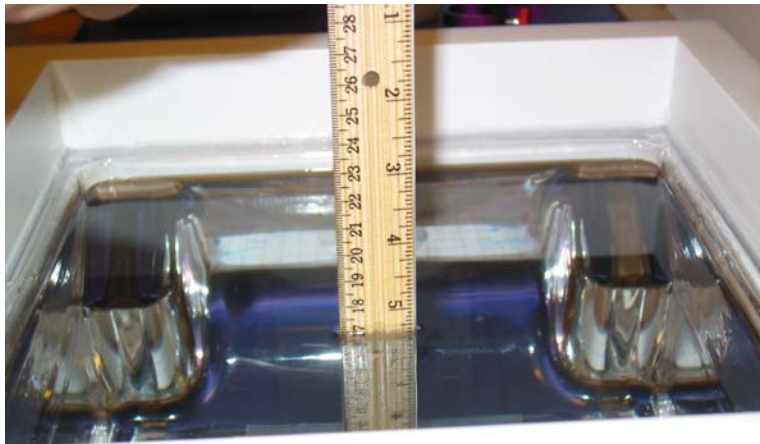

Body Tissue Depth



Bottom Back Configuration 5 mm



Bottom Front Configuration 5 mm




Top Front Configuration 5 mm



Top Back Configuration 5 mm



Left Configuration 5 mm

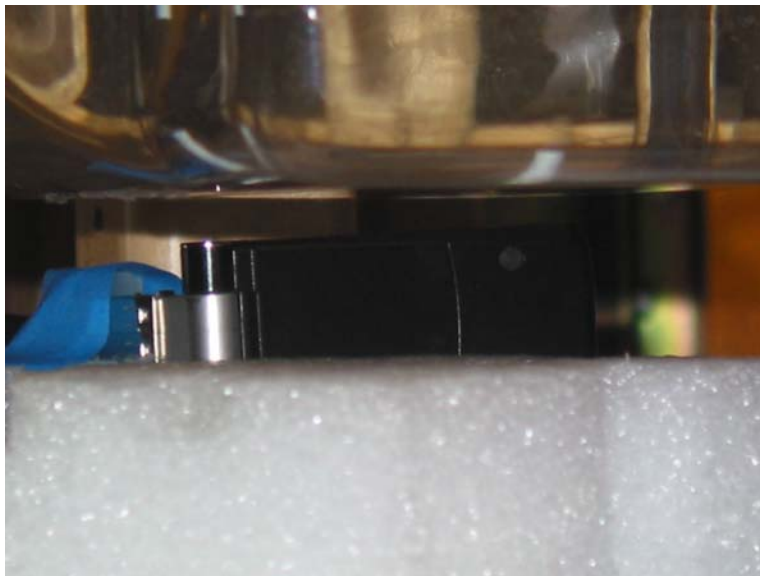

Right Configuration 5 mm



Front of Device



Back of Device